

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
 Data File : VN069207.D
 Acq On : 27 Oct 2021 1:10
 Operator : JC/MD
 Sample : M4337-21
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 DDC-2-PD

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
 Title : SW846 8260

Signal : TIC: VN069207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	8.024	2228	2250	2261	rBV2	225922	535038	2.68%	1.785%
2	8.088	2262	2274	2301	rVB	436331	985173	4.94%	3.287%
3	8.440	2385	2405	2432	rBV	247165	575924	2.89%	1.922%
4	8.971	2581	2603	2629	rBV	638770	1319531	6.62%	4.403%
5	10.446	3133	3153	3185	rBV	984567	1870971	9.39%	6.243%
6	10.979	3331	3352	3392	rBV	11150102	19932549	100.00%	66.512%
7	11.746	3620	3638	3665	rBV	937904	1693987	8.50%	5.653%
8	12.736	3990	4007	4030	rBV	716467	1246863	6.26%	4.161%
9	13.677	4339	4358	4381	rBV	773226	1324866	6.65%	4.421%
10	14.214	4543	4558	4577	rBV2	280227	483613	2.43%	1.614%




Sum of corrected areas: 29968515

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069207.D
Acq On : 27 Oct 2021 1:10
Operator : JC/MD
Sample : M4337-21
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-2-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

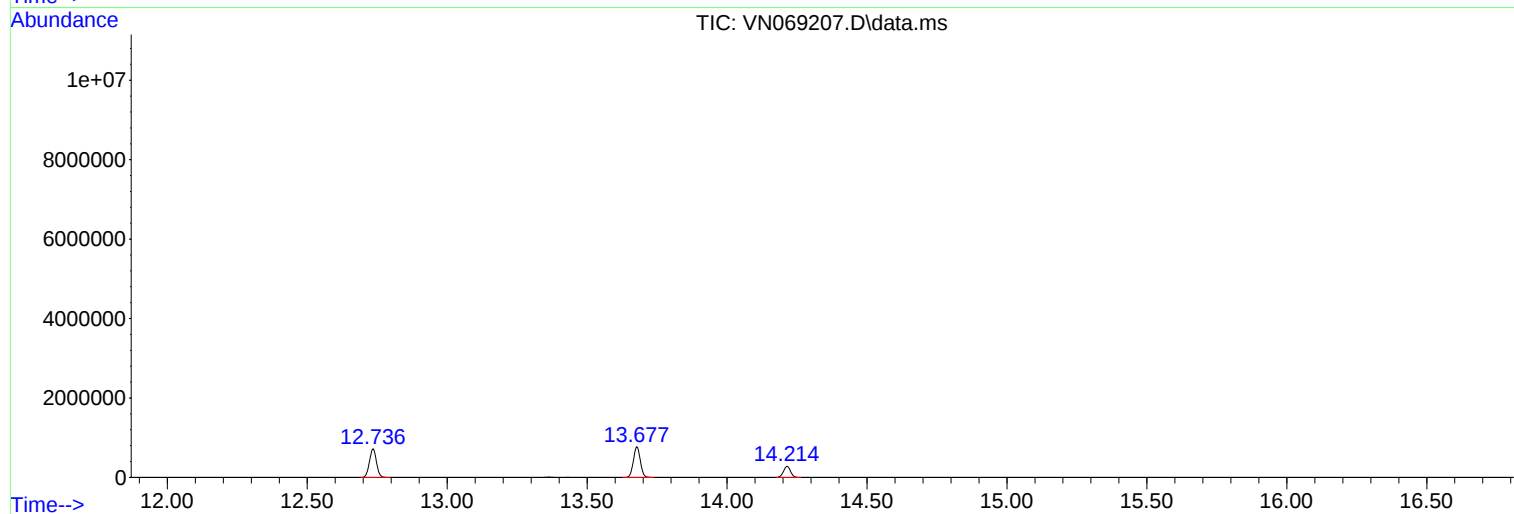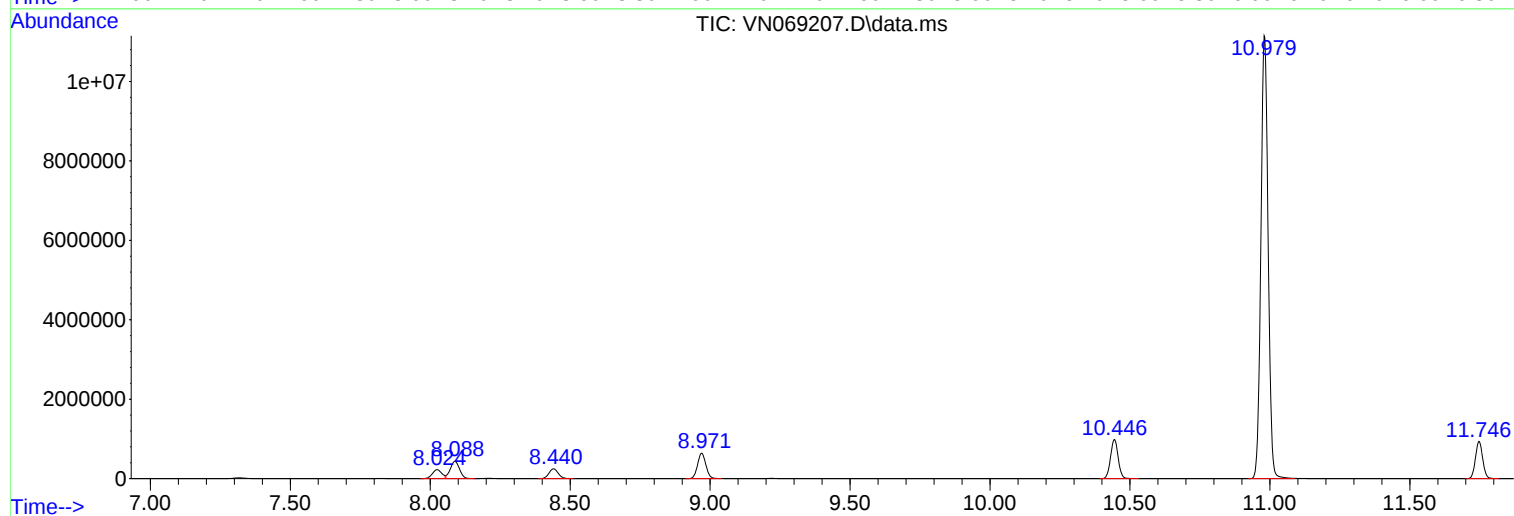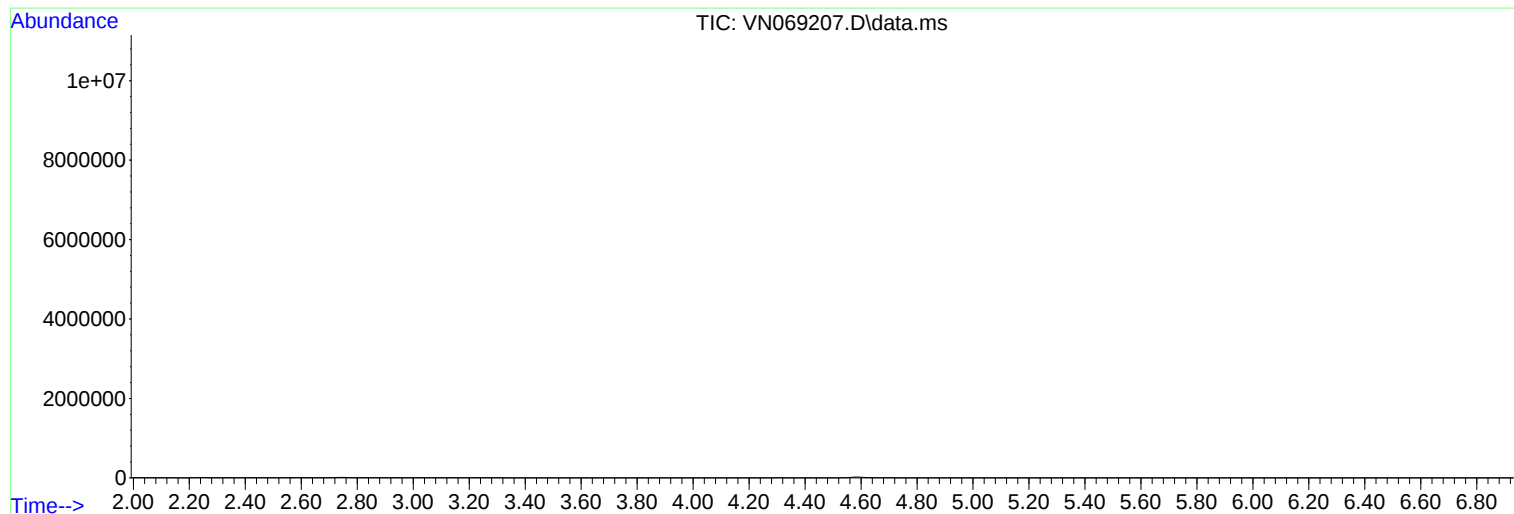

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069207.D
Acq On : 27 Oct 2021 1:10
Operator : JC/MD
Sample : M4337-21
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-2-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069207.D
Acq On : 27 Oct 2021 1:10
Operator : JC/MD
Sample : M4337-21
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-2-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
