

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
 Data File : VN069208.D
 Acq On : 27 Oct 2021 1:35
 Operator : JC/MD
 Sample : M4337-22
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 DDC-2-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M

Title : SW846 8260

Signal : TIC: VN069208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.583	947	967	995	rBV2	26806	89705	4.94%	0.934%
2	7.316	1963	1986	2016	rBV	33989	101630	5.60%	1.058%
3	8.024	2228	2250	2261	rBV	222067	527059	29.02%	5.485%
4	8.088	2262	2274	2305	rVB	424616	960057	52.86%	9.991%
5	8.440	2385	2405	2433	rBV	242357	563713	31.04%	5.867%
6	8.971	2583	2603	2625	rBV	618424	1283619	70.68%	13.359%
7	10.443	3132	3152	3185	rBV	958081	1816113	100.00%	18.901%
8	10.980	3337	3352	3368	rBV2	99792	180616	9.95%	1.880%
9	11.747	3620	3638	3670	rBV	918392	1650934	90.90%	17.182%
10	12.734	3989	4006	4034	rBV	684837	1187222	65.37%	12.356%
11	13.678	4339	4358	4388	rBV	726292	1248071	68.72%	12.989%


Sum of corrected areas: 9608739

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069208.D
Acq On : 27 Oct 2021 1:35
Operator : JC/MD
Sample : M4337-22
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-2-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

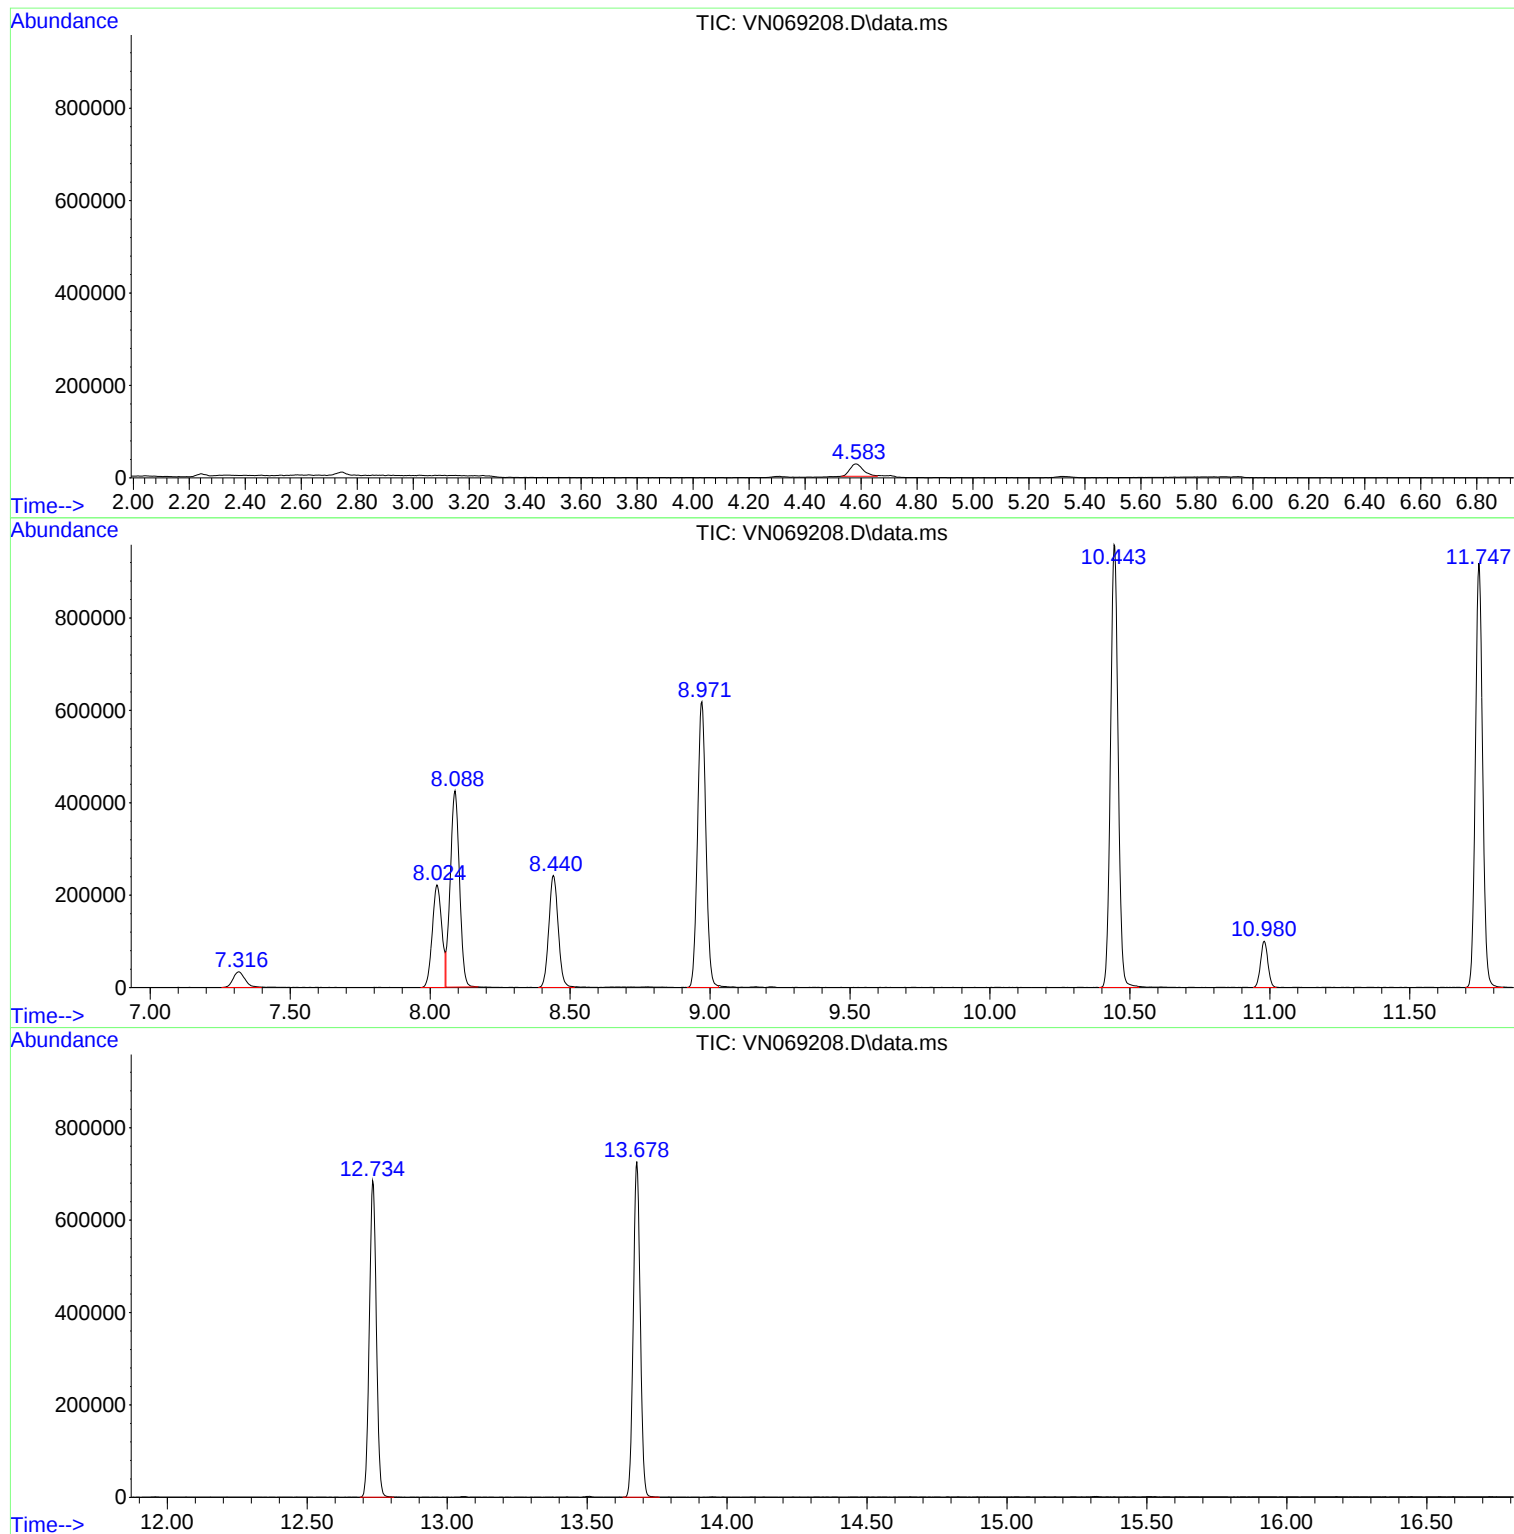

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069208.D
Acq On : 27 Oct 2021 1:35
Operator : JC/MD
Sample : M4337-22
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-2-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069208.D
Acq On : 27 Oct 2021 1:35
Operator : JC/MD
Sample : M4337-22
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-2-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
