

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
 Data File : VN069215.D
 Acq On : 27 Oct 2021 13:51
 Operator : JC/MD
 Sample : M4337-21 10X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 DDC-2-PD

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M

Title : SW846 8260

Signal : TIC: VN069215.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	8.024	2228	2250	2261	rBV	227586	538618	28.06%	4.704%
2	8.088	2262	2274	2303	rVB	434646	990227	51.59%	8.648%
3	8.440	2383	2405	2430	rBV	250304	578182	30.12%	5.049%
4	8.971	2577	2603	2630	rBV	630044	1321673	68.86%	11.542%
5	10.443	3132	3152	3184	rBV	977710	1866041	97.23%	16.296%
6	10.979	3334	3352	3382	rBV	1037775	1919279	100.00%	16.761%
7	11.747	3619	3638	3669	rBV	931850	1695396	88.34%	14.806%
8	12.733	3989	4006	4031	rBV	678339	1202396	62.65%	10.500%
9	13.678	4342	4358	4379	rVB	754352	1274453	66.40%	11.130%
10	14.211	4546	4557	4569	rVB4	26200	45198	2.35%	0.395%
11	15.509	5025	5041	5058	rBV	10211	19411	1.01%	0.170%


Sum of corrected areas: 11450874

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069215.D
Acq On : 27 Oct 2021 13:51
Operator : JC/MD
Sample : M4337-21 10X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-2-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

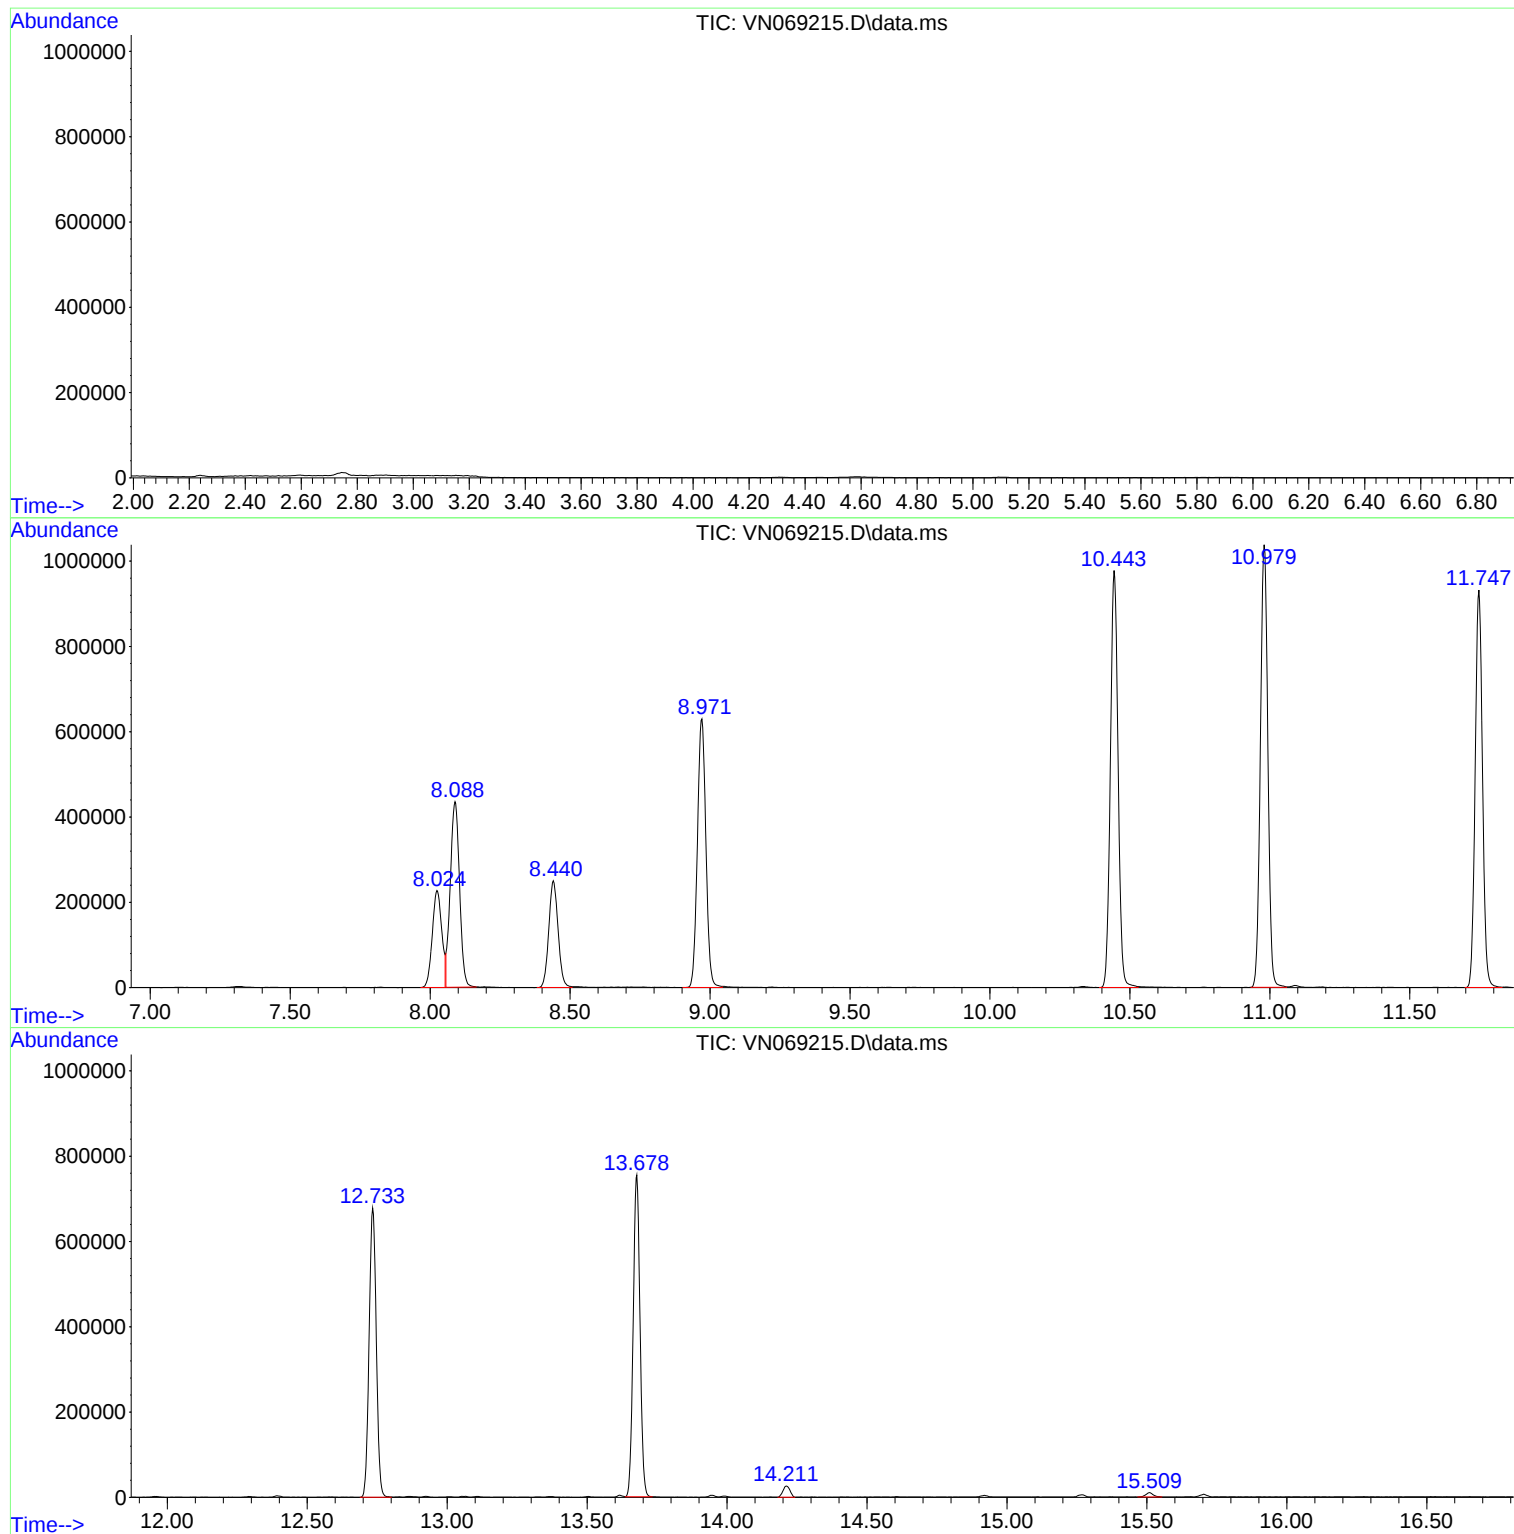

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069215.D
Acq On : 27 Oct 2021 13:51
Operator : JC/MD
Sample : M4337-21 10X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-2-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069215.D
Acq On : 27 Oct 2021 13:51
Operator : JC/MD
Sample : M4337-21 10X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DDC-2-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
