

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
 Data File : VN069223.D
 Acq On : 27 Oct 2021 17:12
 Operator : JC/MD
 Sample : M4338-04
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-3D(ONSITE)

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M

Title : SW846 8260

Signal : TIC: VN069223.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.580	947	966	992	rBV	15852	49474	2.41%	0.468%
2	7.311	1964	1984	2007	rBV	19431	56617	2.75%	0.536%
3	8.024	2220	2250	2261	rBV2	248743	594487	28.91%	5.624%
4	8.088	2262	2274	2300	rVB	482407	1089102	52.96%	10.303%
5	8.440	2384	2405	2433	rBV	276065	636241	30.94%	6.019%
6	8.971	2582	2603	2648	rBV	701202	1466757	71.32%	13.876%
7	10.443	3134	3152	3188	rBV	1082968	2056459	100.00%	19.455%
8	10.980	3339	3352	3367	rVB2	30573	54806	2.67%	0.518%
9	11.747	3617	3638	3672	rBV	1007821	1834802	89.22%	17.358%
10	12.734	3990	4006	4026	rBV	755735	1331829	64.76%	12.600%
11	13.678	4341	4358	4383	rBV	818961	1399915	68.07%	13.244%


Sum of corrected areas: 10570489

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069223.D
Acq On : 27 Oct 2021 17:12
Operator : JC/MD
Sample : M4338-04
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-3D(ONSITE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

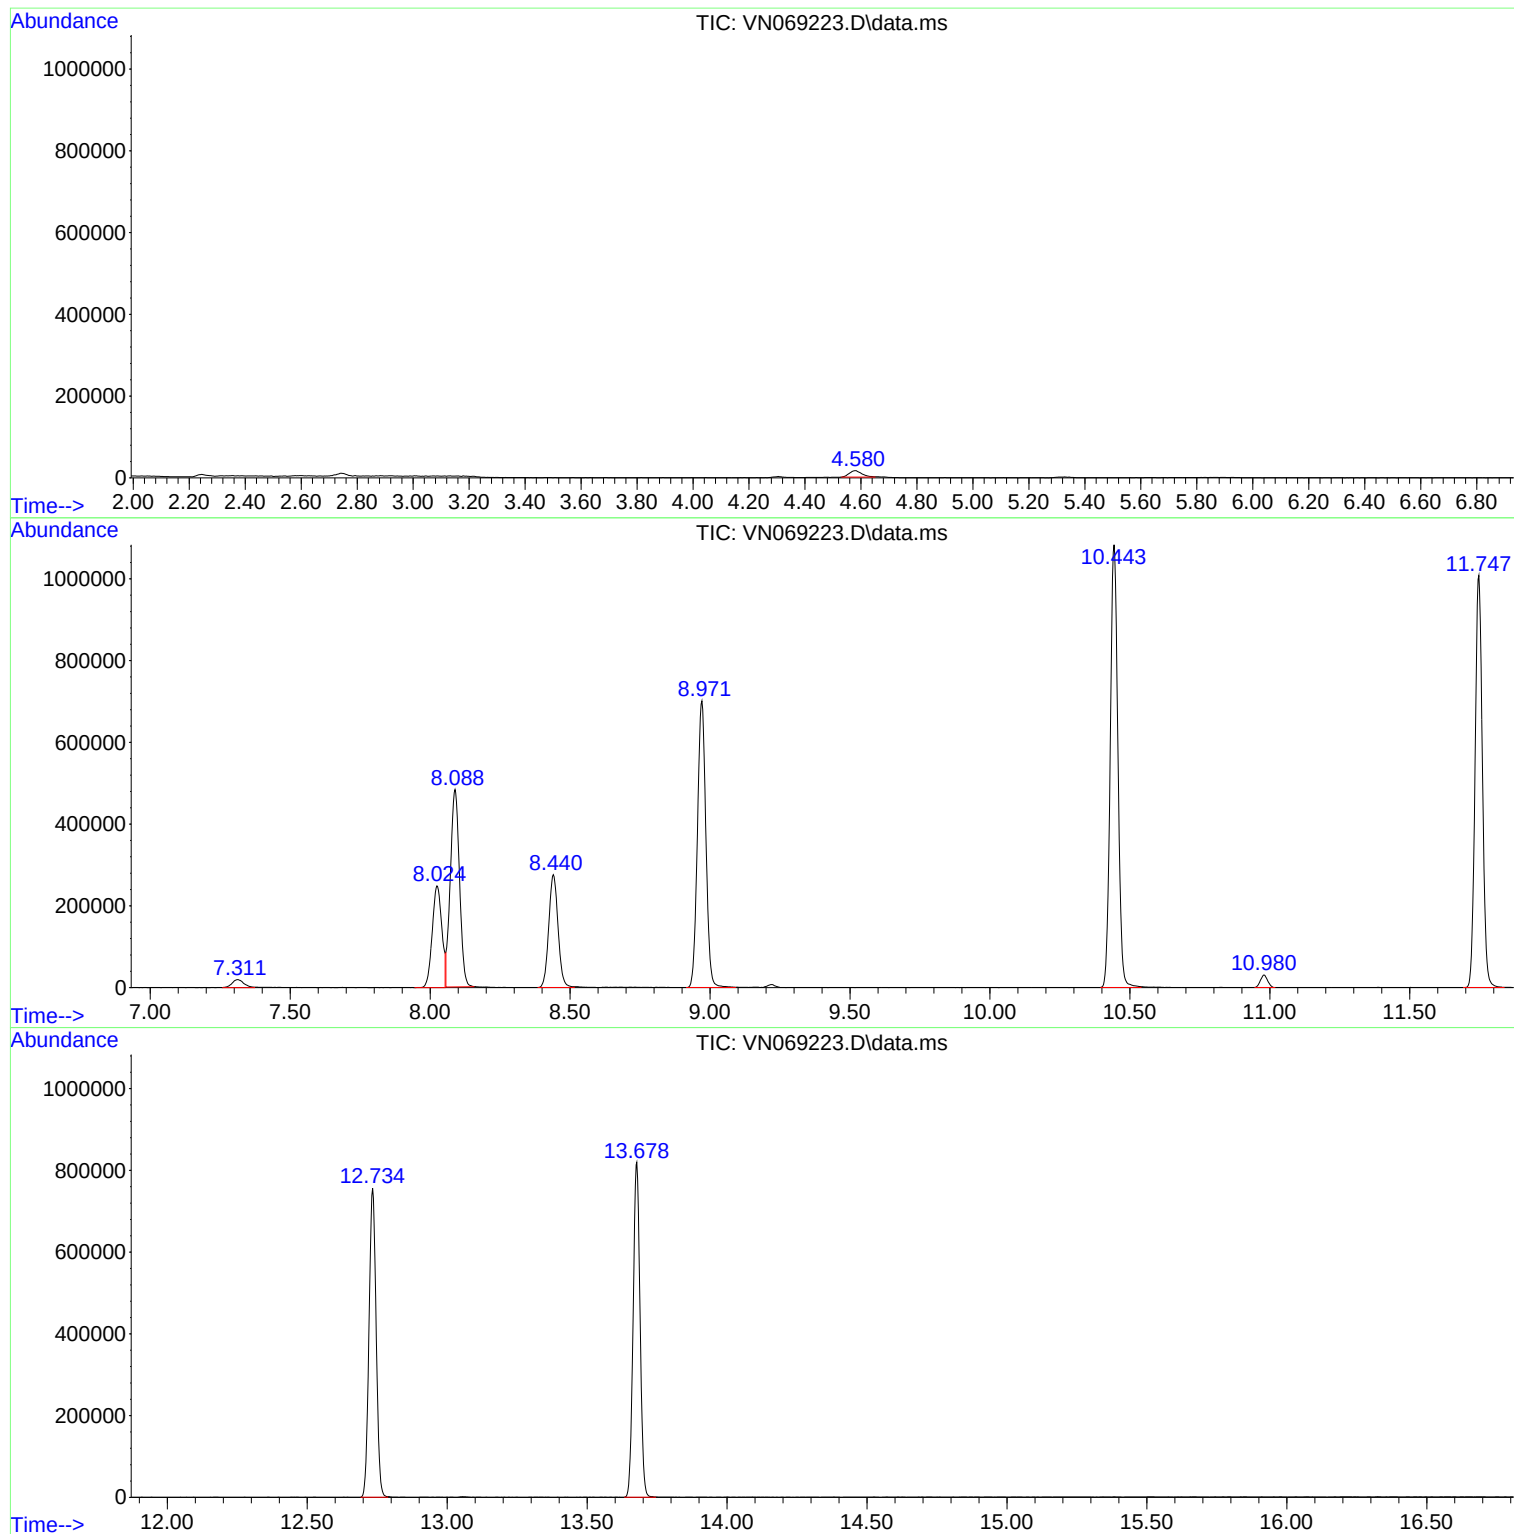

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069223.D
Acq On : 27 Oct 2021 17:12
Operator : JC/MD
Sample : M4338-04
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-3D(ONSITE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069223.D
Acq On : 27 Oct 2021 17:12
Operator : JC/MD
Sample : M4338-04
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-3D(ONSITE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
