


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
Data File : VN069199.D
Acq On : 26 Oct 2021 21:22
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Title : SW846 8260
Last Update : Wed Oct 13 05:44:40 2021

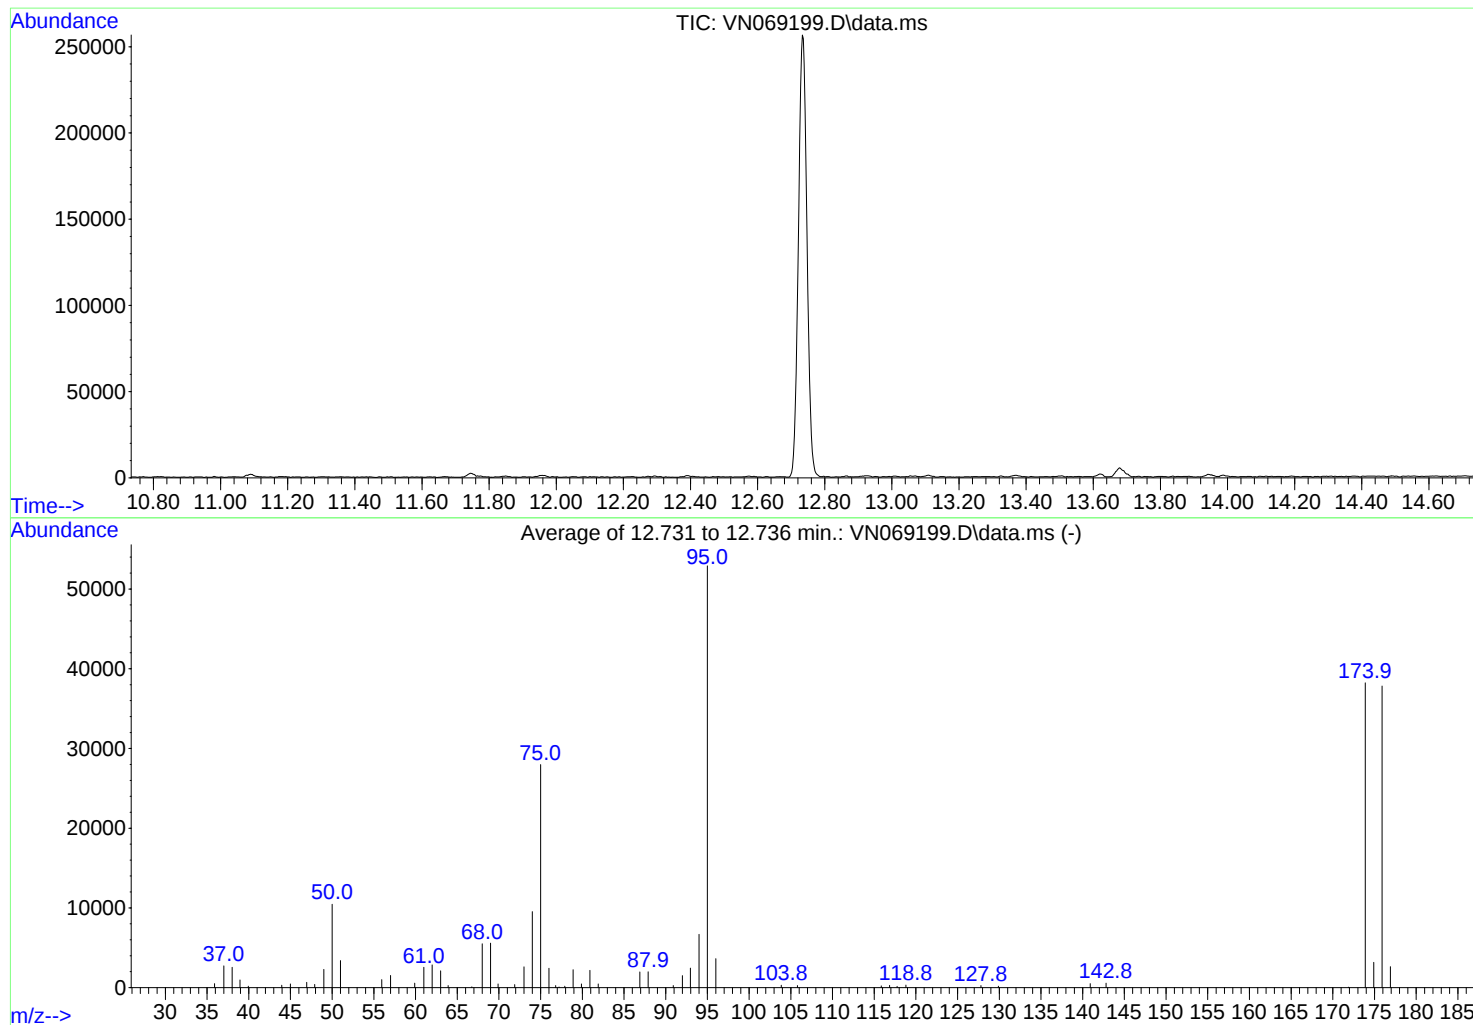

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	10454	PASS
75	95	30	60	52.9	27971	PASS
95	95	100	100	100.0	52909	PASS
96	95	5	9	6.9	3638	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.3	38227	PASS
175	174	5	9	8.3	3171	PASS
176	174	95	101	99.0	37843	PASS
177	176	5	9	7.0	2636	PASS