
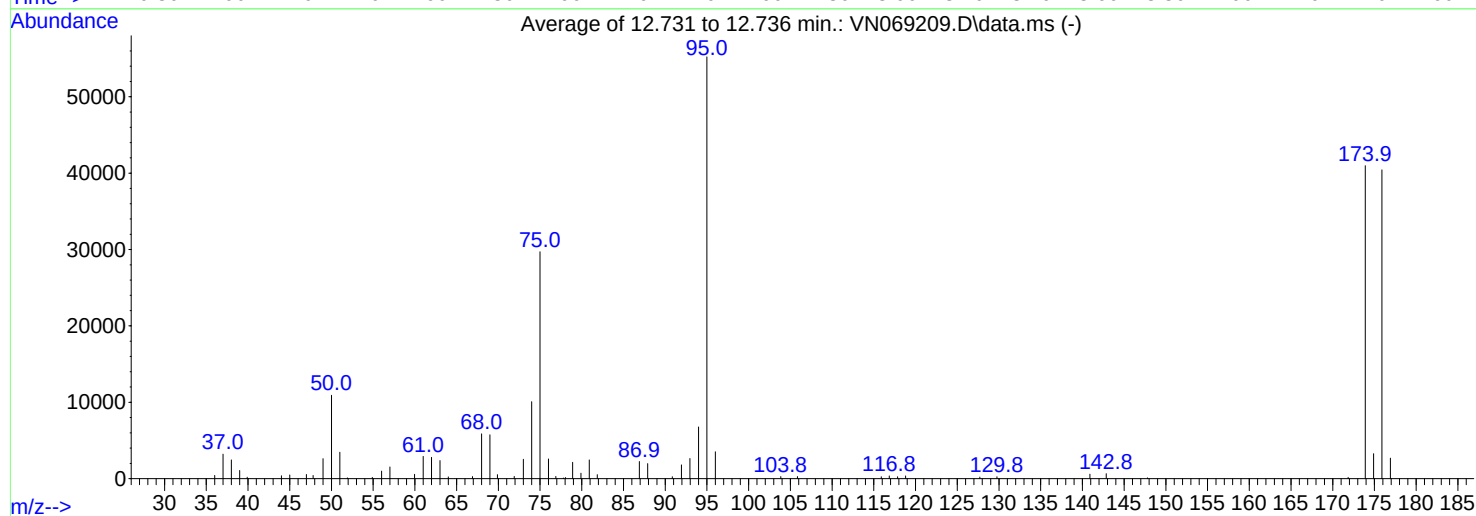


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102721\
 Data File : VN069209.D
 Acq On : 27 Oct 2021 9:30
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
 Title : SW846 8260
 Last Update : Wed Oct 13 05:44:40 2021

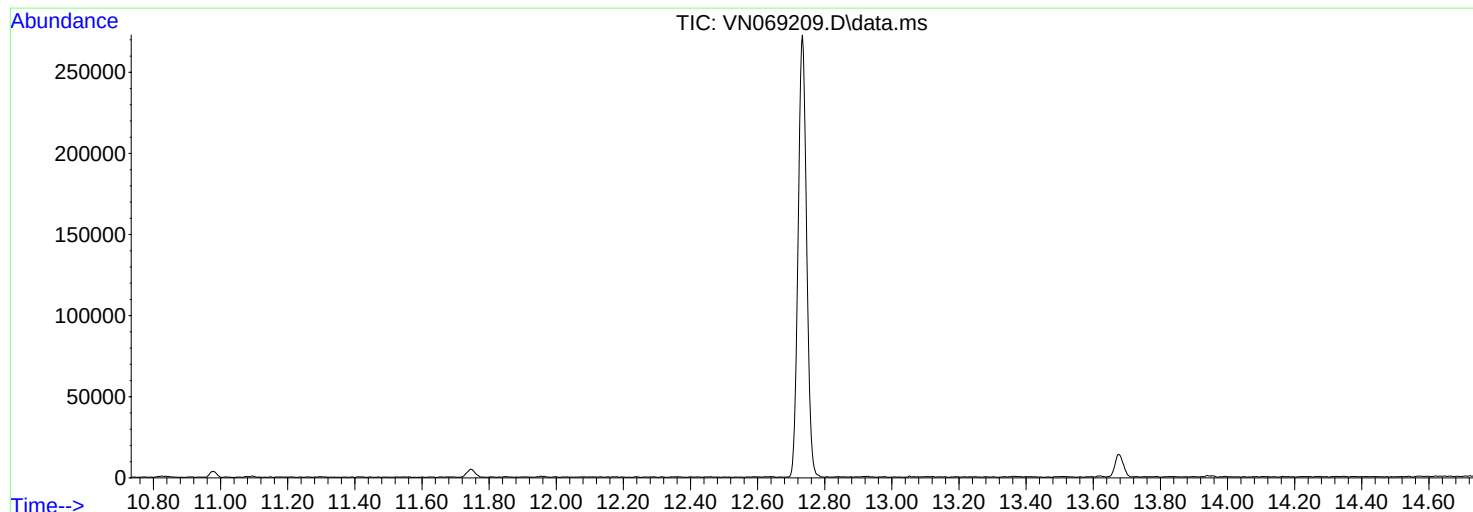

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	10922	PASS
75	95	30	60	53.8	29712	PASS
95	95	100	100	100.0	55229	PASS
96	95	5	9	6.4	3524	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.2	40981	PASS
175	174	5	9	8.0	3270	PASS
176	174	95	101	98.7	40432	PASS
177	176	5	9	6.6	2682	PASS