

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN102722\  
 Data File : VN075042.D  
 Acq On : 27 Oct 2022 15:43  
 Operator : JC\MD  
 Sample : N5284-02  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 MH-1-WC

Quant Time: Oct 28 02:14:51 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N102622W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Oct 27 09:48:49 2022  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response            | Conc      | Units  | Dev(Min) |
|-------------------------------|----------------|------|---------------------|-----------|--------|----------|
| -----                         |                |      |                     |           |        |          |
| Internal Standards            |                |      |                     |           |        |          |
| 1) Pentafluorobenzene         | 8.230          | 168  | 121245              | 50.000    | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 9.106          | 114  | 246523              | 50.000    | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.865         | 117  | 226348              | 50.000    | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.794         | 152  | 93520               | 50.000    | ug/l   | 0.00     |
|                               |                |      |                     |           |        |          |
| System Monitoring Compounds   |                |      |                     |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 8.583          | 65   | 101886              | 62.368    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 74 - 125 |      | Recovery = 124.740% |           |        |          |
| 35) Dibromofluoromethane      | 8.171          | 113  | 78890               | 54.512    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = 109.020% |           |        |          |
| 50) Toluene-d8                | 10.571         | 98   | 309508              | 55.124    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 86 - 113 |      | Recovery = 110.240% |           |        |          |
| 62) 4-Bromofluorobenzene      | 12.853         | 95   | 98605               | 49.993    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 83 - 123 |      | Recovery = 99.980%  |           |        |          |
|                               |                |      |                     |           |        |          |
| Target Compounds              |                |      |                     |           |        | Qvalue   |
| 5) Bromomethane               | 2.889          | 94   | 74                  | Below Cal | #      | 5        |
| 6) Chloroethane               | 2.830          | 64   | 22687               | 13.238    | ug/l # | 58       |
| 11) Tert butyl alcohol        | 5.518          | 59   | 199                 | 0.522     | ug/l # | 72       |
| 14) Allyl chloride            | 5.289          | 41   | 12757               | 6.796     | ug/l # | 19       |
| 16) Acetone                   | 4.453          | 43   | 15175               | 21.938    | ug/l   | 100      |
| 18) Methyl Acetate            | 5.042          | 43   | 2405                | 1.064     | ug/l # | 65       |
| 20) Methylene Chloride        | 5.283          | 84   | 584095              | 378.718   | ug/l   | 95       |
| 25) 2-Butanone                | 7.483          | 43   | 976                 | 0.897     | ug/l # | 43       |
| 30) Chloroform                | 7.971          | 83   | 3204                | 1.126     | ug/l   | 90       |
| 31) Cyclohexane               | 8.230          | 56   | 3157                | 1.299     | ug/l # | 55       |
| 36) 1,1-Dichloropropene       | 8.224          | 75   | 10688               | 4.770     | ug/l # | 49       |
| 37) Ethyl Acetate             | 7.577          | 43   | 7395                | 3.010     | ug/l # | 86       |
| 38) Carbon Tetrachloride      | 8.230          | 117  | 13320               | 5.405     | ug/l # | 16       |
| 43) Isopropyl Acetate         | 8.694          | 43   | 43562               | 11.429    | ug/l # | 77       |
| 47) Bromodichloromethane      | 9.888          | 83   | 1590                | 0.646     | ug/l # | 93       |
| 48) Methyl methacrylate       | 9.677          | 41   | 1050                | 0.601     | ug/l # | 32       |
| 51) 4-Methyl-2-Pentanone      | 10.441         | 43   | 1870                | 0.760     | ug/l # | 75       |
| 54) cis-1,3-Dichloropropene   | 10.359         | 75   | 8851                | 3.210     | ug/l # | 68       |
| 57) 1,3-Dichloropropane       | 11.200         | 76   | 1322                | 0.437     | ug/l # | 42       |
| 59) 2-Hexanone                | 11.171         | 43   | 19451               | 10.420    | ug/l # | 21       |
| 60) Dibromochloromethane      | 11.365         | 129  | 646                 | 0.337     | ug/l   | 81       |
| 71) Bromoform                 | 12.841         | 173  | 687                 | 0.512     | ug/l # | 1        |
| 74) N-amyl acetate            | 12.306         | 43   | 5149                | 1.854     | ug/l # | 44       |
| 76) 1,2,3-Trichloropropane    | 12.853         | 75   | 55193               | 27.796    | ug/l # | 1        |
| 81) trans-1,4-Dichloro-2-b... | 12.853         | 75   | 55193               | 71.351    | ug/l # | 10       |
| 95) Naphthalene               | 15.647         | 128  | 10158               | 1.908     | ug/l   | 99       |
| -----                         |                |      |                     |           |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN102722\  
Data File : VN075042.D  
Acq On : 27 Oct 2022 15:43  
Operator : JC\MD  
Sample : N5284-02  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC

Quant Time: Oct 28 02:14:51 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N102622W.M  
Quant Title : SW846 8260  
QLast Update : Thu Oct 27 09:48:49 2022  
Response via : Initial Calibration




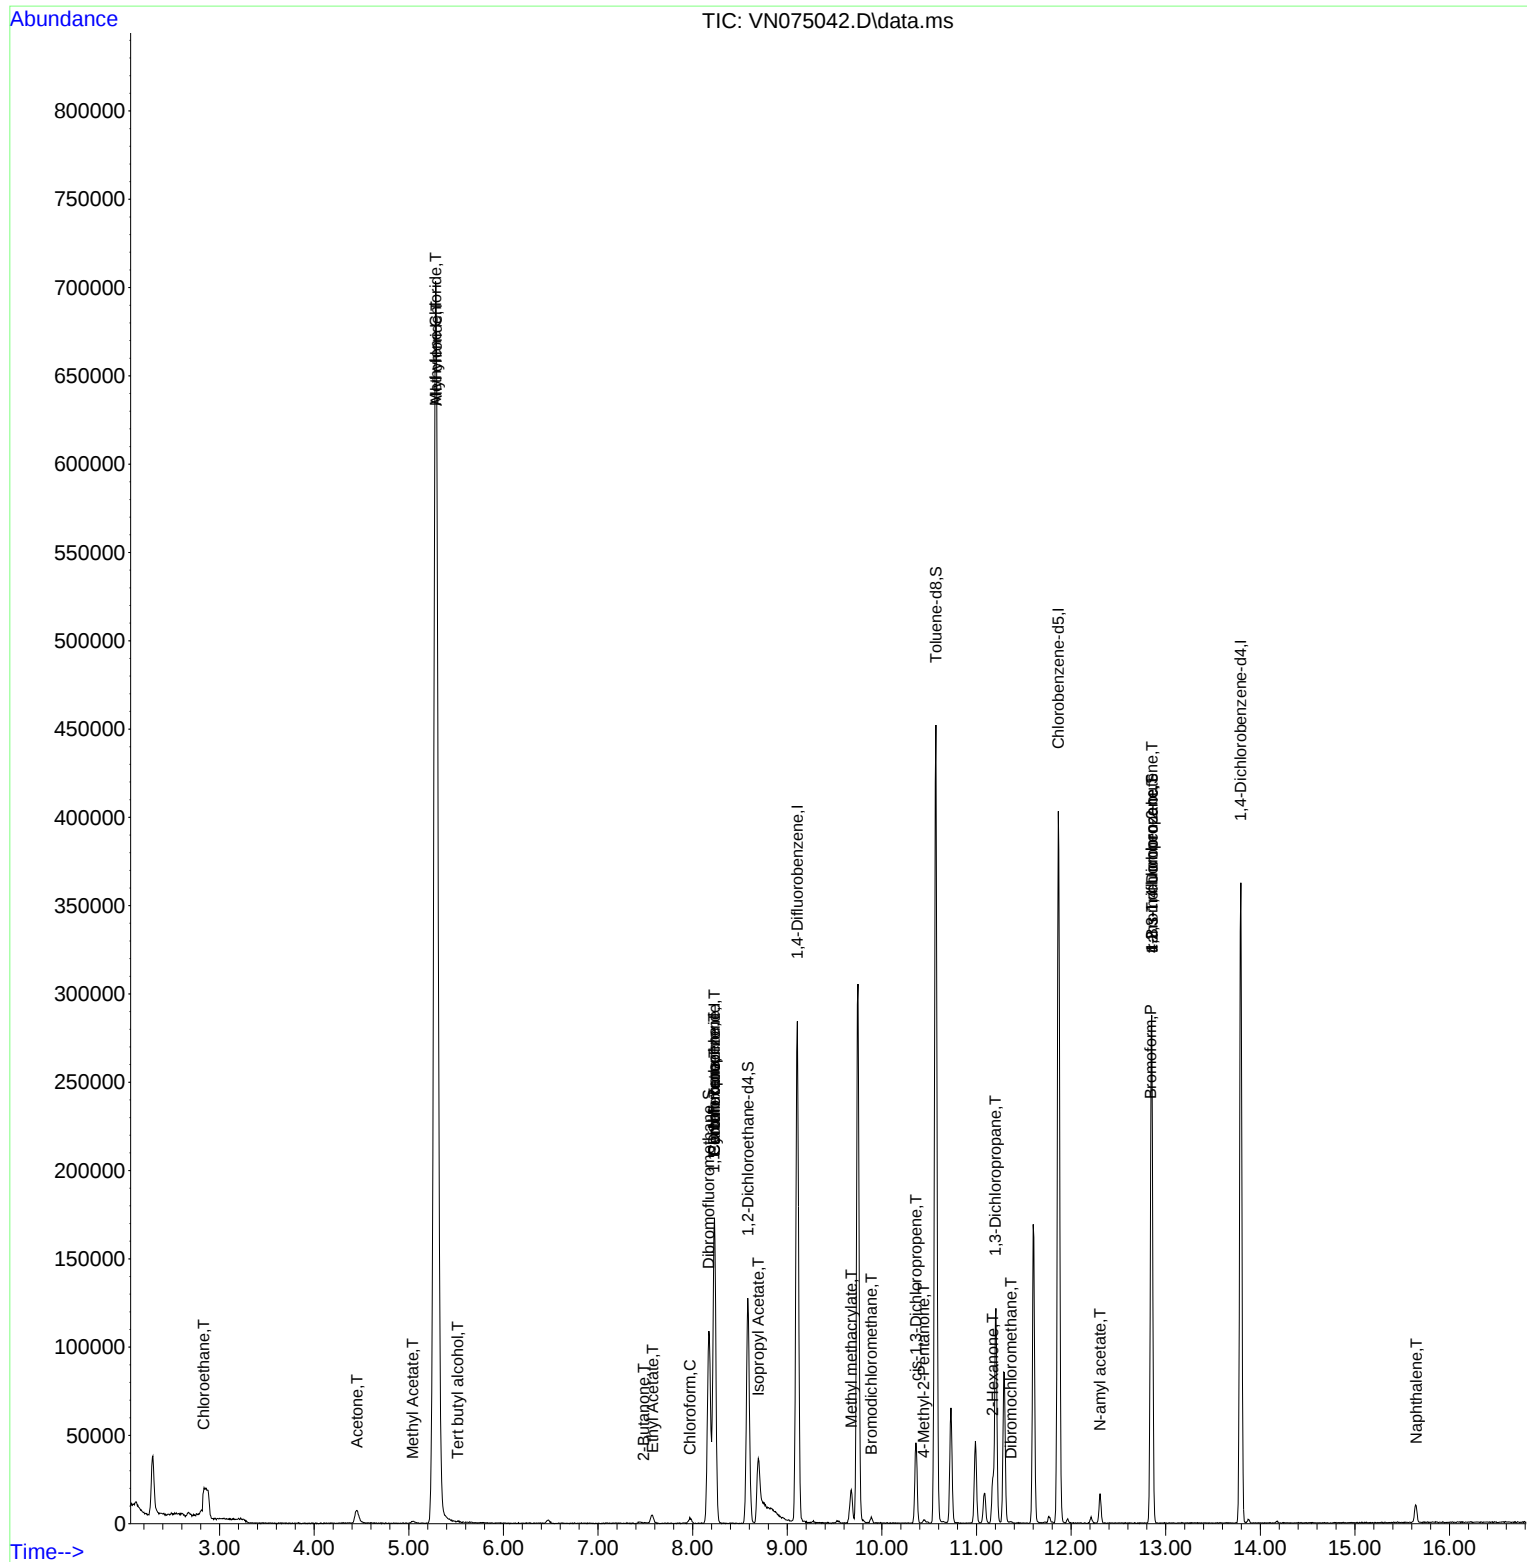


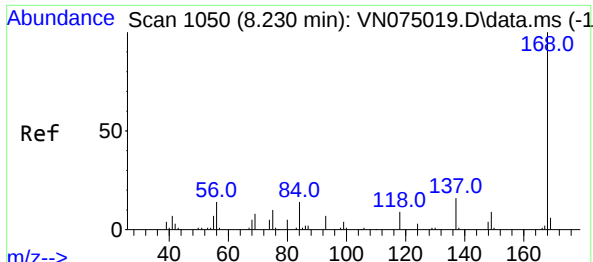

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.230 min Scan# 11  
Delta R.T. -0.000 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


Tgt Ion:168 Resp: 121245  
Ion Ratio Lower Upper  
168 100  
99 62.9 51.6 77.4

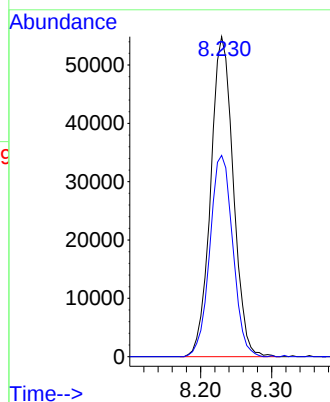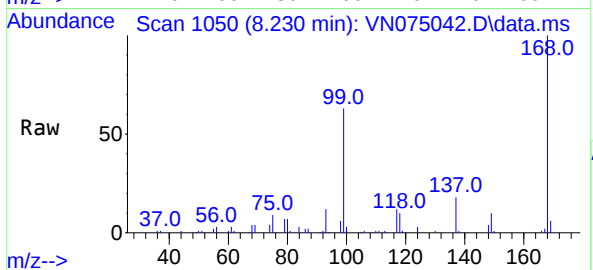

#5  
Bromomethane  
Concen: Below Cal  
RT: 2.889 min Scan# 142  
Delta R.T. -0.029 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Tgt Ion: 94 Resp: 74  
Ion Ratio Lower Upper  
94 100  
96 0.0 71.8 107.6#


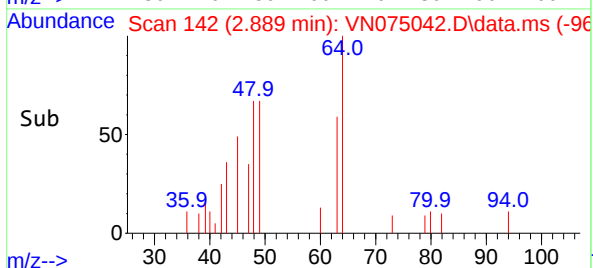

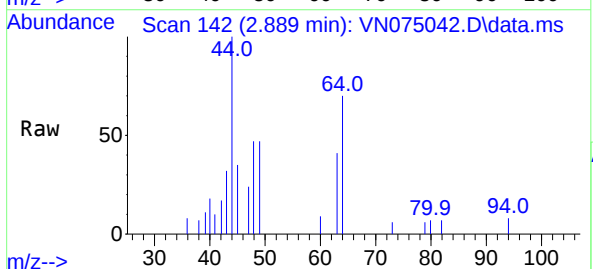




#6  
Chloroethane  
Concen: 13.238 ug/l  
RT: 2.830 min Scan# 11  
Delta R.T. -0.265 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


Tgt Ion: 64 Resp: 22687  
Ion Ratio Lower Upper  
64 100  
66 7.1 23.8 35.8#



#11  
Tert butyl alcohol  
Concen: 0.522 ug/l  
RT: 5.518 min Scan# 589  
Delta R.T. -0.024 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Tgt Ion: 59 Resp: 199  
Ion Ratio Lower Upper  
59 100  
57 0.0 8.5 12.7#




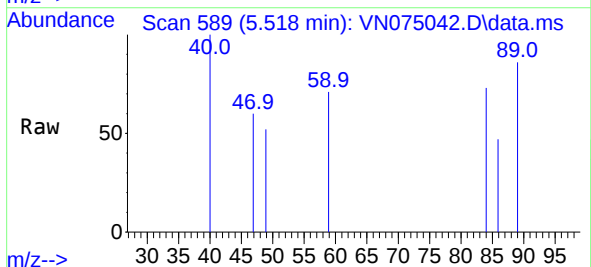


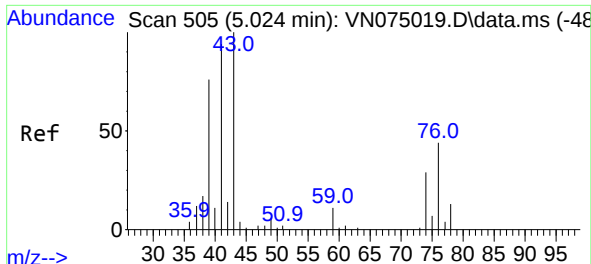

#14  
 Allyl chloride  
 Concen: 6.796 ug/l  
 RT: 5.289 min Scan# 511  
 Delta R.T. 0.265 min  
 Lab File: VN075042.D  
 Acq: 27 Oct 2022 15:43




Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 MH-1-WC


Tgt Ion: 41 Resp: 12757  
 Ion Ratio Lower Upper  
 41 100  
 39 0.0 61.0 91.4#  
 76 0.0 33.4 50.0#



#16  
 Acetone  
 Concen: 21.938 ug/l  
 RT: 4.453 min Scan# 408  
 Delta R.T. 0.011 min  
 Lab File: VN075042.D  
 Acq: 27 Oct 2022 15:43

Tgt Ion: 43 Resp: 15175  
 Ion Ratio Lower Upper  
 43 100  
 58 31.7 25.5 38.3


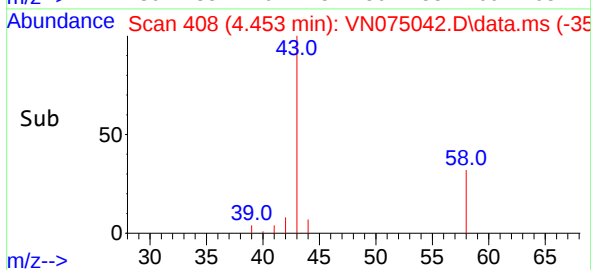

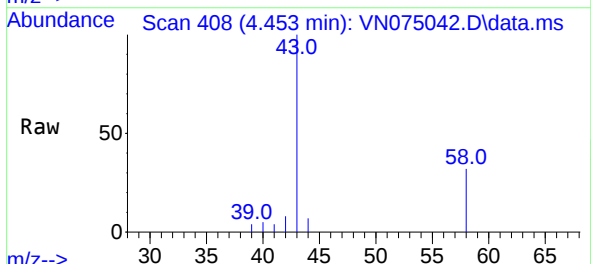




#18  
Methyl Acetate  
Concen: 1.064 ug/l  
RT: 5.042 min Scan# 508  
Delta R.T. -0.000 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


Tgt Ion: 43 Resp: 2405  
Ion Ratio Lower Upper  
43 100  
74 9.0 22.0 33.0#

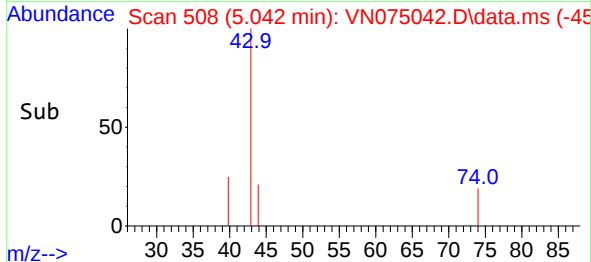

#20  
Methylene Chloride  
Concen: 378.718 ug/l  
RT: 5.283 min Scan# 549  
Delta R.T. -0.000 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Tgt Ion: 84 Resp: 584095  
Ion Ratio Lower Upper  
84 100  
49 112.7 94.9 142.3  
51 34.0 26.8 40.2  
86 62.1 53.7 80.5


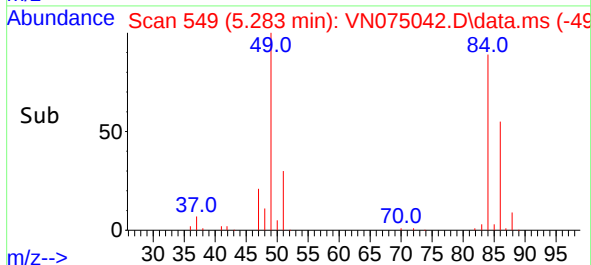
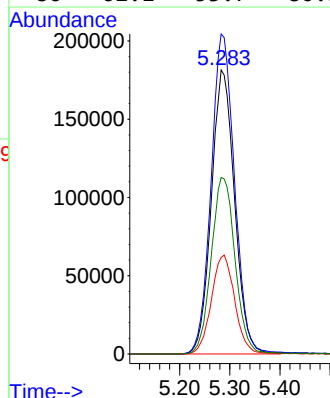
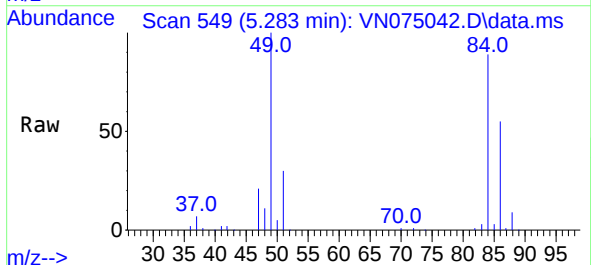




#25  
2-Butanone  
Concen: 0.897 ug/l  
RT: 7.483 min Scan# 91  
Delta R.T. -0.011 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


Tgt Ion: 43 Resp: 976  
Ion Ratio Lower Upper  
43 100  
72 0.0 25.5 38.3#

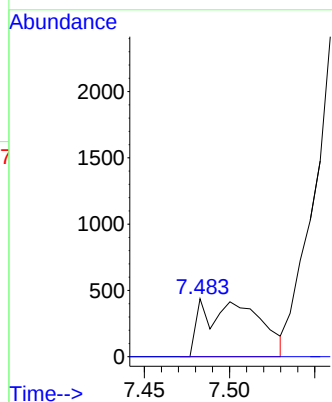

#30  
Chloroform  
Concen: 1.126 ug/l  
RT: 7.971 min Scan# 1006  
Delta R.T. -0.000 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Tgt Ion: 83 Resp: 3204  
Ion Ratio Lower Upper  
83 100  
85 71.8 51.4 77.0


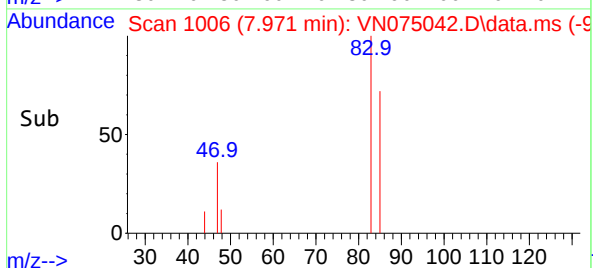






#31  
Cyclohexane  
Concen: 1.299 ug/l  
RT: 8.230 min Scan# 1050  
Delta R.T. -0.029 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


Tgt Ion: 56 Resp: 3157  
Ion Ratio Lower Upper  
56 100  
69 121.5 25.2 37.8#  
84 104.3 77.8 116.8

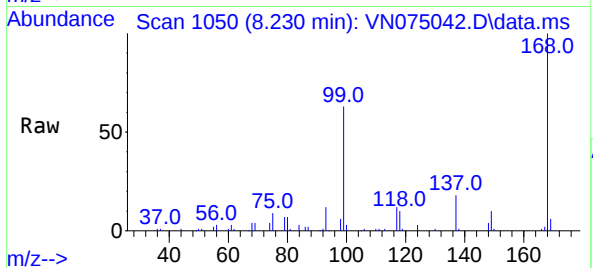

#33  
1,2-Dichloroethane-d4  
Concen: 62.368 ug/l  
RT: 8.583 min Scan# 1110  
Delta R.T. -0.005 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Tgt Ion: 65 Resp: 101886  
Ion Ratio Lower Upper  
65 100  
67 52.1 0.0 102.0


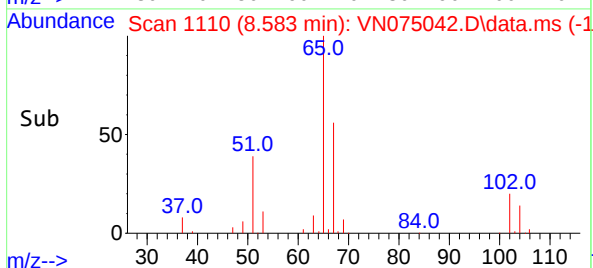
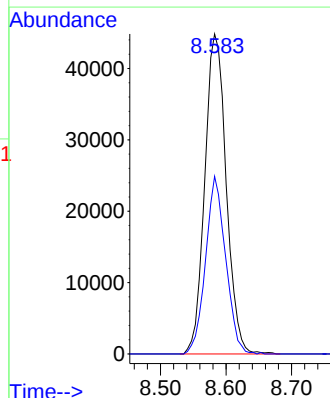





#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 9.106 min Scan# 1199  
Delta R.T. 0.000 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


Tgt Ion:114 Resp: 246523  
Ion Ratio Lower Upper  
114 100  
63 19.4 0.0 39.6  
88 15.3 0.0 29.0

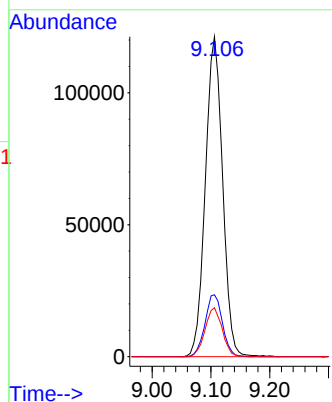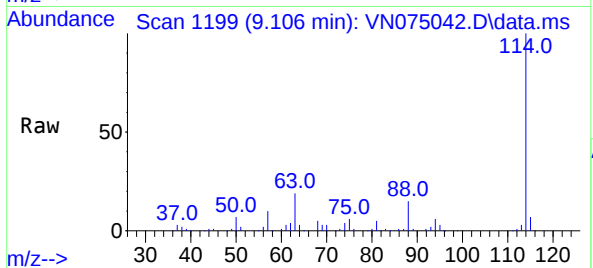

#35  
Dibromofluoromethane  
Concen: 54.512 ug/l  
RT: 8.171 min Scan# 1040  
Delta R.T. -0.000 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Tgt Ion:113 Resp: 78890  
Ion Ratio Lower Upper  
113 100  
111 101.3 80.5 120.7  
192 16.1 13.2 19.8


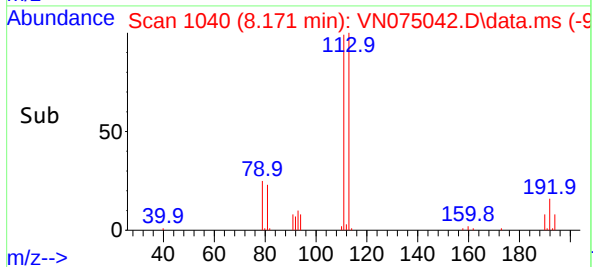
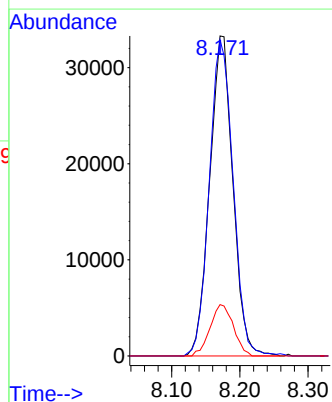
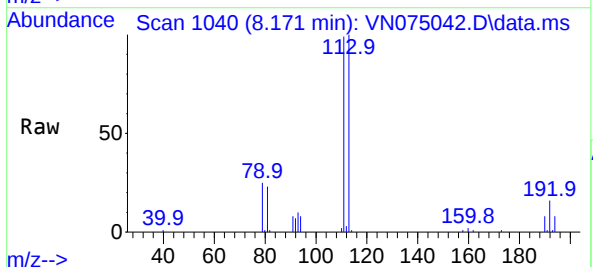




#36  
1,1-Dichloropropene  
Concen: 4.770 ug/l  
RT: 8.224 min Scan# 1049  
Delta R.T. -0.153 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


Tgt Ion: 75 Resp: 10688  
Ion Ratio Lower Upper  
75 100  
110 8.2 17.8 53.3#  
77 0.0 24.6 37.0#

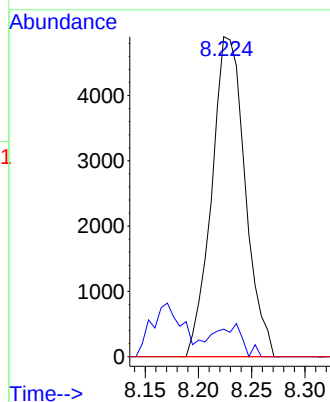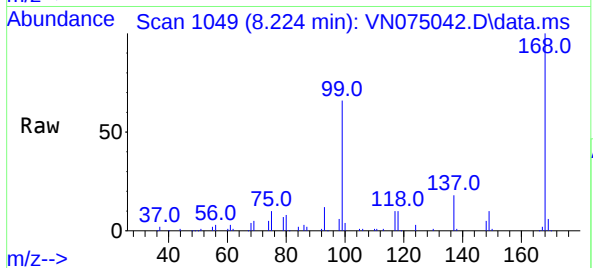

#37  
Ethyl Acetate  
Concen: 3.010 ug/l  
RT: 7.577 min Scan# 939  
Delta R.T. 0.006 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43


Tgt Ion: 43 Resp: 7395  
Ion Ratio Lower Upper  
43 100  
61 7.3 12.2 18.4#  
70 8.7 9.4 14.2#

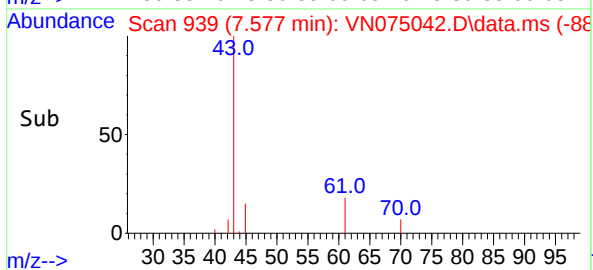






#38  
Carbon Tetrachloride  
Concen: 5.405 ug/l  
RT: 8.230 min Scan# 1107  
Delta R.T. -0.141 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43


Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC

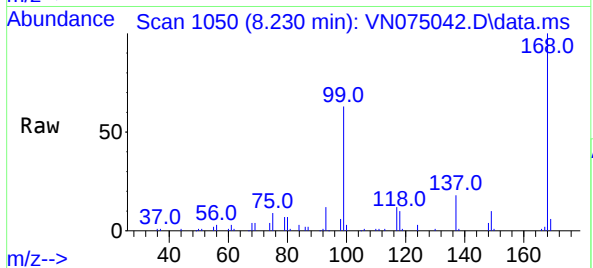



Tgt Ion:117 Resp: 13320  
Ion Ratio Lower Upper  
117 100  
119 5.5 76.7 115.1#  
121 0.0 23.9 35.9#




#43  
Isopropyl Acetate  
Concen: 11.429 ug/l  
RT: 8.694 min Scan# 1129  
Delta R.T. 0.000 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43



Tgt Ion: 43 Resp: 43562  
Ion Ratio Lower Upper  
43 100  
61 13.9 22.4 33.6#  
87 9.2 12.5 18.7#



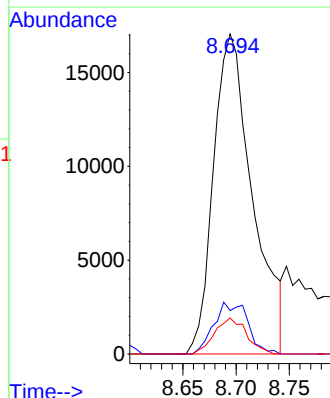
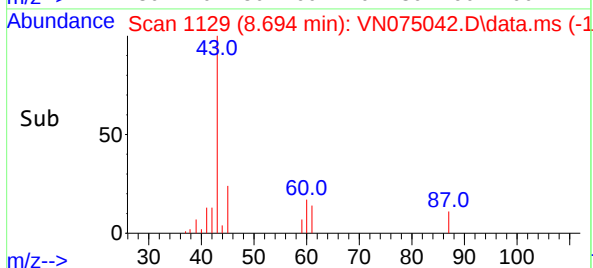




#47  
Bromodichloromethane  
Concen: 0.646 ug/l  
RT: 9.888 min Scan# 11  
Delta R.T. -0.006 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


Tgt Ion: 83 Resp: 1590  
Ion Ratio Lower Upper  
83 100  
85 68.9 52.1 78.1  
127 0.0 6.6 10.0#

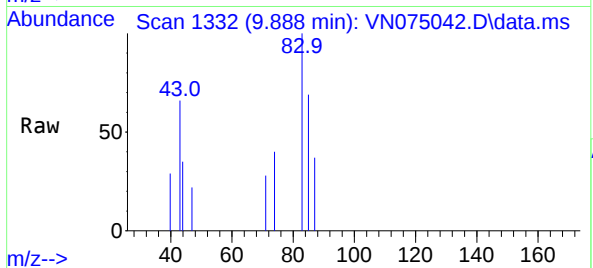

#48  
Methyl methacrylate  
Concen: 0.601 ug/l  
RT: 9.677 min Scan# 1296  
Delta R.T. -0.005 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Tgt Ion: 41 Resp: 1050  
Ion Ratio Lower Upper  
41 100  
69 0.0 80.2 120.2#  
39 52.0 56.2 84.2#


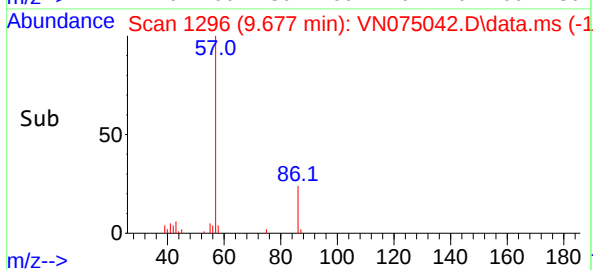






#50  
Toluene-d8  
Concen: 55.124 ug/l  
RT: 10.571 min Scan# 1448  
Delta R.T. -0.000 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


Tgt Ion: 98 Resp: 309508  
Ion Ratio Lower Upper  
98 100  
100 64.6 53.0 79.6

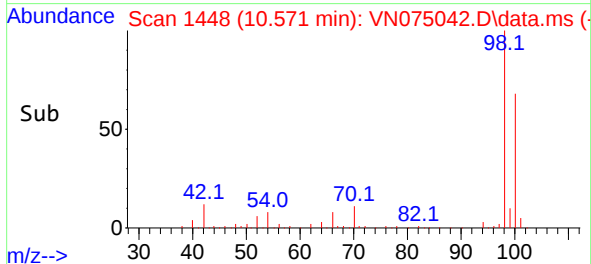

#51  
4-Methyl-2-Pentanone  
Concen: 0.760 ug/l  
RT: 10.441 min Scan# 1426  
Delta R.T. -0.006 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Tgt Ion: 43 Resp: 1870  
Ion Ratio Lower Upper  
43 100  
58 25.9 33.6 50.4#


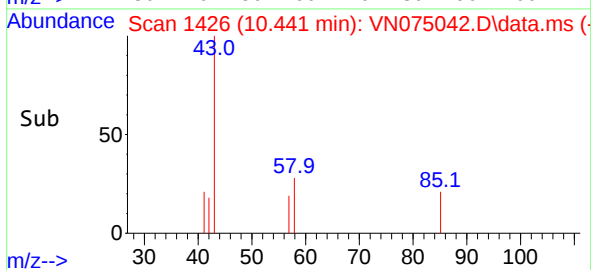

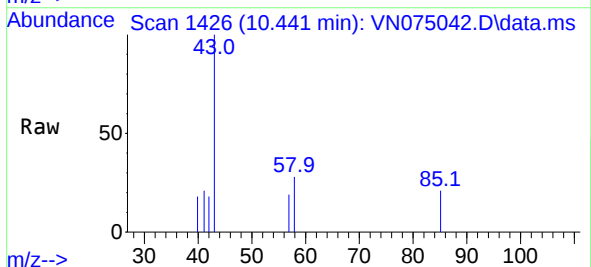




#54  
cis-1,3-Dichloropropene  
Concen: 3.210 ug/l  
RT: 10.359 min Scan# 1405  
Delta R.T. 0.041 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


Tgt Ion: 75 Resp: 8851  
Ion Ratio Lower Upper  
75 100  
77 0.0 23.7 35.5#  
39 33.3 35.8 53.6#

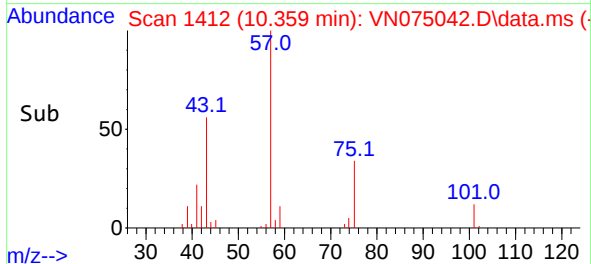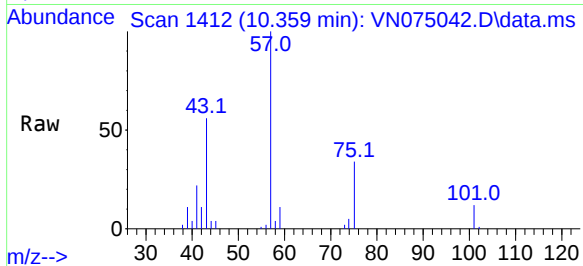

#57  
1,3-Dichloropropane  
Concen: 0.437 ug/l  
RT: 11.200 min Scan# 1555  
Delta R.T. 0.035 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Tgt Ion: 76 Resp: 1322  
Ion Ratio Lower Upper  
76 100  
78 0.0 25.8 38.6#



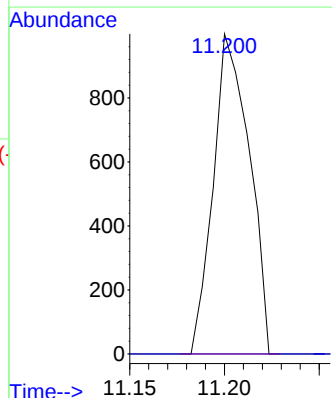
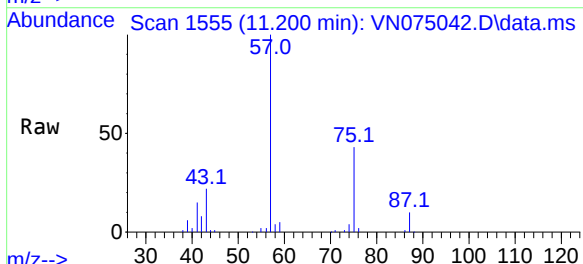




#59  
2-Hexanone  
Concen: 10.420 ug/l  
RT: 11.171 min Scan# 11  
Delta R.T. -0.029 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


Tgt Ion: 43 Resp: 19451  
Ion Ratio Lower Upper  
43 100  
58 0.0 29.6 88.8#

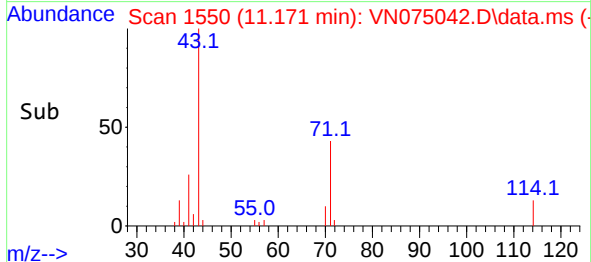

#60  
Dibromochloromethane  
Concen: 0.337 ug/l  
RT: 11.365 min Scan# 1583  
Delta R.T. 0.006 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Tgt Ion:129 Resp: 646  
Ion Ratio Lower Upper  
129 100  
127 60.5 38.6 115.8



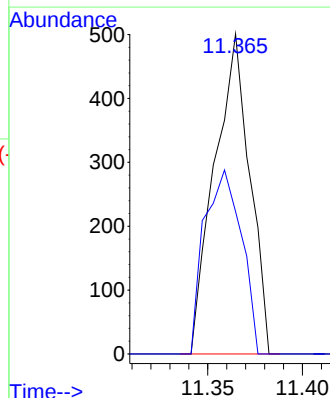
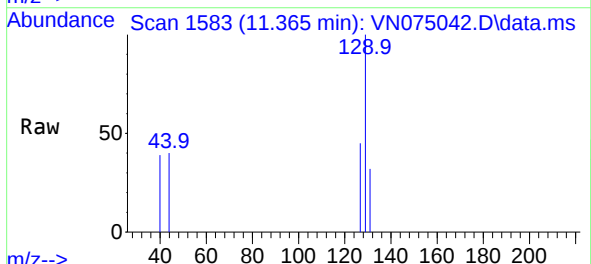




#62  
4-Bromofluorobenzene  
Concen: 49.993 ug/l  
RT: 12.853 min Scan# 11  
Delta R.T. -0.000 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


Tgt Ion: 95 Resp: 98605  
Ion Ratio Lower Upper  
95 100  
174 75.1 0.0 147.4  
176 71.3 0.0 142.2

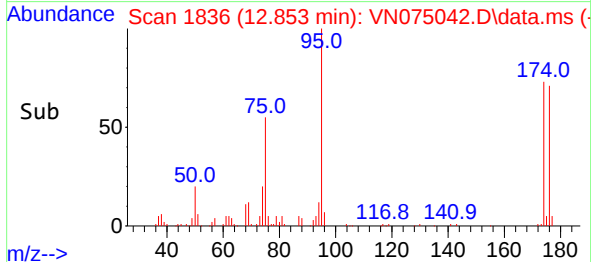

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.865 min Scan# 1668  
Delta R.T. -0.006 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Tgt Ion: 117 Resp: 226348  
Ion Ratio Lower Upper  
117 100  
82 56.5 43.1 64.7  
119 31.5 25.5 38.3


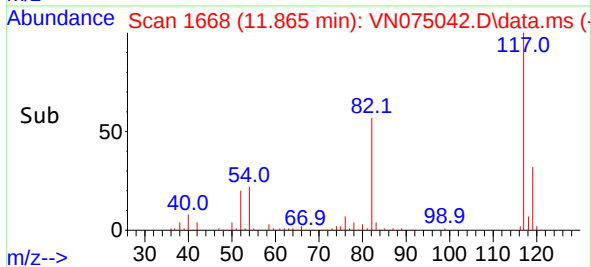

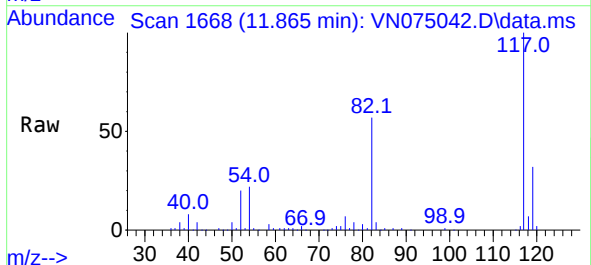




#71  
Bromoform  
Concen: 0.512 ug/l  
RT: 12.841 min Scan# 1834  
Delta R.T. 0.259 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


Tgt Ion:173 Resp: 687  
Ion Ratio Lower Upper  
173 100  
175 687.5 24.6 74.0#  
254 0.0 0.0 0.0

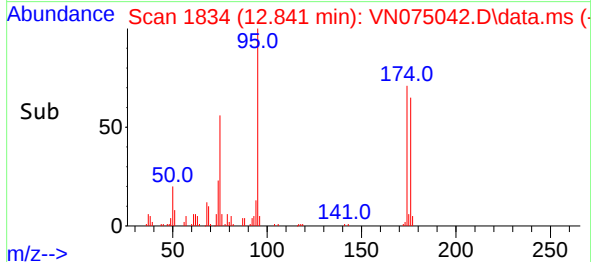

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.794 min Scan# 1996  
Delta R.T. -0.000 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Tgt Ion:152 Resp: 93520  
Ion Ratio Lower Upper  
152 100  
115 60.8 30.2 90.6  
150 153.8 0.0 348.4


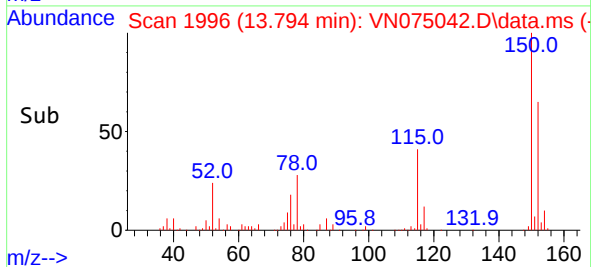

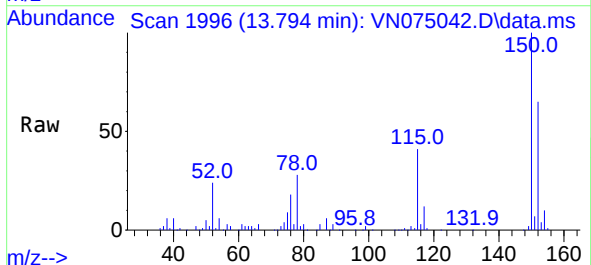




#74  
N-amy1 acetate  
Concen: 1.854 ug/l  
RT: 12.306 min Scan# 11  
Delta R.T. -0.188 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43




Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 43    | Resp: | 5149  |
| Ion      | Ratio | Lower | Upper |
| 43       | 100   |       |       |
| 70       | 1.3   | 39.8  | 59.8# |
| 55       | 2.1   | 19.9  | 29.9# |
| 61       | 6.6   | 21.7  | 32.5# |

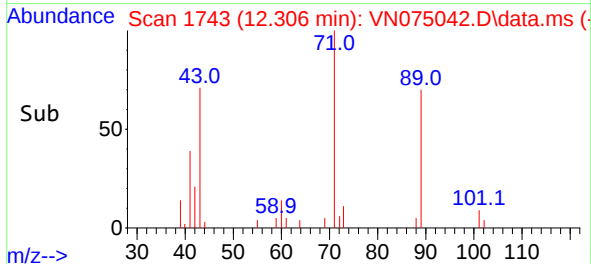

#76  
1,2,3-Trichloropropane  
Concen: 27.796 ug/l  
RT: 12.853 min Scan# 1836  
Delta R.T. -0.141 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 75    | Resp: | 55193  |
| Ion      | Ratio | Lower | Upper  |
| 75       | 100   |       |        |
| 77       | 0.7   | 75.6  | 226.8# |


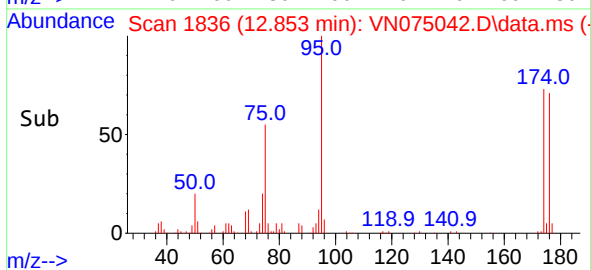

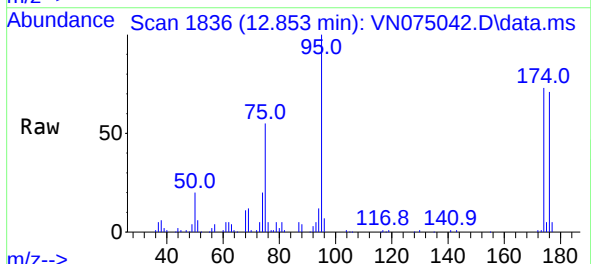




#81  
trans-1,4-Dichloro-2-butene  
Concen: 71.351 ug/l  
RT: 12.853 min Scan# 1836  
Delta R.T. 0.112 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Instrument :  
MSVOA\_N  
ClientSampleId :  
MH-1-WC

Tgt Ion: 75 Resp: 55193  
Ion Ratio Lower Upper  
75 100  
53 0.0 78.5 117.7#  
89 0.0 37.7 56.5#

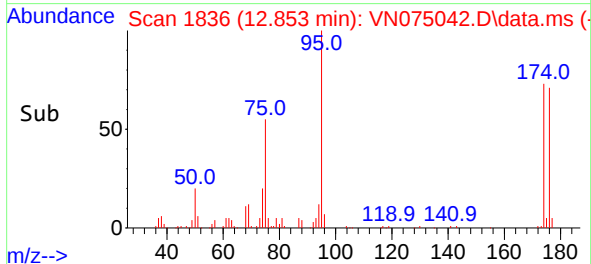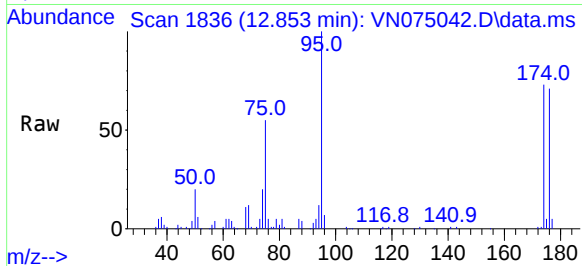

#95  
Naphthalene  
Concen: 1.908 ug/l  
RT: 15.647 min Scan# 2311  
Delta R.T. 0.006 min  
Lab File: VN075042.D  
Acq: 27 Oct 2022 15:43

Tgt Ion: 128 Resp: 10158  
Ion Ratio Lower Upper  
128 100  
127 13.1 10.4 15.6  
129 11.8 8.6 12.8

