

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102722\
 Data File : VN075046.D
 Acq On : 27 Oct 2022 17:19
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Oct 28 02:15:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 09:48:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	101232	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	186599	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	161476	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	66641	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	76427	56.032	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	112.060%
35) Dibromofluoromethane	8.171	113	58980	53.842	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	107.680%
50) Toluene-d8	10.571	98	230516	54.239	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	108.480%
62) 4-Bromofluorobenzene	12.853	95	71030	47.577	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.160%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102722\
Data File : VN075046.D
Acq On : 27 Oct 2022 17:19
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Oct 28 02:15:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 09:48:49 2022
Response via : Initial Calibration



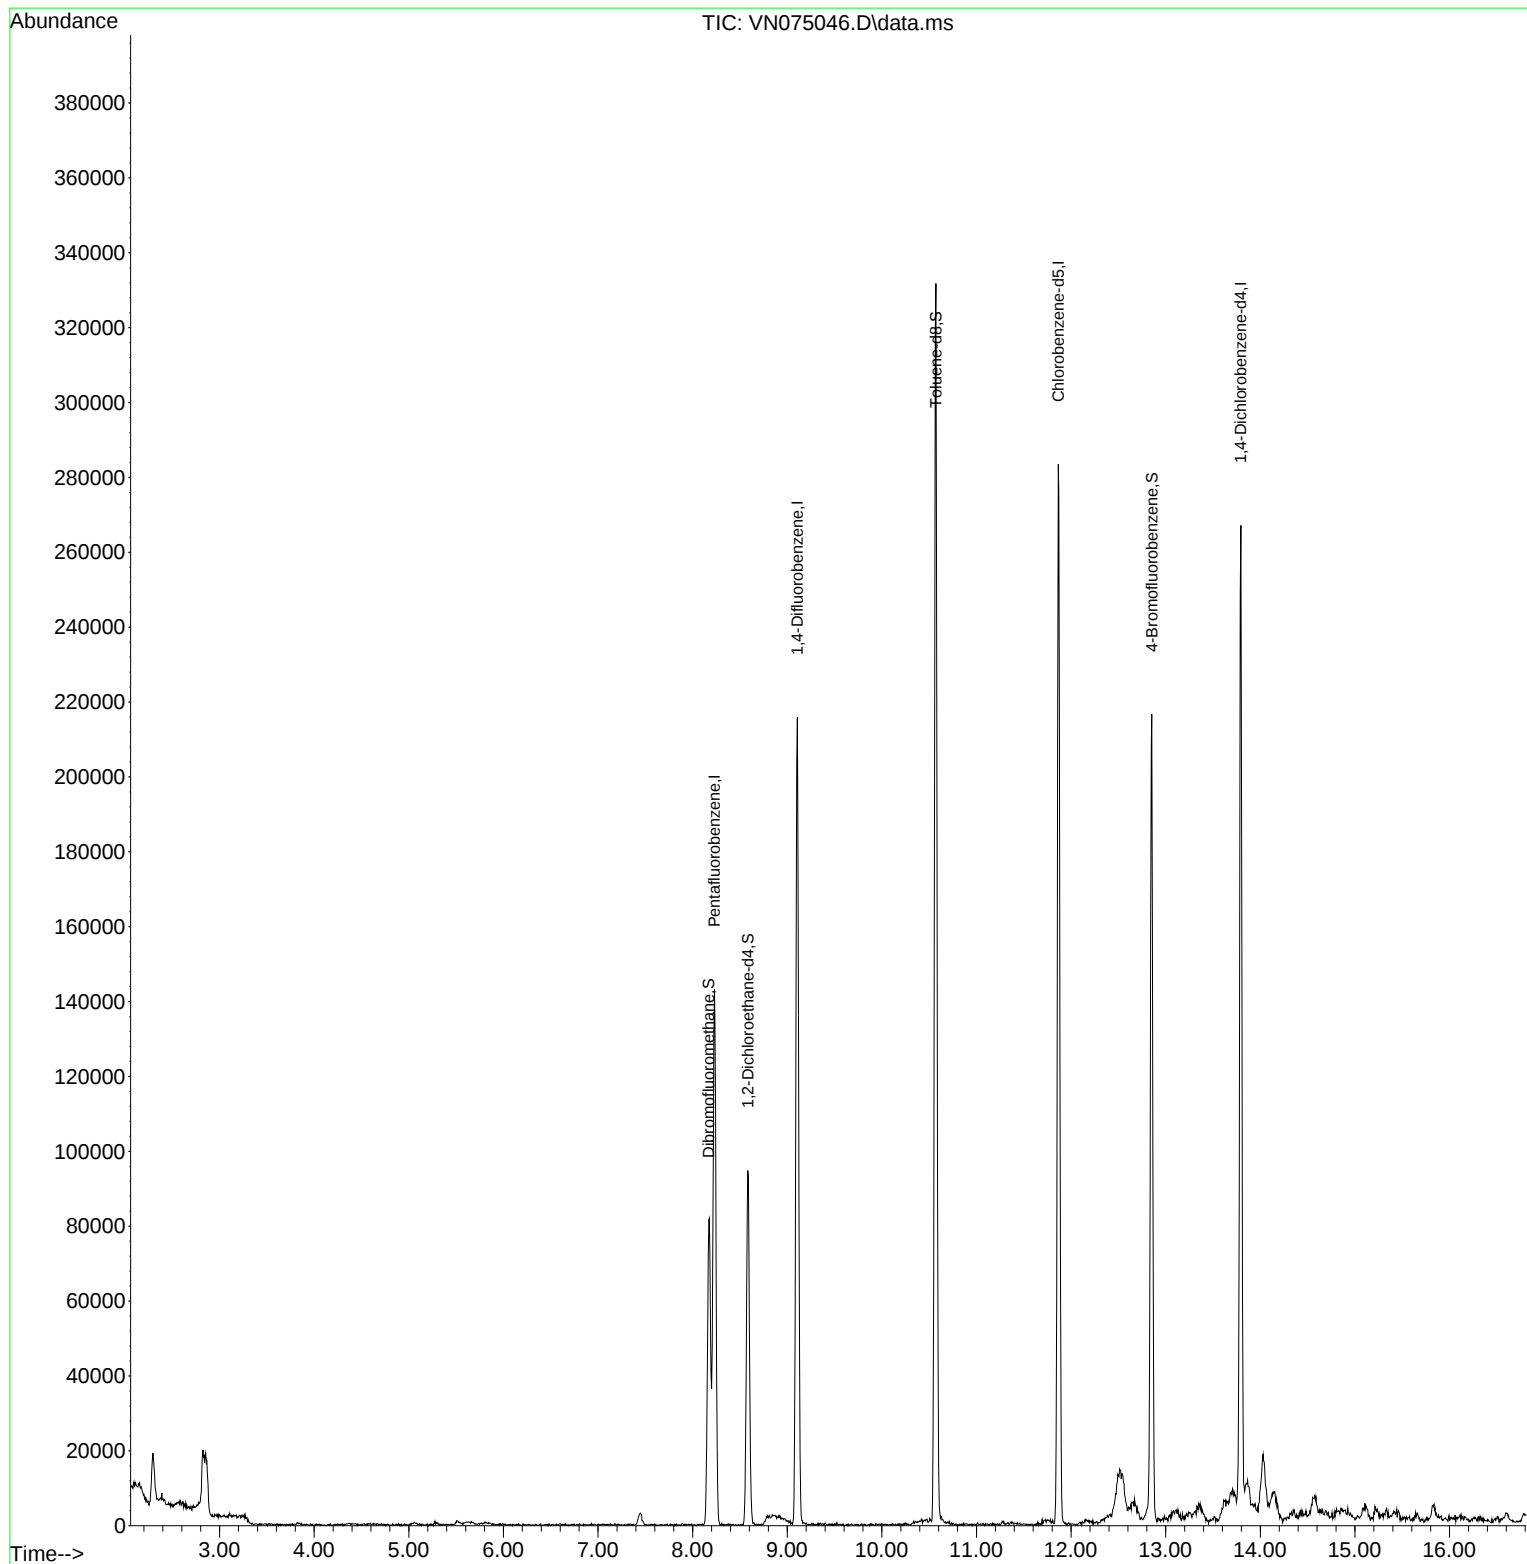




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 110
Delta R.T. -0.000 min
Lab File: VN075046.D
Acq: 27 Oct 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 101232
Ion Ratio Lower Upper
168 100
99 61.2 51.6 77.4

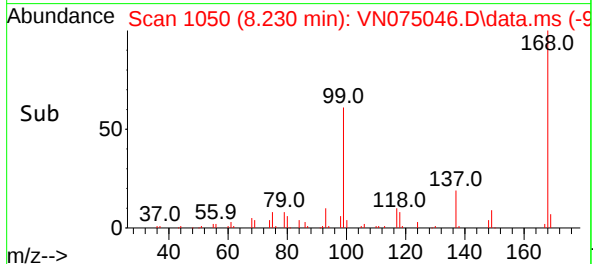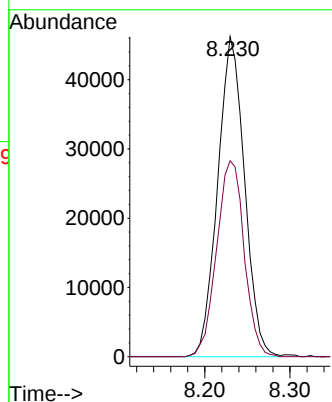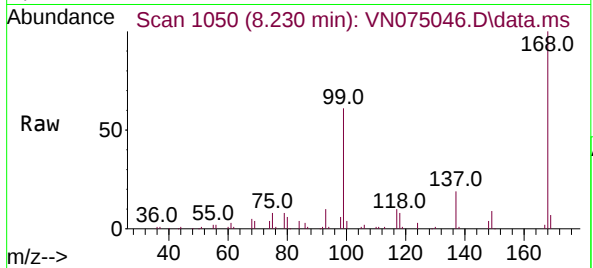

#33
1,2-Dichloroethane-d4
Concen: 56.032 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. -0.005 min
Lab File: VN075046.D
Acq: 27 Oct 2022 17:19

Tgt Ion: 65 Resp: 76427
Ion Ratio Lower Upper
65 100
67 51.7 0.0 102.0

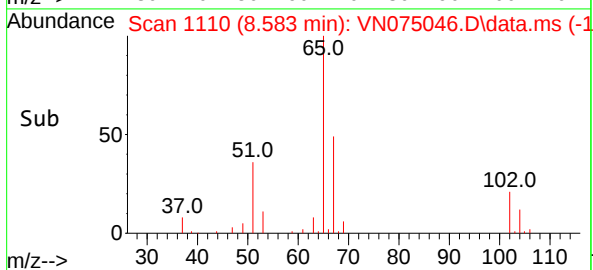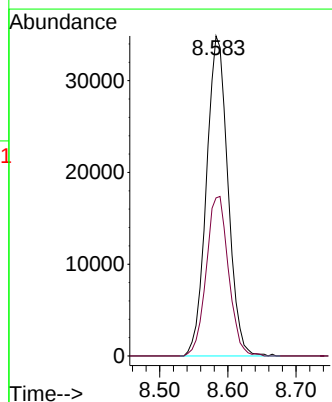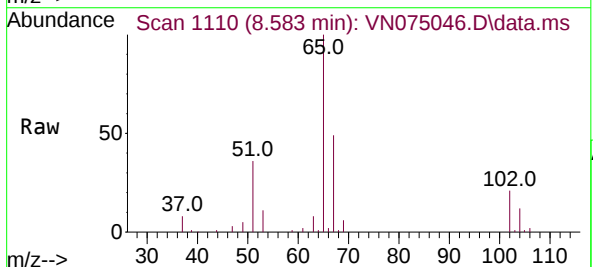

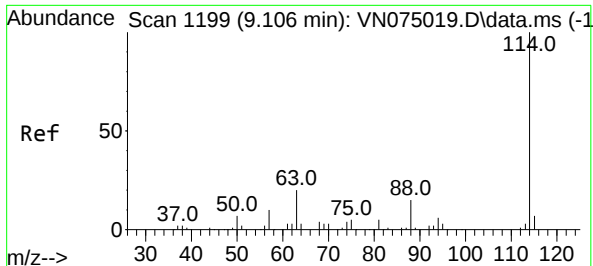

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN075046.D

Acq: 27 Oct 2022 17:19

Instrument :

MSVOA_N

ClientSampleId :

IBLK





Tgt Ion:114 Resp: 186599

Ion Ratio Lower Upper

114 100

63 18.0 0.0 39.6

88 14.6 0.0 29.0

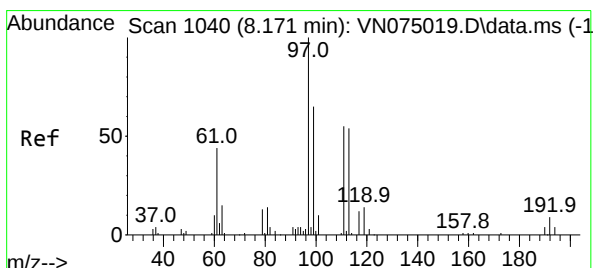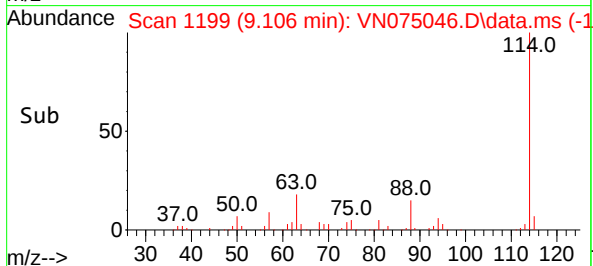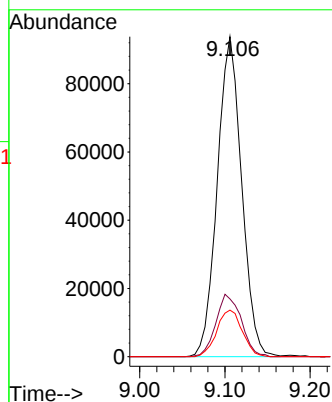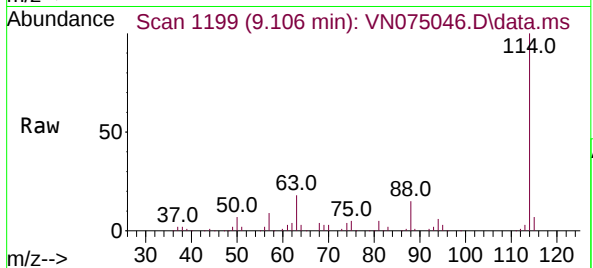

#35

Dibromofluoromethane

Concen: 53.842 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VN075046.D

Acq: 27 Oct 2022 17:19




Tgt Ion:113 Resp: 58980


Ion Ratio Lower Upper

113 100

111 102.6 80.5 120.7

192 16.2 13.2 19.8


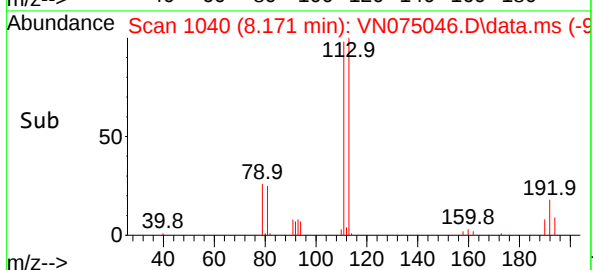
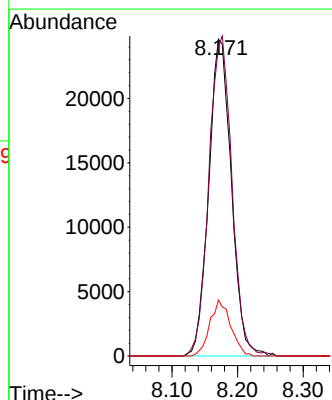
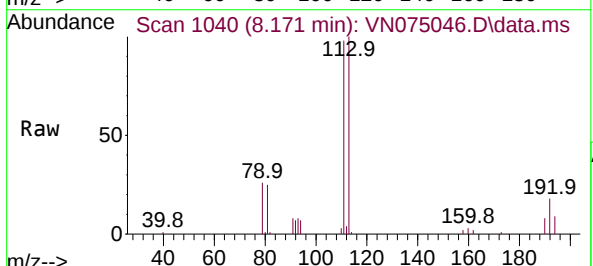


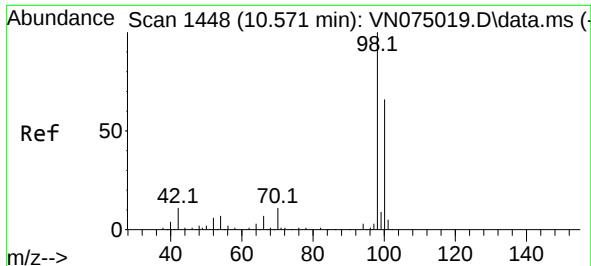

#50
Toluene-d8
Concen: 54.239 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN075046.D
Acq: 27 Oct 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 230516
Ion Ratio Lower Upper
98 100
100 65.2 53.0 79.6

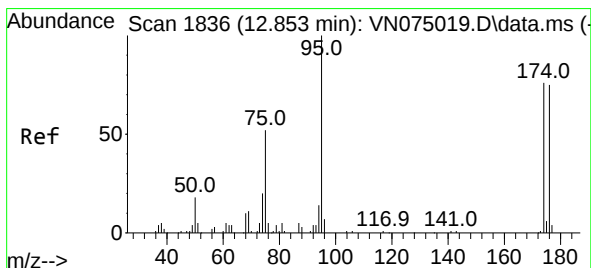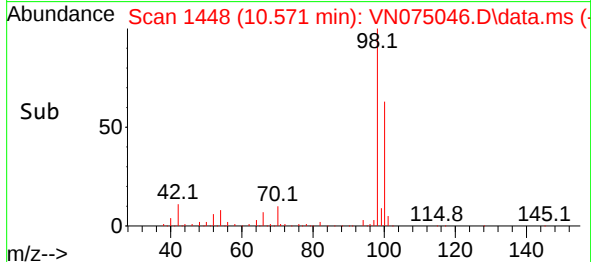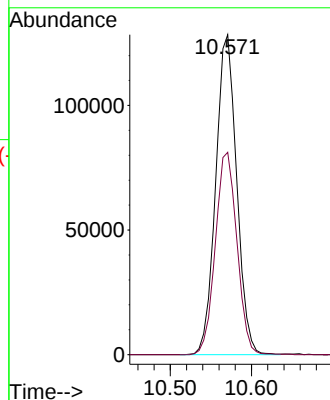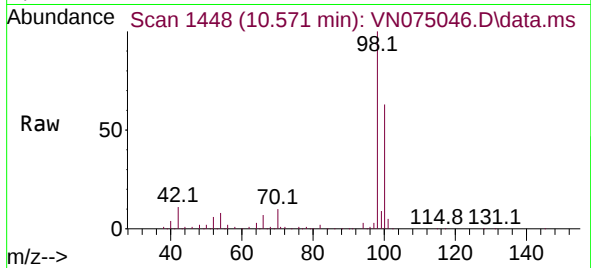

#62
4-Bromofluorobenzene
Concen: 47.577 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN075046.D
Acq: 27 Oct 2022 17:19

Tgt Ion: 95 Resp: 71030
Ion Ratio Lower Upper
95 100
174 75.6 0.0 147.4
176 70.6 0.0 142.2


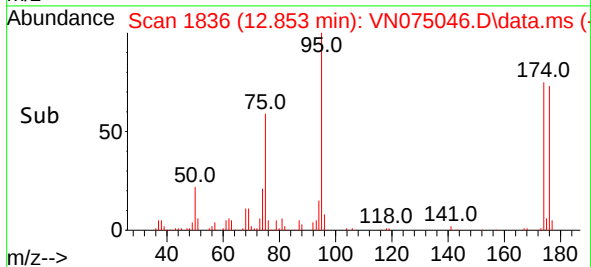
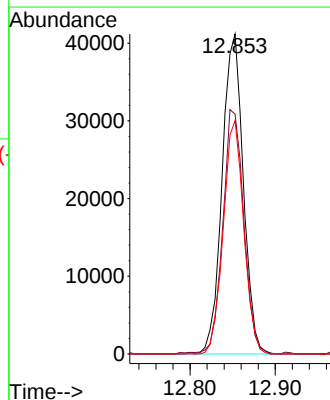
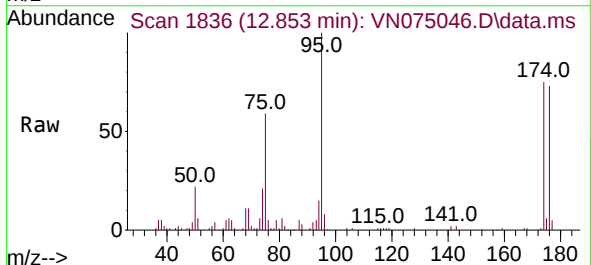


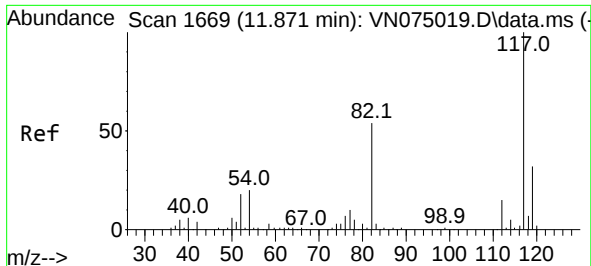

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN075046.D
Acq: 27 Oct 2022 17:19

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 161476
Ion Ratio Lower Upper
117 100
82 57.2 43.1 64.7
119 32.6 25.5 38.3

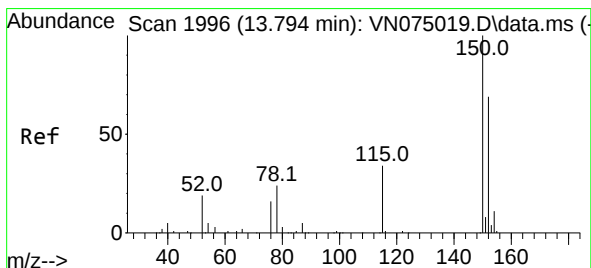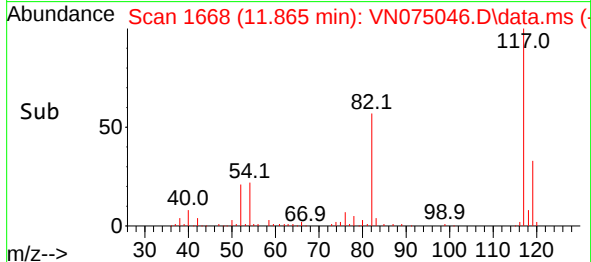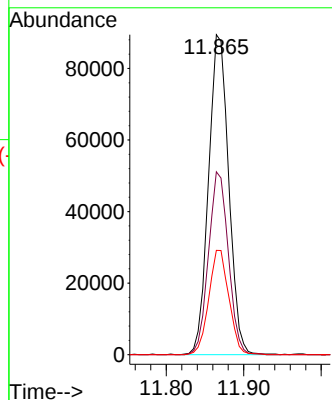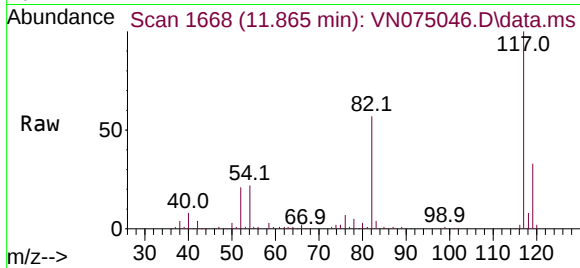

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN075046.D
Acq: 27 Oct 2022 17:19

Tgt Ion:152 Resp: 66641
Ion Ratio Lower Upper
152 100
115 62.6 30.2 90.6
150 158.8 0.0 348.4

