
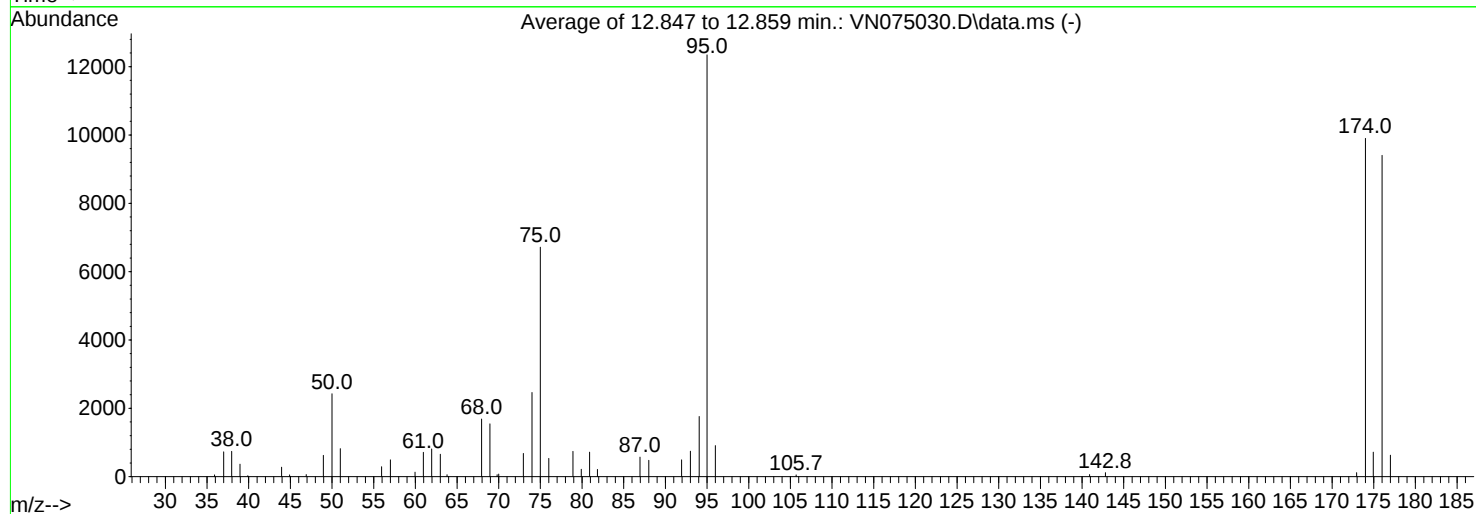


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102722\
Data File : VN075030.D
Acq On : 27 Oct 2022 09:06
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 09:48:49 2022

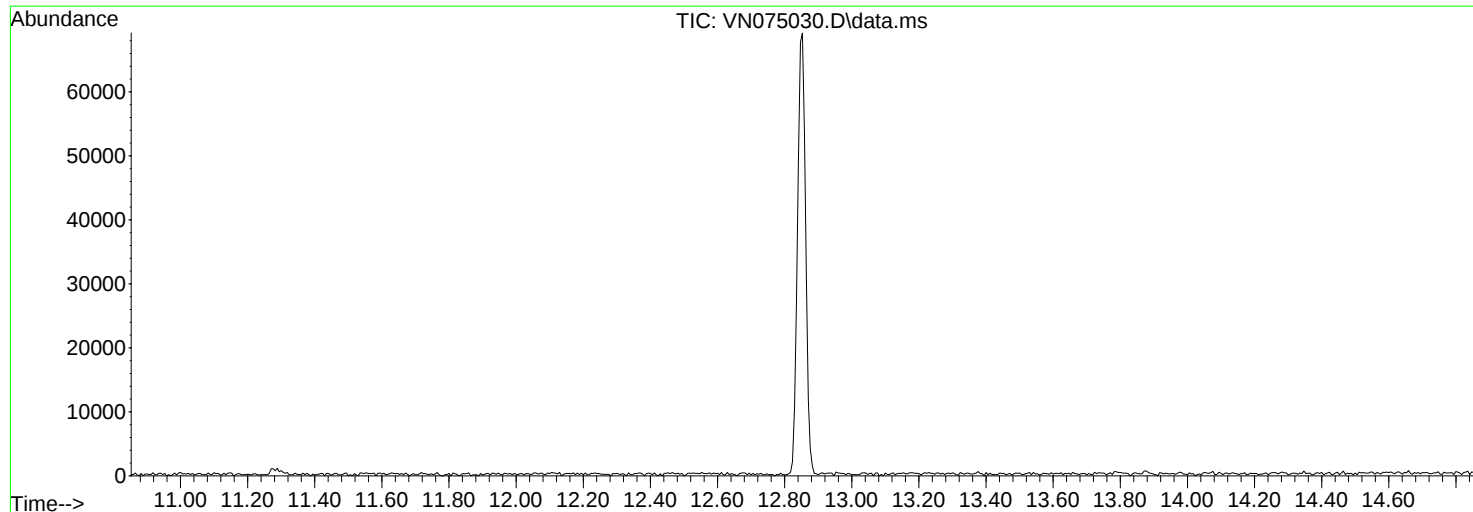

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	2428	PASS
75	95	30	60	54.4	6714	PASS
95	95	100	100	100.0	12347	PASS
96	95	5	9	7.4	909	PASS
173	174	0.00	2	1.2	115	PASS
174	95	50	100	80.2	9902	PASS
175	174	5	9	7.3	719	PASS
176	174	95	101	95.0	9406	PASS
177	176	5	9	6.7	630	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	54	55.95	291	72.95	677	93.00	740
37.00	728	57.00	492	74.00	2463	94.05	1761
37.95	741	59.95	131	75.00	6714	95.00	1234
38.95	364	60.95	711	76.00	534	96.00	905
39.90	29	61.95	812	78.90	738	105.70	54
43.95	277	63.00	655	79.90	217	140.90	59
44.90	52	63.80	57	80.90	715	142.80	117
46.90	63	67.95	1686	81.85	213	172.95	115
48.95	622	68.95	1548	86.95	572	174.00	9902
50.00	2428	69.80	57	88.00	479	174.95	719
51.00	822	70.00	73	91.95	493	176.00	9406

Average of 12.847 to 12.859 min.: VN075030.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
177.00	630						

Instrument :

MSVOA_N

ClientSampleId :

BFB