

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN102819\
 Data File : VN058986.D
 Acq On : 28 Oct 2019 10:53
 Operator : JC/SP
 Sample : VN1028WBL01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1028WBL01

Quant Time: Oct 29 13:43:00 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
 Quant Title : SW846 8260
 QLast Update : Sat Oct 19 00:16:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.65	168	394168	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	627831	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	560953	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	204352	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.01	65	290440	50.24	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.48%	
35) Dibromofluoromethane	7.57	113	211352	51.20	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.40%	
50) Toluene-d8	10.08	98	799813	49.91	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.82%	
62) 4-Bromofluorobenzene	12.40	95	254651	43.28	ug/l	0.00
Spiked Amount	50.000		Recovery	=	86.56%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN102819\
Data File : VN058986.D
Acq On : 28 Oct 2019 10:53
Operator : JC/SP
Sample : VN1028WBL01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1028WBL01

Quant Time: Oct 29 13:43:00 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Quant Title : SW846 8260
QLast Update : Sat Oct 19 00:16:20 2019
Response via : Initial Calibration

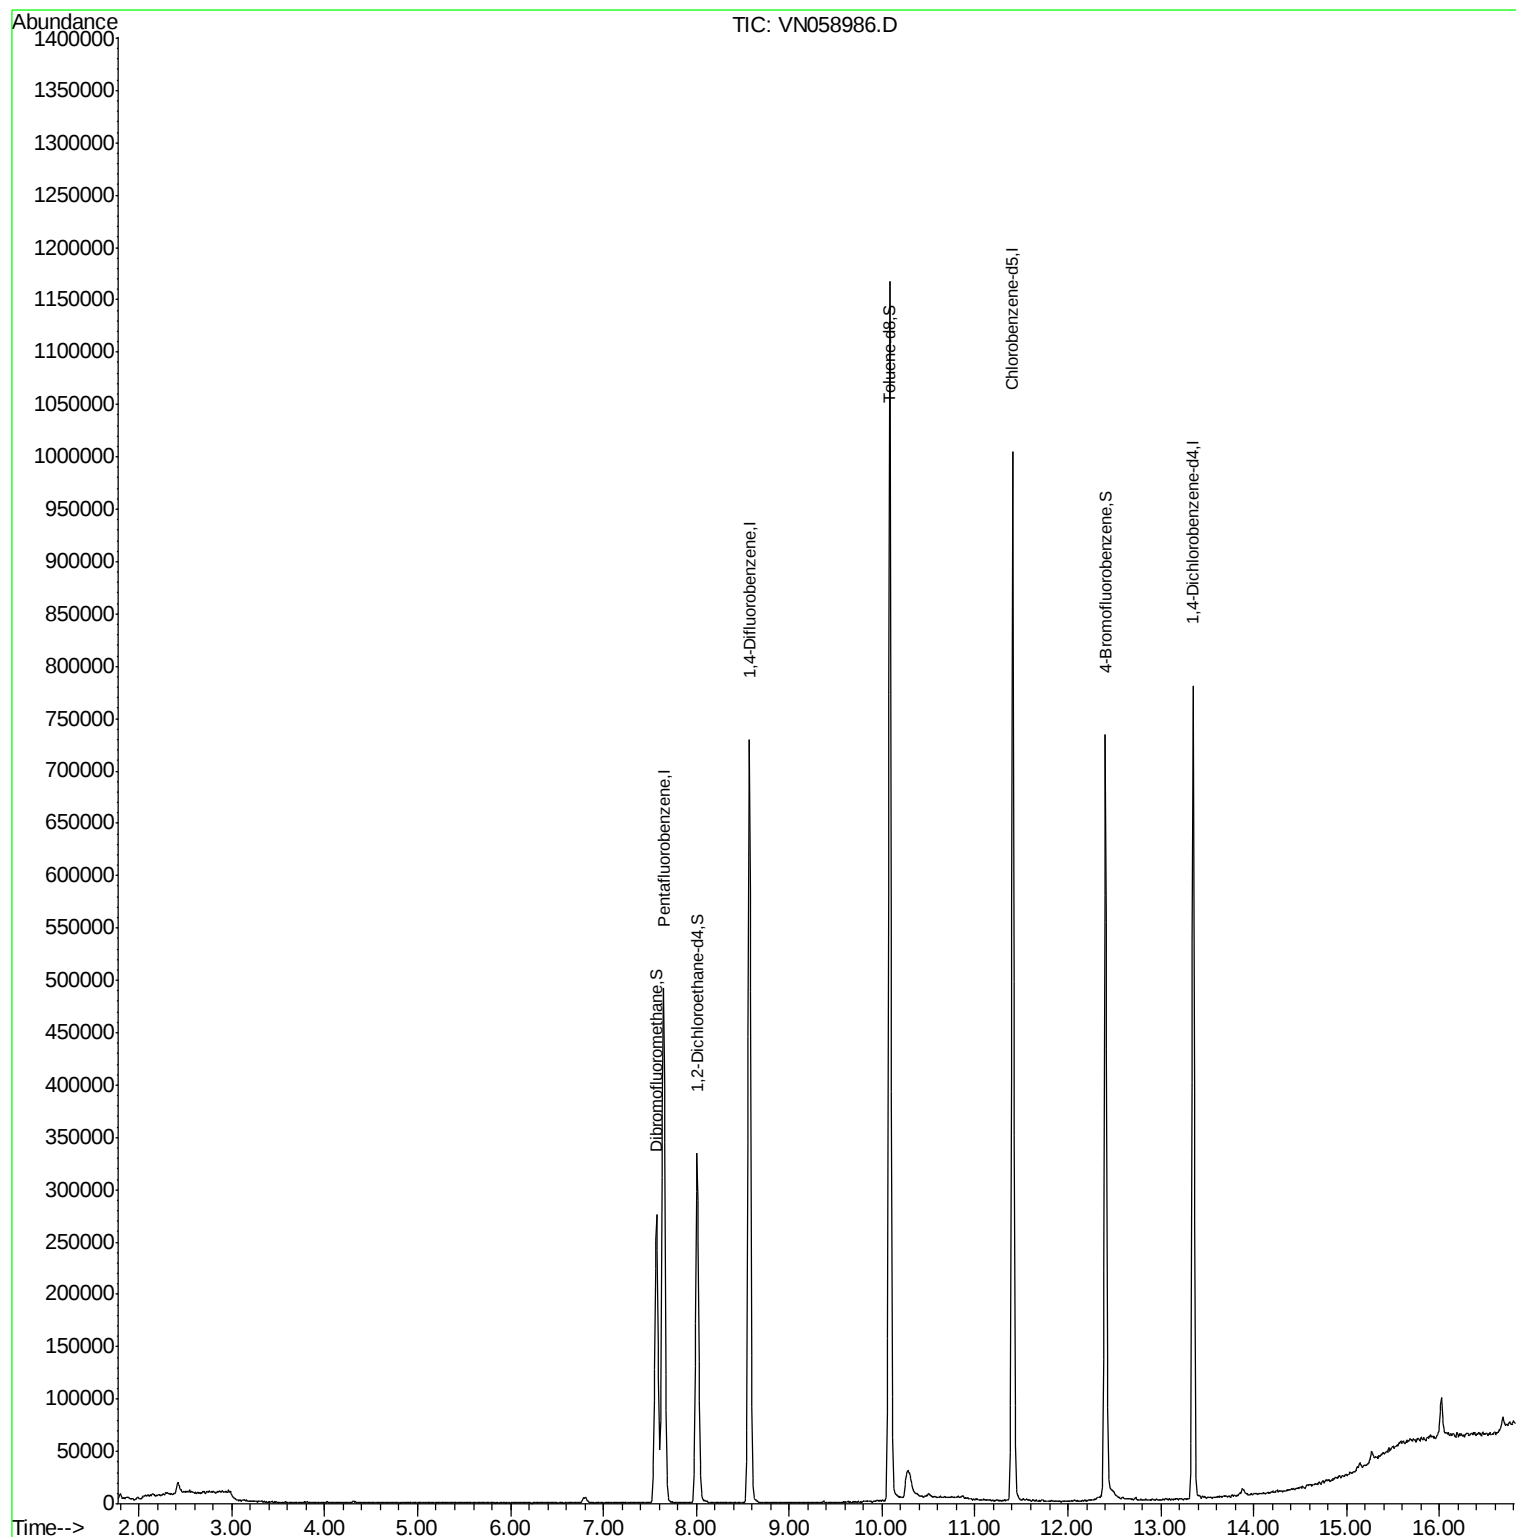



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.65 min Scan# 1827

Delta R.T. 0.00 min

Lab File: VN058986.D

Acq: 28 Oct 2019 10:53

Instrument :

MSVOA_N

ClientSampleId :


VN1028WBL01

Tot Ion:168 Resp: 394168

Ion Ratio Lower Upper

168 100

99 59.4 48.1 72.1

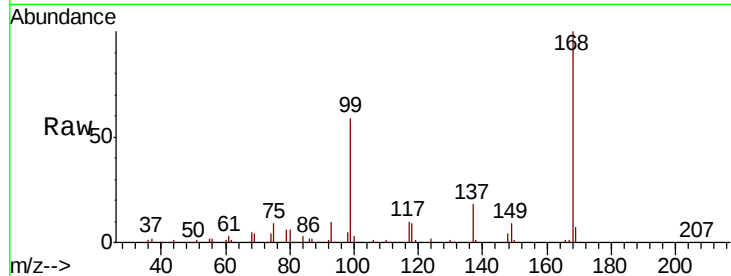

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.65

150000



100000

50000

0

7.60 7.70

Time-->

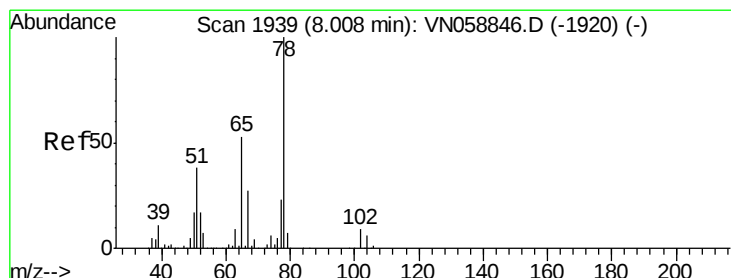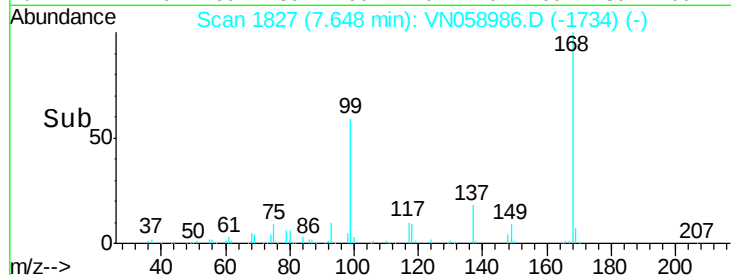

#33

1,2-Dichloroethane-d4

Concen: 50.240 ug/l

RT: 8.01 min Scan# 1939

Delta R.T. 0.00 min

Lab File: VN058986.D


Acq: 28 Oct 2019 10:53

Tgt Ion: 65 Resp: 290440

Ion Ratio Lower Upper

65 100

67 52.0 0.0 103.2

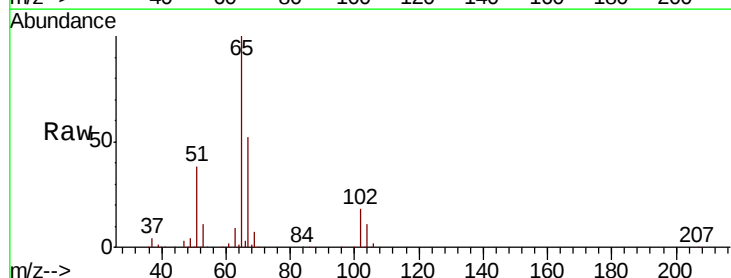

Abundance Ion 64.90 (64.60 to 65.60): VNO

Ion 66.90 (66.60 to 67.60): VNO

8.01


100000


50000

0

7.90 8.00 8.10

Time-->

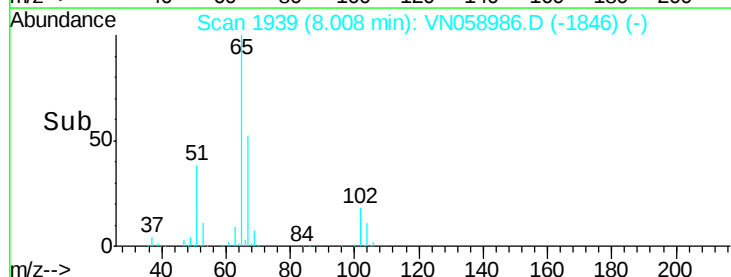


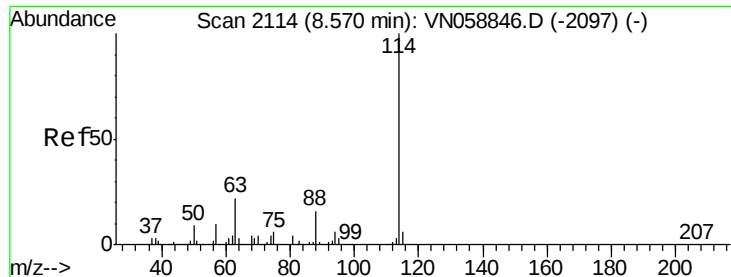




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.57 min Scan# 2114
 Delta R.T. 0.00 min
 Lab File: VN058986.D
 Acq: 28 Oct 2019 10:53

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1028WBL01

Tot Ion	Ratio	Lower	Upper
114	100		
63	22.6	0.0	44.4
88	16.4	0.0	31.4

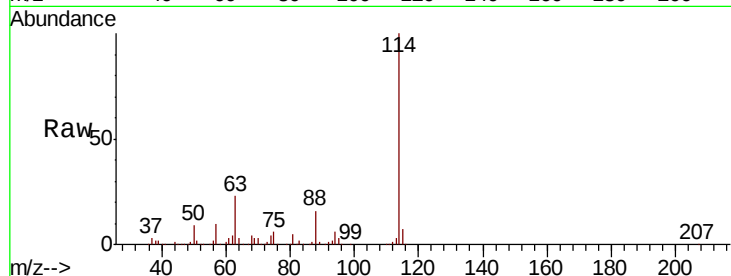


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

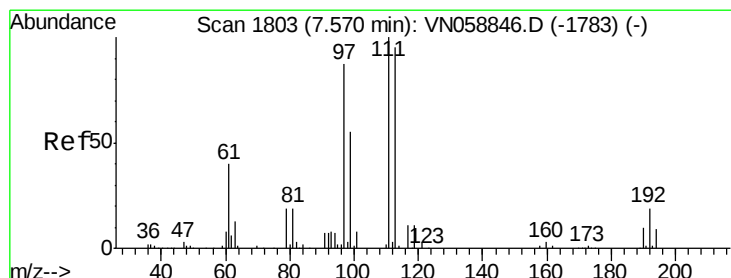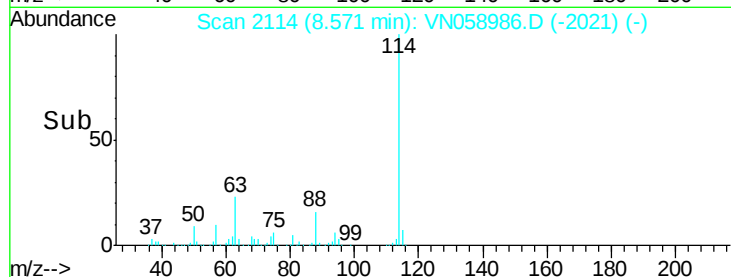
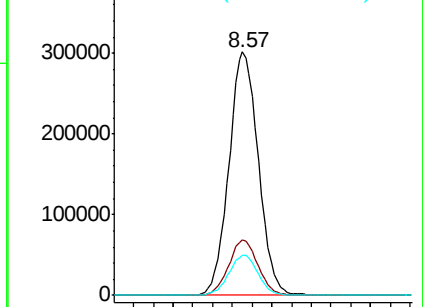



#35
 Dibromofluoromethane
 Concen: 51.202 ug/l
 RT: 7.57 min Scan# 1803
 Delta R.T. 0.00 min
 Lab File: VN058986.D
 Acq: 28 Oct 2019 10:53

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.9	82.0	123.0
192	19.2	15.0	22.6

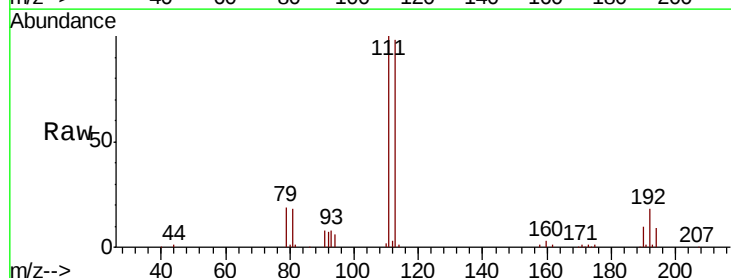

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

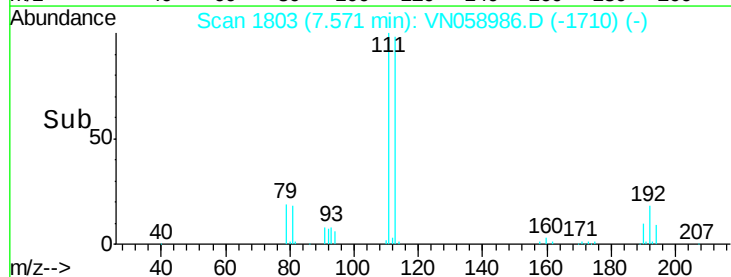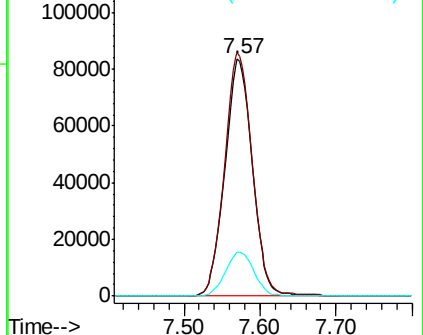

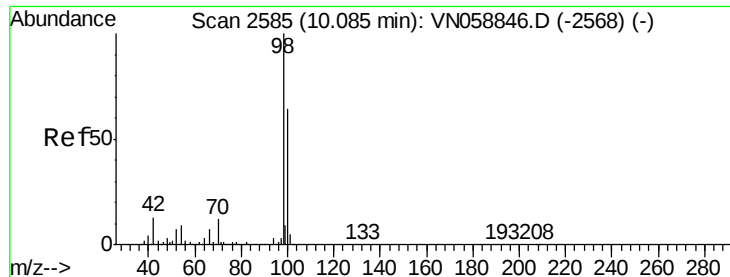

#50

Toluene-d8

Concen: 49.915 ug/l

RT: 10.08 min Scan# 2584

Delta R.T. -0.00 min

Lab File: VN058986.D

Acq: 28 Oct 2019 10:53

Instrument :

MSVOA_N

ClientSampleId :





VN1028WBL01

Tot Ion: 98 Resp: 799813

Ion Ratio Lower Upper

98 100

100 64.2 51.4 77.2

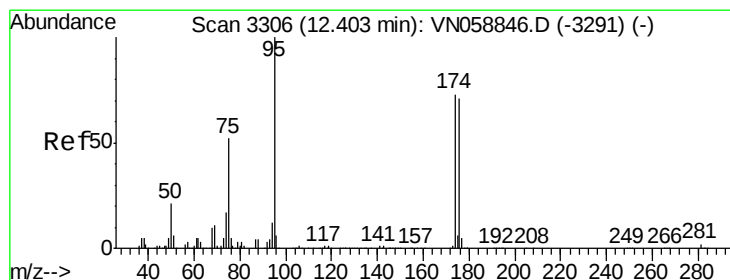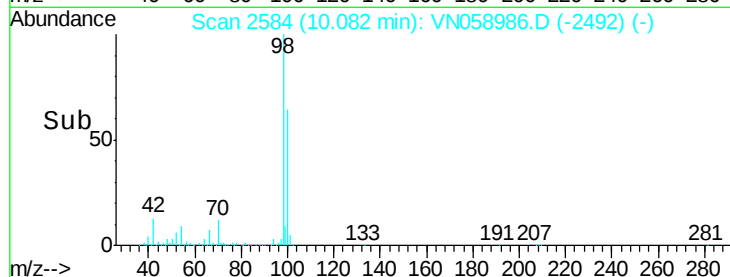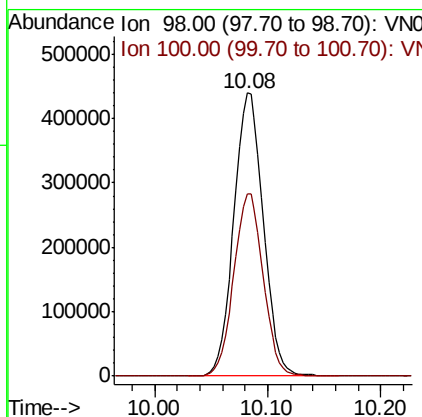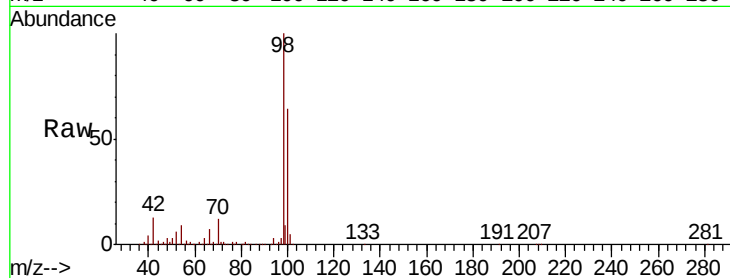

#62

4-Bromofluorobenzene

Concen: 43.276 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN058986.D

Acq: 28 Oct 2019 10:53




Tgt Ion: 95 Resp: 254651


Ion Ratio Lower Upper

95 100

174 76.6 0.0 147.6

176 73.8 0.0 143.2

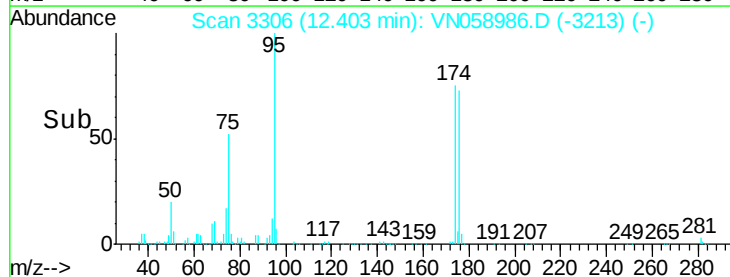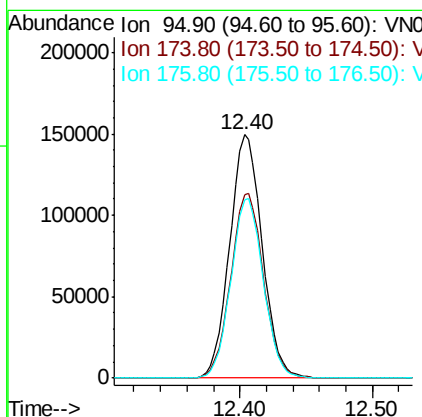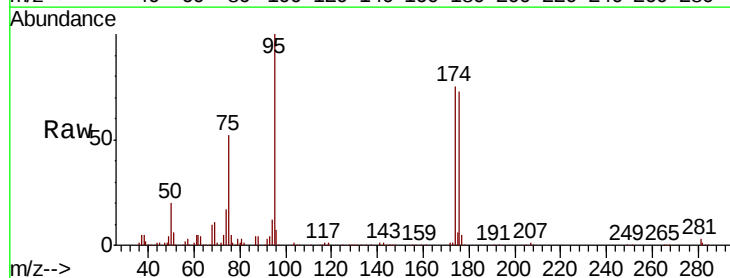

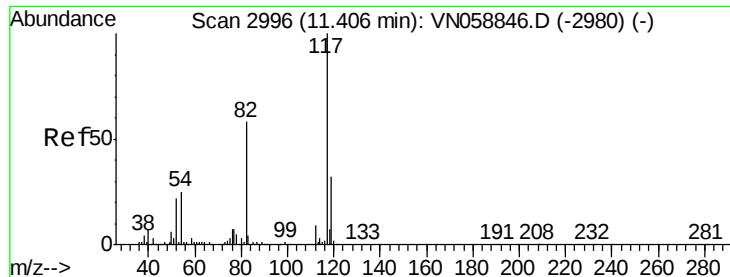

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. 0.00 min

Lab File: VN058986.D

Acq: 28 Oct 2019 10:53

Instrument :

MSVOA_N

ClientSampleId :

VN1028WBL01


Tot Ion:117 Resp: 560953

Ion Ratio Lower Upper

117 100

82 58.5 46.6 69.8




119 32.0 25.6 38.4

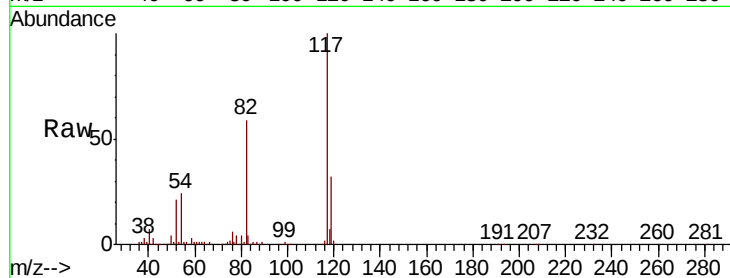

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VN

Ion 118.90 (118.60 to 119.60): V

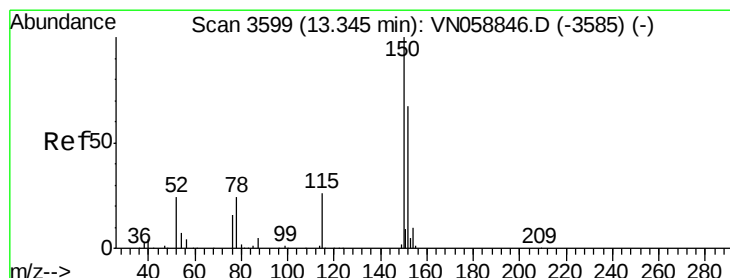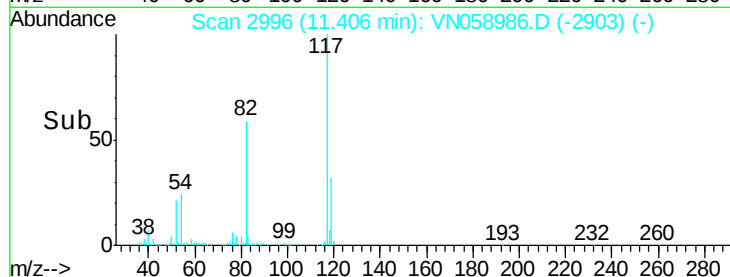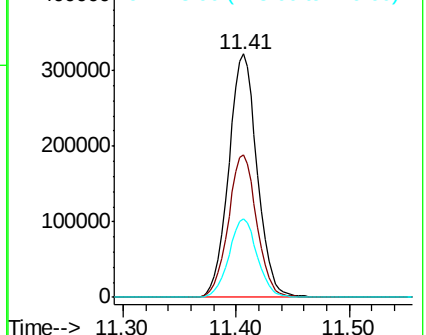

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3600

Delta R.T. 0.00 min

Lab File: VN058986.D

Acq: 28 Oct 2019 10:53


Tgt Ion:152 Resp: 204352

Ion Ratio Lower Upper

152 100

115 60.1 30.5 91.5

150 157.3 0.0 344.4

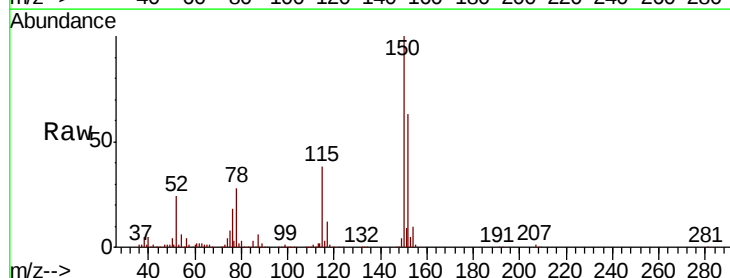

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

