

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102821\
 Data File : VN069256.D
 Acq On : 28 Oct 2021 18:02
 Operator : JC/MD
 Sample : M4360-11
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BP-VPB-RW9-GW-278-280

Quant Time: Oct 28 19:09:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 28 16:09:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	331206	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	584889	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	570662	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	210598	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	221497	46.328	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	92.660%
35) Dibromofluoromethane	8.024	113	169556	46.505	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	93.000%
50) Toluene-d8	10.443	98	731380	50.171	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	100.340%
62) 4-Bromofluorobenzene	12.733	95	261591	47.554	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	95.100%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102821\
Data File : VN069256.D
Acq On : 28 Oct 2021 18:02
Operator : JC/MD
Sample : M4360-11
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-RW9-GW-278-280

Quant Time: Oct 28 19:09:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 28 16:09:15 2021
Response via : Initial Calibration




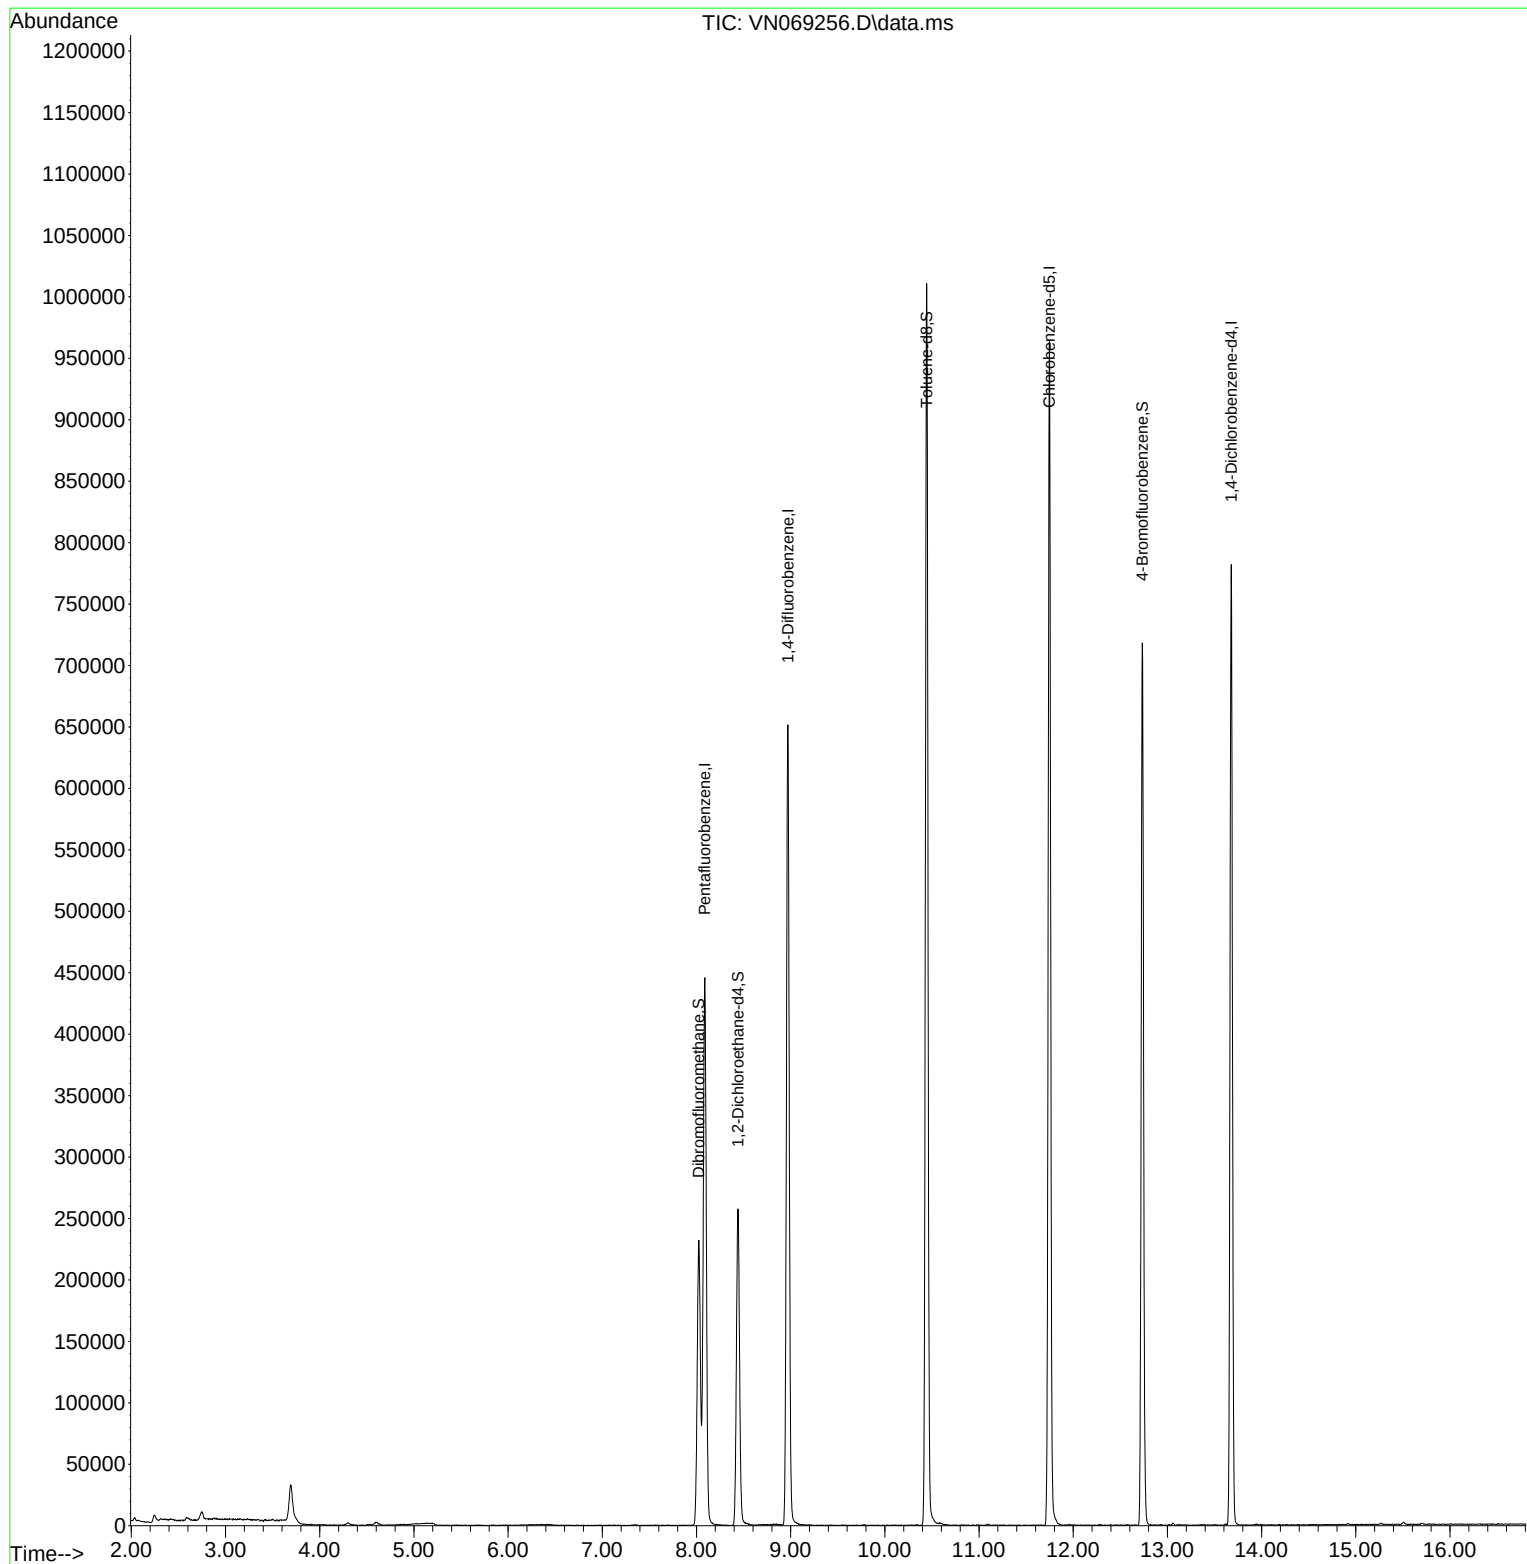


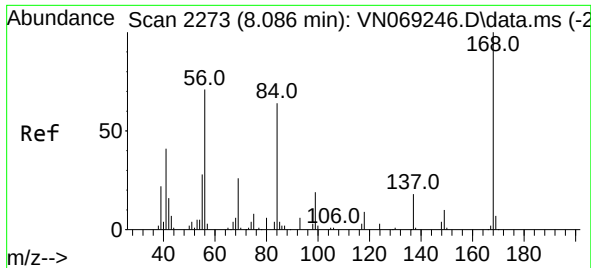

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069256.D
Acq: 28 Oct 2021 18:02




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-RW9-GW-278-280


Tgt Ion:168 Resp: 331206
Ion Ratio Lower Upper
168 100
99 62.0 48.9 73.3

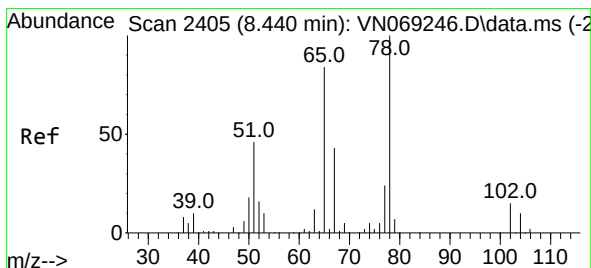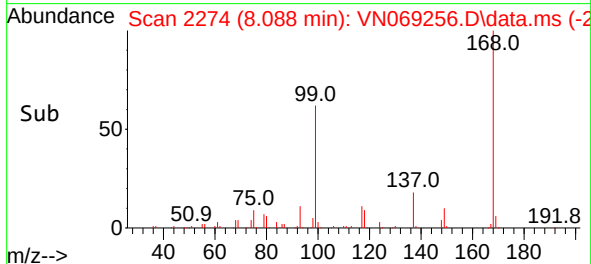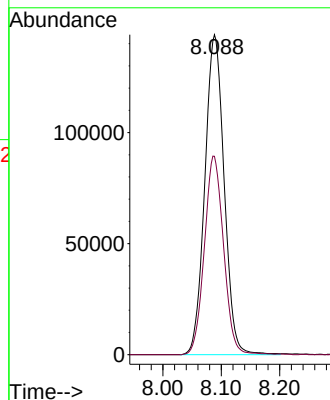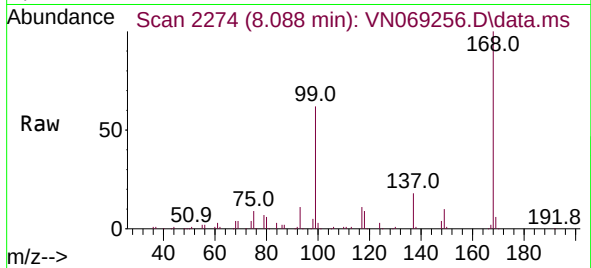

#33
1,2-Dichloroethane-d4
Concen: 46.328 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN069256.D
Acq: 28 Oct 2021 18:02

Tgt Ion: 65 Resp: 221497
Ion Ratio Lower Upper
65 100
67 51.3 0.0 103.8


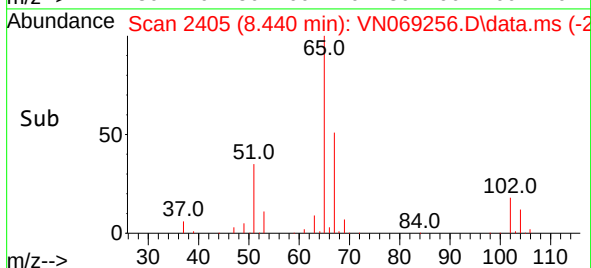
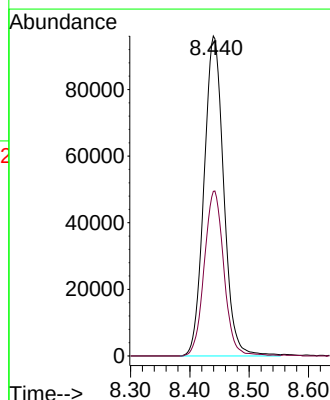
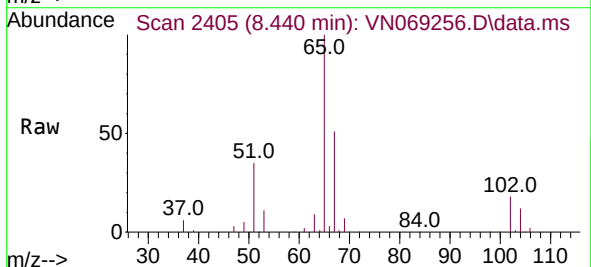


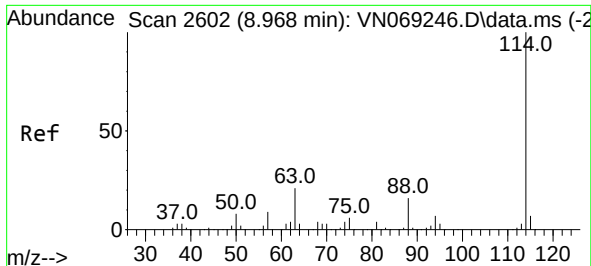

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN069256.D
Acq: 28 Oct 2021 18:02




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-RW9-GW-278-280


Tgt Ion:114 Resp: 584889
Ion Ratio Lower Upper
114 100
63 20.5 0.0 42.6
88 16.0 0.0 32.0

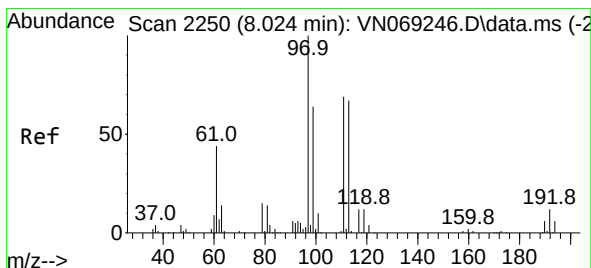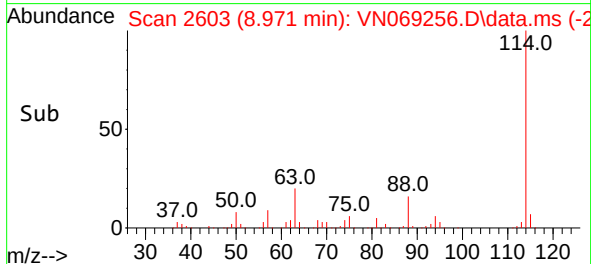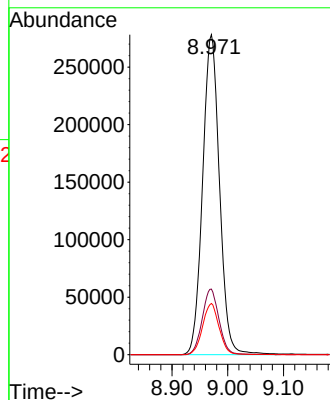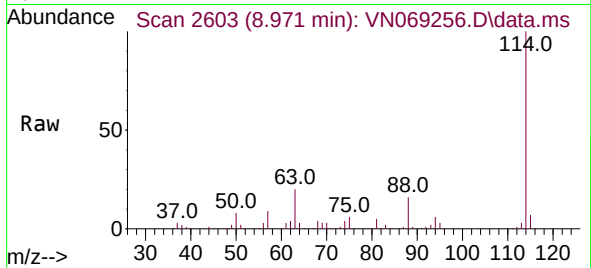

#35
Dibromofluoromethane
Concen: 46.505 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN069256.D
Acq: 28 Oct 2021 18:02

Tgt Ion:113 Resp: 169556
Ion Ratio Lower Upper
113 100
111 103.0 83.2 124.8
192 18.1 15.0 22.4


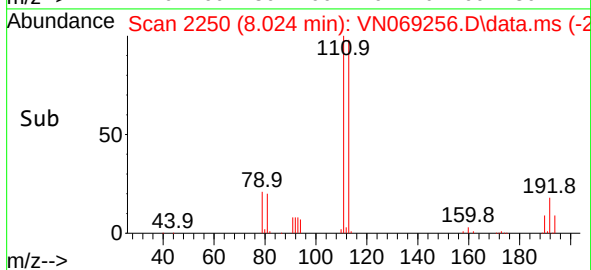
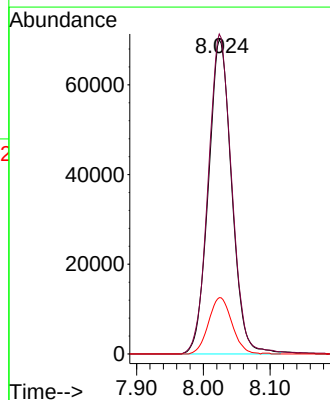
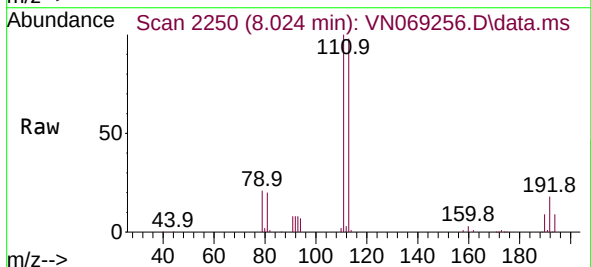


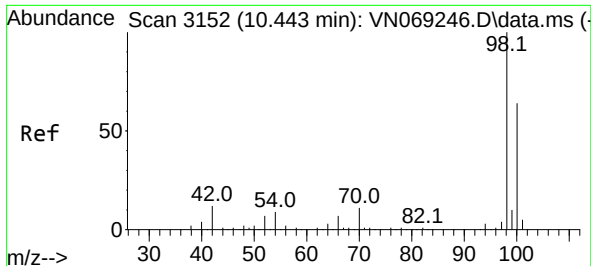

#50
Toluene-d8
Concen: 50.171 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VN069256.D
Acq: 28 Oct 2021 18:02




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-RW9-GW-278-280


Tgt Ion: 98 Resp: 731380
Ion Ratio Lower Upper
98 100
100 63.7 51.5 77.3

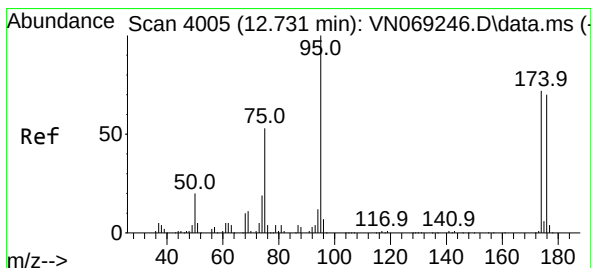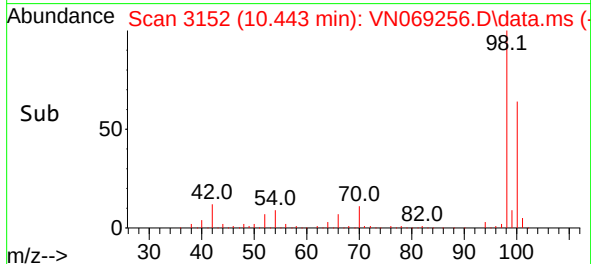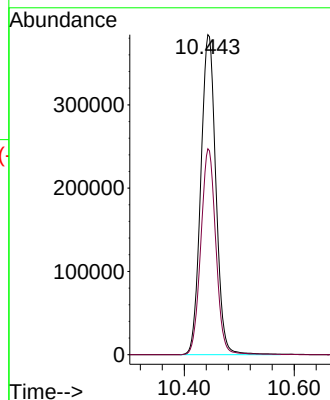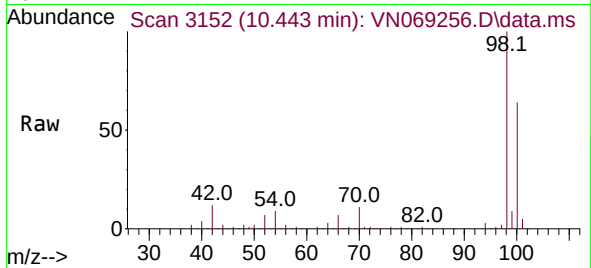

#62
4-Bromofluorobenzene
Concen: 47.554 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.002 min
Lab File: VN069256.D
Acq: 28 Oct 2021 18:02

Tgt Ion: 95 Resp: 261591
Ion Ratio Lower Upper
95 100
174 74.4 0.0 144.8
176 71.6 0.0 140.0

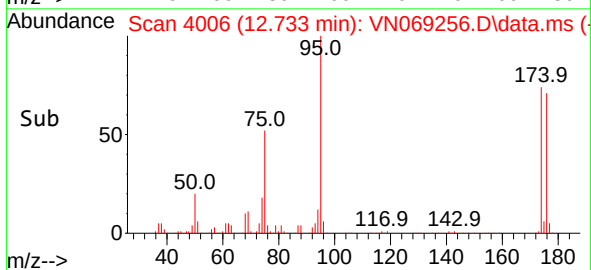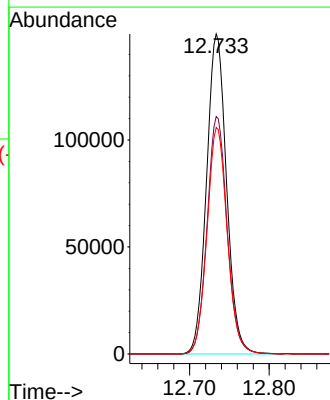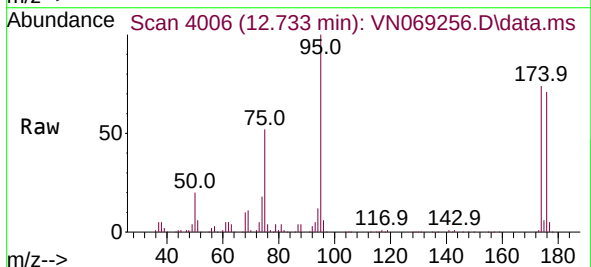

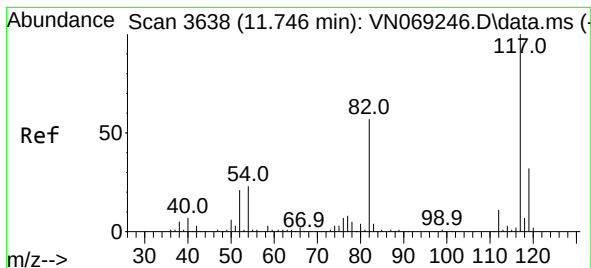

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.746 min Scan# 3638

Delta R.T. -0.000 min

Lab File: VN069256.D

Acq: 28 Oct 2021 18:02

Instrument :

MSVOA_N

ClientSampleId :

BP-VPB-RW9-GW-278-280





Tgt Ion:117 Resp: 570662

Ion Ratio Lower Upper

117 100

82 56.4 46.4 69.6

119 32.2 26.0 39.0

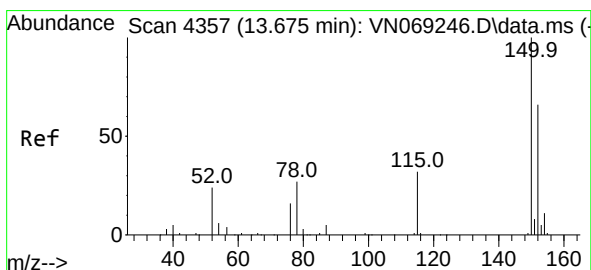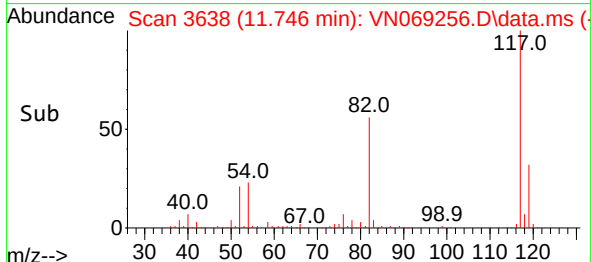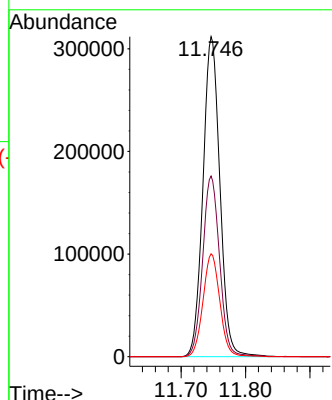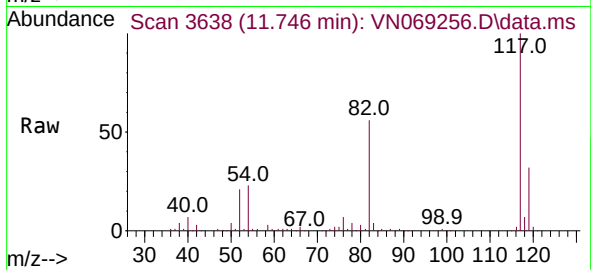

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.677 min Scan# 4358

Delta R.T. 0.002 min

Lab File: VN069256.D

Acq: 28 Oct 2021 18:02

Tgt Ion:152 Resp: 210598

Ion Ratio Lower Upper

152 100

115 63.2 31.4 94.3

150 158.0 0.0 351.0

