


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102821\
Data File : VN069264.D
Acq On : 28 Oct 2021 21:53
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Title : SW846 8260
Last Update : Thu Oct 28 16:09:15 2021

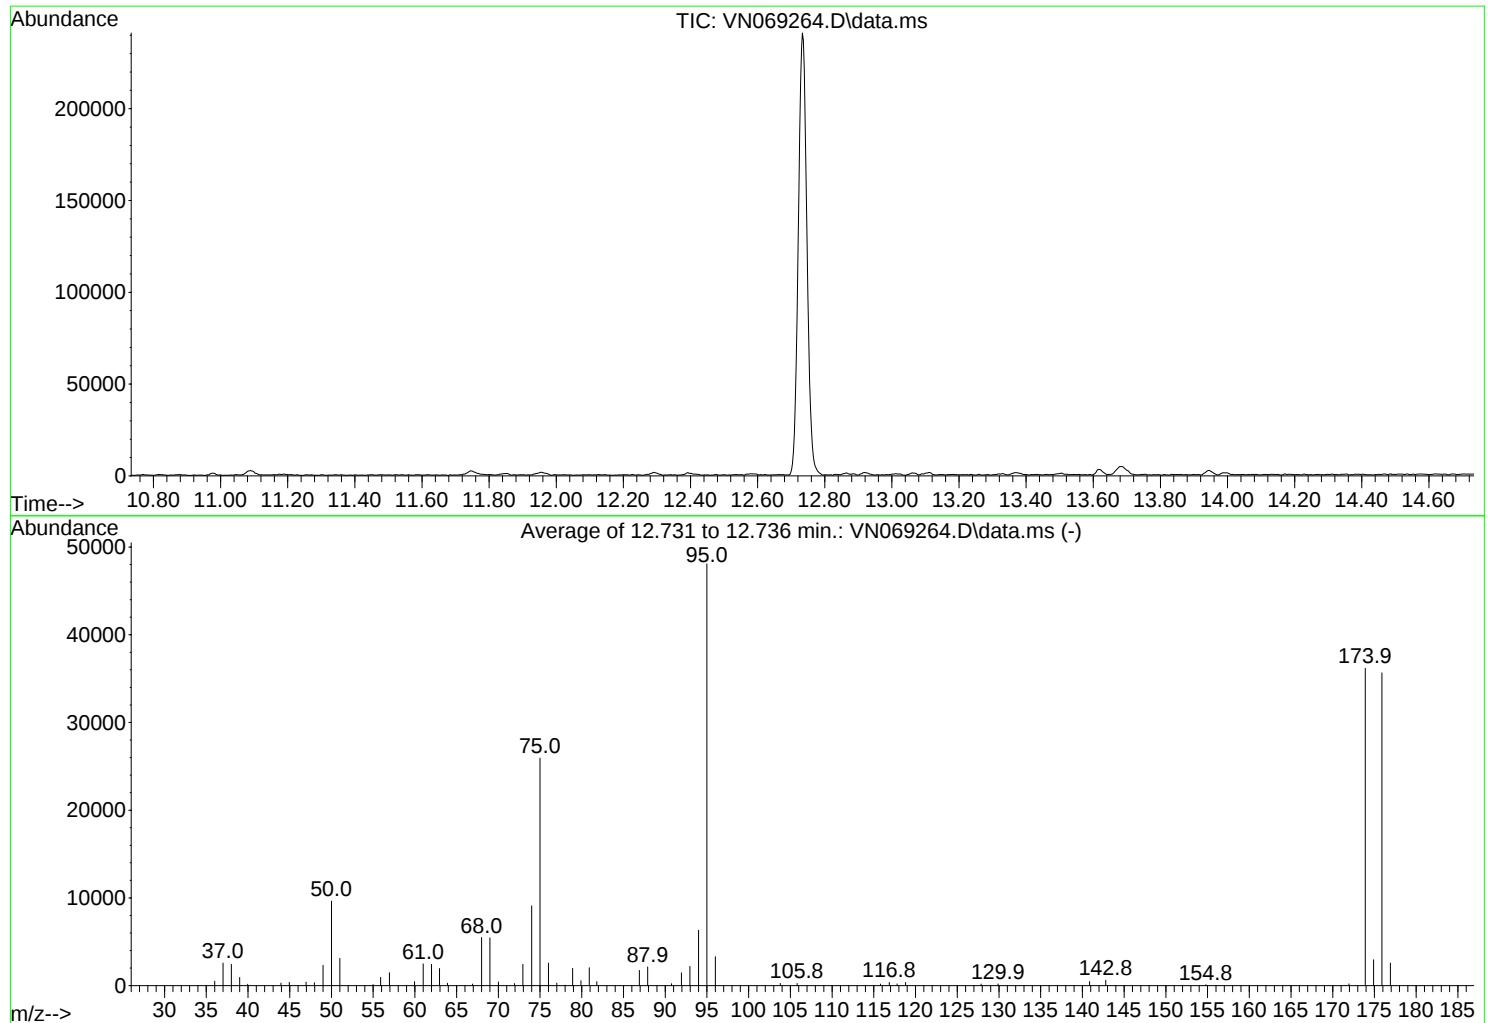

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.0	9625	PASS
75	95	30	60	54.0	25947	PASS
95	95	100	100	100.0	48085	PASS
96	95	5	9	6.9	3308	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.2	36171	PASS
175	174	5	9	8.2	2956	PASS
176	174	95	101	98.6	35664	PASS
177	176	5	9	7.2	2578	PASS