


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102822\
Data File : VN075051.D
Acq On : 28 Oct 2022 09:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N102522W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Oct 27 10:19:47 2022

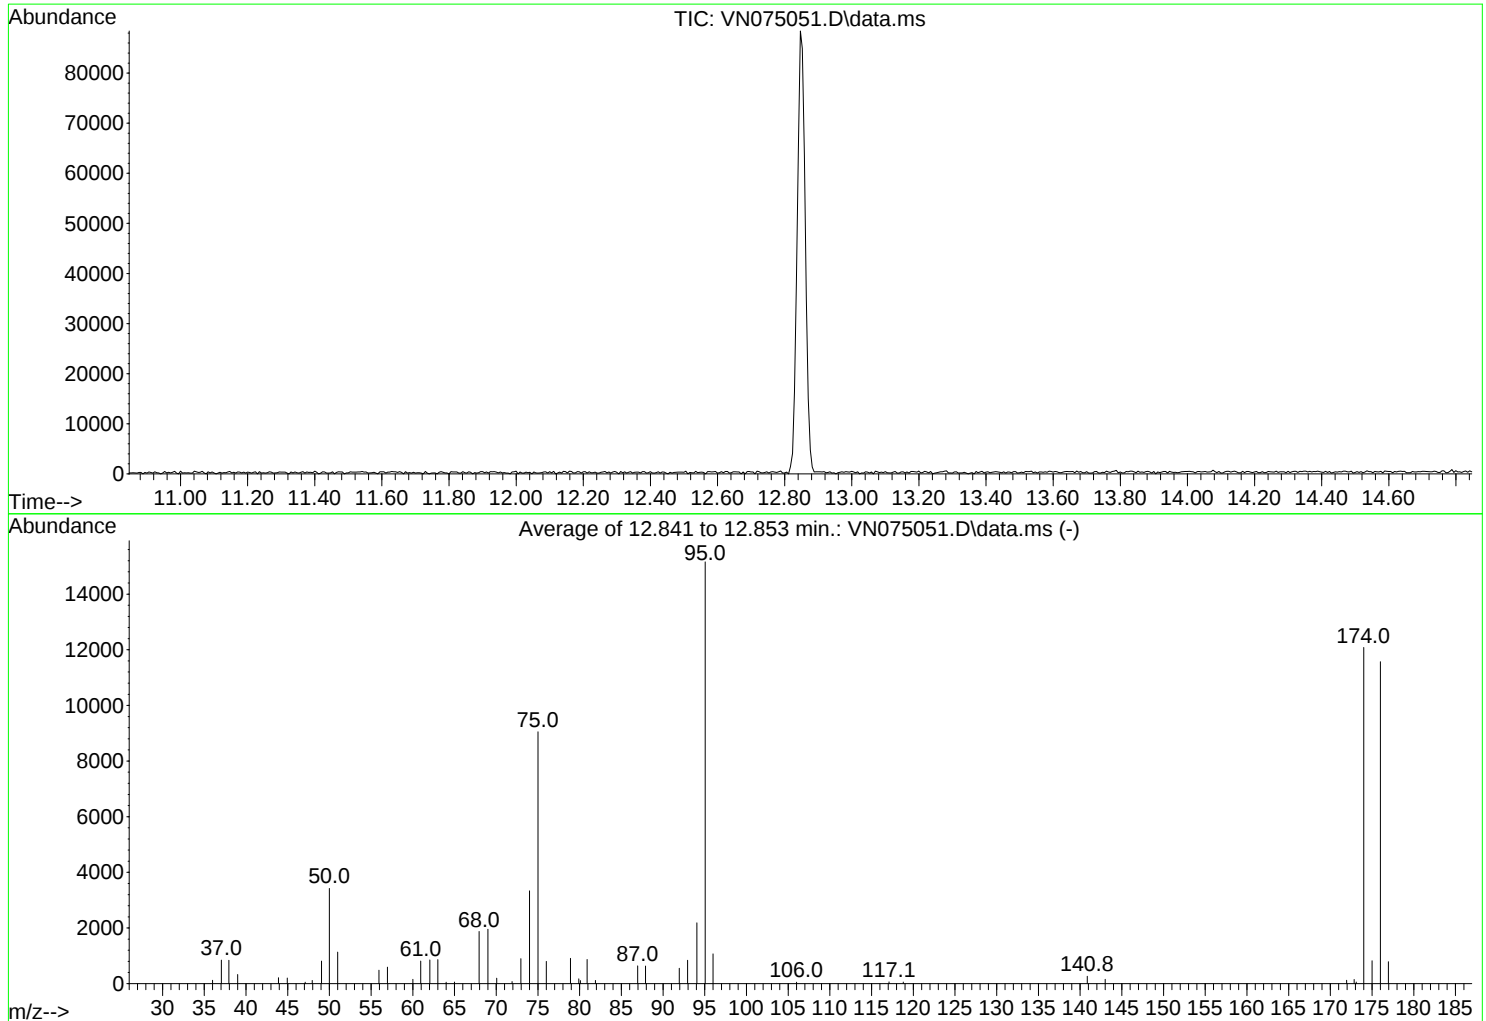

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	3422	PASS
75	95	30	60	59.7	9049	PASS
95	95	100	100	100.0	15160	PASS
96	95	5	9	7.0	1068	PASS
173	174	0.00	2	1.2	151	PASS
174	95	50	100	79.7	12084	PASS
175	174	5	9	6.8	824	PASS
176	174	95	101	95.7	11568	PASS
177	176	5	9	6.8	790	PASS