

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN102920\
 Data File : VN064381.D
 Acq On : 29 Oct 2020 18:08
 Operator : JC/MD
 Sample : PB132688ZHE#12
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132688ZHE#12

Quant Time: Oct 30 05:34:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102720W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 27 12:23:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	233624	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	409084	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	424623	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	181544	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.98	65	188803	50.29	ug/l	0.00
Spiked Amount			Recovery	=	100.58%	
35) Dibromofluoromethane	7.55	113	137502	50.40	ug/l	0.00
Spiked Amount			Recovery	=	100.80%	
50) Toluene-d8	10.06	98	520347	51.57	ug/l	0.00
Spiked Amount			Recovery	=	103.14%	
62) 4-Bromofluorobenzene	12.38	95	223174	56.72	ug/l	0.00
Spiked Amount			Recovery	=	113.44%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.70	59	255	0.468	ug/l #	70
13) Acrolein	3.60	56	30	17.915	ug/l #	10
16) Acetone	3.78	43	14178	3.844	ug/l #	88
18) Methyl Acetate	4.29	43	2517	0.892	ug/l #	85
20) Methylene Chloride	4.50	84	6893	2.589	ug/l	94
25) 2-Butanone	6.80	43	727	0.386	ug/l #	23
29) Tetrahydrofuran	7.18	42	311	0.254	ug/l #	57
31) Cyclohexane	7.62	56	6076	1.394	ug/l #	20
36) 1,1-Dichloropropene	7.62	75	20318	4.921	ug/l #	49
38) Carbon Tetrachloride	7.63	117	25638	5.356	ug/l #	16
43) Isopropyl Acetate	8.13	43	86218	12.094	ug/l #	90
45) 1,2-Dichloropropane	9.23	63	1650	0.536	ug/l #	44
48) Methyl methacrylate	9.23	41	139725	37.989	ug/l #	48
49) 1,4-Dioxane	9.15	88	35	0.646	ug/l #	1
51) 4-Methyl-2-Pentanone	9.95	43	6530	1.576	ug/l	95
54) cis-1,3-Dichloropropene	9.87	75	33533	6.457	ug/l #	64
56) Ethyl methacrylate	10.50	69	1361	0.314	ug/l #	1
57) 1,3-Dichloropropane	10.73	76	5541	1.135	ug/l #	42
59) 2-Hexanone	10.74	43	92398	30.275	ug/l #	52
74) N-amyl acetate	12.01	43	3089	0.516	ug/l #	46
76) 1,2,3-Trichloropropane	12.38	75	126006	28.984	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.70	105	3749	0.326	ug/l	99
81) trans-1,4-Dichloro-2-buten	12.38	75	126006	83.488	ug/l #	8
95) Naphthalene	15.12	128	32	2.395	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN102920\
Data File : VN064381.D
Acq On : 29 Oct 2020 18:08
Operator : JC/MD
Sample : PB132688ZHE#12
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB132688ZHE#12

Quant Time: Oct 30 05:34:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N102720W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 27 12:23:17 2020
Response via : Initial Calibration

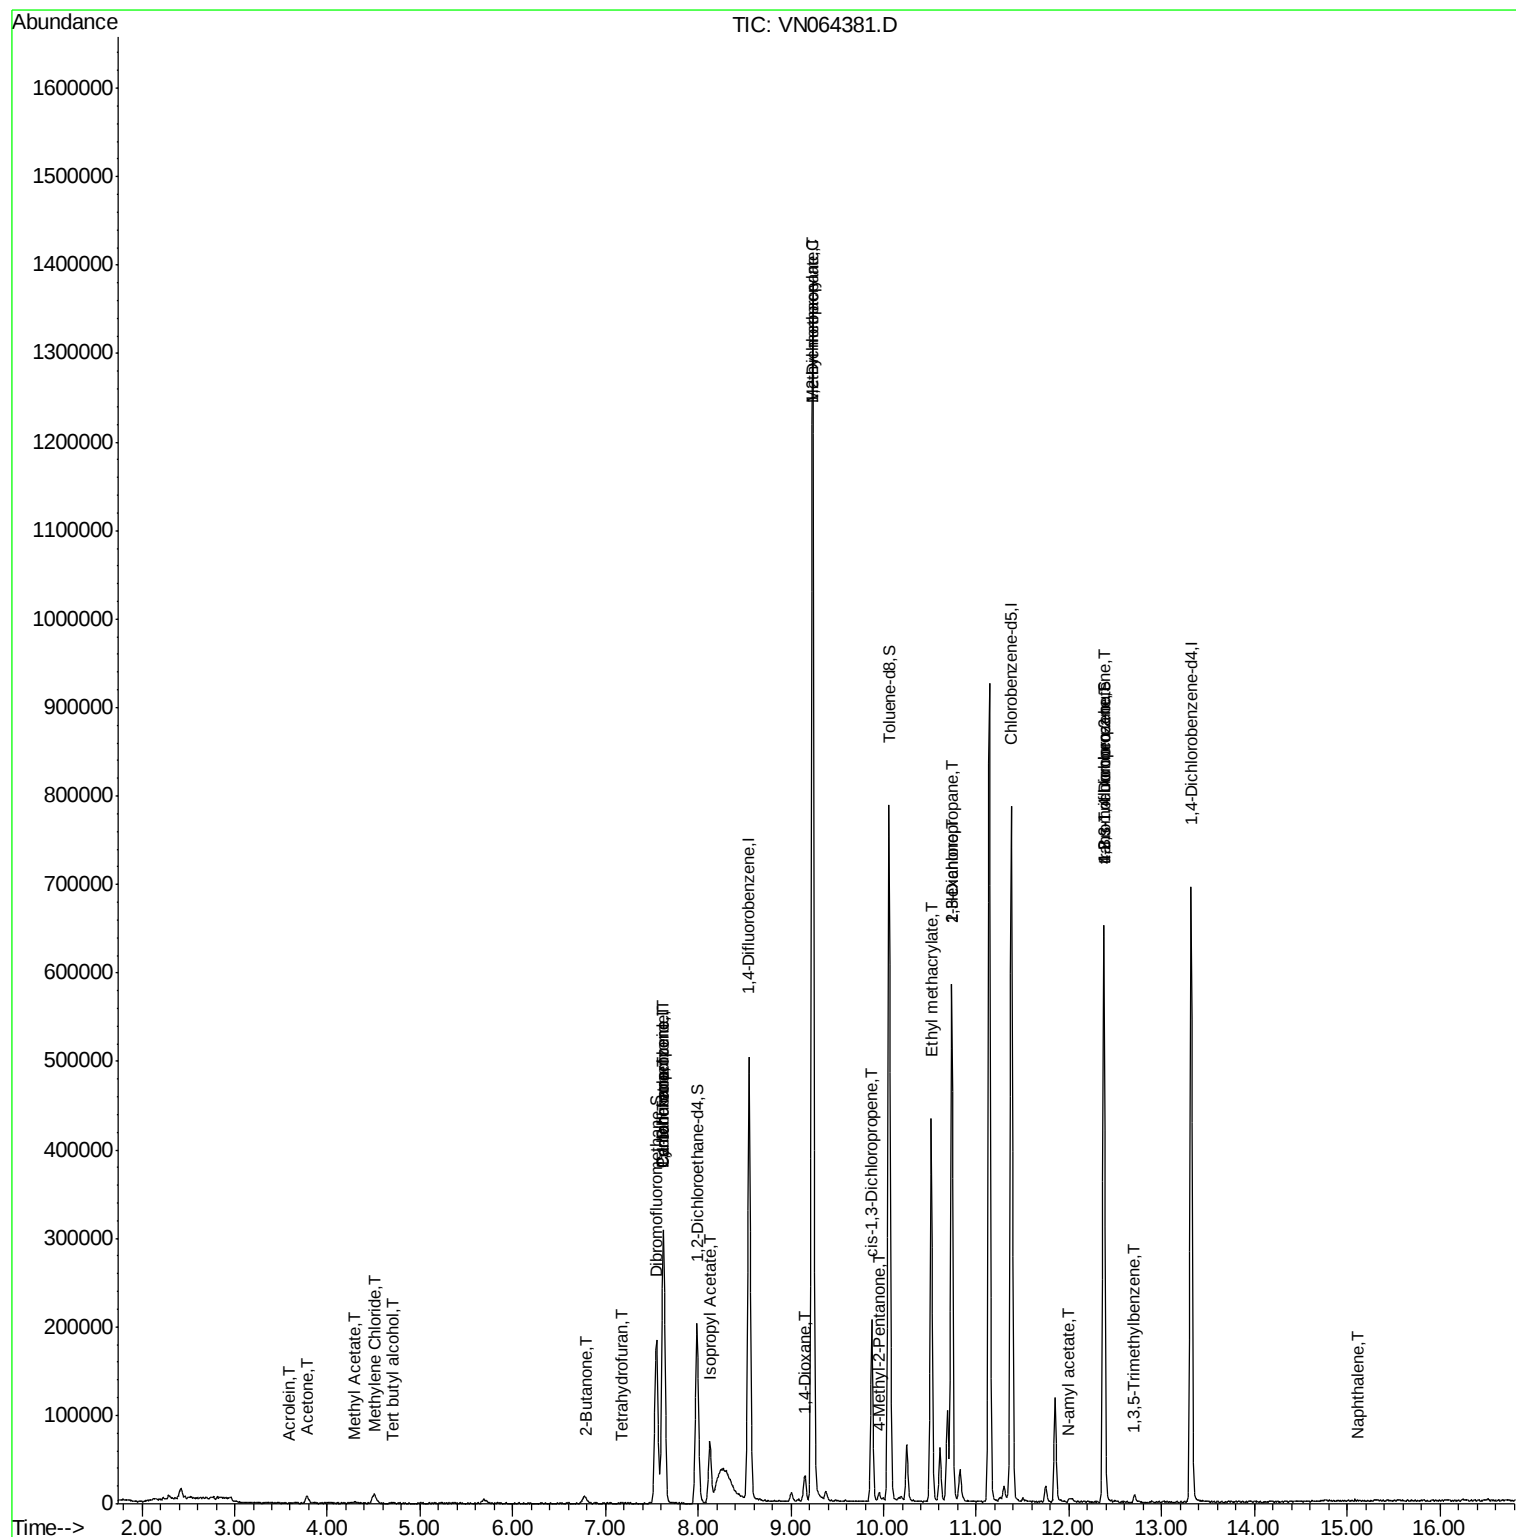

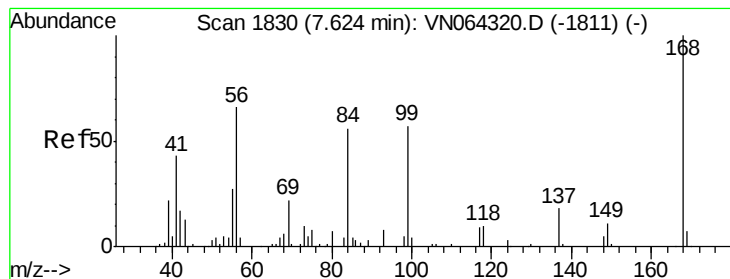

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064381.D

Acq: 29 Oct 2020 18:08

Instrument :

MSVOA_N

ClientSampleId :


PB132688ZHE#12

Tot Ion:168 Resp: 233624

Ion Ratio Lower Upper




168 100

99 65.6 52.7 79.1



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

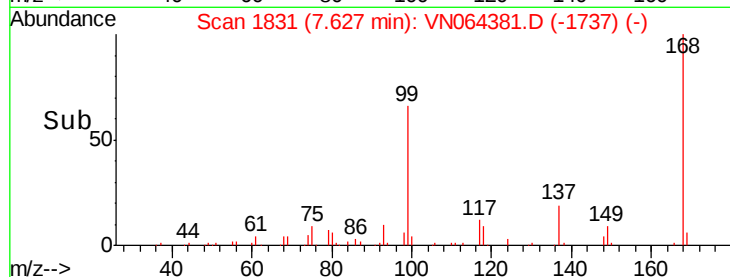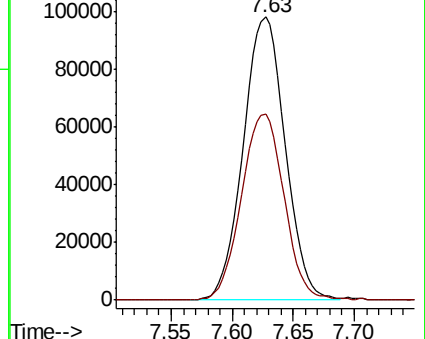

#11

Tert butyl alcohol

Concen: 0.468 ug/l

RT: 4.70 min Scan# 922

Delta R.T. -0.03 min

Lab File: VN064381.D


Acq: 29 Oct 2020 18:08

Tgt Ion: 59 Resp: 255

Ion Ratio Lower Upper



59 100


57 0.0 9.4 14.0#



Abundance Ion 59.00 (58.70 to 59.70): VN

Ion 57.00 (56.70 to 57.70): VN

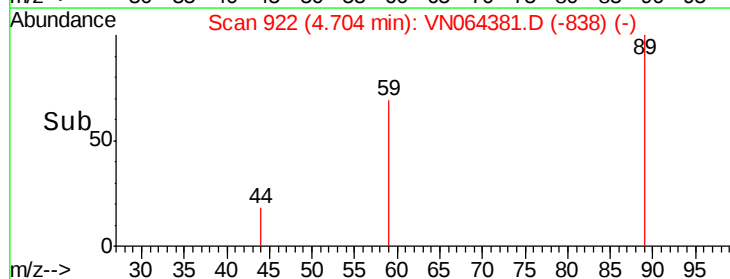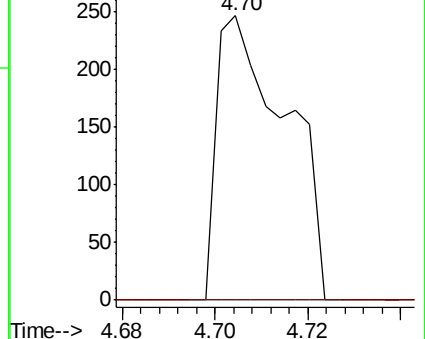



#13

Acrolein

Concen: 17.915 ug/l

RT: 3.60 min Scan# 577

Delta R.T. 0.03 min

Lab File: VN064381.D

Acq: 29 Oct 2020 18:08

Instrument :

MSVOA_N

ClientSampleId :


PB132688ZHE#12

Tot Ion: 56 Resp: 30

Ion Ratio Lower Upper

56 100

55 0.0 62.6 94.0#



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

3.60



150

100

50

0

Time-->

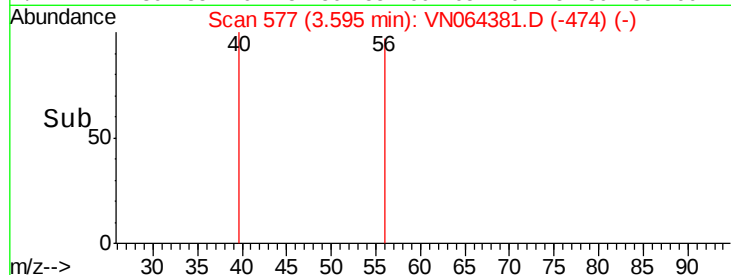

#16

Acetone

Concen: 3.844 ug/l

RT: 3.78 min Scan# 635

Delta R.T. 0.01 min

Lab File: VN064381.D


Acq: 29 Oct 2020 18:08

Tgt Ion: 43 Resp: 14178

Ion Ratio Lower Upper

43 100

58 21.1 22.1 33.1#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

6000

5000

4000


3000


2000

1000

0

Time-->









#18
Methyl Acetate
Concen: 0.892 ug/l
RT: 4.29 min Scan# 793
Delta R.T. 0.01 min
Lab File: VN064381.D
Acq: 29 Oct 2020 18:08




Instrument :
MSVOA_N
ClientSampleId :
PB132688ZHE#12


Tot Ion: 43 Resp: 2517
Ion Ratio Lower Upper
43 100
74 13.7 16.7 25.1#

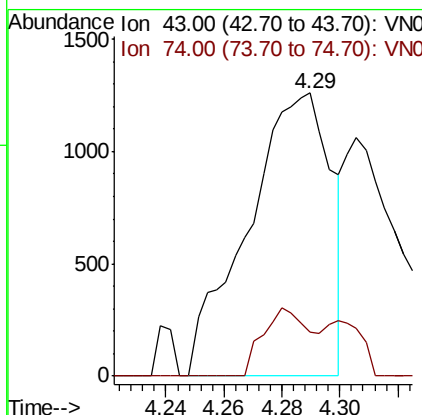

#20
Methylene Chloride
Concen: 2.589 ug/l
RT: 4.50 min Scan# 858
Delta R.T. -0.00 min
Lab File: VN064381.D
Acq: 29 Oct 2020 18:08

Tgt Ion: 84 Resp: 6893
Ion Ratio Lower Upper
84 100
49 122.4 103.6 155.4
51 45.0 31.8 47.8
86 61.7 51.3 76.9


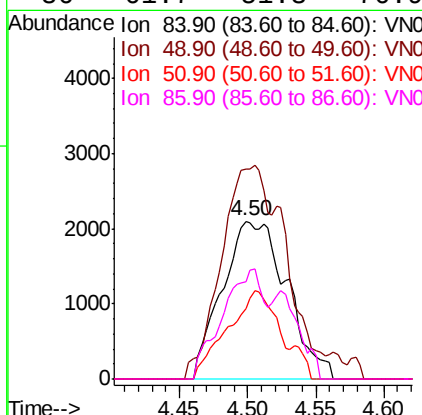




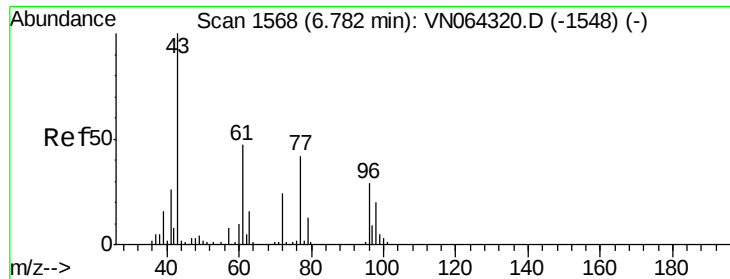

#25
2-Butanone
Concen: 0.386 ug/l
RT: 6.80 min Scan# 1573
Delta R.T. 0.02 min
Lab File: VN064381.D
Acq: 29 Oct 2020 18:08




Instrument :
MSVOA_N
ClientSampleId :
PB132688ZHE#12


Tot Ion: 43 Resp: 727
Ion Ratio Lower Upper
43 100
72 61.1 18.8 28.2#

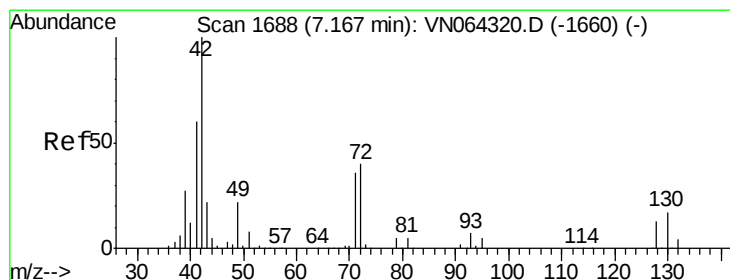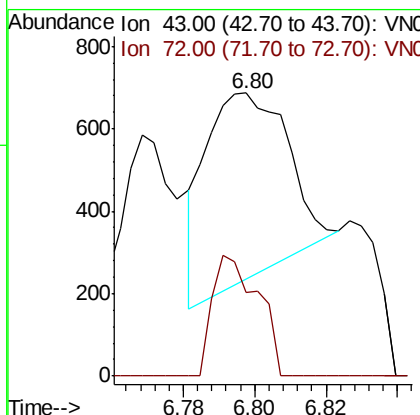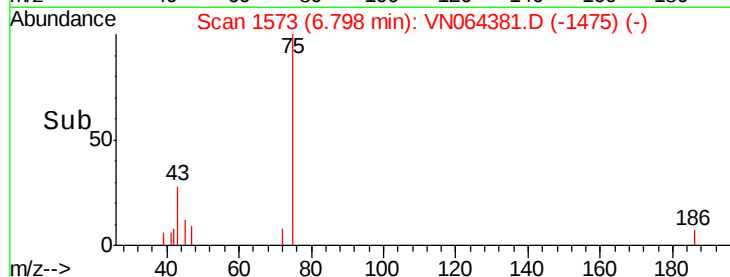

#29
Tetrahydrofuran
Concen: 0.254 ug/l
RT: 7.18 min Scan# 1692
Delta R.T. 0.01 min
Lab File: VN064381.D
Acq: 29 Oct 2020 18:08

Tgt Ion: 42 Resp: 311
Ion Ratio Lower Upper
42 100
72 24.4 31.6 47.4#
71 0.0 29.4 44.0#

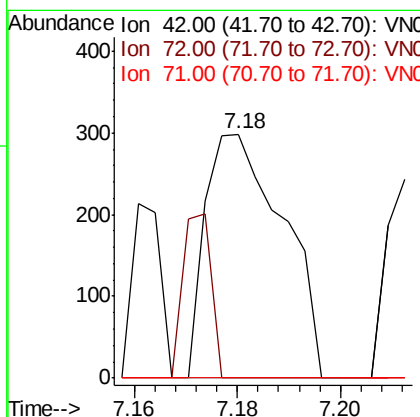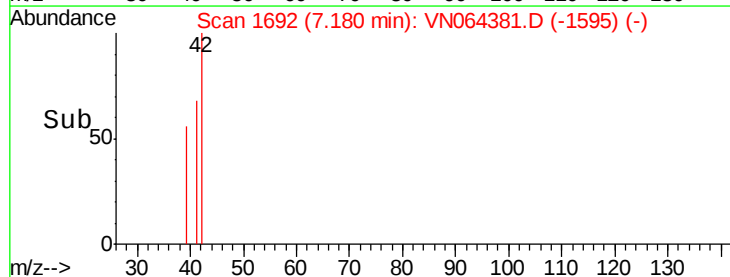


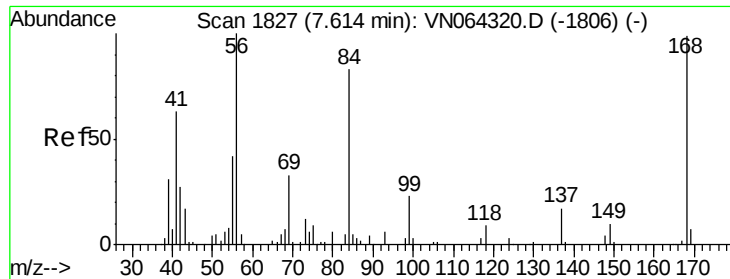




#31
Cyclohexane
Concen: 1.394 ug/l
RT: 7.62 min Scan# 1830
Delta R.T. 0.01 min
Lab File: VN064381.D
Acq: 29 Oct 2020 18:08

Instrument :
MSVOA_N
ClientSampleId :
PB132688ZHE#12

Tot Ion: 56 Resp: 6076
Ion Ratio Lower Upper
56 100
69 167.3 25.8 38.8#
84 98.0 66.3 99.5




Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0

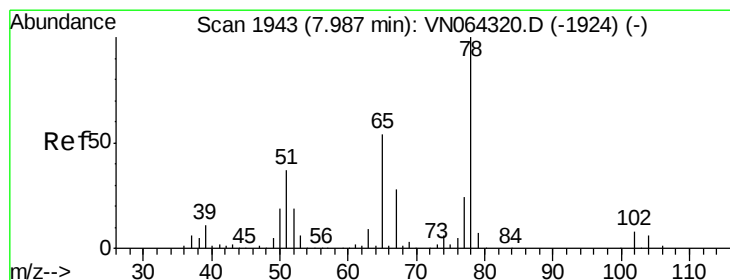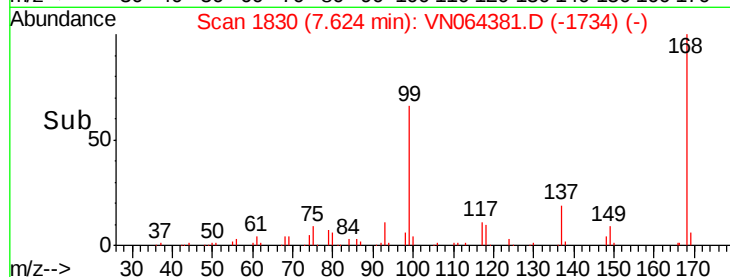
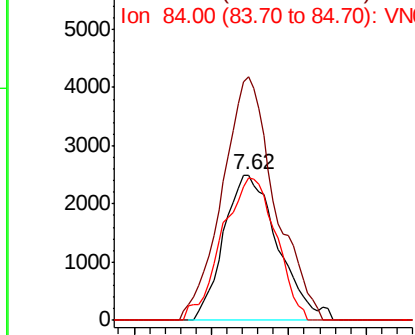



#33
1,2-Dichloroethane-d4
Concen: 50.290 ug/l
RT: 7.98 min Scan# 1942
Delta R.T. -0.00 min
Lab File: VN064381.D
Acq: 29 Oct 2020 18:08

Tgt Ion: 65 Resp: 188803
Ion Ratio Lower Upper
65 100
67 48.9 0.0 99.2



Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

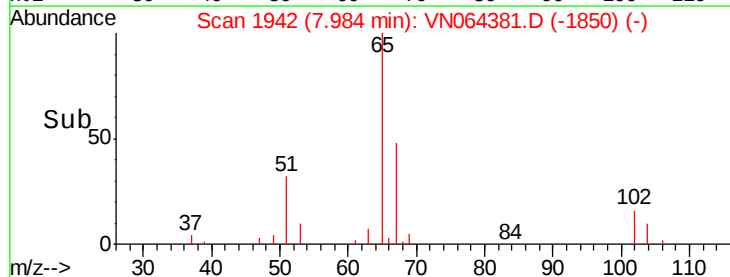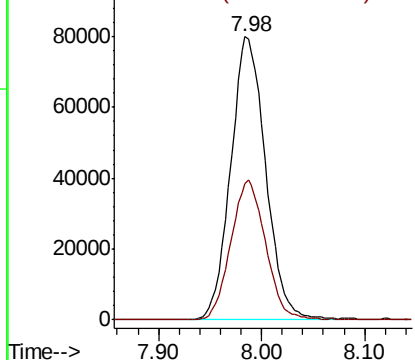

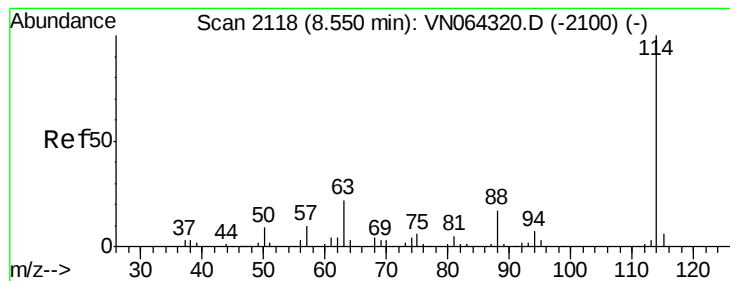

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2118

Delta R.T. -0.00 min

Lab File: VN064381.D

Acq: 29 Oct 2020 18:08

Instrument :

MSVOA_N

ClientSampleId :

PB132688ZHE#12


Tot Ion:114 Resp: 409084

Ion Ratio Lower Upper

114 100

63 22.0 0.0 44.6




88 17.3 0.0 33.4



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

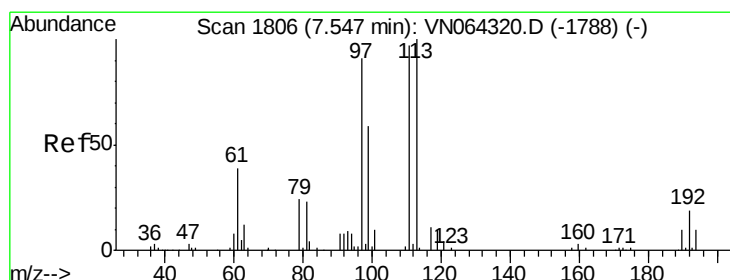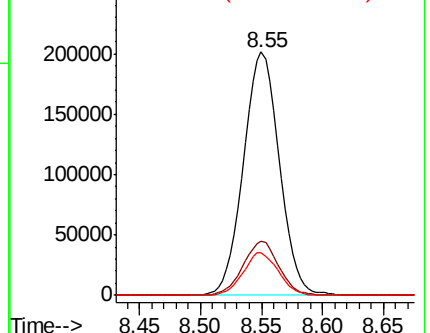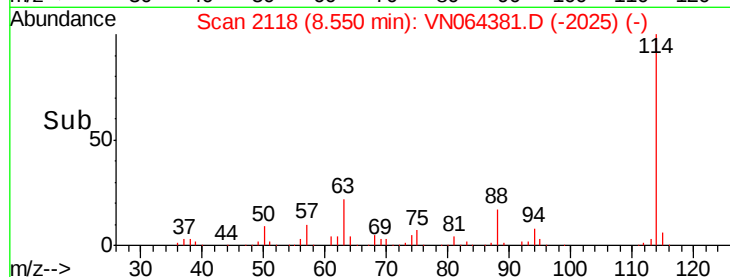

#35

Dibromofluoromethane

Concen: 50.403 ug/l

RT: 7.55 min Scan# 1807

Delta R.T. 0.00 min

Lab File: VN064381.D

Acq: 29 Oct 2020 18:08


Tgt Ion:113 Resp: 137502

Ion Ratio Lower Upper

113 100

111 101.5 81.5 122.3



192 18.3 15.0 22.4




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

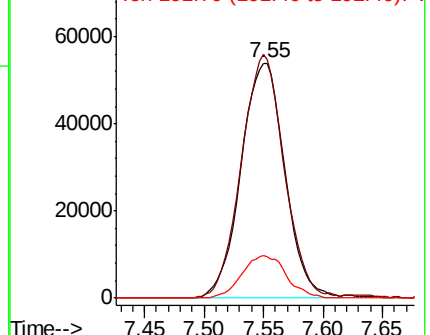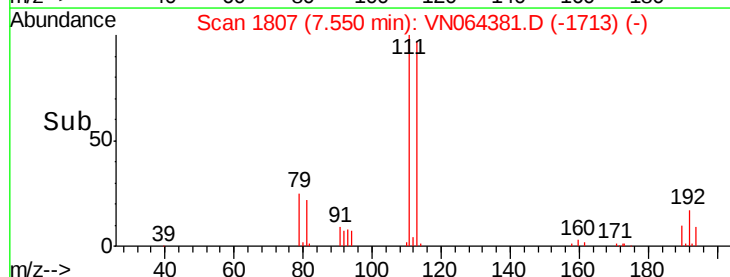







#36
 1,1-Dichloropropene
 Concen: 4.921 ug/l
 RT: 7.62 min Scan# 1830
 Delta R.T. -0.13 min
 Lab File: VN064381.D
 Acq: 29 Oct 2020 18:08

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132688ZHE#12

Tot Ion: 75 Resp: 20318
 Ion Ratio Lower Upper
 75 100
 110 7.0 16.8 50.3#
 77 0.0 24.2 36.4#




Abundance Ion 74.90 (74.60 to 75.60): VN0
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.90 (76.60 to 77.60): VN0


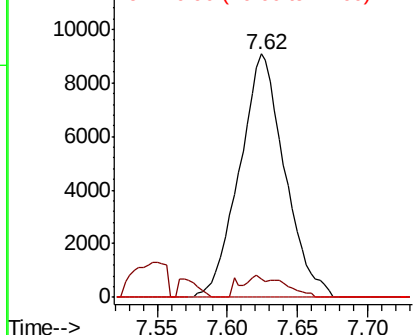



#38
 Carbon Tetrachloride
 Concen: 5.356 ug/l
 RT: 7.63 min Scan# 1831
 Delta R.T. -0.11 min
 Lab File: VN064381.D
 Acq: 29 Oct 2020 18:08

Tgt Ion: 117 Resp: 25638
 Ion Ratio Lower Upper
 117 100
 119 2.9 73.7 110.5#
 121 0.0 22.8 34.2#



Abundance Ion 116.80 (116.50 to 117.50): V
 Ion 118.80 (118.50 to 119.50): V
 Ion 120.80 (120.50 to 121.50): V

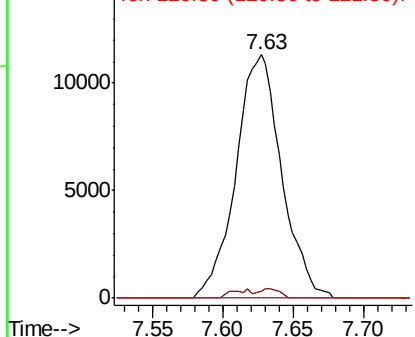

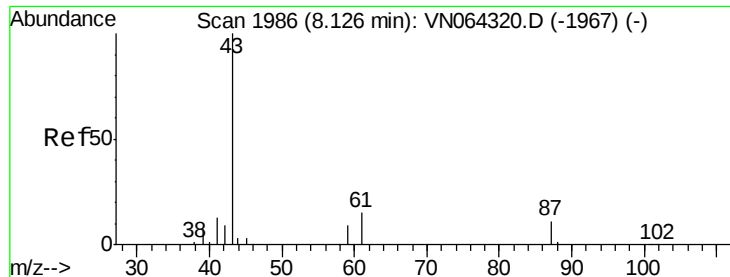

#43

Isopropyl Acetate

Concen: 12.094 ug/l

RT: 8.13 min Scan# 1987

Delta R.T. 0.00 min

Lab File: VN064381.D

Acq: 29 Oct 2020 18:08

Instrument :

MSVOA_N

ClientSampleId :

PB132688ZHE#12


Tot Ion: 43 Resp: 86218

Ion Ratio Lower Upper

43 100

61 17.0 19.1 28.7#




87 12.7 9.3 13.9

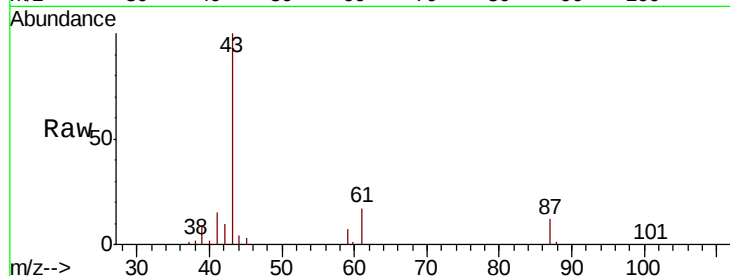

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

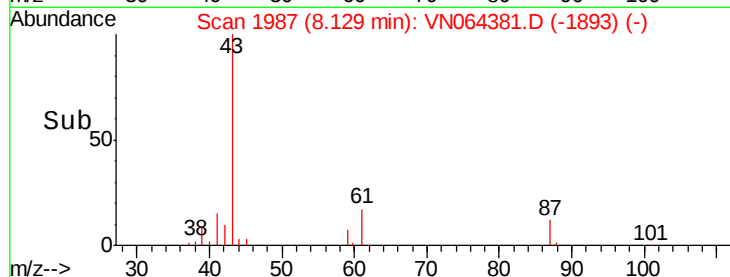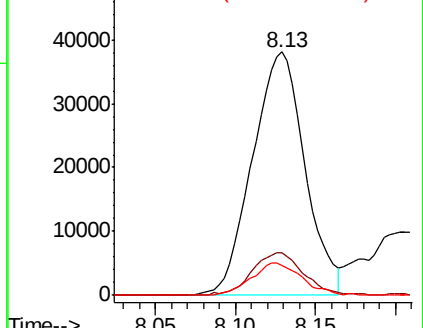

#45

1,2-Dichloropropane

Concen: 0.536 ug/l

RT: 9.23 min Scan# 2330

Delta R.T. 0.15 min

Lab File: VN064381.D


Acq: 29 Oct 2020 18:08

Tgt Ion: 63 Resp: 1650

Ion Ratio Lower Upper



63 100


65 0.0 24.3 36.5#



Abundance Ion 62.90 (62.60 to 63.60): VN0

Ion 64.90 (64.60 to 65.60): VN0



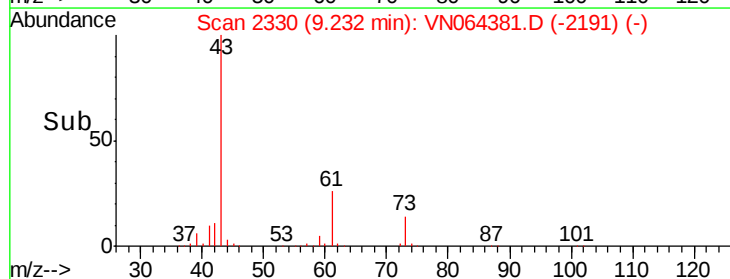
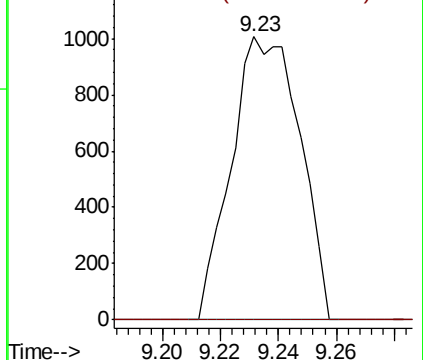




#48
Methvl methacrylate
Concen: 37.989 ug/l
RT: 9.23 min Scan# 2331
Delta R.T. 0.07 min
Lab File: VN064381.D
Acq: 29 Oct 2020 18:08




Instrument :
MSVOA_N
ClientSampleId :
PB132688ZHE#12


Tot Ion: 41 Resp: 139725
Ion Ratio Lower Upper
41 100
69 0.0 59.1 88.7#
39 56.2 51.3 76.9

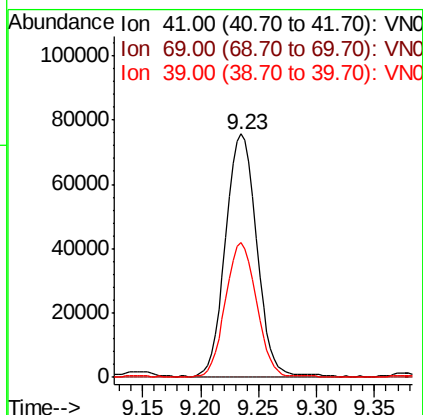

#49
1,4-Dioxane
Concen: 0.646 ug/l
RT: 9.15 min Scan# 2306
Delta R.T. -0.01 min
Lab File: VN064381.D
Acq: 29 Oct 2020 18:08

Tgt Ion: 88 Resp: 35
Ion Ratio Lower Upper
88 100
43 0.0 31.8 47.8#
58 3042.9 60.3 90.5#

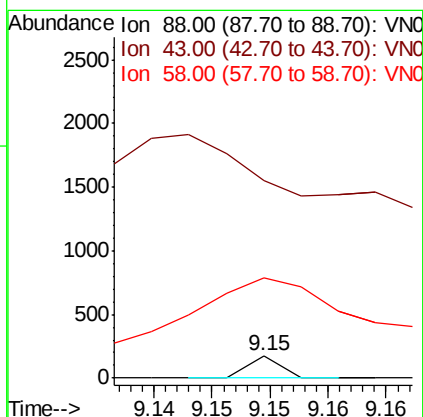



#50

Toluene-d8

Concen: 51.566 ug/l

RT: 10.06 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN064381.D

Acq: 29 Oct 2020 18:08

Instrument :

MSVOA_N

ClientSampleId :


PB132688ZHE#12

Tot Ion: 98 Resp: 520347

Ion Ratio Lower Upper




98 100

100 63.3 50.9 76.3



Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

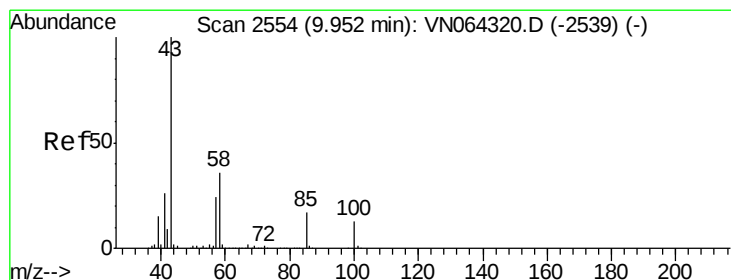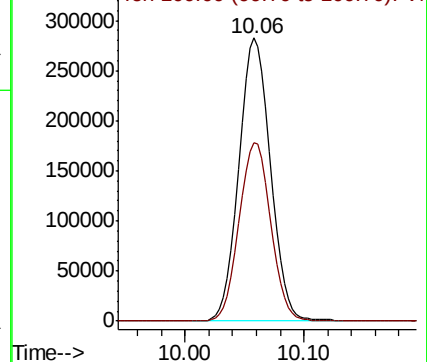

#51

4-Methyl-2-Pentanone

Concen: 1.576 ug/l

RT: 9.95 min Scan# 2554

Delta R.T. -0.00 min

Lab File: VN064381.D


Acq: 29 Oct 2020 18:08

Tgt Ion: 43 Resp: 6530

Ion Ratio Lower Upper



43 100


58 32.8 28.6 42.8



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

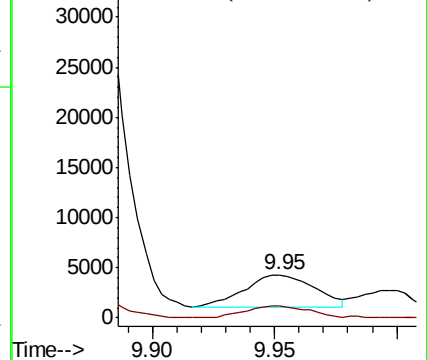







#54

cis-1,3-Dichloropropene
 Concen: 6.457 ug/l
 RT: 9.87 min Scan# 2530
 Delta R.T. 0.07 min
 Lab File: VN064381.D
 Acq: 29 Oct 2020 18:08

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132688ZHE#12




Tot Ion: 75 Resp: 33533
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.0 37.4#
 39 38.3 45.5 68.3#

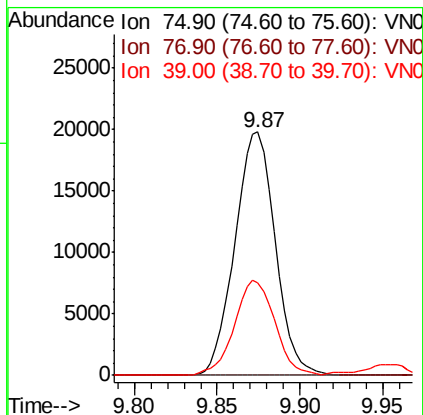


#56

Ethyl methacrylate
 Concen: 0.314 ug/l
 RT: 10.50 min Scan# 2726
 Delta R.T. 0.11 min
 Lab File: VN064381.D
 Acq: 29 Oct 2020 18:08

Tgt Ion: 69 Resp: 1361
 Ion Ratio Lower Upper
 69 100
 41 6251.6 61.4 92.2#
 39 2780.7 36.5 54.7#



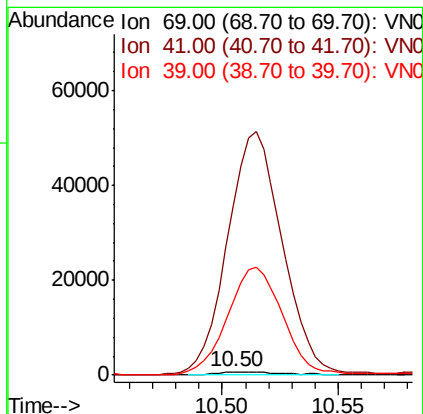





#57
 1,3-Dichloropropane
 Concen: 1.135 ug/l
 RT: 10.73 min Scan# 2797
 Delta R.T. 0.05 min
 Lab File: VN064381.D
 Acq: 29 Oct 2020 18:08




Instrument :
 MSVOA_N
 ClientSampleId :
 PB132688ZHE#12


Tot Ion: 76 Resp: 5541
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.8 38.6#

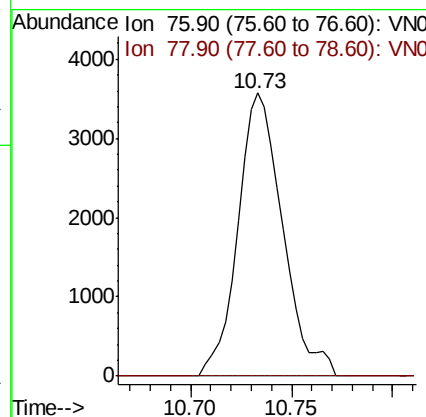

#59
 2-Hexanone
 Concen: 30.275 ug/l
 RT: 10.74 min Scan# 2798
 Delta R.T. 0.02 min
 Lab File: VN064381.D
 Acq: 29 Oct 2020 18:08

Tgt Ion: 43 Resp: 92398
 Ion Ratio Lower Upper
 43 100
 58 17.1 25.0 75.0#

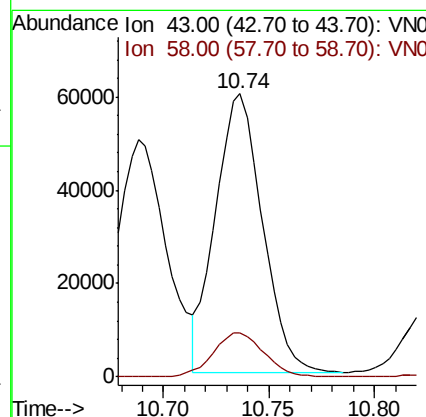



#62

4-Bromofluorobenzene

Concen: 56.725 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.00 min

Lab File: VN064381.D

Acq: 29 Oct 2020 18:08

Instrument :

MSVOA_N

ClientSampleId :

PB132688ZHE#12


Tot Ion: 95 Resp: 223174

Ion Ratio Lower Upper

95 100

174 74.8 0.0 147.4




176 72.0 0.0 143.6



Abundance Ion 94.90 (94.60 to 95.60): VN064381.D (-3215) (-)

Ion 173.80 (173.50 to 174.50): VN064381.D (-3215) (-)

Ion 175.80 (175.50 to 176.50): VN064381.D (-3215) (-)

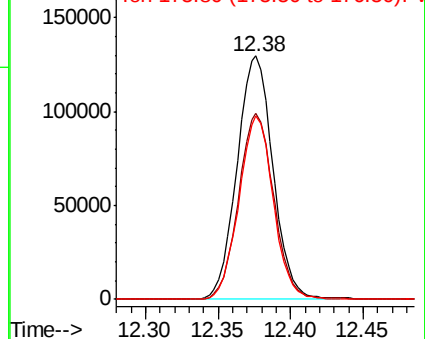

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.38 min Scan# 2998

Delta R.T. -0.00 min

Lab File: VN064381.D

Acq: 29 Oct 2020 18:08


Tgt Ion: 117 Resp: 424623

Ion Ratio Lower Upper

117 100

82 60.3 48.8 73.2



119 31.9 25.1 37.7




Abundance Ion 116.90 (116.60 to 117.60): VN064381.D (-2905) (-)

Ion 82.00 (81.70 to 82.70): VN064381.D (-2905) (-)

Ion 118.90 (118.60 to 119.60): VN064381.D (-2905) (-)

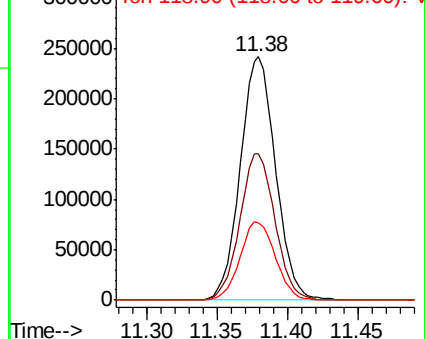



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3601

Delta R.T. 0.00 min

Lab File: VN064381.D

Acq: 29 Oct 2020 18:08

Instrument :

MSVOA_N

ClientSampleId :

PB132688ZHE#12


Tot Ion:152 Resp: 181544

Ion Ratio Lower Upper

152 100

115 61.2 31.5 94.5




150 150.3 0.0 346.2



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

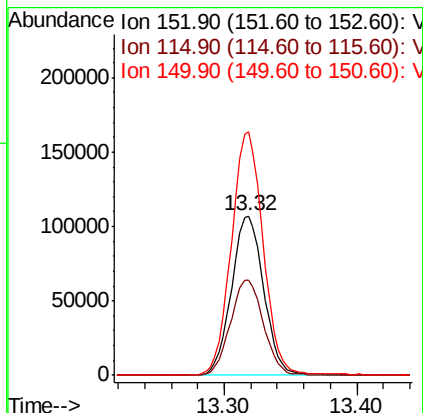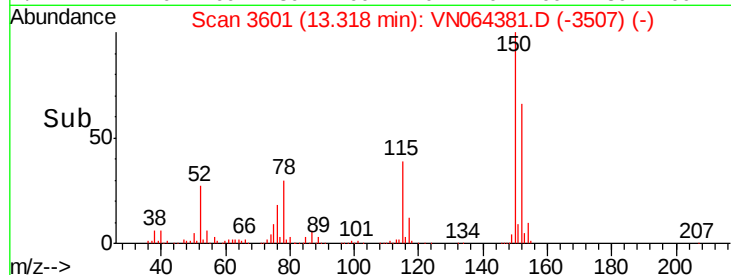

#74

N-ethyl acetate

Concen: 0.516 ug/l

RT: 12.01 min Scan# 3193

Delta R.T. -0.04 min

Lab File: VN064381.D

Acq: 29 Oct 2020 18:08

Tgt Ion: 43 Resp: 3089


Ion Ratio Lower Upper

43 100

70 0.0 30.6 45.8#

55 0.0 18.2 27.4#

61 0.0 17.6 26.4#






Abundance Ion 43.00 (42.70 to 43.70): V

Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V

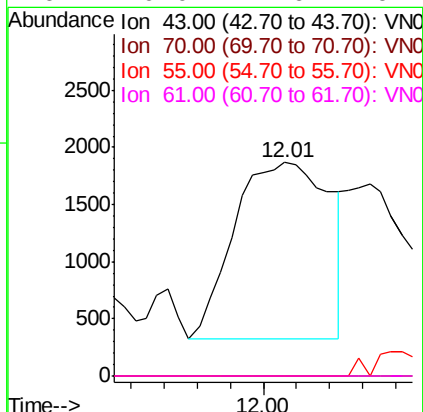



#76

1,2,3-Trichloropropane

Concen: 28.984 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN064381.D

Acq: 29 Oct 2020 18:08

Instrument :

MSVOA_N

ClientSampleId :


PB132688ZHE#12

Tot Ion: 75 Resp: 126006




Ion Ratio Lower Upper

75 100

77 1.0 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN064381.D (-3262) (-)

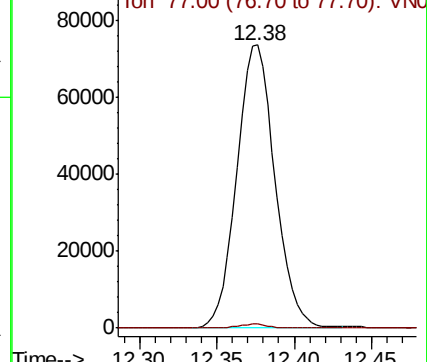

#80

1,3,5-Trimethylbenzene

Concen: 0.326 ug/l

RT: 12.70 min Scan# 3410

Delta R.T. -0.00 min

Lab File: VN064381.D


Acq: 29 Oct 2020 18:08

Tgt Ion: 105 Resp: 3749



Ion Ratio Lower Upper


105 100

120 46.3 22.9 68.8



Abundance Ion 105.00 (104.70 to 105.70): VN064381.D (-3318) (-)

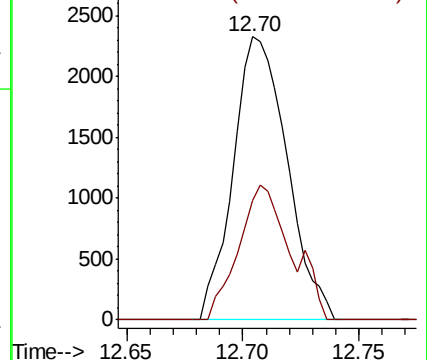



#81

trans-1,4-Dichloro-2-butene

Concen: 83.488 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.10 min

Lab File: VN064381.D

Acq: 29 Oct 2020 18:08

Instrument :

MSVOA_N

ClientSampleId :

PB132688ZHE#12


Tot Ion: 75 Resp: 126006

Ion Ratio Lower Upper

75 100

53 0.0 81.8 122.8#




89 0.0 39.9 59.9#



Abundance Ion 74.90 (74.60 to 75.60): VN064381.D (-3183) (-)

Ion 53.00 (52.70 to 53.70): VN064381.D (-3183) (-)

Ion 88.90 (88.60 to 89.60): VN064381.D (-3183) (-)

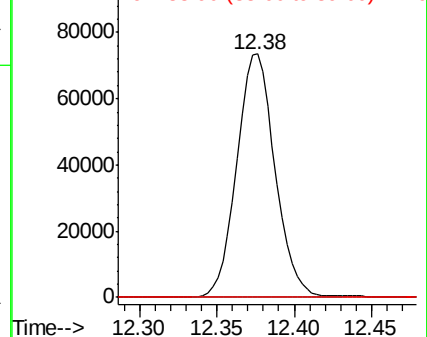

#95

Naphthalene

Concen: 2.395 ug/l

RT: 15.12 min Scan# 4160

Delta R.T. 0.02 min

Lab File: VN064381.D

Acq: 29 Oct 2020 18:08


Tgt Ion: 128 Resp: 32

Ion Ratio Lower Upper

128 100

127 0.0 10.4 15.6#

129 0.0 8.6 13.0#



Abundance Ion 128.00 (127.70 to 128.70): VN064381.D (-4062) (-)

Ion 127.00 (126.70 to 127.70): VN064381.D (-4062) (-)

Ion 129.00 (128.70 to 129.70): VN064381.D (-4062) (-)

