

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN102920\
 Data File : VN064385.D
 Acq On : 29 Oct 2020 19:42
 Operator : JC/MD
 Sample : L4549-01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BUS-WASH-RECLAMATION-PIT

Quant Time: Oct 30 05:35:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N102720W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 27 12:23:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.62	168	218002	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	382617	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	385778	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	168895	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	178205	50.87	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.74%	
35) Dibromofluoromethane	7.55	113	127658	50.03	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.06%	
50) Toluene-d8	10.06	98	489507	51.87	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.74%	
62) 4-Bromofluorobenzene	12.38	95	208245	56.59	ug/l	0.00
Spiked Amount	50.000		Recovery	=	113.18%	


Target Compounds						Qvalue
11) Tert butyl alcohol	4.75	59	414	0.814	ug/l #	70
13) Acrolein	3.55	56	32	17.949	ug/l #	1
16) Acetone	3.78	43	46633	32.658	ug/l	98
18) Methyl Acetate	4.27	43	723	0.275	ug/l #	55
20) Methylene Chloride	4.50	84	10326	4.156	ug/l	97
25) 2-Butanone	6.79	43	15346	8.724	ug/l	94
29) Tetrahydrofuran	7.17	42	689	0.603	ug/l #	59
31) Cyclohexane	7.62	56	6292	1.548	ug/l #	38
36) 1,1-Dichloropropene	7.62	75	19777	5.122	ug/l #	47
37) Ethyl Acetate	6.79	43	15346	3.934	ug/l #	75
38) Carbon Tetrachloride	7.63	117	23443	5.237	ug/l #	20
41) Methacrylonitrile	7.15	41	414	0.214	ug/l #	19
43) Isopropyl Acetate	8.13	43	24163	3.624	ug/l #	85
48) Methyl methacrylate	9.14	41	2220	0.645	ug/l #	22
51) 4-Methyl-2-Pentanone	9.95	43	79097	20.408	ug/l	100
52) Toluene	10.12	92	1134885	167.324	ug/l	98
53) t-1,3-Dichloropropene	10.13	75	15534	3.292	ug/l #	1
54) cis-1,3-Dichloropropene	9.87	75	21496	4.426	ug/l #	61
56) Ethyl methacrylate	10.32	69	5314	1.311	ug/l #	46
57) 1,3-Dichloropropane	10.74	76	1402	0.307	ug/l #	42
59) 2-Hexanone	10.74	43	25067	8.782	ug/l #	58
74) N-amyl acetate	12.01	43	4344	0.780	ug/l #	51
76) 1,2,3-Trichloropropane	12.38	75	118437	29.283	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.38	75	118437	84.350	ug/l #	8
95) Naphthalene	15.11	128	762	2.468	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN102920\
Data File : VN064385.D
Acq On : 29 Oct 2020 19:42
Operator : JC/MD
Sample : L4549-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

Quant Time: Oct 30 05:35:24 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N102720W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 27 12:23:17 2020
Response via : Initial Calibration

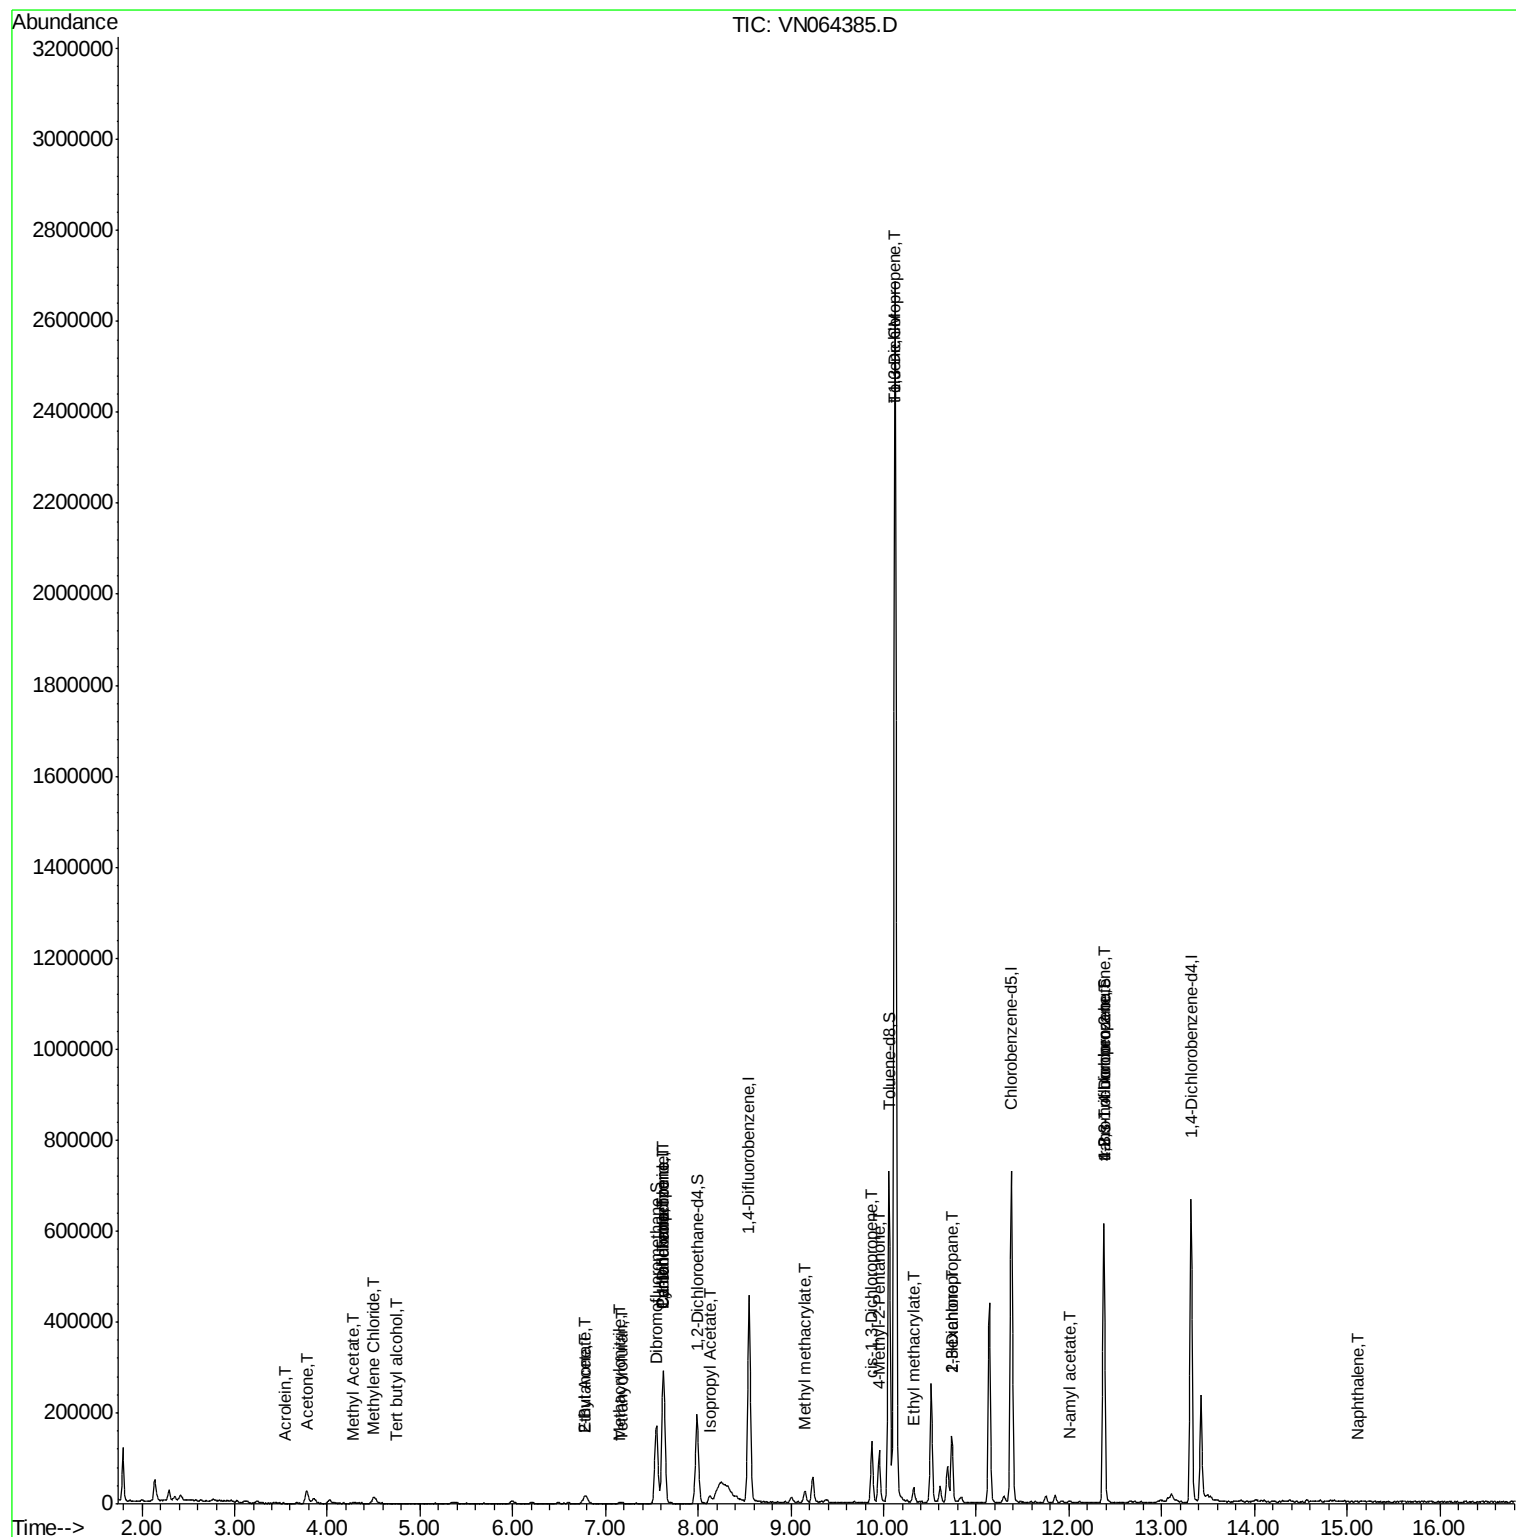

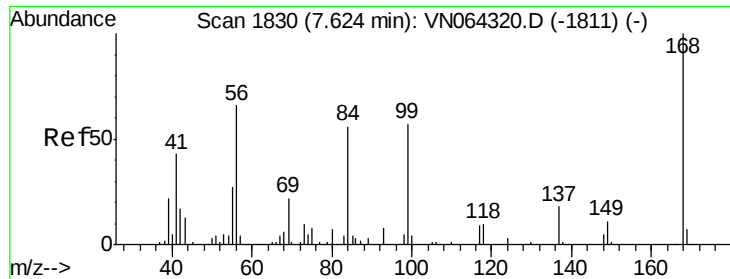

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.62 min Scan# 1830

Delta R.T. -0.00 min

Lab File: VN064385.D

Acq: 29 Oct 2020 19:42

Instrument :

MSVOA_N

ClientSampleId :


BUS-WASH-RECLAMATION-PIT

Tot Ion:168 Resp: 218002

Ion Ratio Lower Upper

168 100

99 67.0 52.7 79.1

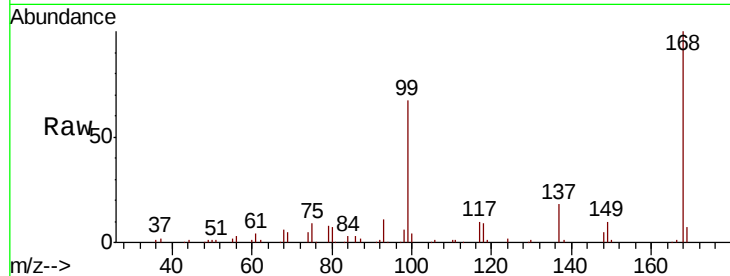

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.62

100000

80000

60000



40000

20000

0

Time-->

7.55 7.60 7.65 7.70

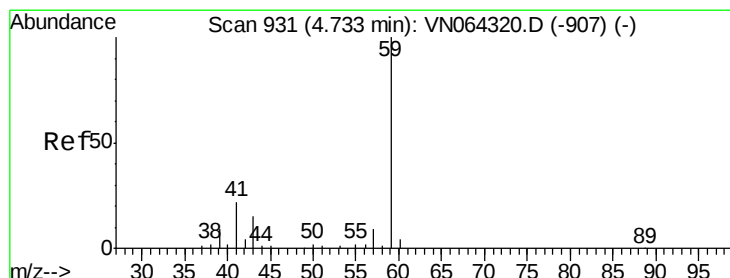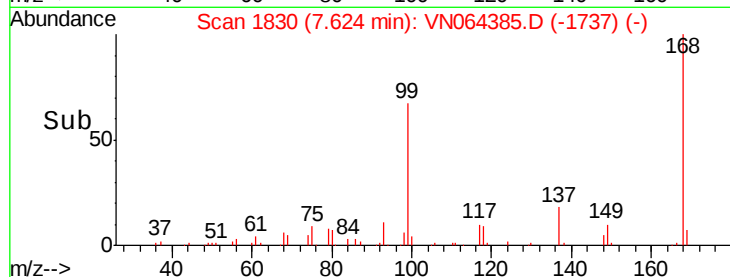

#11

Tert butyl alcohol

Concen: 0.814 ug/l

RT: 4.75 min Scan# 935

Delta R.T. 0.01 min

Lab File: VN064385.D


Acq: 29 Oct 2020 19:42

Tgt Ion: 59 Resp: 414

Ion Ratio Lower Upper

59 100

57 0.0 9.4 14.0#

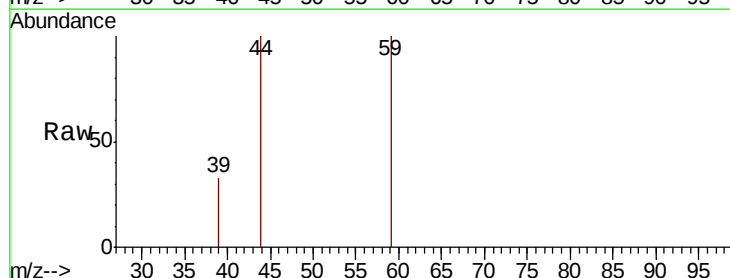

Abundance Ion 59.00 (58.70 to 59.70): VN

Ion 57.00 (56.70 to 57.70): VN

4.75

600

500

400

300


200


100

0

Time-->

4.73 4.74 4.75 4.76 4.77

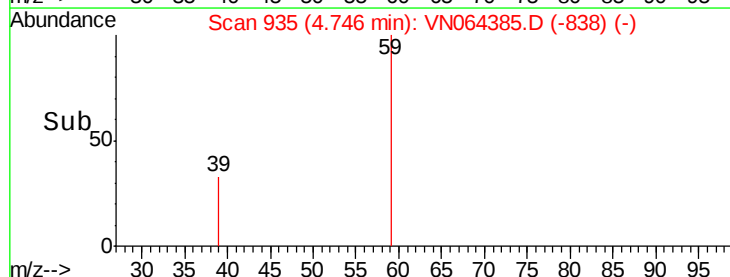



#13

Acrolein

Concen: 17.949 ug/l

RT: 3.55 min Scan# 563

Delta R.T. -0.01 min

Lab File: VN064385.D

Acq: 29 Oct 2020 19:42

Instrument :

MSVOA_N

ClientSampleId :





BUS-WASH-RECLAMATION-PIT

Tot Ion: 56 Resp: 32

Ion Ratio Lower Upper

56 100

55 356.3 62.6 94.0#

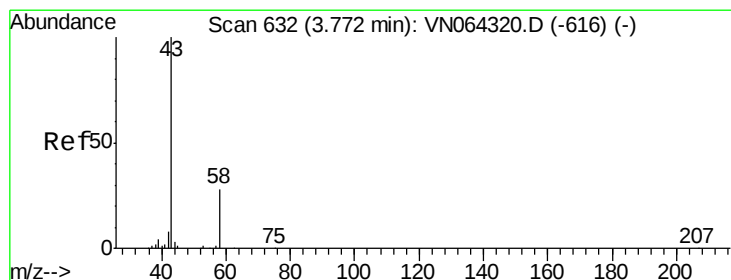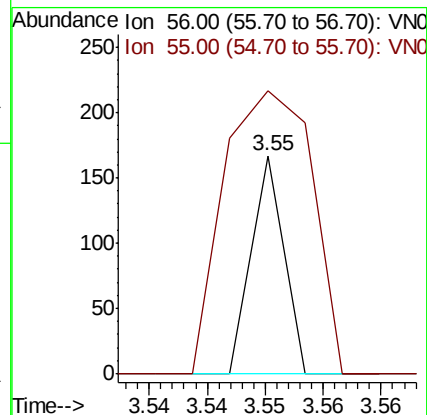

#16

Acetone

Concen: 32.658 ug/l

RT: 3.78 min Scan# 633

Delta R.T. 0.00 min

Lab File: VN064385.D




Acq: 29 Oct 2020 19:42


Tgt Ion: 43 Resp: 46633

Ion Ratio Lower Upper

43 100

58 26.4 22.1 33.1


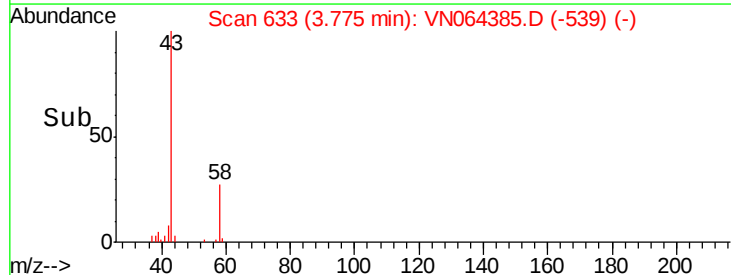
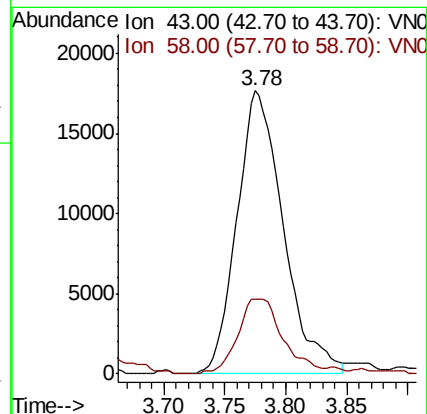





#18
Methyl Acetate
Concen: 0.275 ug/l
RT: 4.27 min Scan# 787
Delta R.T. -0.01 min
Lab File: VN064385.D
Acq: 29 Oct 2020 19:42




Instrument :
MSVOA_N
ClientSampleId :
BUS-WASH-RECLAMATION-PIT


Tot Ion: 43 Resp: 723
Ion Ratio Lower Upper
43 100
74 0.0 16.7 25.1#

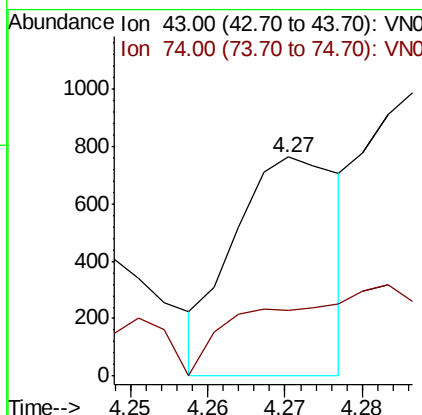

#20
Methylene Chloride
Concen: 4.156 ug/l
RT: 4.50 min Scan# 859
Delta R.T. -0.00 min
Lab File: VN064385.D
Acq: 29 Oct 2020 19:42

Tgt Ion: 84 Resp: 10326
Ion Ratio Lower Upper
84 100
49 133.5 103.6 155.4
51 40.0 31.8 47.8
86 61.3 51.3 76.9


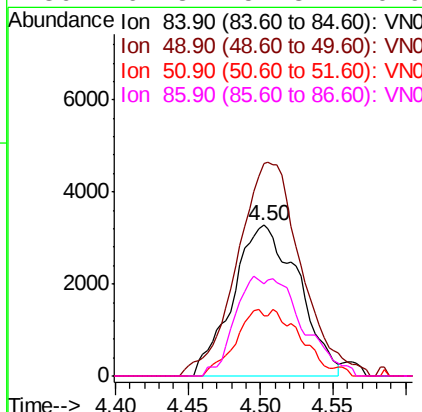




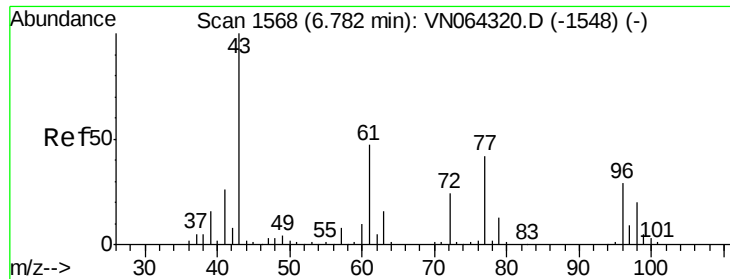

#25
2-Butanone
Concen: 8.724 ug/l
RT: 6.79 min Scan# 1571
Delta R.T. 0.01 min
Lab File: VN064385.D
Acq: 29 Oct 2020 19:42




Instrument :
MSVOA_N
ClientSampleId :
BUS-WASH-RECLAMATION-PIT


Tot Ion: 43 Resp: 15346
Ion Ratio Lower Upper
43 100
72 26.7 18.8 28.2

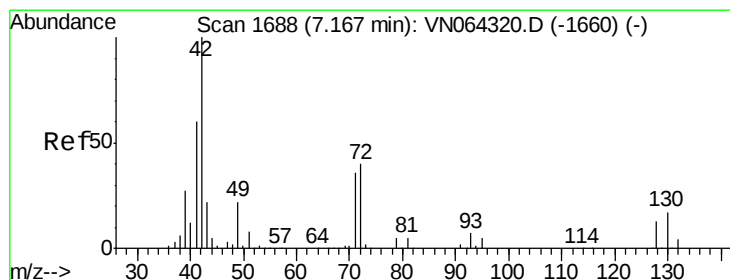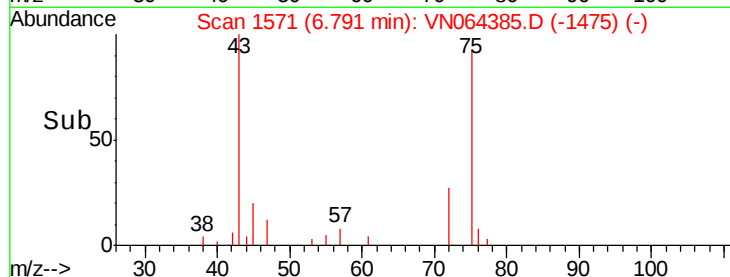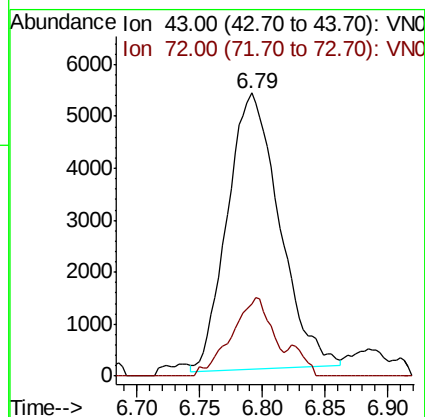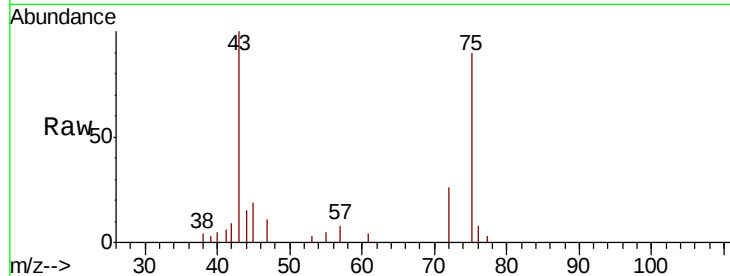

#29
Tetrahydrofuran
Concen: 0.603 ug/l
RT: 7.17 min Scan# 1690
Delta R.T. 0.01 min
Lab File: VN064385.D
Acq: 29 Oct 2020 19:42

Tgt Ion: 42 Resp: 689
Ion Ratio Lower Upper
42 100
72 0.0 31.6 47.4#
71 27.1 29.4 44.0#

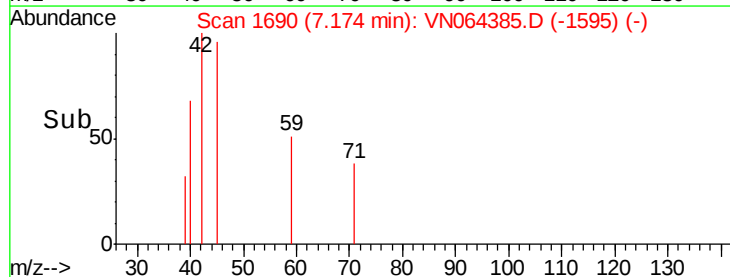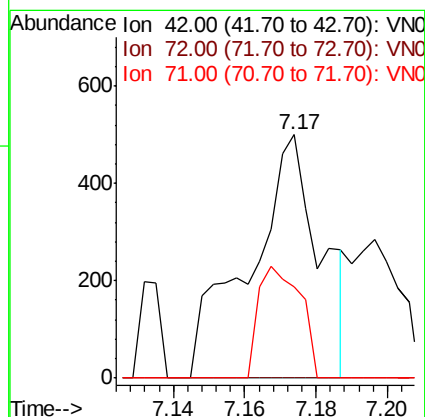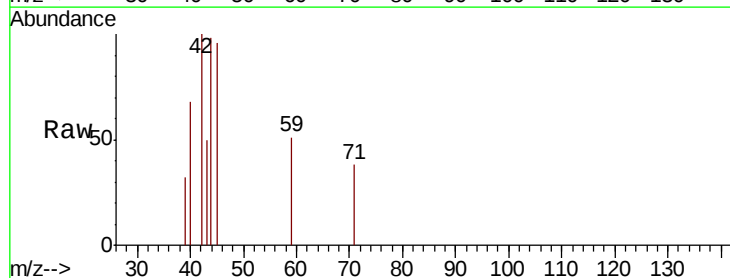







#31
Cyclohexane
Concen: 1.548 ug/l
RT: 7.62 min Scan# 1830
Delta R.T. 0.01 min
Lab File: VN064385.D
Acq: 29 Oct 2020 19:42

Instrument :
MSVOA_N
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

Tot Ion: 56 Resp: 6292
Ion Ratio Lower Upper
56 100
69 138.4 25.8 38.8#
84 94.2 66.3 99.5




Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0


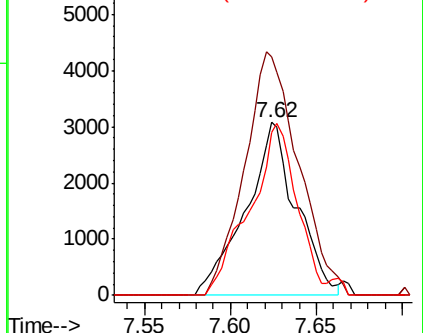



#33
1,2-Dichloroethane-d4
Concen: 50.868 ug/l
RT: 7.99 min Scan# 1943
Delta R.T. -0.00 min
Lab File: VN064385.D
Acq: 29 Oct 2020 19:42

Tgt Ion: 65 Resp: 178205
Ion Ratio Lower Upper
65 100
67 48.3 0.0 99.2



Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

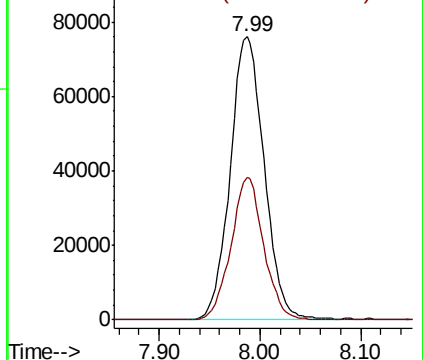







#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.55 min Scan# 2118
Delta R.T. -0.00 min
Lab File: VN064385.D
Acq: 29 Oct 2020 19:42

Instrument :
MSVOA_N
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

Tot Ion:114 Resp: 382617
Ion Ratio Lower Upper
114 100
63 22.2 0.0 44.6
88 17.9 0.0 33.4




Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VN
Ion 87.90 (87.60 to 88.60): VN


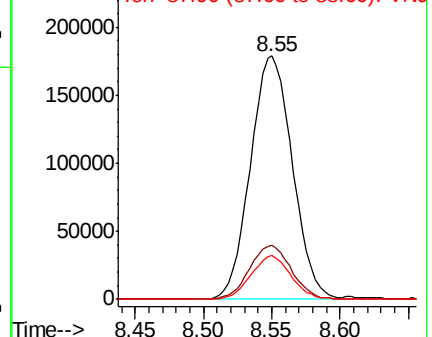



#35
Dibromofluoromethane
Concen: 50.031 ug/l
RT: 7.55 min Scan# 1807
Delta R.T. 0.00 min
Lab File: VN064385.D
Acq: 29 Oct 2020 19:42

Tgt Ion:113 Resp: 127658
Ion Ratio Lower Upper
113 100
111 103.6 81.5 122.3
192 18.0 15.0 22.4



Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

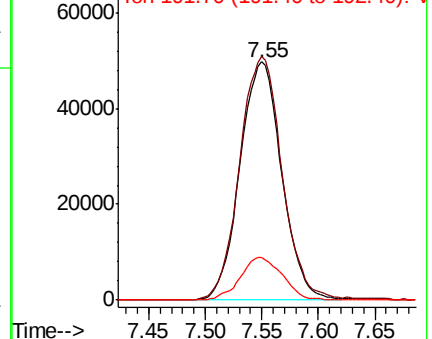



#36

1,1-Dichloropropene

Concen: 5.122 ug/l

RT: 7.62 min Scan# 1830

Delta R.T. -0.13 min

Lab File: VN064385.D

Acq: 29 Oct 2020 19:42

Instrument :

MSVOA_N

ClientSampleId :

BUS-WASH-RECLAMATION-PIT





Tot Ion: 75 Resp: 19777

Ion Ratio Lower Upper

75 100

110 4.6 16.8 50.3#

77 0.0 24.2 36.4#

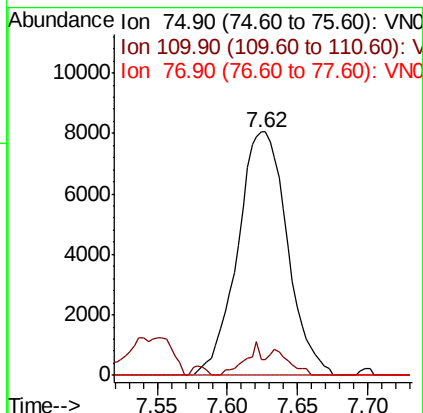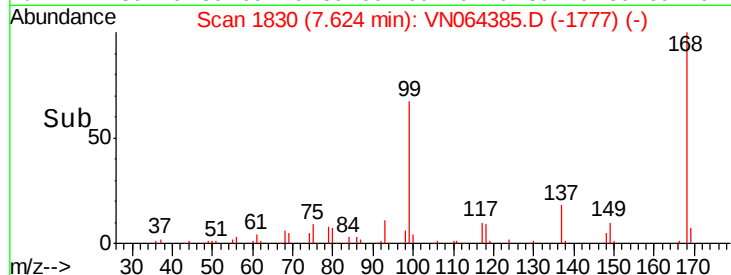

#37

Ethyl Acetate

Concen: 3.934 ug/l

RT: 6.79 min Scan# 1571

Delta R.T. -0.09 min

Lab File: VN064385.D

Acq: 29 Oct 2020 19:42




Tgt Ion: 43 Resp: 15346


Ion Ratio Lower Upper

43 100

61 2.7 10.0 15.0#

70 0.0 7.1 10.7#


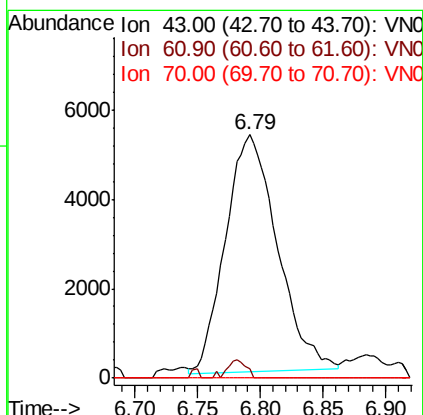






#38
Carbon Tetrachloride
Concen: 5.237 ug/l
RT: 7.63 min Scan# 1831
Delta R.T. -0.11 min
Lab File: VN064385.D
Acq: 29 Oct 2020 19:42




Instrument :
MSVOA_N
ClientSampleId :
BUS-WASH-RECLAMATION-PIT


Tot Ion:117 Resp: 23443
Ion Ratio Lower Upper
117 100
119 8.2 73.7 110.5#
121 0.0 22.8 34.2#

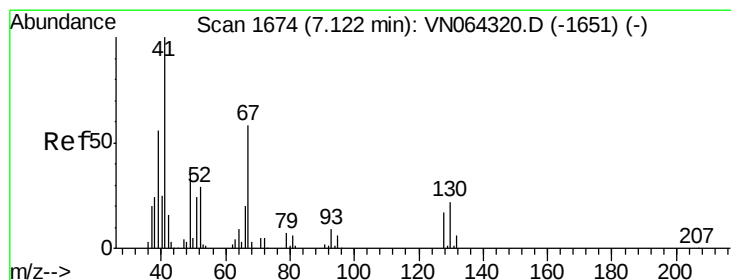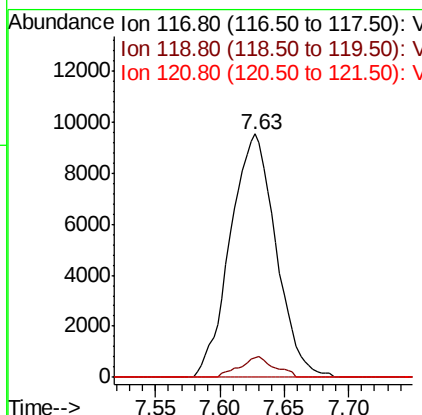

#41
Methacrylonitrile
Concen: 0.214 ug/l
RT: 7.15 min Scan# 1682
Delta R.T. 0.03 min
Lab File: VN064385.D
Acq: 29 Oct 2020 19:42

Tgt Ion: 41 Resp: 414
Ion Ratio Lower Upper
41 100
39 122.7 48.6 72.8#
67 0.0 61.4 92.2#
52 0.0 27.6 41.4#

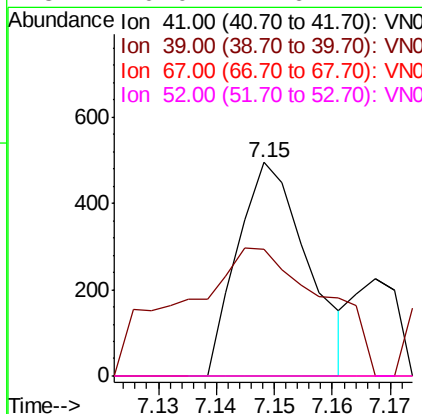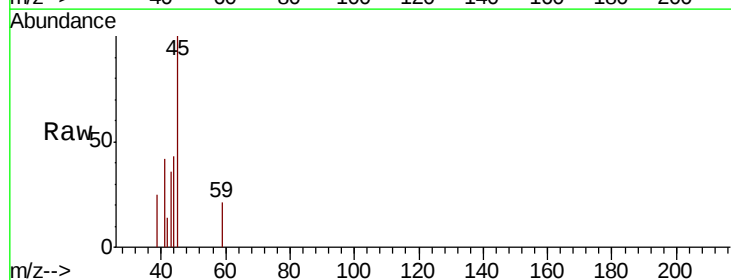

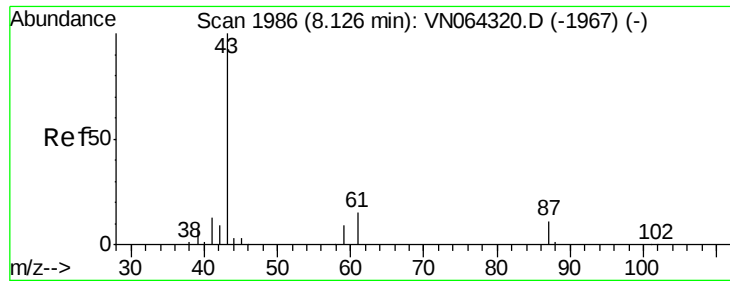

#43

Isopropyl Acetate

Concen: 3.624 ug/l

RT: 8.13 min Scan# 1986

Delta R.T. -0.00 min

Lab File: VN064385.D

Acq: 29 Oct 2020 19:42

Instrument :

MSVOA_N

ClientSampleId :

BUS-WASH-RECLAMATION-PIT


Tot Ion: 43 Resp: 24163

Ion Ratio Lower Upper




43 100

61 13.4 19.1 28.7#

87 10.3 9.3 13.9

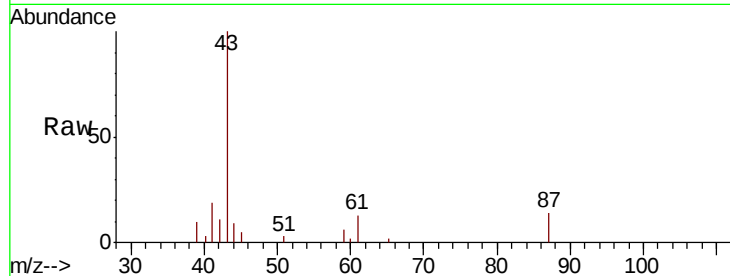

Abundance Ion 43.00 (42.70 to 43.70): VN064385.D (-1893) (-)

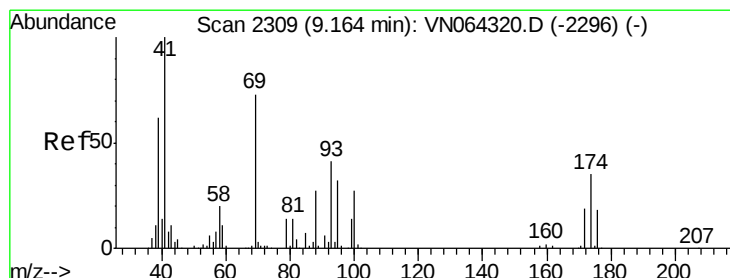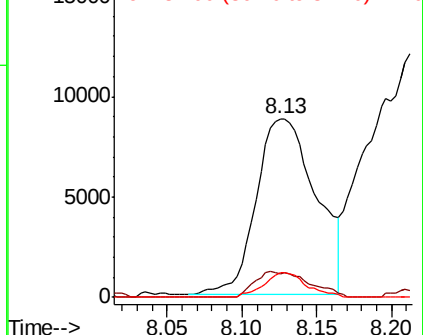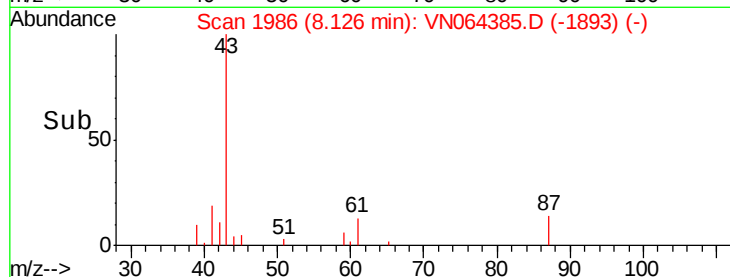

#48

Methyl methacrylate

Concen: 0.645 ug/l

RT: 9.14 min Scan# 2301

Delta R.T. -0.03 min

Lab File: VN064385.D

Acq: 29 Oct 2020 19:42


Tgt Ion: 41 Resp: 2220

Ion Ratio Lower Upper



41 100


69 0.0 59.1 88.7#

39 11.2 51.3 76.9#

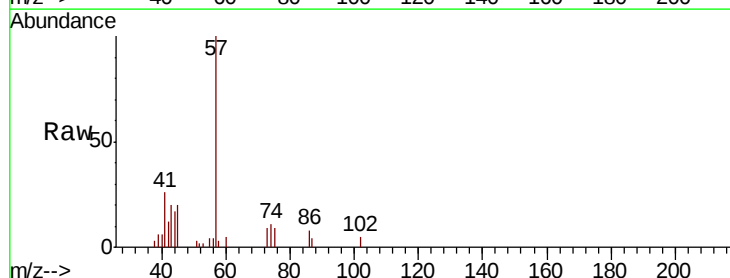

Abundance Ion 41.00 (40.70 to 41.70): VN064385.D (-2216) (-)

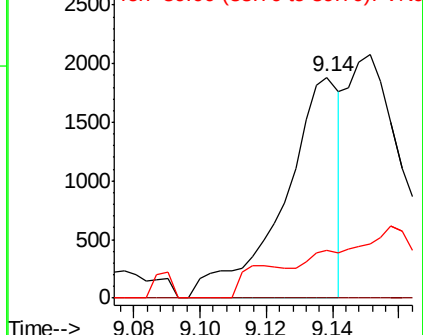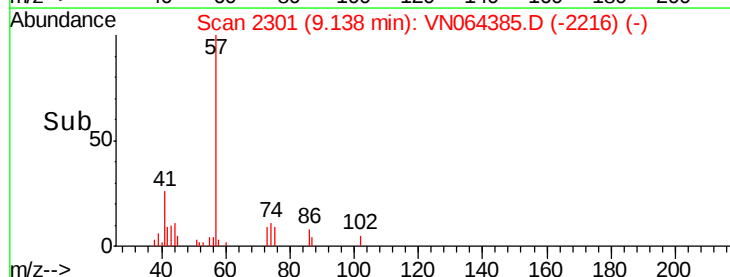



#50

Toluene-d8

Concen: 51.866 ug/l

RT: 10.06 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN064385.D

Acq: 29 Oct 2020 19:42

Instrument :

MSVOA_N

ClientSampleId :





BUS-WASH-RECLAMATION-PIT

Tot Ion: 98 Resp: 489507

Ion Ratio Lower Upper

98 100

100 63.0 50.9 76.3

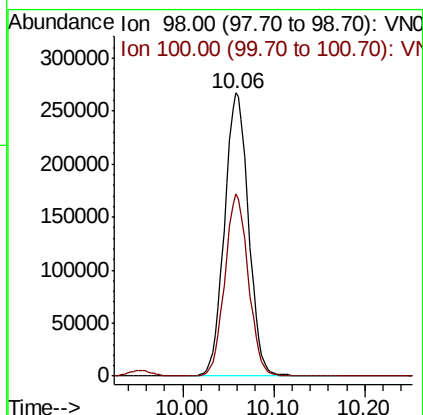

#51

4-Methyl-2-Pentanone

Concen: 20.408 ug/l

RT: 9.95 min Scan# 2554

Delta R.T. -0.00 min

Lab File: VN064385.D




Acq: 29 Oct 2020 19:42


Tgt Ion: 43 Resp: 79097

Ion Ratio Lower Upper

43 100

58 36.0 28.6 42.8

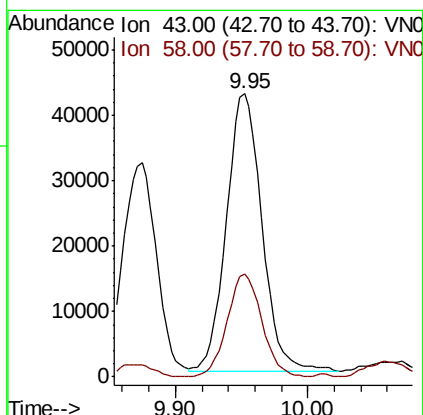



#52

Toluene

Concen: 167.324 ug/l

RT: 10.12 min Scan# 2607

Delta R.T. -0.00 min

Lab File: VN064385.D

Acq: 29 Oct 2020 19:42

Instrument :

MSVOA_N

ClientSampleId :





BUS-WASH-RECLAMATION-PIT

Tot Ion: 92 Resp: 1134885

Ion Ratio Lower Upper

92 100

91 171.7 139.9 209.9

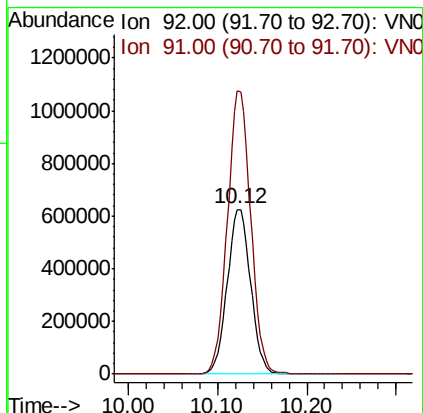

#53

t-1,3-Dichloropropene

Concen: 3.292 ug/l

RT: 10.13 min Scan# 2608

Delta R.T. -0.23 min

Lab File: VN064385.D




Acq: 29 Oct 2020 19:42


Tgt Ion: 75 Resp: 15534

Ion Ratio Lower Upper

75 100

77 177.7 24.8 37.2#

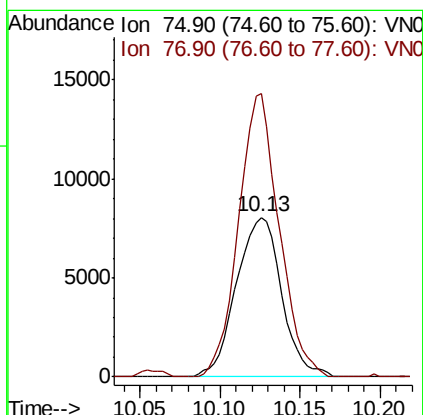




#54




cis-1,3-Dichloropropene
 Concen: 4.426 ug/l
 RT: 9.87 min Scan# 2530
 Delta R.T. 0.07 min
 Lab File: VN064385.D
 Acq: 29 Oct 2020 19:42

Instrument :
 MSVOA_N
 ClientSampleId :
 BUS-WASH-RECLAMATION-PIT

Tot Ion: 75 Resp: 21496
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.0 37.4#
 39 35.6 45.5 68.3#




Abundance Ion 74.90 (74.60 to 75.60): VN0
 Ion 76.90 (76.60 to 77.60): VN0
 Ion 39.00 (38.70 to 39.70): VN0

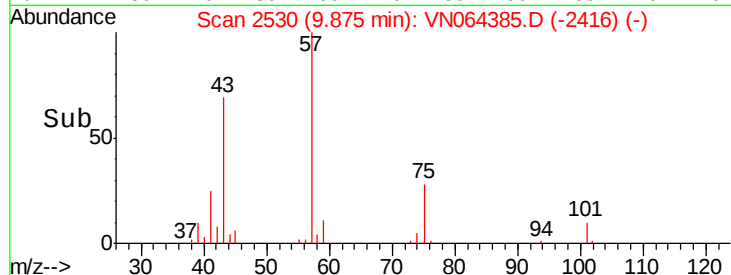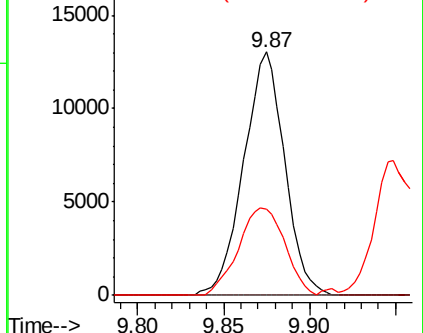



#56


Ethyl methacrylate
 Concen: 1.311 ug/l
 RT: 10.32 min Scan# 2669
 Delta R.T. -0.08 min
 Lab File: VN064385.D
 Acq: 29 Oct 2020 19:42

Tgt Ion: 69 Resp: 5314
 Ion Ratio Lower Upper
 69 100
 41 116.2 61.4 92.2#
 39 0.0 36.5 54.7#



Abundance Ion 69.00 (68.70 to 69.70): VN0
 Ion 41.00 (40.70 to 41.70): VN0
 Ion 39.00 (38.70 to 39.70): VN0




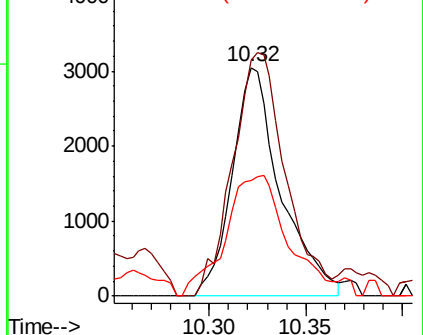




#57
 1,3-Dichloropropane
 Concen: 0.307 ug/l
 RT: 10.74 min Scan# 2798
 Delta R.T. 0.06 min
 Lab File: VN064385.D
 Acq: 29 Oct 2020 19:42




Instrument :
 MSVOA_N
 ClientSampleId :
 BUS-WASH-RECLAMATION-PIT


Tot Ion: 76 Resp: 1402
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.8 38.6#

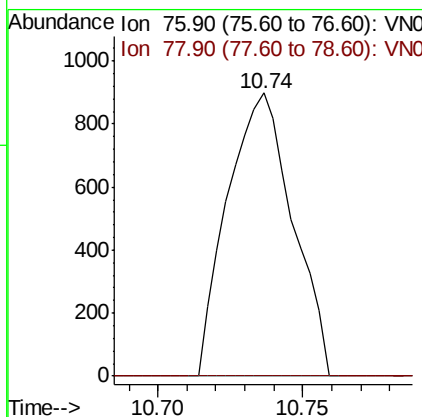

#59
 2-Hexanone
 Concen: 8.782 ug/l
 RT: 10.74 min Scan# 2798
 Delta R.T. 0.02 min
 Lab File: VN064385.D
 Acq: 29 Oct 2020 19:42

Tgt Ion: 43 Resp: 25067
 Ion Ratio Lower Upper
 43 100
 58 21.1 25.0 75.0#



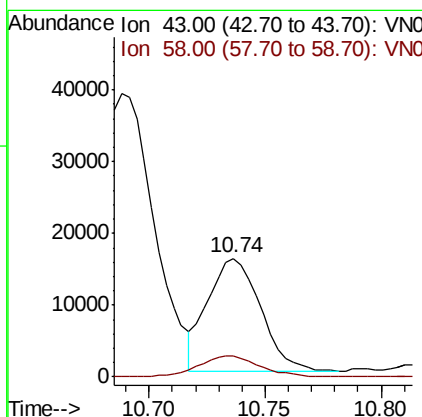



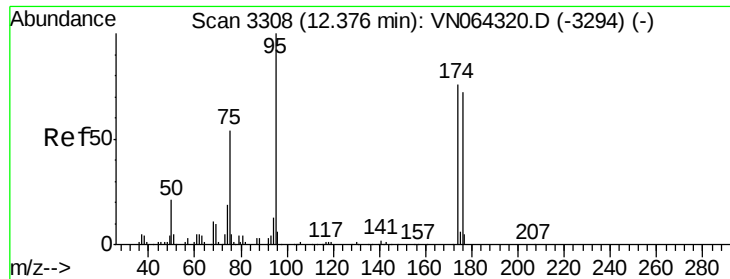

#62
4-Bromofluorobenzene
Concen: 56.591 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. -0.00 min
Lab File: VN064385.D
Acq: 29 Oct 2020 19:42




Instrument :
MSVOA_N
ClientSampleId :
BUS-WASH-RECLAMATION-PIT


Tot Ion: 95 Resp: 208245
Ion Ratio Lower Upper
95 100
174 73.1 0.0 147.4
176 71.4 0.0 143.6

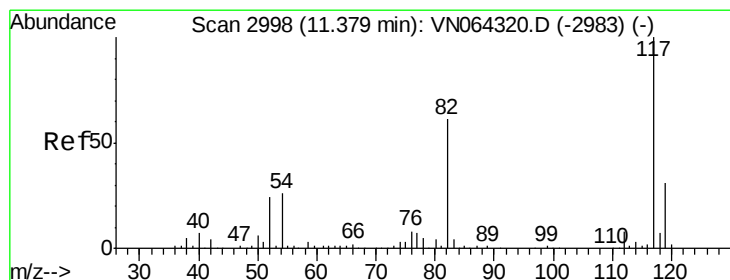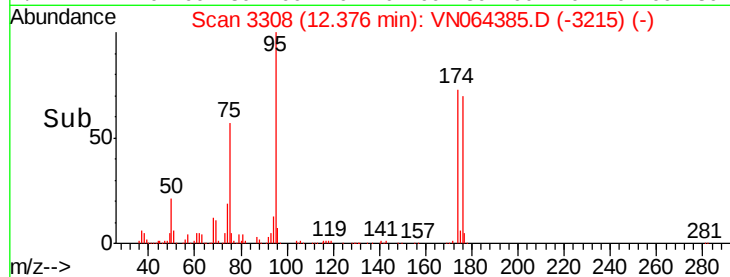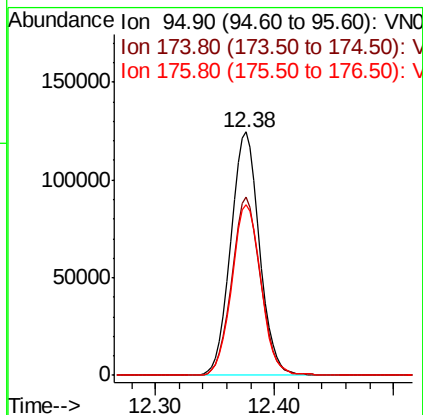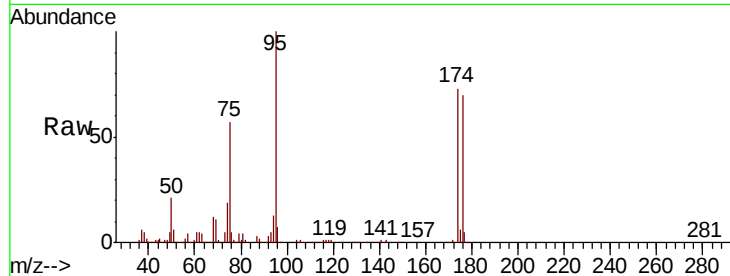

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. -0.00 min
Lab File: VN064385.D
Acq: 29 Oct 2020 19:42

Tgt Ion: 117 Resp: 385778
Ion Ratio Lower Upper
117 100
82 59.8 48.8 73.2
119 32.2 25.1 37.7

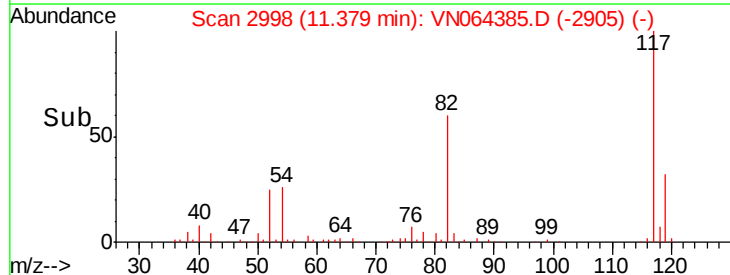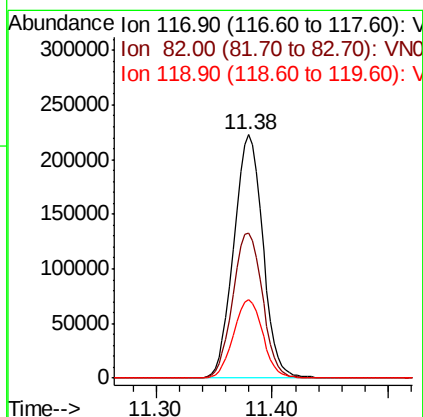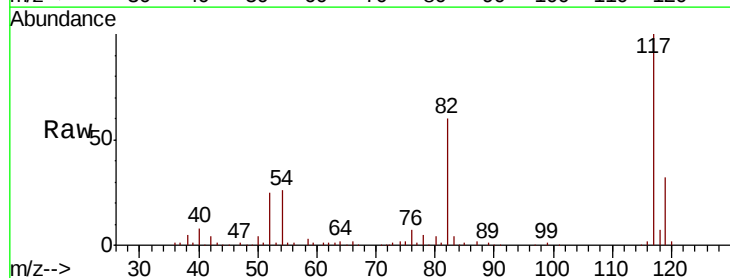



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3601

Delta R.T. 0.00 min

Lab File: VN064385.D

Acq: 29 Oct 2020 19:42

Instrument :

MSVOA_N

ClientSampleId :

BUS-WASH-RECLAMATION-PIT


Tot Ion:152 Resp: 168895

Ion Ratio Lower Upper

152 100

115 63.5 31.5 94.5




150 157.2 0.0 346.2



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

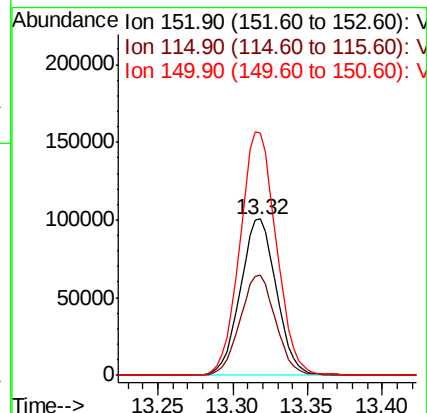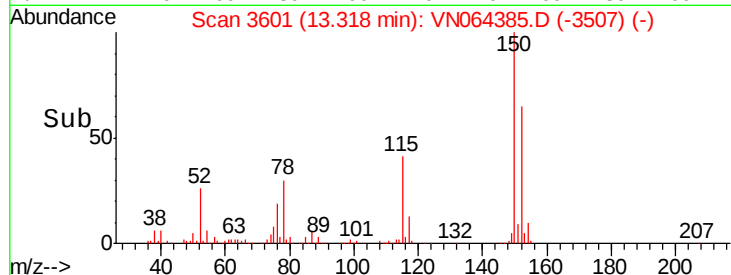

#74

N-ethyl acetate

Concen: 0.780 ug/l

RT: 12.01 min Scan# 3194

Delta R.T. -0.03 min

Lab File: VN064385.D

Acq: 29 Oct 2020 19:42

Tgt Ion: 43 Resp: 4344


Ion Ratio Lower Upper

43 100

70 0.0 30.6 45.8#

55 9.1 18.2 27.4#

61 0.0 17.6 26.4#






Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

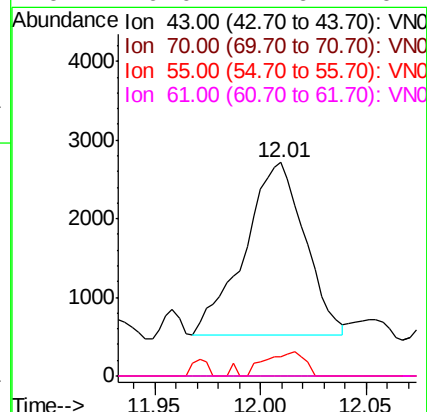

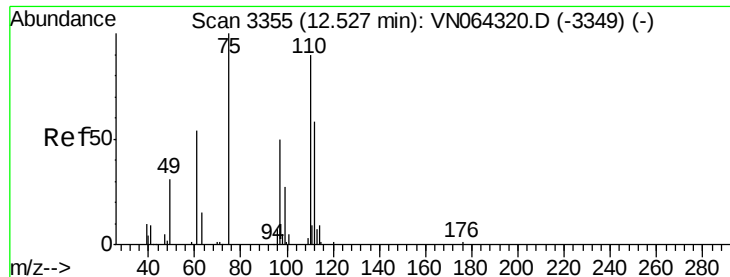

#76

1,2,3-Trichloropropane

Concen: 29.283 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN064385.D

Acq: 29 Oct 2020 19:42

Instrument :

MSVOA_N

ClientSampleId :





BUS-WASH-RECLAMATION-PIT

Tot Ion: 75 Resp: 118437

Ion Ratio Lower Upper

75 100

77 1.0 0.0 0.0#

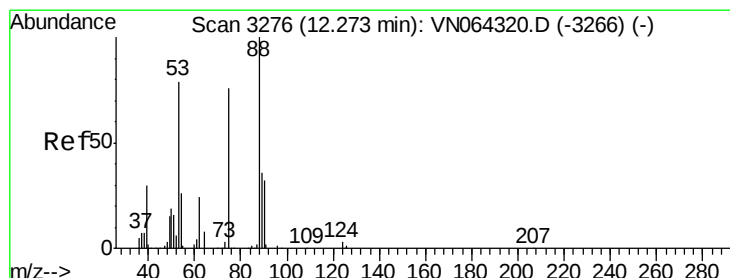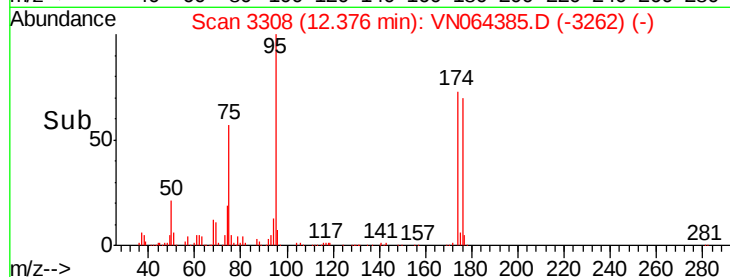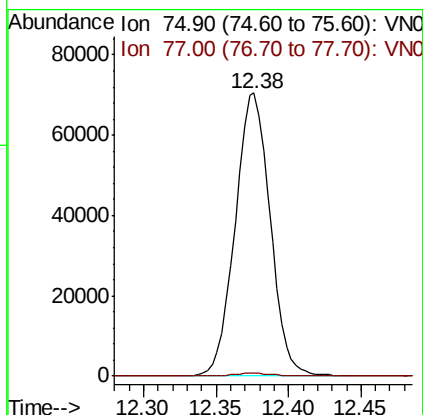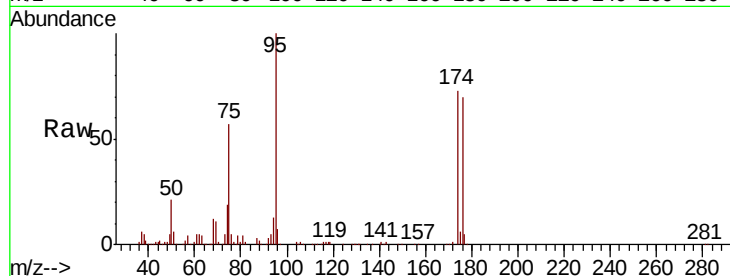

#81

trans-1,4-Dichloro-2-butene

Concen: 84.350 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.10 min

Lab File: VN064385.D

Acq: 29 Oct 2020 19:42




Tgt Ion: 75 Resp: 118437


Ion Ratio Lower Upper

75 100

53 0.0 81.8 122.8#

89 0.1 39.9 59.9#

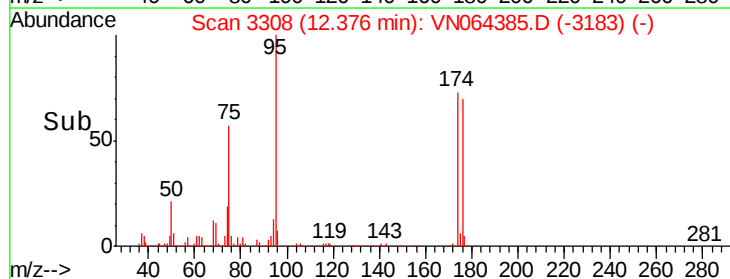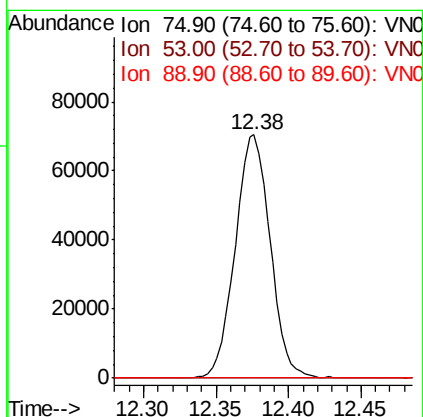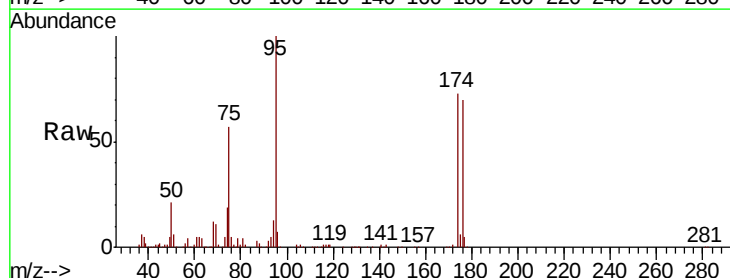

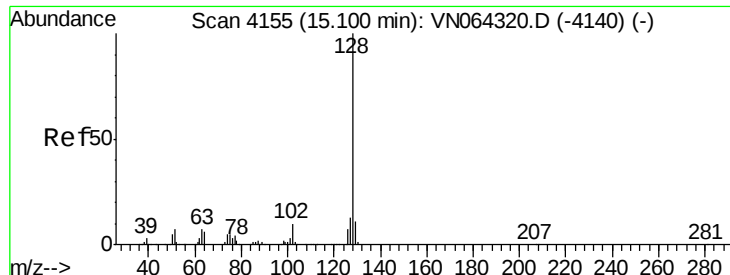

#95

Naphthalene

Concen: 2.468 ug/l

RT: 15.11 min Scan# 4158

Delta R.T. 0.01 min

Lab File: VN064385.D

Acq: 29 Oct 2020 19:42

Instrument :

MSVOA_N

ClientSampleId :

BUS-WASH-RECLAMATION-PIT


Tot Ion:128 Resp: 762

Ion Ratio Lower Upper

128 100

127 0.0 10.4 15.6#

129 0.0 8.6 13.0#

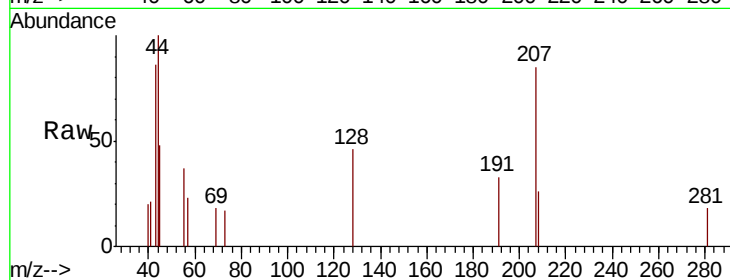

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

