


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN102920\  
 Data File : VN064364.D  
 Acq On : 29 Oct 2020 9:24  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N102720W.M  
 Title : SW846 8260  
 Last Update : Tue Oct 27 12:23:17 2020

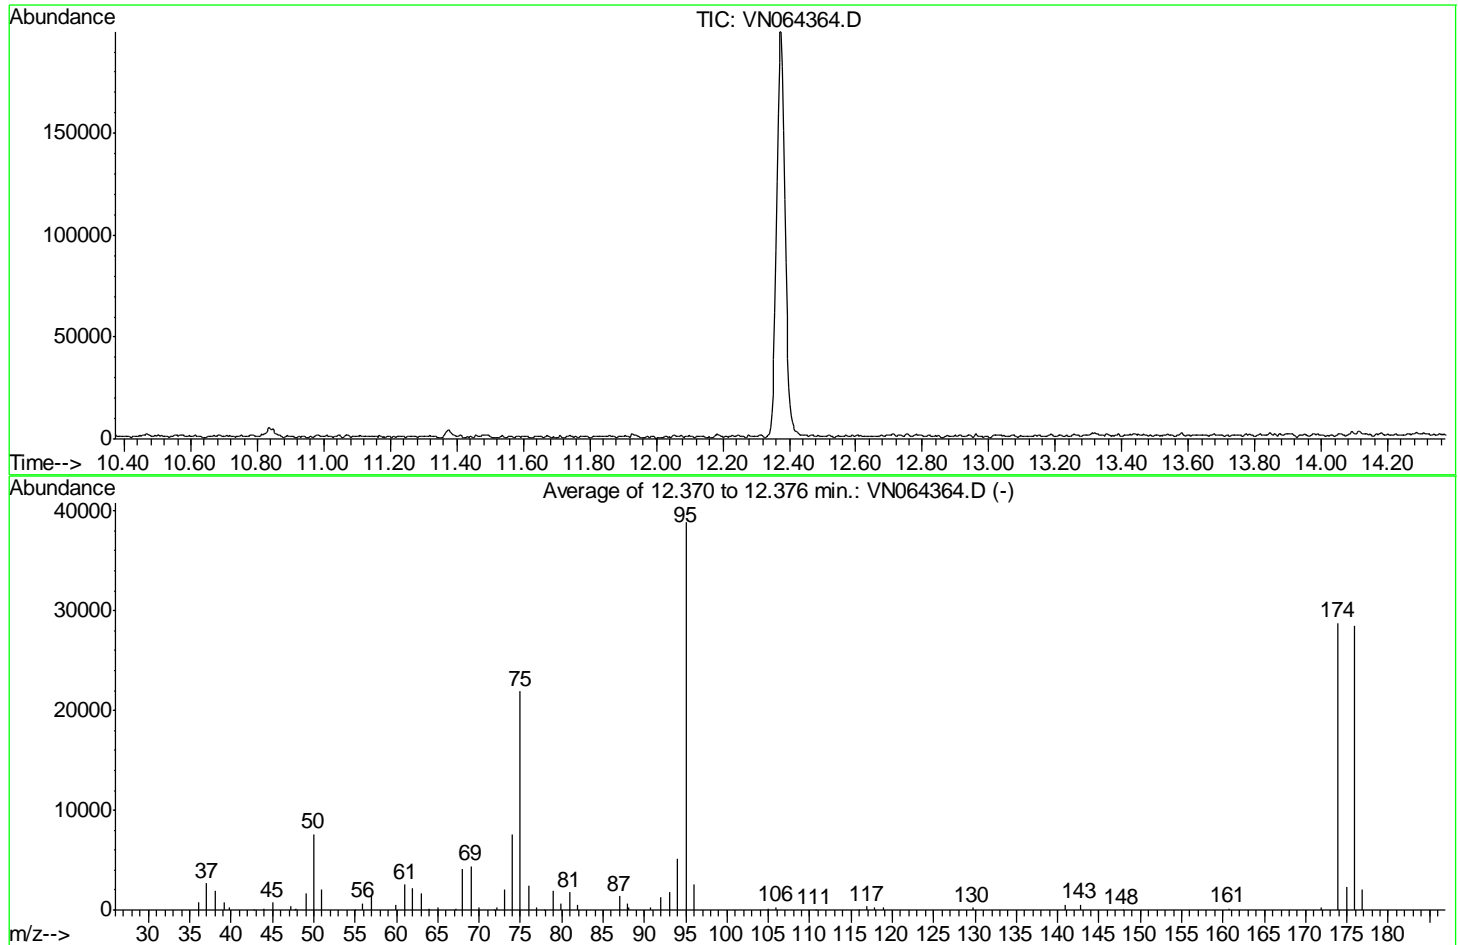

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	7581	PASS
75	95	30	60	56.4	21920	PASS
95	95	100	100	100.0	38864	PASS
96	95	5	9	6.7	2608	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.0	28770	PASS
175	174	5	9	8.1	2344	PASS
176	174	95	101	99.2	28544	PASS
177	176	5	9	7.2	2042	PASS