

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102925\
 Data File : VN088153.D
 Acq On : 29 Oct 2025 12:42
 Operator : JC\MD
 Sample : Q3468-06DL 10X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-12DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
 Title : SW846 8260

Signal : TIC: VN088153.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.536	89	99	108	rBV2	20555	42036	1.39%	0.171%
2	3.265	216	223	234	rVB4	24625	59113	1.96%	0.240%
3	3.659	282	290	302	rVB5	15037	48288	1.60%	0.196%
4	3.865	318	325	333	rBV5	14790	35162	1.17%	0.143%
5	4.153	366	374	381	rVB5	12261	34693	1.15%	0.141%
6	5.383	569	583	585	rBV5	14790	43700	1.45%	0.177%
7	7.312	902	911	920	rBV3	22637	65280	2.17%	0.265%
8	7.424	922	930	938	rBV3	11093	30459	1.01%	0.124%
9	8.147	1044	1053	1058	rBV	215710	518331	17.19%	2.105%
10	8.206	1058	1063	1078	rVB	314775	746816	24.77%	3.033%
11	8.576	1113	1126	1138	rBV3	364805	1241008	41.16%	5.040%
12	9.082	1202	1212	1226	rBV	588171	1213202	40.24%	4.927%
13	9.576	1283	1296	1303	rBV6	10895	33798	1.12%	0.137%
14	10.547	1450	1461	1467	rBV	836512	1585461	52.59%	6.439%
15	10.612	1467	1472	1487	rVV	329889	605399	20.08%	2.459%
16	10.741	1487	1494	1500	rVV3	41223	70237	2.33%	0.285%
17	10.812	1500	1506	1512	rVB	40580	71003	2.36%	0.288%
18	11.847	1673	1682	1690	rBV	831901	1538728	51.04%	6.249%
19	11.941	1690	1698	1709	rVV	1767195	3014925	100.00%	12.244%
20	12.053	1709	1717	1729	rVB	902536	1624879	53.89%	6.599%
21	12.376	1764	1772	1785	rBV	1223999	2126488	70.53%	8.636%
22	12.676	1816	1823	1831	rBV	45008	81404	2.70%	0.331%
23	12.829	1841	1849	1867	rBV	594723	1145524	38.00%	4.652%
24	13.017	1873	1881	1887	rBV	87682	155832	5.17%	0.633%
25	13.111	1887	1897	1912	rVB	142384	352334	11.69%	1.431%
26	13.311	1924	1931	1944	rBV	588628	1001028	33.20%	4.065%
27	13.459	1949	1956	1968	rVV	1152550	1900660	63.04%	7.719%
28	13.770	2002	2009	2011	rBV	914007	1551967	51.48%	6.303%
29	13.929	2030	2036	2037	rBV2	36804	52136	1.73%	0.212%
30	13.970	2037	2043	2059	rVB	787020	1435489	47.61%	5.830%
31	14.153	2068	2074	2080	rBV2	83810	156777	5.20%	0.637%
32	14.217	2080	2085	2089	rBV	55574	96874	3.21%	0.393%
33	14.306	2095	2100	2107	rVV	93976	152384	5.05%	0.619%
34	14.376	2107	2112	2115	rVV3	25229	46027	1.53%	0.187%
35	14.417	2115	2119	2128	rVB2	108502	194920	6.47%	0.792%
36	14.547	2137	2141	2148	rVB2	38340	62375	2.07%	0.253%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102925\
Data File : VN088153.D
Acq On : 29 Oct 2025 12:42
Operator : JC\MD
Sample : Q3468-06DL 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-12DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M

Title : SW846 8260

37	14.629	2148	2155	2158	rBV2	53996	92158	3.06%	0.374%
38	14.670	2158	2162	2168	rVB	53168	86858	2.88%	0.353%
39	14.905	2196	2202	2214	rVB	68559	125040	4.15%	0.508%
40	15.029	2214	2223	2231	rBV3	164449	356252	11.82%	1.447%
41	15.188	2241	2250	2255	rBV5	27364	55317	1.83%	0.225%
42	15.294	2260	2268	2274	rBV8	14980	40457	1.34%	0.164%
43	15.405	2279	2287	2296	rVB6	14492	38644	1.28%	0.157%
44	15.611	2314	2322	2334	rBV	296918	605558	20.09%	2.459%
45	15.717	2334	2340	2347	rVV2	40396	88371	2.93%	0.359%




Sum of corrected areas: 24623392

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102925\
Data File : VN088153.D
Acq On : 29 Oct 2025 12:42
Operator : JC\MD
Sample : Q3468-06DL 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-12DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

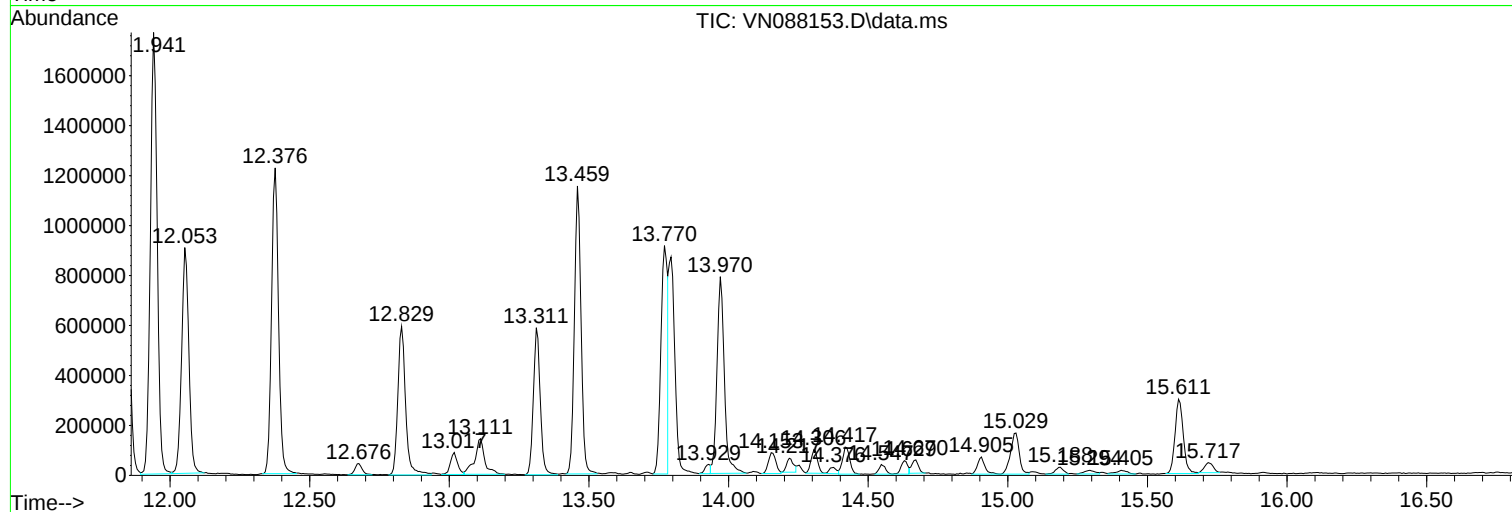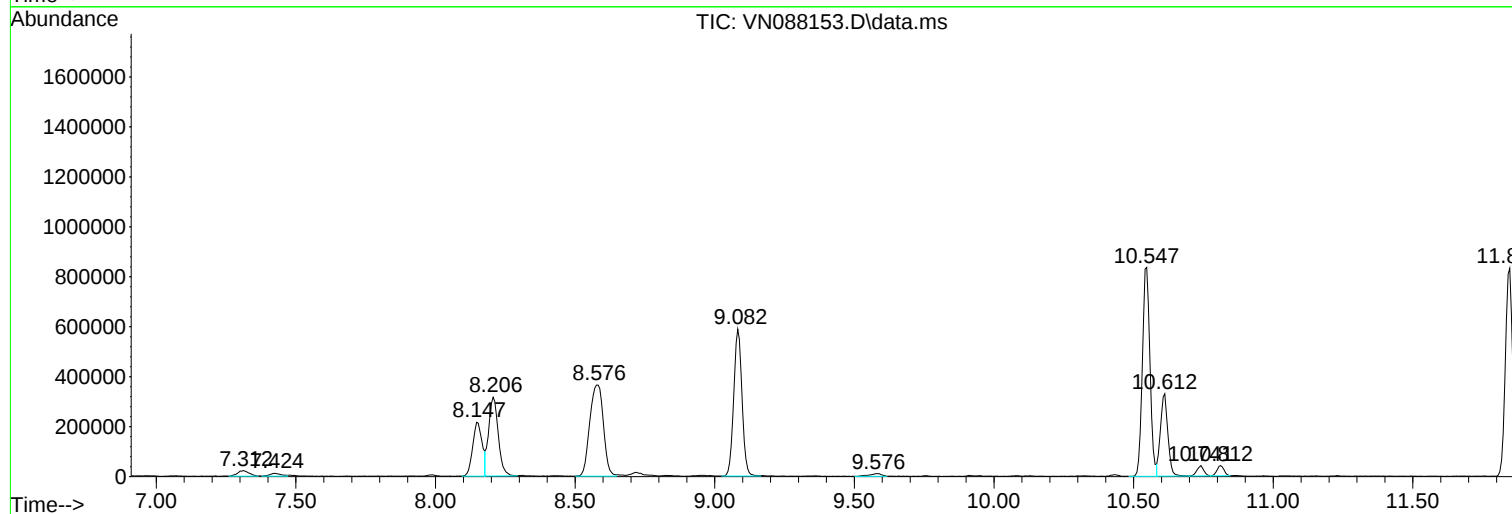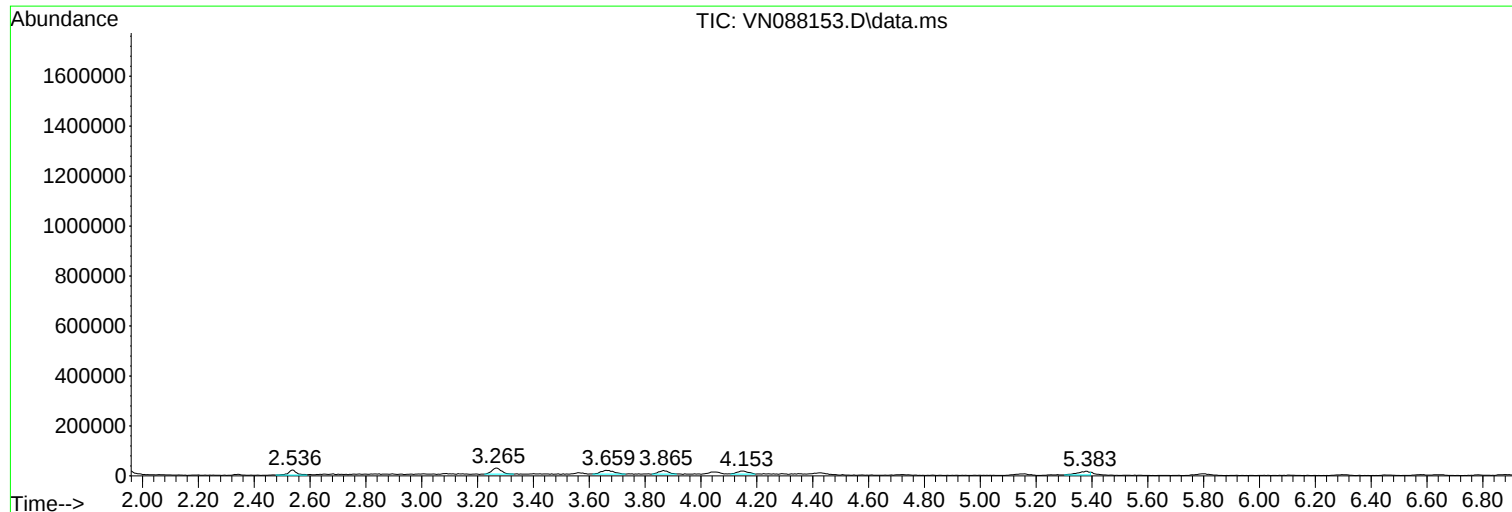

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102925\
Data File : VN088153.D
Acq On : 29 Oct 2025 12:42
Operator : JC\MD
Sample : Q3468-06DL 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-12DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102925\
Data File : VN088153.D
Acq On : 29 Oct 2025 12:42
Operator : JC\MD
Sample : Q3468-06DL 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-12DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc