


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN103019\
Data File : VN059014.D
Acq On : 30 Oct 2019 8:37
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Title : SW846 8260
Last Update : Sat Oct 19 00:16:20 2019

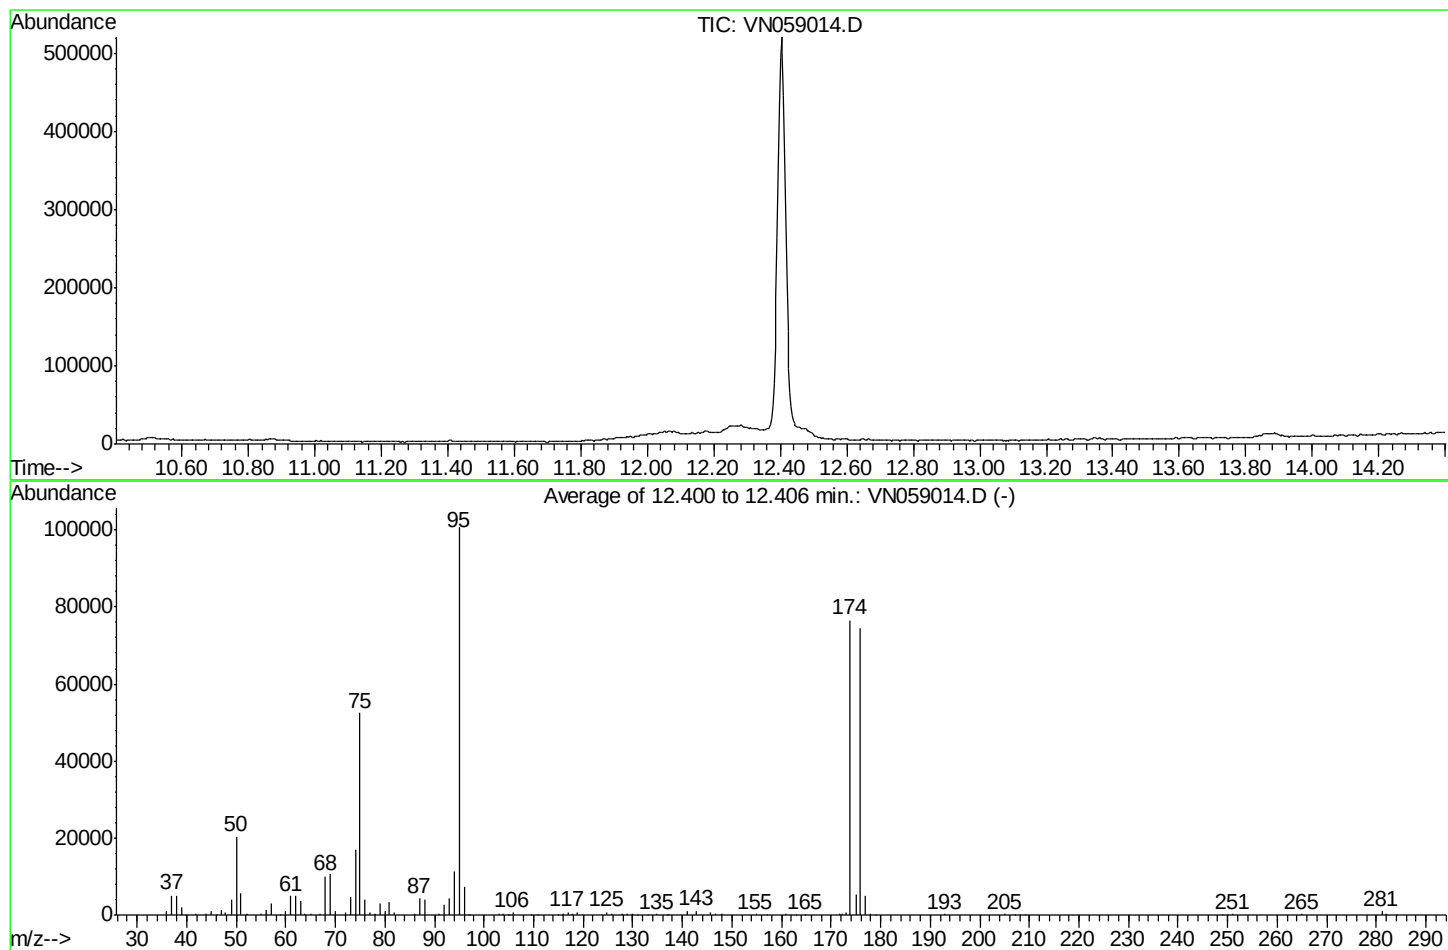

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	20410	PASS
75	95	30	60	52.0	52392	PASS
95	95	100	100	100.0	100677	PASS
96	95	5	9	7.3	7380	PASS
173	174	0.00	2	1.0	773	PASS
174	95	50	100	76.0	76493	PASS
175	174	5	9	7.1	5467	PASS
176	174	95	101	97.5	74576	PASS
177	176	5	9	6.9	5123	PASS