
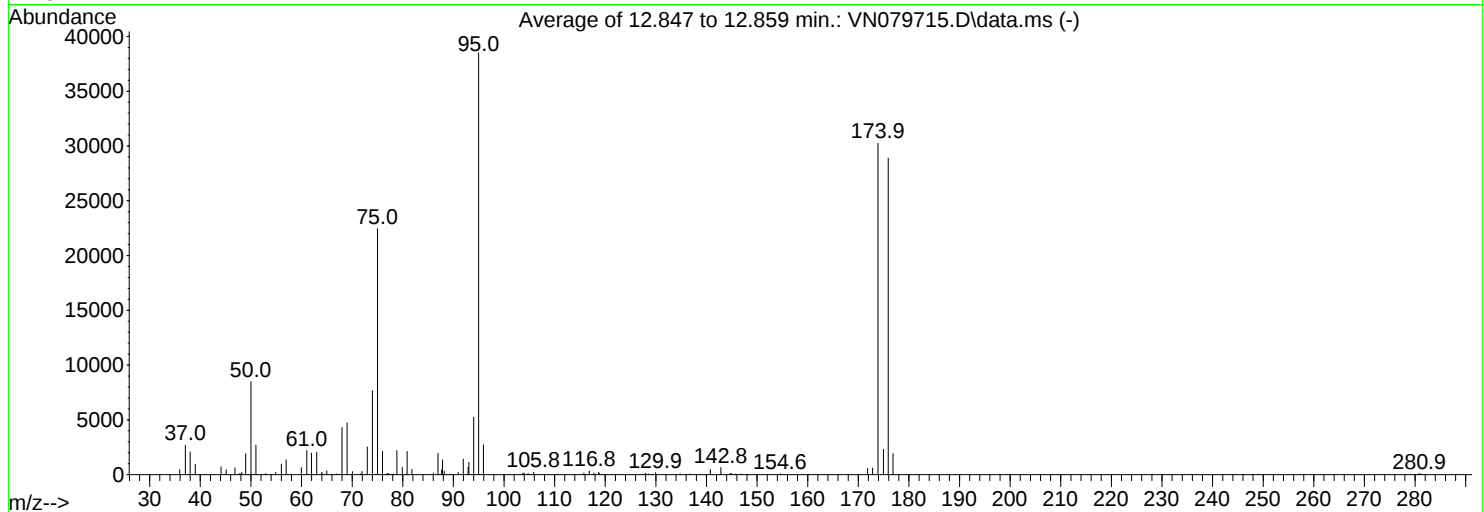


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN103023\
Data File : VN079715.D
Acq On : 30 Oct 2023 09:22
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103023W.M
Title : SW846 8260
Last Update : Tue Oct 31 07:23:24 2023

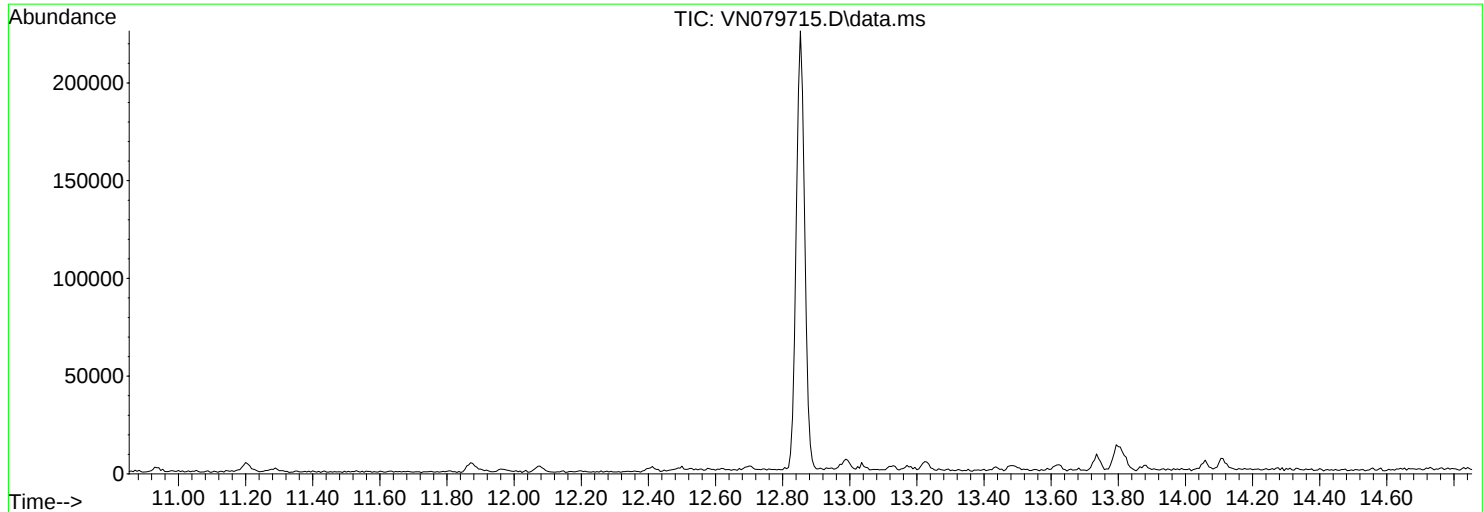

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	8505	PASS
75	95	30	60	58.3	22445	PASS
95	95	100	100	100.0	38501	PASS
96	95	5	9	7.1	2720	PASS
173	174	0.00	2	2.0	602	PASS
174	95	50	100	78.6	30251	PASS
175	174	5	9	7.6	2311	PASS
176	174	95	101	95.6	28909	PASS
177	176	5	9	6.7	1923	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	452	48.95	1914	63.00	2048	74.00	766
37.05	2678	50.00	8505	63.90	136	75.00	2244
38.00	2068	51.00	2697	64.05	207	76.00	214
39.00	935	52.95	105	65.00	348	76.70	6
39.90	16	54.90	205	66.90	69	77.00	102
44.10	722	56.00	971	68.00	4301	77.20	96
45.10	436	56.95	1359	69.00	4735	77.70	51
46.85	632	58.00	53	70.05	275	78.20	59
47.70	95	59.95	646	71.70	63	78.85	2191
47.90	91	61.05	2208	71.95	292	79.90	674
48.20	201	61.95	1966	73.00	2522	80.85	2113

Average of 12.847 to 12.859 min.: VN079715.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.80	489	95.00	38501	127.80	52	146.90	64
86.05	142	95.95	2720	128.00	127	154.60	57
86.95	1949	103.70	114	128.60	52	171.85	565
87.70	420	103.95	165	129.95	194	172.80	602
87.85	1349	104.75	116	134.80	73	173.90	30251
88.20	309	105.85	218	136.80	53	174.95	2311
90.95	209	115.80	152	140.75	475	175.90	28909
91.95	1422	116.85	334	142.85	641	176.85	1923
92.90	679	117.75	153	144.70	97	280.60	81
93.05	1125	118.70	216	144.90	119	280.90	91
94.00	5226	118.90	99	145.80	60	281.20	65

Instrument :

MSVOA_N

ClientSampleId :

BFB