


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN103118\
Data File : VN052065.D
Acq On : 31 Oct 2018 10:12
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N103018W.M
Title : SW846 8260
Last Update : Wed Oct 31 02:45:22 2018

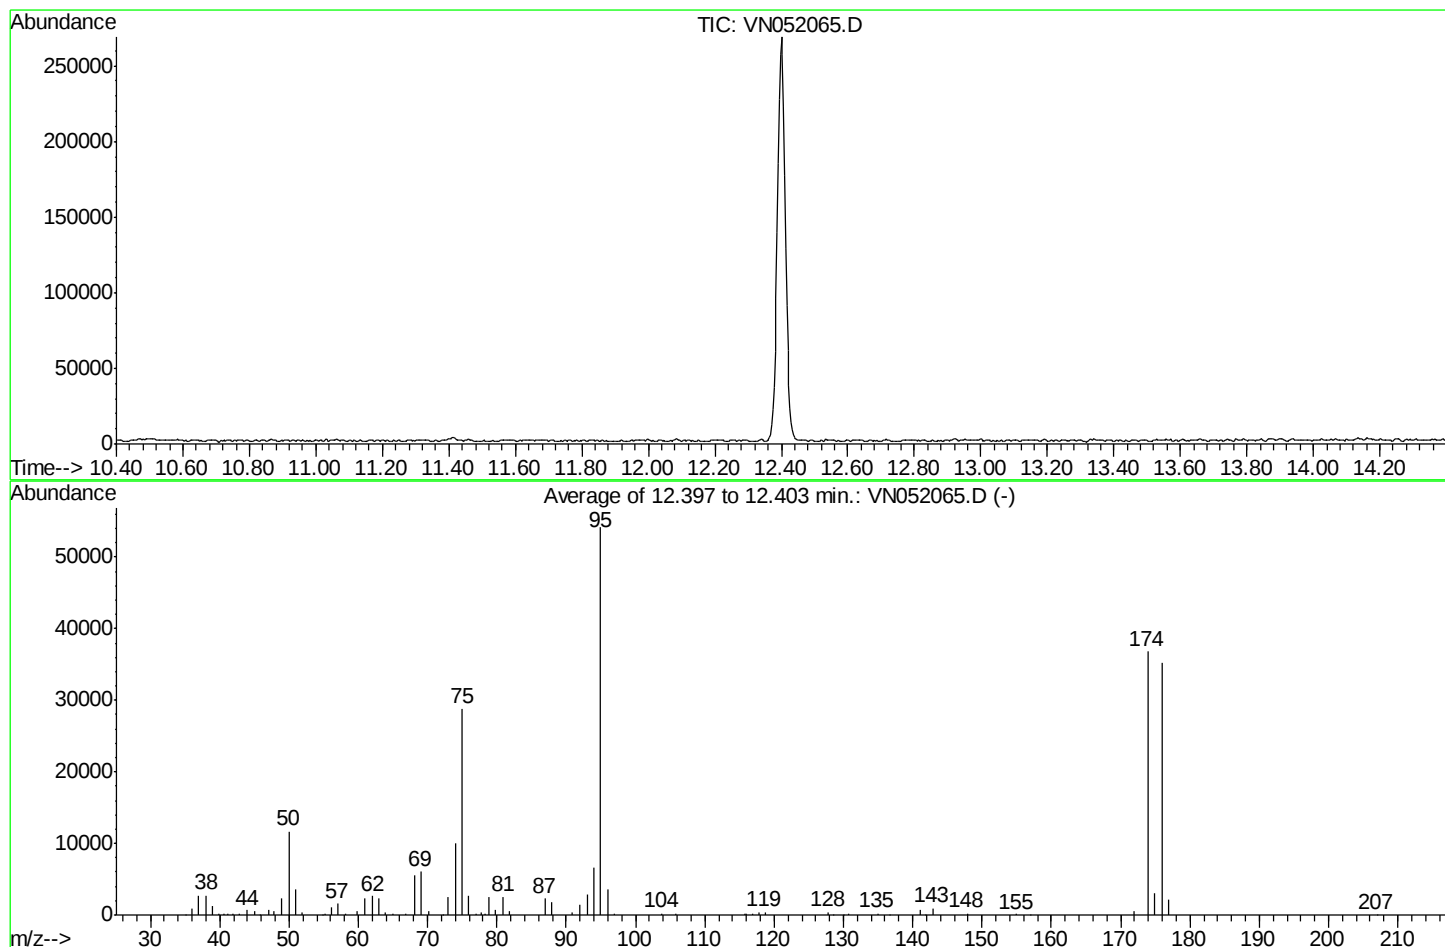

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	11645	PASS
75	95	30	60	53.3	28869	PASS
95	95	100	100	100.0	54154	PASS
96	95	5	9	6.5	3509	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	67.9	36778	PASS
175	174	5	9	8.2	3011	PASS
176	174	95	101	95.9	35264	PASS
177	176	5	9	6.3	2213	PASS