



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN103122\
Data File : VN075077.D
Acq On : 31 Oct 2022 10:42
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 09:48:49 2022

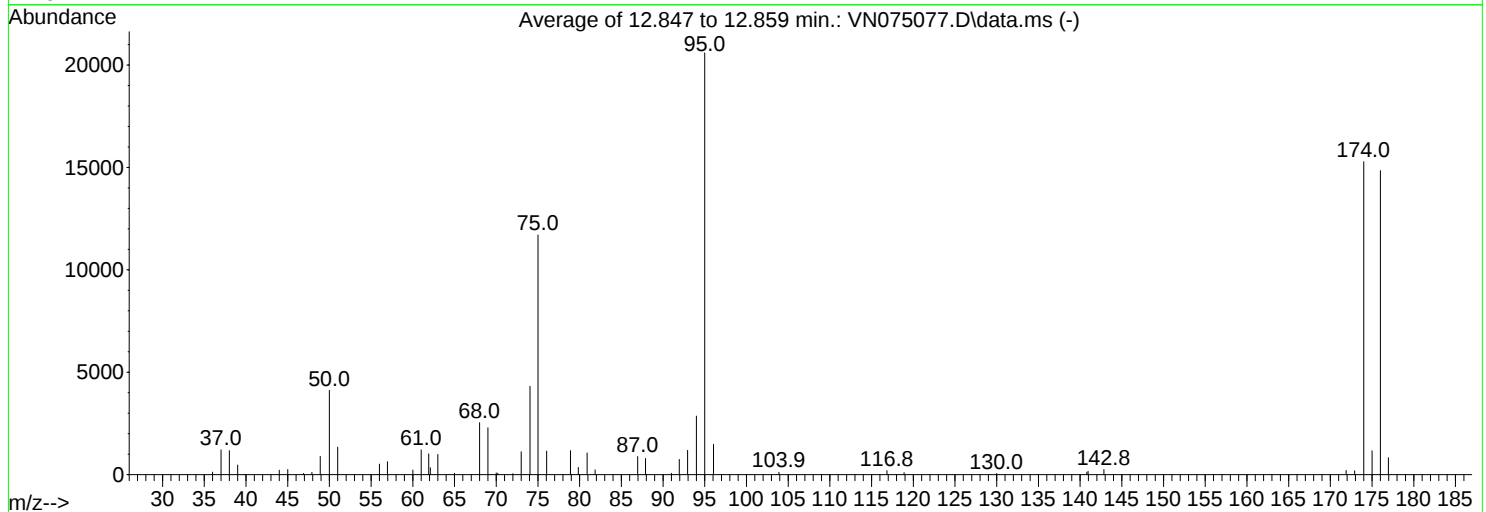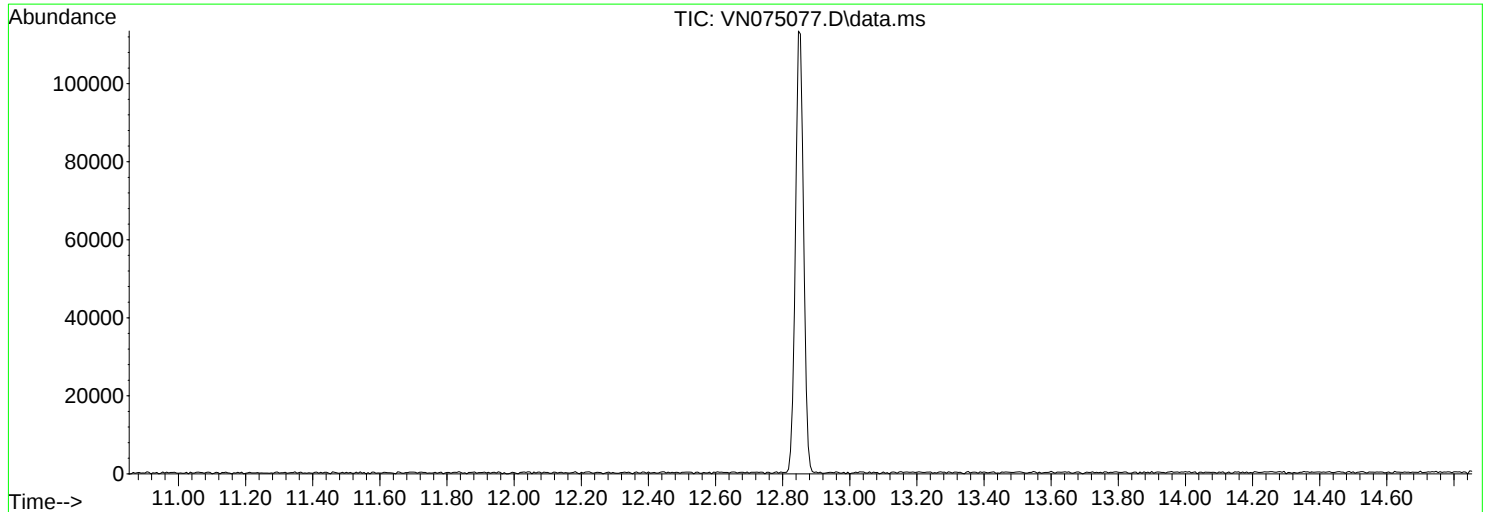

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	4114	PASS
75	95	30	60	56.8	11701	PASS
95	95	100	100	100.0	20597	PASS
96	95	5	9	7.2	1482	PASS
173	174	0.00	2	1.2	185	PASS
174	95	50	100	74.2	15281	PASS
175	174	5	9	7.6	1165	PASS
176	174	95	101	97.1	14842	PASS
177	176	5	9	5.6	826	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	127	51.00	1347	70.00	90	86.95	884
37.00	1212	56.00	519	70.20	73	87.90	791
38.00	1169	56.95	631	72.00	50	91.00	6
39.00	468	60.00	224	73.00	1115	91.95	73
39.85	16	61.00	1208	74.05	4311	92.95	1188
44.00	218	61.90	1016	75.00	11701	94.00	2861
45.00	249	62.10	335	76.05	1149	95.00	20597
46.90	63	63.00	986	78.90	1171	96.05	1482
47.90	108	65.00	72	79.85	352	103.90	121
48.90	894	68.00	2538	80.90	1064	116.85	197
50.00	4114	69.00	2291	81.85	234	118.90	105

Average of 12.847 to 12.859 min.: VN075077.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
130.00	54						
140.80	121						
140.95	162						
142.85	252						
171.90	202						
172.90	185						
174.00	15281						
175.00	1165						
176.00	14842						
176.95	826						

Instrument :

MSVOA_N

ClientSampleId :

BFB