
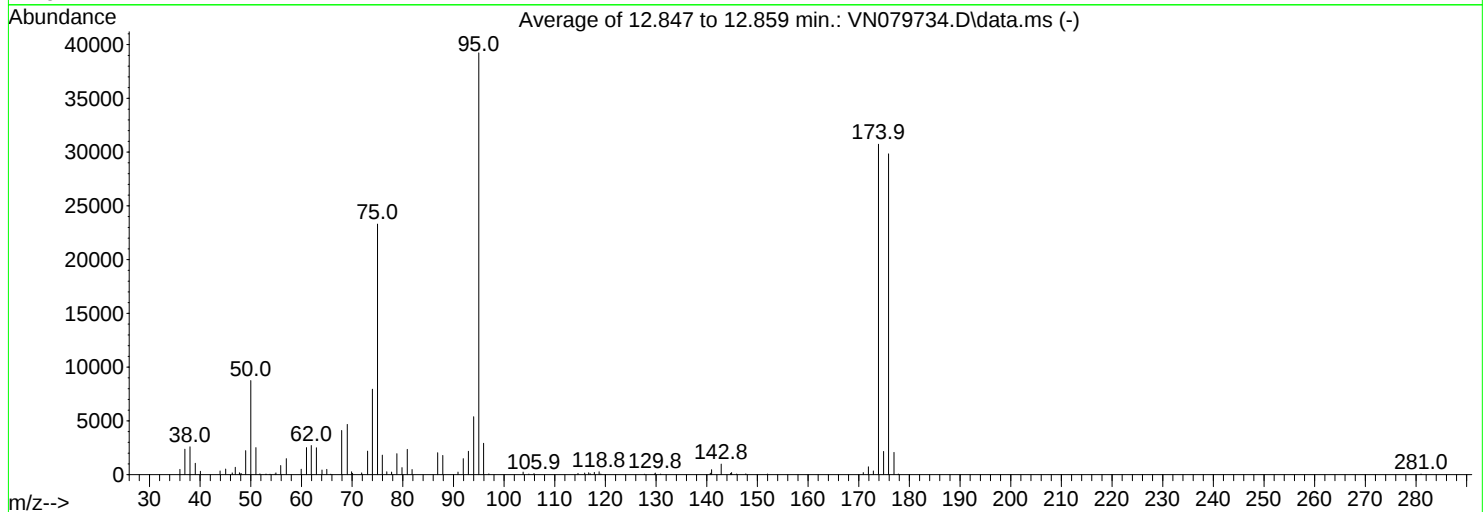


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN103123\
Data File : VN079734.D
Acq On : 31 Oct 2023 10:06
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103023W.M
Title : SW846 8260
Last Update : Tue Oct 31 07:23:24 2023

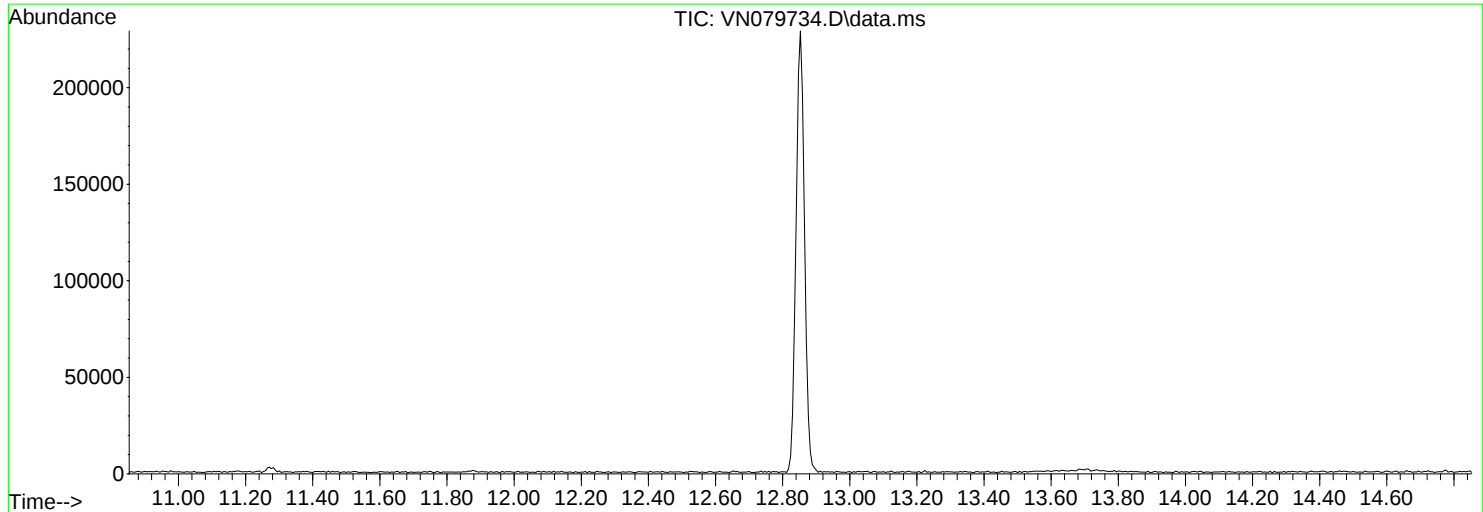

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	8750	PASS
75	95	30	60	59.4	23304	PASS
95	95	100	100	100.0	39235	PASS
96	95	5	9	7.4	2917	PASS
173	174	0.00	2	1.1	344	PASS
174	95	50	100	78.3	30728	PASS
175	174	5	9	7.0	2157	PASS
176	174	95	101	97.1	29837	PASS
177	176	5	9	7.0	2075	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	493	48.10	103	59.95	502	71.90	160
37.00	2371	49.00	2239	61.00	2517	73.05	218
38.00	2596	50.00	8750	61.95	2703	74.00	794
39.05	1053	51.00	2516	62.95	2502	75.00	2330
40.05	317	51.80	70	64.05	438	75.95	1819
43.95	347	53.00	56	65.00	492	76.85	273
45.05	515	53.80	51	65.80	51	77.80	234
46.35	169	54.80	56	67.95	4109	78.85	1954
46.95	678	54.95	158	69.05	4671	79.85	661
47.75	182	55.90	850	69.90	264	80.90	2356
47.90	92	57.00	1491	70.10	114	81.85	476

Average of 12.847 to 12.859 min.: VN079734.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.90	2047	105.90	110	130.90	60	172.90	344
87.90	1783	114.60	118	140.70	136	173.90	30728
90.90	238	115.90	146	140.95	458	174.90	2157
91.95	1494	116.70	178	142.85	980	175.90	29837
92.95	2177	117.00	88	144.70	118	176.95	2075
94.00	5392	117.80	204	144.90	195	177.80	64
95.00	39235	118.75	268	145.90	61	281.00	59
95.95	2917	119.10	63	147.70	69		
97.00	75	127.70	53	152.00	66		
103.75	236	129.70	65	170.90	198		
104.90	56	129.85	144	171.90	726		

Instrument :

MSVOA_N

ClientSampleId :

BFB