
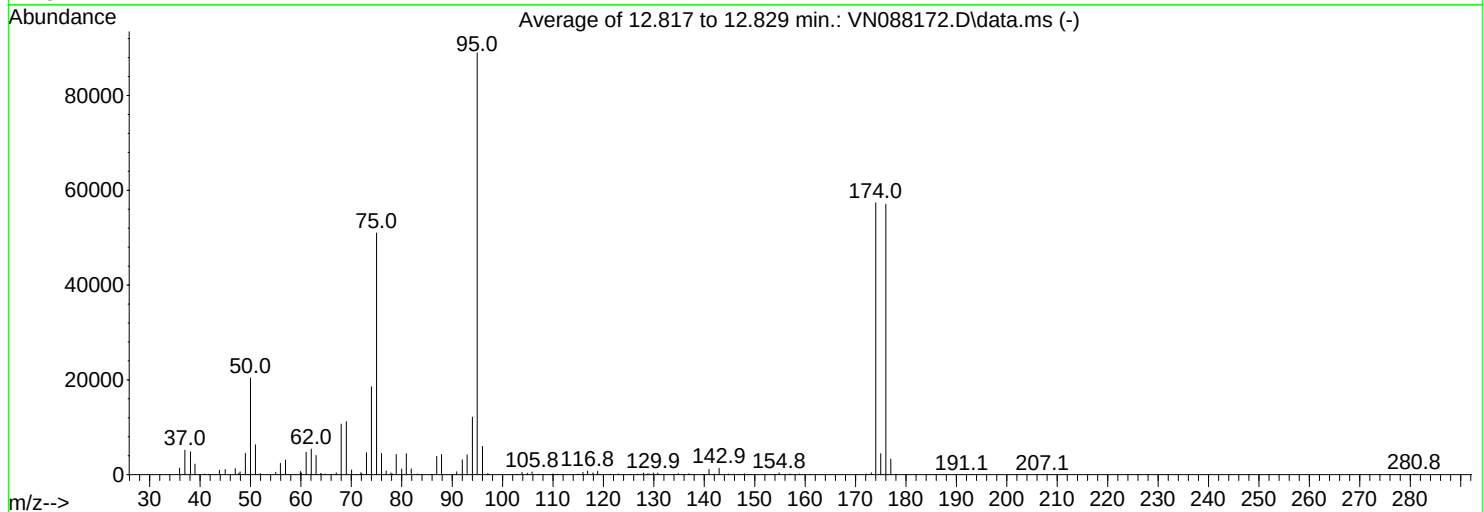


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN103125\
Data File : VN088172.D
Acq On : 31 Oct 2025 08:08
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Title : SW846 8260
Last Update : Mon Nov 03 01:16:06 2025

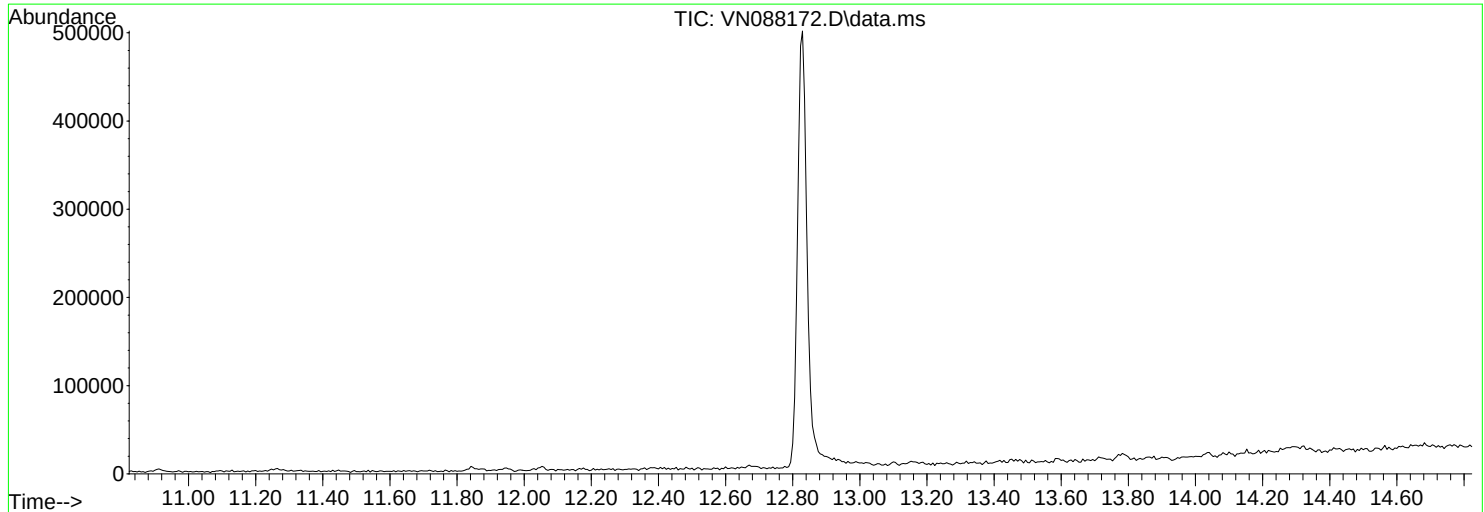

AutoFind: Scans 1847, 1848, 1849; Background Corrected with Scan 1839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	20392	PASS
75	95	30	60	57.3	50971	PASS
95	95	100	100	100.0	89005	PASS
96	95	5	9	6.7	5981	PASS
173	174	0.00	2	0.7	401	PASS
174	95	50	100	64.4	57349	PASS
175	174	5	9	7.7	4409	PASS
176	174	95	101	99.5	57061	PASS
177	176	5	9	5.7	3280	PASS

Average of 12.817 to 12.829 min.: VN088172.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	1379	47.70	297	60.10	367	71.05	21
37.00	5155	47.95	600	61.05	4725	71.90	411
38.10	4824	49.00	4486	62.05	5393	72.10	20
39.00	2236	50.00	20392	63.00	4065	73.00	462
40.95	134	51.00	6329	63.90	198	74.00	18531
41.70	52	51.95	287	64.10	184	75.00	50971
42.95	48	55.00	519	64.80	126	76.00	4485
43.85	956	55.95	2355	67.00	388	76.90	774
45.00	1077	56.95	3090	68.00	10657	77.85	379
46.00	60	59.00	60	69.00	11161	78.10	183
47.00	1272	59.90	662	70.05	976	78.90	4270

Average of 12.817 to 12.829 min.: VN088172.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.00	1187	94.95	89005	115.95	484	128.75	127
80.90	4443	96.00	5981	116.85	757	129.05	158
81.90	1216	97.10	278	117.80	104	129.90	367
83.05	147	102.70	53	117.95	358	130.80	345
85.80	78	103.85	517	118.85	700	134.85	255
86.95	3855	104.95	308	121.30	73	136.90	175
87.90	4258	105.85	570	122.95	149	137.10	115
90.90	594	107.20	88	123.90	51	139.80	81
92.00	3152	110.00	173	125.30	59	140.95	1114
92.95	4187	110.90	111	126.80	100	141.80	68
94.00	12150	114.95	129	127.95	331	142.10	139

Average of 12.817 to 12.829 min.: VN088172.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
142.95	1367	157.10	72	191.10	59		
144.00	68	158.90	150	193.20	59		
144.85	144	161.00	50	207.10	9		
145.90	153	172.00	69	280.80	127		
146.80	71	172.20	130	281.20	86		
147.95	217	173.10	401	282.20	59		
148.80	86	174.00	57349				
152.00	64	175.00	4409				
153.90	52	176.00	57061				
154.85	385	177.00	3280				
156.90	152	178.00	76				