


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110118\
 Data File : VN052089.D
 Acq On : 1 Nov 2018 7:50
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N110118W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Nov 02 05:39:38 2018

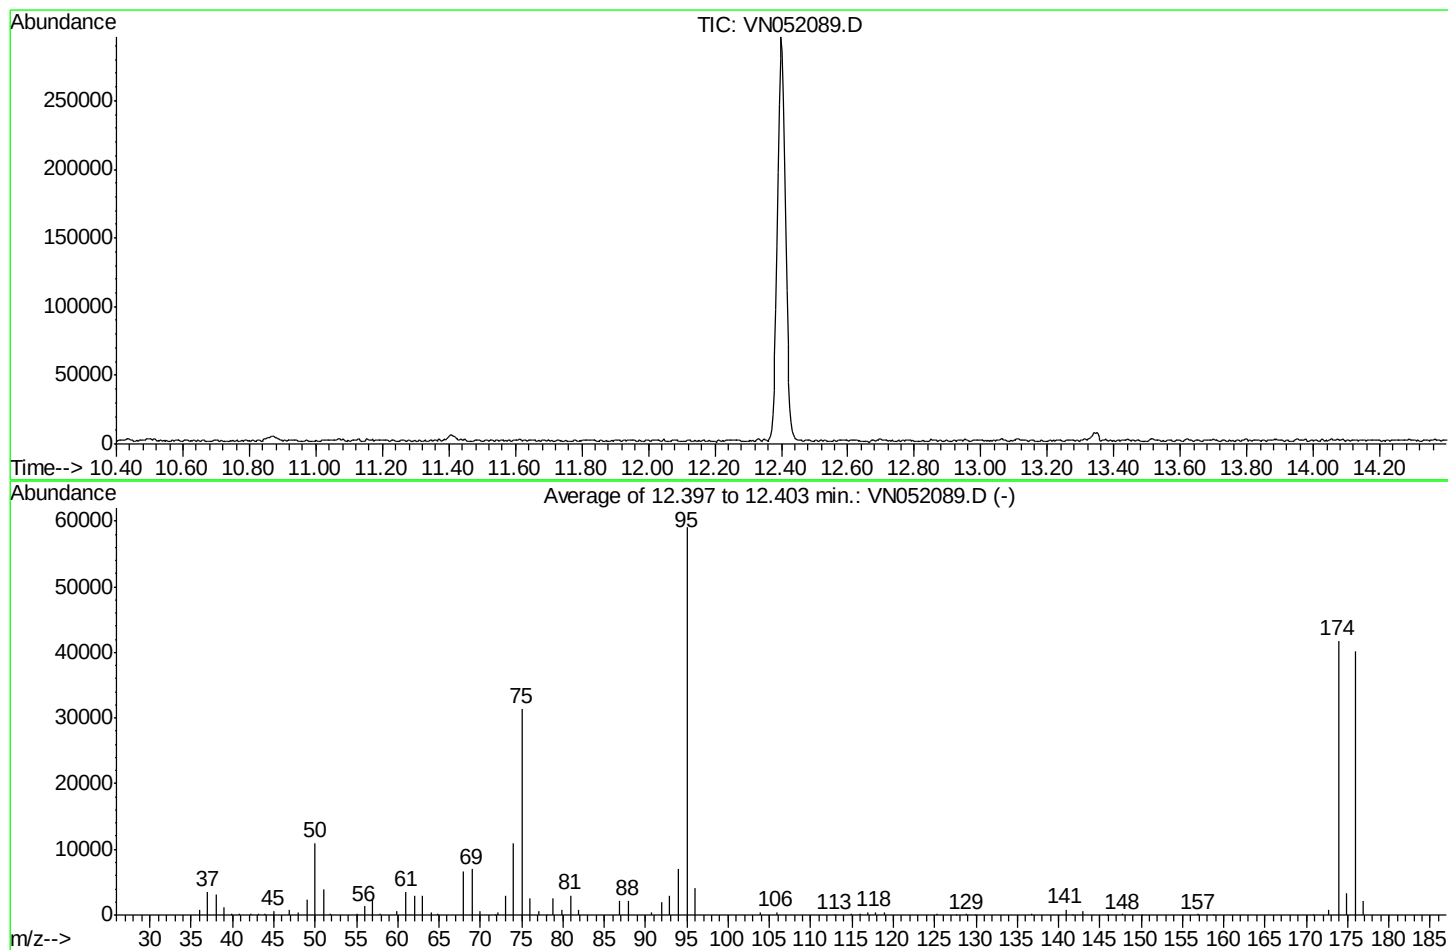

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	10936	PASS
75	95	30	60	53.2	31429	PASS
95	95	100	100	100.0	59045	PASS
96	95	5	9	7.0	4148	PASS
173	174	0.00	2	1.9	782	PASS
174	95	50	100	70.8	41813	PASS
175	174	5	9	8.1	3376	PASS
176	174	95	101	96.1	40178	PASS
177	176	5	9	5.6	2234	PASS