


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN110119\
 Data File : VN059049.D
 Acq On : 1 Nov 2019 8:18
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110119W.M
 Title : SW846 8260
 Last Update : Sat Nov 02 05:43:23 2019

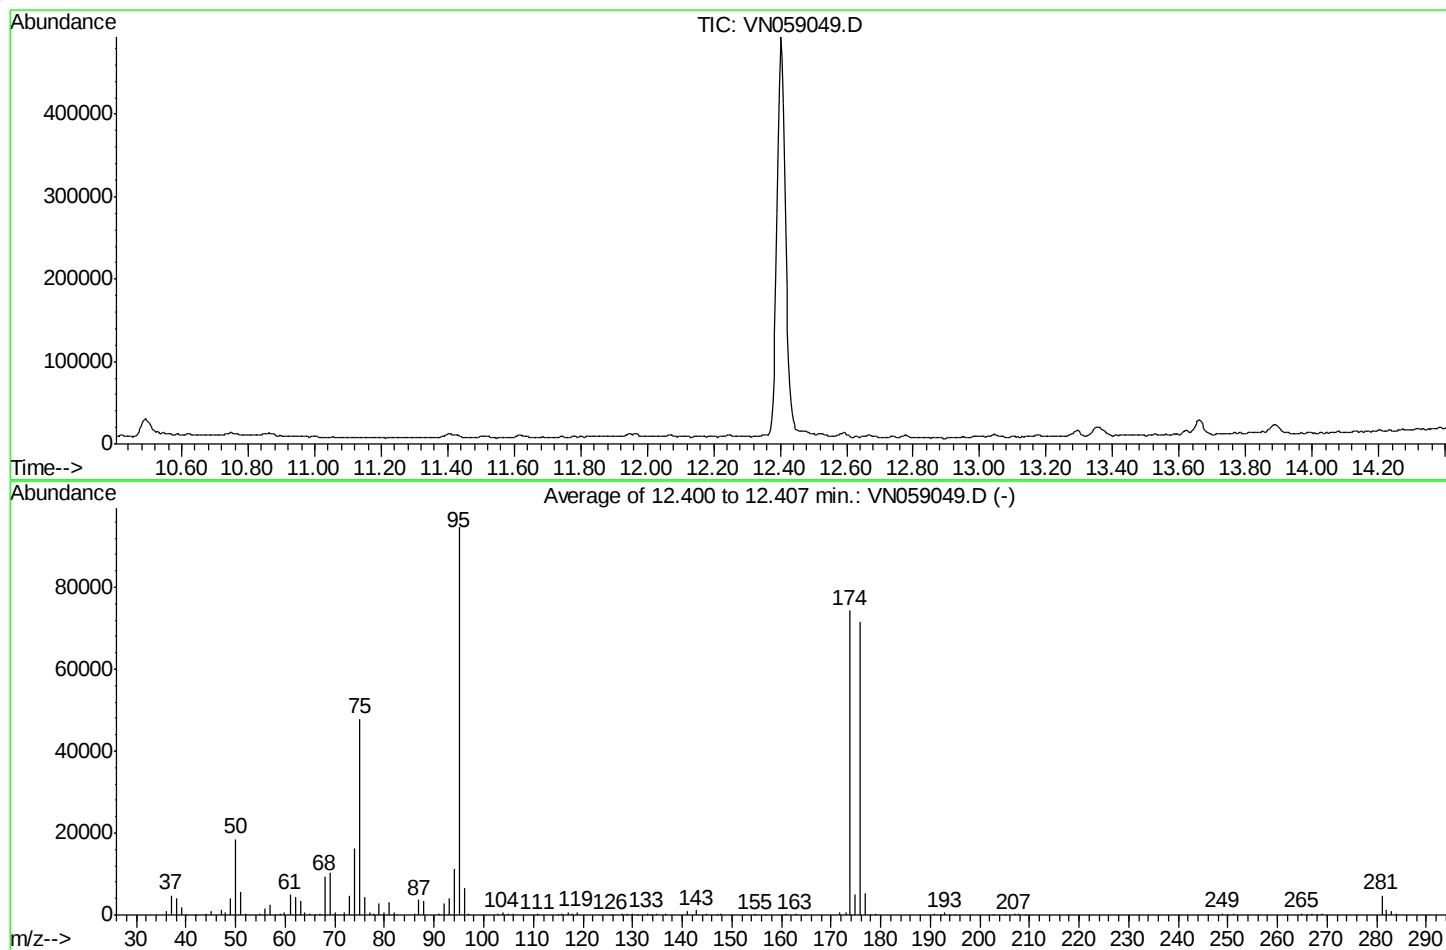

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	18541	PASS
75	95	30	60	50.6	47898	PASS
95	95	100	100	100.0	94618	PASS
96	95	5	9	7.0	6657	PASS
173	174	0.00	2	0.9	703	PASS
174	95	50	100	78.5	74272	PASS
175	174	5	9	6.9	5159	PASS
176	174	95	101	96.3	71528	PASS
177	176	5	9	7.3	5189	PASS