

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
 Data File : VN069324.D
 Acq On : 1 Nov 2021 16:58
 Operator : JC/MD
 Sample : M4411-02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 01 17:39:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 28 16:09:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	322328	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	586514	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	590705	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	224865	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	222529	47.825	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	95.660%		
35) Dibromofluoromethane	8.024	113	165482	45.262	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	90.520%		
50) Toluene-d8	10.443	98	734321	50.233	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	100.460%		
62) 4-Bromofluorobenzene	12.733	95	269296	48.819	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	97.640%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.309	50	565	Below Cal	#	87
11) Tert butyl alcohol	5.390	59	82	13.493	ug/l #	72
16) Acetone	4.299	43	39811	20.082	ug/l	99
18) Methyl Acetate	4.865	43	9940	1.475	ug/l #	69
20) Methylene Chloride	5.095	84	9807	2.579	ug/l	96
23) Vinyl Acetate	6.616	43	53	6.595	ug/l #	72
25) 2-Butanone	7.351	43	11571	5.418	ug/l	93
29) Tetrahydrofuran	7.699	42	3926	4.924	ug/l #	78
31) Cyclohexane	8.086	56	7353	1.181	ug/l #	1
36) 1,1-Dichloropropene	8.088	75	27076	5.355	ug/l #	50
37) Ethyl Acetate	7.351	43	11571	2.008	ug/l #	68
38) Carbon Tetrachloride	8.088	117	34380	6.867	ug/l #	15
41) Methacrylonitrile	7.697	41	2425	0.854	ug/l #	37
43) Isopropyl Acetate	8.566	43	36833	4.091	ug/l #	86
45) 1,2-Dichloropropane	9.625	63	1947	0.503	ug/l #	43
48) Methyl methacrylate	9.547	41	8089	1.860	ug/l #	13
49) 1,4-Dioxane	9.630	88	58	35.388	ug/l #	1
51) 4-Methyl-2-Pentanone	10.336	43	6254	7.334	ug/l #	75
54) cis-1,3-Dichloropropene	10.245	75	49572	8.455	ug/l #	62
56) Ethyl methacrylate	10.880	69	231	1.714	ug/l #	1
57) 1,3-Dichloropropane	11.092	76	29183	4.372	ug/l #	42
59) 2-Hexanone	11.092	43	420245	89.334	ug/l #	50
70) Styrene	12.299	104	215	1.471	ug/l #	24
71) Bromoform	12.725	173	464	2.993	ug/l #	1
74) N-amyl acetate	12.200	43	17880	2.401	ug/l #	52
76) 1,2,3-Trichloropropane	12.733	75	143997	24.348	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.733	75	143997	69.847	ug/l #	12
93) 1,2,4-Trichlorobenzene	15.271	180	285	2.562	ug/l #	34
95) Naphthalene	15.509	128	1976	3.472	ug/l #	69
96) 1,2,3-Trichlorobenzene	15.697	180	164	2.251	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
Data File : VN069324.D
Acq On : 1 Nov 2021 16:58
Operator : JC/MD
Sample : M4411-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Nov 01 17:39:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 28 16:09:15 2021
Response via : Initial Calibration




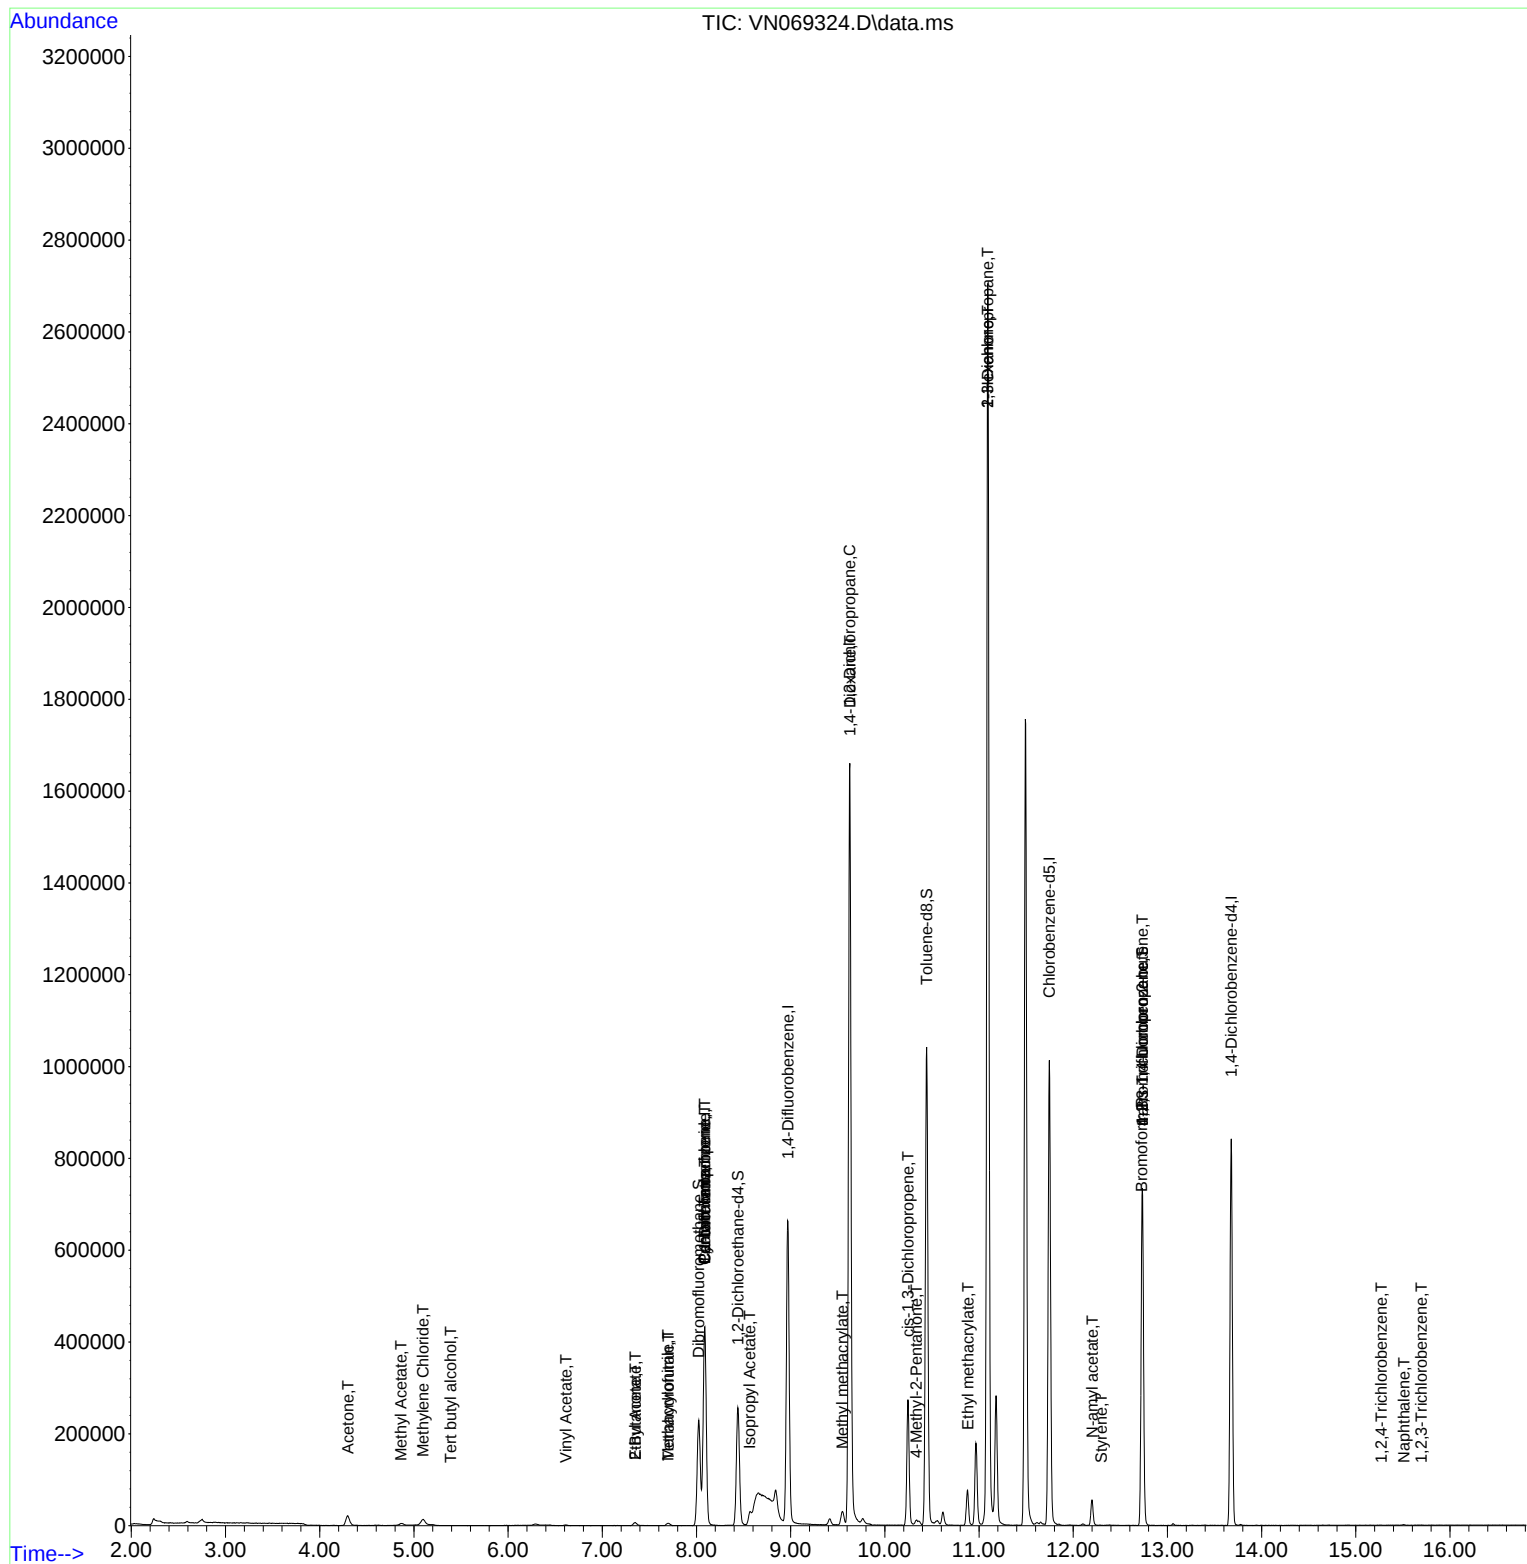




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 322328
Ion Ratio Lower Upper
168 100
99 62.3 48.9 73.3

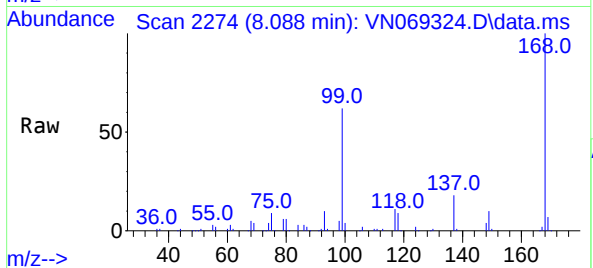

#3
Chloromethane
Concen: Below Cal
RT: 2.309 min Scan# 119
Delta R.T. 0.008 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Tgt Ion: 50 Resp: 565
Ion Ratio Lower Upper
50 100
52 40.3 26.3 39.5#


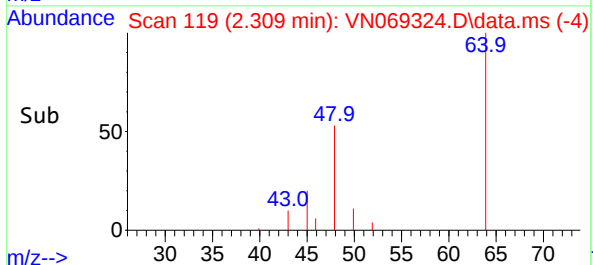

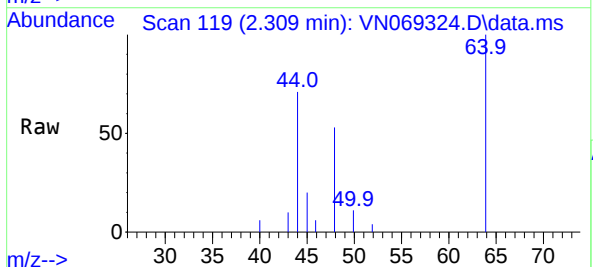




#11
Tert butyl alcohol
Concen: 13.493 ug/l
RT: 5.390 min Scan# 11
Delta R.T. 0.027 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 59 Resp: 82
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#



#16
Acetone
Concen: 20.082 ug/l
RT: 4.299 min Scan# 861
Delta R.T. 0.016 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Tgt Ion: 43 Resp: 39811
Ion Ratio Lower Upper
43 100
58 29.9 24.5 36.7

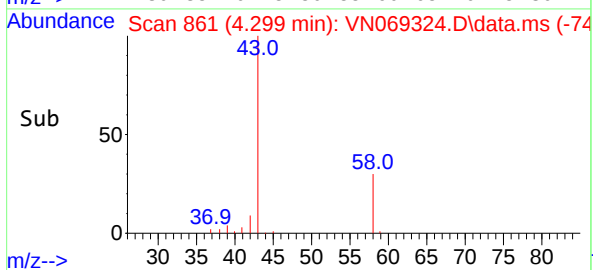



#18

Methyl Acetate

Concen: 1.475 ug/l

RT: 4.865 min Scan# 1107

Delta R.T. 0.014 min

Lab File: VN069324.D

Acq: 1 Nov 2021 16:58

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 9940

Ion Ratio Lower Upper

43 100

74 8.4 18.9 28.3#

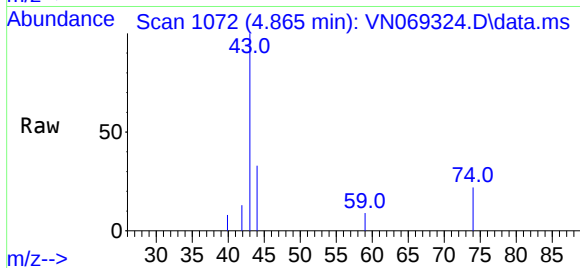

#20

Methylene Chloride

Concen: 2.579 ug/l

RT: 5.095 min Scan# 1158

Delta R.T. 0.000 min

Lab File: VN069324.D

Acq: 1 Nov 2021 16:58

Tgt Ion: 84 Resp: 9807




Ion Ratio Lower Upper


84 100

49 114.6 97.6 146.4

51 35.2 30.3 45.5

86 65.2 51.8 77.6


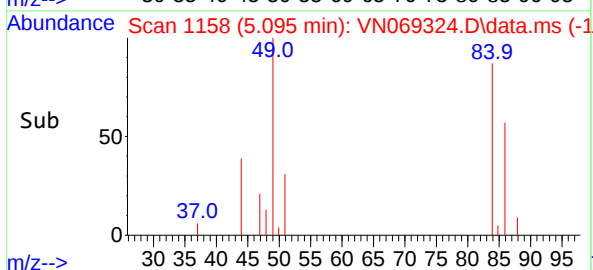
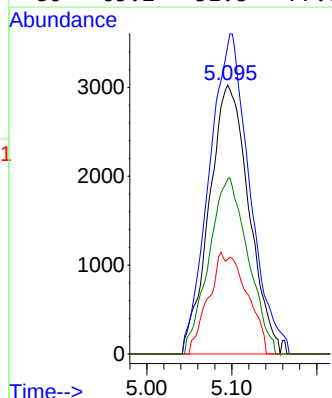
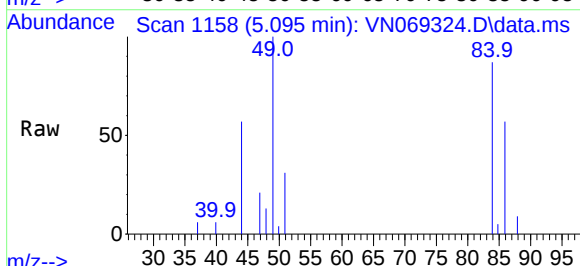




#23
 Vinyl Acetate
 Concen: 6.595 ug/l
 RT: 6.616 min Scan# 11
 Delta R.T. 0.183 min
 Lab File: VN069324.D
 Acq: 1 Nov 2021 16:58




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 43 Resp: 53
 Ion Ratio Lower Upper
 43 100
 86 0.0 8.3 12.5#

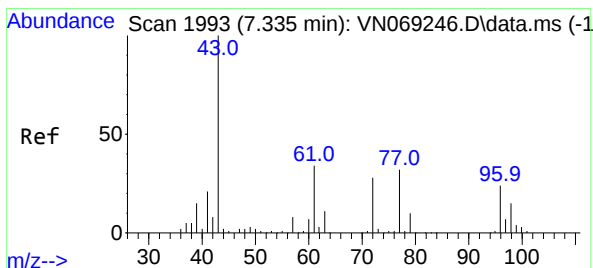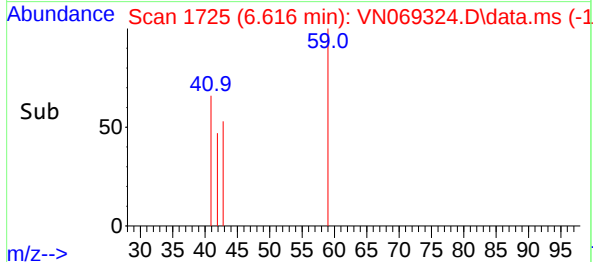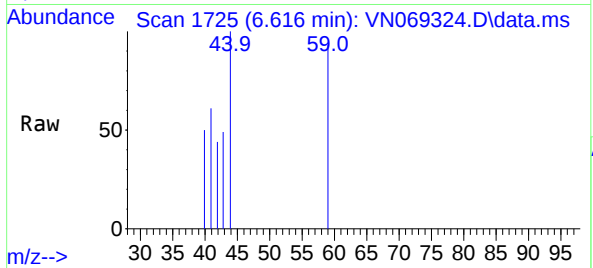

#25
 2-Butanone
 Concen: 5.418 ug/l
 RT: 7.351 min Scan# 1999
 Delta R.T. 0.016 min
 Lab File: VN069324.D
 Acq: 1 Nov 2021 16:58

Tgt Ion: 43 Resp: 11571
 Ion Ratio Lower Upper
 43 100
 72 30.2 21.2 31.8


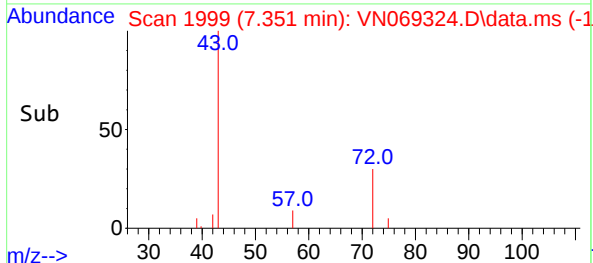
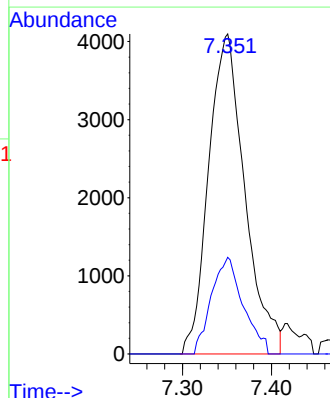
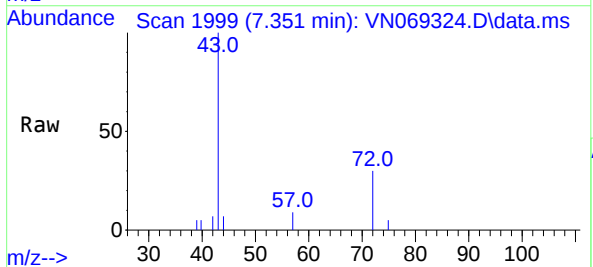




#29
Tetrahydrofuran
Concen: 4.924 ug/l
RT: 7.699 min Scan# 2122
Delta R.T. 0.018 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 42 Resp: 3926
Ion Ratio Lower Upper
42 100
72 19.3 35.4 53.2#
71 44.7 33.8 50.6

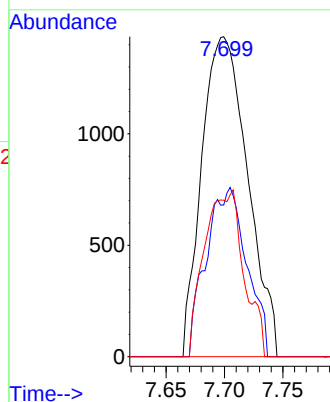

#31
Cyclohexane
Concen: 1.181 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.010 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Tgt Ion: 56 Resp: 7353
Ion Ratio Lower Upper
56 100
69 171.5 26.9 40.3#
84 128.6 67.6 101.4#

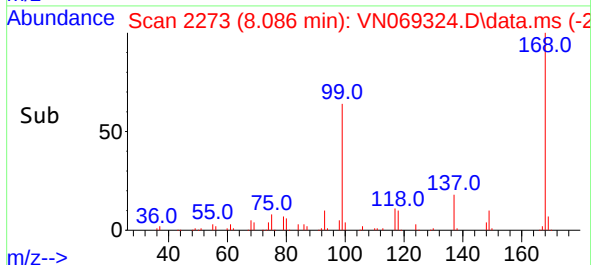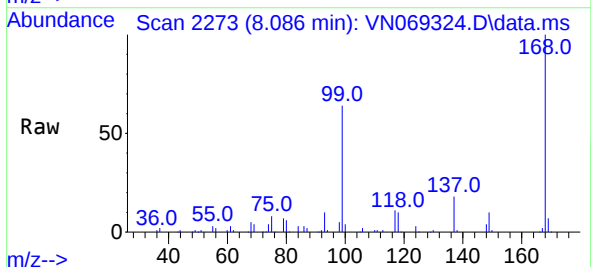



#33

1,2-Dichloroethane-d4

Concen: 47.825 ug/l

RT: 8.440 min Scan# 2405

Delta R.T. -0.000 min

Lab File: VN069324.D

Acq: 1 Nov 2021 16:58

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 222529

Ion Ratio Lower Upper

65 100

67 51.5 0.0 103.8

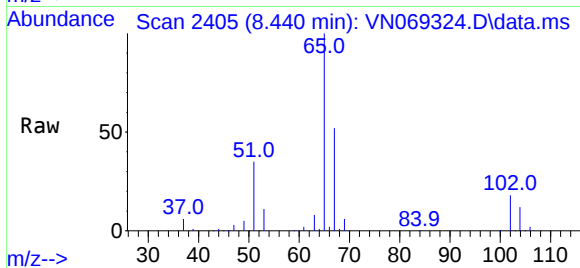

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.971 min Scan# 2603

Delta R.T. 0.003 min

Lab File: VN069324.D

Acq: 1 Nov 2021 16:58




Tgt Ion: 114 Resp: 586514


Ion Ratio Lower Upper

114 100

63 20.7 0.0 42.6


88 15.9 0.0 32.0

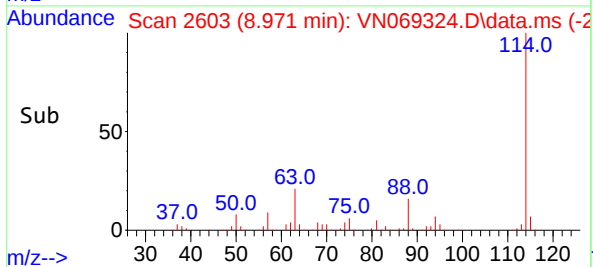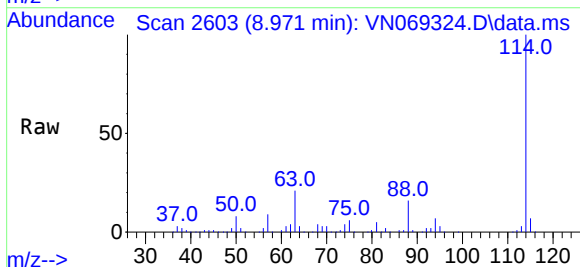






#35
Dibromofluoromethane
Concen: 45.262 ug/l
RT: 8.024 min Scan# 2113
Delta R.T. -0.000 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Instrument :
MSVOA_N
ClientSampleId :



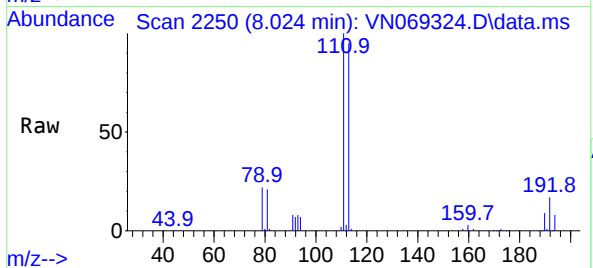



Tgt Ion:113 Resp: 165482
Ion Ratio Lower Upper
113 100
111 104.9 83.2 124.8
192 18.5 15.0 22.4

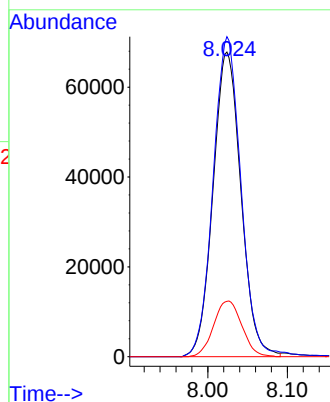

#36
1,1-Dichloropropene
Concen: 5.355 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58


Tgt Ion: 75 Resp: 27076
Ion Ratio Lower Upper
75 100
110 9.8 17.9 53.8#
77 0.0 24.7 37.1#

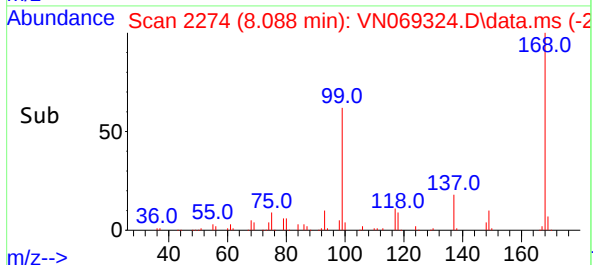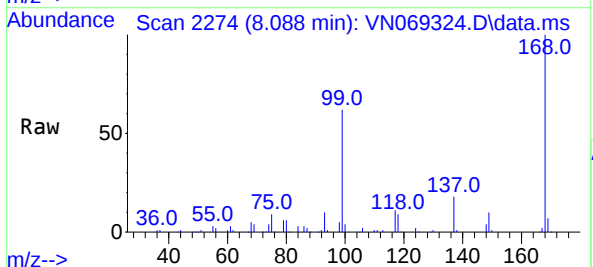






#37
Ethyl Acetate
Concen: 2.008 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. -0.061 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Instrument : MSVOA_N
ClientSampleId :

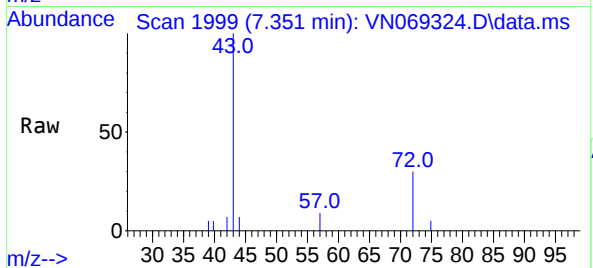

Tgt Ion: 43 Resp: 11571




Ion	Ratio	Lower	Upper
43	100		
61	0.0	11.2	16.8#
70	0.0	8.4	12.6#

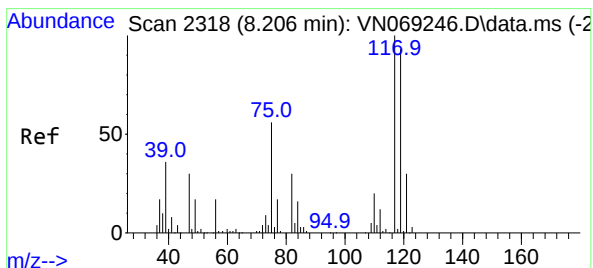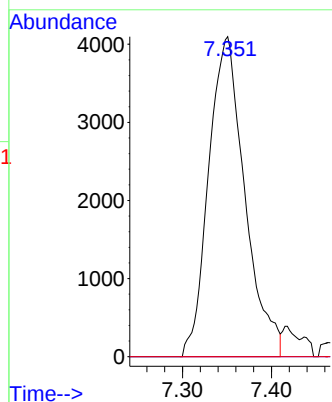


#38
Carbon Tetrachloride
Concen: 6.867 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.118 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Tgt Ion: 117 Resp: 34380


Ion	Ratio	Lower	Upper
117	100		
119	4.3	76.9	115.3#
121	0.0	24.6	37.0#

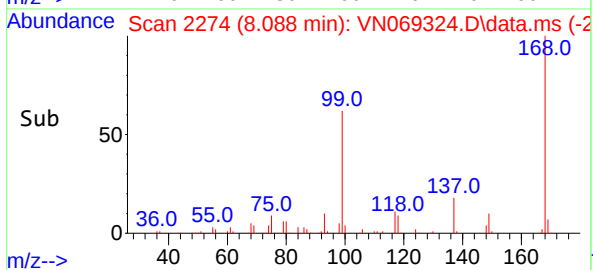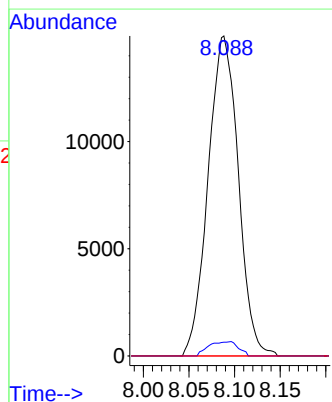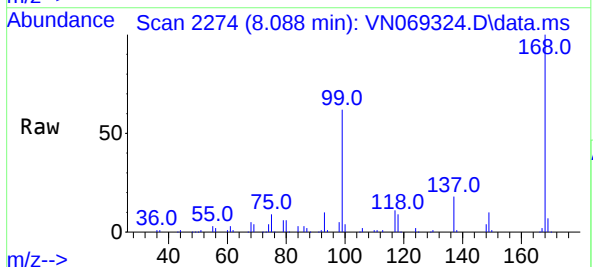






#41
Methacrylonitrile
Concen: 0.854 ug/l
RT: 7.697 min Scan# 2106
Delta R.T. 0.059 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Instrument :
MSVOA_N
ClientSampleId :



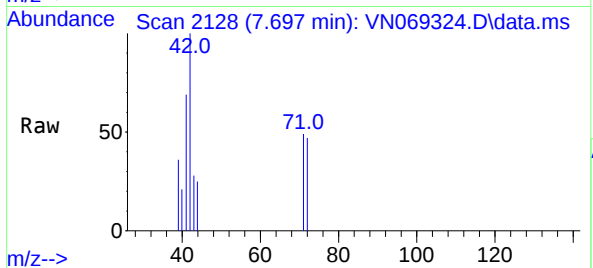



Tgt Ion: 41 Resp: 2425
Ion Ratio Lower Upper
41 100
39 35.1 44.9 67.3#
67 0.0 62.6 93.8#
52 0.0 26.2 39.4#



#43
Isopropyl Acetate
Concen: 4.091 ug/l
RT: 8.566 min Scan# 2452
Delta R.T. 0.006 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Tgt Ion: 43 Resp: 36833
Ion Ratio Lower Upper
43 100
61 16.3 20.4 30.6#
87 10.9 10.7 16.1


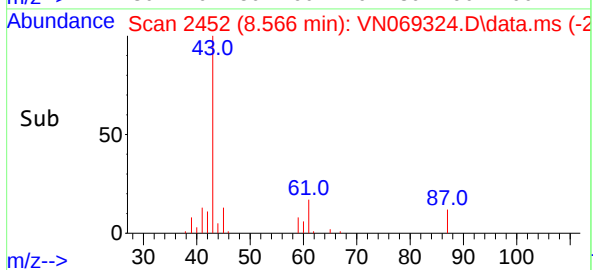






#45
1,2-Dichloropropane
Concen: 0.503 ug/l
RT: 9.625 min Scan# 21
Delta R.T. 0.134 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 63 Resp: 1947
Ion Ratio Lower Upper
63 100
65 0.0 25.6 38.4#

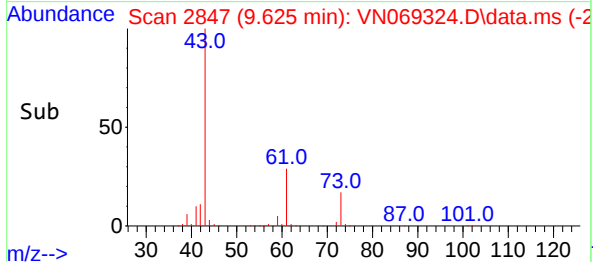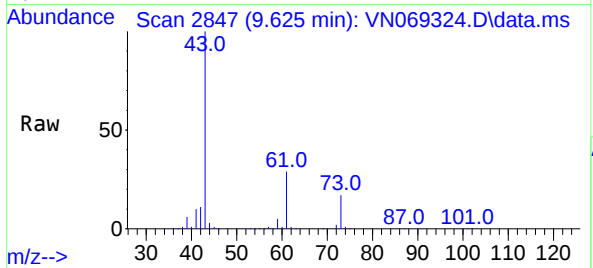

#48
Methyl methacrylate
Concen: 1.860 ug/l
RT: 9.547 min Scan# 2818
Delta R.T. -0.014 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Tgt Ion: 41 Resp: 8089
Ion Ratio Lower Upper
41 100
69 0.0 66.4 99.6#
39 0.0 50.2 75.2#


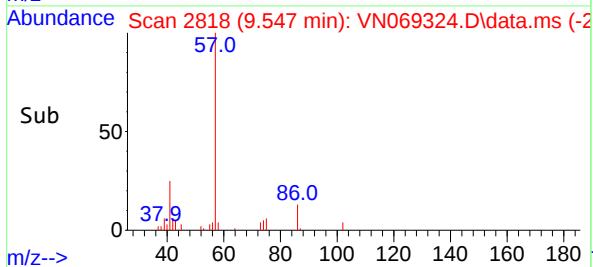

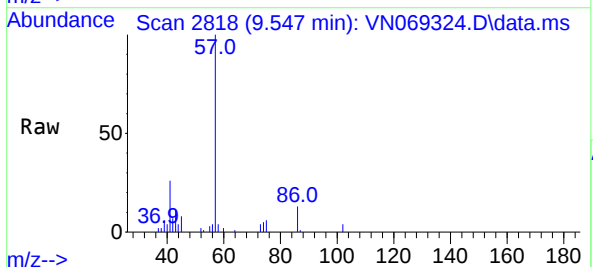




#49
1,4-Dioxane
Concen: 35.388 ug/l
RT: 9.630 min Scan# 2826
Delta R.T. 0.061 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 88 Resp: 58
Ion Ratio Lower Upper
88 100
43 2839712.1 24.9 37.3#
58 12137.9 56.9 85.3#



#50
Toluene-d8
Concen: 50.233 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Tgt Ion: 98 Resp: 734321
Ion Ratio Lower Upper
98 100
100 64.2 51.5 77.3

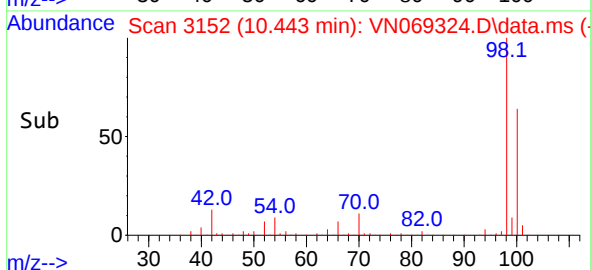



#51

4-Methyl-2-Pentanone

Concen: 7.334 ug/l

RT: 10.336 min Scan# 3112

Delta R.T. 0.006 min

Lab File: VN069324.D

Acq: 1 Nov 2021 16:58

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 6254

Ion Ratio Lower Upper

43 100

58 23.7 31.0 46.4#

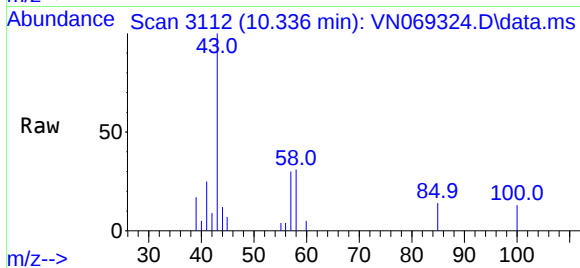

#54

cis-1,3-Dichloropropene

Concen: 8.455 ug/l

RT: 10.245 min Scan# 3078

Delta R.T. 0.054 min

Lab File: VN069324.D

Acq: 1 Nov 2021 16:58




Tgt Ion: 75 Resp: 49572


Ion Ratio Lower Upper

75 100

77 0.5 25.6 38.4#


39 34.2 42.9 64.3#

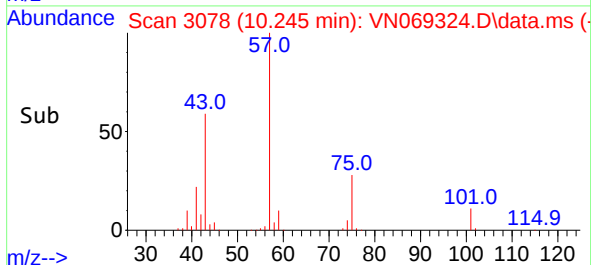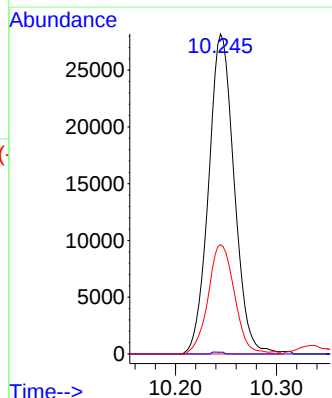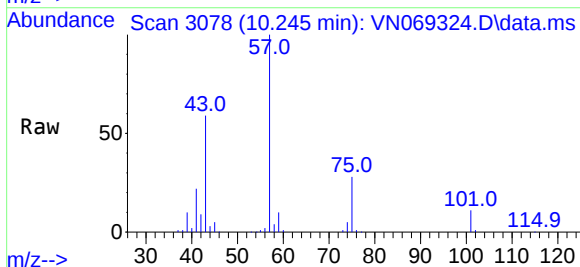






#56
Ethyl methacrylate
Concen: 1.714 ug/l
RT: 10.880 min Scan# 31
Delta R.T. 0.118 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 69 Resp: 231
Ion Ratio Lower Upper
69 100
41 6828.1 53.3 79.9#
39 3157.6 33.3 49.9#

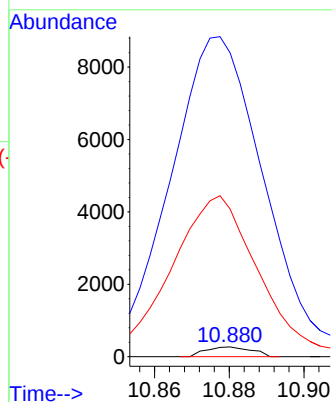

#57
1,3-Dichloropropane
Concen: 4.372 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.046 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Tgt Ion: 76 Resp: 29183
Ion Ratio Lower Upper
76 100
78 0.0 25.8 38.8#



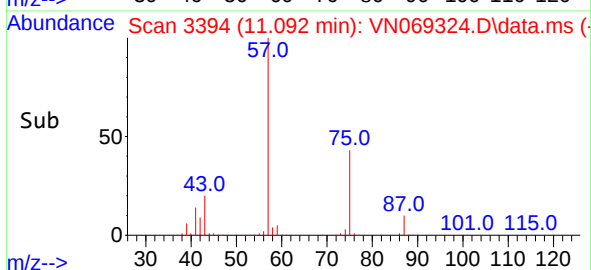





#59
2-Hexanone
Concen: 89.334 ug/l
RT: 11.092 min Scan# 31
Delta R.T. 0.005 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 420245
Ion Ratio Lower Upper
43 100
58 18.3 26.9 80.7#

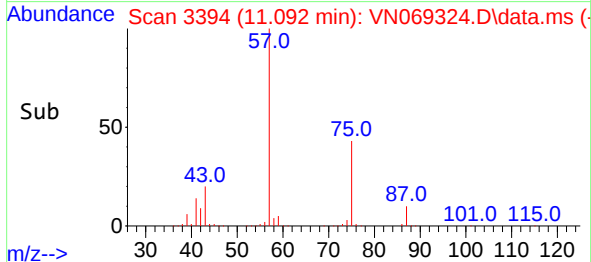

#62
4-Bromofluorobenzene
Concen: 48.819 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.002 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Tgt Ion: 95 Resp: 269296
Ion Ratio Lower Upper
95 100
174 74.0 0.0 144.8
176 72.2 0.0 140.0



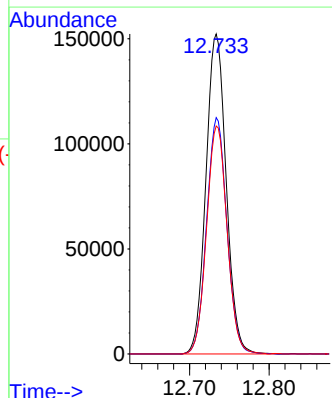





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 30
Delta R.T. 0.000 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 590705
Ion Ratio Lower Upper
117 100
82 57.1 46.4 69.6
119 32.1 26.0 39.0



#70
Styrene
Concen: 1.471 ug/l
RT: 12.299 min Scan# 3844
Delta R.T. 0.003 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Tgt Ion:104 Resp: 215
Ion Ratio Lower Upper
104 100
78 0.0 42.2 63.4#
103 0.0 44.4 66.6#


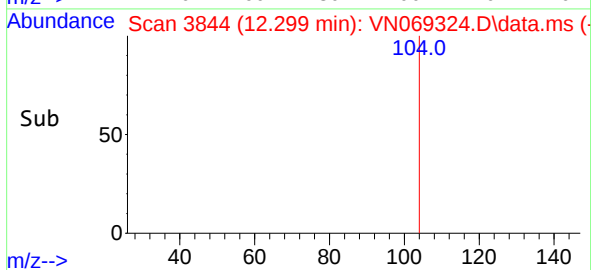






#71
Bromoform
Concen: 2.993 ug/l
RT: 12.725 min Scan# 4003
Delta R.T. 0.265 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:173 Resp: 464
Ion Ratio Lower Upper
173 100
175 3015.3 23.8 71.5#
254 0.0 0.0 0.0



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.002 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

Tgt Ion:152 Resp: 224865
Ion Ratio Lower Upper
152 100
115 63.0 31.4 94.3
150 156.9 0.0 351.0


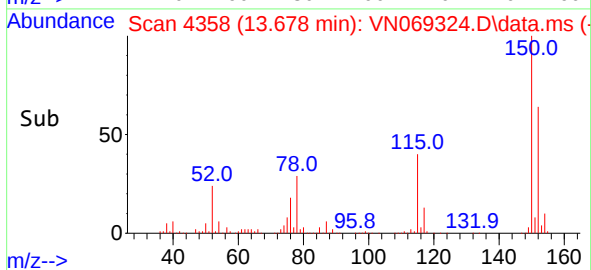






#74
N-amy1 acetate
Concen: 2.401 ug/l
RT: 12.200 min Scan# 31
Delta R.T. -0.187 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 17880
Ion Ratio Lower Upper
43 100
70 0.6 32.2 48.2#
55 4.2 18.0 27.0#
61 9.5 19.0 28.4#



#76
1,2,3-Trichloropropane
Concen: 24.348 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.148 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58


Tgt Ion: 75 Resp: 143997
Ion Ratio Lower Upper
75 100
77 1.1 96.2 288.4#

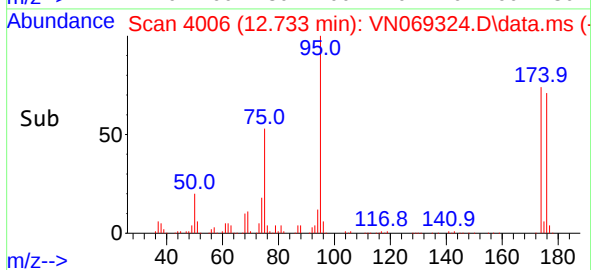






#81
trans-1,4-Dichloro-2-butene
Concen: 69.847 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.107 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58


Instrument :
MSVOA_N
ClientSampleId :

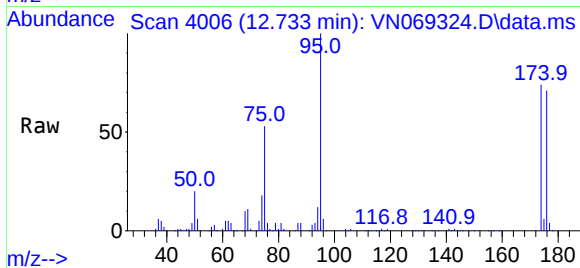



Tgt Ion: 75 Resp: 143997
Ion Ratio Lower Upper
75 100
53 0.0 75.4 113.2#
89 0.0 36.9 55.3#




#93
1,2,4-Trichlorobenzene
Concen: 2.562 ug/l
RT: 15.271 min Scan# 4952
Delta R.T. 0.006 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

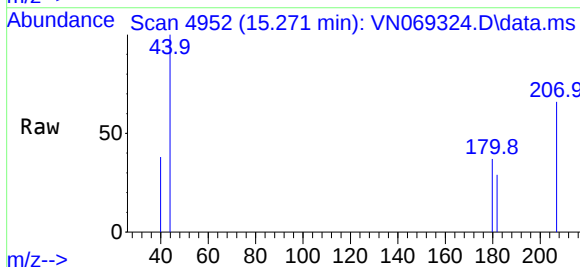


Tgt Ion:180 Resp: 285
Ion Ratio Lower Upper
180 100
182 28.4 47.9 143.7#
145 0.0 16.4 49.2#

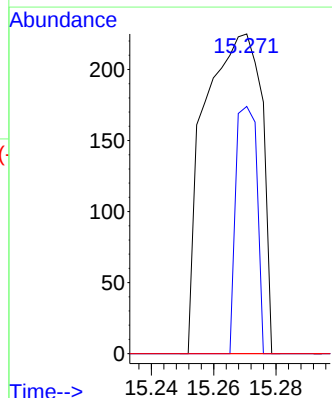






#95
Naphthalene
Concen: 3.472 ug/l
RT: 15.509 min Scan# 5040
Delta R.T. 0.002 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58


Instrument :
MSVOA_N
ClientSampleId :



Tgt Ion:128 Resp: 1976
Ion Ratio Lower Upper
128 100
127 0.0 10.5 15.7#
129 0.0 8.9 13.3#

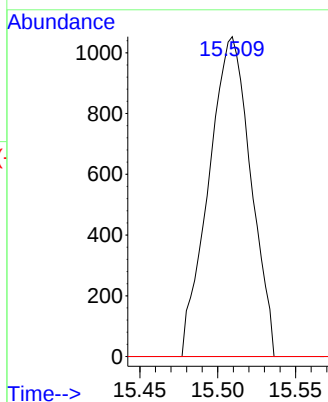

#96
1,2,3-Trichlorobenzene
Concen: 2.251 ug/l
RT: 15.697 min Scan# 5111
Delta R.T. -0.005 min
Lab File: VN069324.D
Acq: 1 Nov 2021 16:58

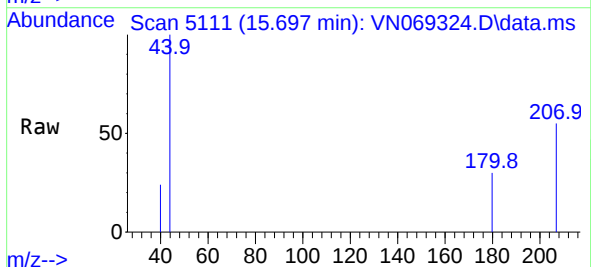

Tgt Ion:180 Resp: 164
Ion Ratio Lower Upper
180 100
182 0.0 48.1 144.3#
145 0.0 17.4 52.2#

