

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
 Data File : VN069326.D
 Acq On : 1 Nov 2021 17:49
 Operator : JC/MD
 Sample : M4411-04
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 02 05:50:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 28 16:09:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	325201	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	595132	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	593206	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	224011	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	228892	48.758	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	97.520%
35) Dibromofluoromethane	8.024	113	172648	46.538	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	93.080%
50) Toluene-d8	10.443	98	739841	49.878	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	99.760%
62) 4-Bromofluorobenzene	12.733	95	270033	48.243	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	96.480%


Target Compounds			Qvalue			
3) Chloromethane	2.306	50	784	Below Cal	#	42
5) Bromomethane	2.874	94	733	0.268	ug/l #	65
11) Tert butyl alcohol	5.398	59	373	13.794	ug/l #	72
16) Acetone	4.293	43	43350	21.674	ug/l	96
18) Methyl Acetate	4.862	43	3570	0.525	ug/l #	62
20) Methylene Chloride	5.095	84	9206	2.400	ug/l	93
23) Vinyl Acetate	6.605	43	85	6.598	ug/l #	72
25) 2-Butanone	7.351	43	12029	5.533	ug/l	99
29) Tetrahydrofuran	7.705	42	3856	4.871	ug/l #	66
31) Cyclohexane	8.086	56	7981	1.270	ug/l #	21
36) 1,1-Dichloropropene	8.086	75	27487	5.357	ug/l #	49
37) Ethyl Acetate	7.351	43	12029	2.057	ug/l #	68
38) Carbon Tetrachloride	8.088	117	34887	6.868	ug/l #	15
41) Methacrylonitrile	7.702	41	2381	0.826	ug/l #	40
43) Isopropyl Acetate	8.566	43	32184	3.586	ug/l #	89
45) 1,2-Dichloropropane	9.625	63	1981	0.504	ug/l #	43
48) Methyl methacrylate	9.544	41	7788	1.765	ug/l #	13
49) 1,4-Dioxane	9.633	88	76	35.543	ug/l #	1
51) 4-Methyl-2-Pentanone	10.333	43	7174	7.456	ug/l	99
53) t-1,3-Dichloropropene	10.432	75	49	1.946	ug/l #	76
54) cis-1,3-Dichloropropene	10.247	75	48830	8.253	ug/l #	63
56) Ethyl methacrylate	10.875	69	181	1.707	ug/l #	1
57) 1,3-Dichloropropane	11.092	76	28217	4.166	ug/l #	42
59) 2-Hexanone	11.092	43	410038	86.209	ug/l #	51
60) Dibromochloromethane	11.497	129	115	1.999	ug/l #	10
70) Styrene	12.299	104	134	1.465	ug/l #	24
71) Bromoform	12.733	173	1181	3.176	ug/l #	1
76) 1,2,3-Trichloropropane	12.731	75	145482	24.693	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.731	75	145482	70.776	ug/l #	12
93) 1,2,4-Trichlorobenzene	15.273	180	82	2.509	ug/l #	60
95) Naphthalene	15.507	128	2000	3.475	ug/l #	72
96) 1,2,3-Trichlorobenzene	15.710	180	28	2.214	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
Data File : VN069326.D
Acq On : 1 Nov 2021 17:49
Operator : JC/MD
Sample : M4411-04
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Nov 02 05:50:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 28 16:09:15 2021
Response via : Initial Calibration




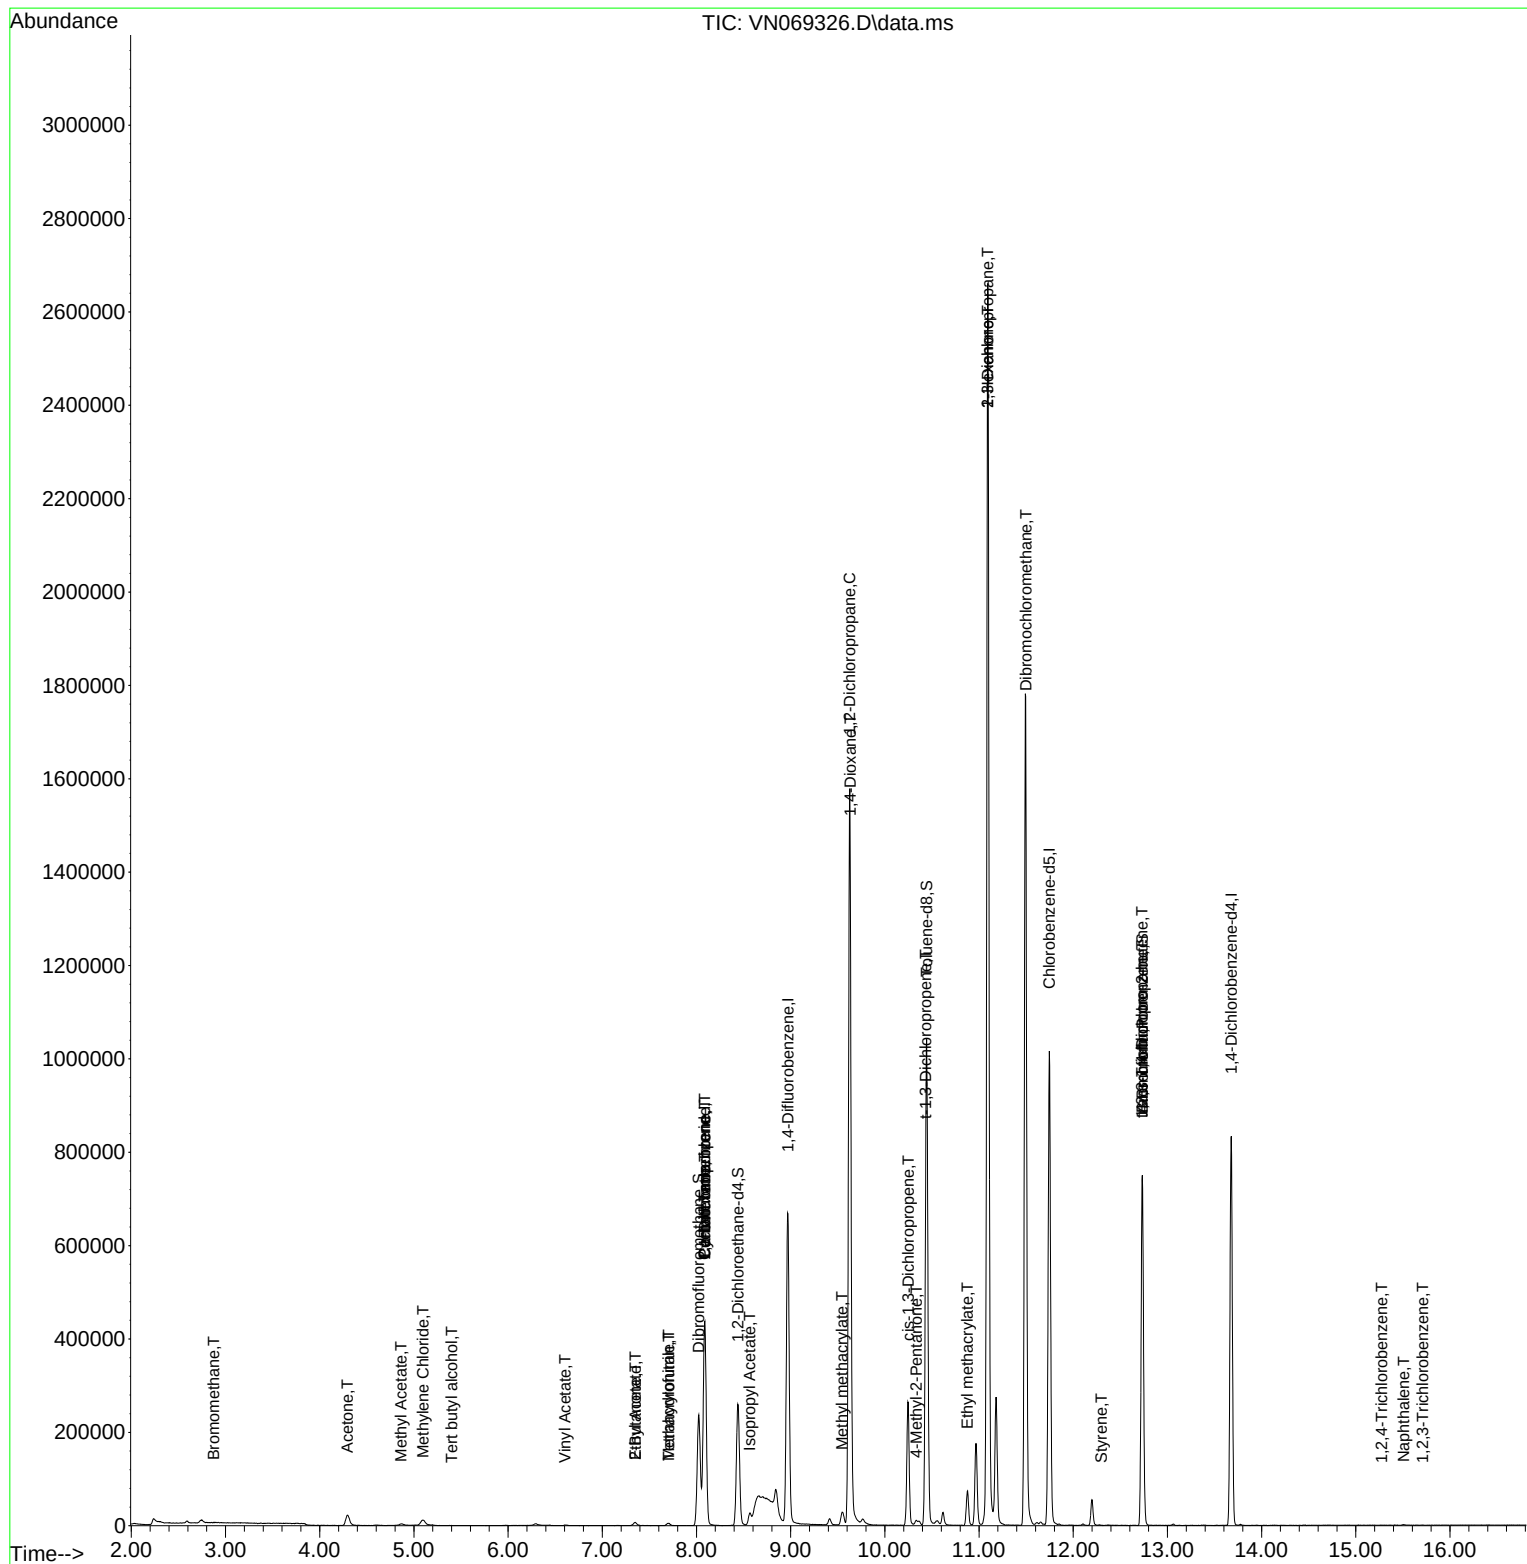




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 325201
Ion Ratio Lower Upper
168 100
99 61.7 48.9 73.3

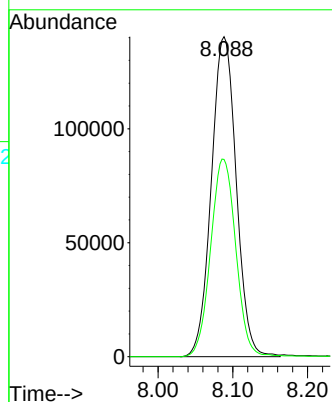

#3
Chloromethane
Concen: Below Cal
RT: 2.306 min Scan# 118
Delta R.T. 0.005 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49

Tgt Ion: 50 Resp: 784
Ion Ratio Lower Upper
50 100
52 0.0 26.3 39.5#


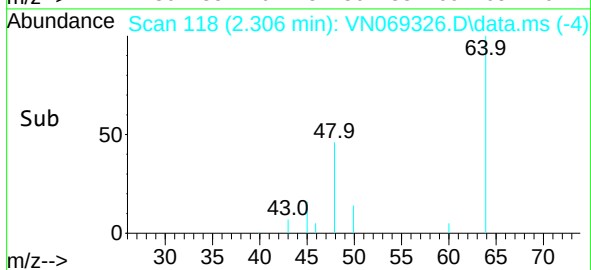
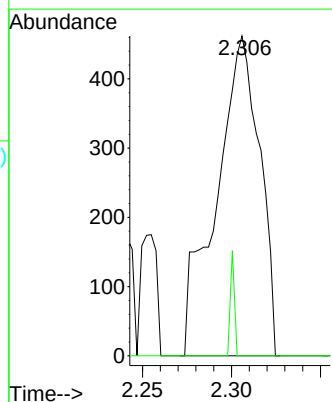



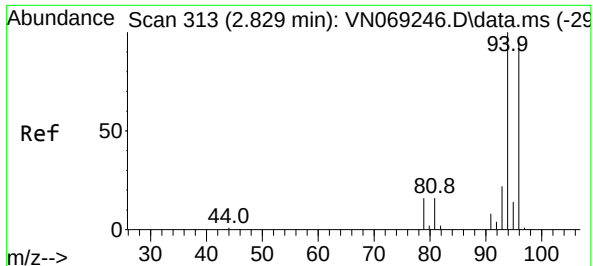

#5
Bromomethane
Concen: 0.268 ug/l
RT: 2.874 min Scan# 31
Delta R.T. 0.045 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 733
Ion Ratio Lower Upper
94 100
96 59.1 74.2 111.4#

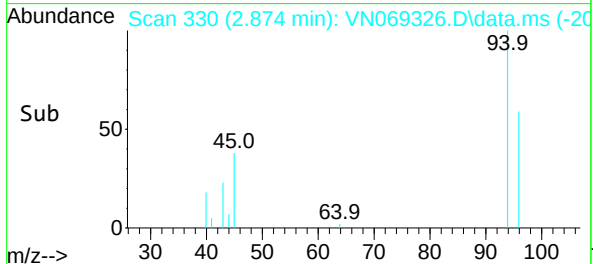

#11
Tert butyl alcohol
Concen: 13.794 ug/l
RT: 5.398 min Scan# 1271
Delta R.T. 0.035 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49

Tgt Ion: 59 Resp: 373
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#




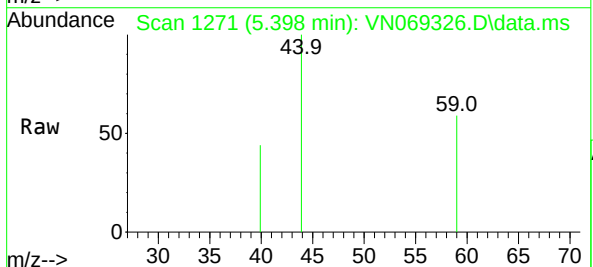




#16
Acetone
Concen: 21.674 ug/l
RT: 4.293 min Scan# 855
Delta R.T. 0.010 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 43350
Ion Ratio Lower Upper
43 100
58 28.3 24.5 36.7

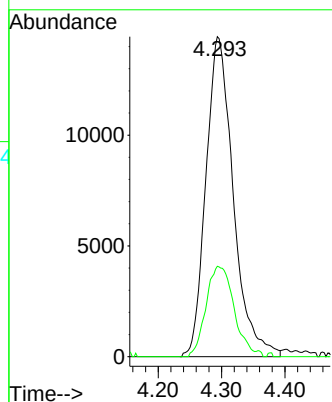

#18
Methyl Acetate
Concen: 0.525 ug/l
RT: 4.862 min Scan# 1071
Delta R.T. 0.011 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49


Tgt Ion: 43 Resp: 3570
Ion Ratio Lower Upper
43 100
74 42.4 18.9 28.3#

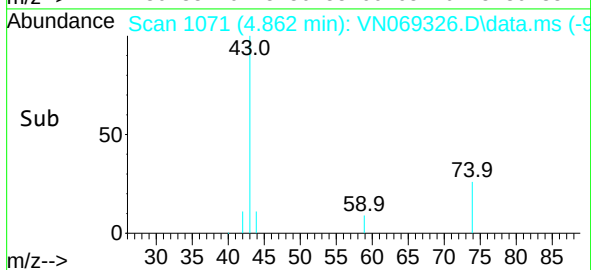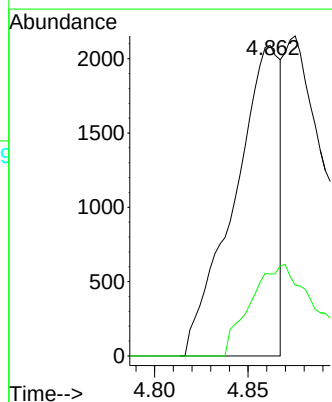



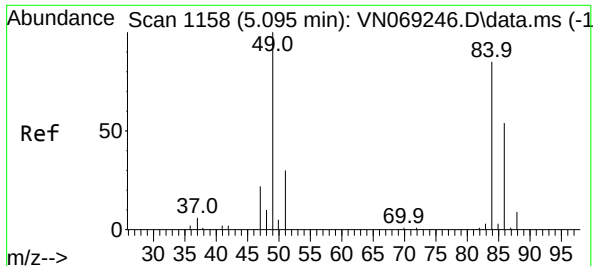


#20
Methylene Chloride
Concen: 2.400 ug/l
RT: 5.095 min Scan# 1158
Delta R.T. 0.000 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion	Ratio	Lower	Upper
84	100		
49	113.5	97.6	146.4
51	33.6	30.3	45.5
86	61.0	51.8	77.6

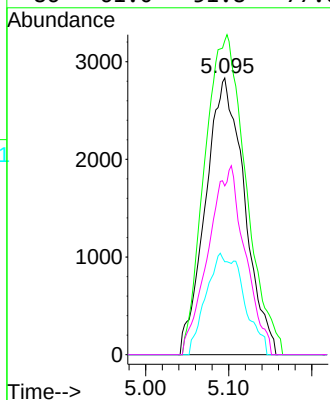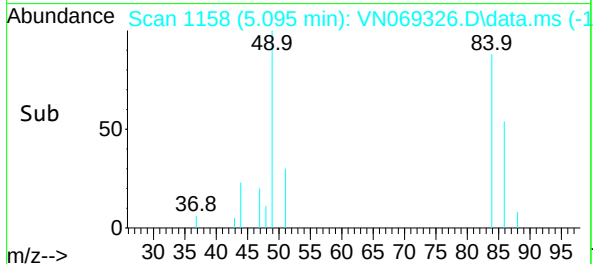


#23
Vinyl Acetate
Concen: 6.598 ug/l
RT: 6.605 min Scan# 1721
Delta R.T. 0.172 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49

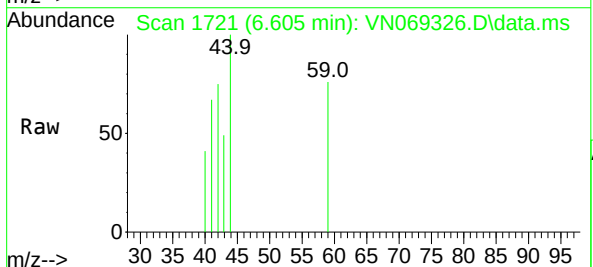

Tgt Ion	Ratio	Lower	Upper
43	100		
86	0.0	8.3	12.5

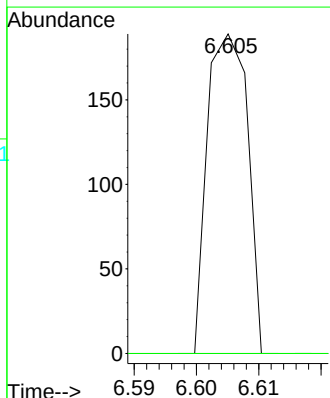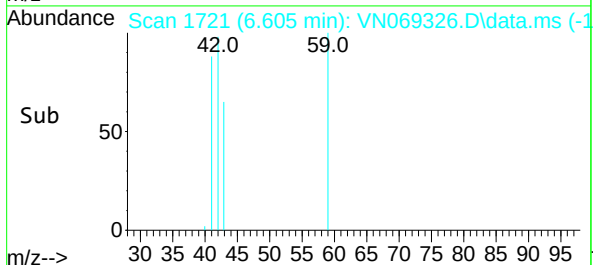



#25

2-Butanone

Concen: 5.533 ug/l

RT: 7.351 min Scan# 1999

Delta R.T. 0.016 min

Lab File: VN069326.D

Acq: 1 Nov 2021 17:49

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 12029

Ion Ratio Lower Upper

43 100

72 26.0 21.2 31.8

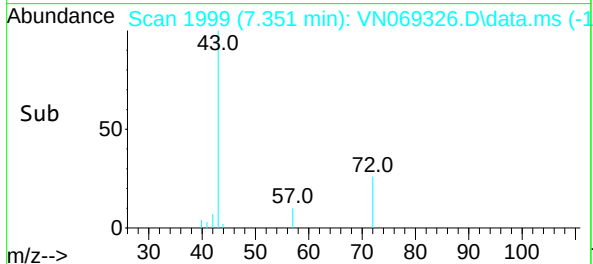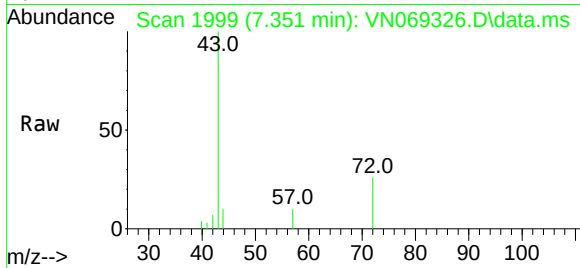

#29

Tetrahydrofuran

Concen: 4.871 ug/l

RT: 7.705 min Scan# 2131

Delta R.T. 0.024 min

Lab File: VN069326.D

Acq: 1 Nov 2021 17:49




Tgt Ion: 42 Resp: 3856


Ion Ratio Lower Upper

42 100

72 19.9 35.4 53.2#


71 22.8 33.8 50.6#

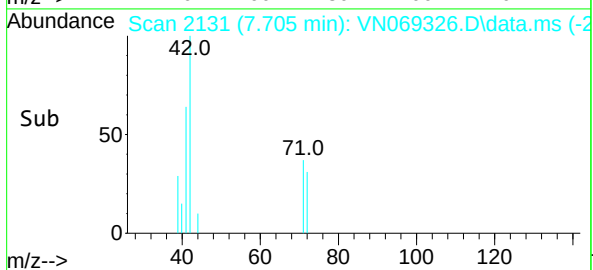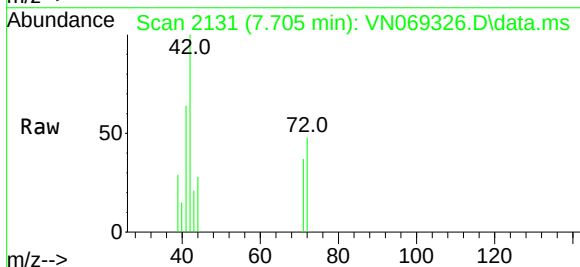






#31
Cyclohexane
Concen: 1.270 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.010 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49

Instrument :
MSVOA_N
ClientSampleId :



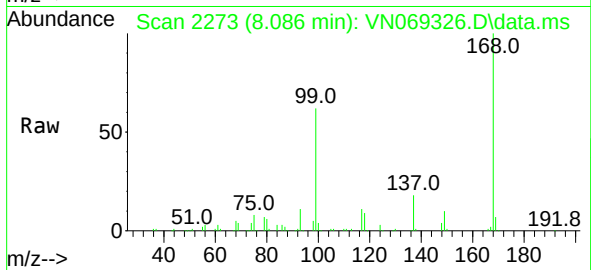



Tgt Ion: 56 Resp: 7981
Ion Ratio Lower Upper
56 100
69 146.4 26.9 40.3#
84 113.8 67.6 101.4#



#33
1,2-Dichloroethane-d4
Concen: 48.758 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49

Tgt Ion: 65 Resp: 228892
Ion Ratio Lower Upper
65 100
67 50.7 0.0 103.8

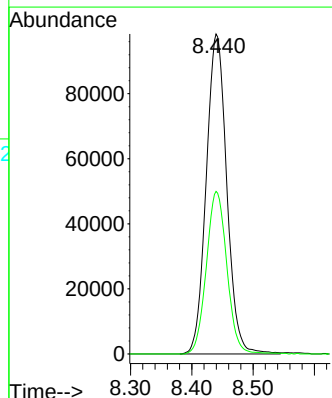



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.971 min Scan# 2

Delta R.T. 0.003 min

Lab File: VN069326.D

Acq: 1 Nov 2021 17:49

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 595132

Ion Ratio Lower Upper

114 100

63 21.2 0.0 42.6

88 15.4 0.0 32.0



#35

Dibromofluoromethane

Concen: 46.538 ug/l

RT: 8.024 min Scan# 2250

Delta R.T. -0.000 min

Lab File: VN069326.D

Acq: 1 Nov 2021 17:49




Tgt Ion:113 Resp: 172648


Ion Ratio Lower Upper

113 100

111 102.8 83.2 124.8


192 18.2 15.0 22.4

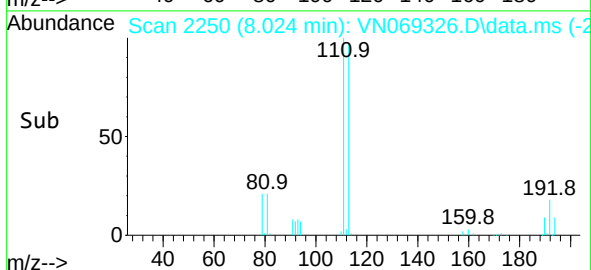






#36
 1,1-Dichloropropene
 Concen: 5.357 ug/l
 RT: 8.086 min Scan# 21
 Delta R.T. -0.136 min
 Lab File: VN069326.D
 Acq: 1 Nov 2021 17:49


Instrument :
 MSVOA_N
 ClientSampleId :





Tgt Ion: 75 Resp: 27487
 Ion Ratio Lower Upper
 75 100
 110 9.0 17.9 53.8#
 77 0.0 24.7 37.1#




#37
 Ethyl Acetate
 Concen: 2.057 ug/l
 RT: 7.351 min Scan# 1999
 Delta R.T. -0.061 min
 Lab File: VN069326.D
 Acq: 1 Nov 2021 17:49




Tgt Ion: 43 Resp: 12029
 Ion Ratio Lower Upper
 43 100
 61 0.0 11.2 16.8#
 70 0.0 8.4 12.6#

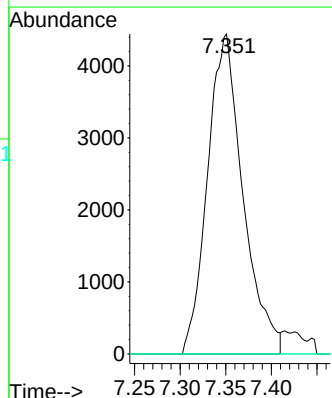






#38
Carbon Tetrachloride
Concen: 6.868 ug/l
RT: 8.088 min Scan# 21
Delta R.T. -0.118 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:117 Resp: 34887
Ion Ratio Lower Upper
117 100
119 4.5 76.9 115.3#
121 0.0 24.6 37.0#




#41
Methacrylonitrile
Concen: 0.826 ug/l
RT: 7.702 min Scan# 2130
Delta R.T. 0.064 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49



Tgt Ion: 41 Resp: 2381
Ion Ratio Lower Upper
41 100
39 42.3 44.9 67.3#
67 0.0 62.6 93.8#
52 0.0 26.2 39.4#



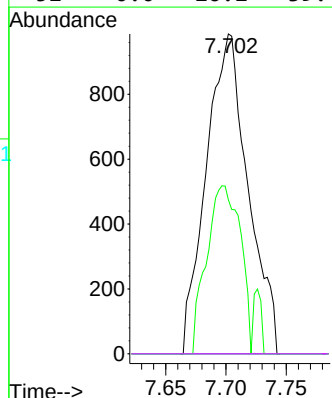



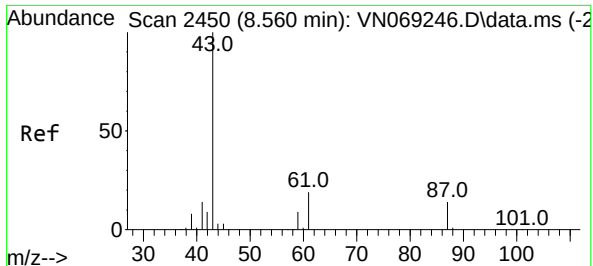

#43
Isopropyl Acetate
Concen: 3.586 ug/l
RT: 8.566 min Scan# 2450
Delta R.T. 0.006 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 32184
Ion Ratio Lower Upper
43 100
61 17.5 20.4 30.6#
87 12.4 10.7 16.1

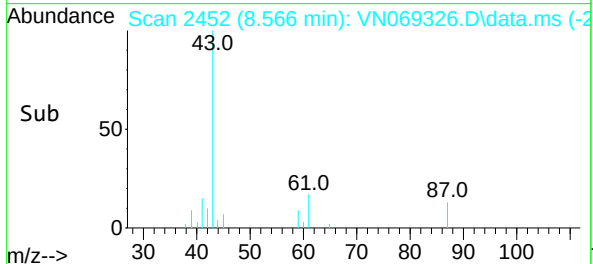

#45
1,2-Dichloropropane
Concen: 0.504 ug/l
RT: 9.625 min Scan# 2847
Delta R.T. 0.134 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49


Tgt Ion: 63 Resp: 1981
Ion Ratio Lower Upper
63 100
65 0.0 25.6 38.4#

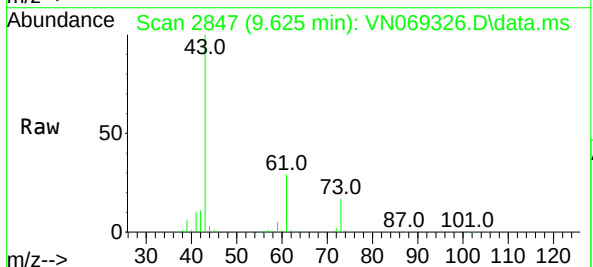






#48
Methyl methacrylate
Concen: 1.765 ug/l
RT: 9.544 min Scan# 21
Delta R.T. -0.017 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 41 Resp: 7788
Ion Ratio Lower Upper
41 100
69 0.0 66.4 99.6#
39 0.0 50.2 75.2#

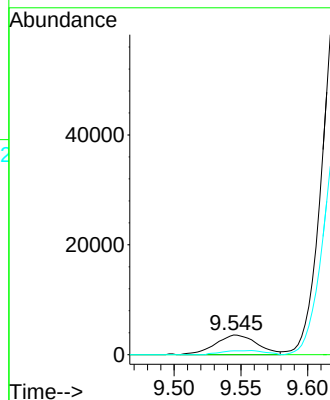


#49
1,4-Dioxane
Concen: 35.543 ug/l
RT: 9.633 min Scan# 2850
Delta R.T. 0.064 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49

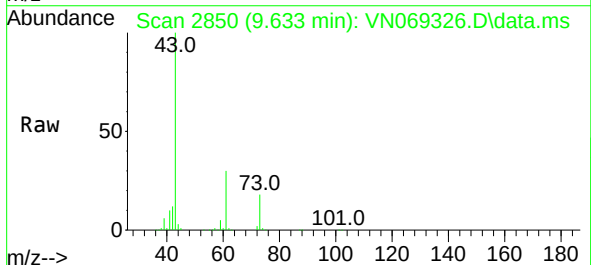

Tgt Ion: 88 Resp: 76
Ion Ratio Lower Upper
88 100
43 2068197.4 24.9 37.3#
58 8525.0 56.9 85.3#



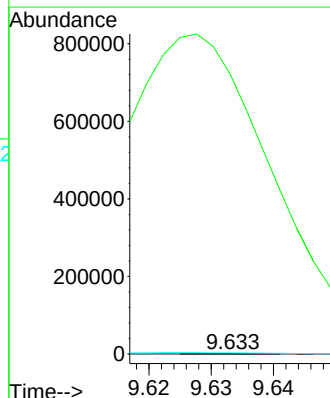
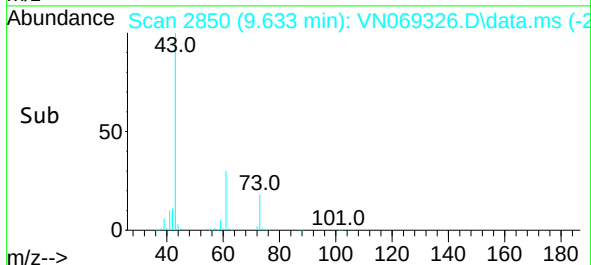




#50
Toluene-d8
Concen: 49.878 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 739841
Ion Ratio Lower Upper
98 100
100 63.9 51.5 77.3

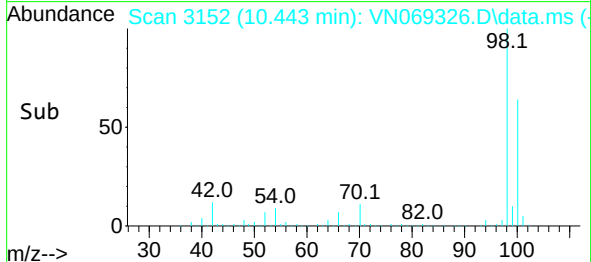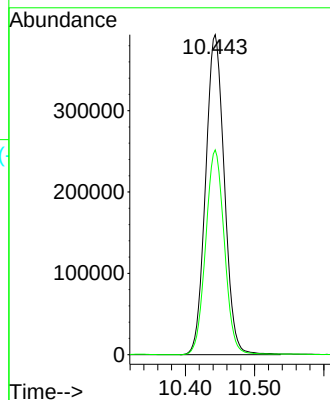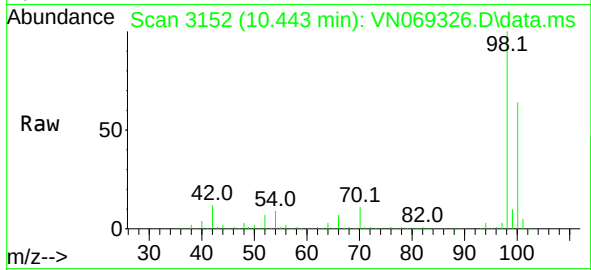

#51
4-Methyl-2-Pentanone
Concen: 7.456 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.003 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49


Tgt Ion: 43 Resp: 7174
Ion Ratio Lower Upper
43 100
58 39.4 31.0 46.4

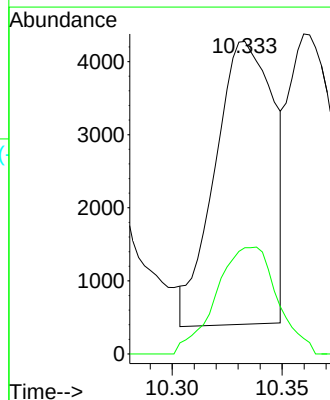






#53
 t-1,3-Dichloropropene
 Concen: 1.946 ug/l
 RT: 10.432 min Scan# 31
 Delta R.T. -0.287 min
 Lab File: VN069326.D
 Acq: 1 Nov 2021 17:49

Instrument :
 MSVOA_N
 ClientSampleId :







Tgt Ion: 75 Resp: 49
 Ion Ratio Lower Upper
 75 100
 77 45.4 25.4 38.2#

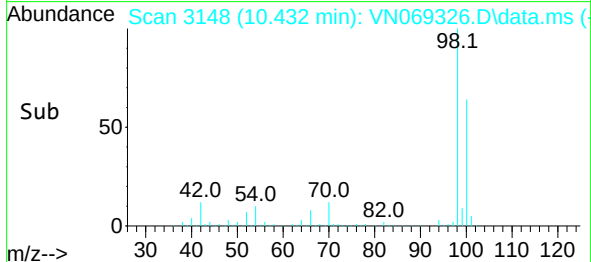

#54
 cis-1,3-Dichloropropene
 Concen: 8.253 ug/l
 RT: 10.247 min Scan# 3079
 Delta R.T. 0.056 min
 Lab File: VN069326.D
 Acq: 1 Nov 2021 17:49

Tgt Ion: 75 Resp: 48830
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.6 38.4#
 39 36.1 42.9 64.3#




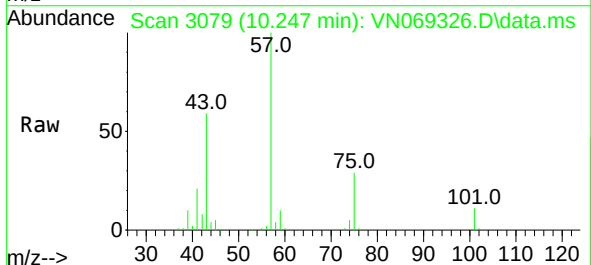


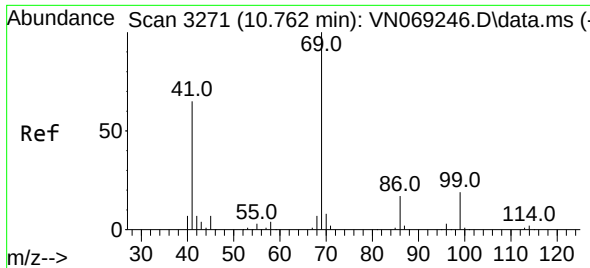

#56
Ethyl methacrylate
Concen: 1.707 ug/l
RT: 10.875 min Scan# 31
Delta R.T. 0.113 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 69 Resp: 181
Ion Ratio Lower Upper
69 100
41 8615.5 53.3 79.9#
39 3877.3 33.3 49.9#

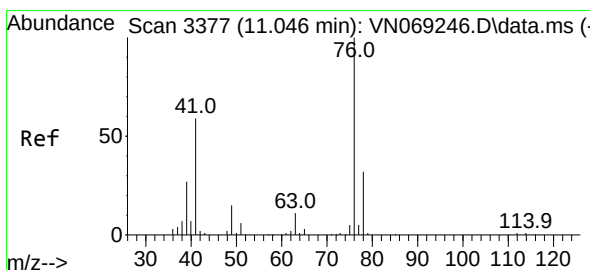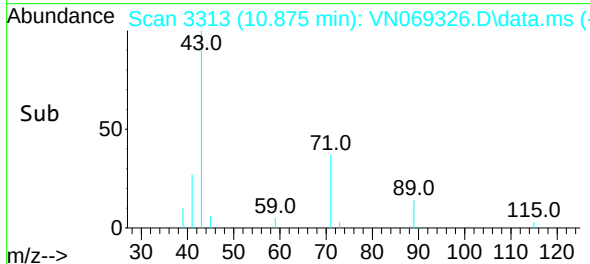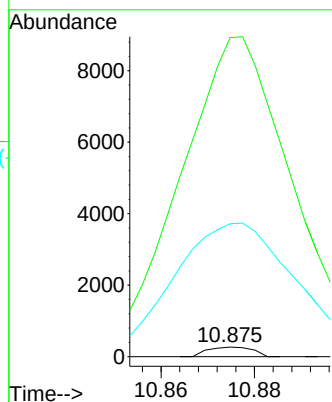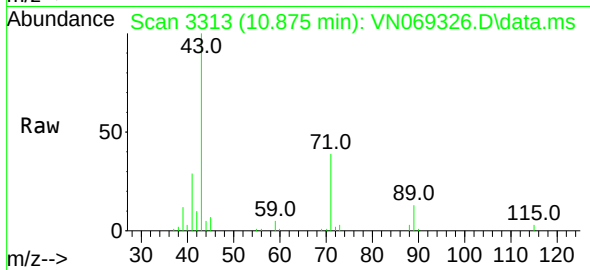

#57
1,3-Dichloropropane
Concen: 4.166 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.046 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49

Tgt Ion: 76 Resp: 28217
Ion Ratio Lower Upper
76 100
78 0.0 25.8 38.8#


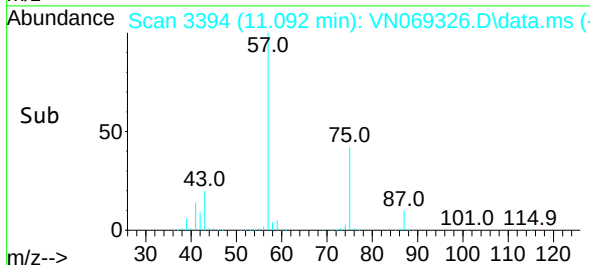

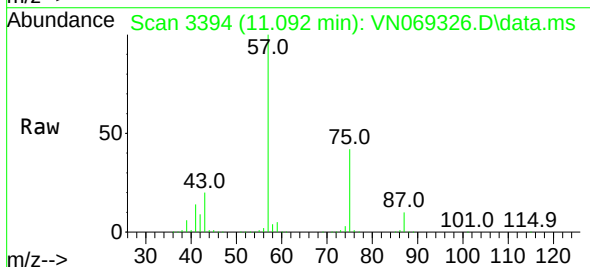




#59
2-Hexanone
Concen: 86.209 ug/l
RT: 11.092 min Scan# 31
Delta R.T. 0.005 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 410038
Ion Ratio Lower Upper
43 100
58 18.7 26.9 80.7#

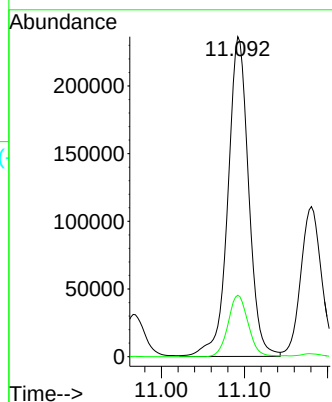

#60
Dibromochloromethane
Concen: 1.999 ug/l
RT: 11.497 min Scan# 3545
Delta R.T. 0.257 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49

Tgt Ion:129 Resp: 115
Ion Ratio Lower Upper
129 100
127 0.0 39.1 117.2#


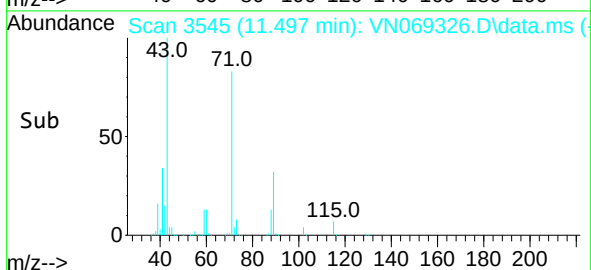

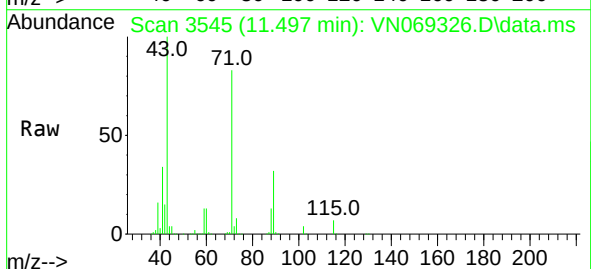




#62
4-Bromofluorobenzene
Concen: 48.243 ug/l
RT: 12.733 min Scan# 4005
Delta R.T. 0.002 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 270033
Ion Ratio Lower Upper
95 100
174 74.8 0.0 144.8
176 72.3 0.0 140.0

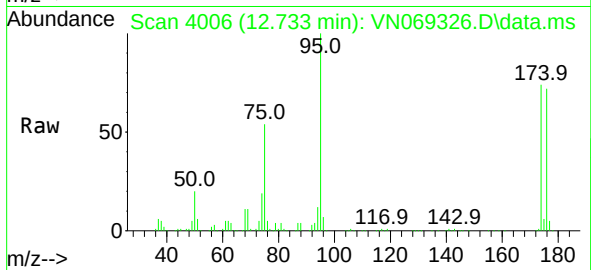

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. -0.000 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49


Tgt Ion: 117 Resp: 593206
Ion Ratio Lower Upper
117 100
82 56.1 46.4 69.6
119 32.0 26.0 39.0

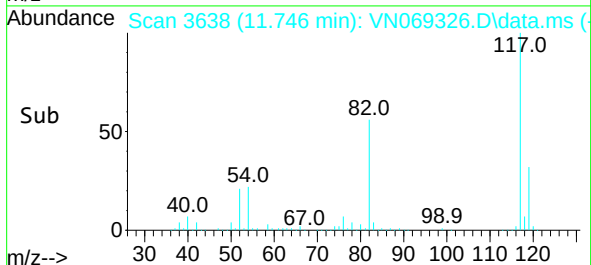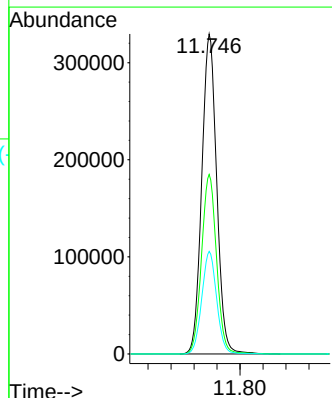






#70
Styrene
Concen: 1.465 ug/l
RT: 12.299 min Scan# 3844
Delta R.T. 0.003 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49

Instrument :
MSVOA_N
ClientSampleId :



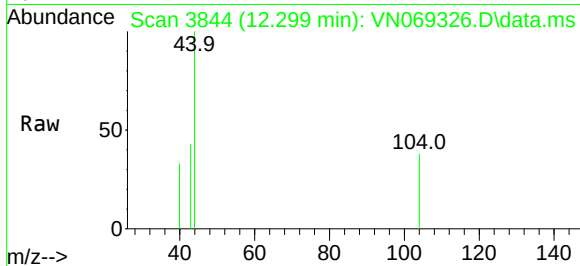



Tgt Ion:104 Resp: 134
Ion Ratio Lower Upper
104 100
78 0.0 42.2 63.4#
103 0.0 44.4 66.6#



#71
Bromoform
Concen: 3.176 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.273 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49


Tgt Ion:173 Resp: 1181
Ion Ratio Lower Upper
173 100
175 1204.9 23.8 71.5#
254 0.0 0.0 0.0

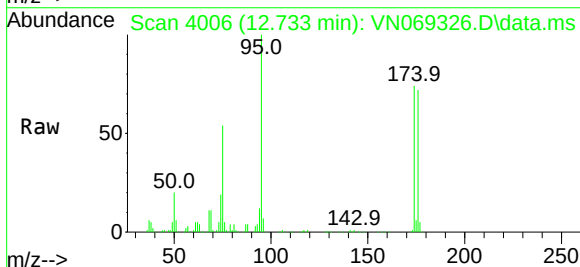



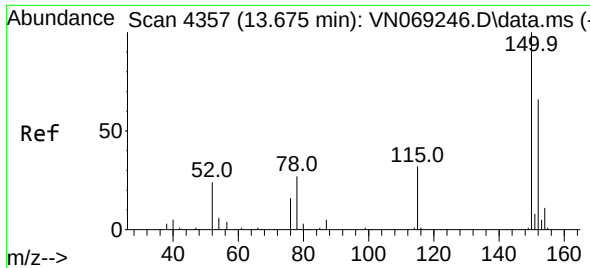


#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.677 min Scan# 41
 Delta R.T. 0.002 min
 Lab File: VN069326.D
 Acq: 1 Nov 2021 17:49

Instrument :
 MSVOA_N
 ClientSampleId :



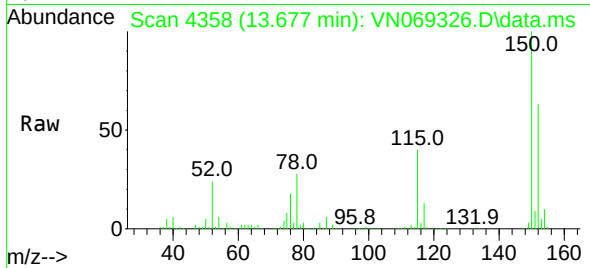



Tgt Ion:152 Resp: 224011
 Ion Ratio Lower Upper
 152 100
 115 63.9 31.4 94.3
 150 157.8 0.0 351.0

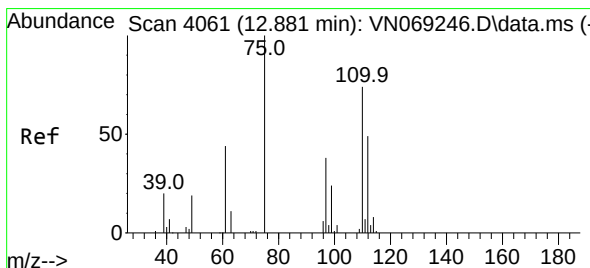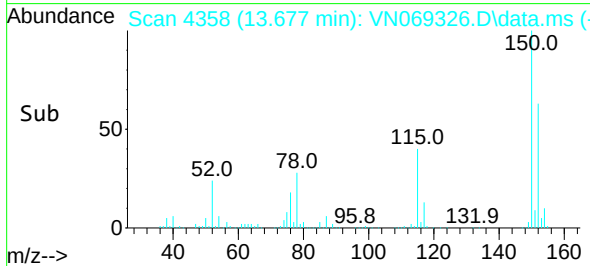

#76
 1,2,3-Trichloropropane
 Concen: 24.693 ug/l
 RT: 12.731 min Scan# 4005
 Delta R.T. -0.150 min
 Lab File: VN069326.D
 Acq: 1 Nov 2021 17:49

Tgt Ion: 75 Resp: 145482
 Ion Ratio Lower Upper
 75 100
 77 0.9 96.2 288.4#


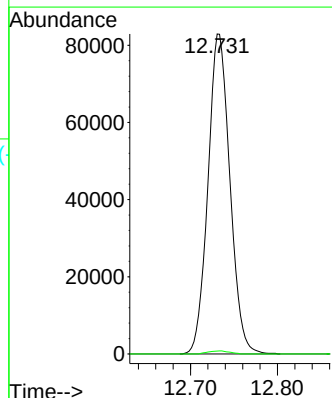
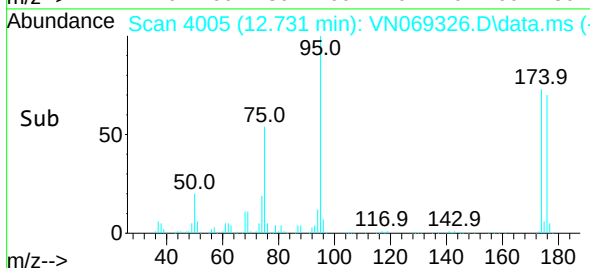
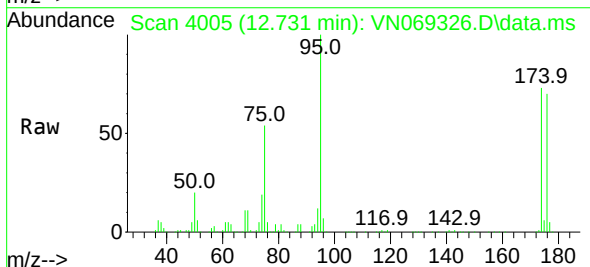




#81
 trans-1,4-Dichloro-2-butene
 Concen: 70.776 ug/l
 RT: 12.731 min Scan# 4005
 Delta R.T. 0.105 min
 Lab File: VN069326.D
 Acq: 1 Nov 2021 17:49




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 145482
 Ion Ratio Lower Upper
 75 100
 53 0.0 75.4 113.2#
 89 0.0 36.9 55.3#

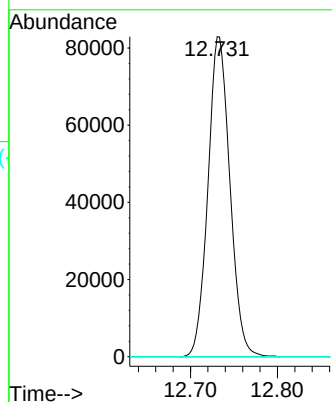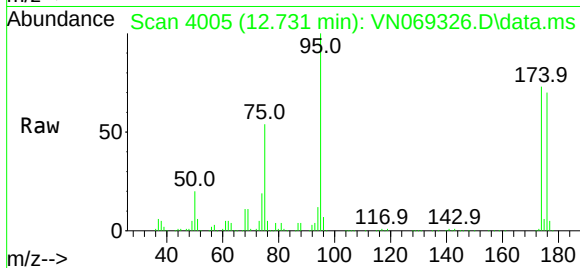

#93
 1,2,4-Trichlorobenzene
 Concen: 2.509 ug/l
 RT: 15.273 min Scan# 4953
 Delta R.T. 0.008 min
 Lab File: VN069326.D
 Acq: 1 Nov 2021 17:49


Tgt Ion:180 Resp: 82
 Ion Ratio Lower Upper
 180 100
 182 62.2 47.9 143.7
 145 0.0 16.4 49.2#

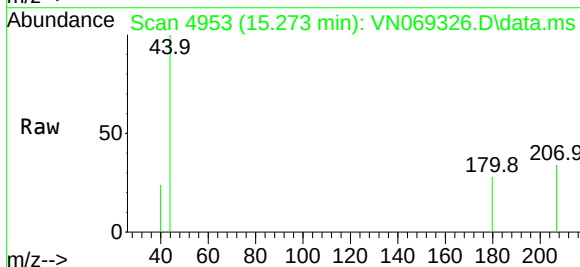



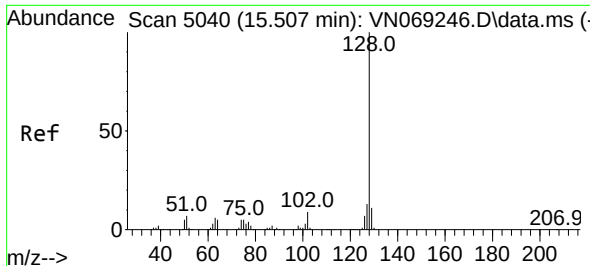


#95
Naphthalene
Concen: 3.475 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49

Instrument :
MSVOA_N
ClientSampleId :

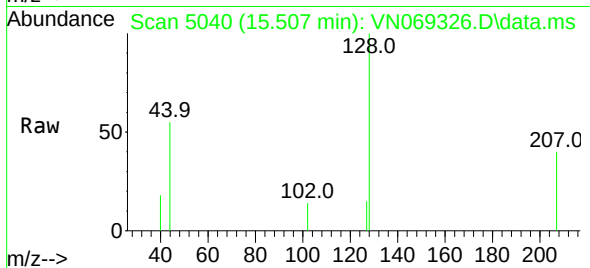

Tgt Ion:128 Resp: 2000
Ion Ratio Lower Upper
128 100
127 2.7 10.5 15.7#
129 0.0 8.9 13.3#

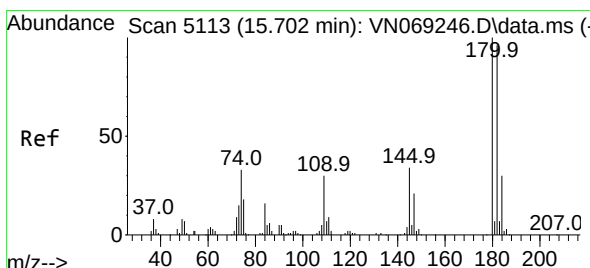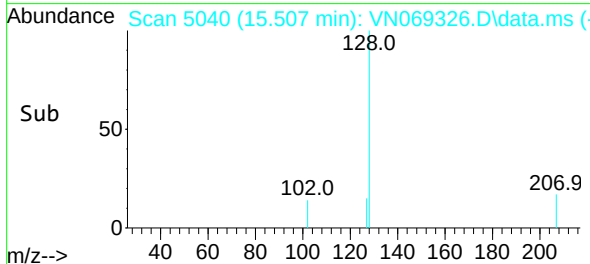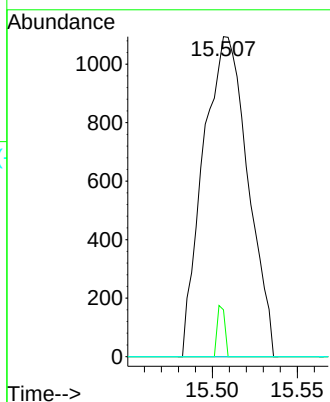

#96
1,2,3-Trichlorobenzene
Concen: 2.214 ug/l
RT: 15.710 min Scan# 5116
Delta R.T. 0.008 min
Lab File: VN069326.D
Acq: 1 Nov 2021 17:49

Tgt Ion:180 Resp: 28
Ion Ratio Lower Upper
180 100
182 317.9 48.1 144.3#
145 0.0 17.4 52.2#

