

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
 Data File : VN069334.D
 Acq On : 1 Nov 2021 21:15
 Operator : JC/MD
 Sample : M4430-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :


Quant Time: Nov 02 05:51:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 28 16:09:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	8.088	168	283571	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	511146	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	524167	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	221477	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	198422	48.473	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	96.940%		
35) Dibromofluoromethane	8.024	113	147864	46.406	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	92.820%		
50) Toluene-d8	10.443	98	647102	50.794	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	101.580%		
62) 4-Bromofluorobenzene	12.733	95	255488	53.145	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	106.280%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.303	50	226	Below Cal	#	42
11) Tert butyl alcohol	5.315	59	686	14.223	ug/l #	72
13) Acrolein	3.990	56	241	1.337	ug/l #	1
16) Acetone	4.307	43	5516	3.163	ug/l	90
25) 2-Butanone	7.335	43	601	1.857	ug/l #	48
26) 2,2-Dichloropropane	7.327	77	161	0.868	ug/l #	53
27) cis-1,2-Dichloroethene	7.337	96	2409	0.708	ug/l	80
30) Chloroform	7.820	83	1378	0.235	ug/l	99
31) Cyclohexane	8.086	56	8482	1.548	ug/l #	20
36) 1,1-Dichloropropene	8.086	75	23546	5.343	ug/l #	49
38) Carbon Tetrachloride	8.088	117	29954	6.866	ug/l #	16
40) Benzene	8.461	78	11879	0.896	ug/l	98
43) Isopropyl Acetate	8.662	43	9727	1.559	ug/l #	55
44) Trichloroethene	9.217	130	2098	0.629	ug/l	86
51) 4-Methyl-2-Pentanone	10.339	43	215	6.439	ug/l #	36
52) Toluene	10.505	92	2323	0.267	ug/l	100
59) 2-Hexanone	11.095	43	311	8.069	ug/l #	25
60) Dibromochloromethane	10.980	129	2531	2.587	ug/l #	10
64) Tetrachloroethene	10.977	164	2376	0.710	ug/l	92
67) Ethyl Benzene	11.846	91	46951	2.498	ug/l	99
68) m/p-Xylenes	11.958	106	36143	5.163	ug/l	97
71) Bromoform	12.731	173	882	3.129	ug/l #	1
76) 1,2,3-Trichloropropane	12.733	75	136372	23.411	ug/l #	1
78) n-propylbenzene	12.924	91	12021	0.570	ug/l	98
80) 1,3,5-Trimethylbenzene	13.061	105	17177	1.111	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.733	75	136372	67.323	ug/l #	12
83) tert-Butylbenzene	13.372	119	4879	0.362	ug/l #	54
84) 1,2,4-Trimethylbenzene	13.369	105	42291	2.798	ug/l	99
85) sec-Butylbenzene	13.369	105	42291	2.264	ug/l #	57
90) Hexachloroethane	14.214	117	321	2.136	ug/l #	12
95) Naphthalene	15.509	128	7099	3.907	ug/l	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 02 05:51:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 28 16:09:15 2021
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 283571
Ion Ratio Lower Upper
168 100
99 60.6 48.9 73.3



#3
Chloromethane
Concen: Below Cal
RT: 2.303 min Scan# 117
Delta R.T. 0.002 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Tgt Ion: 50 Resp: 226
Ion Ratio Lower Upper
50 100
52 0.0 26.3 39.5#



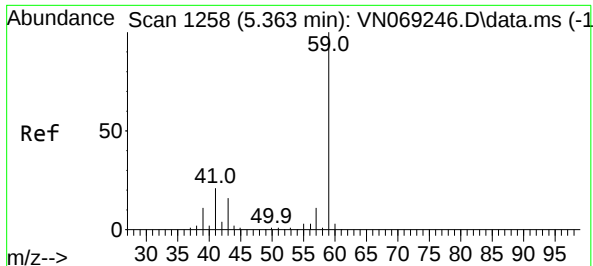

#11

Tert butyl alcohol

Concen: 14.223 ug/l

RT: 5.315 min Scan# 11

Delta R.T. -0.048 min


Lab File: VN069334.D

Acq: 1 Nov 2021 21:15

Instrument :

MSVOA_N

ClientSampleId :



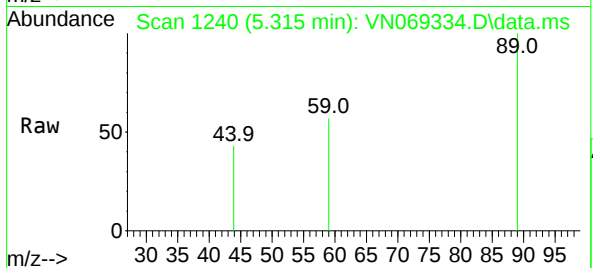


Tgt Ion: 59 Resp: 686

Ion Ratio Lower Upper

59 100

57 0.0 8.3 12.5#

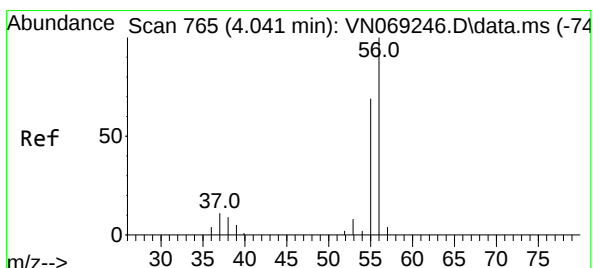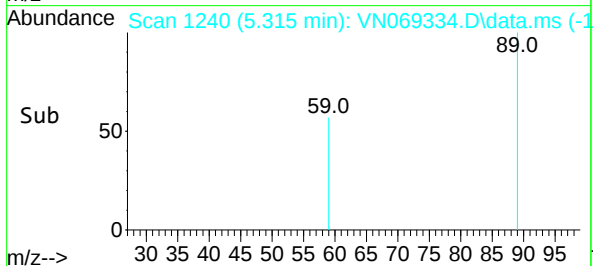

#13

Acrolein

Concen: 1.337 ug/l

RT: 3.990 min Scan# 746

Delta R.T. -0.051 min

Lab File: VN069334.D




Acq: 1 Nov 2021 21:15


Tgt Ion: 56 Resp: 241

Ion Ratio Lower Upper

56 100

55 5395.4 58.1 87.1#


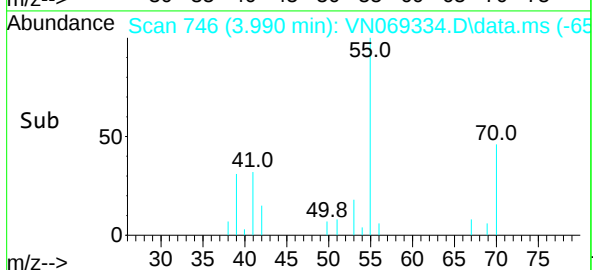

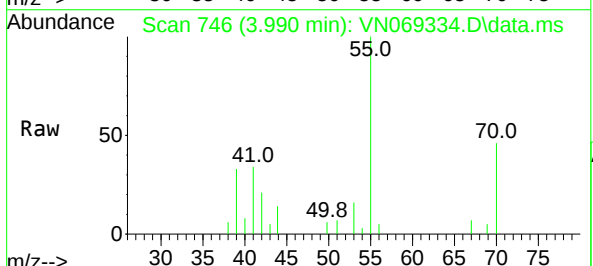




#16
Acetone
Concen: 3.163 ug/l
RT: 4.307 min Scan# 855
Delta R.T. 0.024 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 5516
Ion Ratio Lower Upper
43 100
58 25.3 24.5 36.7

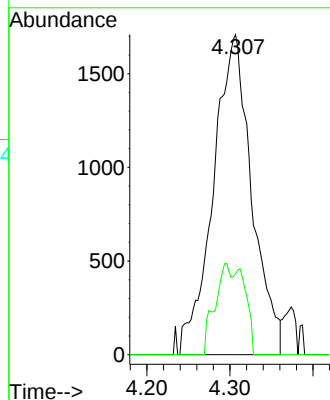

#25
2-Butanone
Concen: 1.857 ug/l
RT: 7.335 min Scan# 1993
Delta R.T. -0.000 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Tgt Ion: 43 Resp: 601
Ion Ratio Lower Upper
43 100
72 0.0 21.2 31.8#

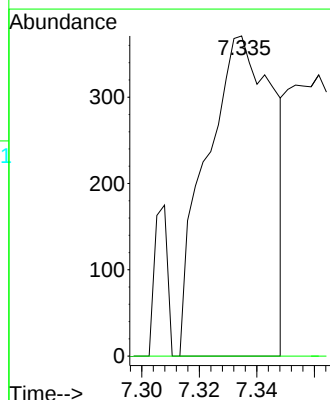

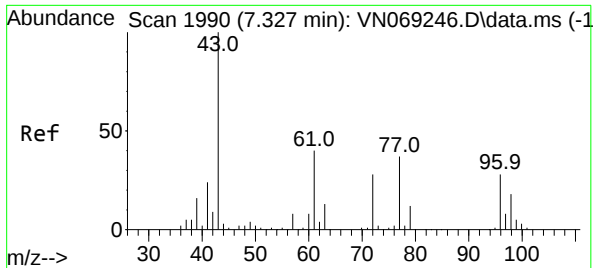

#26

2,2-Dichloropropane

Concen: 0.868 ug/l

RT: 7.327 min Scan# 1990

Delta R.T. -0.000 min

Lab File: VN069334.D

Acq: 1 Nov 2021 21:15

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 77 Resp: 161

Ion Ratio Lower Upper

77 100

97 0.0 11.2 33.6#

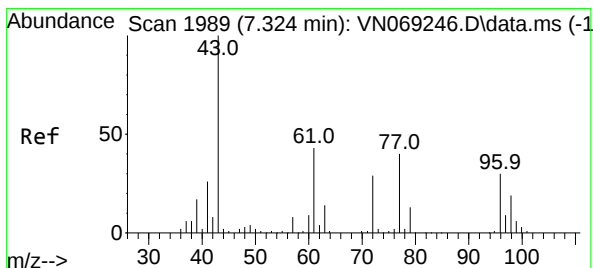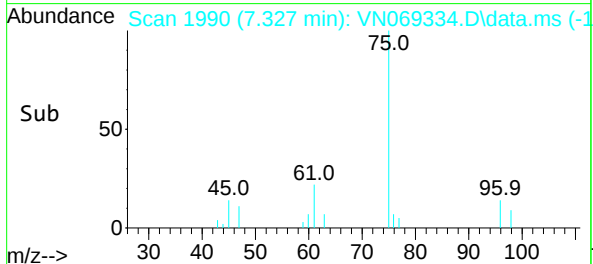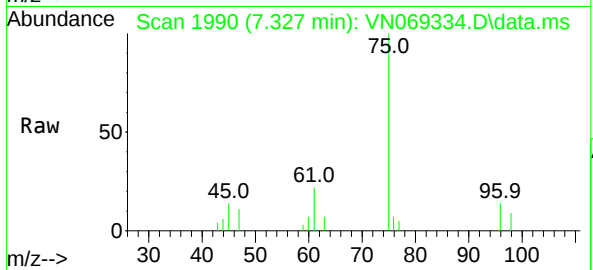

#27

cis-1,2-Dichloroethene

Concen: 0.708 ug/l

RT: 7.337 min Scan# 1994

Delta R.T. 0.013 min

Lab File: VN069334.D

Acq: 1 Nov 2021 21:15




Tgt Ion: 96 Resp: 2409


Ion Ratio Lower Upper

96 100

61 160.1 0.0 290.6

98 34.1 0.0 127.2


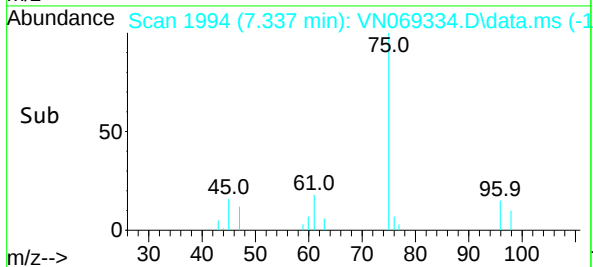

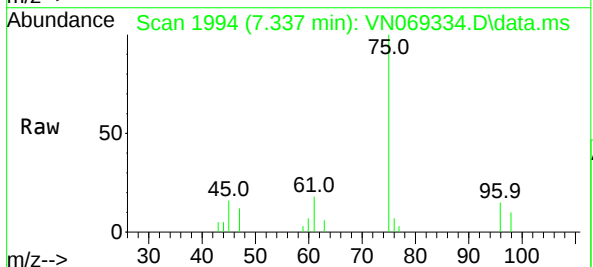




#30
Chloroform
Concen: 0.235 ug/l
RT: 7.820 min Scan# 2174
Delta R.T. 0.000 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 83 Resp: 1378
Ion Ratio Lower Upper
83 100
85 64.8 51.1 76.7



#31
Cyclohexane
Concen: 1.548 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.010 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Tgt Ion: 56 Resp: 8482
Ion Ratio Lower Upper
56 100
69 141.9 26.9 40.3#
84 117.3 67.6 101.4#





#33

1,2-Dichloroethane-d4

Concen: 48.473 ug/l

RT: 8.440 min Scan# 2405

Delta R.T. -0.000 min

Lab File: VN069334.D

Acq: 1 Nov 2021 21:15

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 198422

Ion Ratio Lower Upper

65 100

67 51.7 0.0 103.8



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.971 min Scan# 2603

Delta R.T. 0.003 min

Lab File: VN069334.D

Acq: 1 Nov 2021 21:15




Tgt Ion: 114 Resp: 511146


Ion Ratio Lower Upper

114 100

63 21.3 0.0 42.6


88 15.4 0.0 32.0








#35
Dibromofluoromethane
Concen: 46.406 ug/l
RT: 8.024 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:113 Resp: 147864
Ion Ratio Lower Upper
113 100
111 105.3 83.2 124.8
192 18.7 15.0 22.4




#36
1,1-Dichloropropene
Concen: 5.343 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.136 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15




Tgt Ion: 75 Resp: 23546
Ion Ratio Lower Upper
75 100
110 8.5 17.9 53.8#
77 0.0 24.7 37.1#








#38
Carbon Tetrachloride
Concen: 6.866 ug/l
RT: 8.088 min Scan# 21
Delta R.T. -0.118 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:117 Resp: 29954
Ion Ratio Lower Upper
117 100
119 5.4 76.9 115.3#
121 0.0 24.6 37.0#

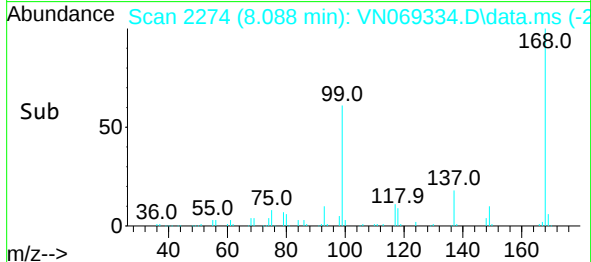

#40
Benzene
Concen: 0.896 ug/l
RT: 8.461 min Scan# 2413
Delta R.T. 0.000 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15


Tgt Ion: 78 Resp: 11879
Ion Ratio Lower Upper
78 100
77 25.0 19.1 28.7

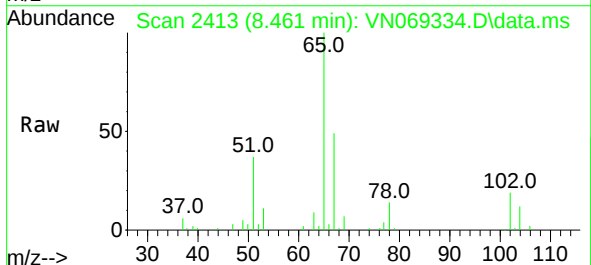






#43
Isopropyl Acetate
Concen: 1.559 ug/l
RT: 8.662 min Scan# 2450
Delta R.T. 0.102 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 9727
Ion Ratio Lower Upper
43 100
61 0.0 20.4 30.6#
87 0.0 10.7 16.1#

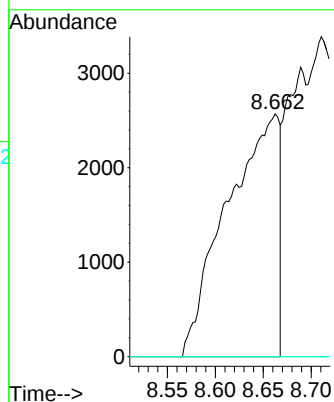

#44
Trichloroethene
Concen: 0.629 ug/l
RT: 9.217 min Scan# 2695
Delta R.T. 0.000 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Tgt Ion:130 Resp: 2098
Ion Ratio Lower Upper
130 100
95 118.1 0.0 208.0



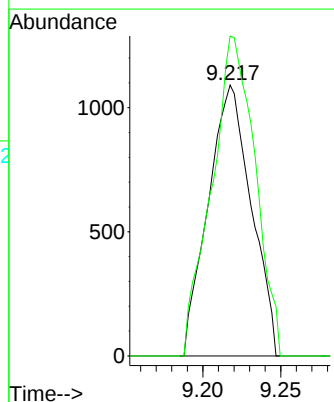





#50
Toluene-d8
Concen: 50.794 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 647102
Ion Ratio Lower Upper
98 100
100 63.9 51.5 77.3



#51
4-Methyl-2-Pentanone
Concen: 6.439 ug/l
RT: 10.339 min Scan# 3113
Delta R.T. 0.008 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Tgt Ion: 43 Resp: 215
Ion Ratio Lower Upper
43 100
58 0.0 31.0 46.4#









#52
Toluene
Concen: 0.267 ug/l
RT: 10.505 min Scan# 3175
Delta R.T. -0.000 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 92 Resp: 2323
Ion Ratio Lower Upper
92 100
91 172.4 138.5 207.7

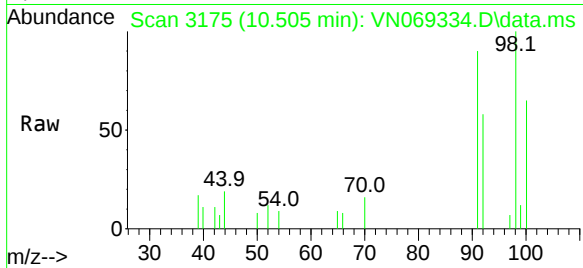

#59
2-Hexanone
Concen: 8.069 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Tgt Ion: 43 Resp: 311
Ion Ratio Lower Upper
43 100
58 0.0 26.9 80.7#




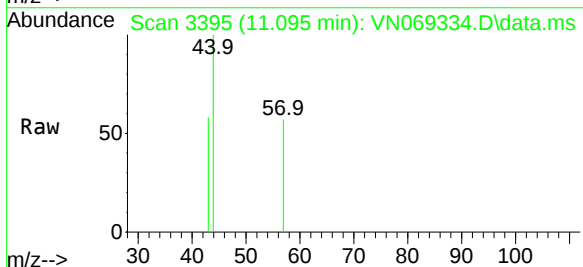




#60
Dibromochloromethane
Concen: 2.587 ug/l
RT: 10.980 min Scan# 31
Delta R.T. -0.261 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:129 Resp: 2531
Ion Ratio Lower Upper
129 100
127 0.0 39.1 117.2#

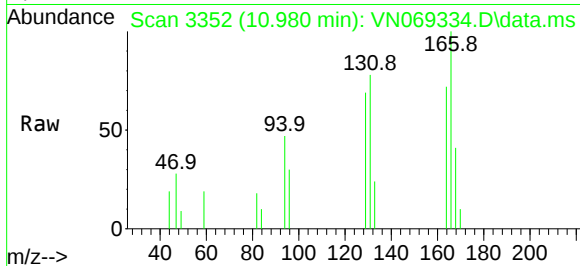

#62
4-Bromofluorobenzene
Concen: 53.145 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.002 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Tgt Ion: 95 Resp: 255488
Ion Ratio Lower Upper
95 100
174 76.1 0.0 144.8
176 72.6 0.0 140.0




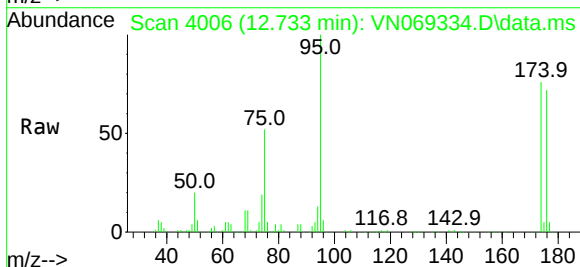




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3
Delta R.T. 0.000 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 524167
Ion Ratio Lower Upper
117 100
82 55.9 46.4 69.6
119 32.4 26.0 39.0

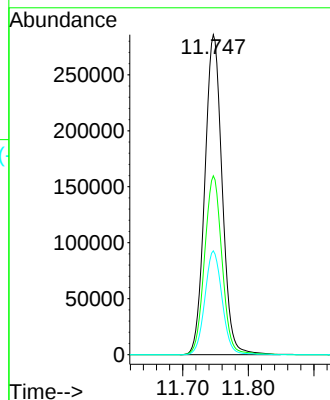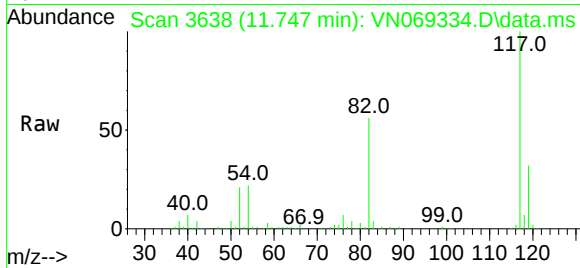

#64
Tetrachloroethene
Concen: 0.710 ug/l
RT: 10.977 min Scan# 3351
Delta R.T. -0.002 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Tgt Ion:164 Resp: 2376
Ion Ratio Lower Upper
164 100
166 133.4 99.8 149.8
129 88.2 79.2 118.8
131 100.4 76.3 114.5



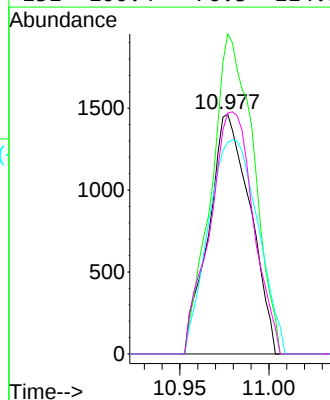
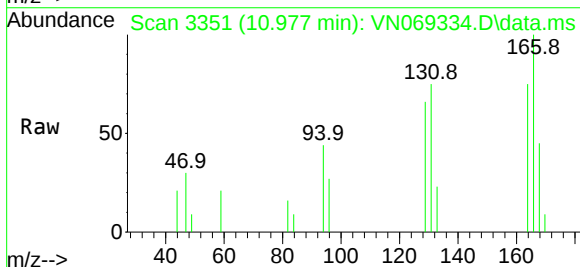


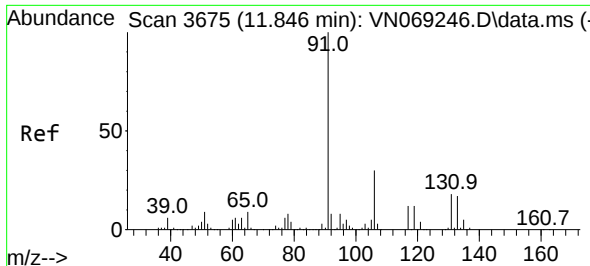

#67
Ethyl Benzene
Concen: 2.498 ug/l
RT: 11.846 min Scan# 3675
Delta R.T. -0.000 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 46951
Ion Ratio Lower Upper
91 100
106 30.4 24.8 37.2

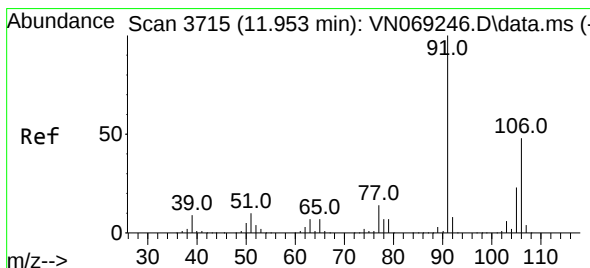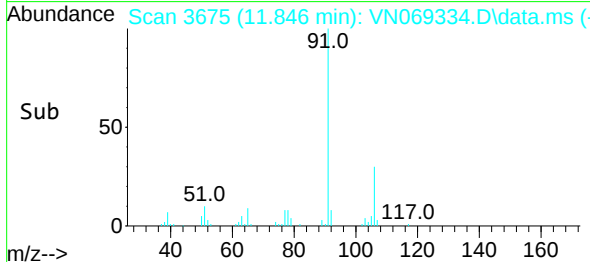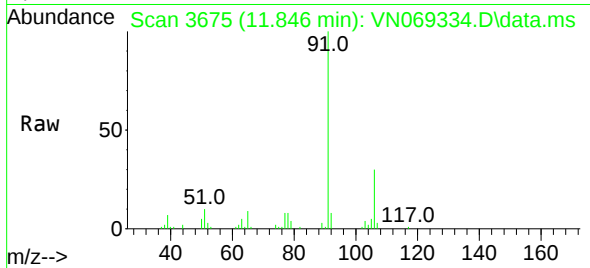

#68
m/p-Xylenes
Concen: 5.163 ug/l
RT: 11.958 min Scan# 3717
Delta R.T. 0.005 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15


Tgt Ion:106 Resp: 36143
Ion Ratio Lower Upper
106 100
91 213.6 166.8 250.2

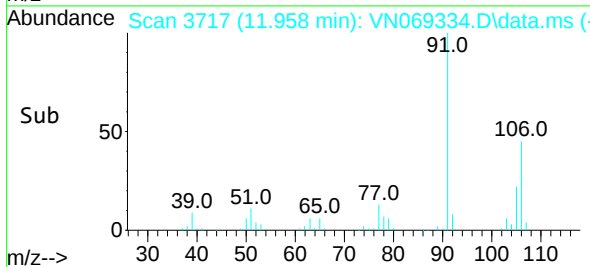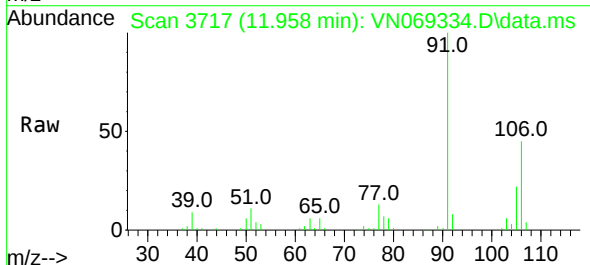



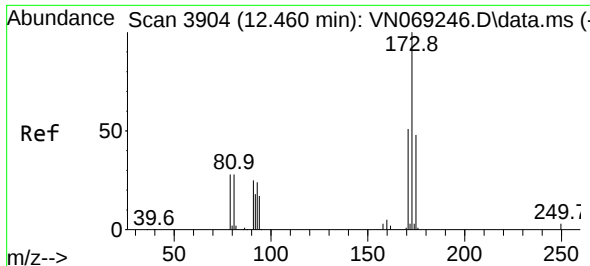


#71
Bromoform
Concen: 3.129 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.271 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Instrument :
MSVOA_N
ClientSampleId :



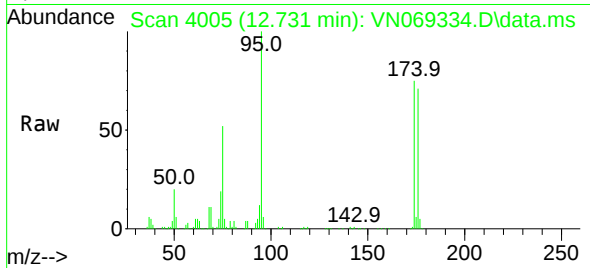



Tgt Ion:173 Resp: 882
Ion Ratio Lower Upper
173 100
175 1552.0 23.8 71.5#
254 0.0 0.0 0.0

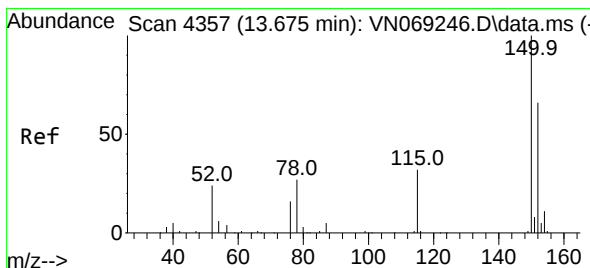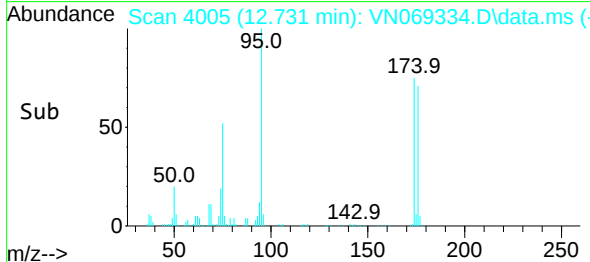

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Tgt Ion:152 Resp: 221477
Ion Ratio Lower Upper
152 100
115 63.1 31.4 94.3
150 158.3 0.0 351.0

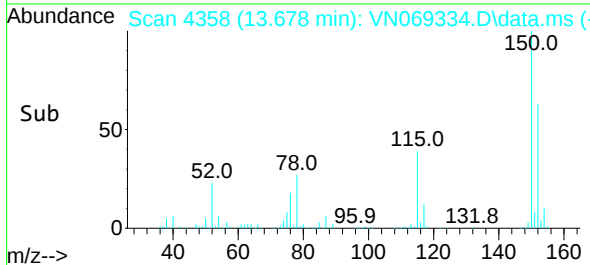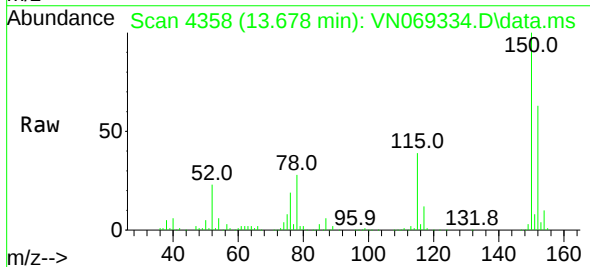



#76

1,2,3-Trichloropropane

Concen: 23.411 ug/l

RT: 12.733 min Scan# 4061

Delta R.T. -0.148 min

Lab File: VN069334.D

Acq: 1 Nov 2021 21:15

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 75 Resp: 136372

Ion Ratio Lower Upper

75 100

77 0.9 96.2 288.4#



#78

n-propylbenzene

Concen: 0.570 ug/l

RT: 12.924 min Scan# 4077

Delta R.T. 0.003 min

Lab File: VN069334.D




Acq: 1 Nov 2021 21:15


Tgt Ion: 91 Resp: 12021

Ion Ratio Lower Upper

91 100

120 21.7 11.4 34.1









#80
1,3,5-Trimethylbenzene
Concen: 1.111 ug/l
RT: 13.061 min Scan# 4128
Delta R.T. -0.000 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:105 Resp: 17177
Ion Ratio Lower Upper
105 100
120 48.2 23.4 70.2

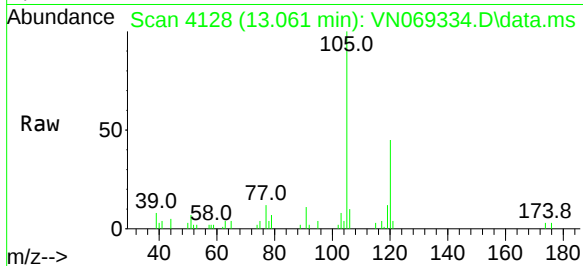

#81
trans-1,4-Dichloro-2-butene
Concen: 67.323 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.107 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Tgt Ion: 75 Resp: 136372
Ion Ratio Lower Upper
75 100
53 0.0 75.4 113.2#
89 0.0 36.9 55.3#




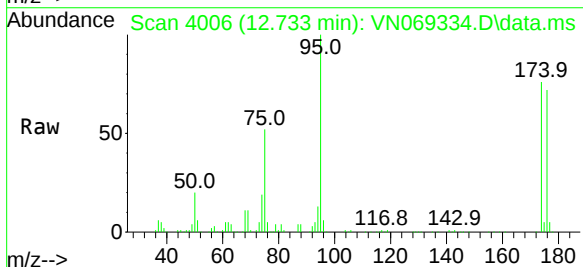




#83
tert-Butylbenzene
Concen: 0.362 ug/l
RT: 13.372 min Scan# 41
Delta R.T. 0.046 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:119 Resp: 4879
Ion Ratio Lower Upper
119 100
91 105.6 34.6 103.9#
134 0.0 12.6 37.6#

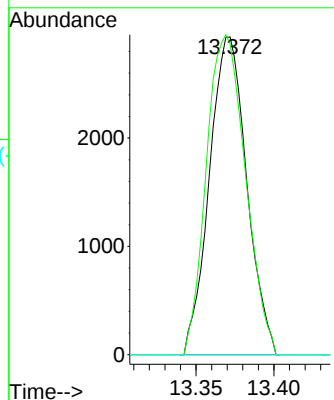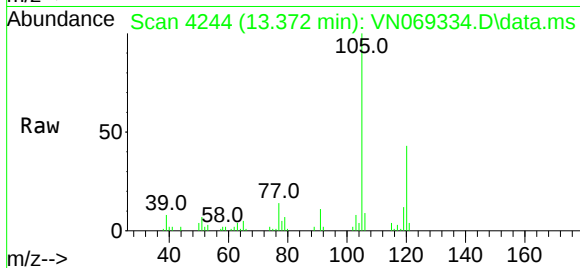

#84
1,2,4-Trimethylbenzene
Concen: 2.798 ug/l
RT: 13.369 min Scan# 4243
Delta R.T. 0.000 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Tgt Ion:105 Resp: 42291
Ion Ratio Lower Upper
105 100
120 42.9 21.9 65.5


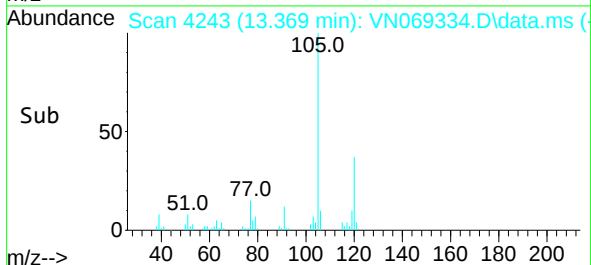
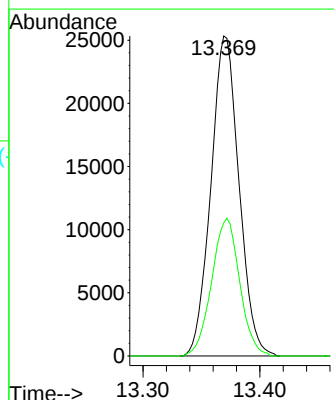
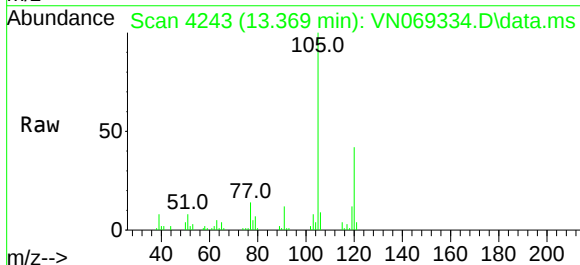




#85
 sec-Butylbenzene
 Concen: 2.264 ug/l
 RT: 13.369 min Scan# 41
 Delta R.T. -0.134 min
 Lab File: VN069334.D
 Acq: 1 Nov 2021 21:15




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:105 Resp: 42291
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.8 29.4#

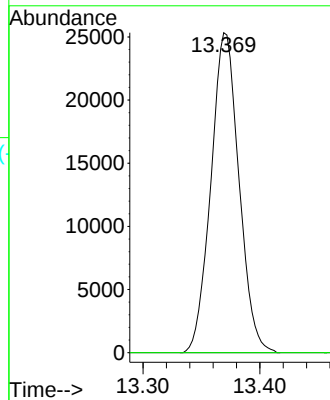

#90
 Hexachloroethane
 Concen: 2.136 ug/l
 RT: 14.214 min Scan# 4558
 Delta R.T. 0.003 min
 Lab File: VN069334.D
 Acq: 1 Nov 2021 21:15


Tgt Ion:117 Resp: 321
 Ion Ratio Lower Upper
 117 100
 201 0.0 37.1 111.5#

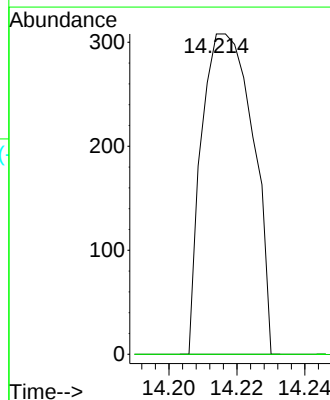



#95
Naphthalene
Concen: 3.907 ug/l
RT: 15.509 min Scan# 50
Delta R.T. 0.002 min
Lab File: VN069334.D
Acq: 1 Nov 2021 21:15

Instrument :
MSVOA_N
ClientSampleId :



Tgt Ion:128 Resp: 7099
Ion Ratio Lower Upper
128 100
127 11.3 10.5 15.7
129 10.0 8.9 13.3

