

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
 Data File : VN069329.D
 Acq On : 1 Nov 2021 19:06
 Operator : JC/MD
 Sample : M4423-02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-REF-5

Quant Time: Nov 02 05:50:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 28 16:09:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	283007	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	511749	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	507019	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	199334	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	197061	48.236	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	96.480%
35) Dibromofluoromethane	8.024	113	148740	46.626	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	93.260%
50) Toluene-d8	10.443	98	635151	49.797	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	99.600%
62) 4-Bromofluorobenzene	12.733	95	236856	49.211	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	98.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
Data File : VN069329.D
Acq On : 1 Nov 2021 19:06
Operator : JC/MD
Sample : M4423-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-REF-5

Quant Time: Nov 02 05:50:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 28 16:09:15 2021
Response via : Initial Calibration




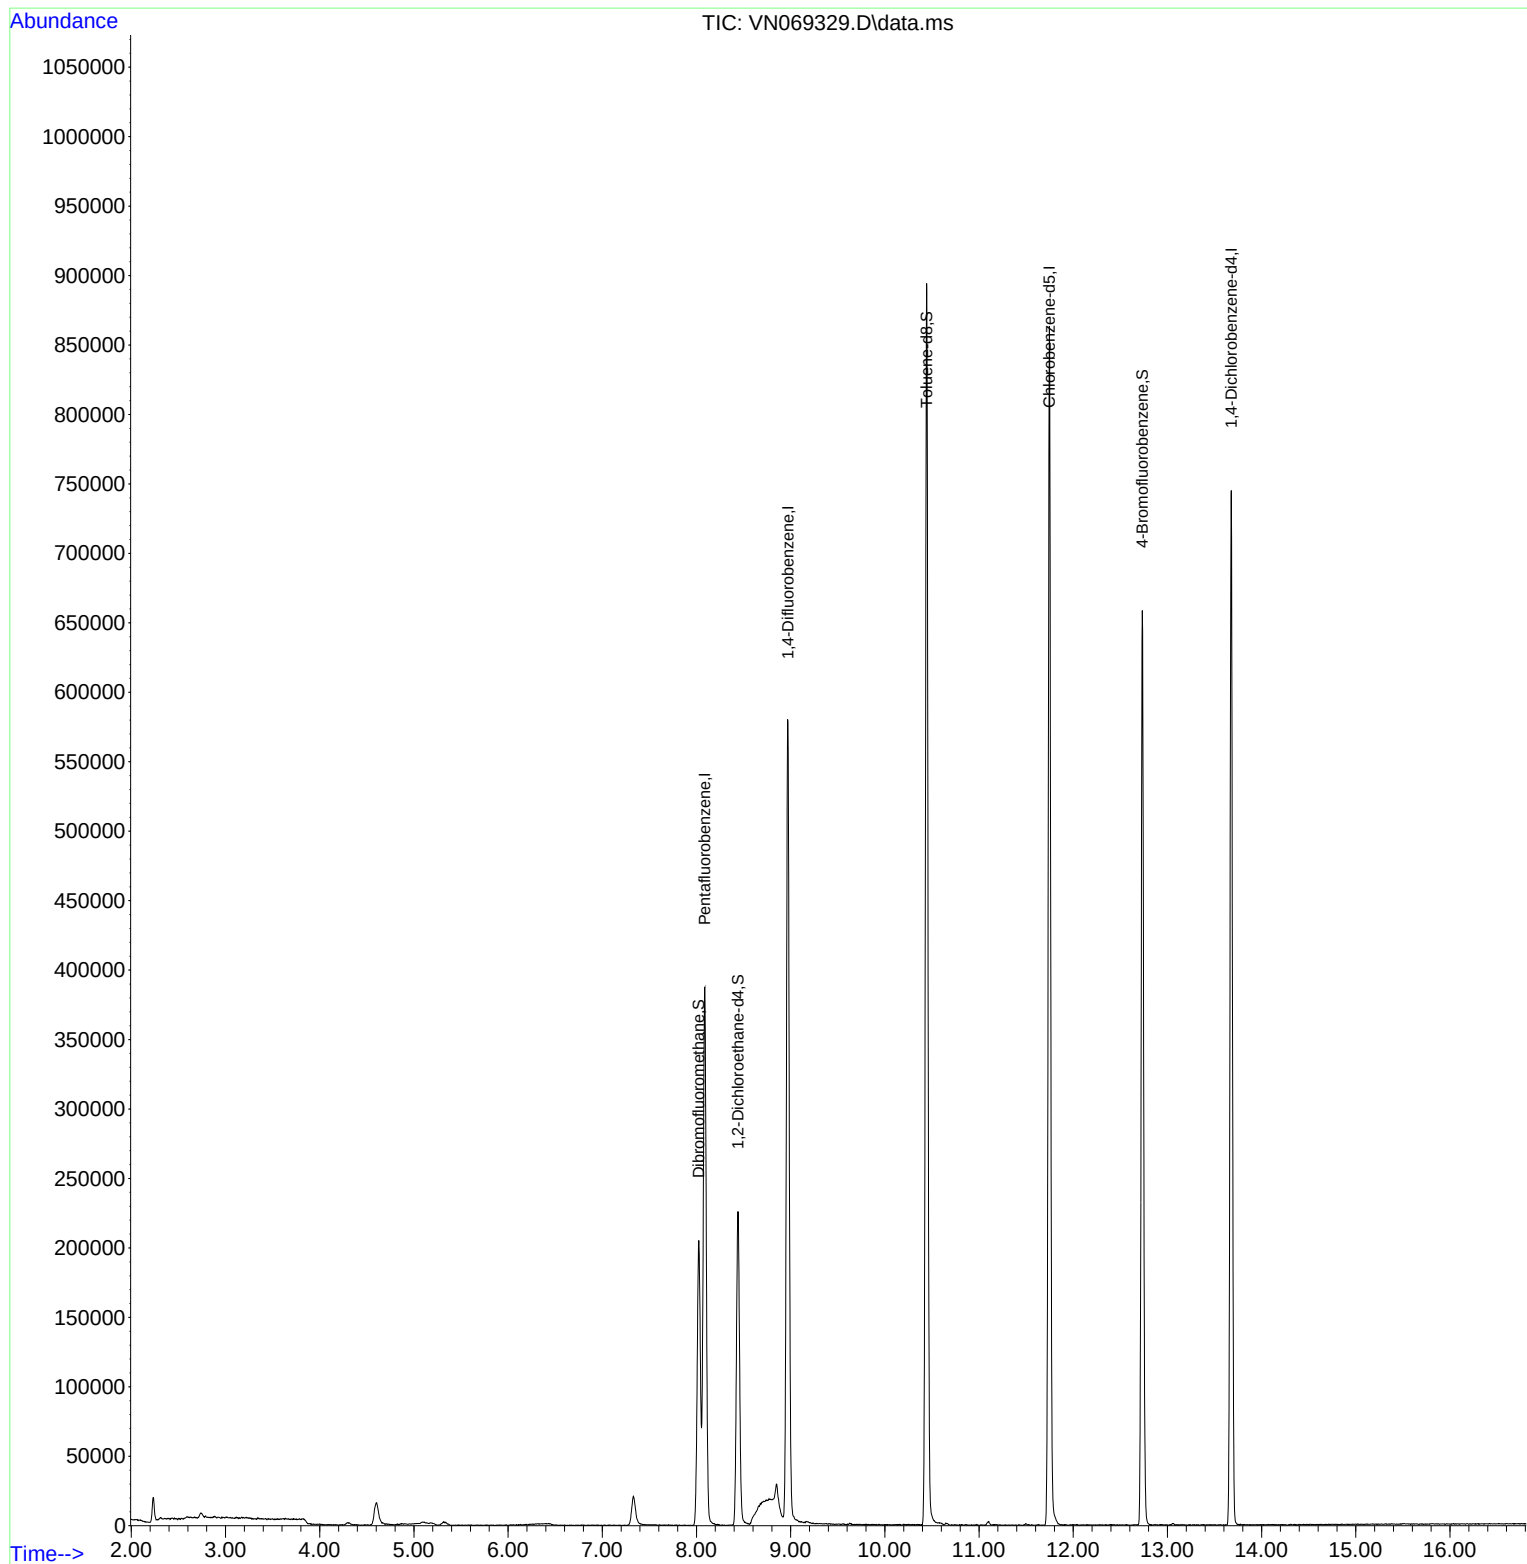


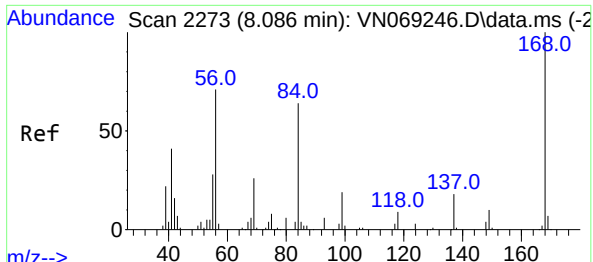

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069329.D
Acq: 1 Nov 2021 19:06




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-REF-5


Tgt Ion:168 Resp: 283007
Ion Ratio Lower Upper
168 100
99 62.7 48.9 73.3

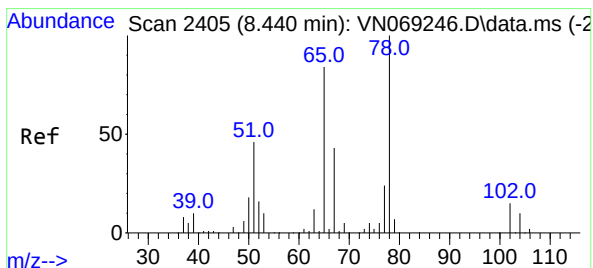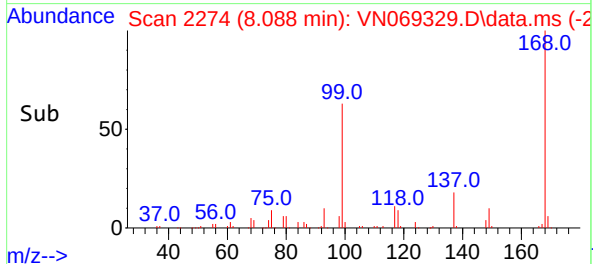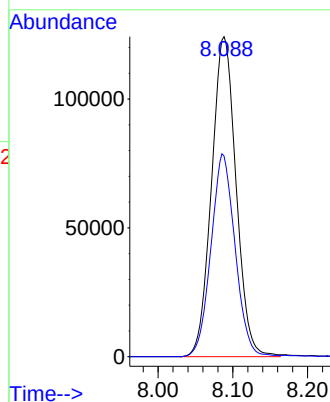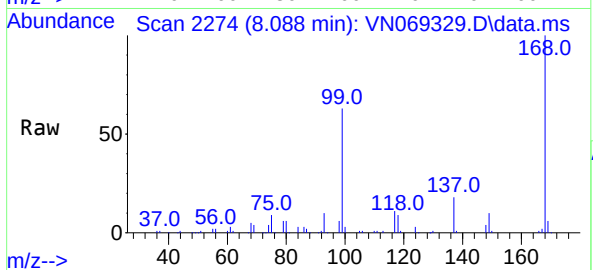

#33
1,2-Dichloroethane-d4
Concen: 48.236 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN069329.D
Acq: 1 Nov 2021 19:06

Tgt Ion: 65 Resp: 197061
Ion Ratio Lower Upper
65 100
67 50.6 0.0 103.8

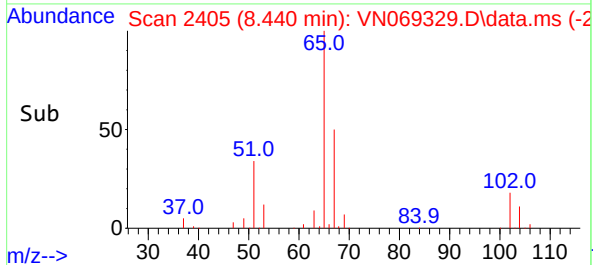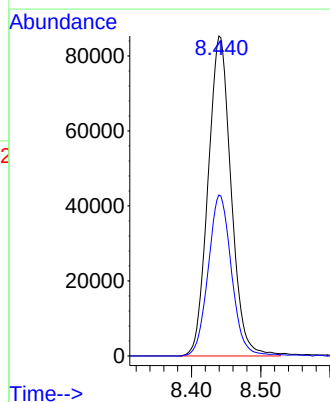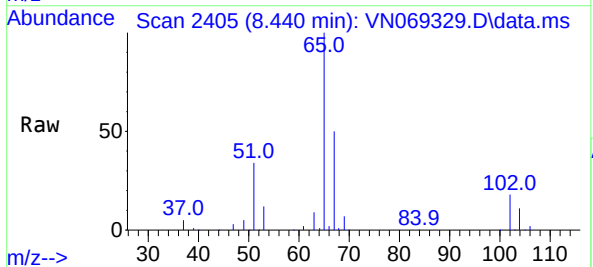

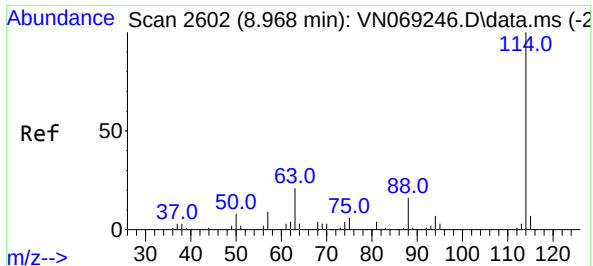

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.971 min Scan# 2

Delta R.T. 0.003 min

Lab File: VN069329.D

Acq: 1 Nov 2021 19:06

Instrument :

MSVOA_N

ClientSampleId :

STORAGE-BLANK-REF-5





Tgt Ion:114 Resp: 511749

Ion Ratio Lower Upper

114 100

63 20.3 0.0 42.6

88 15.9 0.0 32.0

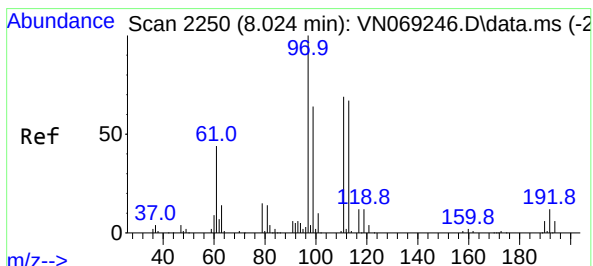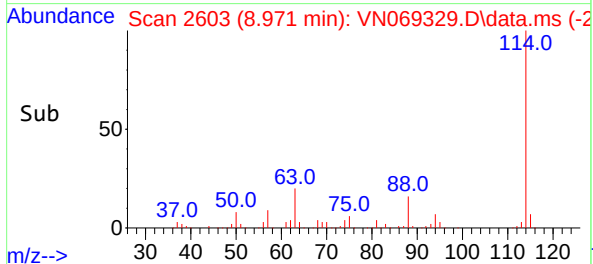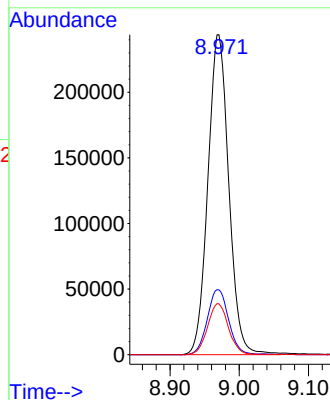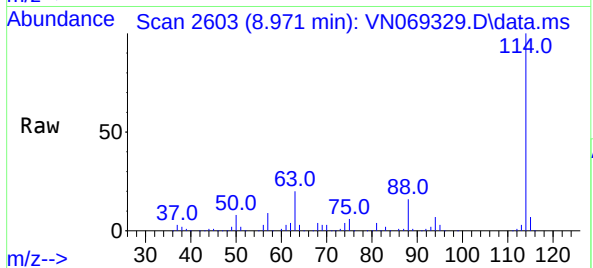

#35

Dibromofluoromethane

Concen: 46.626 ug/l

RT: 8.024 min Scan# 2250

Delta R.T. -0.000 min

Lab File: VN069329.D

Acq: 1 Nov 2021 19:06




Tgt Ion:113 Resp: 148740


Ion Ratio Lower Upper

113 100

111 103.4 83.2 124.8

192 18.0 15.0 22.4


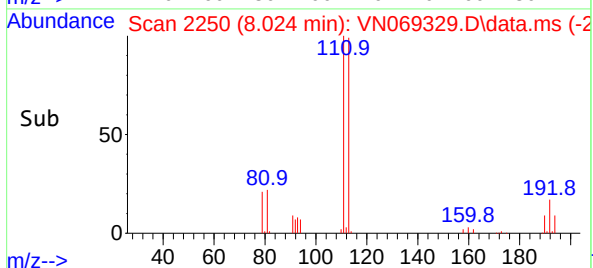
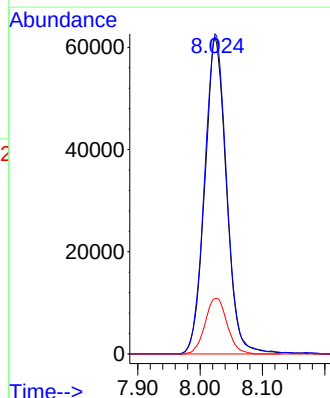
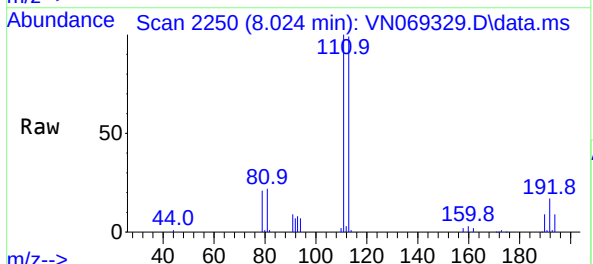


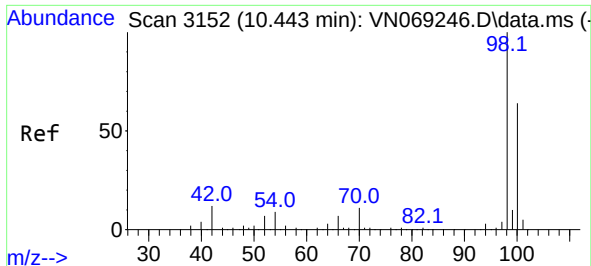

#50
Toluene-d8
Concen: 49.797 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VN069329.D
Acq: 1 Nov 2021 19:06




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-REF-5


Tgt Ion: 98 Resp: 635151
Ion Ratio Lower Upper
98 100
100 64.3 51.5 77.3

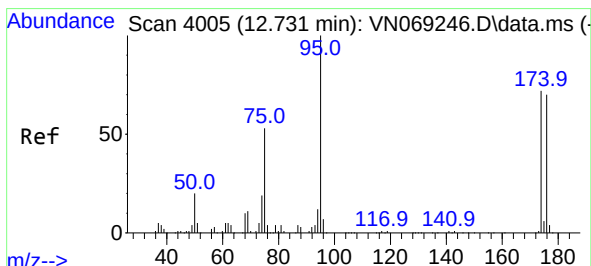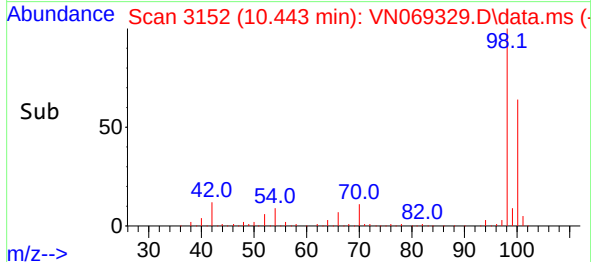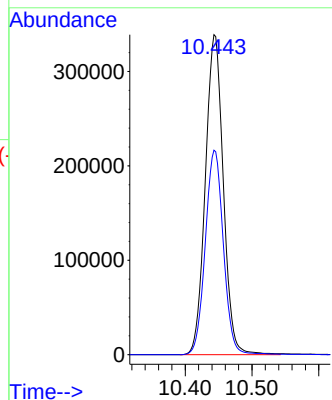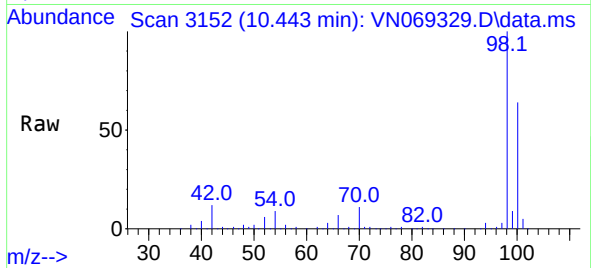

#62
4-Bromofluorobenzene
Concen: 49.211 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.002 min
Lab File: VN069329.D
Acq: 1 Nov 2021 19:06

Tgt Ion: 95 Resp: 236856
Ion Ratio Lower Upper
95 100
174 75.5 0.0 144.8
176 72.4 0.0 140.0


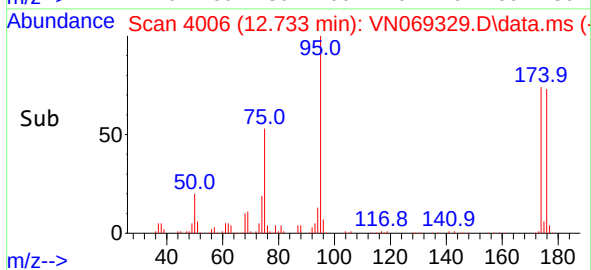
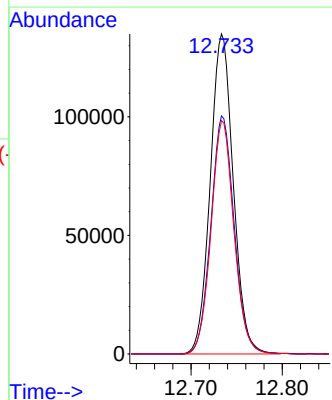
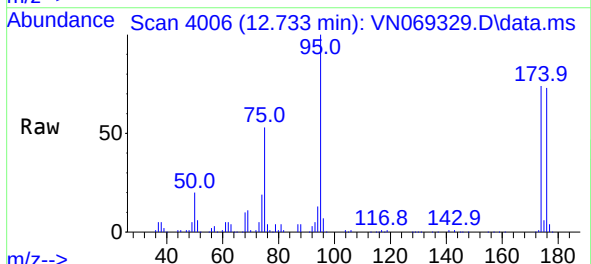


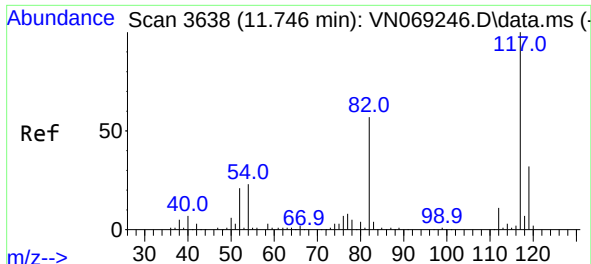

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 30
Delta R.T. -0.000 min
Lab File: VN069329.D
Acq: 1 Nov 2021 19:06

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-REF-5

Tgt Ion:117 Resp: 507019
Ion Ratio Lower Upper
117 100
82 57.5 46.4 69.6
119 31.6 26.0 39.0

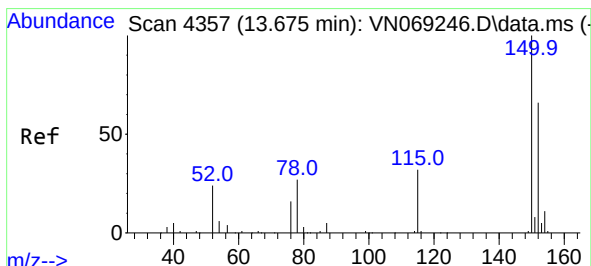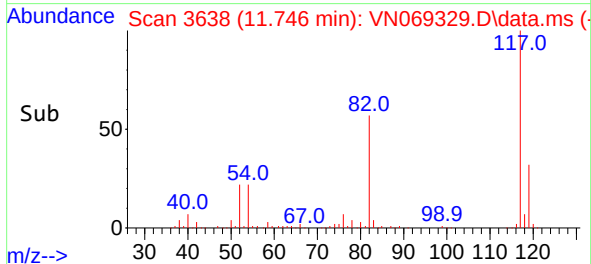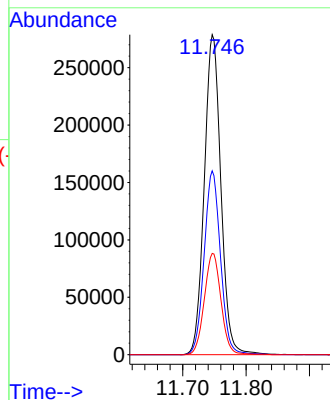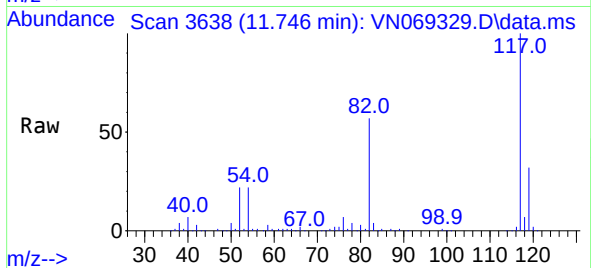

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. 0.002 min
Lab File: VN069329.D
Acq: 1 Nov 2021 19:06

Tgt Ion:152 Resp: 199334
Ion Ratio Lower Upper
152 100
115 62.6 31.4 94.3
150 157.1 0.0 351.0

