

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
 Data File : VN069325.D
 Acq On : 1 Nov 2021 17:24
 Operator : JC/MD
 Sample : M4336-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-7

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M

Title : SW846 8260

Signal : TIC: VN069325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.231	77	90	107	rBV	92728	144043	7.67%	1.422%
2	4.599	955	973	1005	rBV	15056	46618	2.48%	0.460%
3	7.329	1970	1991	2015	rBV	15729	46377	2.47%	0.458%
4	8.024	2229	2250	2261	rBV2	227323	539421	28.71%	5.324%
5	8.088	2262	2274	2299	rVB2	427111	973132	51.79%	9.604%
6	8.440	2383	2405	2433	rBV	253969	580788	30.91%	5.732%
7	8.700	2446	2502	2504	rBV2	33154	184868	9.84%	1.825%
8	8.968	2585	2602	2631	rVB	641636	1334935	71.04%	13.175%
9	10.443	3134	3152	3179	rBV	1007610	1879147	100.00%	18.546%
10	11.095	3382	3395	3406	rBV	16592	28264	1.50%	0.279%
11	11.746	3620	3638	3675	rBV	942877	1718894	91.47%	16.964%
12	12.733	3989	4006	4030	rBV	729589	1268332	67.50%	12.518%
13	13.675	4341	4357	4378	rBV	796471	1387548	73.84%	13.694%


Sum of corrected areas: 10132367

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
Data File : VN069325.D
Acq On : 1 Nov 2021 17:24
Operator : JC/MD
Sample : M4336-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

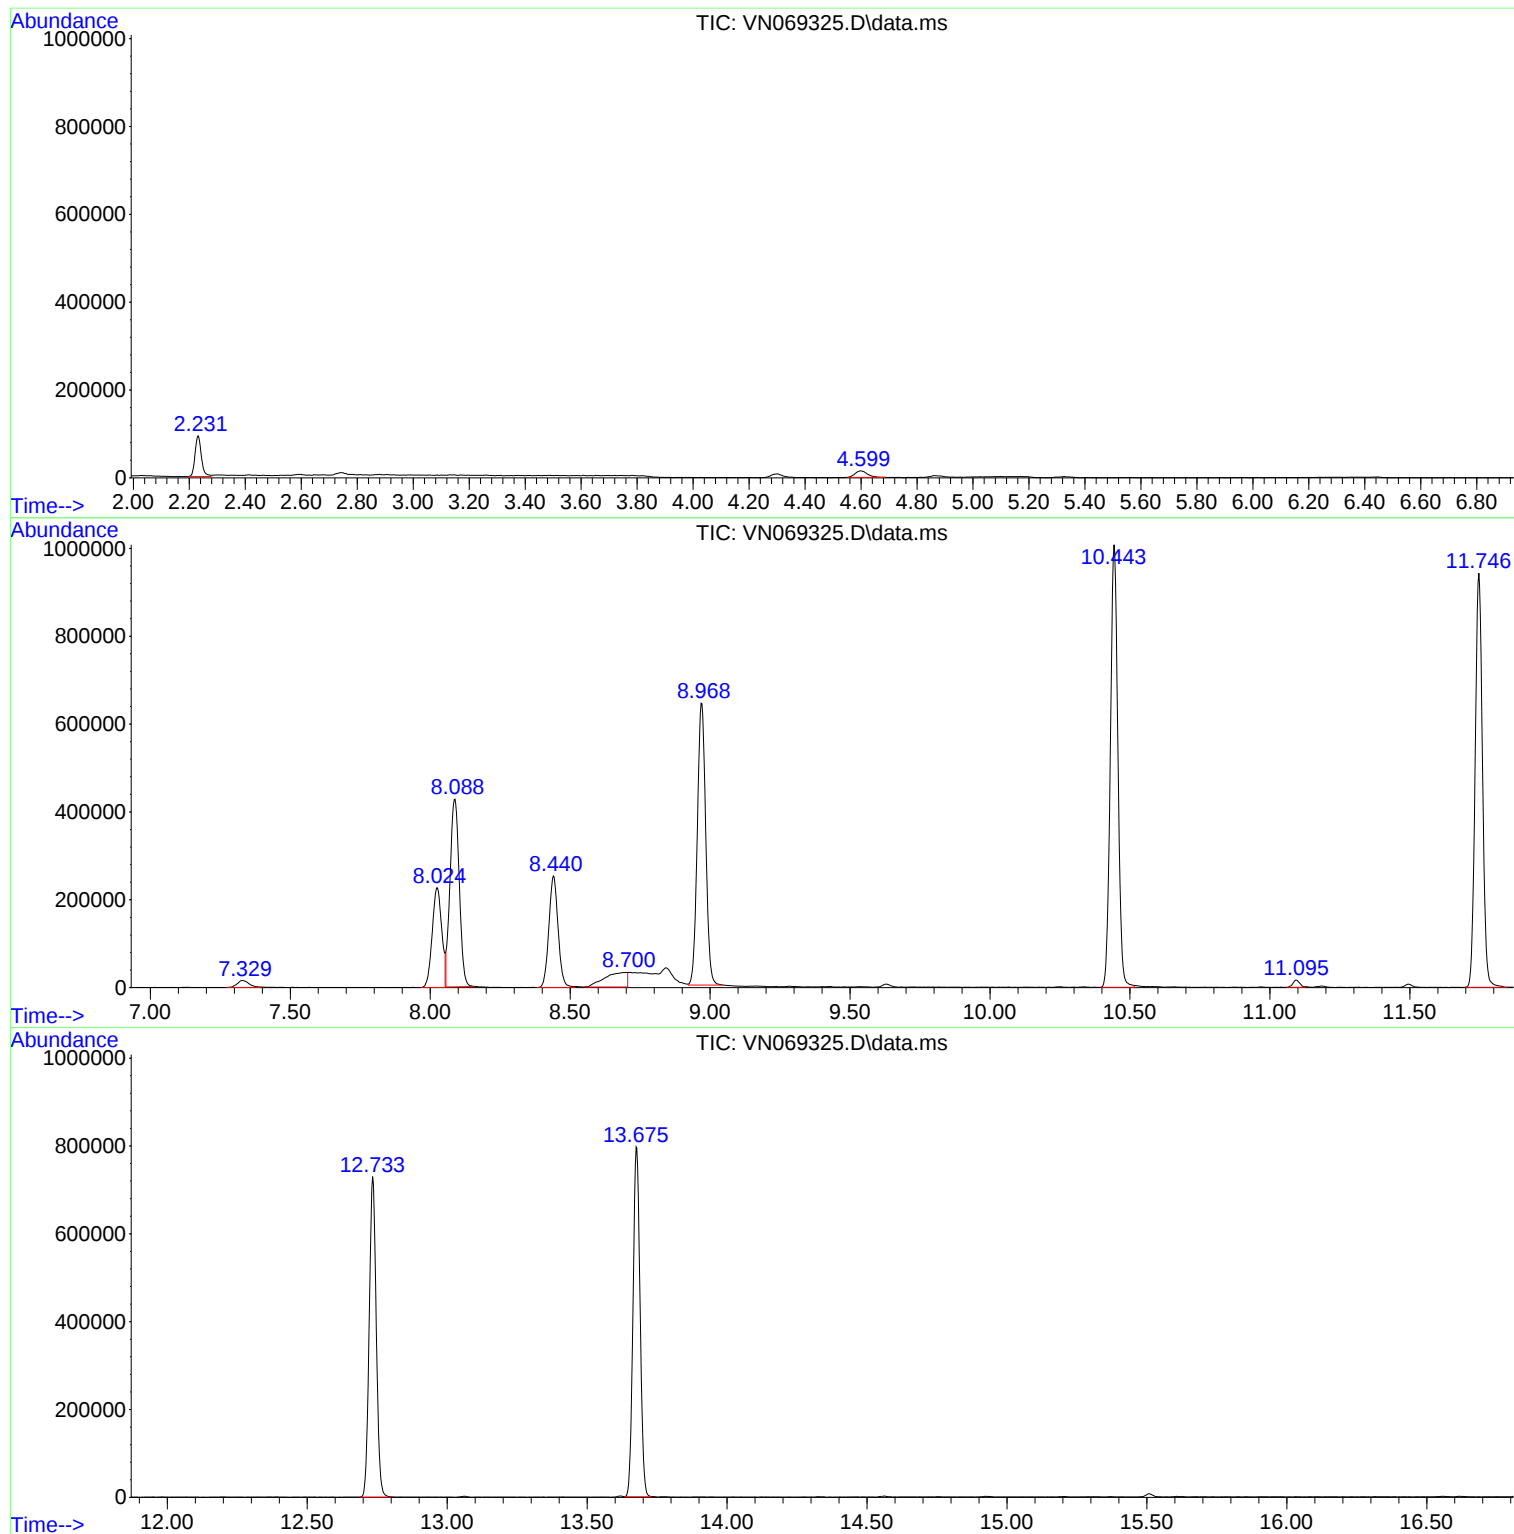

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
Data File : VN069325.D
Acq On : 1 Nov 2021 17:24
Operator : JC/MD
Sample : M4336-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Acetic acid Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.700	6.92 ug/l	184868	1,4-Difluorobenzene	8.971

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Acetic acid	60	C2H4O2	000064-19-7	90
2			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	64
3			Ammonium acetate	77	C2H7NO2	000631-61-8	43
4			Thiirane	60	C2H4S	000420-12-2	9
5			Hydrazine, 1,1-dimethyl-	60	C2H8N2	000057-14-7	7

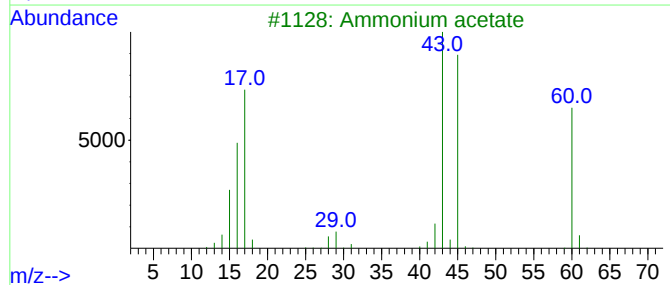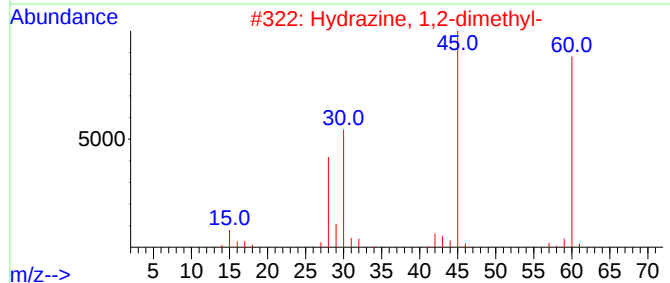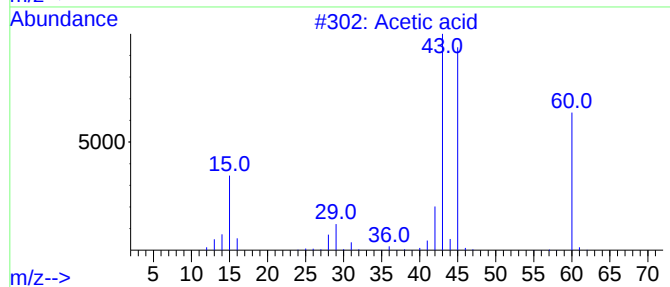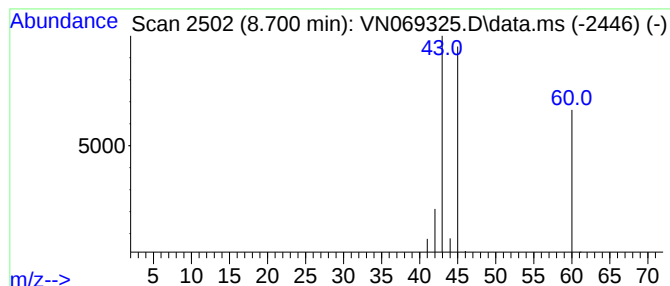

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
Data File : VN069325.D
Acq On : 1 Nov 2021 17:24
Operator : JC/MD
Sample : M4336-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Acetic acid	8.700	6.9	ug/l	184868	2	8.971	1334940	50.0