

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
Data File : VN069330.D
Acq On : 1 Nov 2021 19:32
Operator : JC/MD
Sample : M4423-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M

Title : SW846 8260

Signal : TIC: VN069330.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.233	80	91	109	rBV	17947	29741	1.75%	0.331%
2	4.599	953	973	992	rBV2	11605	37481	2.20%	0.417%
3	7.335	1971	1993	2017	rBV2	14512	44772	2.63%	0.499%
4	8.024	2228	2250	2261	rBV2	204692	487345	28.60%	5.426%
5	8.088	2262	2274	2301	rVB	384932	865075	50.76%	9.632%
6	8.440	2385	2405	2431	rBV	225494	524488	30.78%	5.840%
7	8.971	2585	2603	2630	rVB	573228	1200978	70.47%	13.372%
8	10.443	3134	3152	3177	rBV	910977	1704262	100.00%	18.976%
9	11.746	3621	3638	3673	rBV	874059	1590060	93.30%	17.705%
10	12.733	3989	4006	4034	rBV	671771	1178357	69.14%	13.120%
11	13.677	4340	4358	4388	rBV	754861	1318542	77.37%	14.681%




Sum of corrected areas: 8981101

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
Data File : VN069330.D
Acq On : 1 Nov 2021 19:32
Operator : JC/MD
Sample : M4423-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

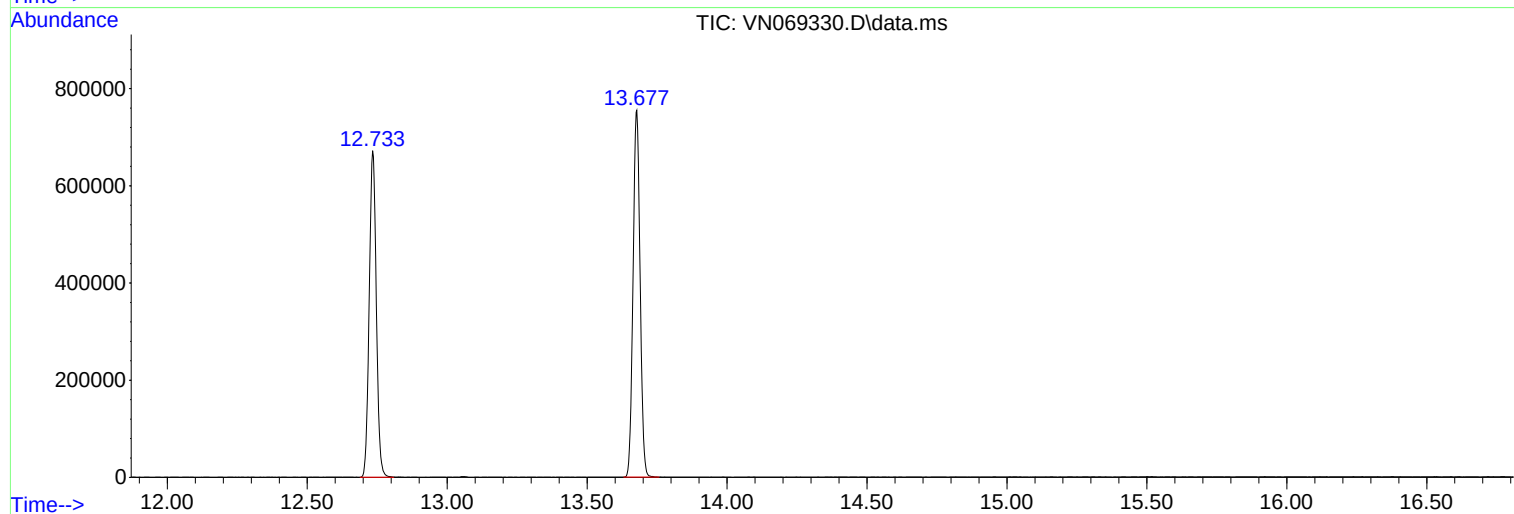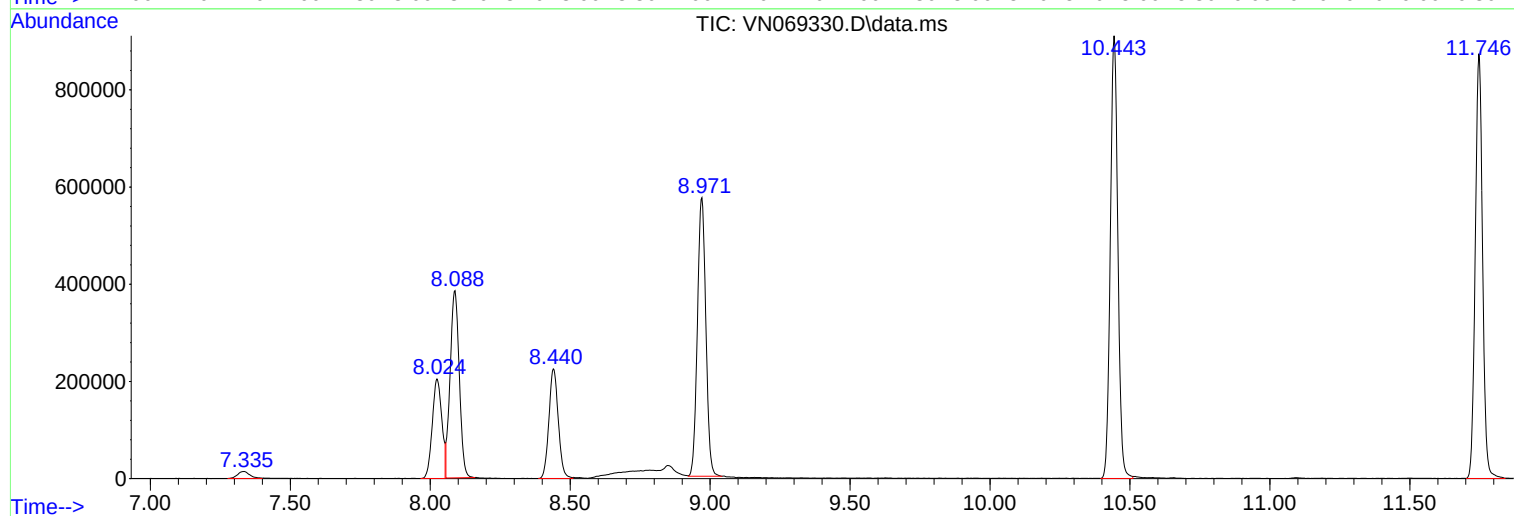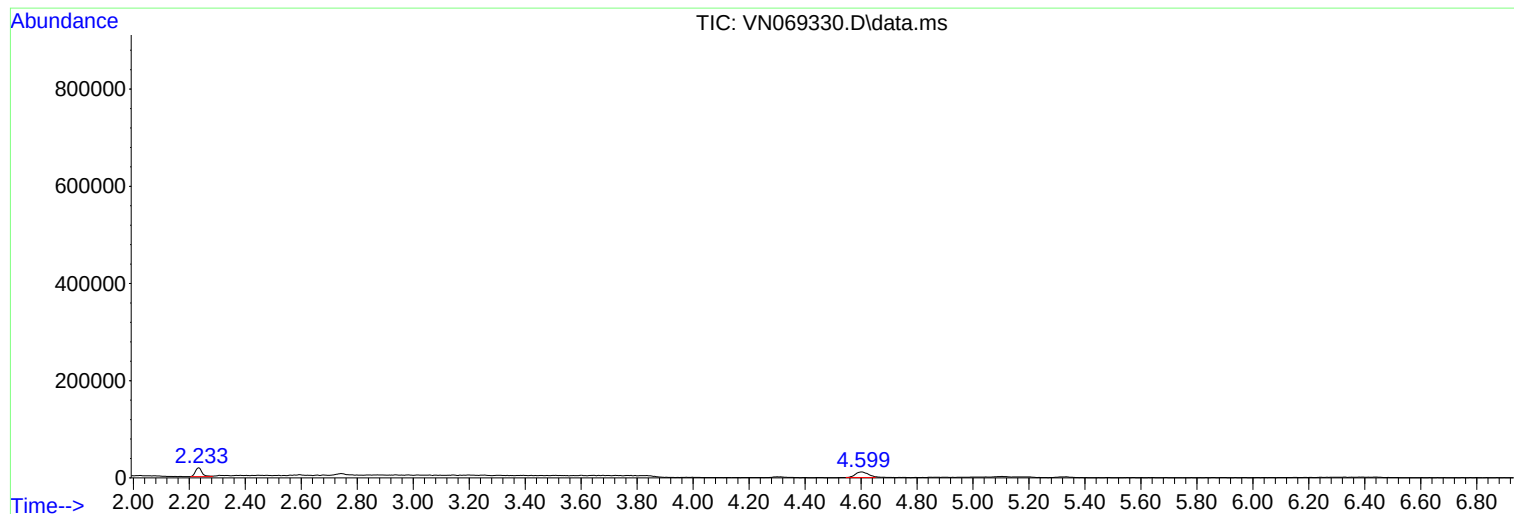

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
Data File : VN069330.D
Acq On : 1 Nov 2021 19:32
Operator : JC/MD
Sample : M4423-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
Data File : VN069330.D
Acq On : 1 Nov 2021 19:32
Operator : JC/MD
Sample : M4423-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc