
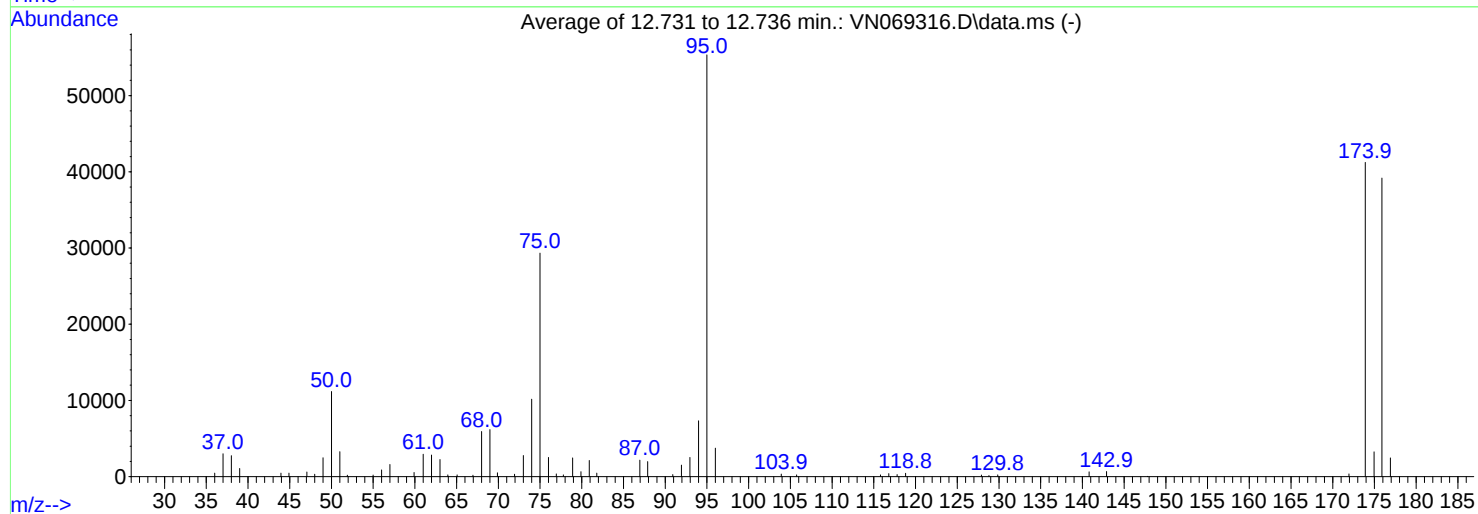


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110121\
 Data File : VN069316.D
 Acq On : 1 Nov 2021 9:53
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
 Title : SW846 8260
 Last Update : Thu Oct 28 16:09:15 2021

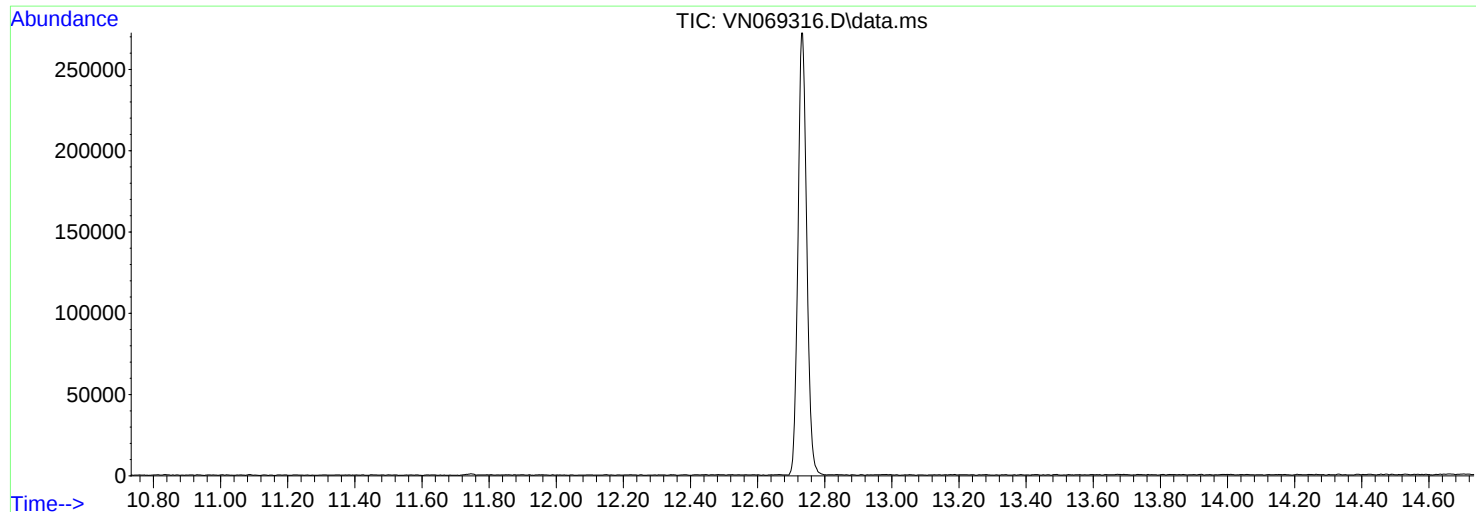

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3988

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	11177	PASS
75	95	30	60	53.0	29336	PASS
95	95	100	100	100.0	55347	PASS
96	95	5	9	6.7	3735	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.5	41235	PASS
175	174	5	9	7.9	3246	PASS
176	174	95	101	95.0	39184	PASS
177	176	5	9	6.3	2450	PASS