

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110122\
 Data File : VN075103.D
 Acq On : 01 Nov 2022 17:34
 Operator : JC\MD
 Sample : N5417-07
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 AUD-1904

Quant Time: Nov 02 07:11:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 09:48:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	103781	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	186754	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	167276	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	71958	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	76775	54.905	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 109.800%	
35) Dibromofluoromethane	8.171	113	57330	52.292	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 104.580%	
50) Toluene-d8	10.565	98	226243	53.190	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 106.380%	
62) 4-Bromofluorobenzene	12.853	95	74199	49.659	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 99.320%	
Target Compounds						
					Qvalue	
5) Bromomethane	2.965	94	139	Below Cal	#	5
11) Tert butyl alcohol	5.536	59	466	1.429	ug/l #	72
16) Acetone	4.453	43	4529	7.649	ug/l #	84
19) Methyl tert-butyl Ether	5.812	73	818	0.200	ug/l #	56
25) 2-Butanone	7.500	43	698	0.749	ug/l #	43
31) Cyclohexane	8.230	56	2455	1.180	ug/l #	22
36) 1,1-Dichloropropene	8.230	75	9201	5.421	ug/l #	49
37) Ethyl Acetate	7.500	43	698	0.375	ug/l #	66
38) Carbon Tetrachloride	8.230	117	11548	6.185	ug/l #	15
40) Benzene	8.612	78	1797	0.346	ug/l	93
52) Toluene	10.629	92	7005	2.016	ug/l	93
59) 2-Hexanone	11.194	43	486	0.344	ug/l #	57
67) Ethyl Benzene	11.965	91	4780	0.744	ug/l	97
68) m/p-Xylenes	12.071	106	7277	2.823	ug/l	96
69) o-Xylene	12.400	106	6861	2.692	ug/l	99
71) Bromoform	12.853	173	984	0.992	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	12.865	83	71	Below Cal	#	26
76) 1,2,3-Trichloropropane	12.853	75	41025	26.851	ug/l #	1
78) n-propylbenzene	13.035	91	2240	0.345	ug/l	99
79) 2-Chlorotoluene	13.094	91	1973	0.498	ug/l #	41
80) 1,3,5-Trimethylbenzene	13.171	105	5417	1.116	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.853	75	41025	68.927	ug/l #	10
82) 4-Chlorotoluene	13.094	91	1973	0.498	ug/l #	41
83) tert-Butylbenzene	13.482	119	2624	0.609	ug/l #	64
84) 1,2,4-Trimethylbenzene	13.482	105	22872	4.659	ug/l	100
86) p-Isopropyltoluene	13.670	119	1301	0.261	ug/l	95
89) n-Butylbenzene	14.059	91	1079	0.269	ug/l	87
90) Hexachloroethane	14.335	117	779	0.853	ug/l #	19
95) Naphthalene	15.641	128	32009	7.812	ug/l	99
96) 1,2,3-Trichlorobenzene	15.835	180	266	0.251	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110122\
Data File : VN075103.D
Acq On : 01 Nov 2022 17:34
Operator : JC\MD
Sample : N5417-07
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1904

Quant Time: Nov 02 07:11:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 09:48:49 2022
Response via : Initial Calibration




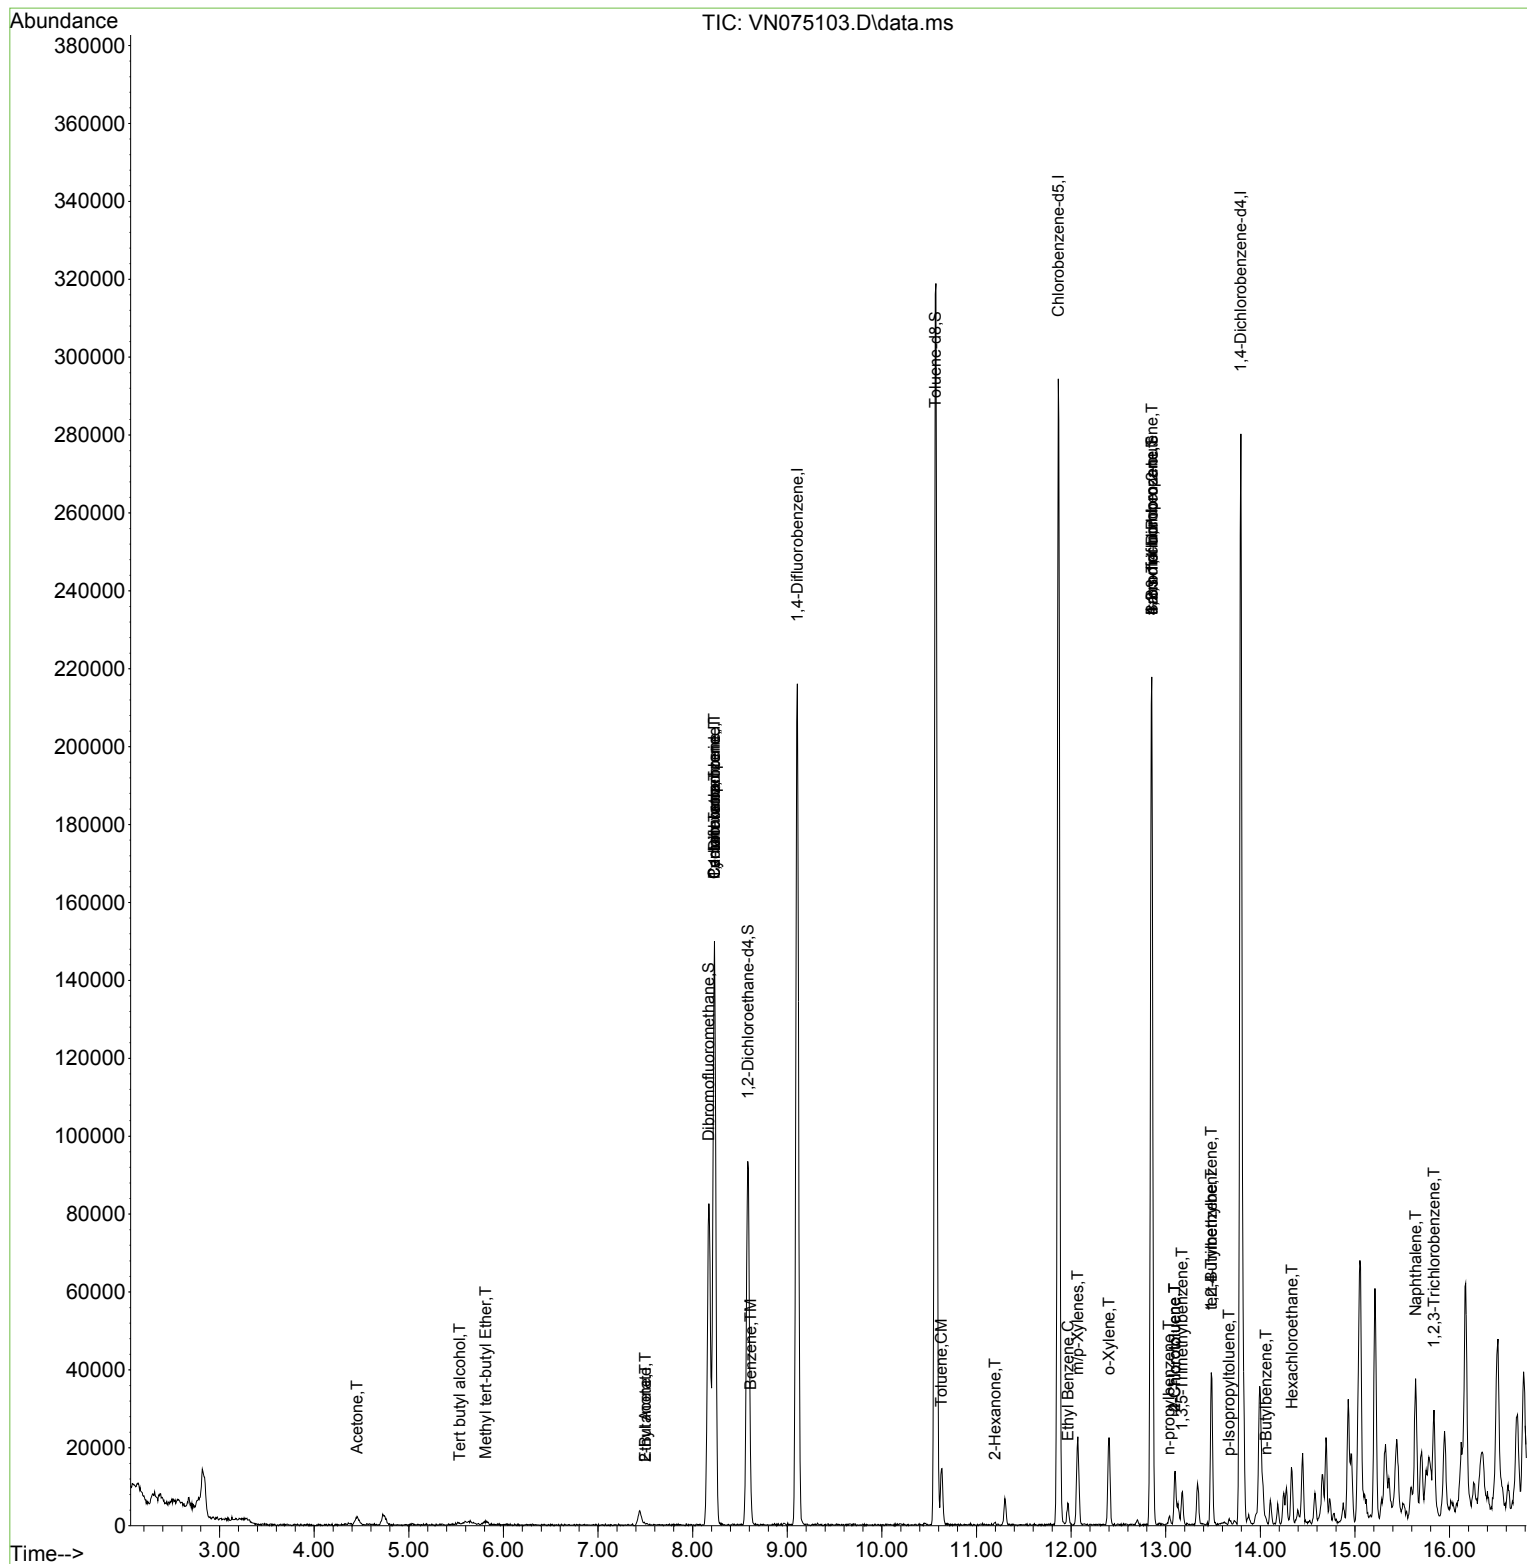




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion:168 Resp: 103781
Ion Ratio Lower Upper
168 100
99 63.5 51.6 77.4

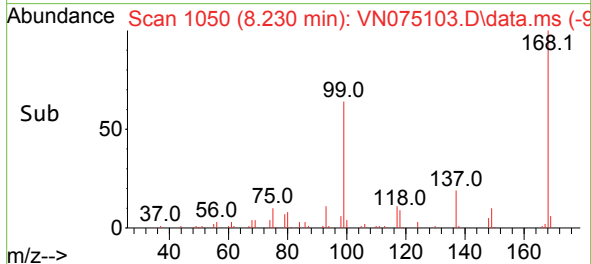

#5
Bromomethane
Concen: Below Cal
RT: 2.965 min Scan# 155
Delta R.T. 0.047 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion: 94 Resp: 139
Ion Ratio Lower Upper
94 100
96 0.0 71.8 107.6#


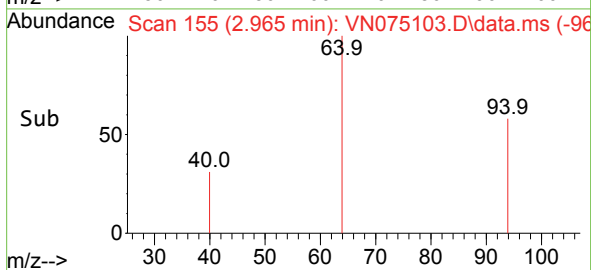






#11
Tert butyl alcohol
Concen: 1.429 ug/l
RT: 5.536 min Scan# 51
Delta R.T. -0.006 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion: 59 Resp: 466
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#

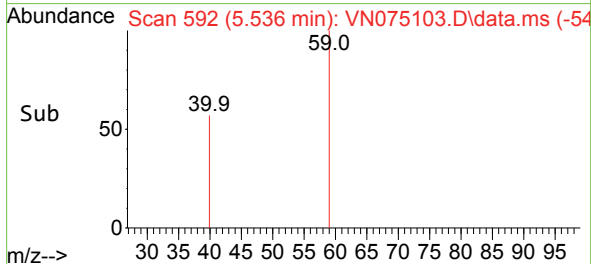

#16
Acetone
Concen: 7.649 ug/l
RT: 4.453 min Scan# 408
Delta R.T. 0.011 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion: 43 Resp: 4529
Ion Ratio Lower Upper
43 100
58 22.9 25.5 38.3#


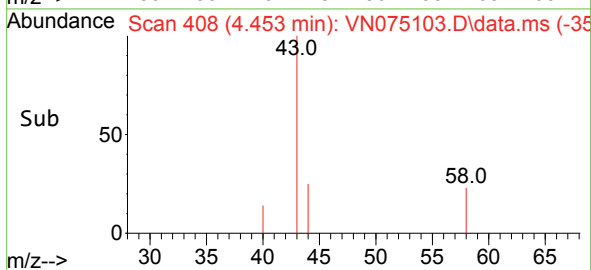

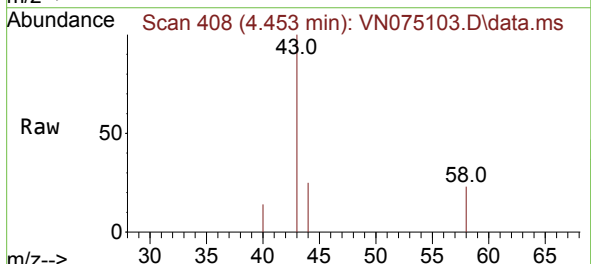


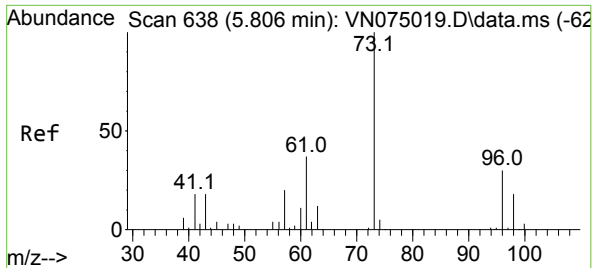

#19
Methyl tert-butyl Ether
Concen: 0.200 ug/l
RT: 5.812 min Scan# 61
Delta R.T. 0.006 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion: 73 Resp: 818
Ion Ratio Lower Upper
73 100
57 0.0 16.3 24.5#

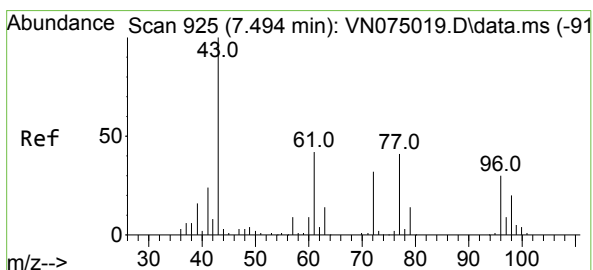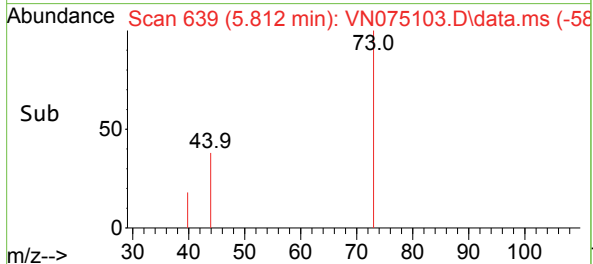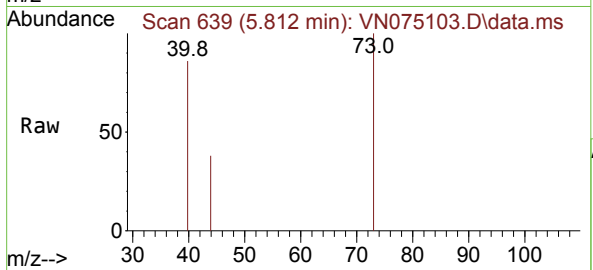

#25
2-Butanone
Concen: 0.749 ug/l
RT: 7.500 min Scan# 926
Delta R.T. 0.006 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion: 43 Resp: 698
Ion Ratio Lower Upper
43 100
72 0.0 25.5 38.3#


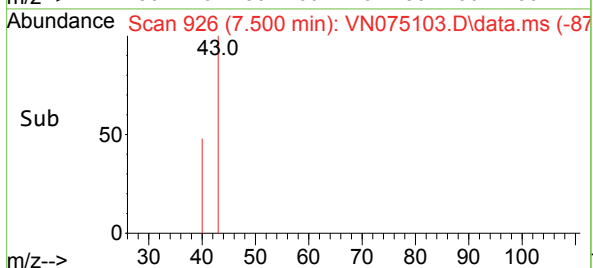

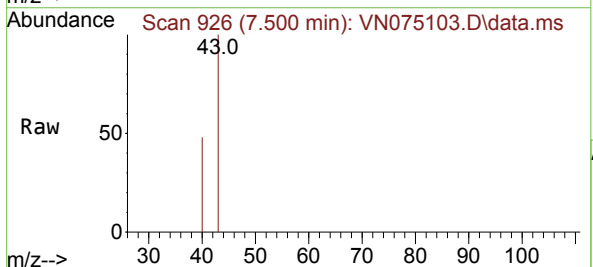




#31
Cyclohexane
Concen: 1.180 ug/l
RT: 8.230 min Scan# 1105
Delta R.T. -0.029 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion: 56 Resp: 2455
Ion Ratio Lower Upper
56 100
69 139.9 25.2 37.8#
84 136.7 77.8 116.8#

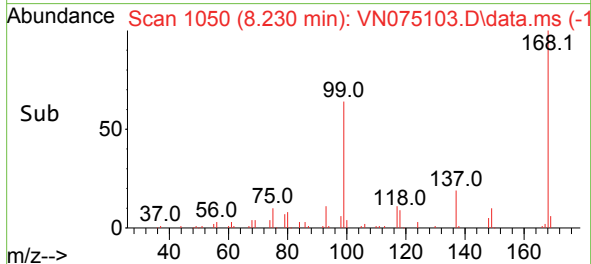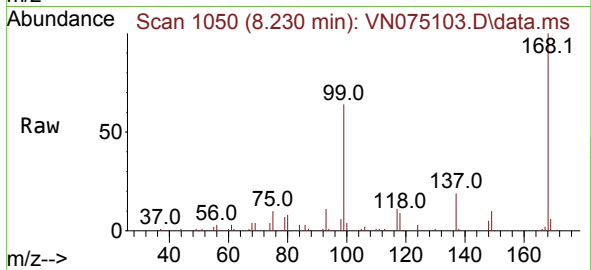

#33
1,2-Dichloroethane-d4
Concen: 54.905 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. -0.005 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion: 65 Resp: 76775
Ion Ratio Lower Upper
65 100
67 51.5 0.0 102.0


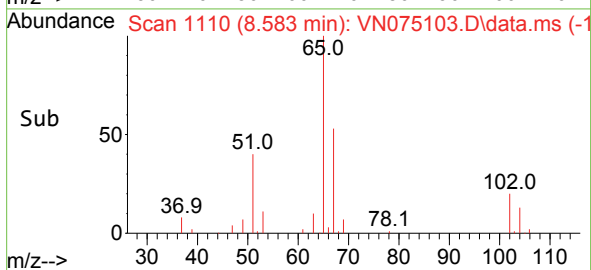






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 1199
Delta R.T. 0.000 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion:114 Resp: 186754
Ion Ratio Lower Upper
114 100
63 20.7 0.0 39.6
88 15.0 0.0 29.0

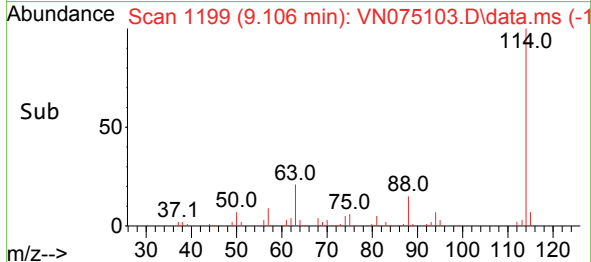

#35
Dibromofluoromethane
Concen: 52.292 ug/l
RT: 8.171 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion:113 Resp: 57330
Ion Ratio Lower Upper
113 100
111 106.3 80.5 120.7
192 17.5 13.2 19.8

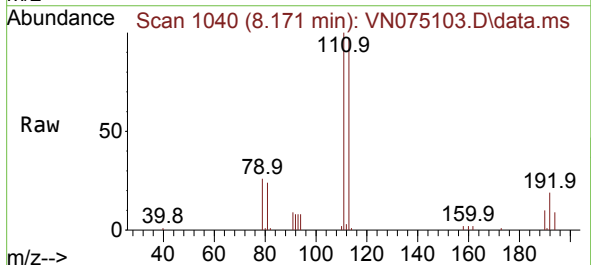



#36

1,1-Dichloropropene

Concen: 5.421 ug/l

RT: 8.230 min Scan# 1

Delta R.T. -0.147 min

Lab File: VN075103.D

Acq: 01 Nov 2022 17:34

Instrument :

MSVOA_N

ClientSampleId :

AUD-1904





Tgt Ion: 75 Resp: 9201

Ion Ratio Lower Upper

75 100

110 8.0 17.8 53.3#

77 0.0 24.6 37.0#



#37

Ethyl Acetate

Concen: 0.375 ug/l

RT: 7.500 min Scan# 926

Delta R.T. -0.071 min

Lab File: VN075103.D

Acq: 01 Nov 2022 17:34




Tgt Ion: 43 Resp: 698


Ion Ratio Lower Upper

43 100

61 0.0 12.2 18.4#

70 0.0 9.4 14.2#

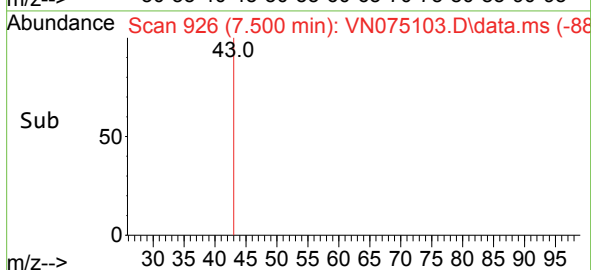

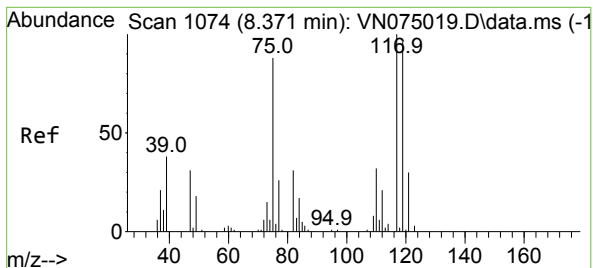

#38

Carbon Tetrachloride

Concen: 6.185 ug/l

RT: 8.230 min Scan# 1105

Delta R.T. -0.141 min

Lab File: VN075103.D

Acq: 01 Nov 2022 17:34

Instrument :

MSVOA_N

ClientSampleId :

AUD-1904





Tgt Ion:117 Resp: 11548

Ion Ratio Lower Upper

117 100

119 3.5 76.7 115.1#

121 0.0 23.9 35.9#

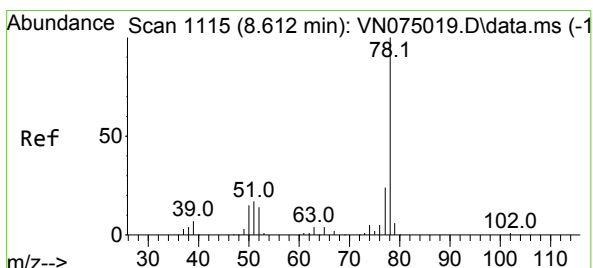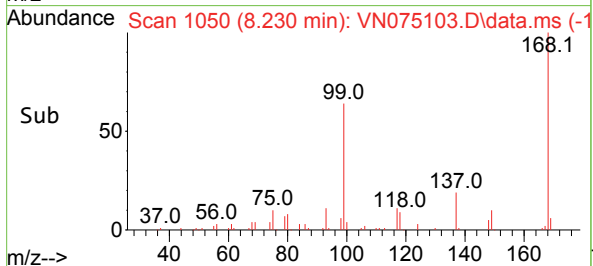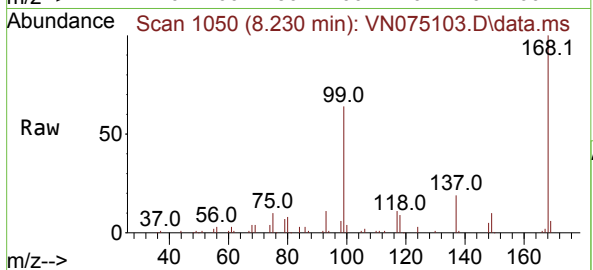

#40

Benzene

Concen: 0.346 ug/l

RT: 8.612 min Scan# 1115

Delta R.T. -0.000 min

Lab File: VN075103.D




Acq: 01 Nov 2022 17:34


Tgt Ion: 78 Resp: 1797

Ion Ratio Lower Upper

78 100

77 27.9 19.4 29.0


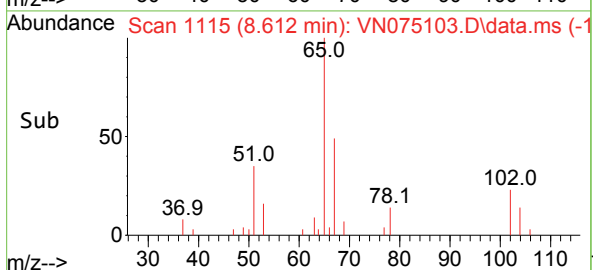

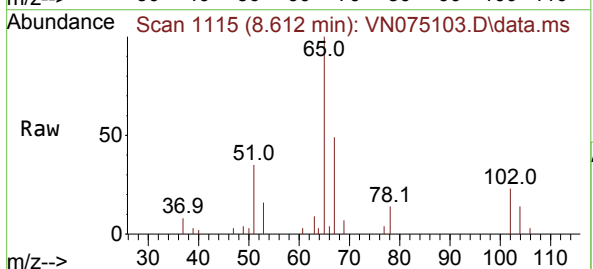


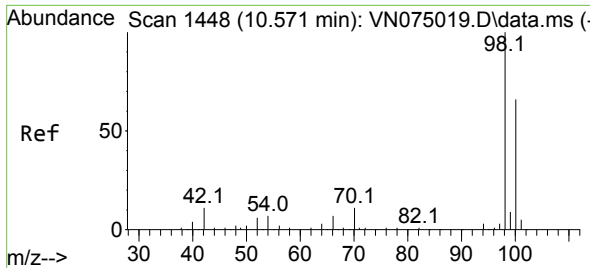

#50
Toluene-d8
Concen: 53.190 ug/l
RT: 10.565 min Scan# 1447
Delta R.T. -0.006 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion: 98 Resp: 226243
Ion Ratio Lower Upper
98 100
100 65.8 53.0 79.6

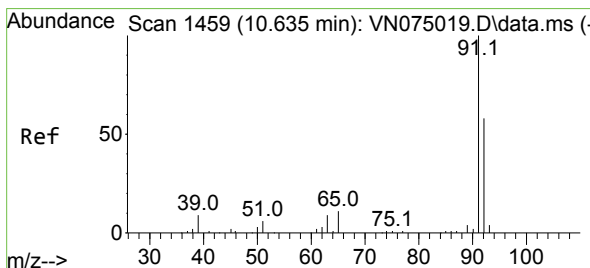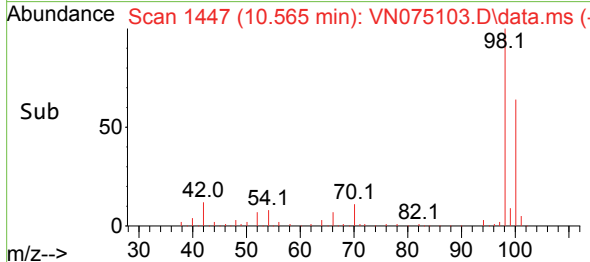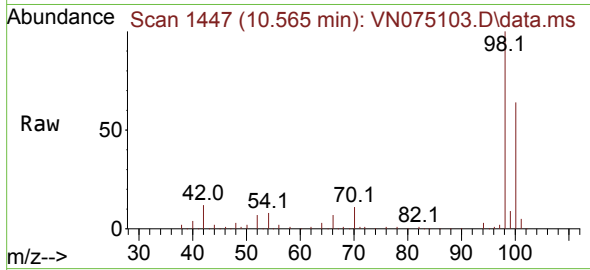

#52
Toluene
Concen: 2.016 ug/l
RT: 10.629 min Scan# 1458
Delta R.T. -0.006 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion: 92 Resp: 7005
Ion Ratio Lower Upper
92 100
91 159.1 135.4 203.2


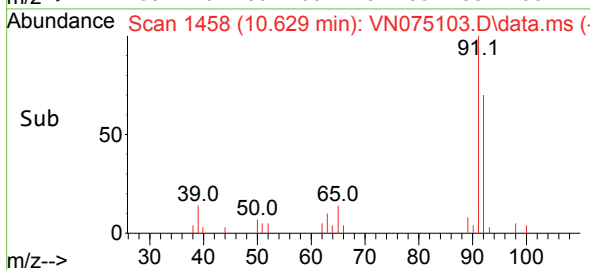

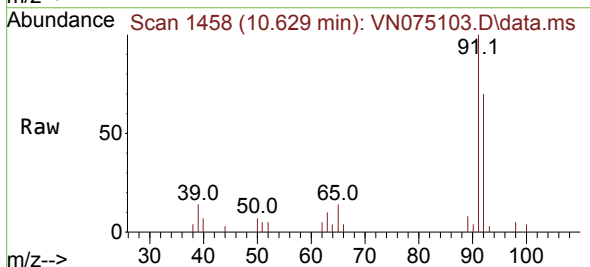




#59
2-Hexanone
Concen: 0.344 ug/l
RT: 11.194 min Scan# 11554
Delta R.T. -0.006 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion: 43 Resp: 486
Ion Ratio Lower Upper
43 100
58 27.2 29.6 88.8#

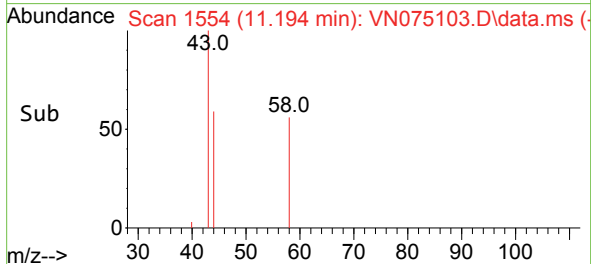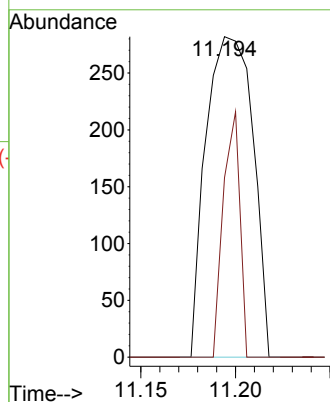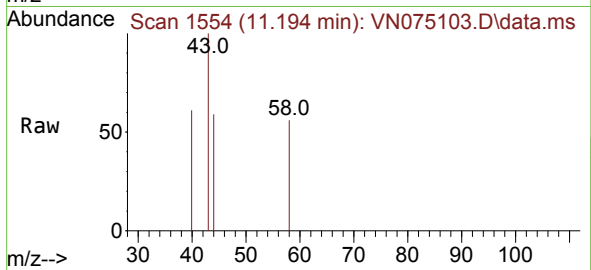

#62
4-Bromofluorobenzene
Concen: 49.659 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion: 95 Resp: 74199
Ion Ratio Lower Upper
95 100
174 74.4 0.0 147.4
176 72.7 0.0 142.2


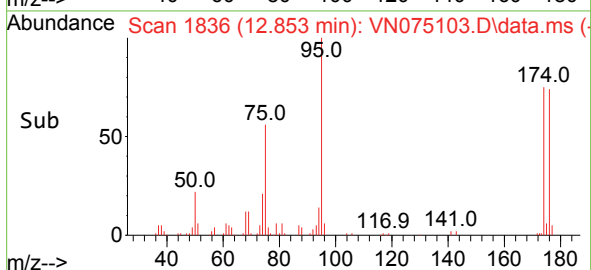

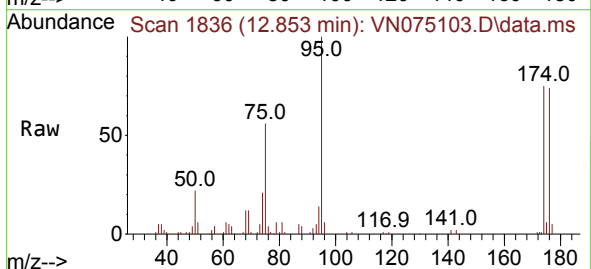


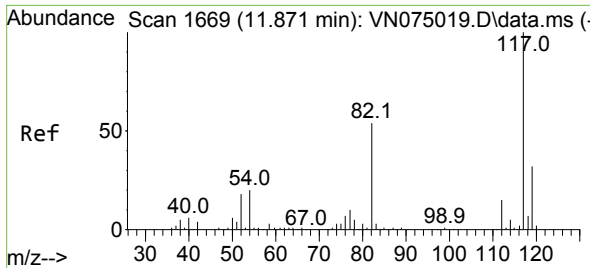

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1668
Delta R.T. -0.006 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion:117 Resp: 167276
Ion Ratio Lower Upper
117 100
82 57.2 43.1 64.7
119 31.7 25.5 38.3

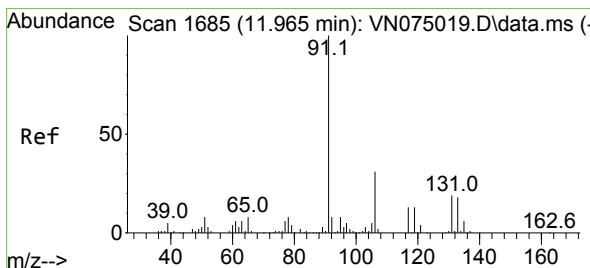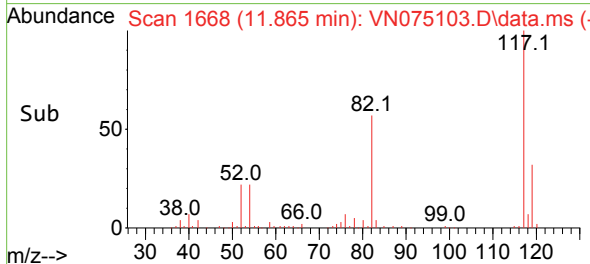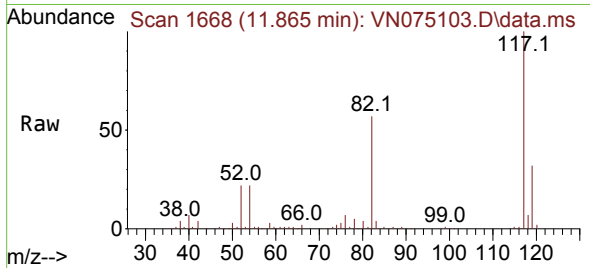

#67
Ethyl Benzene
Concen: 0.744 ug/l
RT: 11.965 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion: 91 Resp: 4780
Ion Ratio Lower Upper
91 100
106 29.5 24.9 37.3


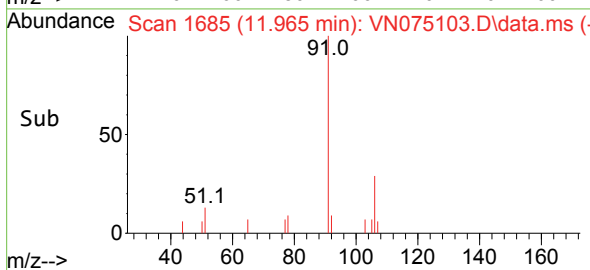

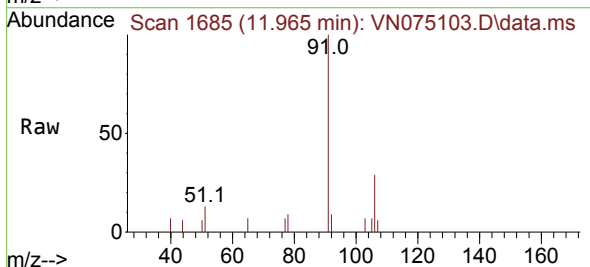




#68
m/p-Xylenes
Concen: 2.823 ug/l
RT: 12.071 min Scan# 1703
Delta R.T. -0.005 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion:106 Resp: 7277
Ion Ratio Lower Upper
106 100
91 201.2 156.0 234.0

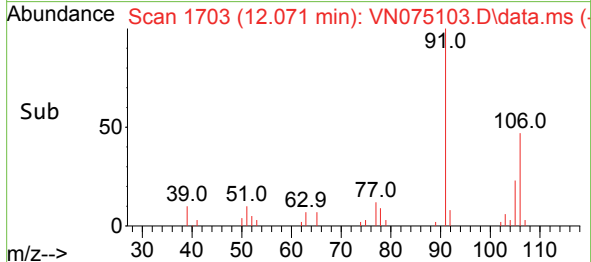

#69
o-Xylene
Concen: 2.692 ug/l
RT: 12.400 min Scan# 1759
Delta R.T. -0.000 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion:106 Resp: 6861
Ion Ratio Lower Upper
106 100
91 212.4 105.2 315.5




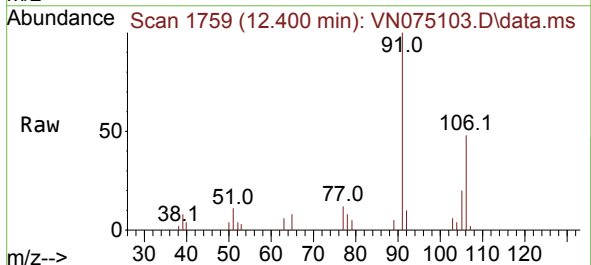




#71
Bromoform
Concen: 0.992 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.271 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion:173 Resp: 984
Ion Ratio Lower Upper
173 100
175 375.1 24.6 74.0#
254 0.0 0.0 0.0

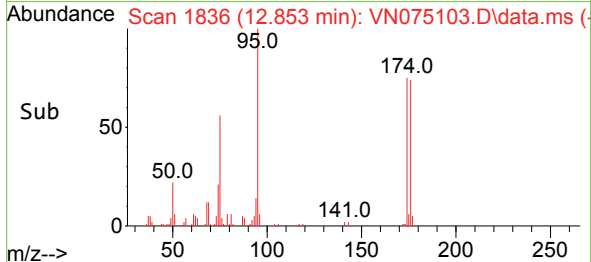

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion:152 Resp: 71958
Ion Ratio Lower Upper
152 100
115 61.4 30.2 90.6
150 159.4 0.0 348.4


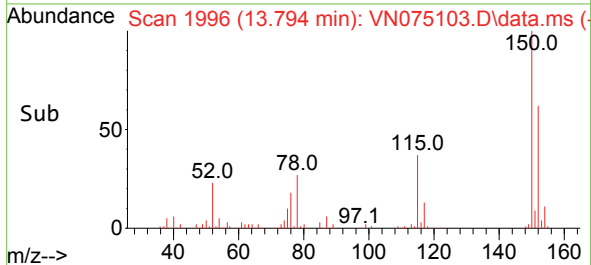






#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.865 min Scan# 1838
Delta R.T. -0.076 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion: 83 Resp: 71
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.3#
85 0.0 31.6 94.7#

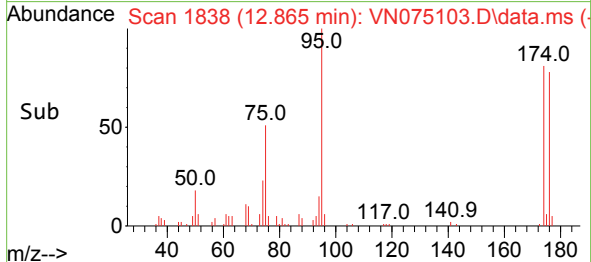

#76
1,2,3-Trichloropropane
Concen: 26.851 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion: 75 Resp: 41025
Ion Ratio Lower Upper
75 100
77 1.1 75.6 226.8#









#78
n-propylbenzene
Concen: 0.345 ug/l
RT: 13.035 min Scan# 1867
Delta R.T. 0.000 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion: 91 Resp: 2240
Ion Ratio Lower Upper
91 100
120 23.1 11.9 35.5

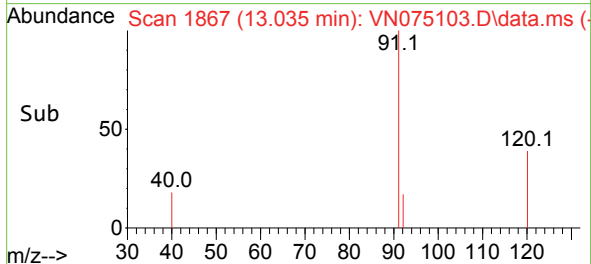

#79
2-Chlorotoluene
Concen: 0.498 ug/l
RT: 13.094 min Scan# 1877
Delta R.T. -0.035 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion: 91 Resp: 1973
Ion Ratio Lower Upper
91 100
126 0.0 16.9 50.7#


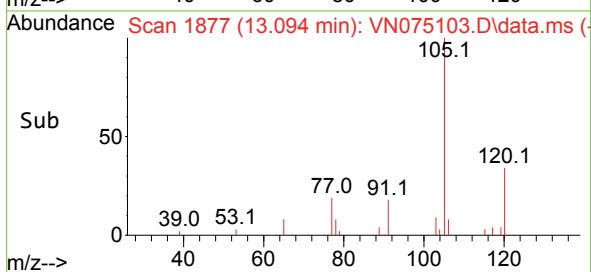

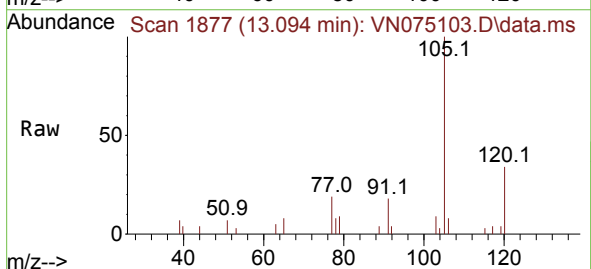




#80
1,3,5-Trimethylbenzene
Concen: 1.116 ug/l
RT: 13.171 min Scan# 1890
Delta R.T. -0.005 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion:105 Resp: 5417
Ion Ratio Lower Upper
105 100
120 48.2 24.7 74.1

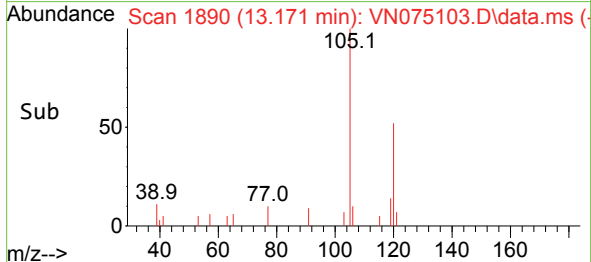

#81
trans-1,4-Dichloro-2-butene
Concen: 68.927 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.112 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion: 75 Resp: 41025
Ion Ratio Lower Upper
75 100
53 0.0 78.5 117.7#
89 0.0 37.7 56.5#









#82
4-Chlorotoluene
Concen: 0.498 ug/l
RT: 13.094 min Scan# 11
Delta R.T. -0.035 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion: 91 Resp: 1973
Ion Ratio Lower Upper
91 100
126 0.0 16.9 50.7#

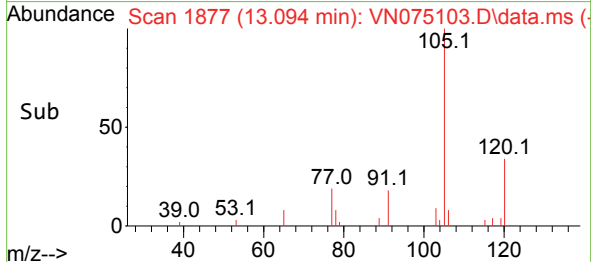

#83
tert-Butylbenzene
Concen: 0.609 ug/l
RT: 13.482 min Scan# 1943
Delta R.T. 0.041 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion: 119 Resp: 2624
Ion Ratio Lower Upper
119 100
91 90.6 32.8 98.4
134 0.0 12.3 36.9#

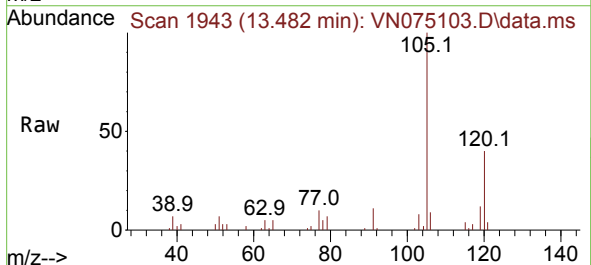



#84

1,2,4-Trimethylbenzene

Concen: 4.659 ug/l

RT: 13.482 min Scan# 1943

Delta R.T. 0.000 min

Lab File: VN075103.D

Acq: 01 Nov 2022 17:34

Instrument :

MSVOA_N

ClientSampleId :





AUD-1904

Tgt Ion:105 Resp: 22872

Ion Ratio Lower Upper

105 100

120 45.6 22.7 68.1



#86

p-Isopropyltoluene

Concen: 0.261 ug/l

RT: 13.670 min Scan# 1975

Delta R.T. -0.065 min

Lab File: VN075103.D

Acq: 01 Nov 2022 17:34




Tgt Ion:119 Resp: 1301


Ion Ratio Lower Upper

119 100

134 26.6 13.1 39.3

91 18.8 11.9 35.5


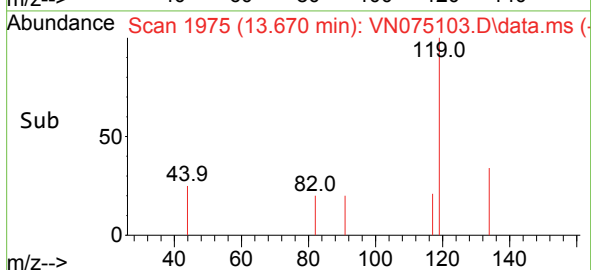






#89
n-Butylbenzene
Concen: 0.269 ug/l
RT: 14.059 min Scan# 2041
Delta R.T. -0.000 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34




Instrument :
MSVOA_N
ClientSampleId :
AUD-1904


Tgt Ion: 91 Resp: 1079
Ion Ratio Lower Upper
91 100
92 63.8 26.5 79.4
134 22.0 13.0 39.0

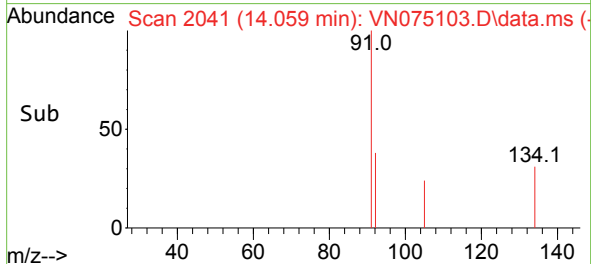

#90
Hexachloroethane
Concen: 0.853 ug/l
RT: 14.335 min Scan# 2088
Delta R.T. 0.000 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion: 117 Resp: 779
Ion Ratio Lower Upper
117 100
201 0.0 31.5 94.5#


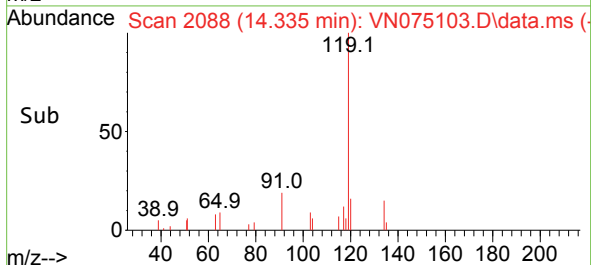

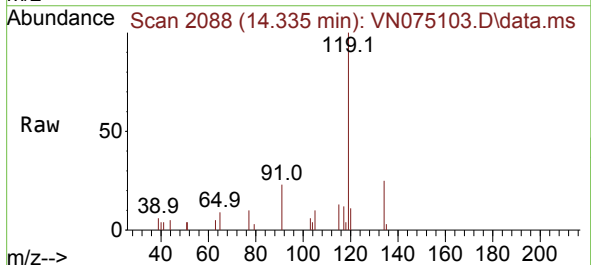


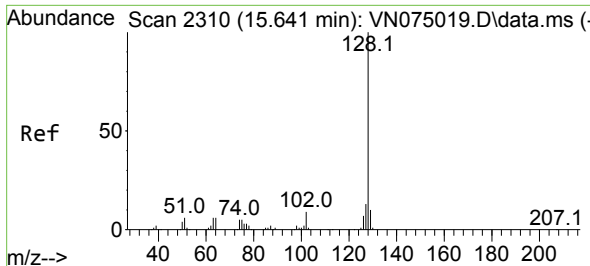

#95
Naphthalene
Concen: 7.812 ug/l
RT: 15.641 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Instrument :
MSVOA_N
ClientSampleId :
AUD-1904

Tgt Ion:128 Resp: 32009
Ion Ratio Lower Upper
128 100
127 12.3 10.4 15.6
129 10.9 8.6 12.8

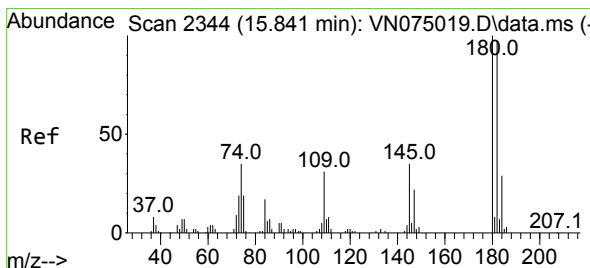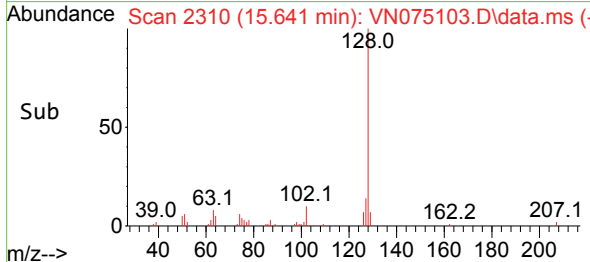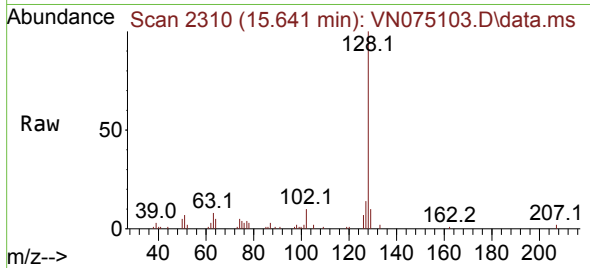

#96
1,2,3-Trichlorobenzene
Concen: 0.251 ug/l
RT: 15.835 min Scan# 2343
Delta R.T. -0.006 min
Lab File: VN075103.D
Acq: 01 Nov 2022 17:34

Tgt Ion:180 Resp: 266
Ion Ratio Lower Upper
180 100
182 72.2 47.3 141.8
145 615.4 17.6 52.9#

