
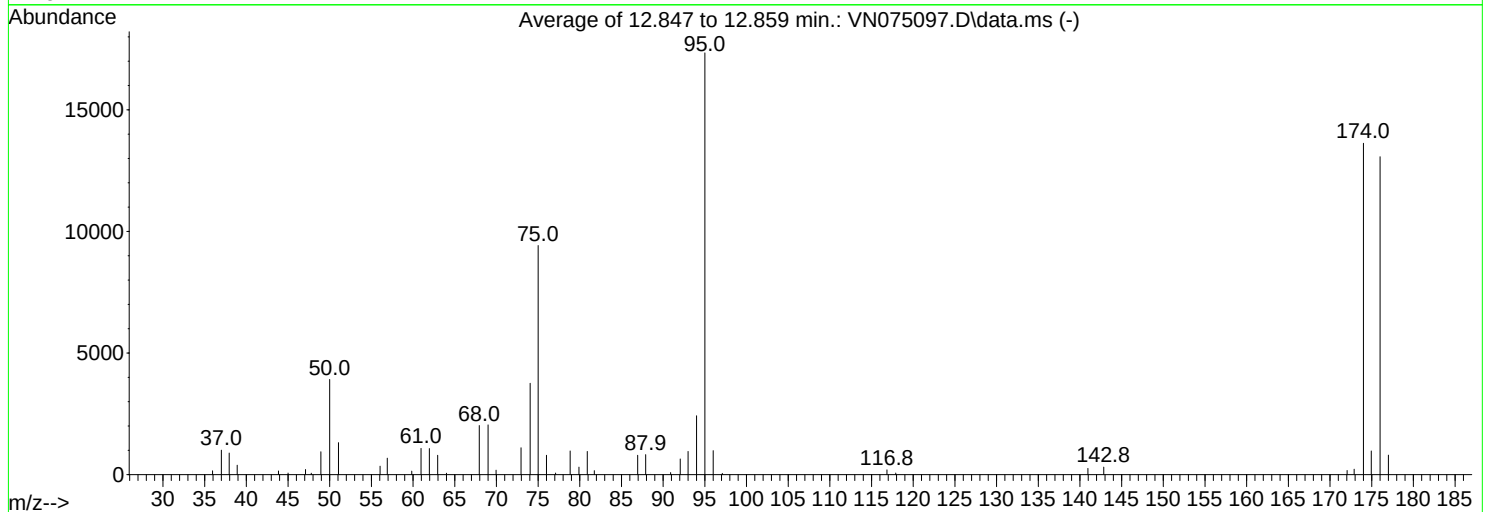


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110122\
Data File : VN075097.D
Acq On : 01 Nov 2022 08:52
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 09:48:49 2022

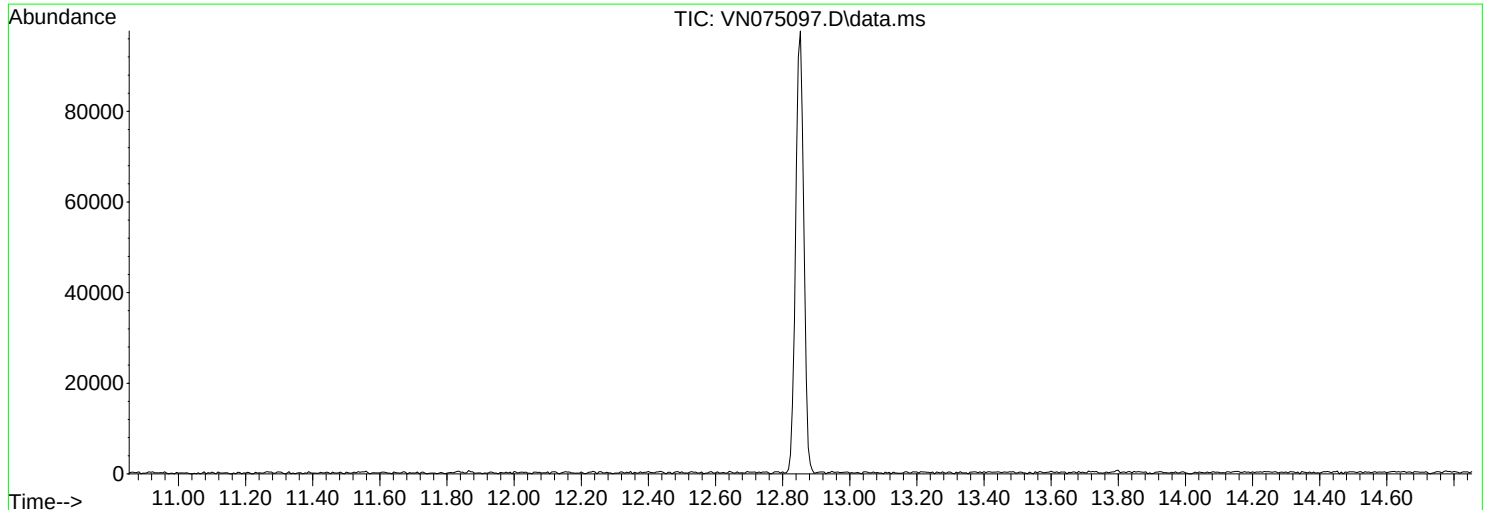

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.6	3913	PASS
75	95	30	60	54.3	9418	PASS
95	95	100	100	100.0	17343	PASS
96	95	5	9	5.7	989	PASS
173	174	0.00	2	1.7	227	PASS
174	95	50	100	78.6	13624	PASS
175	174	5	9	7.2	976	PASS
176	174	95	101	95.9	13069	PASS
177	176	5	9	6.1	801	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	161	56.05	349	74.05	3756	92.05	644
37.00	1008	56.90	675	75.00	9418	93.00	951
37.95	890	59.85	145	76.00	796	94.00	242
38.90	386	60.95	1079	77.10	67	95.00	1734
43.85	152	61.95	1072	78.85	972	96.00	989
45.00	63	62.95	795	79.90	307	97.10	54
47.10	209	64.00	59	80.90	954	116.85	200
47.80	57	67.95	2019	81.75	165	117.90	63
48.95	939	69.00	2045	86.95	798	140.95	254
50.00	3913	69.95	184	87.90	824	142.85	307
51.05	1317	72.95	1103	90.90	86	172.05	173

Average of 12.847 to 12.859 min.: VN075097.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.90	227						
174.00	13624						
174.95	976						
176.00	13069						
177.00	801						

Instrument :

MSVOA_N

ClientSampleId :

BFB