

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110123\
 Data File : VN079769.D
 Acq On : 01 Nov 2023 14:10
 Operator : JC\MD
 Sample : VN1101WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1101WBL01

Quant Time: Nov 02 05:53:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 02 05:49:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	223934	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	430062	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	431748	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	172986	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	172352	50.518	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	101.040%
35) Dibromofluoromethane	8.171	113	150789	49.540	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.080%
50) Toluene-d8	10.571	98	545513	48.683	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.360%
62) 4-Bromofluorobenzene	12.853	95	182937	49.226	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.460%


Target Compounds				Qvalue		
3) Chloromethane	2.365	50	2993	0.223	ug/l #	79
5) Bromomethane	2.965	94	1309	0.610	ug/l #	43
6) Chloroethane	3.165	64	607	0.218	ug/l	97
10) Methyl Iodide	4.589	142	1794	0.617	ug/l #	89
11) Tert butyl alcohol	5.518	59	264	0.606	ug/l #	72
13) Acrolein	4.183	56	55	2.713	ug/l #	1
15) Acrylonitrile	5.730	53	652	0.480	ug/l #	54
16) Acetone	4.453	43	1074	0.896	ug/l #	40
17) Carbon Disulfide	4.718	76	4123	0.593	ug/l #	75
20) Methylene Chloride	5.277	84	1861	0.615	ug/l #	75
25) 2-Butanone	7.500	43	555	0.316	ug/l #	37
30) Chloroform	7.971	83	2324	0.411	ug/l	87
31) Cyclohexane	8.224	56	5458	1.211	ug/l #	4
36) 1,1-Dichloropropene	8.230	75	19464	4.479	ug/l #	47
38) Carbon Tetrachloride	8.230	117	24827	5.668	ug/l #	15
47) Bromodichloromethane	9.882	83	1234	0.255	ug/l #	69
51) 4-Methyl-2-Pentanone	10.465	43	1125	0.286	ug/l #	70
59) 2-Hexanone	11.206	43	2919	0.970	ug/l #	55
71) Bromoform	12.841	173	1202	0.502	ug/l #	1
76) 1,2,3-Trichloropropane	12.853	75	101465	24.984	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	101465	67.976	ug/l #	15
87) 1,3-Dichlorobenzene	13.735	146	1635	0.273	ug/l	96
88) 1,4-Dichlorobenzene	13.735	146	1635	0.269	ug/l	93
89) n-Butylbenzene	14.059	91	3540	0.435	ug/l	93
91) 1,2-Dichlorobenzene	14.100	146	1651	0.292	ug/l	89
92) 1,2-Dibromo-3-Chloropr...	14.717	75	377	0.478	ug/l #	54
93) 1,2,4-Trichlorobenzene	15.394	180	2683	1.000	ug/l	91
94) Hexachlorobutadiene	15.511	225	2053	1.687	ug/l	96
95) Naphthalene	15.641	128	11702	1.286	ug/l	97
96) 1,2,3-Trichlorobenzene	15.847	180	3067	1.166	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110123\
Data File : VN079769.D
Acq On : 01 Nov 2023 14:10
Operator : JC\MD
Sample : VN1101WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1101WBL01

Quant Time: Nov 02 05:53:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 02 05:49:08 2023
Response via : Initial Calibration

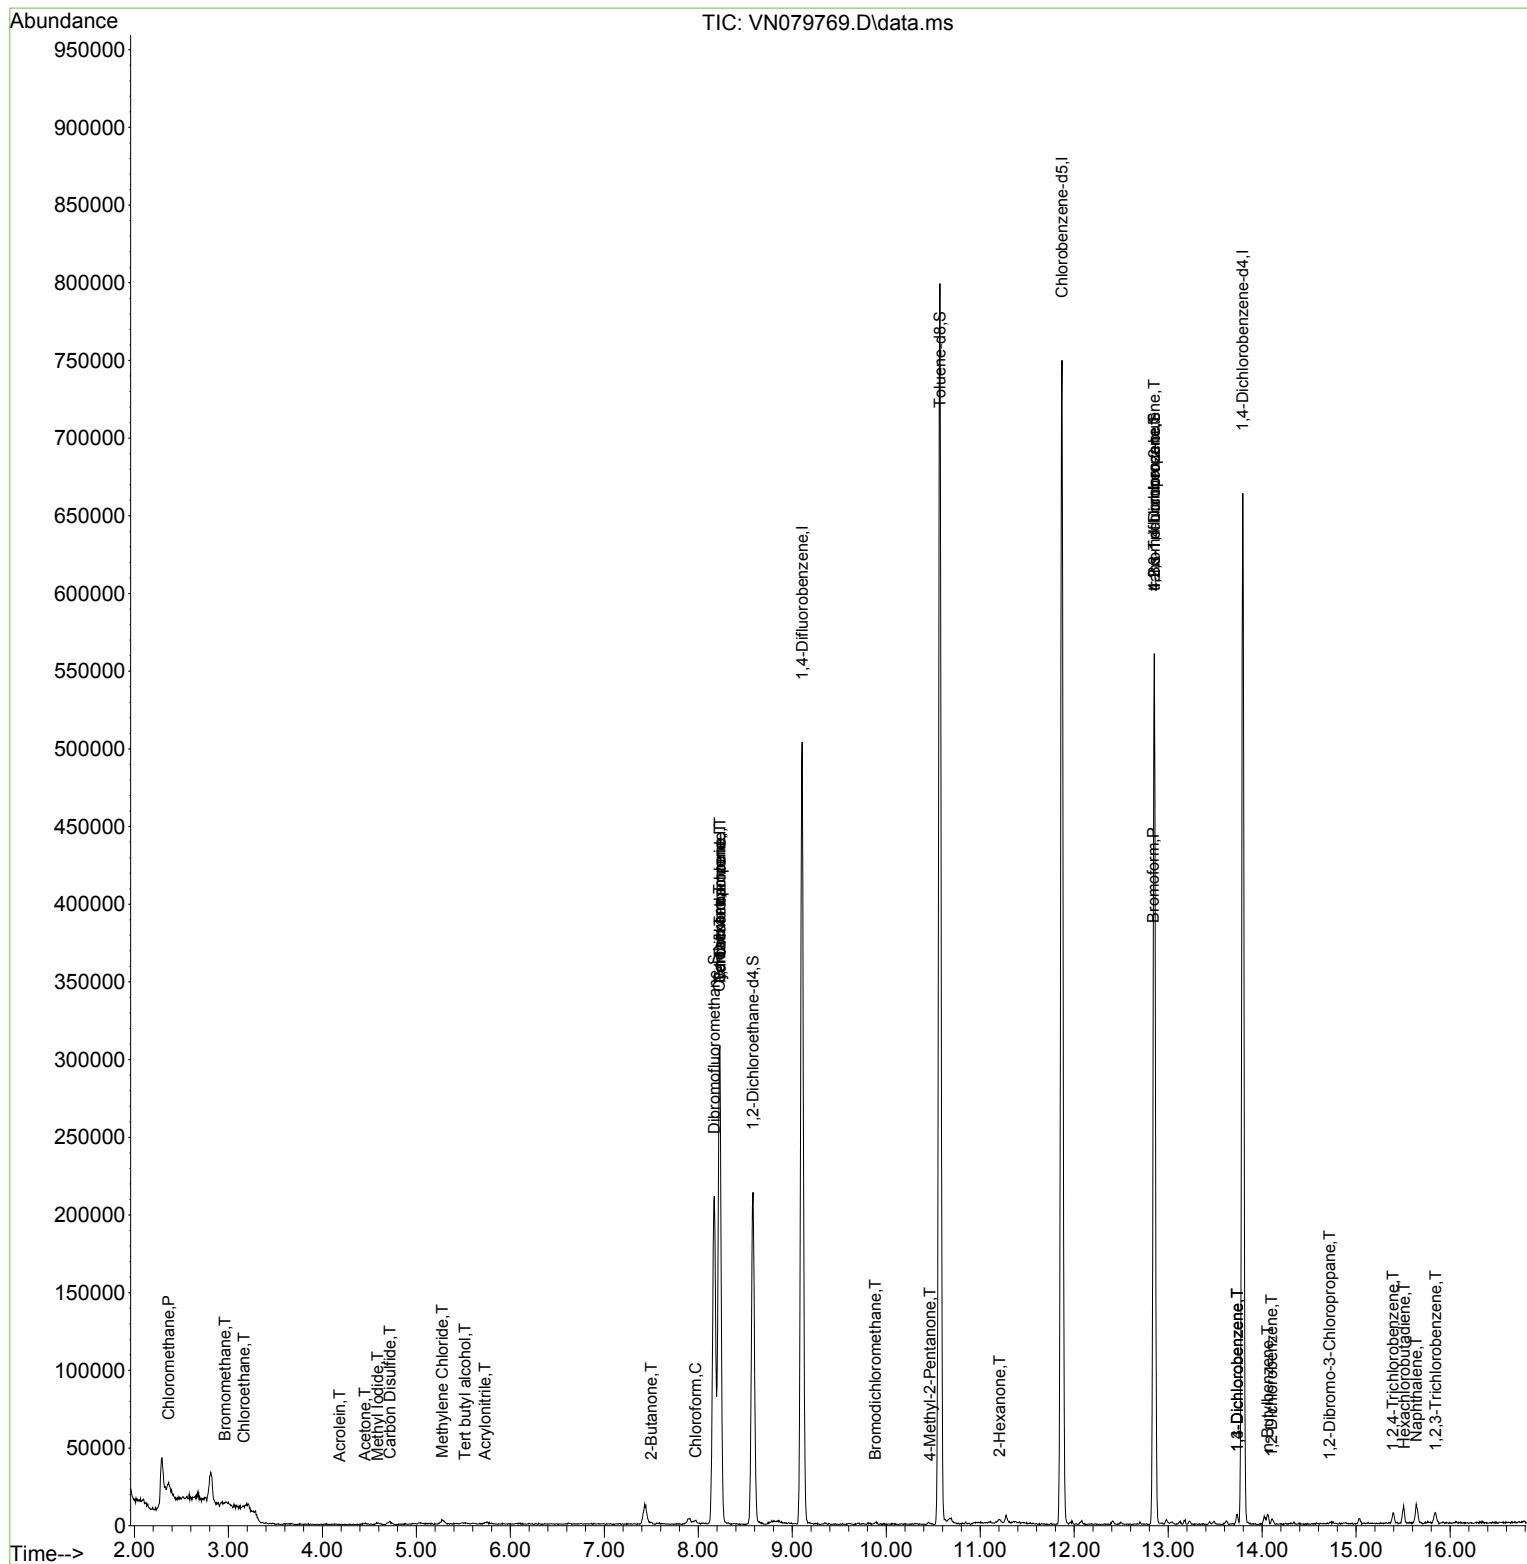



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.230 min Scan# 1

Delta R.T. 0.001 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10

Instrument :

MSVOA_N

ClientSampleId :





VN1101WBL01

Tgt Ion:168 Resp: 223934

Ion Ratio Lower Upper

168 100

99 61.6 53.0 79.6

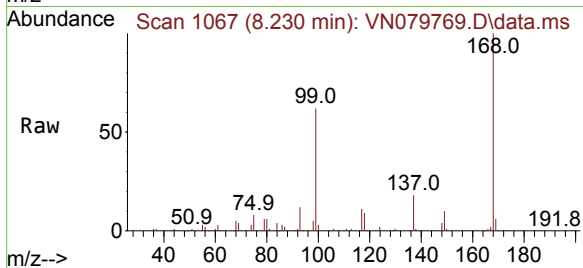

#3

Chloromethane

Concen: 0.223 ug/l

RT: 2.365 min Scan# 70

Delta R.T. 0.006 min

Lab File: VN079769.D




Acq: 01 Nov 2023 14:10

Tgt Ion: 50 Resp: 2993

Ion Ratio Lower Upper

50 100

52 21.1 26.5 39.7#


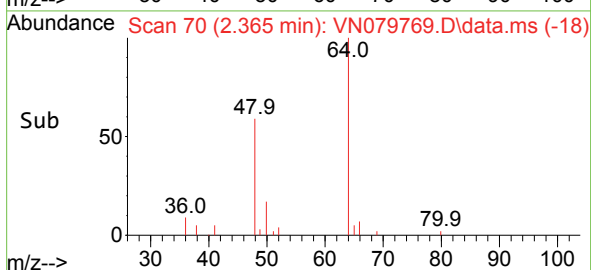

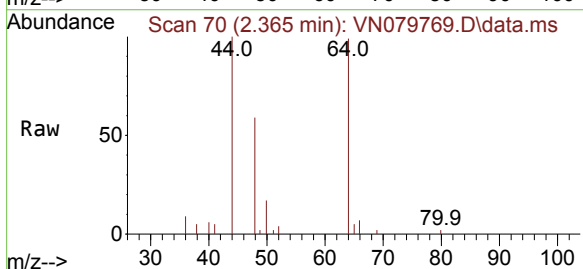




#5
Bromomethane
Concen: 0.610 ug/l
RT: 2.965 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10




Instrument :
MSVOA_N
ClientSampleId :
VN1101WBL01


Tgt Ion: 94 Resp: 1309
Ion Ratio Lower Upper
94 100
96 37.3 73.1 109.7#

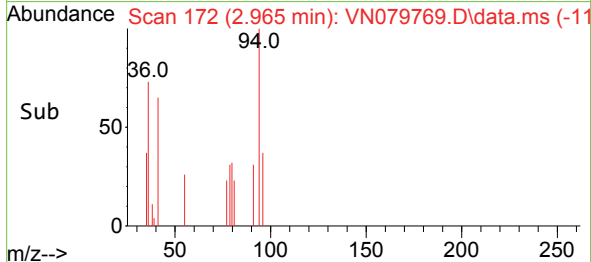

#6
Chloroethane
Concen: 0.218 ug/l
RT: 3.165 min Scan# 206
Delta R.T. 0.047 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10


Tgt Ion: 64 Resp: 607
Ion Ratio Lower Upper
64 100
66 33.5 25.4 38.2

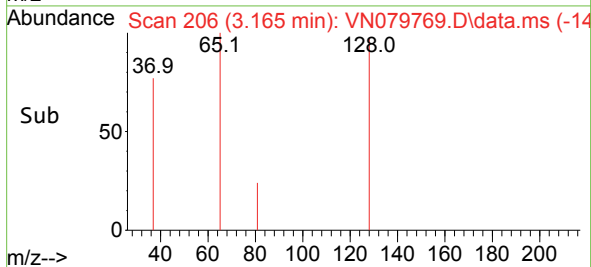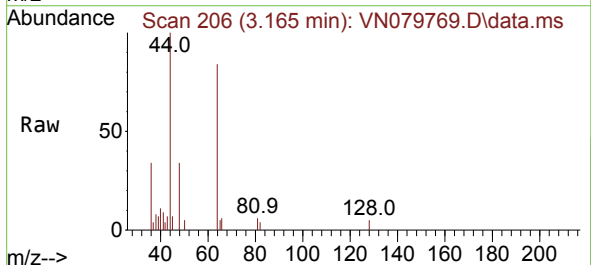






#10
Methyl Iodide
Concen: 0.617 ug/l
RT: 4.589 min Scan# 448
Delta R.T. -0.006 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10


Instrument :
MSVOA_N
ClientSampleId :
VN1101WBL01





Tgt Ion:142 Resp: 1794
Ion Ratio Lower Upper
142 100
127 49.2 37.6 56.4
141 0.0 11.4 17.0#

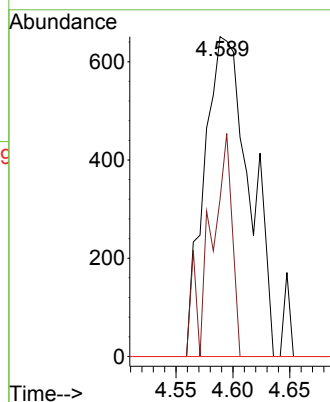


#11
Tert butyl alcohol
Concen: 0.606 ug/l
RT: 5.518 min Scan# 606
Delta R.T. 0.000 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10



Tgt Ion: 59 Resp: 264
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

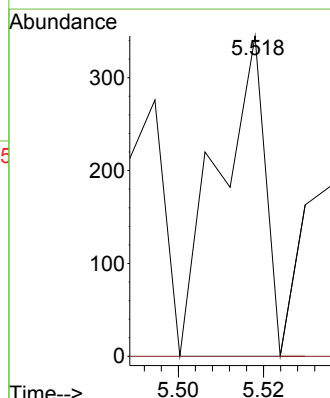



#13

Acrolein

Concen: 2.713 ug/l

RT: 4.183 min Scan# 31

Delta R.T. -0.000 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10

Instrument :

MSVOA_N

ClientSampleId :





VN1101WBL01

Tgt Ion: 56 Resp: 55

Ion Ratio Lower Upper

56 100

55 358.2 54.5 81.7#

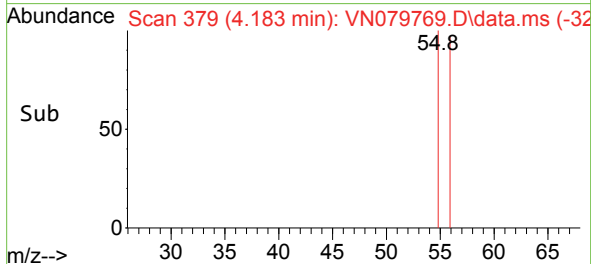

#15

Acrylonitrile

Concen: 0.480 ug/l

RT: 5.730 min Scan# 642

Delta R.T. 0.006 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10




Tgt Ion: 53 Resp: 652


Ion Ratio Lower Upper

53 100

52 129.1 65.3 97.9#

51 18.3 28.9 43.3#


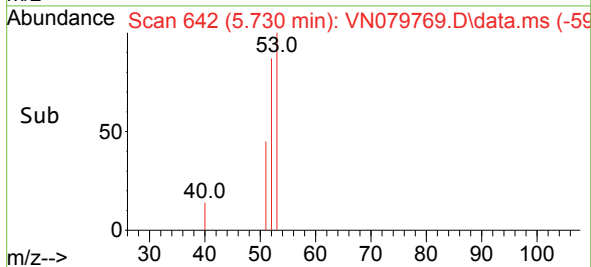

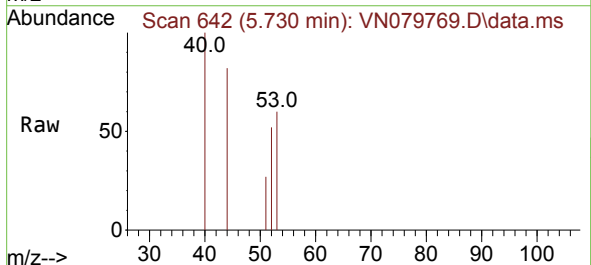




#16
Acetone
Concen: 0.896 ug/l
RT: 4.453 min Scan# 41
Delta R.T. 0.024 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10




Instrument :
MSVOA_N
ClientSampleId :
VN1101WBL01


Tgt Ion: 43 Resp: 1074
Ion Ratio Lower Upper
43 100
58 0.0 28.0 42.0#

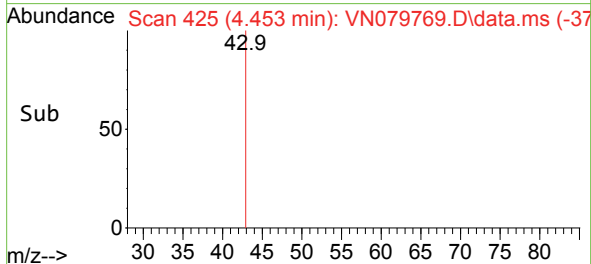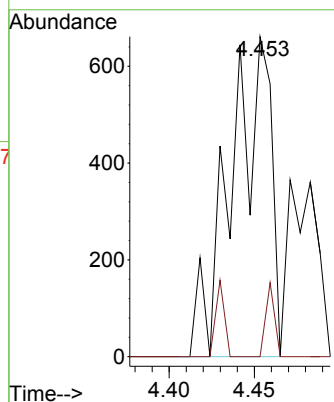

#17
Carbon Disulfide
Concen: 0.593 ug/l
RT: 4.718 min Scan# 470
Delta R.T. 0.006 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10


Tgt Ion: 76 Resp: 4123
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.0#

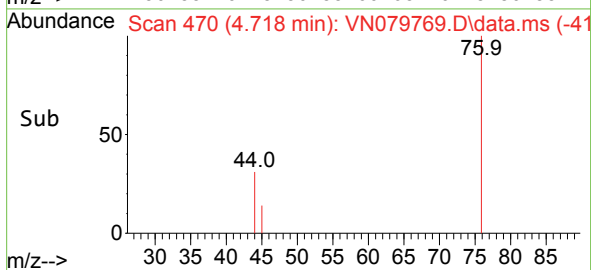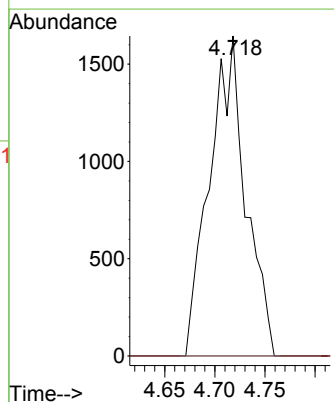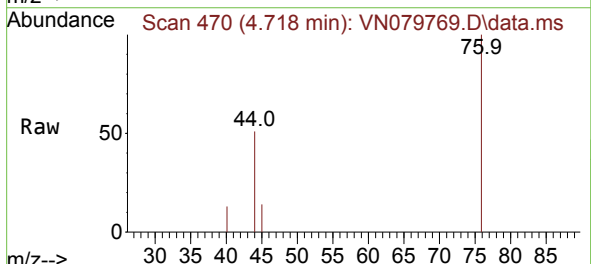





#20
Methylene Chloride
Concen: 0.615 ug/l
RT: 5.277 min Scan# 501
Delta R.T. 0.006 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10

Instrument :
MSVOA_N
ClientSampleId :
VN1101WBL01







Tgt Ion:	84	Resp:	1861
Ion	Ratio	Lower	Upper
84	100		
49	143.6	79.7	119.5#
51	36.2	25.2	37.8
86	63.5	53.3	79.9



#25
2-Butanone
Concen: 0.316 ug/l
RT: 7.500 min Scan# 943
Delta R.T. 0.012 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10

Tgt Ion:	43	Resp:	555
Ion	Ratio	Lower	Upper
43	100		
72	0.0	30.2	45.2#


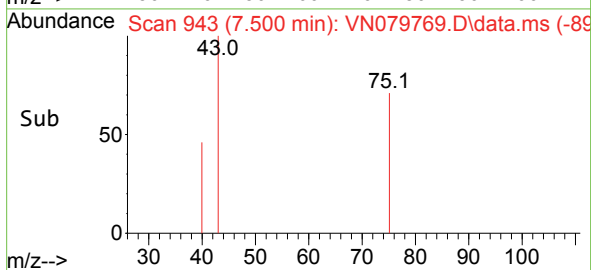

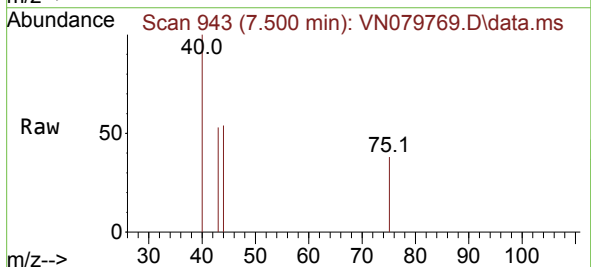




#30
Chloroform
Concen: 0.411 ug/l
RT: 7.971 min Scan# 1023
Delta R.T. 0.000 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10




Instrument :
MSVOA_N
ClientSampleId :
VN1101WBL01


Tgt Ion: 83 Resp: 2324
Ion Ratio Lower Upper
83 100
85 80.2 55.4 83.0

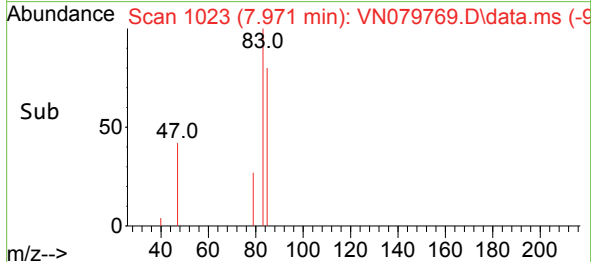

#31
Cyclohexane
Concen: 1.211 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.035 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10

Tgt Ion: 56 Resp: 5458
Ion Ratio Lower Upper
56 100
69 142.4 26.8 40.2#
84 167.5 81.8 122.6#

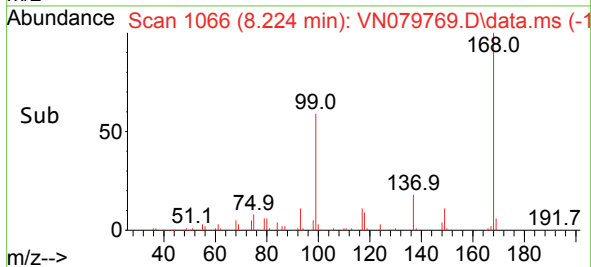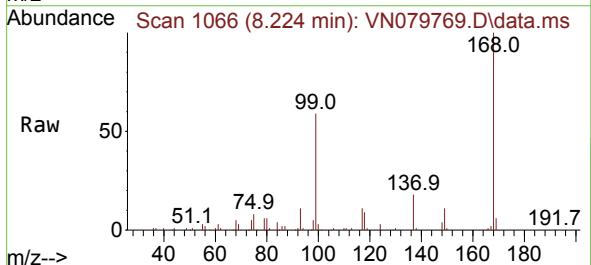



#33

1,2-Dichloroethane-d4

Concen: 50.518 ug/l

RT: 8.582 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10

Instrument :

MSVOA_N

ClientSampleId :





VN1101WBL01

Tgt Ion: 65 Resp: 172352

Ion Ratio Lower Upper

65 100

67 52.1 0.0 106.6

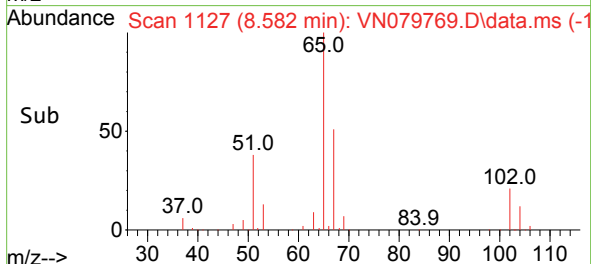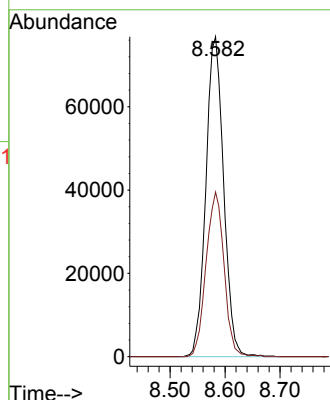

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. 0.000 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10




Tgt Ion: 114 Resp: 430062


Ion Ratio Lower Upper

114 100

63 19.7 0.0 36.4

88 13.8 0.0 30.6

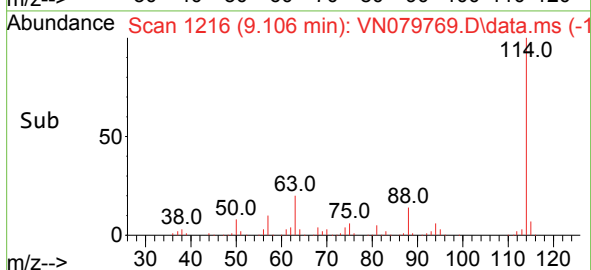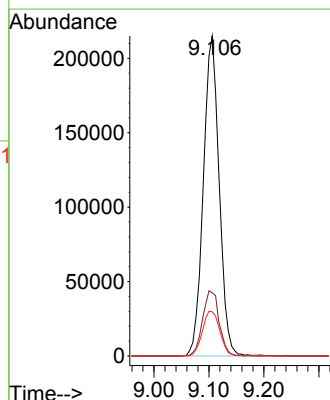



#35

Dibromofluoromethane

Concen: 49.540 ug/l

RT: 8.171 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10

Instrument :

MSVOA_N

ClientSampleId :

VN1101WBL01





Tgt Ion:113 Resp: 150789

Ion Ratio Lower Upper

113 100

111 104.4 82.6 123.8

192 17.3 12.7 19.1

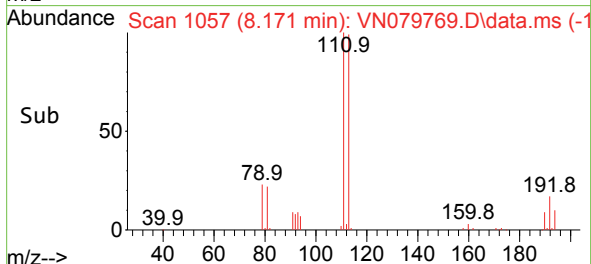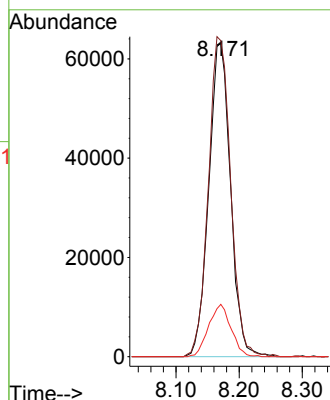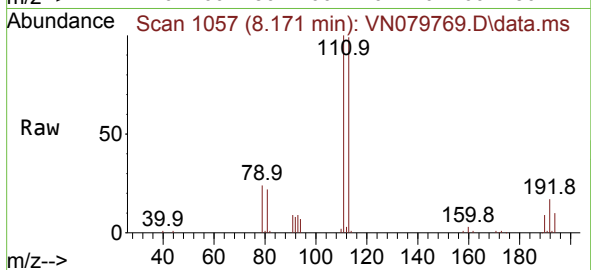

#36

1,1-Dichloropropene

Concen: 4.479 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.147 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10




Tgt Ion: 75 Resp: 19464


Ion Ratio Lower Upper

75 100

110 8.1 19.1 57.3#

77 0.0 25.0 37.4#

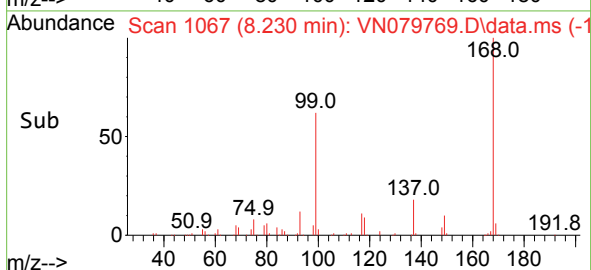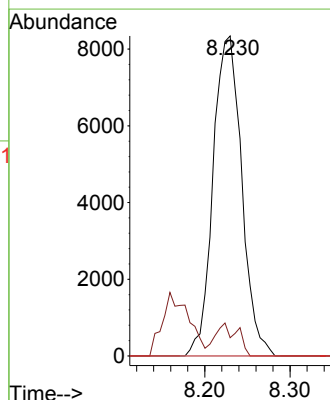



#38

Carbon Tetrachloride

Concen: 5.668 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.129 min

Lab File: VN079769.D


Acq: 01 Nov 2023 14:10

Instrument :

MSVOA_N

ClientSampleId :

VN1101WBL01

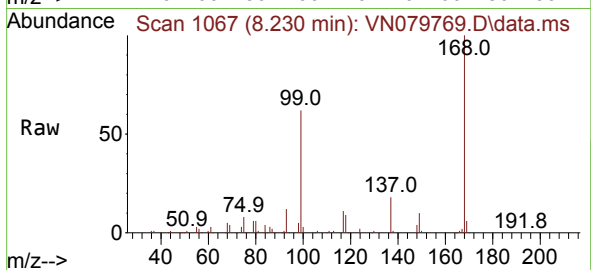




Tgt Ion:117 Resp: 24827

Ion Ratio Lower Upper

117 100

119 4.4 77.3 115.9#

121 0.0 23.3 34.9#

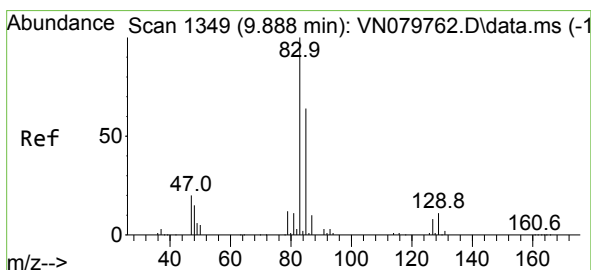

#47

Bromodichloromethane

Concen: 0.255 ug/l

RT: 9.882 min Scan# 1348

Delta R.T. -0.006 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10




Tgt Ion: 83 Resp: 1234


Ion Ratio Lower Upper

83 100

85 37.5 49.6 74.4#

127 0.0 7.0 10.6#


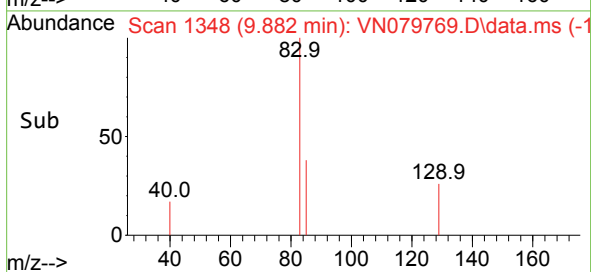
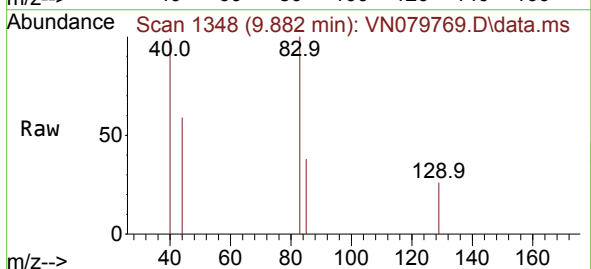



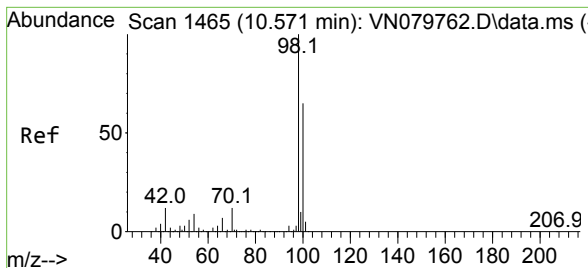

#50
Toluene-d8
Concen: 48.683 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10




Instrument :
MSVOA_N
ClientSampleId :
VN1101WBL01


Tgt Ion: 98 Resp: 545513
Ion Ratio Lower Upper
98 100
100 65.0 52.0 78.0

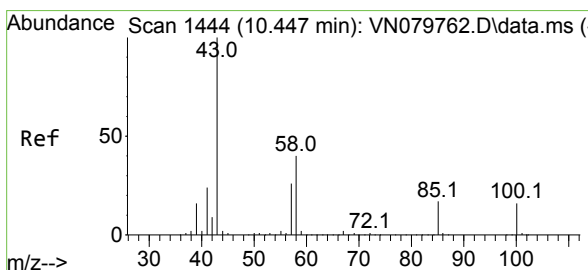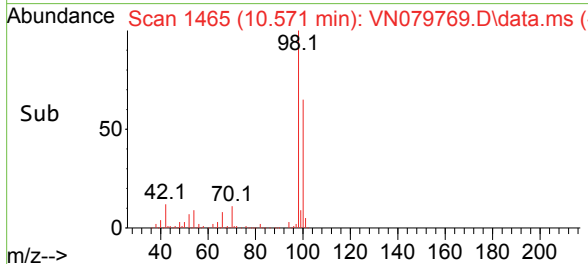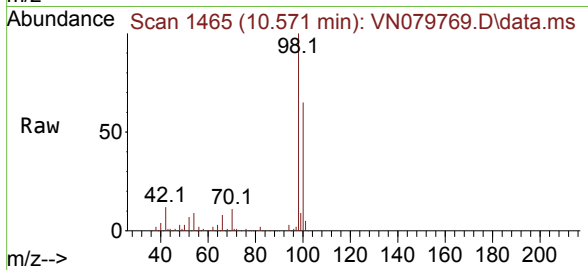

#51
4-Methyl-2-Pentanone
Concen: 0.286 ug/l
RT: 10.465 min Scan# 1447
Delta R.T. 0.018 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10

Tgt Ion: 43 Resp: 1125
Ion Ratio Lower Upper
43 100
58 26.0 36.6 54.8#


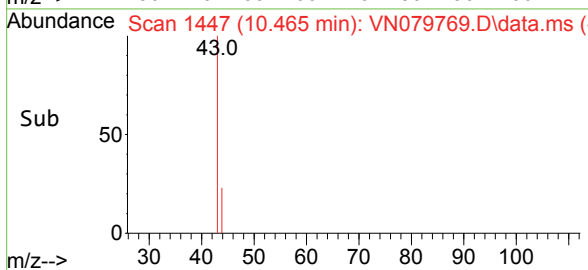

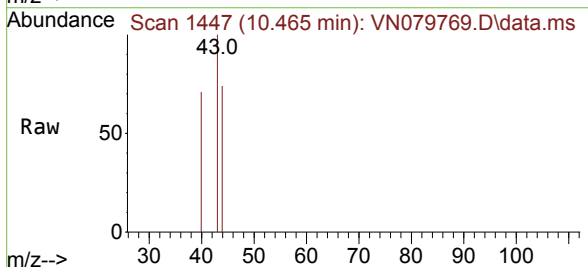


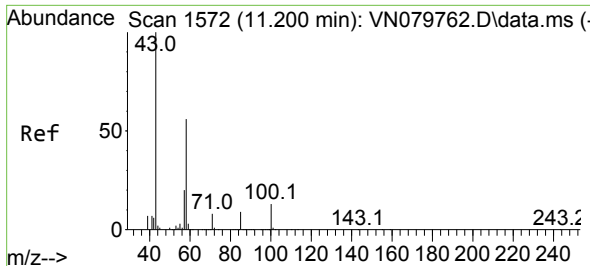

#59
2-Hexanone
Concen: 0.970 ug/l
RT: 11.206 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10




Instrument :
MSVOA_N
ClientSampleId :
VN1101WBL01


Tgt Ion: 43 Resp: 2919
Ion Ratio Lower Upper
43 100
58 28.5 31.7 95.1#

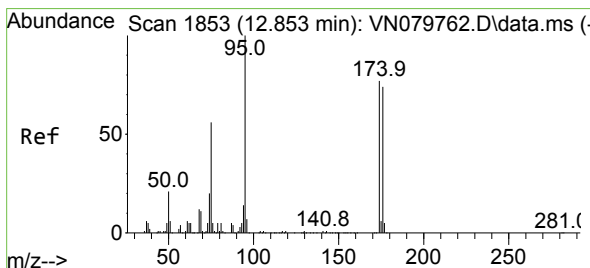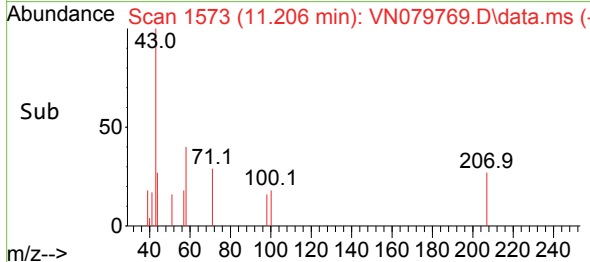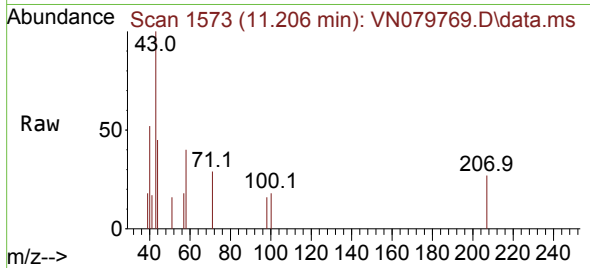

#62
4-Bromofluorobenzene
Concen: 49.226 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10

Tgt Ion: 95 Resp: 182937
Ion Ratio Lower Upper
95 100
174 78.5 0.0 143.8
176 75.4 0.0 135.8


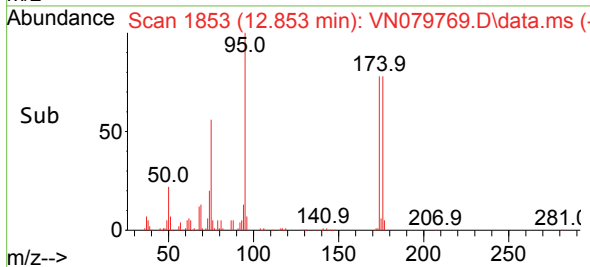

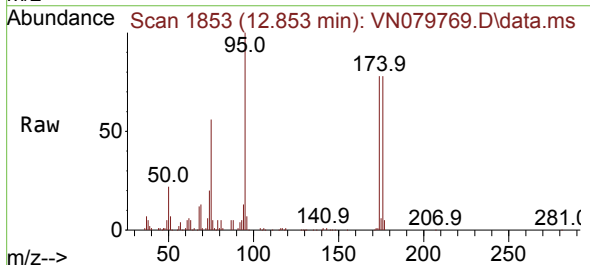




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10




Instrument :
MSVOA_N
ClientSampleId :
VN1101WBL01


Tgt Ion:117 Resp: 431748
Ion Ratio Lower Upper
117 100
82 56.6 44.0 66.0
119 32.1 25.6 38.4

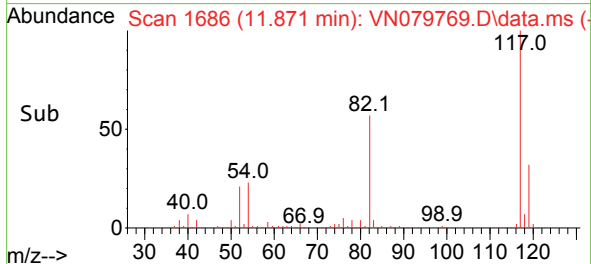

#71
Bromoform
Concen: 0.502 ug/l
RT: 12.841 min Scan# 1851
Delta R.T. 0.259 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10

Tgt Ion:173 Resp: 1202
Ion Ratio Lower Upper
173 100
175 734.1 24.3 73.0#
254 0.0 0.0 0.0


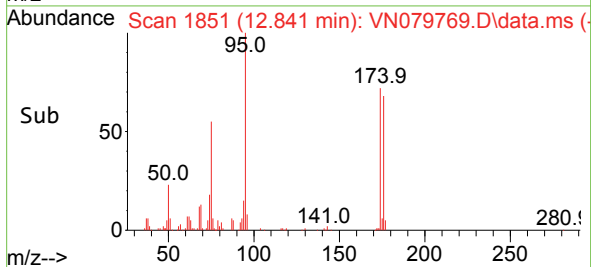

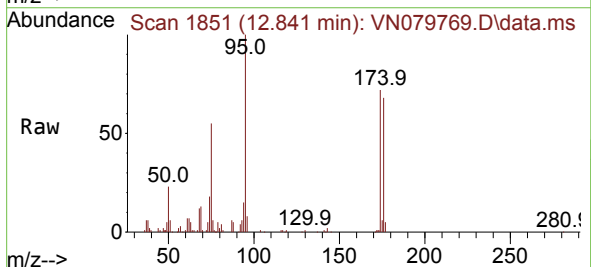


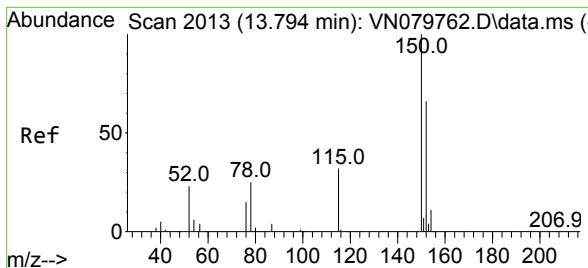

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 2013
 Delta R.T. 0.000 min
 Lab File: VN079769.D
 Acq: 01 Nov 2023 14:10




Instrument :
 MSVOA_N
 ClientSampleId :
 VN1101WBL01


Tgt Ion:152 Resp: 172986
 Ion Ratio Lower Upper
 152 100
 115 61.0 32.3 96.8
 150 157.0 0.0 355.8

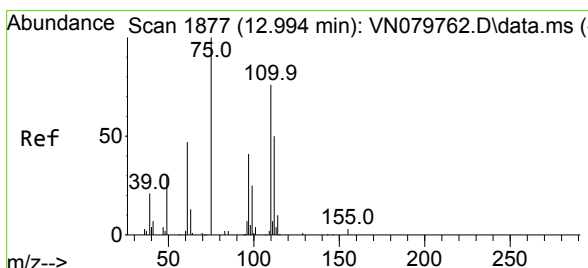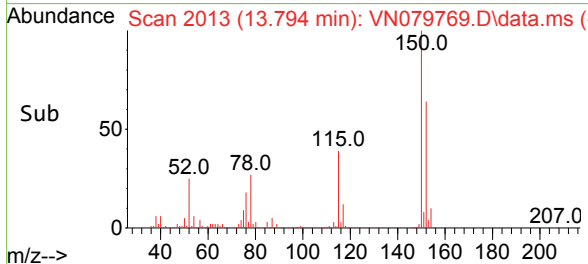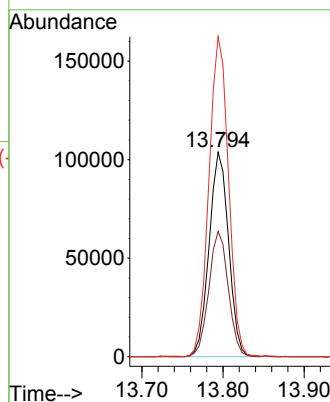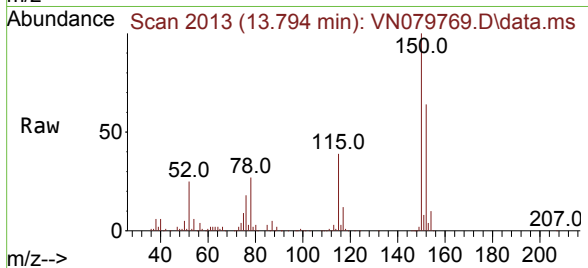

#76
 1,2,3-Trichloropropane
 Concen: 24.984 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. -0.141 min
 Lab File: VN079769.D
 Acq: 01 Nov 2023 14:10

Tgt Ion: 75 Resp: 101465
 Ion Ratio Lower Upper
 75 100
 77 1.2 84.5 253.5#


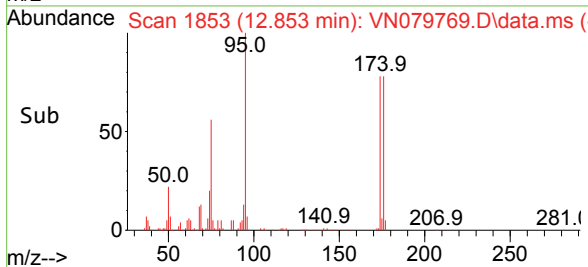
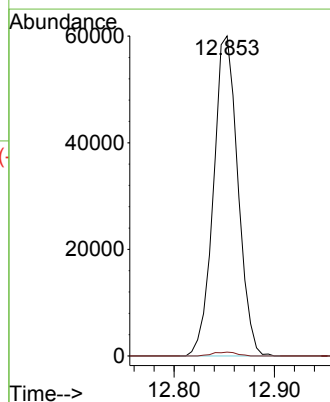
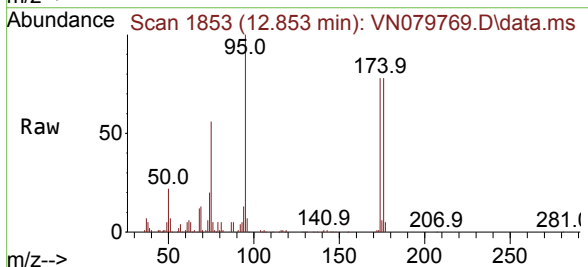


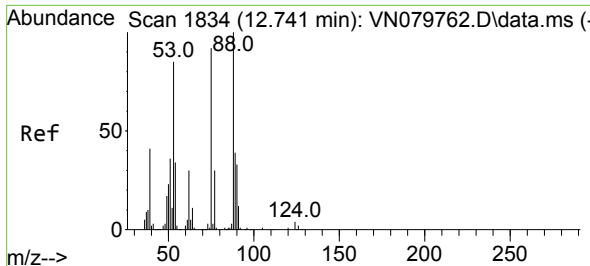

#81
trans-1,4-Dichloro-2-butene
Concen: 67.976 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.118 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10




Instrument :
MSVOA_N
ClientSampleId :
VN1101WBL01


Tgt Ion: 75 Resp: 101465
Ion Ratio Lower Upper
75 100
53 0.1 67.4 101.2#
89 0.0 38.8 58.2#

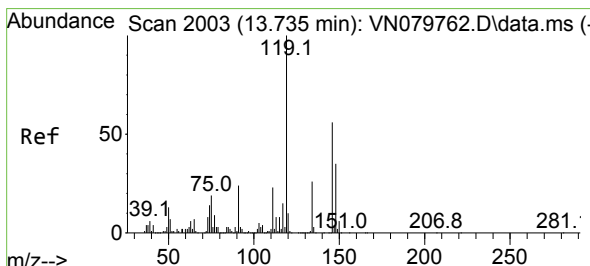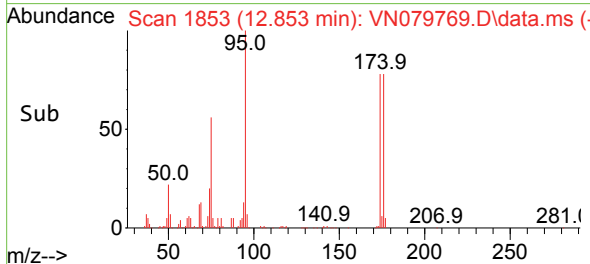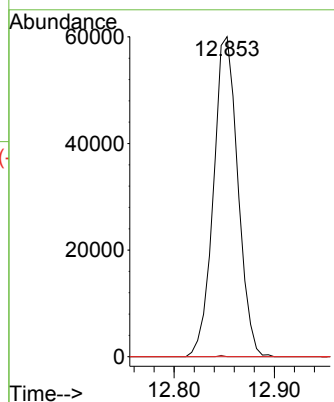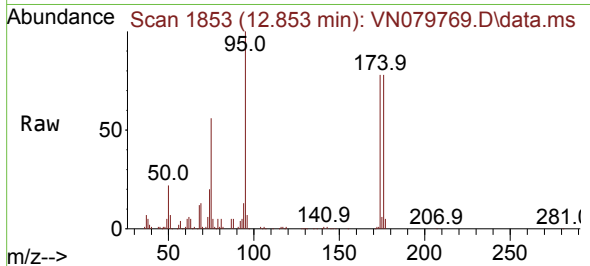

#87
1,3-Dichlorobenzene
Concen: 0.273 ug/l
RT: 13.735 min Scan# 2003
Delta R.T. 0.000 min
Lab File: VN079769.D
Acq: 01 Nov 2023 14:10

Tgt Ion:146 Resp: 1635
Ion Ratio Lower Upper
146 100
111 44.4 22.1 66.3
148 69.2 32.0 96.0


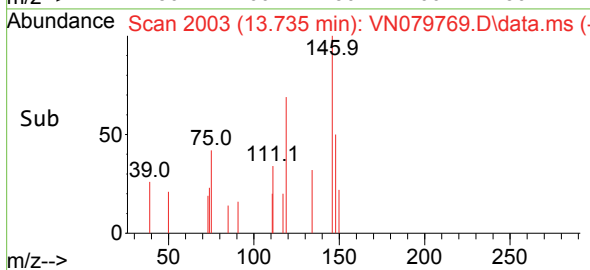
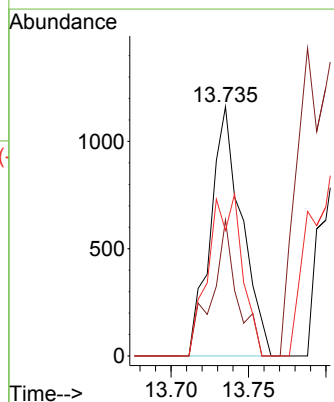
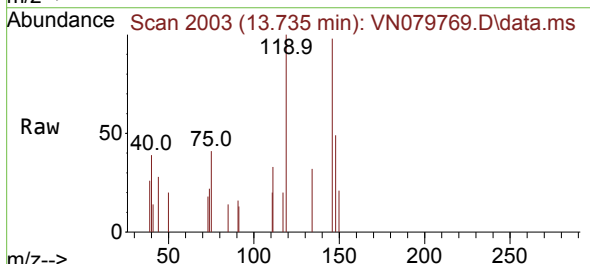


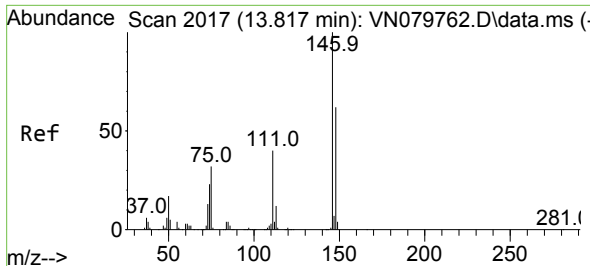

#88
 1,4-Dichlorobenzene
 Concen: 0.269 ug/l
 RT: 13.735 min Scan# 2017
 Delta R.T. -0.082 min
 Lab File: VN079769.D
 Acq: 01 Nov 2023 14:10




Instrument :
 MSVOA_N
 ClientSampleId :
 VN1101WBL01


Tgt Ion:146 Resp: 1635
 Ion Ratio Lower Upper
 146 100
 111 44.4 20.6 61.8
 148 69.2 31.6 94.8

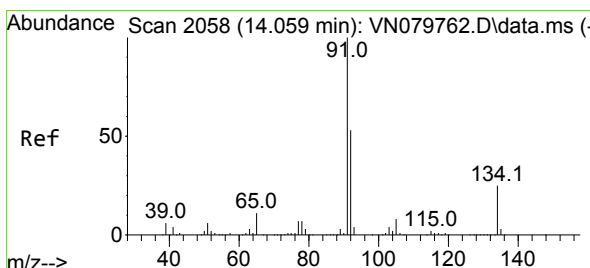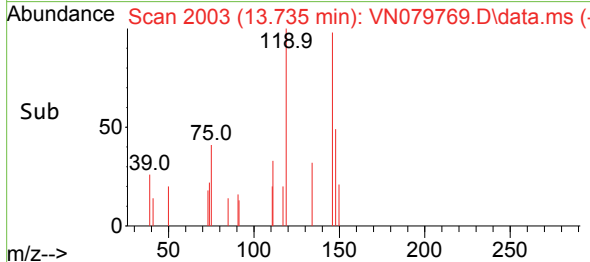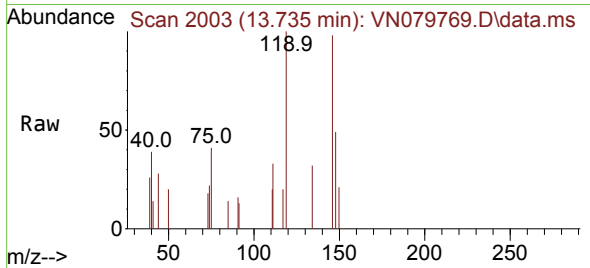

#89
 n-Butylbenzene
 Concen: 0.435 ug/l
 RT: 14.059 min Scan# 2058
 Delta R.T. 0.000 min
 Lab File: VN079769.D
 Acq: 01 Nov 2023 14:10

Tgt Ion: 91 Resp: 3540
 Ion Ratio Lower Upper
 91 100
 92 55.0 26.4 79.0
 134 32.7 12.6 37.6

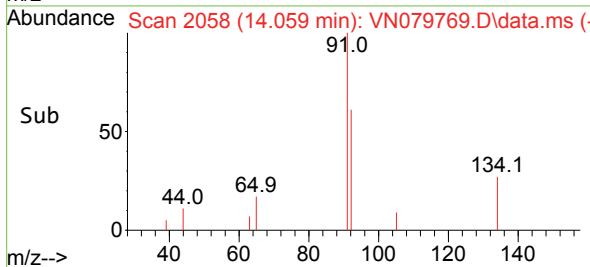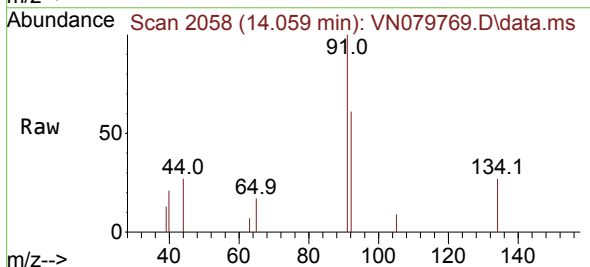



#91

1,2-Dichlorobenzene

Concen: 0.292 ug/l

RT: 14.100 min Scan# 2066

Delta R.T. -0.006 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10

Instrument :

MSVOA_N

ClientSampleId :

VN1101WBL01





Tgt Ion:146 Resp: 1651

Ion Ratio Lower Upper

146 100

111 33.1 22.0 66.0

148 68.9 31.8 95.3

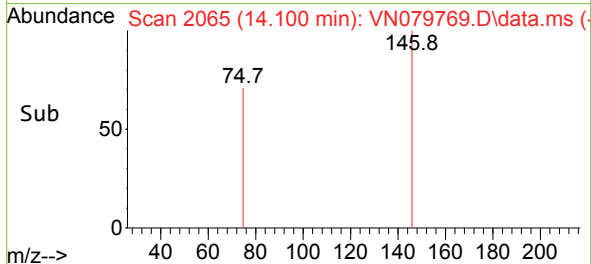

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.478 ug/l

RT: 14.717 min Scan# 2170

Delta R.T. -0.006 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10




Tgt Ion: 75 Resp: 377


Ion Ratio Lower Upper

75 100

155 17.8 39.1 117.2#

157 72.1 50.3 150.9

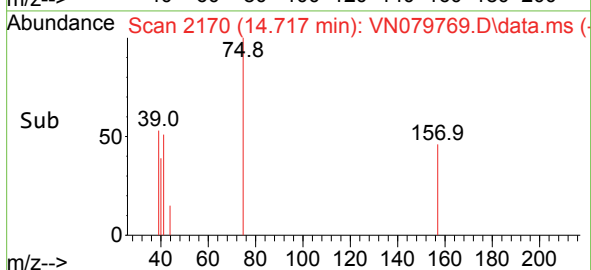



#93

1,2,4-Trichlorobenzene

Concen: 1.000 ug/l

RT: 15.394 min Scan# 21

Delta R.T. 0.000 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10

Instrument :

MSVOA_N

ClientSampleId :

VN1101WBL01





Tgt Ion:180 Resp: 2683

Ion Ratio Lower Upper

180 100

182 95.0 46.1 138.2

145 19.5 16.6 49.8

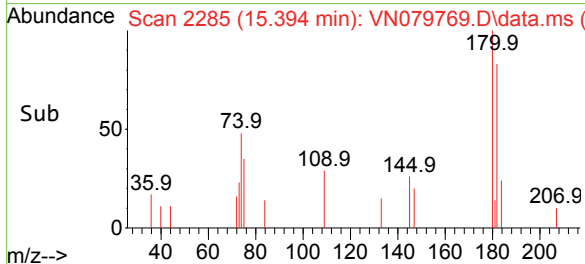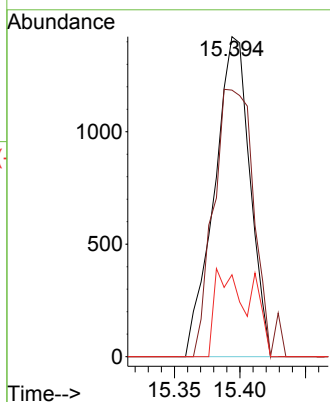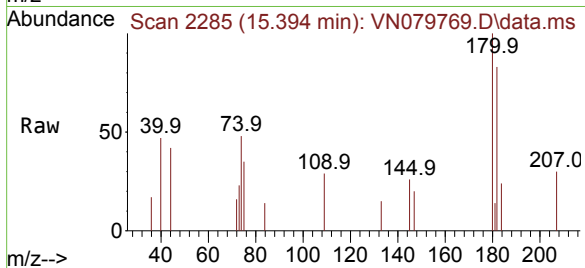

#94

Hexachlorobutadiene

Concen: 1.687 ug/l

RT: 15.511 min Scan# 2305

Delta R.T. 0.006 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10




Tgt Ion:225 Resp: 2053


Ion Ratio Lower Upper

225 100

223 63.7 31.3 93.8

227 59.3 31.9 95.9

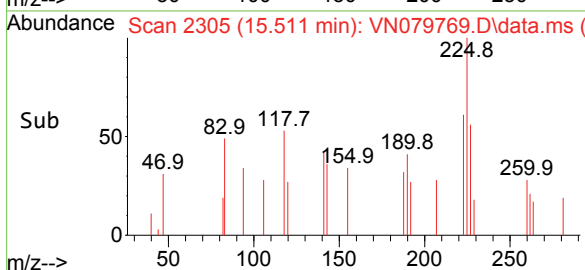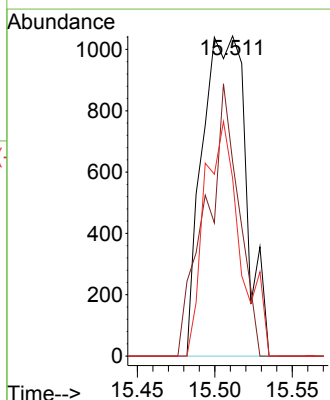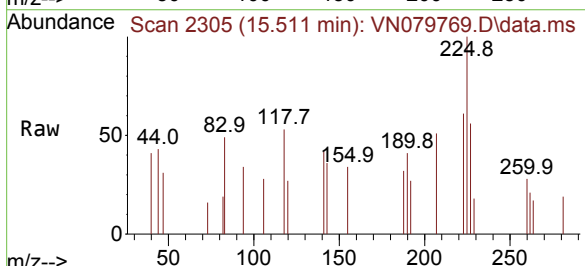



#95

Naphthalene

Concen: 1.286 ug/l

RT: 15.641 min Scan# 21

Delta R.T. 0.000 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10

Instrument :

MSVOA_N

ClientSampleId :

VN1101WBL01





Tgt Ion:128 Resp: 11702

Ion Ratio Lower Upper

128 100

127 13.7 10.0 15.0

129 9.5 8.7 13.1

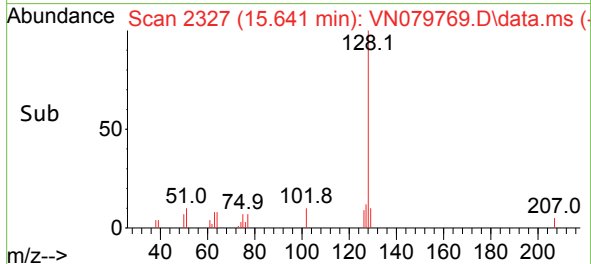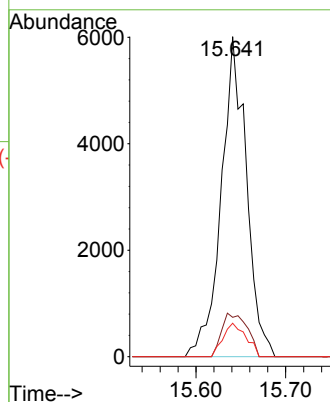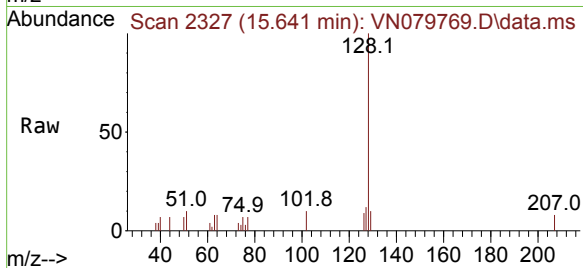

#96

1,2,3-Trichlorobenzene

Concen: 1.166 ug/l

RT: 15.847 min Scan# 2362

Delta R.T. 0.006 min

Lab File: VN079769.D

Acq: 01 Nov 2023 14:10

Tgt Ion:180 Resp: 3067

Ion Ratio Lower Upper

180 100

182 90.5 46.2 138.6

145 26.5 17.5 52.6

