

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110123\
 Data File : VN079773.D
 Acq On : 01 Nov 2023 15:55
 Operator : JC\MD
 Sample : 05173-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BP-VPB-188-GW-58-60

Quant Time: Nov 02 05:55:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 02 05:49:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	221604	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	426722	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	426036	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	172385	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	173049	51.255	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 102.520%	
35) Dibromofluoromethane	8.171	113	151298	50.096	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.200%	
50) Toluene-d8	10.571	98	546772	49.178	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 98.360%	
62) 4-Bromofluorobenzene	12.853	95	188852	51.216	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 102.440%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110123\
Data File : VN079773.D
Acq On : 01 Nov 2023 15:55
Operator : JC\MD
Sample : 05173-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-188-GW-58-60


Quant Time: Nov 02 05:55:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 02 05:49:08 2023
Response via : Initial Calibration

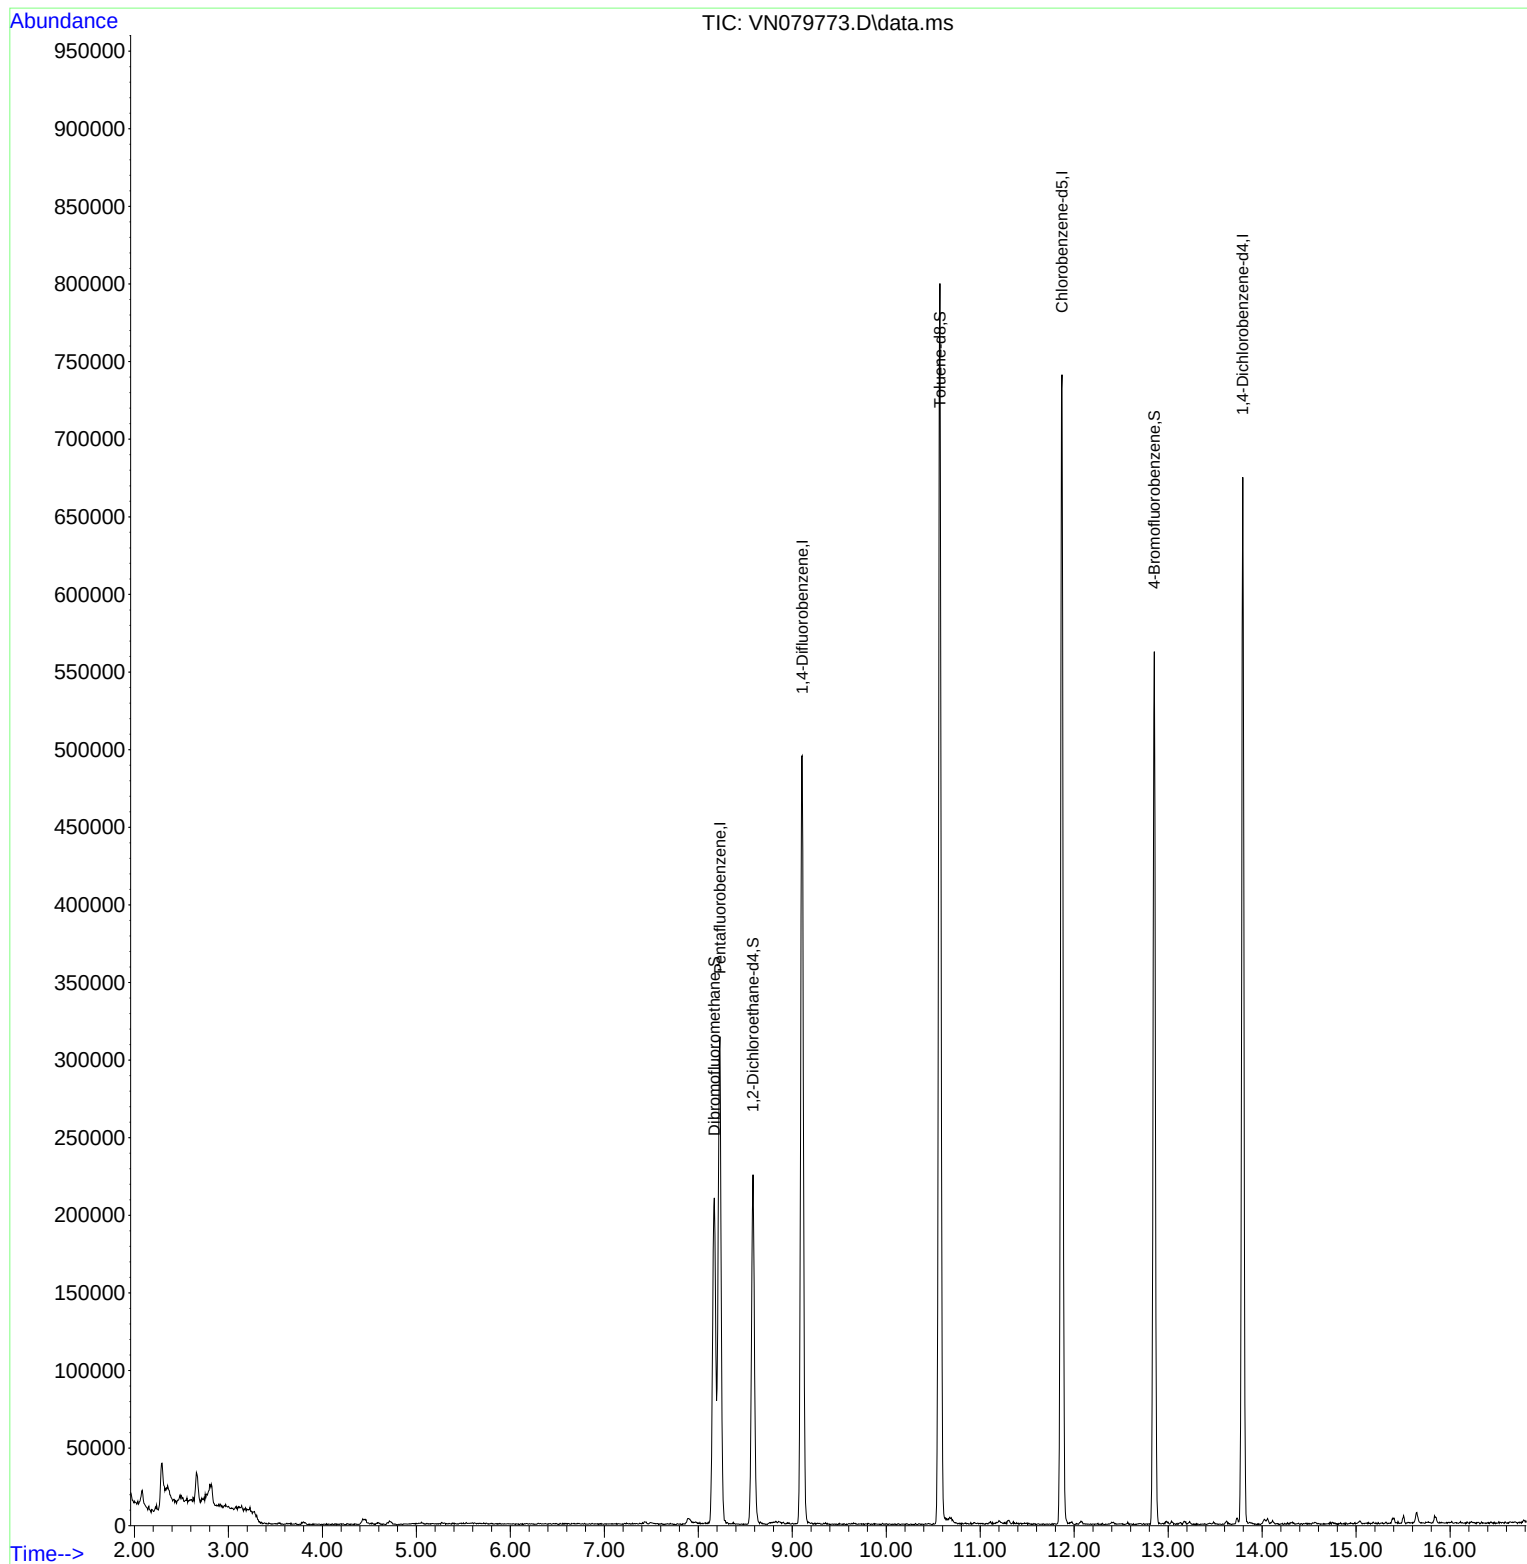



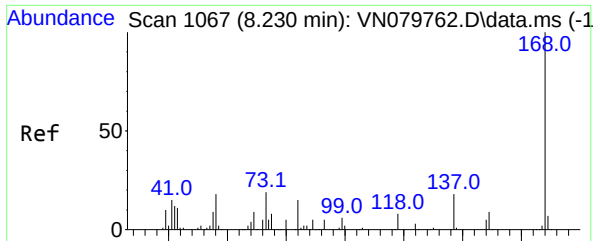


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. 0.001 min
Lab File: VN079773.D
Acq: 01 Nov 2023 15:55

Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-188-GW-58-60



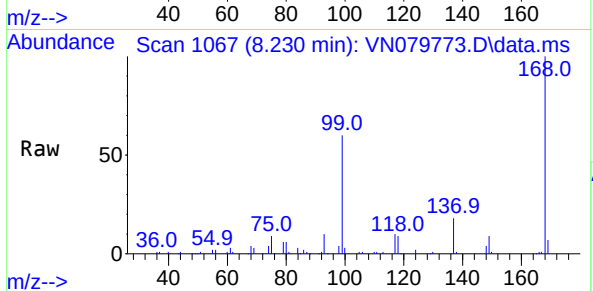



Tgt Ion:168 Resp: 221604
Ion Ratio Lower Upper
168 100
99 60.2 53.0 79.6

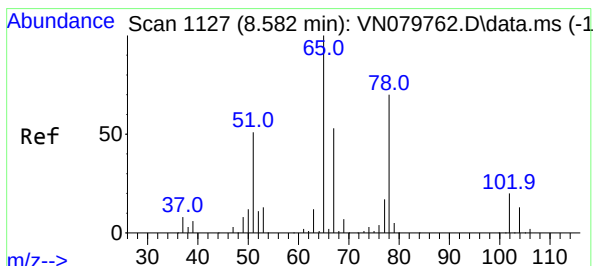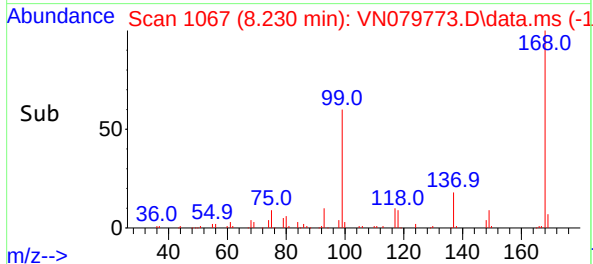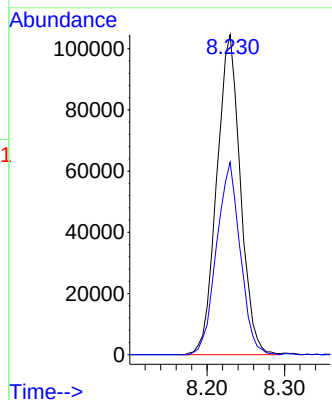

#33
1,2-Dichloroethane-d4
Concen: 51.255 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VN079773.D
Acq: 01 Nov 2023 15:55

Tgt Ion: 65 Resp: 173049
Ion Ratio Lower Upper
65 100
67 52.4 0.0 106.6


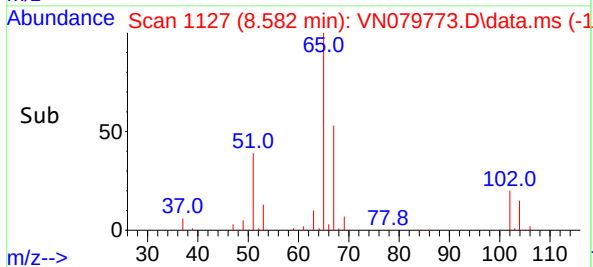
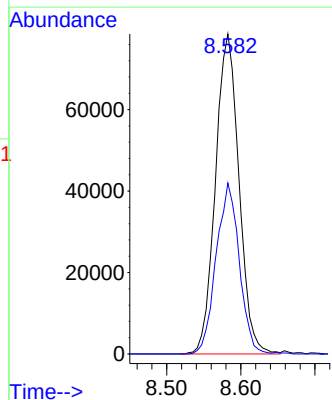
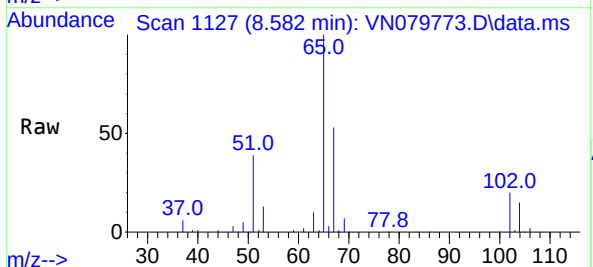


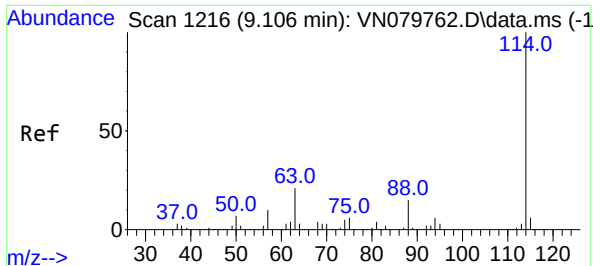

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN079773.D
Acq: 01 Nov 2023 15:55




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-188-GW-58-60


Tgt Ion:114 Resp: 426722
Ion Ratio Lower Upper
114 100
63 19.8 0.0 36.4
88 15.5 0.0 30.6

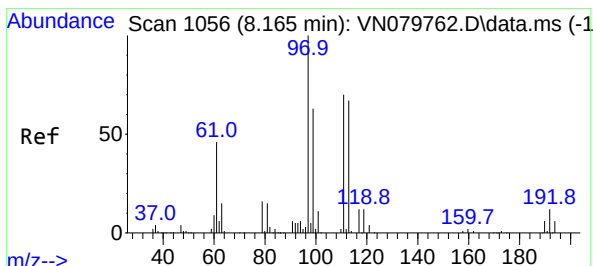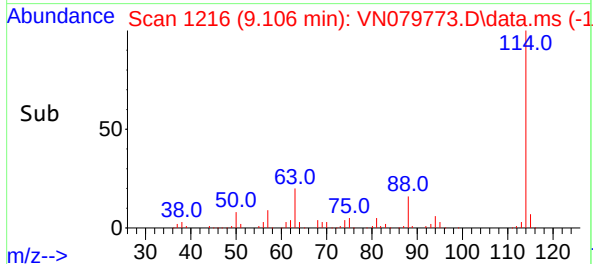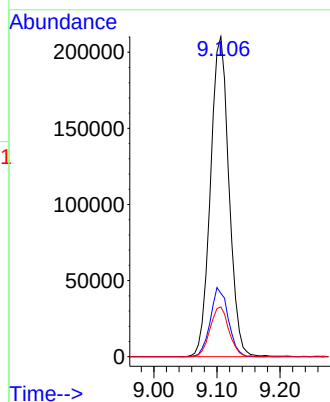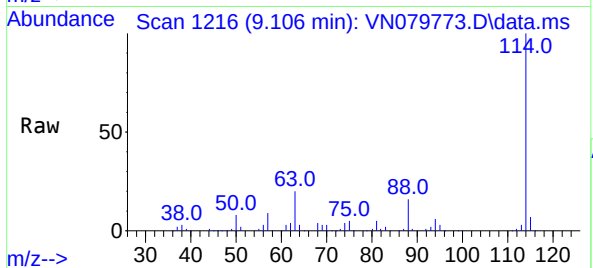

#35
Dibromofluoromethane
Concen: 50.096 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. 0.000 min
Lab File: VN079773.D
Acq: 01 Nov 2023 15:55

Tgt Ion:113 Resp: 151298
Ion Ratio Lower Upper
113 100
111 104.2 82.6 123.8
192 17.3 12.7 19.1


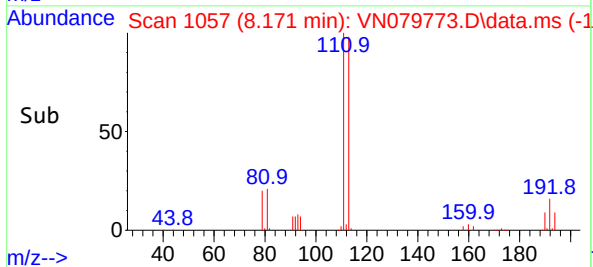
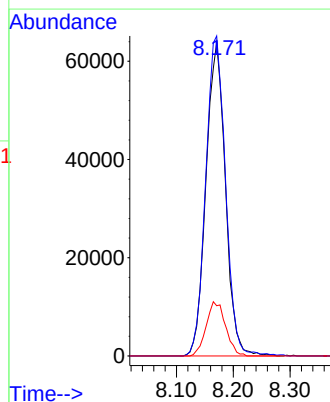
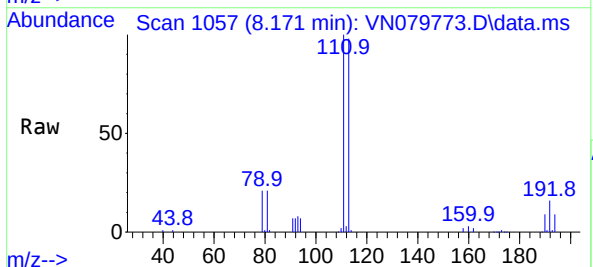


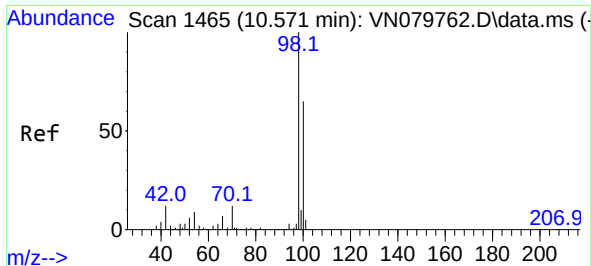

#50
Toluene-d8
Concen: 49.178 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN079773.D
Acq: 01 Nov 2023 15:55




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-188-GW-58-60


Tgt Ion: 98 Resp: 546772
Ion Ratio Lower Upper
98 100
100 63.7 52.0 78.0

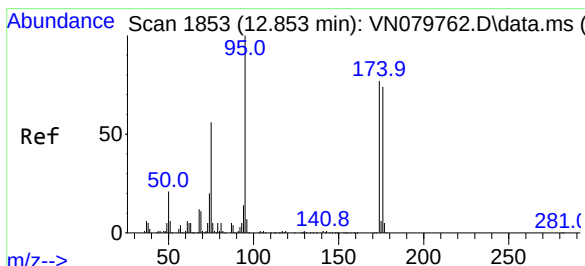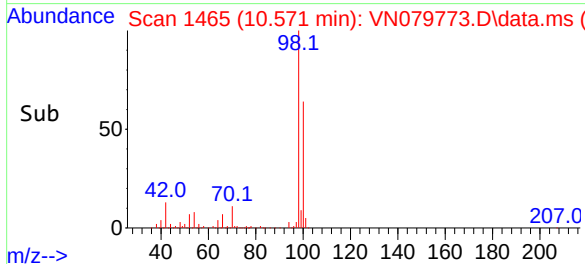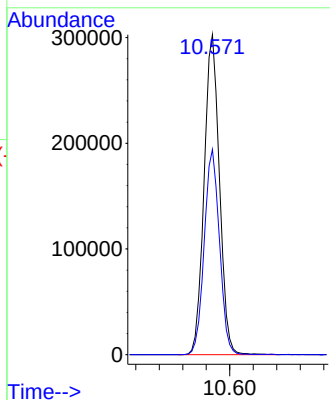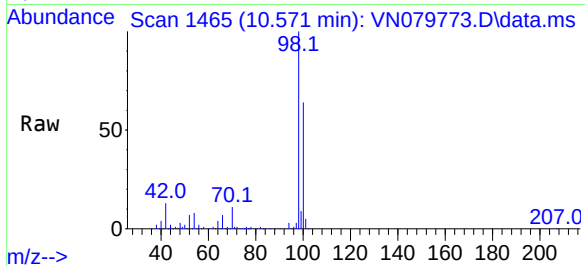

#62
4-Bromofluorobenzene
Concen: 51.216 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN079773.D
Acq: 01 Nov 2023 15:55


Tgt Ion: 95 Resp: 188852
Ion Ratio Lower Upper
95 100
174 75.3 0.0 143.8
176 73.0 0.0 135.8

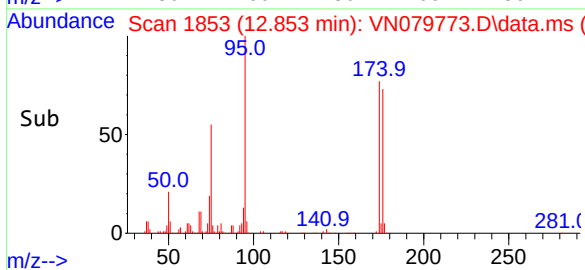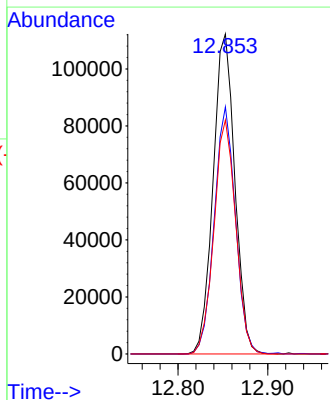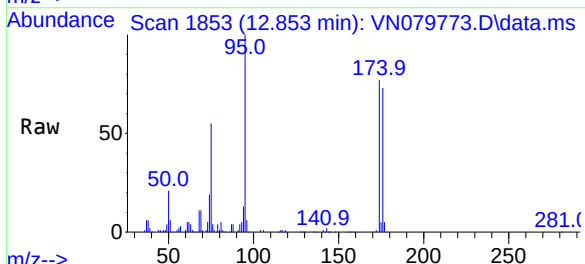



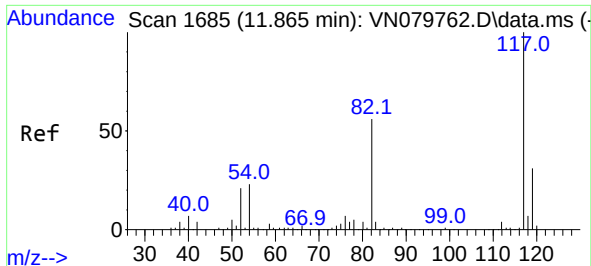


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN079773.D
Acq: 01 Nov 2023 15:55

Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-188-GW-58-60

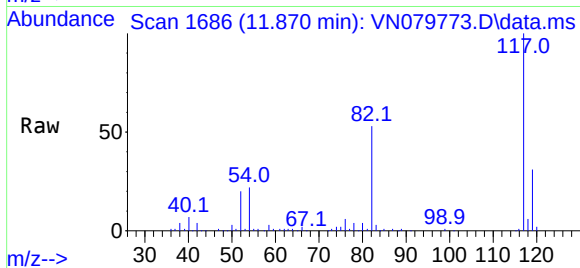

Tgt Ion:117 Resp: 426036
Ion Ratio Lower Upper
117 100
82 53.4 44.0 66.0
119 31.3 25.6 38.4

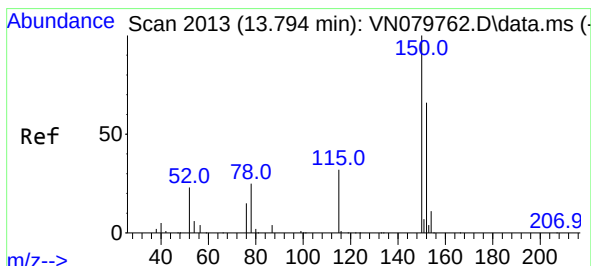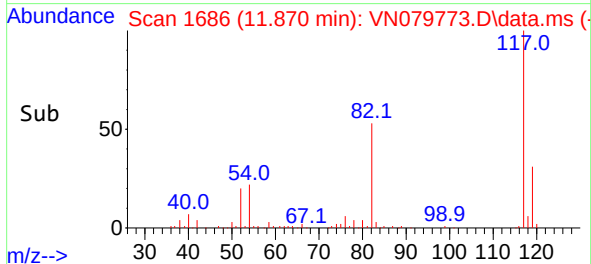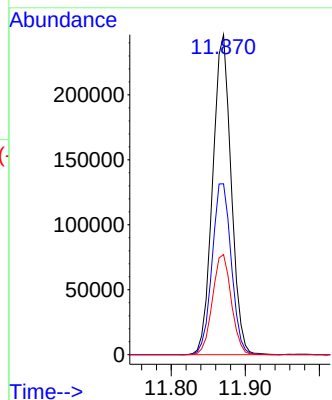

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN079773.D
Acq: 01 Nov 2023 15:55

Tgt Ion:152 Resp: 172385
Ion Ratio Lower Upper
152 100
115 61.7 32.3 96.8
150 155.8 0.0 355.8

