
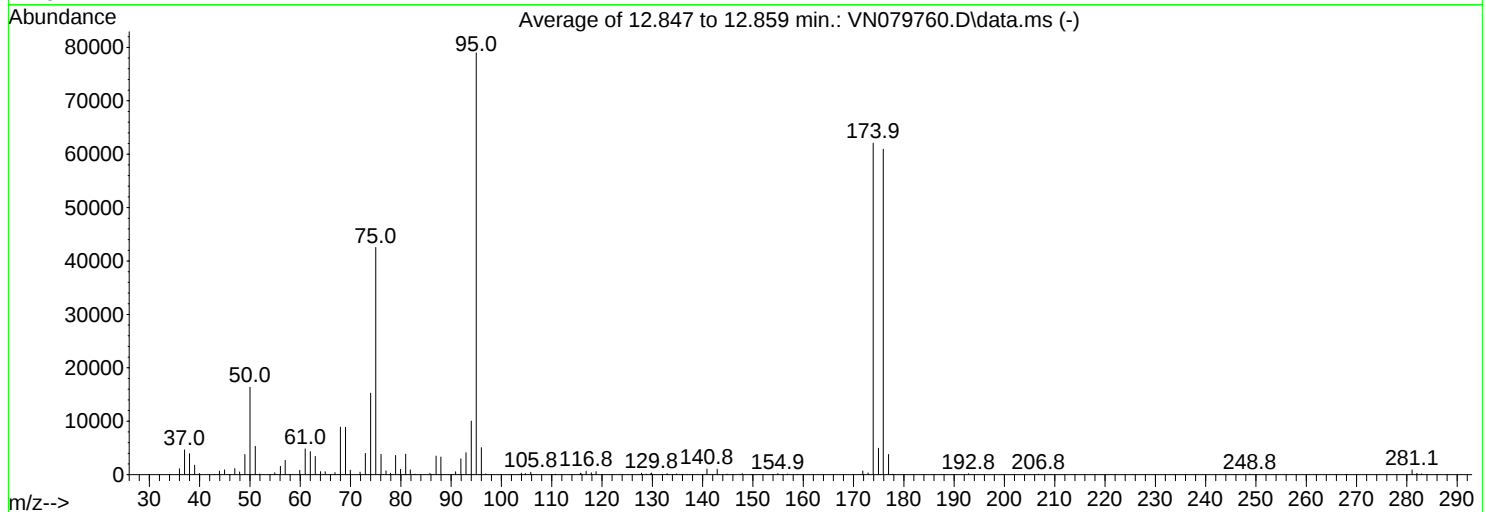


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110123\
Data File : VN079760.D
Acq On : 01 Nov 2023 09:15
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Title : SW846 8260
Last Update : Thu Nov 02 05:49:08 2023

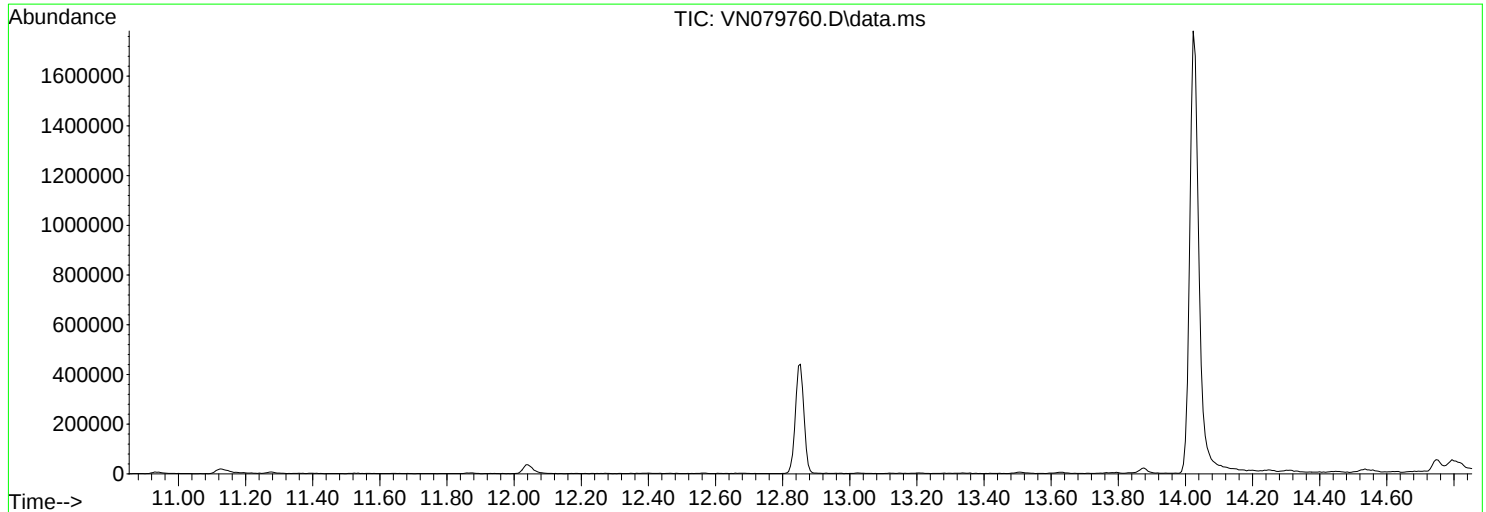

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.7	16358	PASS
75	95	30	60	53.9	42531	PASS
95	95	100	100	100.0	78973	PASS
96	95	5	9	6.4	5075	PASS
173	174	0.00	2	0.5	336	PASS
174	95	50	100	78.6	62080	PASS
175	174	5	9	8.0	4950	PASS
176	174	95	101	98.2	60944	PASS
177	176	5	9	6.2	3774	PASS

Average of 12.847 to 12.859 min.: VN079760.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	1123	49.00	3787	63.00	3429	76.05	3791
37.00	4648	50.00	16358	64.05	583	77.05	721
38.00	3938	51.05	5300	64.95	545	77.95	27
39.00	1769	51.95	121	66.90	399	78.95	360
39.95	207	54.95	348	68.00	8915	79.95	976
42.90	62	56.05	1566	69.00	8880	80.95	3848
43.95	648	57.00	2677	69.95	848	81.90	889
44.95	892	57.90	58	71.90	487	82.80	77
46.00	57	59.90	827	72.95	3978	85.80	237
47.00	1130	61.00	4833	74.00	15257	87.00	3483
47.95	525	62.00	4311	75.00	42531	87.95	3296

Average of 12.847 to 12.859 min.: VN079760.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.90	542	110.80	76	134.80	166	156.85	118
91.95	2957	115.70	268	136.90	55	158.80	68
92.95	4113	115.90	137	140.85	1055	171.85	697
94.00	10025	116.85	642	142.90	1033	172.90	336
95.00	78973	117.85	368	144.80	75	173.90	62080
96.00	5075	118.80	568	145.00	96	174.95	4950
96.90	159	127.85	287	146.10	61	175.90	60944
103.70	67	128.80	134	147.90	169	176.95	3774
103.95	270	129.70	168	149.80	73	177.80	77
104.75	199	129.85	299	154.95	200	192.85	182
105.85	466	132.95	205	155.80	54	206.80	96

Average of 12.847 to 12.859 min.: VN079760.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
248.80	89						
281.05	889						
282.00	254						
282.90	143						

Instrument :

MSVOA_N

ClientSampleId :

BFB