

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110221\
 Data File : VN069341.D
 Acq On : 2 Nov 2021 12:08
 Operator : JC/MD
 Sample : M4438-02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 03 00:47:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 28 16:09:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	276962	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	489420	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	494386	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	200479	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	189529	47.405	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	94.820%		
35) Dibromofluoromethane	8.024	113	144330	47.308	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	94.620%		
50) Toluene-d8	10.443	98	616119	50.509	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	101.020%		
62) 4-Bromofluorobenzene	12.733	95	237759	51.652	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	103.300%		
Target Compounds						Qvalue
3) Chloromethane	2.309	50	450	Below Cal	#	85
6) Chloroethane	3.003	64	512	0.212	ug/l #	43
10) Methyl Iodide	4.422	142	55	2.473	ug/l #	41
11) Tert butyl alcohol	5.385	59	838	14.428	ug/l #	72
16) Acetone	4.299	43	33901	19.902	ug/l	97
17) Carbon Disulfide	4.529	76	12904	1.945	ug/l	99
25) 2-Butanone	7.345	43	9280	5.166	ug/l	95
26) 2,2-Dichloropropane	7.327	77	867	1.003	ug/l #	53
31) Cyclohexane	8.091	56	6491	1.213	ug/l #	24
36) 1,1-Dichloropropene	8.088	75	23001	5.451	ug/l #	50
37) Ethyl Acetate	7.345	43	9280	1.930	ug/l #	75
38) Carbon Tetrachloride	8.088	117	28268	6.782	ug/l #	16
40) Benzene	8.464	78	6625	0.522	ug/l	95
43) Isopropyl Acetate	8.533	43	166	0.478	ug/l #	55
51) 4-Methyl-2-Pentanone	10.328	43	5187	7.328	ug/l	92
53) t-1,3-Dichloropropene	10.719	75	83	1.953	ug/l #	43
56) Ethyl methacrylate	10.762	69	5350	2.526	ug/l	94
59) 2-Hexanone	11.095	43	4335	9.006	ug/l	80
60) Dibromochloromethane	10.982	129	50	1.988	ug/l #	10
70) Styrene	12.296	104	623	1.506	ug/l #	70
71) Bromoform	12.733	173	705	3.090	ug/l #	1
76) 1,2,3-Trichloropropane	12.733	75	125922	23.881	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.733	75	125922	68.590	ug/l #	12
83) tert-Butylbenzene	13.323	119	70944	5.812	ug/l	97
88) 1,4-Dichlorobenzene	13.694	146	1463	0.292	ug/l #	1
89) n-Butylbenzene	13.943	91	3100	0.271	ug/l	93
90) Hexachloroethane	14.324	117	2420	2.901	ug/l #	12
92) 1,2-Dibromo-3-Chloropr...	14.321	75	303	1.921	ug/l #	5
93) 1,2,4-Trichlorobenzene	15.268	180	1650	2.969	ug/l	89
95) Naphthalene	15.507	128	8594	4.109	ug/l	96
96) 1,2,3-Trichlorobenzene	15.702	180	1749	2.732	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110221\
Data File : VN069341.D
Acq On : 2 Nov 2021 12:08
Operator : JC/MD
Sample : M4438-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Nov 03 00:47:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 28 16:09:15 2021
Response via : Initial Calibration

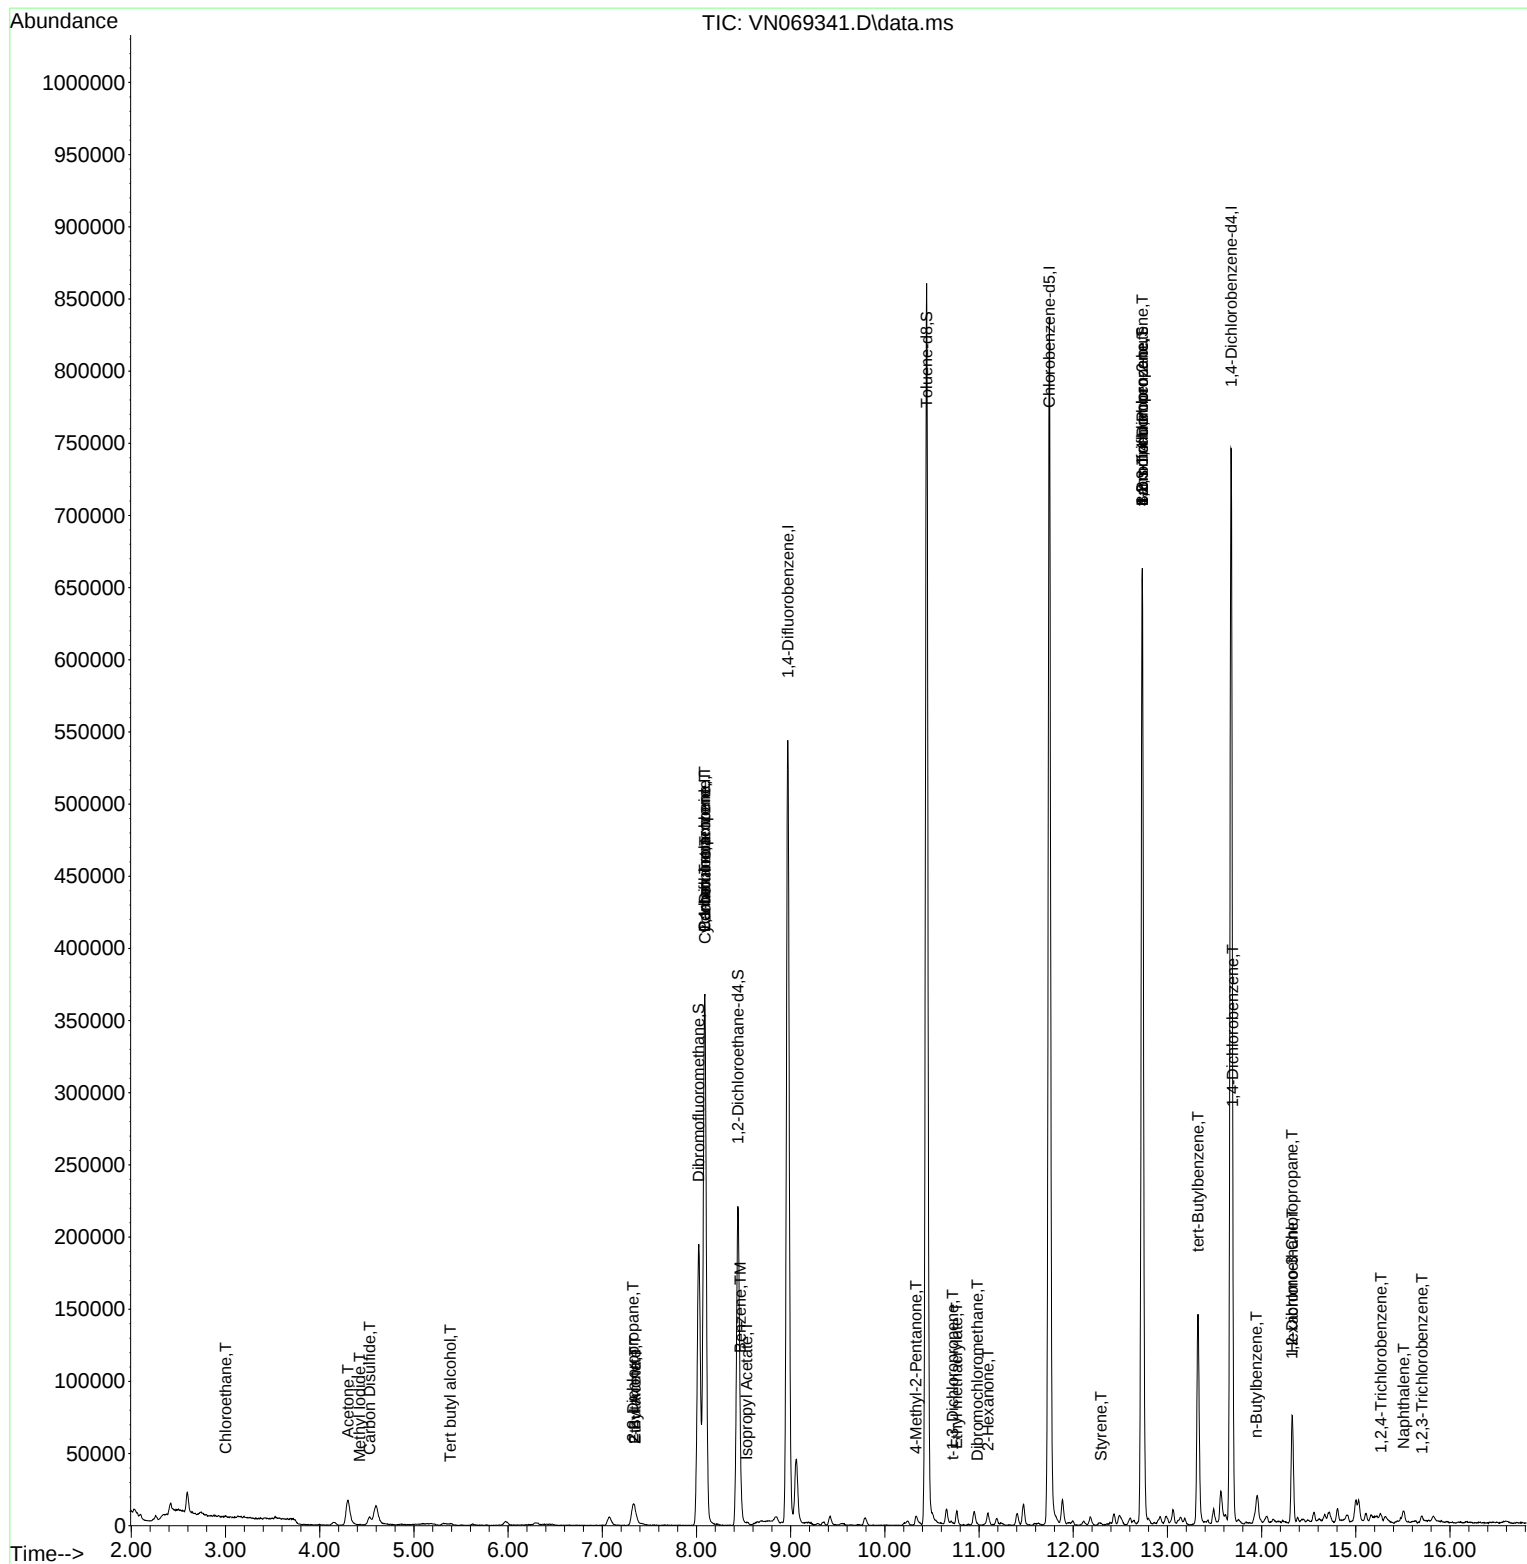



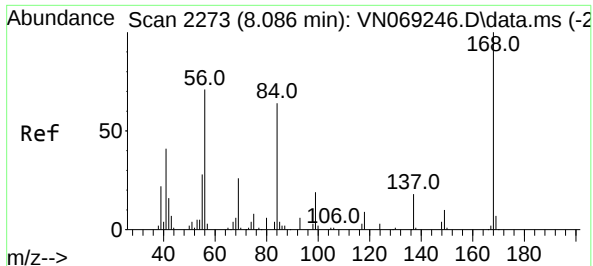


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

Instrument :
MSVOA_N
ClientSampleId :



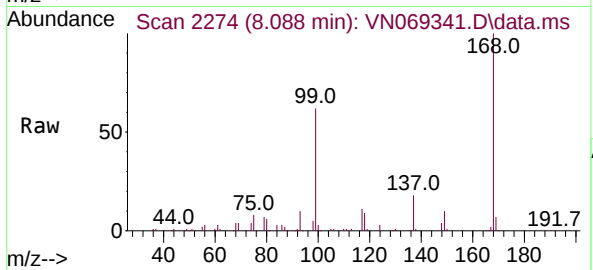



Tgt Ion:168 Resp: 276962
Ion Ratio Lower Upper
168 100
99 61.9 48.9 73.3

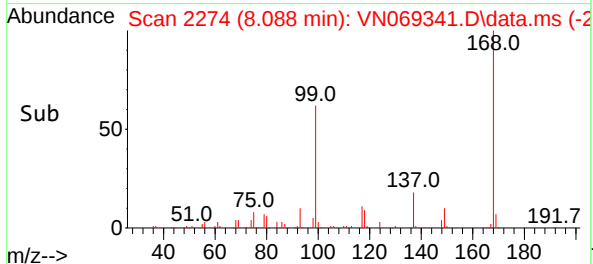

#3
Chloromethane
Concen: Below Cal
RT: 2.309 min Scan# 119
Delta R.T. 0.008 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

Tgt Ion: 50 Resp: 450
Ion Ratio Lower Upper
50 100
52 41.6 26.3 39.5#


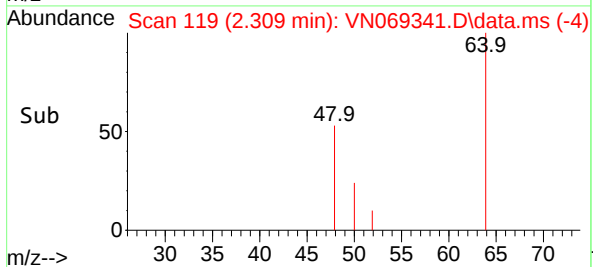

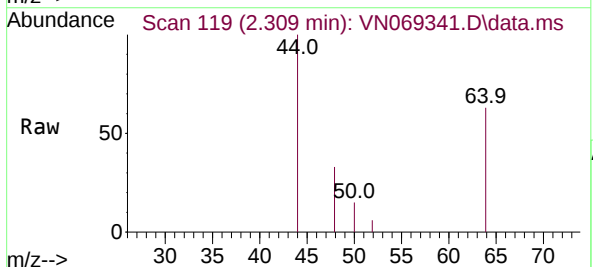




#6
Chloroethane
Concen: 0.212 ug/l
RT: 3.003 min Scan# 31
Delta R.T. 0.000 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 64 Resp: 512
Ion Ratio Lower Upper
64 100
66 0.0 25.6 38.4#

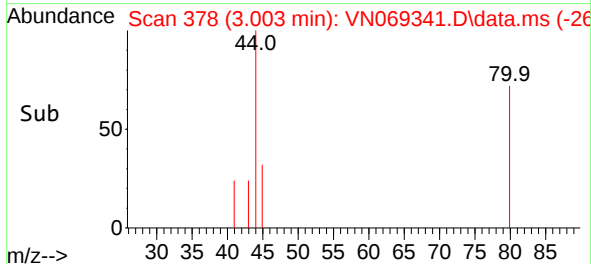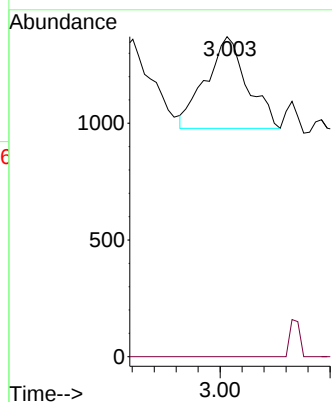

#10
Methyl Iodide
Concen: 2.473 ug/l
RT: 4.422 min Scan# 907
Delta R.T. -0.000 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

Tgt Ion: 142 Resp: 55
Ion Ratio Lower Upper
142 100
127 0.0 34.4 51.6#
141 0.0 11.3 16.9#


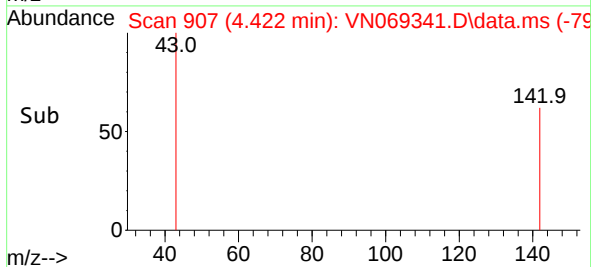

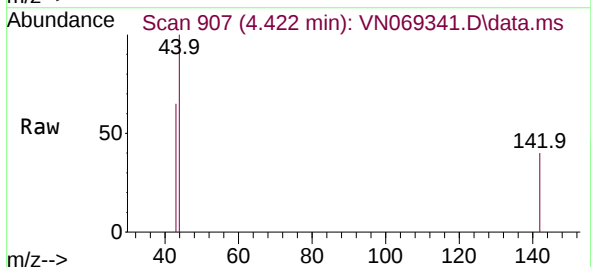




#11
Tert butyl alcohol
Concen: 14.428 ug/l
RT: 5.385 min Scan# 11
Delta R.T. 0.022 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 59 Resp: 838
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

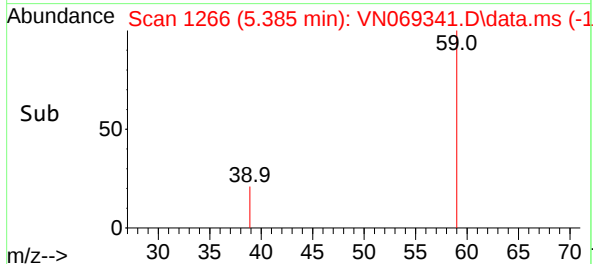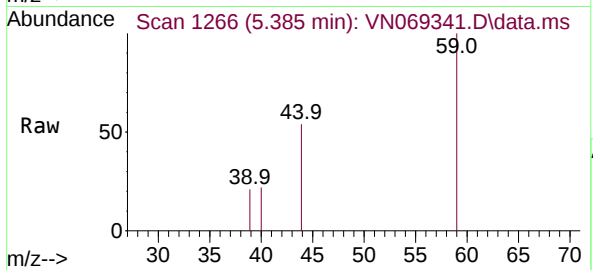

#16
Acetone
Concen: 19.902 ug/l
RT: 4.299 min Scan# 861
Delta R.T. 0.016 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08


Tgt Ion: 43 Resp: 33901
Ion Ratio Lower Upper
43 100
58 32.4 24.5 36.7

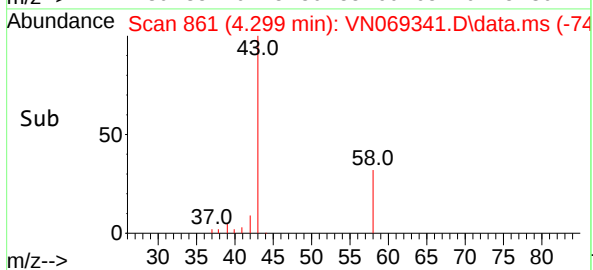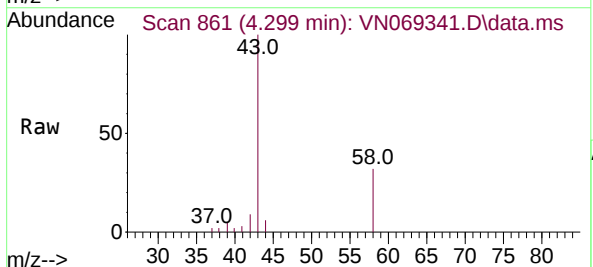



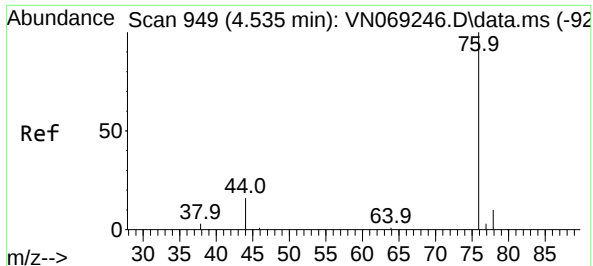


#17
Carbon Disulfide
Concen: 1.945 ug/l
RT: 4.529 min Scan# 949
Delta R.T. -0.006 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

Instrument :
MSVOA_N
ClientSampleId :



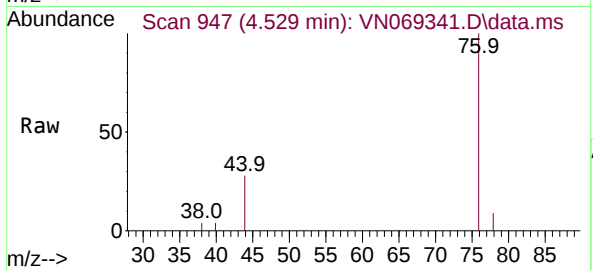



Tgt Ion: 76 Resp: 12904
Ion Ratio Lower Upper
76 100
78 9.4 7.2 10.8

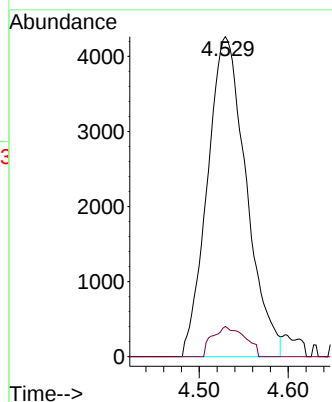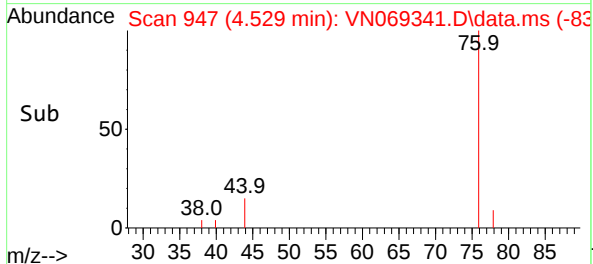

#25
2-Butanone
Concen: 5.166 ug/l
RT: 7.345 min Scan# 1997
Delta R.T. 0.010 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

Tgt Ion: 43 Resp: 9280
Ion Ratio Lower Upper
43 100
72 23.9 21.2 31.8

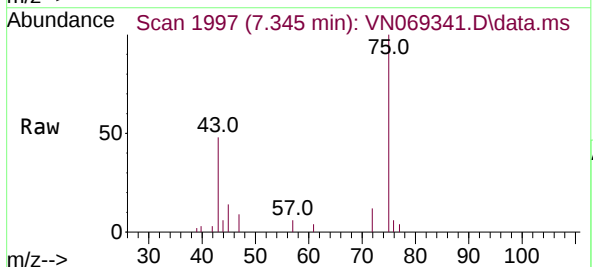



#26

2,2-Dichloropropane

Concen: 1.003 ug/l

RT: 7.327 min Scan# 1990

Delta R.T. -0.000 min

Lab File: VN069341.D

Acq: 2 Nov 2021 12:08

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 77 Resp: 867

Ion Ratio Lower Upper

77 100

97 0.0 11.2 33.6#

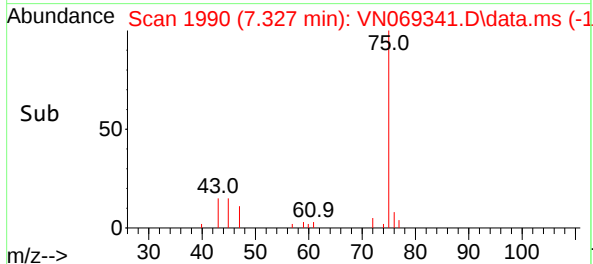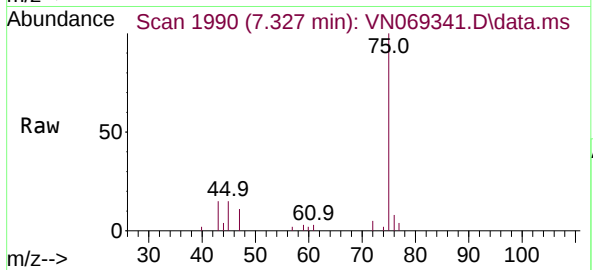

#31

Cyclohexane

Concen: 1.213 ug/l

RT: 8.091 min Scan# 2275

Delta R.T. -0.005 min

Lab File: VN069341.D

Acq: 2 Nov 2021 12:08




Tgt Ion: 56 Resp: 6491


Ion Ratio Lower Upper

56 100

69 150.4 26.9 40.3#

84 107.4 67.6 101.4#


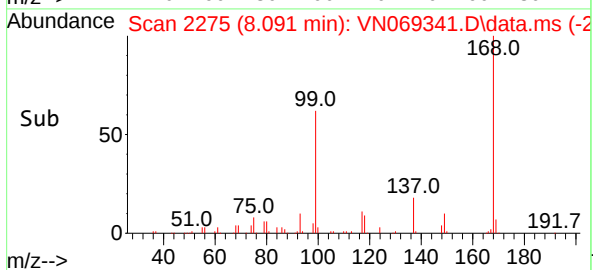

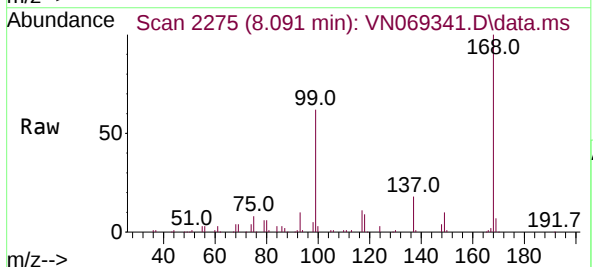


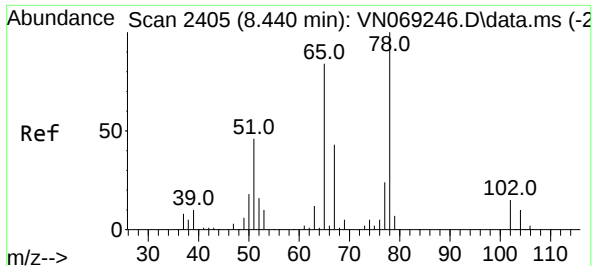

#33
 1,2-Dichloroethane-d4
 Concen: 47.405 ug/l
 RT: 8.440 min Scan# 2405
 Delta R.T. -0.000 min
 Lab File: VN069341.D
 Acq: 2 Nov 2021 12:08




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 65 Resp: 189529
 Ion Ratio Lower Upper
 65 100
 67 51.8 0.0 103.8

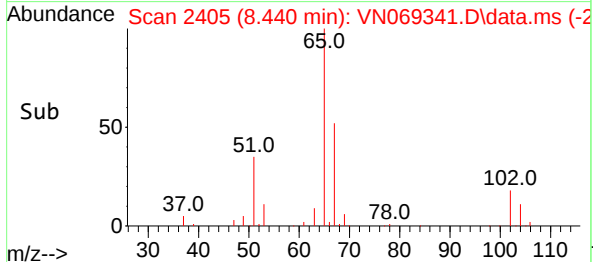

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.971 min Scan# 2603
 Delta R.T. 0.003 min
 Lab File: VN069341.D
 Acq: 2 Nov 2021 12:08


Tgt Ion: 114 Resp: 489420
 Ion Ratio Lower Upper
 114 100
 63 21.2 0.0 42.6
 88 16.1 0.0 32.0

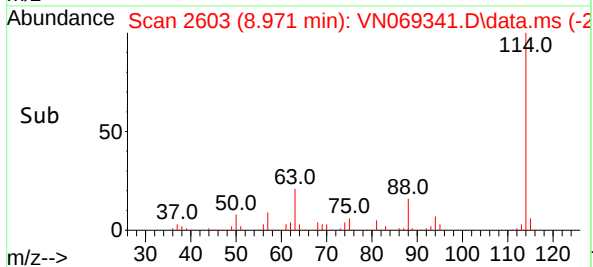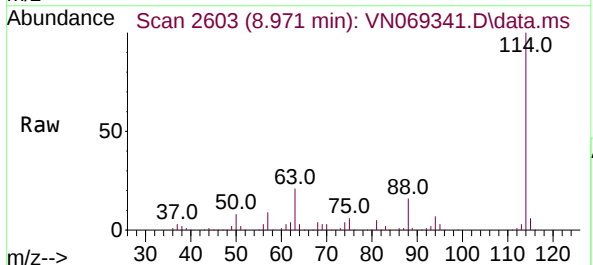






#35
Dibromofluoromethane
Concen: 47.308 ug/l
RT: 8.024 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

Instrument :
MSVOA_N
ClientSampleId :



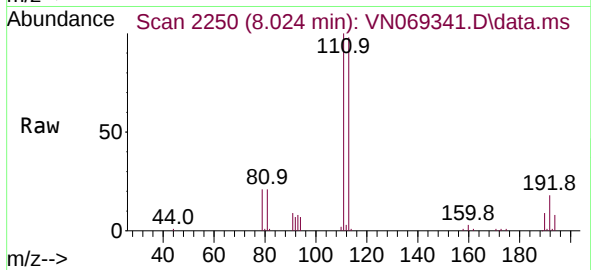



Tgt Ion:113 Resp: 144330
Ion Ratio Lower Upper
113 100
111 101.8 83.2 124.8
192 18.1 15.0 22.4

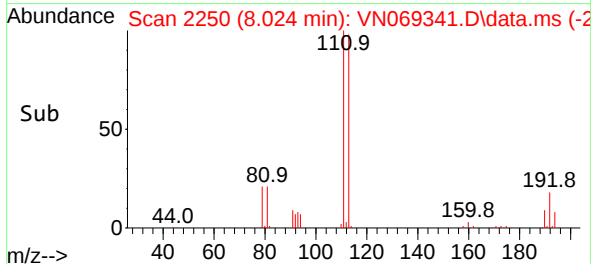

#36
1,1-Dichloropropene
Concen: 5.451 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

Tgt Ion: 75 Resp: 23001
Ion Ratio Lower Upper
75 100
110 9.8 17.9 53.8#
77 0.0 24.7 37.1#

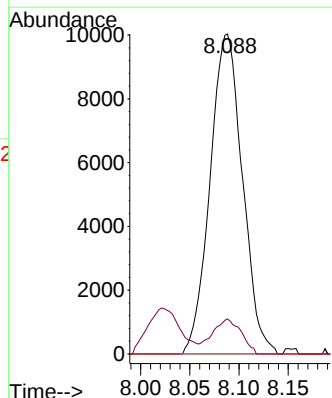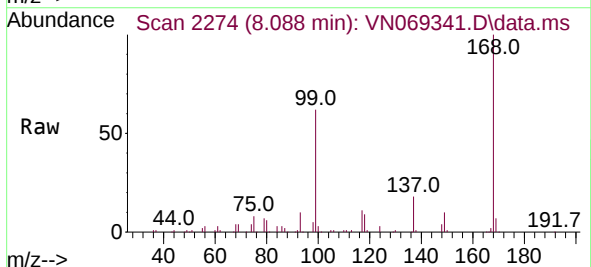

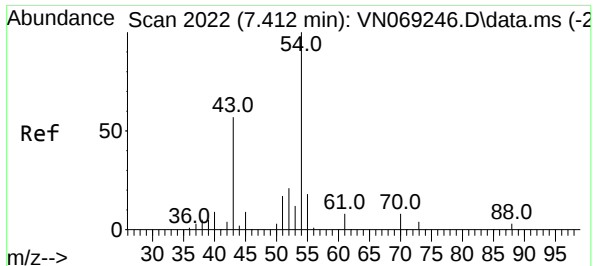

#37

Ethyl Acetate

Concen: 1.930 ug/l

RT: 7.345 min Scan# 19

Delta R.T. -0.067 min


Lab File: VN069341.D

Acq: 2 Nov 2021 12:08




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion: 43	Resp:	9280
Ion	Ratio	Lower Upper
43	100	
61	4.6	11.2 16.8#
70	0.0	8.4 12.6#

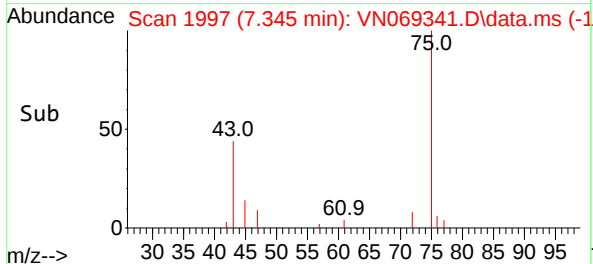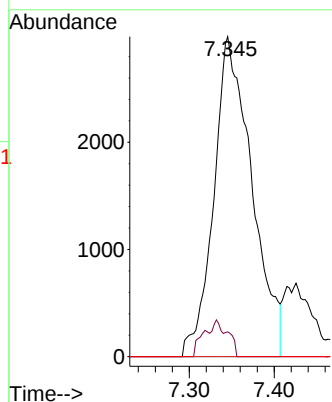

#38

Carbon Tetrachloride

Concen: 6.782 ug/l




RT: 8.088 min Scan# 2274


Delta R.T. -0.118 min

Lab File: VN069341.D

Acq: 2 Nov 2021 12:08

Tgt Ion: 117	Resp:	28268
Ion	Ratio	Lower Upper
117	100	
119	4.7	76.9 115.3#
121	0.0	24.6 37.0#


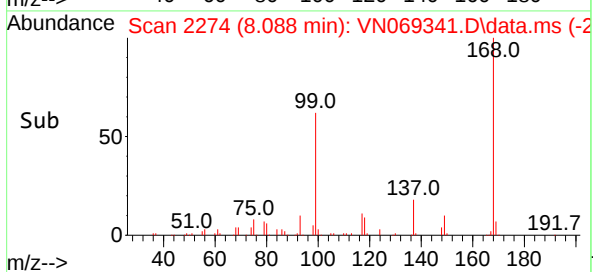

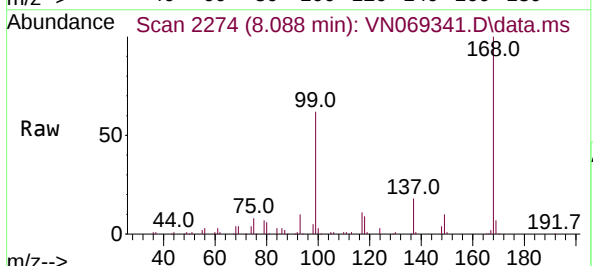




#40
Benzene
Concen: 0.522 ug/l
RT: 8.464 min Scan# 2413
Delta R.T. 0.003 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 78 Resp: 6625
Ion Ratio Lower Upper
78 100
77 26.5 19.1 28.7

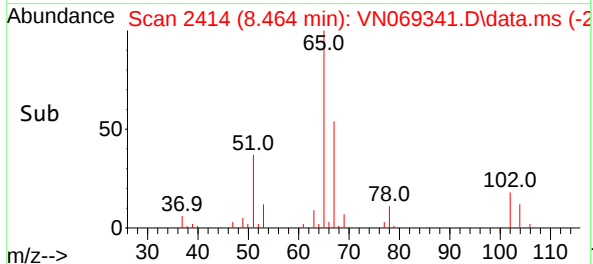

#43
Isopropyl Acetate
Concen: 0.478 ug/l
RT: 8.533 min Scan# 2440
Delta R.T. -0.027 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

Tgt Ion: 43 Resp: 166
Ion Ratio Lower Upper
43 100
61 0.0 20.4 30.6#
87 0.0 10.7 16.1#


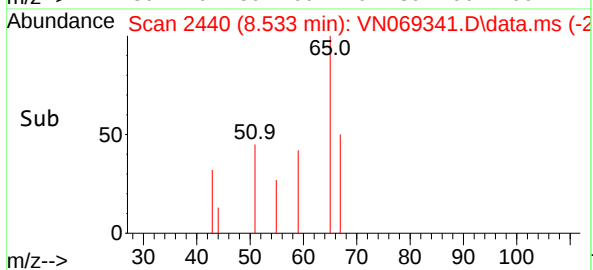

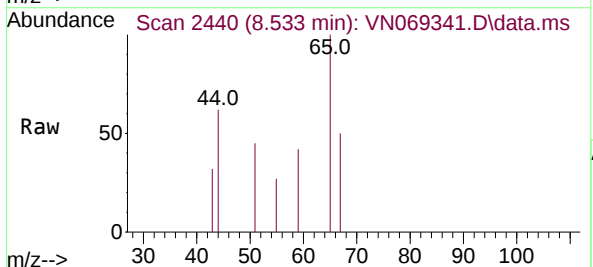




#50
Toluene-d8
Concen: 50.509 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 616119
Ion Ratio Lower Upper
98 100
100 64.0 51.5 77.3

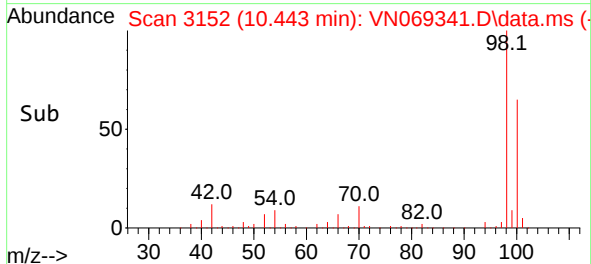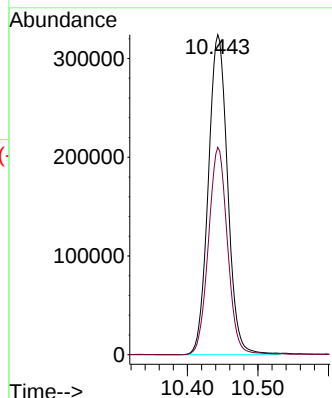

#51
4-Methyl-2-Pentanone
Concen: 7.328 ug/l
RT: 10.328 min Scan# 3109
Delta R.T. -0.002 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

Tgt Ion: 43 Resp: 5187
Ion Ratio Lower Upper
43 100
58 34.1 31.0 46.4



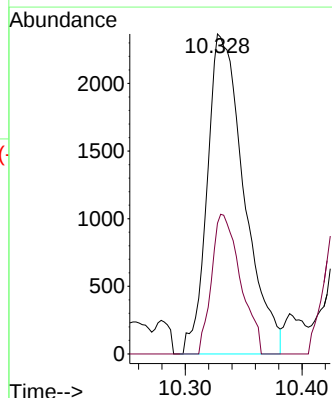
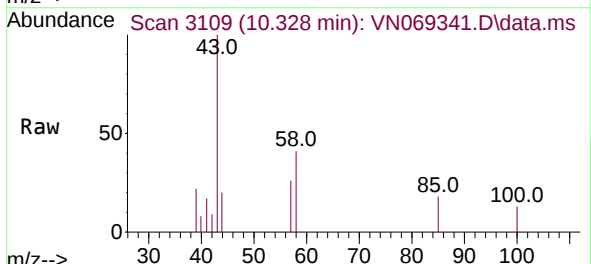




#53
t-1,3-Dichloropropene
Concen: 1.953 ug/l
RT: 10.719 min Scan# 31
Delta R.T. 0.000 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 83
Ion Ratio Lower Upper
75 100
77 0.0 25.4 38.2#

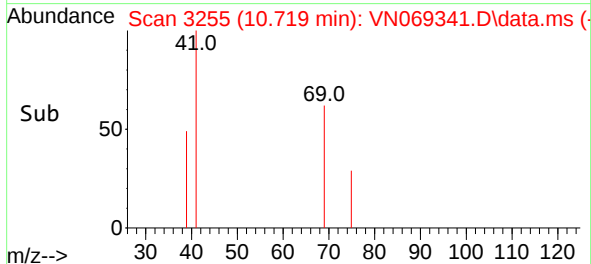

#56
Ethyl methacrylate
Concen: 2.526 ug/l
RT: 10.762 min Scan# 3271
Delta R.T. 0.000 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

Tgt Ion: 69 Resp: 5350
Ion Ratio Lower Upper
69 100
41 71.0 53.3 79.9
39 46.3 33.3 49.9


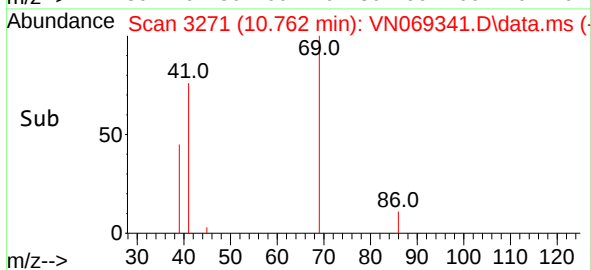

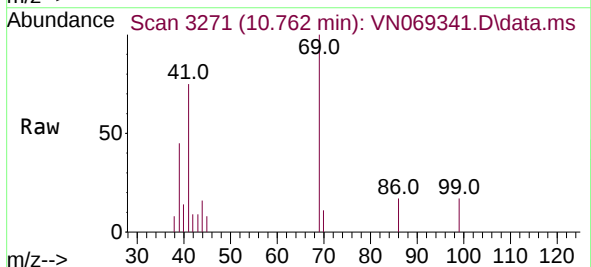




#59
2-Hexanone
Concen: 9.006 ug/l
RT: 11.095 min Scan# 31
Delta R.T. 0.008 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 4335
Ion Ratio Lower Upper
43 100
58 39.2 26.9 80.7

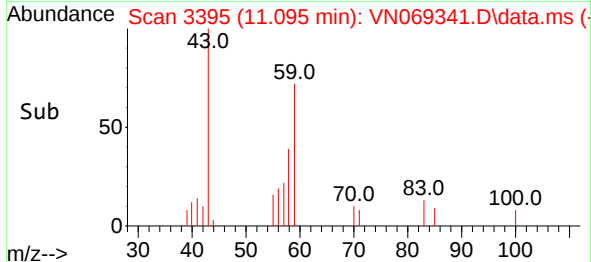

#60
Dibromochloromethane
Concen: 1.988 ug/l
RT: 10.982 min Scan# 3353
Delta R.T. -0.258 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

Tgt Ion:129 Resp: 50
Ion Ratio Lower Upper
129 100
127 0.0 39.1 117.2#


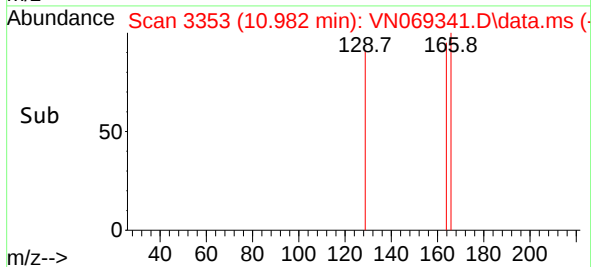

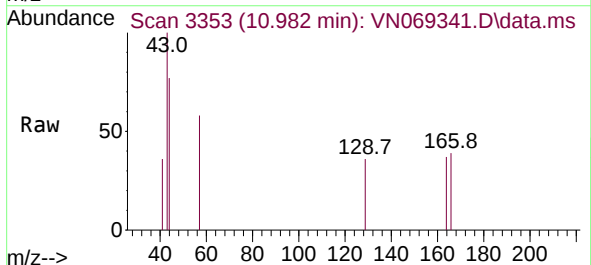




#62
4-Bromofluorobenzene
Concen: 51.652 ug/l
RT: 12.733 min Scan# 4005
Delta R.T. 0.002 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 237759
Ion Ratio Lower Upper
95 100
174 75.2 0.0 144.8
176 72.5 0.0 140.0

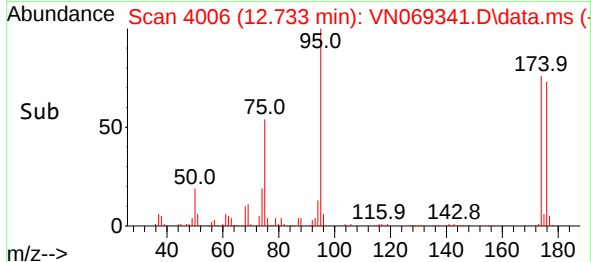

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. -0.000 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08


Tgt Ion: 117 Resp: 494386
Ion Ratio Lower Upper
117 100
82 55.6 46.4 69.6
119 32.3 26.0 39.0

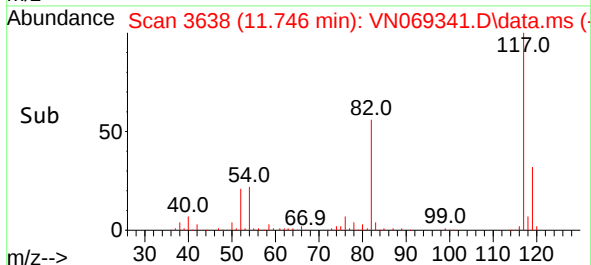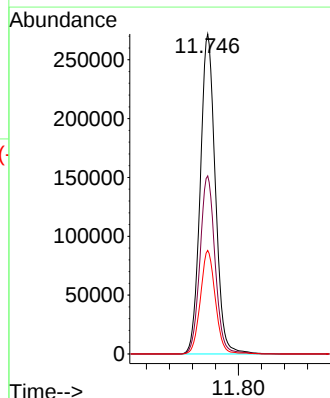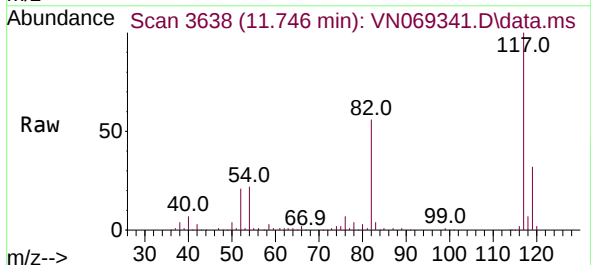






#70
Styrene
Concen: 1.506 ug/l
RT: 12.296 min Scan# 3843
Delta R.T. 0.000 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:104 Resp: 623
Ion Ratio Lower Upper
104 100
78 36.0 42.2 63.4#
103 30.0 44.4 66.6#

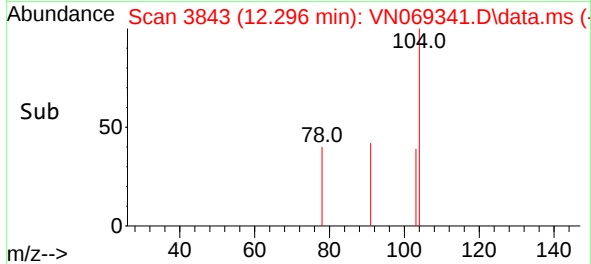

#71
Bromoform
Concen: 3.090 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.273 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

Tgt Ion:173 Resp: 705
Ion Ratio Lower Upper
173 100
175 1765.5 23.8 71.5#
254 0.0 0.0 0.0



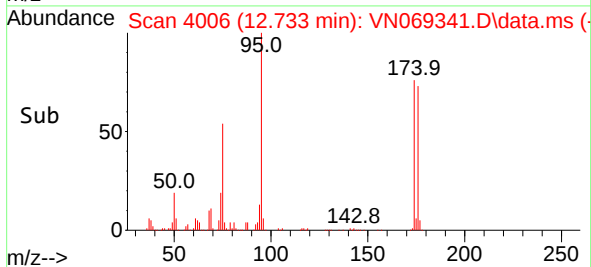
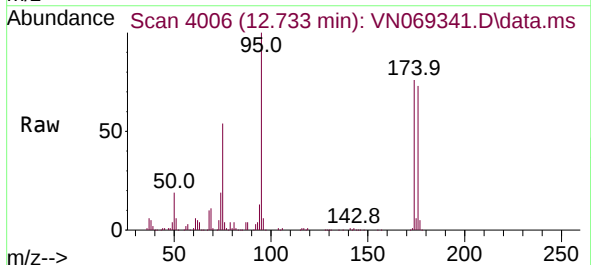


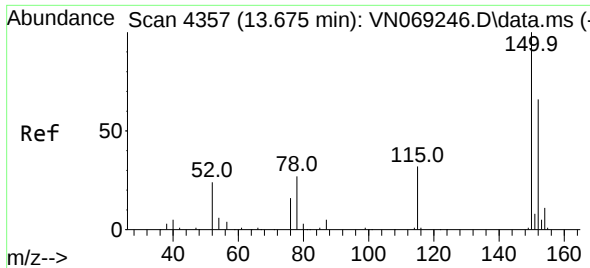

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.677 min Scan# 41
 Delta R.T. 0.002 min
 Lab File: VN069341.D
 Acq: 2 Nov 2021 12:08




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:152 Resp: 200479
 Ion Ratio Lower Upper
 152 100
 115 63.2 31.4 94.3
 150 158.5 0.0 351.0

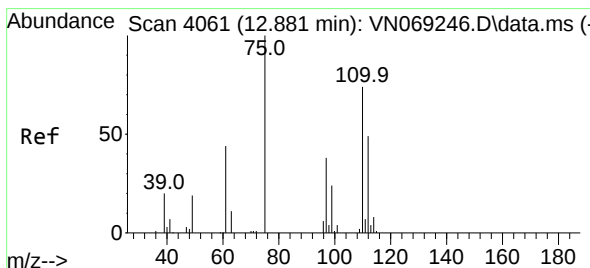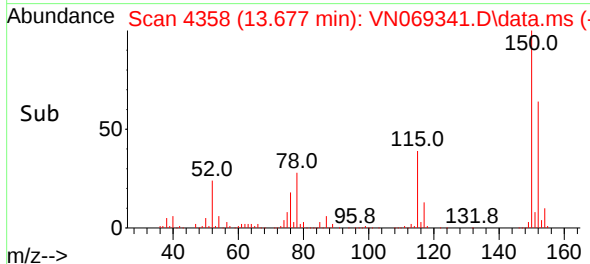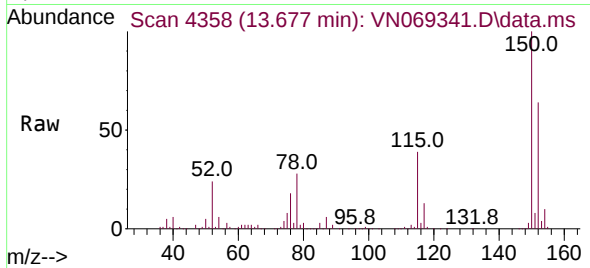

#76
 1,2,3-Trichloropropane
 Concen: 23.881 ug/l
 RT: 12.733 min Scan# 4006
 Delta R.T. -0.148 min
 Lab File: VN069341.D
 Acq: 2 Nov 2021 12:08


Tgt Ion: 75 Resp: 125922
 Ion Ratio Lower Upper
 75 100
 77 1.0 96.2 288.4#

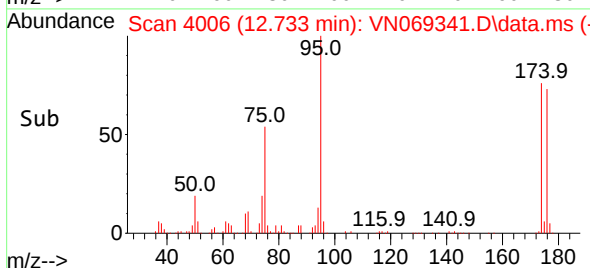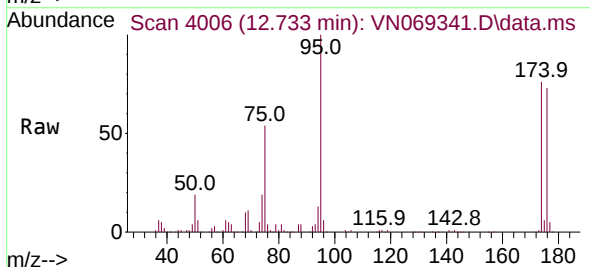






#81
trans-1,4-Dichloro-2-butene
Concen: 68.590 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.107 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08


Instrument :
MSVOA_N
ClientSampleId :

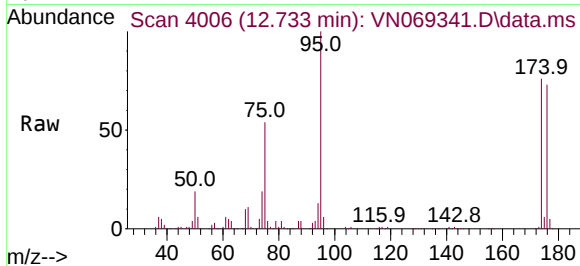



Tgt Ion: 75 Resp: 125922
Ion Ratio Lower Upper
75 100
53 0.0 75.4 113.2#
89 0.0 36.9 55.3#

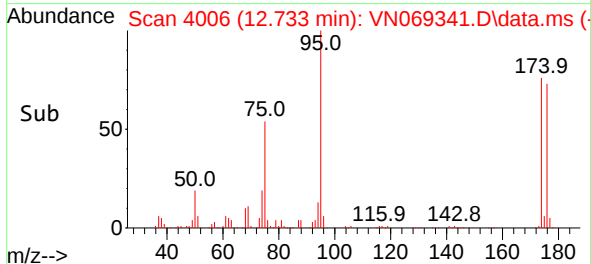


#83
tert-Butylbenzene
Concen: 5.812 ug/l
RT: 13.323 min Scan# 4226
Delta R.T. -0.003 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

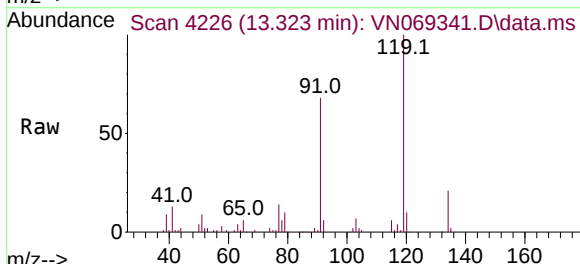


Tgt Ion: 119 Resp: 70944
Ion Ratio Lower Upper
119 100
91 71.2 34.6 103.9
134 23.1 12.6 37.6

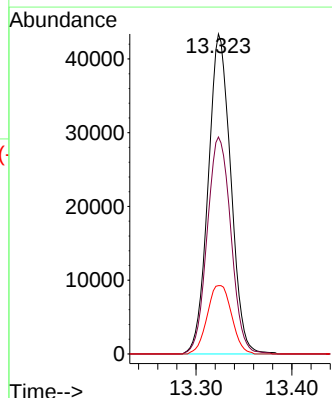






#88
1,4-Dichlorobenzene
Concen: 0.292 ug/l
RT: 13.694 min Scan# 411
Delta R.T. -0.002 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08


Instrument :
MSVOA_N
ClientSampleId :

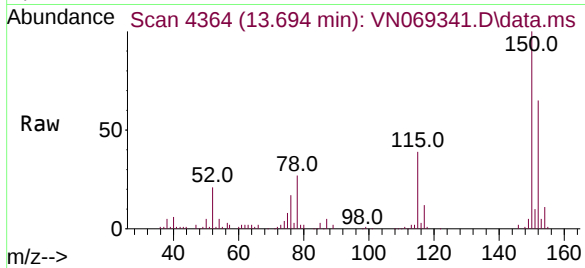



Tgt Ion:146 Resp: 1463
Ion Ratio Lower Upper
146 100
111 233.9 20.6 61.8#
148 125.6 32.1 96.5#

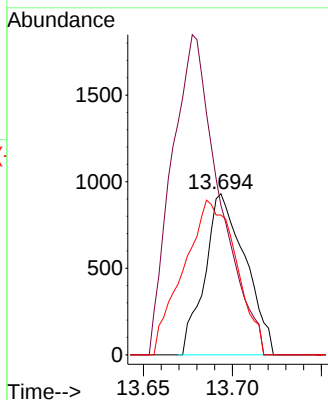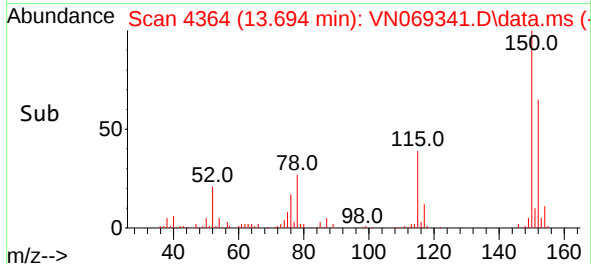


#89
n-Butylbenzene
Concen: 0.271 ug/l
RT: 13.943 min Scan# 4457
Delta R.T. -0.000 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

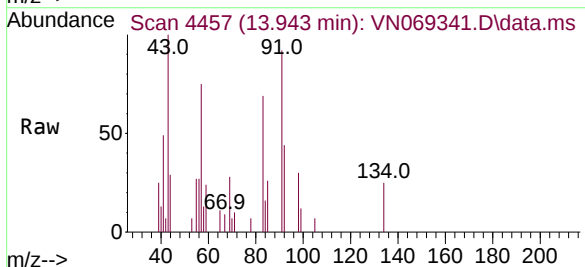

Tgt Ion: 91 Resp: 3100
Ion Ratio Lower Upper
91 100
92 44.6 26.0 78.0
134 24.8 12.5 37.5



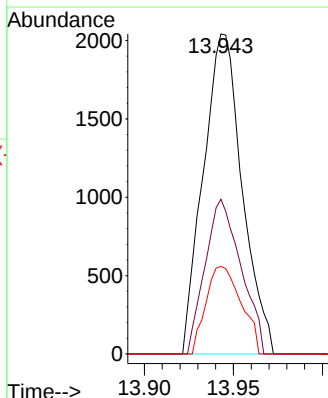





#90
Hexachloroethane
Concen: 2.901 ug/l
RT: 14.324 min Scan# 41
Delta R.T. 0.113 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 2420
Ion Ratio Lower Upper
117 100
201 0.0 37.1 111.5#

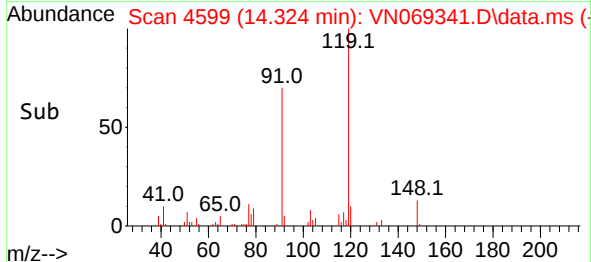

#92
1,2-Dibromo-3-Chloropropane
Concen: 1.921 ug/l
RT: 14.321 min Scan# 4598
Delta R.T. -0.284 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08


Tgt Ion: 75 Resp: 303
Ion Ratio Lower Upper
75 100
155 0.0 38.8 116.4#
157 0.0 50.2 150.6#

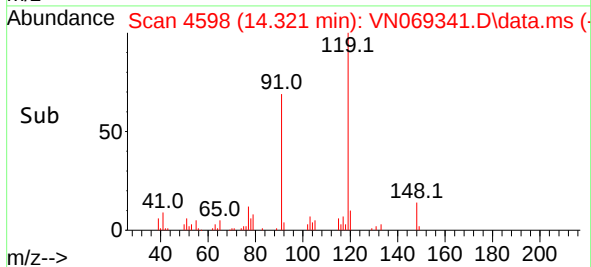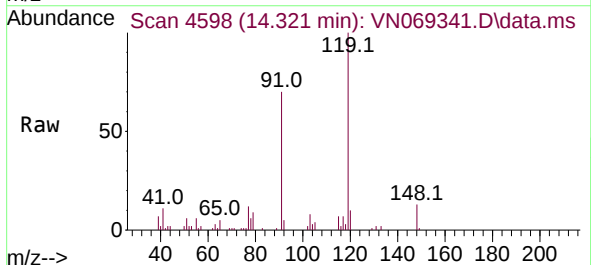






#93
1,2,4-Trichlorobenzene
Concen: 2.969 ug/l
RT: 15.268 min Scan# 4950
Delta R.T. 0.003 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:180 Resp: 1650
Ion Ratio Lower Upper
180 100
182 102.3 47.9 143.7
145 20.1 16.4 49.2

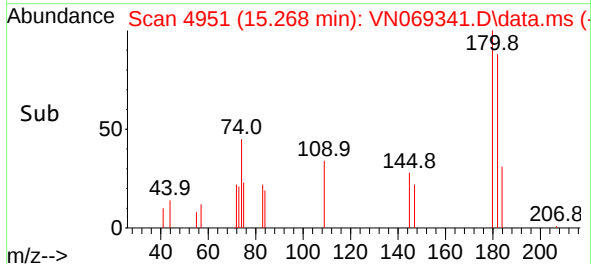


#95
Naphthalene
Concen: 4.109 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN069341.D
Acq: 2 Nov 2021 12:08

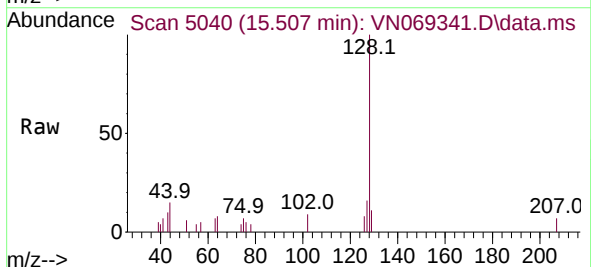


Tgt Ion:128 Resp: 8594
Ion Ratio Lower Upper
128 100
127 14.7 10.5 15.7
129 9.2 8.9 13.3

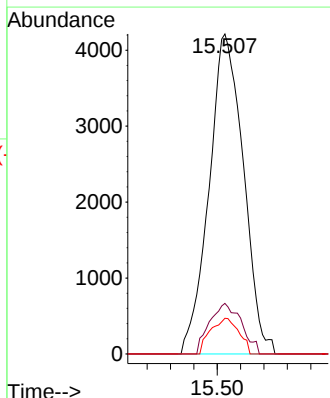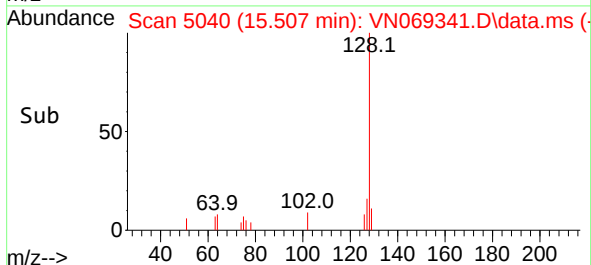



#96
 1,2,3-Trichlorobenzene
 Concen: 2.732 ug/l
 RT: 15.702 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: VN069341.D
 Acq: 2 Nov 2021 12:08

Instrument :
 MSVOA_N
 ClientSampleId :

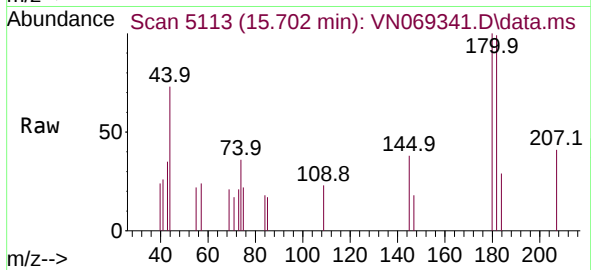

Tgt Ion:	180	Resp:	1749
Ion	Ratio	Lower	Upper
180	100		
182	98.6	48.1	144.3
145	21.3	17.4	52.2

