

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110221\
 Data File : VN069342.D
 Acq On : 2 Nov 2021 12:33
 Operator : JC/MD
 Sample : M4438-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FDR-20211101-WC-LM

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
 Title : SW846 8260

Signal : TIC: VN069342.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.593	215	225	243	rVB2	12848	23046	1.30%	0.226%
2	4.299	843	861	886	rBV	13734	40318	2.27%	0.396%
3	7.340	1972	1995	2012	rBV4	10013	31797	1.79%	0.312%
4	8.024	2228	2250	2261	rBV2	212334	504088	28.33%	4.951%
5	8.086	2261	2273	2303	rVB2	392674	913995	51.36%	8.977%
6	8.440	2384	2405	2435	rBV	234714	560625	31.50%	5.506%
7	8.968	2582	2602	2622	rBV	592076	1236732	69.50%	12.146%
8	9.059	2624	2636	2657	rVB3	36461	83714	4.70%	0.822%
9	10.443	3133	3152	3191	rBV	931773	1779587	100.00%	17.478%
10	10.762	3262	3271	3288	rVB2	11095	19646	1.10%	0.193%
11	11.470	3524	3535	3552	rVB2	14843	26673	1.50%	0.262%
12	11.747	3615	3638	3676	rBV	918358	1682696	94.56%	16.526%
13	11.886	3679	3690	3707	rVB4	13683	24812	1.39%	0.244%
14	12.734	3990	4006	4029	rBV	735691	1286025	72.27%	12.631%
15	13.324	4206	4226	4245	rBV	146517	254409	14.30%	2.499%
16	13.568	4302	4317	4330	rBV3	17929	34855	1.96%	0.342%
17	13.675	4342	4357	4380	rBV	843509	1473143	82.78%	14.468%
18	13.954	4440	4461	4478	rBV6	16690	39537	2.22%	0.388%
19	14.327	4587	4600	4613	rBV	74921	123831	6.96%	1.216%
20	14.804	4764	4778	4790	rBV2	11299	18836	1.06%	0.185%
21	15.002	4839	4852	4855	rBV9	15075	23522	1.32%	0.231%


Sum of corrected areas: 10181887

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110221\
Data File : VN069342.D
Acq On : 2 Nov 2021 12:33
Operator : JC/MD
Sample : M4438-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FDR-20211101-WC-LM

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

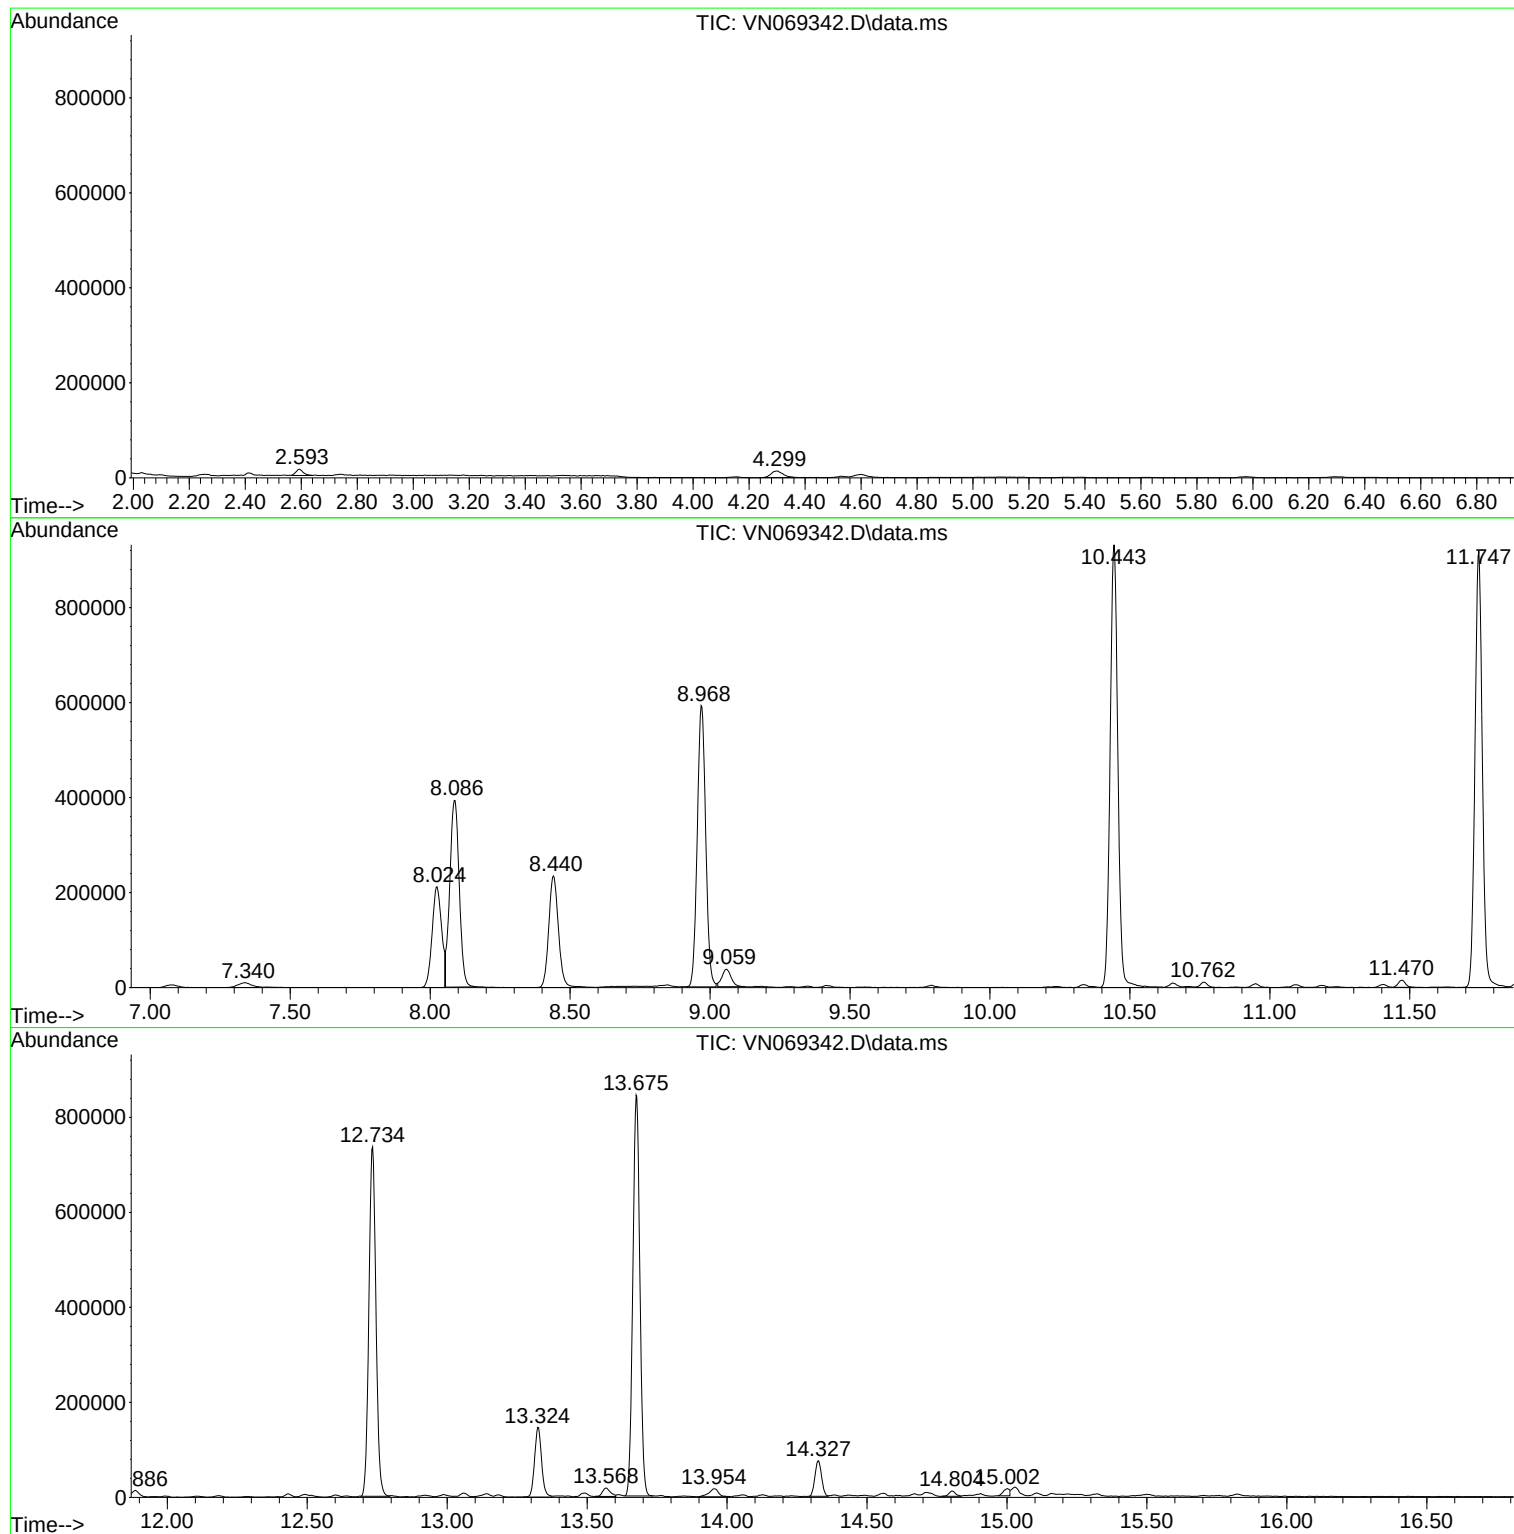

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110221\
Data File : VN069342.D
Acq On : 2 Nov 2021 12:33
Operator : JC/MD
Sample : M4438-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FDR-20211101-WC-LM

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110221\
Data File : VN069342.D
Acq On : 2 Nov 2021 12:33
Operator : JC/MD
Sample : M4438-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FDR-20211101-WC-LM

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102821W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc