
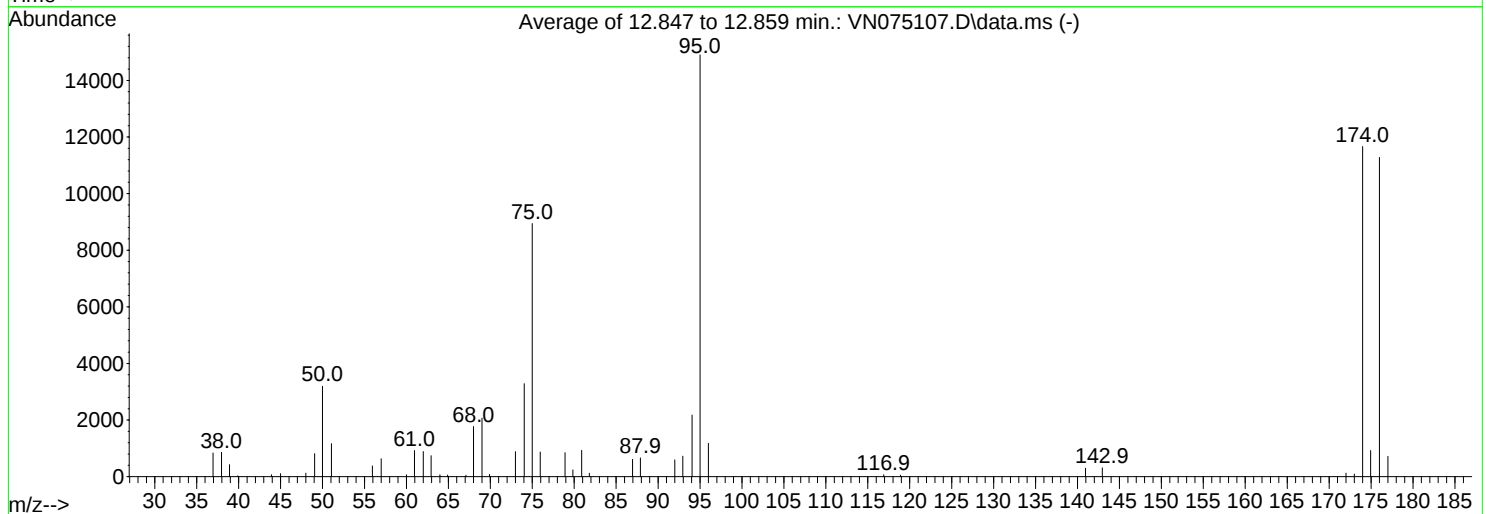


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110222\
Data File : VN075107.D
Acq On : 02 Nov 2022 10:45
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 09:48:49 2022

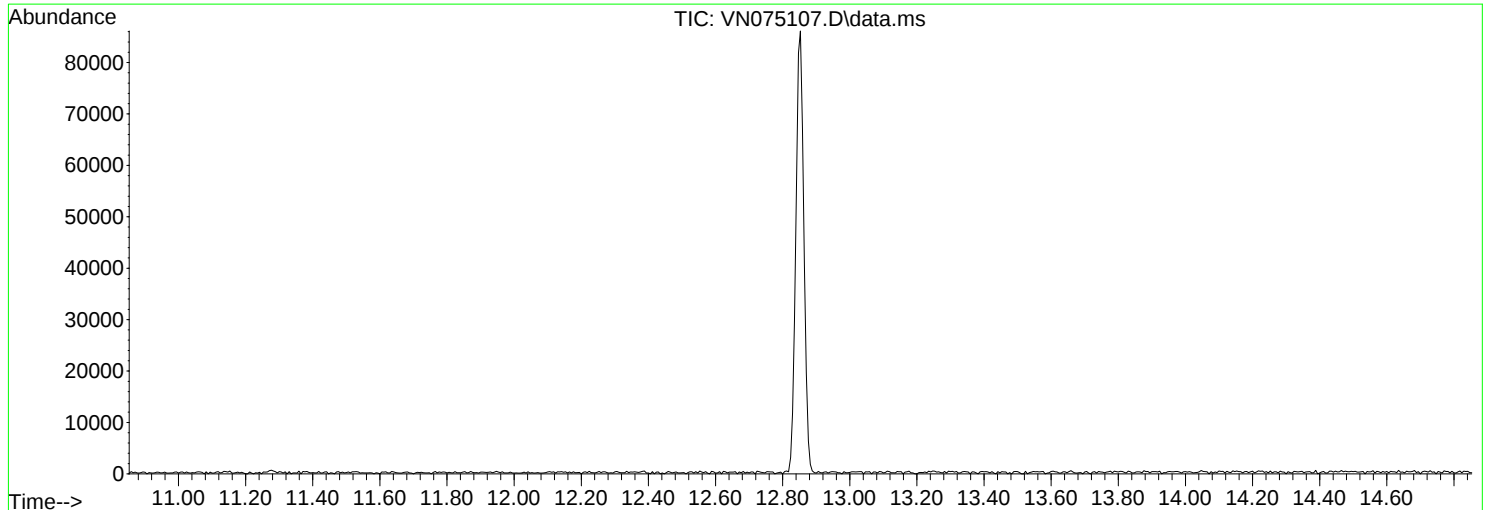

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	3194	PASS
75	95	30	60	60.0	8942	PASS
95	95	100	100	100.0	14904	PASS
96	95	5	9	7.9	1175	PASS
173	174	0.00	2	0.8	91	PASS
174	95	50	100	78.2	11661	PASS
175	174	5	9	7.9	921	PASS
176	174	95	101	96.7	11277	PASS
177	176	5	9	6.4	717	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.95	837	57.00	635	73.00	883	92.95	724
37.95	857	60.00	70	74.05	3286	94.05	217
38.90	425	60.95	924	75.00	8942	95.00	1490
39.90	29	62.00	885	75.95	871	96.00	117
43.90	69	62.95	742	78.90	849	116.90	70
45.00	106	64.00	66	79.85	240	118.90	51
48.00	123	64.90	55	80.90	925	140.95	298
49.05	816	67.10	51	81.80	120	142.95	313
50.00	3194	68.00	1770	86.95	608	172.00	126
51.05	1165	69.00	2071	87.90	662	173.00	91
55.95	381	69.90	82	92.00	592	174.00	11661

Average of 12.847 to 12.859 min.: VN075107.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.95	921						
176.00	11277						
177.00	717						

Instrument :

MSVOA_N

ClientSampleId :

BFB