

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110223\
 Data File : VN079820.D
 Acq On : 03 Nov 2023 03:11
 Operator : JC\MD
 Sample : 05222-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 03 05:35:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 02 05:49:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.229	168	230769	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	449923	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	461734	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	176666	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	200082	56.909	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 113.820%	
35) Dibromofluoromethane	8.171	113	171161	53.750	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 107.500%	
50) Toluene-d8	10.570	98	593091	50.593	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 101.180%	
62) 4-Bromofluorobenzene	12.853	95	195312	50.236	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 100.480%	


Target Compounds			Qvalue			
3) Chloromethane	2.359	50	1183	Below Cal	#	86
5) Bromomethane	2.959	94	1046	0.473	ug/l	92
10) Methyl Iodide	4.606	142	1199	0.400	ug/l #	80
13) Acrolein	4.206	56	55	2.709	ug/l #	16
16) Acetone	4.441	43	997	0.807	ug/l #	84
31) Cyclohexane	8.229	56	6384	1.374	ug/l #	53
36) 1,1-Dichloropropene	8.229	75	21494	4.727	ug/l #	47
38) Carbon Tetrachloride	8.229	117	24709	5.392	ug/l #	17
44) Trichloroethene	9.353	130	1713	0.507	ug/l	63
52) Toluene	10.629	92	2142	0.265	ug/l	99
71) Bromoform	12.853	173	1549	0.605	ug/l #	1
76) 1,2,3-Trichloropropane	12.853	75	107009	25.800	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	107009	70.196	ug/l #	15
93) 1,2,4-Trichlorobenzene	15.411	180	857	0.313	ug/l #	69
94) Hexachlorobutadiene	15.500	225	314	0.253	ug/l	71
95) Naphthalene	15.641	128	3501	0.377	ug/l #	94
96) 1,2,3-Trichlorobenzene	15.841	180	690	0.257	ug/l #	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110223\
Data File : VN079820.D
Acq On : 03 Nov 2023 03:11
Operator : JC\MD
Sample : 05222-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Nov 03 05:35:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 02 05:49:08 2023
Response via : Initial Calibration

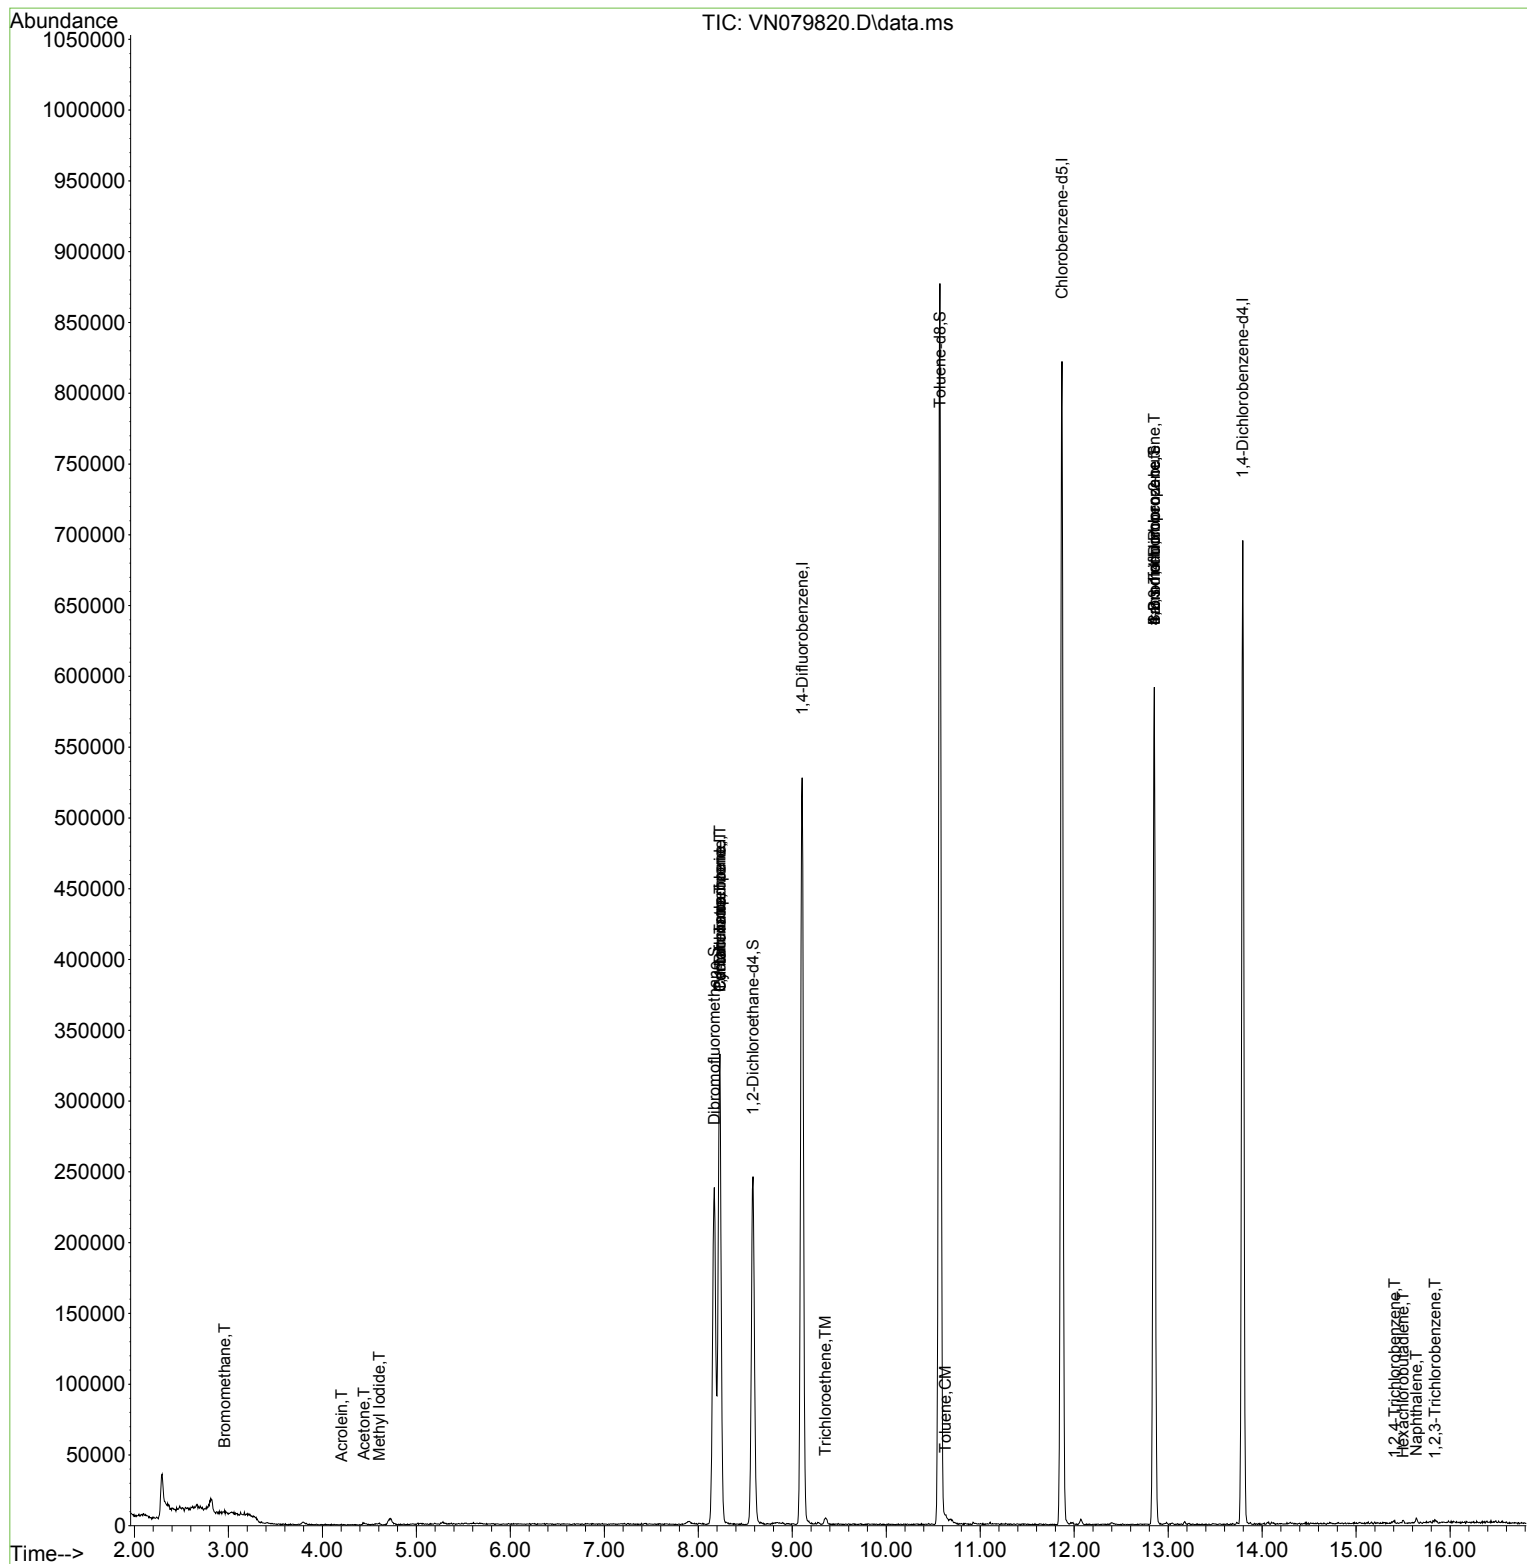






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. 0.000 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11

Instrument :
MSVOA_N
ClientSampleId :






Tgt Ion:168 Resp: 230769
Ion Ratio Lower Upper
168 100
99 57.9 53.0 79.6

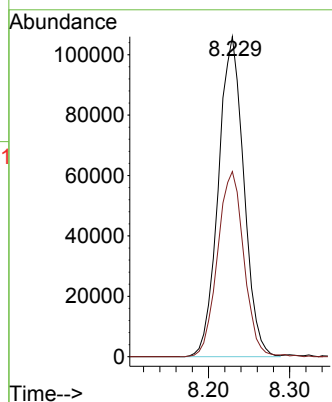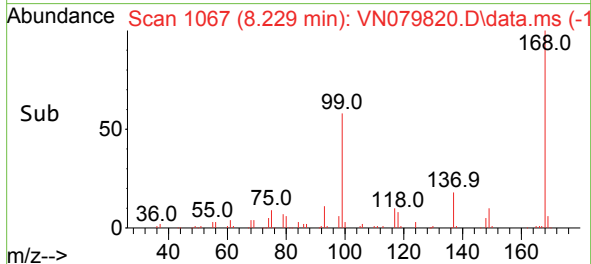

#3
Chloromethane
Concen: Below Cal
RT: 2.359 min Scan# 69
Delta R.T. 0.000 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11

Tgt Ion: 50 Resp: 1183
Ion Ratio Lower Upper
50 100
52 25.4 26.5 39.7#


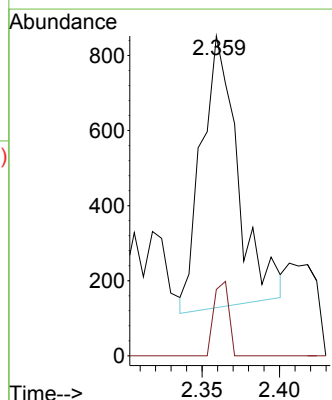

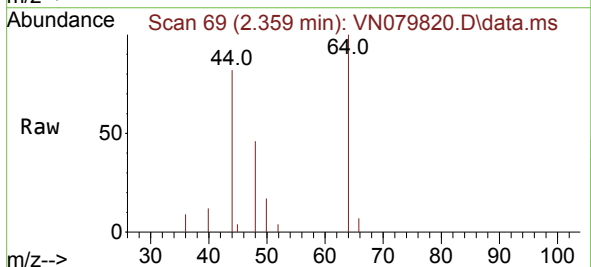




#5
Bromomethane
Concen: 0.473 ug/l
RT: 2.959 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 1046
Ion Ratio Lower Upper
94 100
96 99.2 73.1 109.7

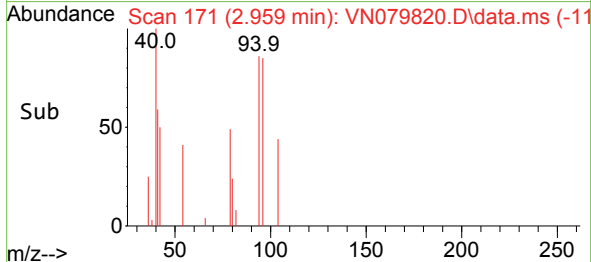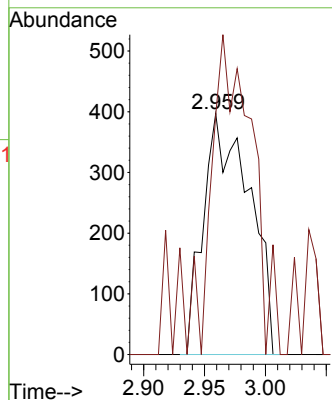

#10
Methyl Iodide
Concen: 0.400 ug/l
RT: 4.606 min Scan# 451
Delta R.T. 0.012 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11


Tgt Ion:142 Resp: 1199
Ion Ratio Lower Upper
142 100
127 36.2 37.6 56.4#
141 0.0 11.4 17.0#

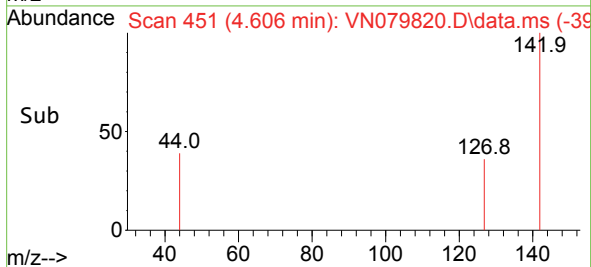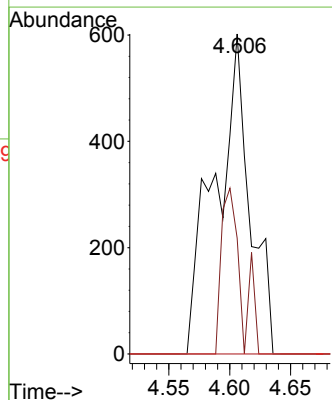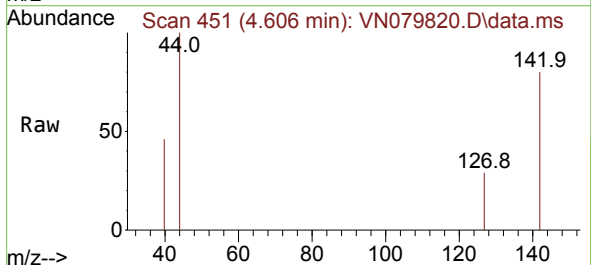






#13
Acrolein
Concen: 2.709 ug/l
RT: 4.206 min Scan# 383
Delta R.T. 0.023 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 55
Ion Ratio Lower Upper
56 100
55 0.0 54.5 81.7#

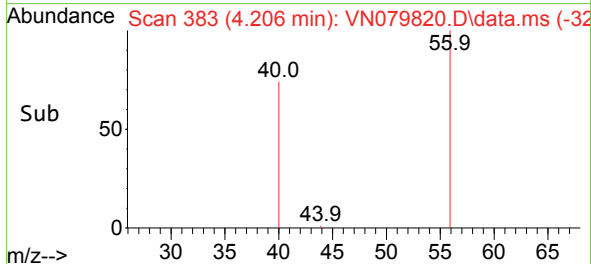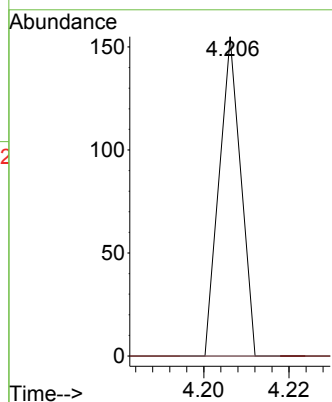

#16
Acetone
Concen: 0.807 ug/l
RT: 4.441 min Scan# 423
Delta R.T. 0.012 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11

Tgt Ion: 43 Resp: 997
Ion Ratio Lower Upper
43 100
58 44.1 28.0 42.0#

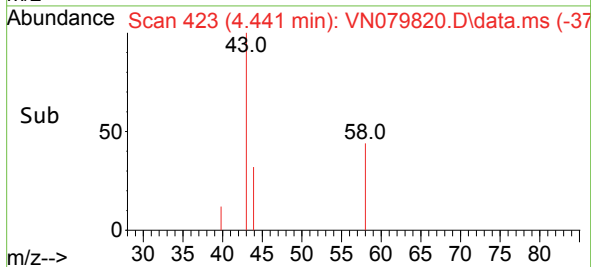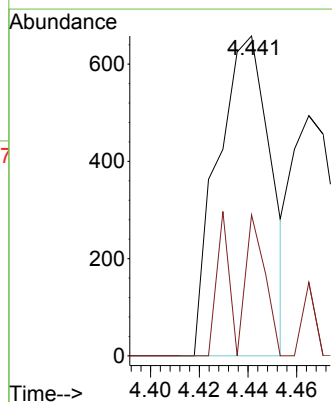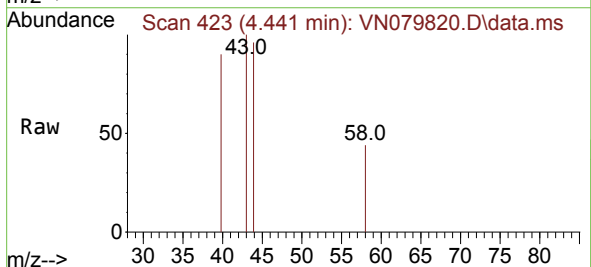



#31

Cyclohexane

Concen: 1.374 ug/l

RT: 8.229 min Scan# 1067

Delta R.T. -0.029 min


Lab File: VN079820.D

Acq: 03 Nov 2023 03:11

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 56 Resp: 6384

Ion Ratio Lower Upper

56 100

69 142.2 26.8 40.2#

84 101.9 81.8 122.6

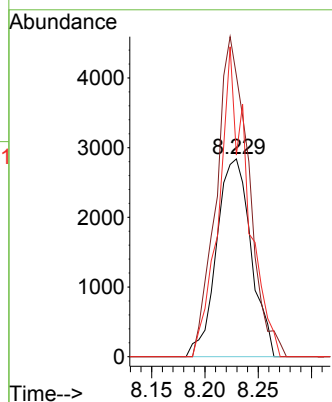

#33

1,2-Dichloroethane-d4

Concen: 56.909 ug/l

RT: 8.582 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VN079820.D




Acq: 03 Nov 2023 03:11


Tgt Ion: 65 Resp: 200082

Ion Ratio Lower Upper

65 100

67 51.6 0.0 106.6


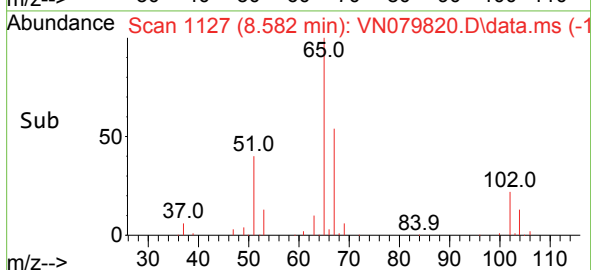

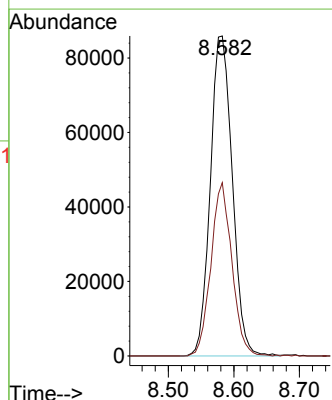




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:114 Resp: 449923
Ion Ratio Lower Upper
114 100
63 21.1 0.0 36.4
88 14.9 0.0 30.6

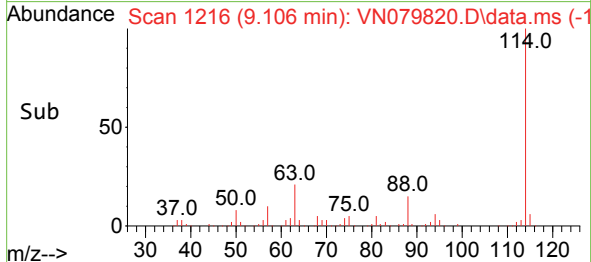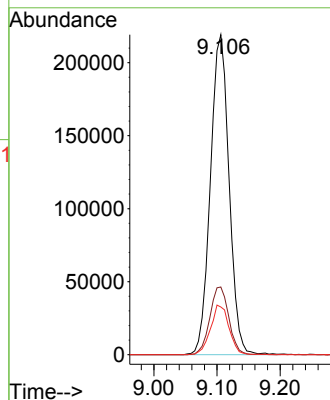

#35
Dibromofluoromethane
Concen: 53.750 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. -0.000 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11

Tgt Ion:113 Resp: 171161
Ion Ratio Lower Upper
113 100
111 102.6 82.6 123.8
192 16.9 12.7 19.1


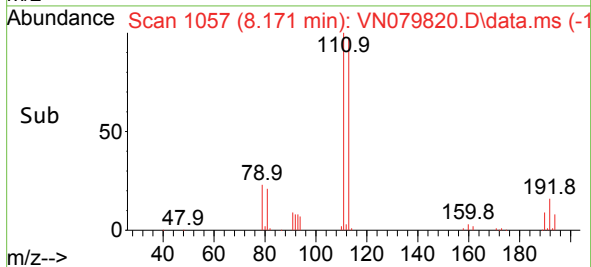
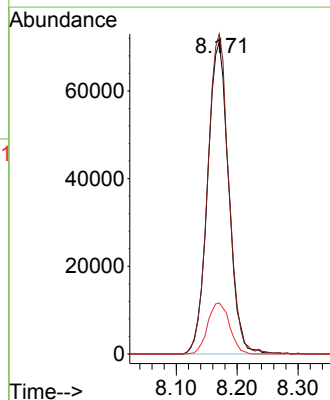
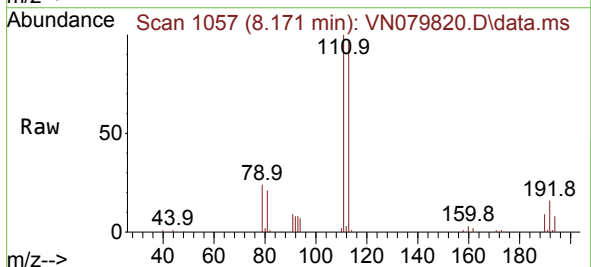




#36
1,1-Dichloropropene
Concen: 4.727 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 21494
Ion Ratio Lower Upper
75 100
110 7.7 19.1 57.3#
77 0.0 25.0 37.4#

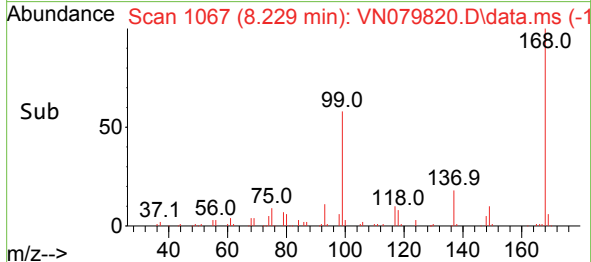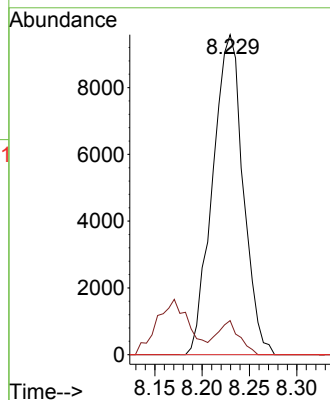

#38
Carbon Tetrachloride
Concen: 5.392 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.129 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11

Tgt Ion: 117 Resp: 24709
Ion Ratio Lower Upper
117 100
119 6.9 77.3 115.9#
121 0.0 23.3 34.9#

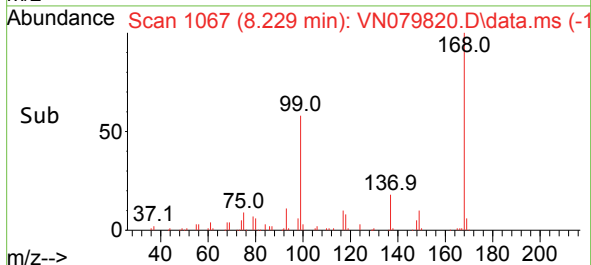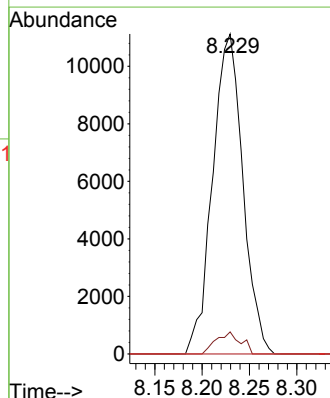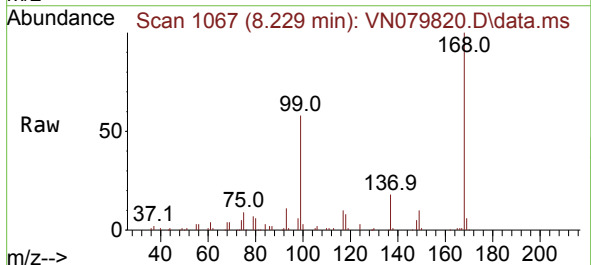



#44

Trichloroethene

Concen: 0.507 ug/l

RT: 9.353 min Scan# 1258

Delta R.T. -0.000 min

Lab File: VN079820.D

Acq: 03 Nov 2023 03:11

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:130 Resp: 1713

Ion Ratio Lower Upper

130 100

95 64.4 0.0 204.6

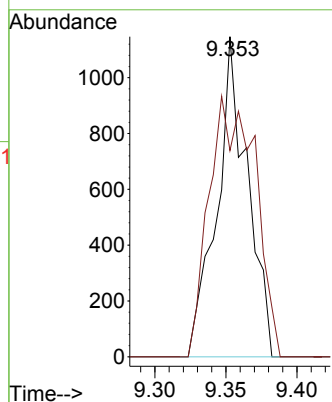

#50

Toluene-d8

Concen: 50.593 ug/l

RT: 10.570 min Scan# 1465

Delta R.T. -0.000 min

Lab File: VN079820.D




Acq: 03 Nov 2023 03:11


Tgt Ion: 98 Resp: 593091

Ion Ratio Lower Upper

98 100

100 63.8 52.0 78.0


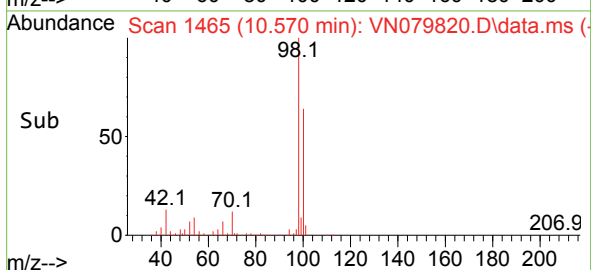
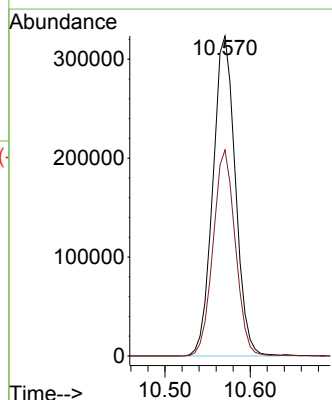



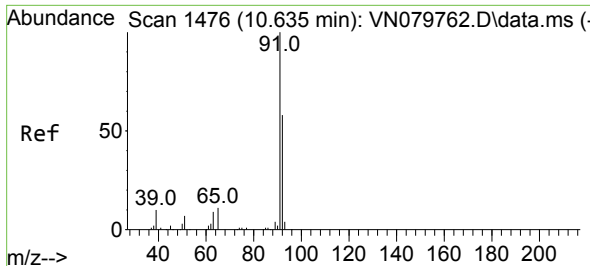

#52
Toluene
Concen: 0.265 ug/l
RT: 10.629 min Scan# 1475
Delta R.T. -0.006 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 92 Resp: 2142
Ion Ratio Lower Upper
92 100
91 173.8 137.4 206.0

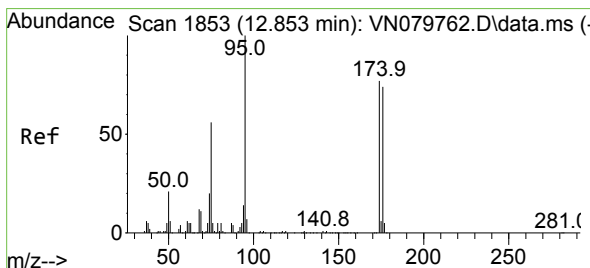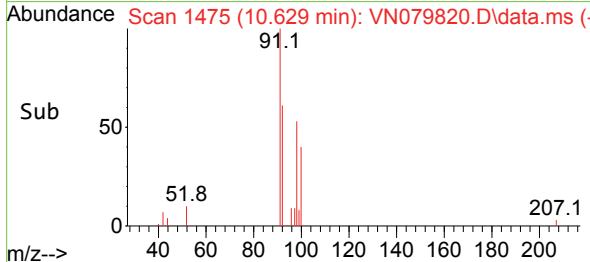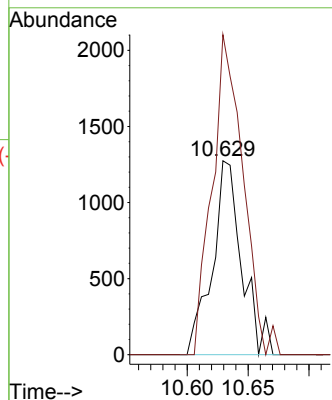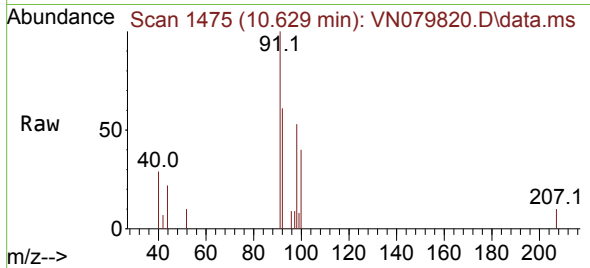

#62
4-Bromofluorobenzene
Concen: 50.236 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11


Tgt Ion: 95 Resp: 195312
Ion Ratio Lower Upper
95 100
174 74.8 0.0 143.8
176 73.5 0.0 135.8

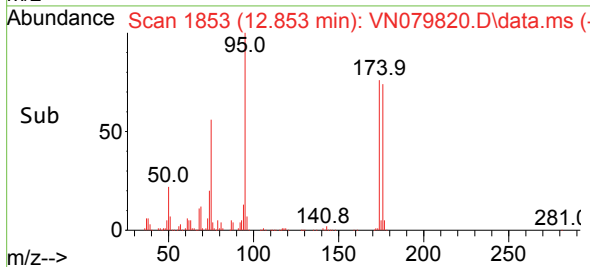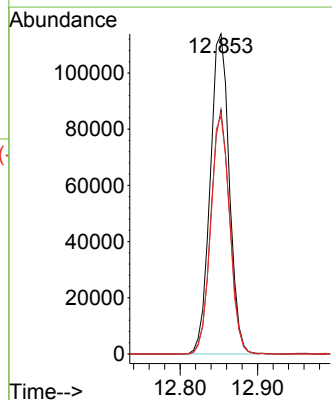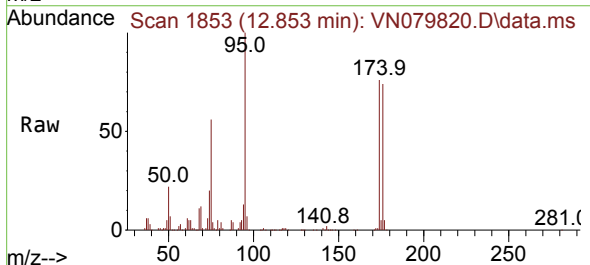



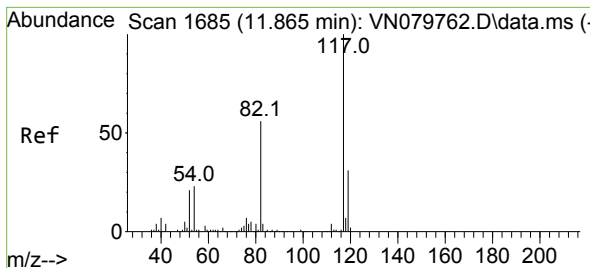


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1170
Delta R.T. -0.000 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11


Instrument :
MSVOA_N
ClientSampleId :

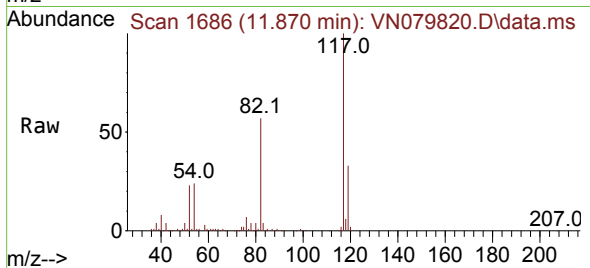



Tgt Ion:117 Resp: 461734
Ion Ratio Lower Upper
117 100
82 56.7 44.0 66.0
119 33.1 25.6 38.4

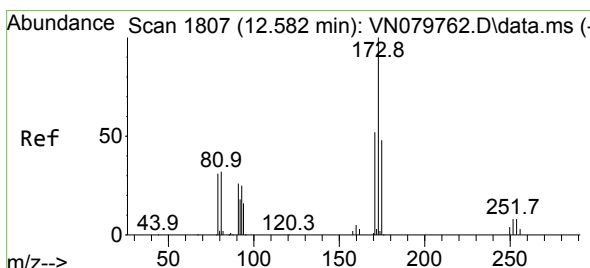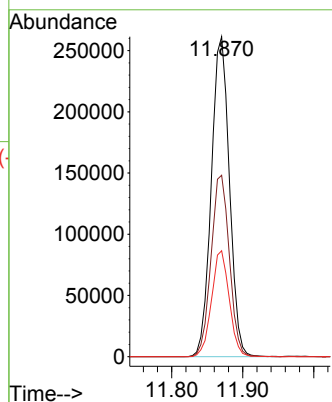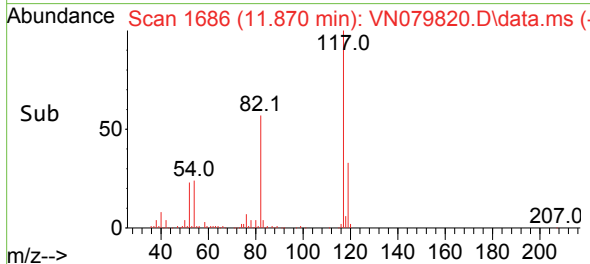


#71
Bromoform
Concen: 0.605 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.271 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11

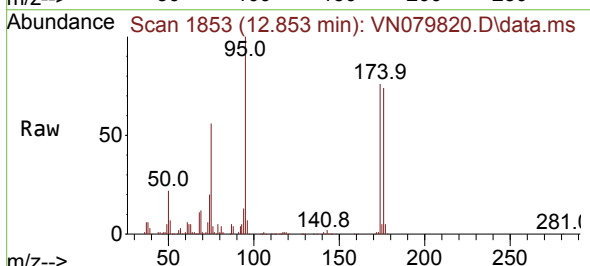

Tgt Ion:173 Resp: 1549
Ion Ratio Lower Upper
173 100
175 574.8 24.3 73.0#
254 0.0 0.0 0.0

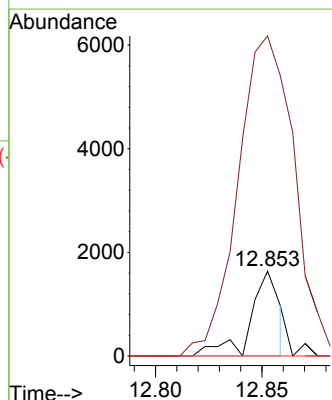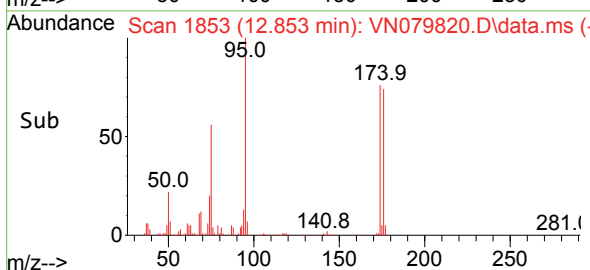

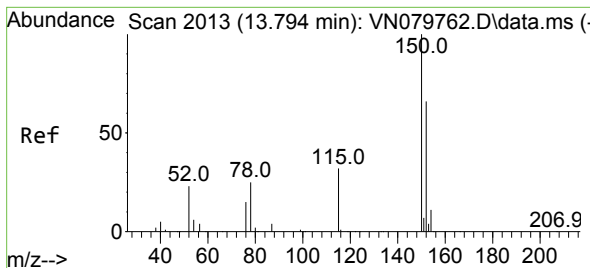

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. -0.000 min


Lab File: VN079820.D

Acq: 03 Nov 2023 03:11

Instrument :

MSVOA_N

ClientSampleId :

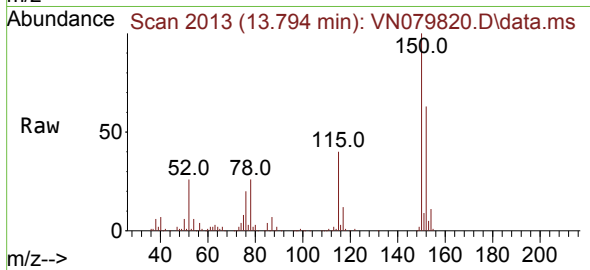




Tgt Ion:152 Resp: 176666

Ion Ratio Lower Upper

152 100

115 63.4 32.3 96.8

150 159.4 0.0 355.8

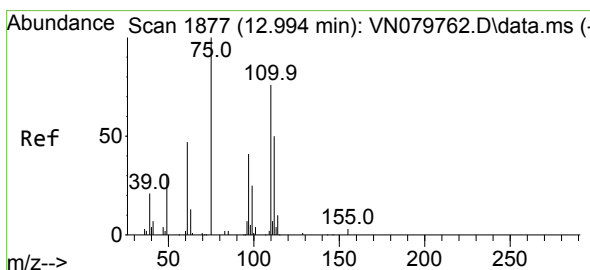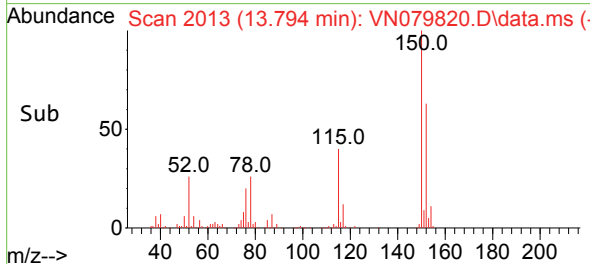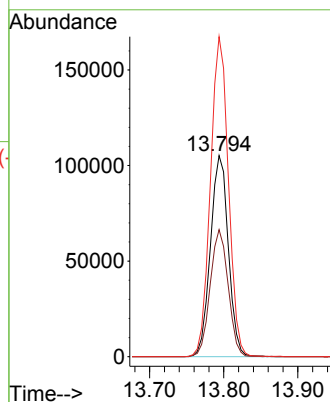

#76

1,2,3-Trichloropropane

Concen: 25.800 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.141 min

Lab File: VN079820.D




Acq: 03 Nov 2023 03:11


Tgt Ion: 75 Resp: 107009

Ion Ratio Lower Upper

75 100


77 1.2 84.5 253.5#

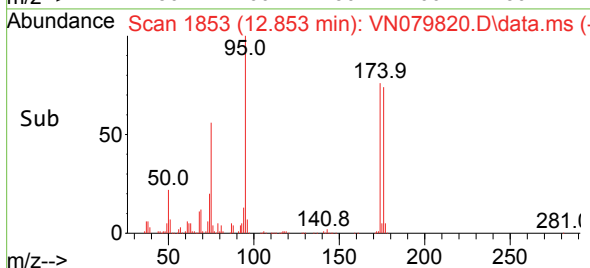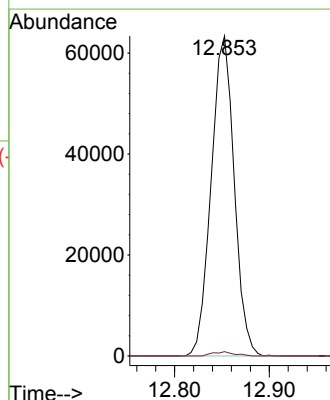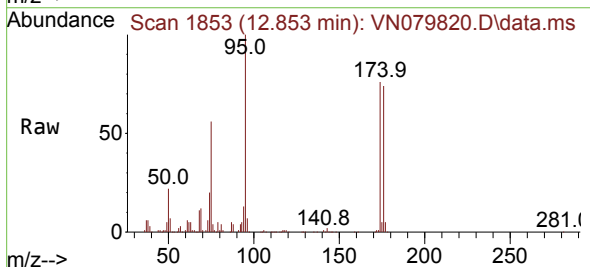



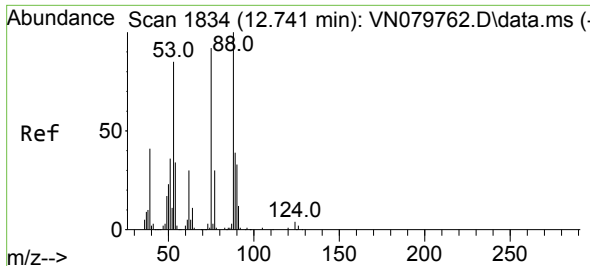


#81
trans-1,4-Dichloro-2-butene
Concen: 70.196 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.118 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11


Instrument :
MSVOA_N
ClientSampleId :

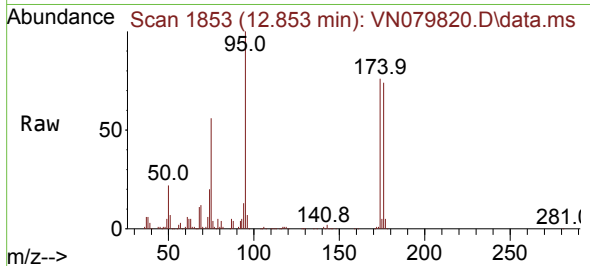



Tgt Ion: 75 Resp: 107009
Ion Ratio Lower Upper
75 100
53 0.1 67.4 101.2#
89 0.0 38.8 58.2#

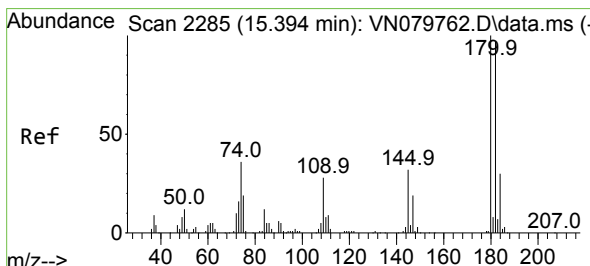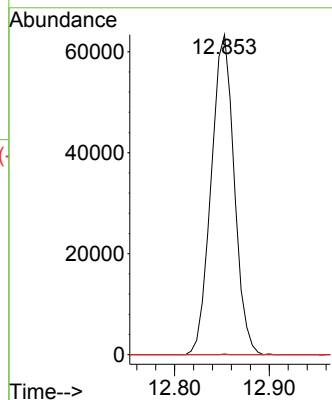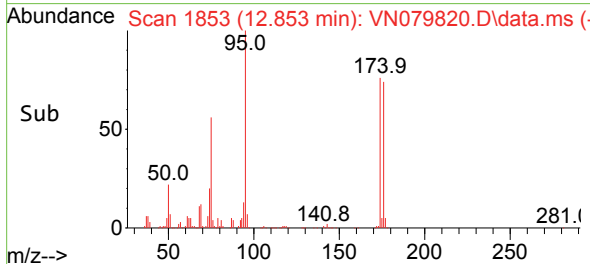


#93
1,2,4-Trichlorobenzene
Concen: 0.313 ug/l
RT: 15.411 min Scan# 2288
Delta R.T. 0.018 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11

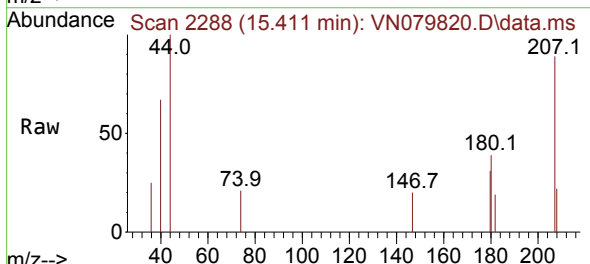


Tgt Ion:180 Resp: 857
Ion Ratio Lower Upper
180 100
182 71.8 46.1 138.2
145 0.0 16.6 49.8#

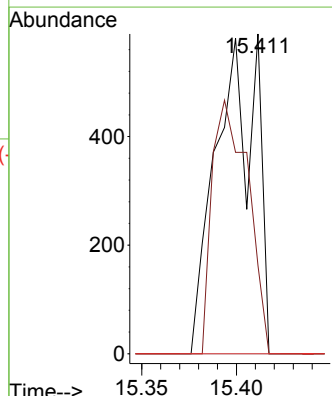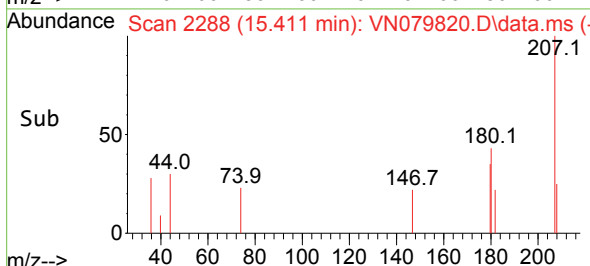






#94
Hexachlorobutadiene
Concen: 0.253 ug/l
RT: 15.500 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:225 Resp: 314
Ion Ratio Lower Upper
225 100
223 93.6 31.3 93.8
227 49.4 31.9 95.9

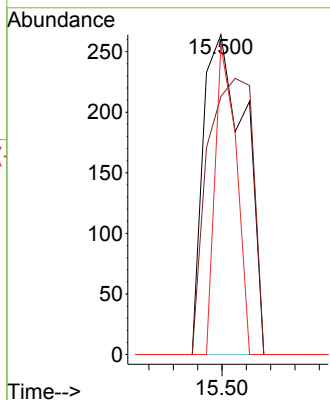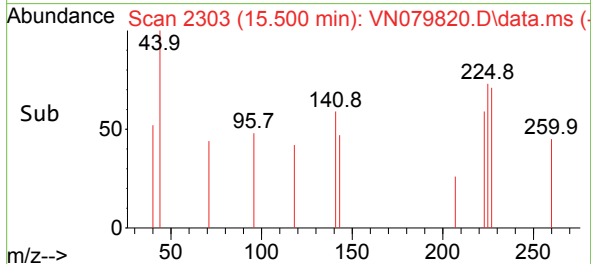

#95
Naphthalene
Concen: 0.377 ug/l
RT: 15.641 min Scan# 2327
Delta R.T. -0.000 min
Lab File: VN079820.D
Acq: 03 Nov 2023 03:11


Tgt Ion:128 Resp: 3501
Ion Ratio Lower Upper
128 100
127 9.3 10.0 15.0#
129 9.9 8.7 13.1

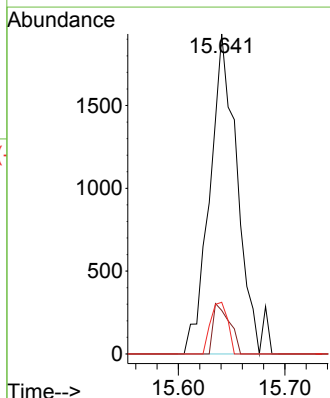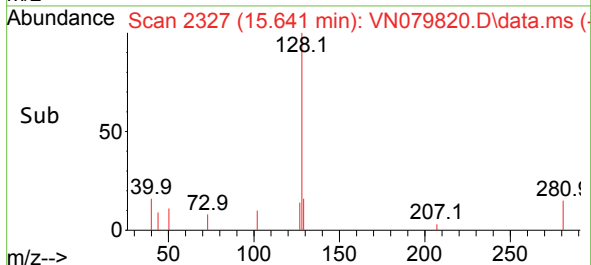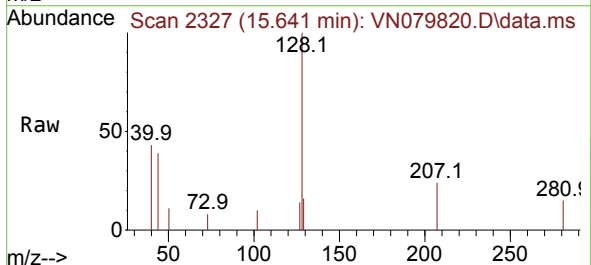



#96
 1,2,3-Trichlorobenzene
 Concen: 0.257 ug/l
 RT: 15.841 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN079820.D
 Acq: 03 Nov 2023 03:11

Instrument :
 MSVOA_N
 ClientSampleId :

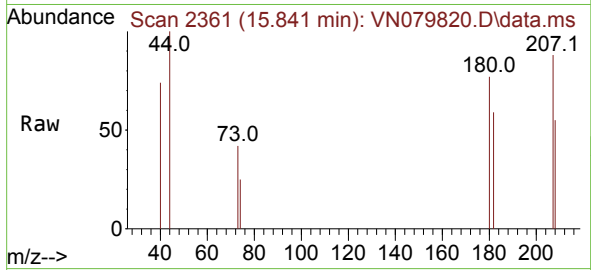

Tgt Ion:180 Resp: 690
 Ion Ratio Lower Upper
 180 100
 182 107.1 46.2 138.6
 145 12.2 17.5 52.6#

