

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110223\
 Data File : VN079798.D
 Acq On : 02 Nov 2023 15:35
 Operator : JC\MD
 Sample : 05225-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BP-VPB-188-TB-20231031

Quant Time: Nov 03 04:02:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 02 05:49:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	217256	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	439031	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	451836	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	177065	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	195785	59.150	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	118.300%
35) Dibromofluoromethane	8.171	113	167149	53.793	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	107.580%
50) Toluene-d8	10.571	98	581020	50.793	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.580%
62) 4-Bromofluorobenzene	12.853	95	191698	50.530	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	101.060%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110223\
Data File : VN079798.D
Acq On : 02 Nov 2023 15:35
Operator : JC\MD
Sample : 05225-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-188-TB-20231031

Quant Time: Nov 03 04:02:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 02 05:49:08 2023
Response via : Initial Calibration




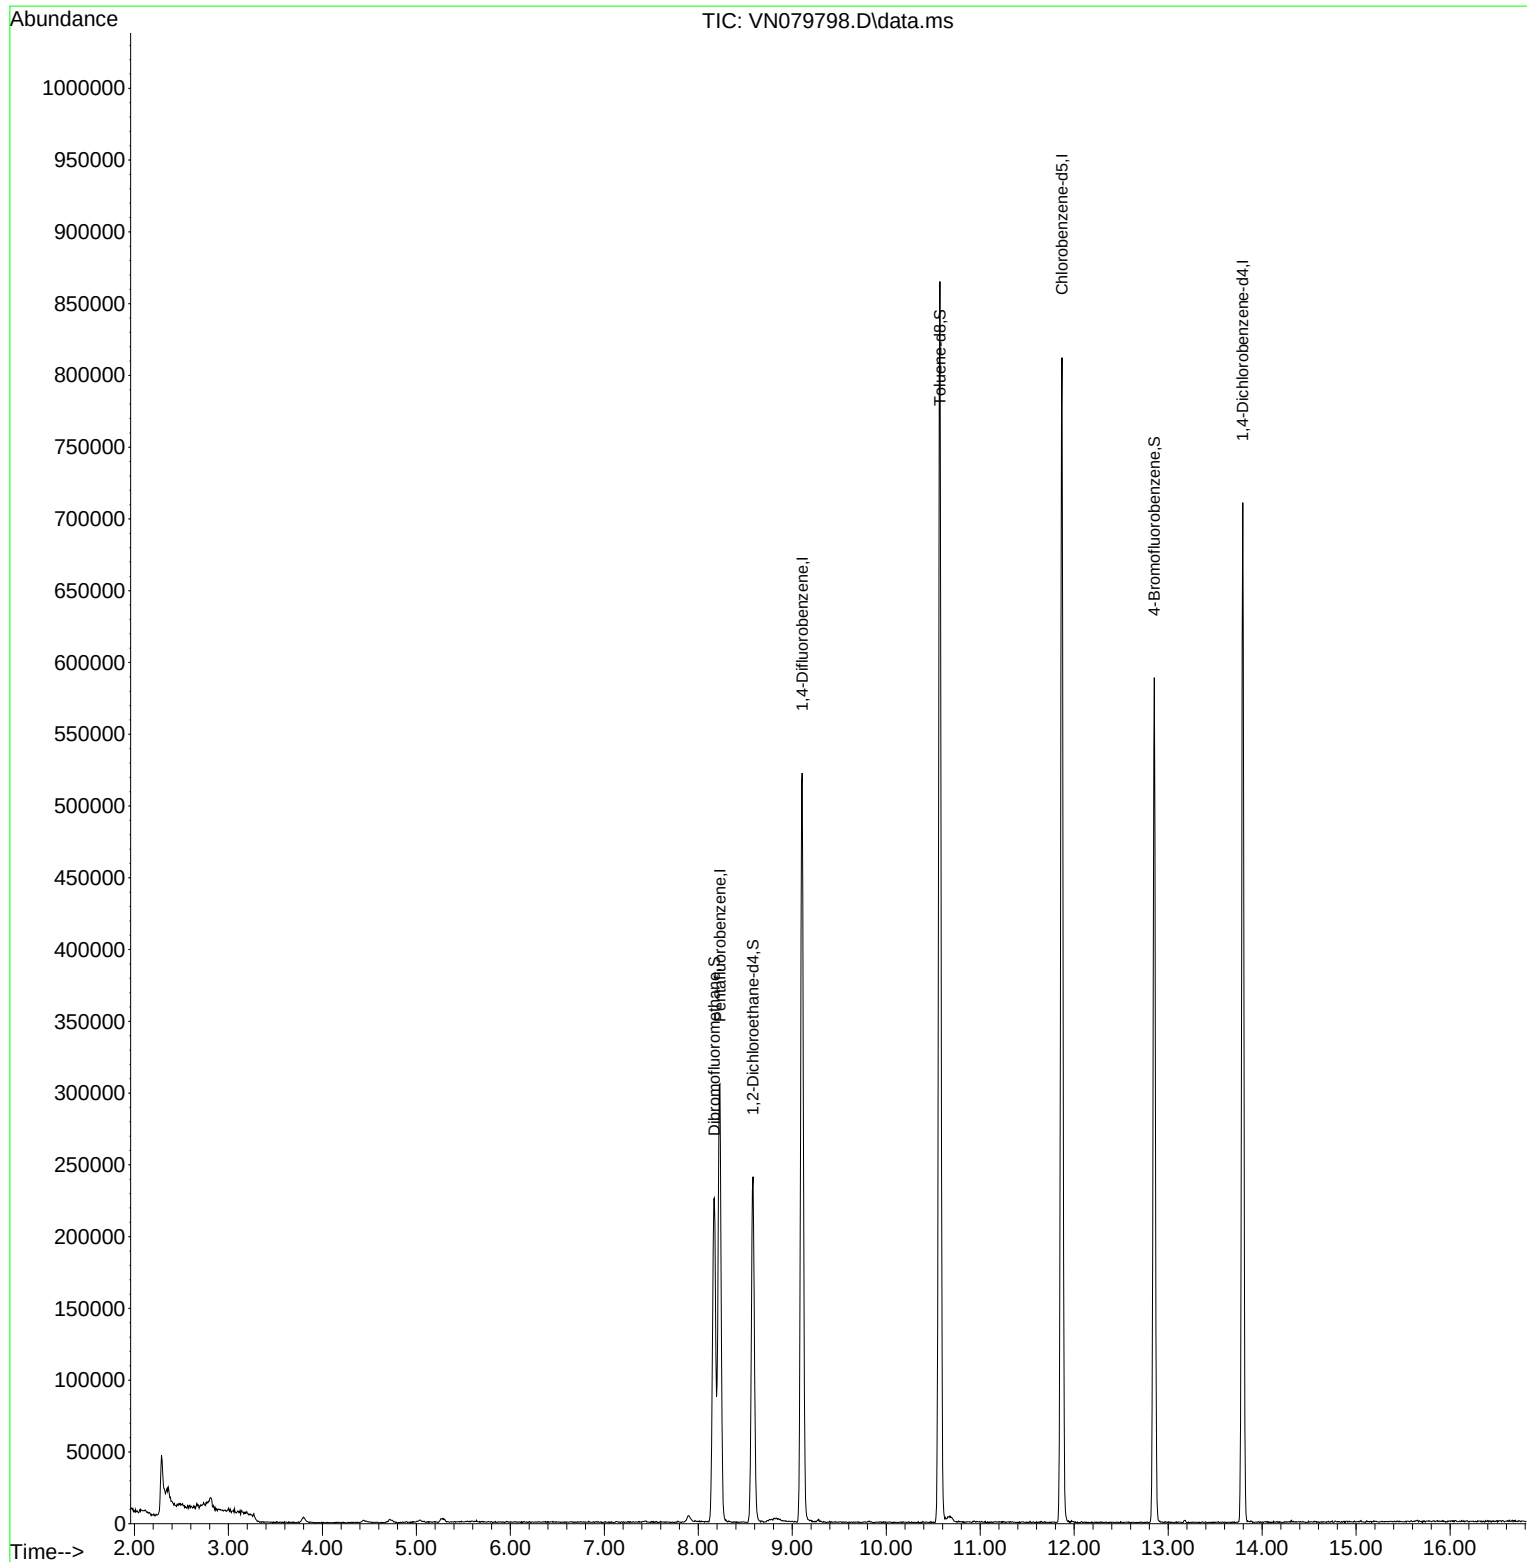


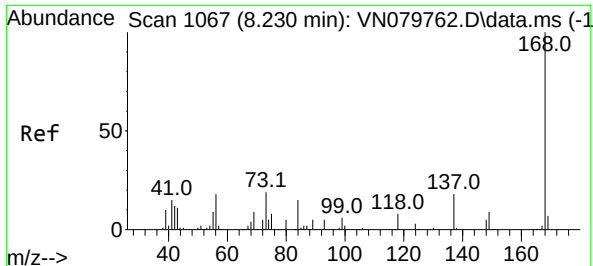

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. 0.001 min
Lab File: VN079798.D
Acq: 02 Nov 2023 15:35




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-188-TB-20231031


Tgt Ion:168 Resp: 217256
Ion Ratio Lower Upper
168 100
99 58.1 53.0 79.6

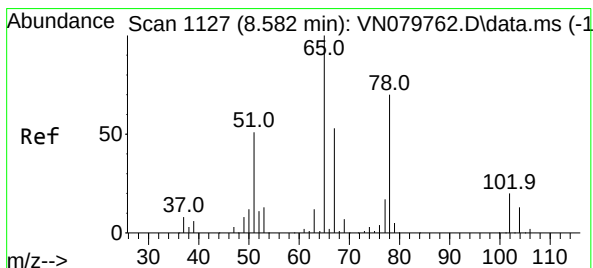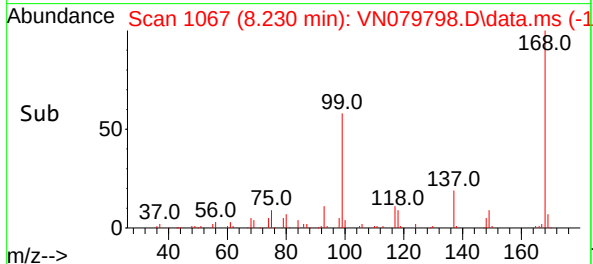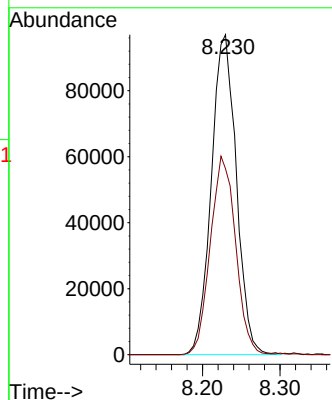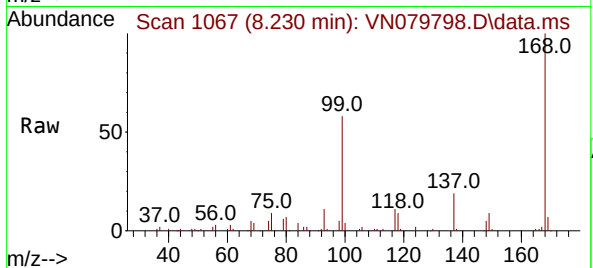

#33
1,2-Dichloroethane-d4
Concen: 59.150 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VN079798.D
Acq: 02 Nov 2023 15:35

Tgt Ion: 65 Resp: 195785
Ion Ratio Lower Upper
65 100
67 51.9 0.0 106.6

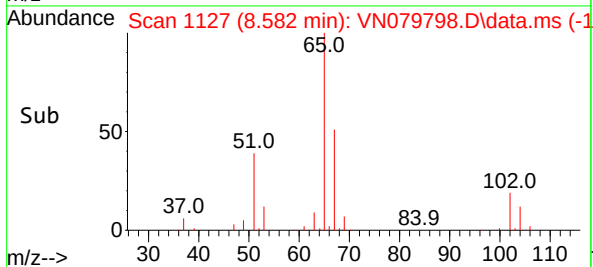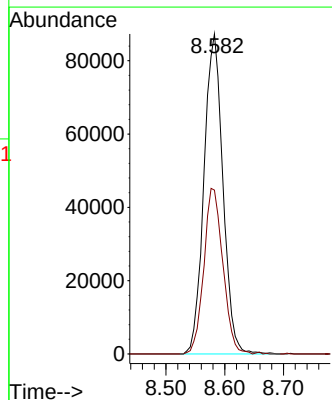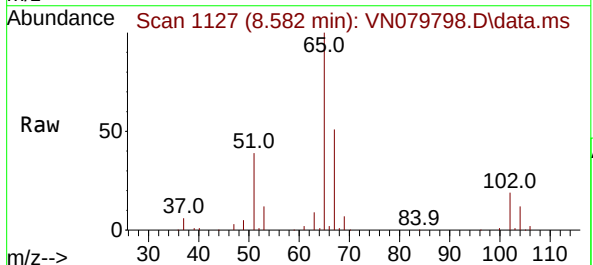

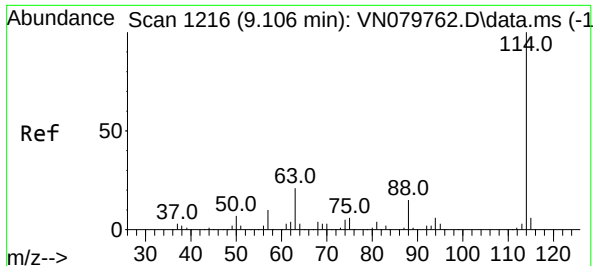

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 114

Delta R.T. 0.000 min

Lab File: VN079798.D

Acq: 02 Nov 2023 15:35

Instrument :

MSVOA_N

ClientSampleId :

BP-VPB-188-TB-20231031





Tgt Ion:114 Resp: 439031

Ion Ratio Lower Upper

114 100

63 22.8 0.0 36.4

88 16.1 0.0 30.6

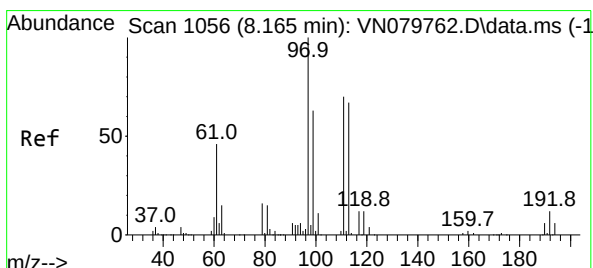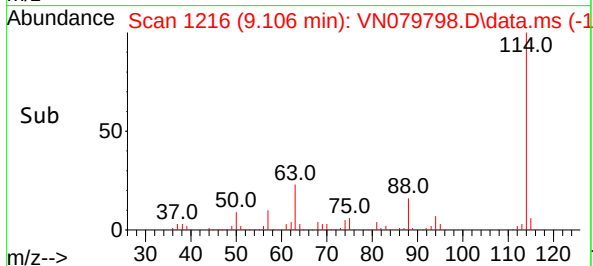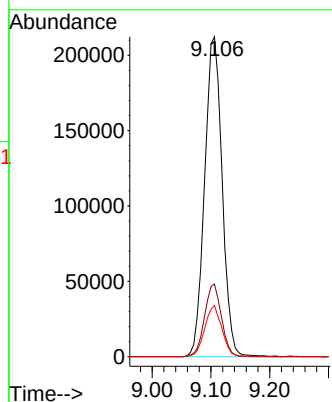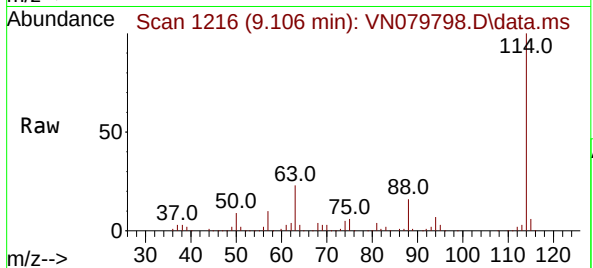

#35

Dibromofluoromethane

Concen: 53.793 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.000 min

Lab File: VN079798.D

Acq: 02 Nov 2023 15:35




Tgt Ion:113 Resp: 167149


Ion Ratio Lower Upper

113 100

111 100.9 82.6 123.8

192 17.5 12.7 19.1


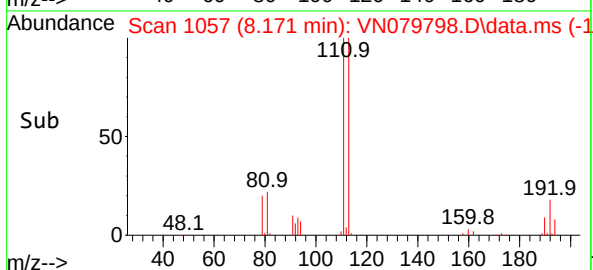
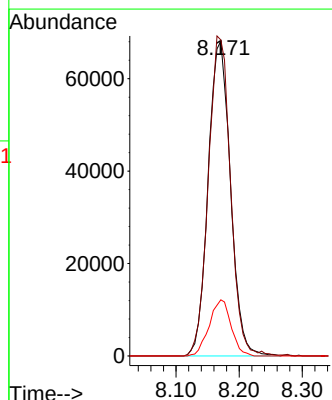
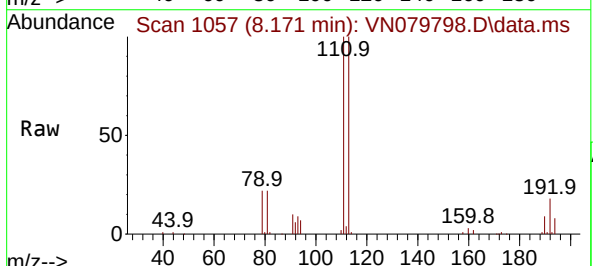


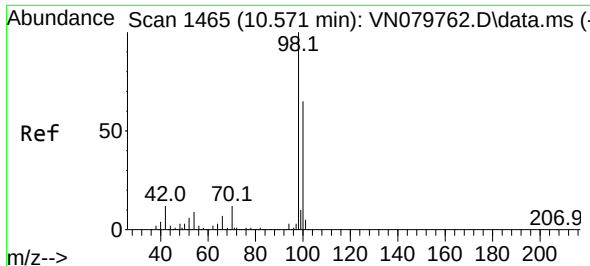

#50
Toluene-d8
Concen: 50.793 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN079798.D
Acq: 02 Nov 2023 15:35




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-188-TB-20231031


Tgt Ion: 98 Resp: 581020
Ion Ratio Lower Upper
98 100
100 62.6 52.0 78.0

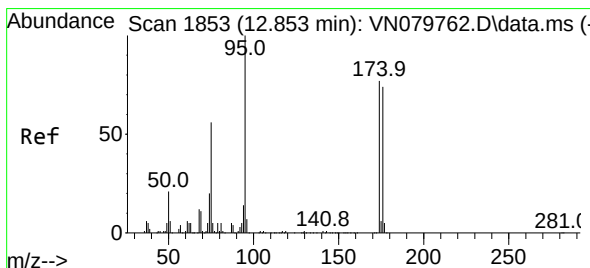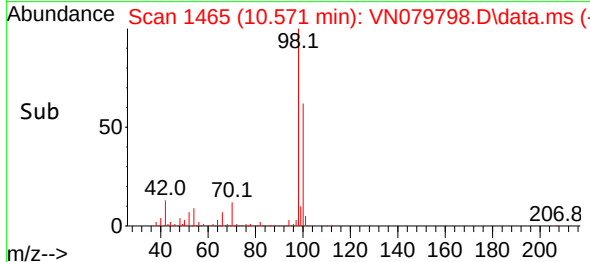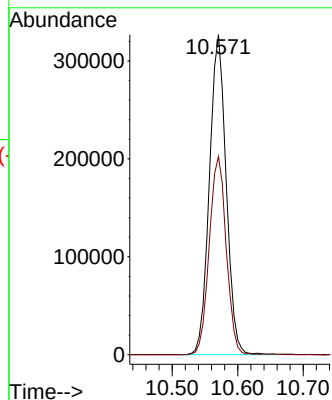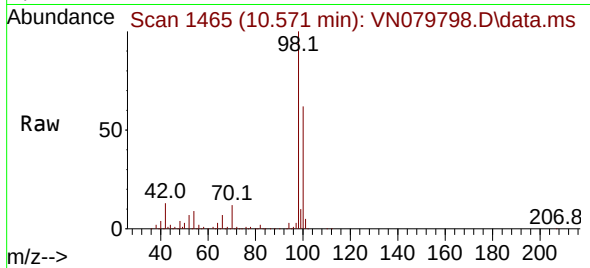

#62
4-Bromofluorobenzene
Concen: 50.530 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN079798.D
Acq: 02 Nov 2023 15:35

Tgt Ion: 95 Resp: 191698
Ion Ratio Lower Upper
95 100
174 74.8 0.0 143.8
176 70.5 0.0 135.8


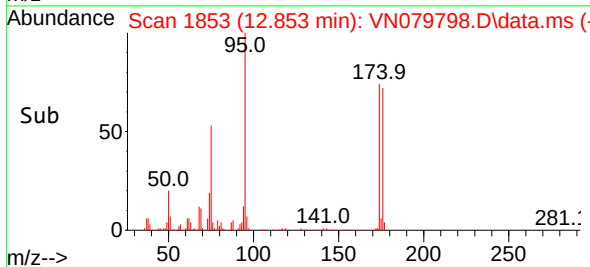
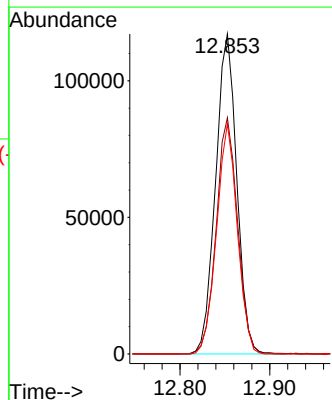
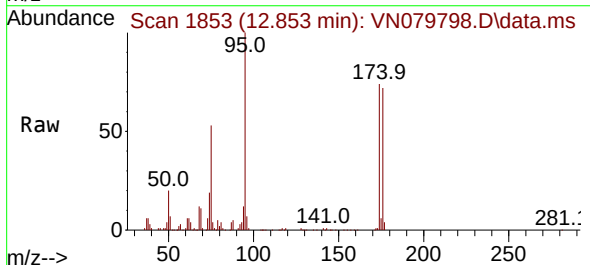


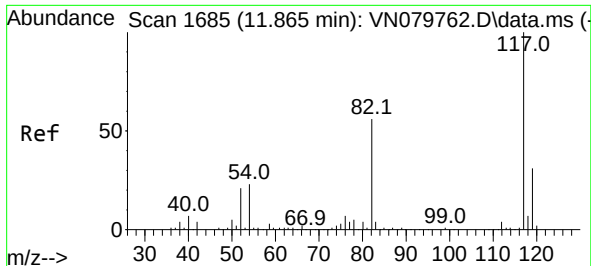

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN079798.D
Acq: 02 Nov 2023 15:35

Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-188-TB-20231031

Tgt Ion:117 Resp: 451836
Ion Ratio Lower Upper
117 100
82 57.0 44.0 66.0
119 31.7 25.6 38.4

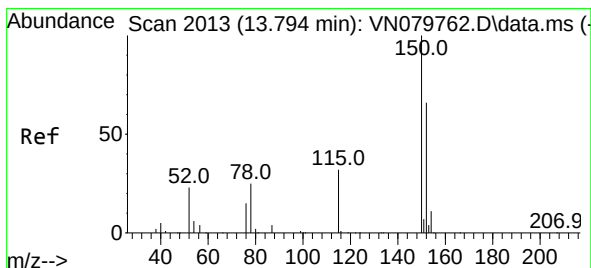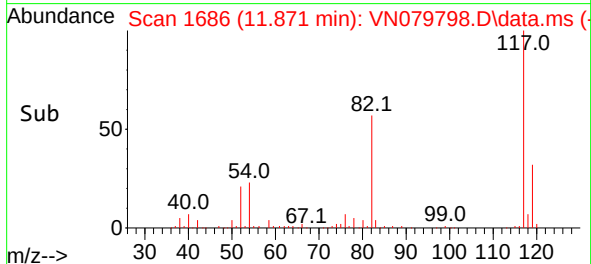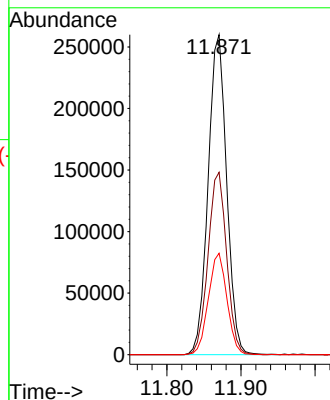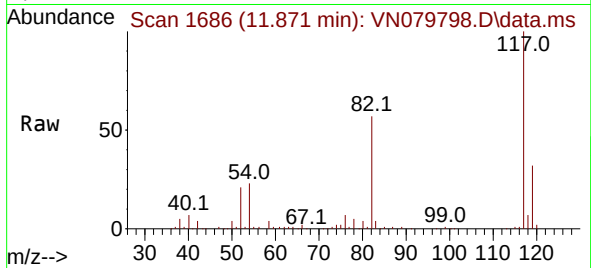

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN079798.D
Acq: 02 Nov 2023 15:35

Tgt Ion:152 Resp: 177065
Ion Ratio Lower Upper
152 100
115 62.1 32.3 96.8
150 158.6 0.0 355.8

