
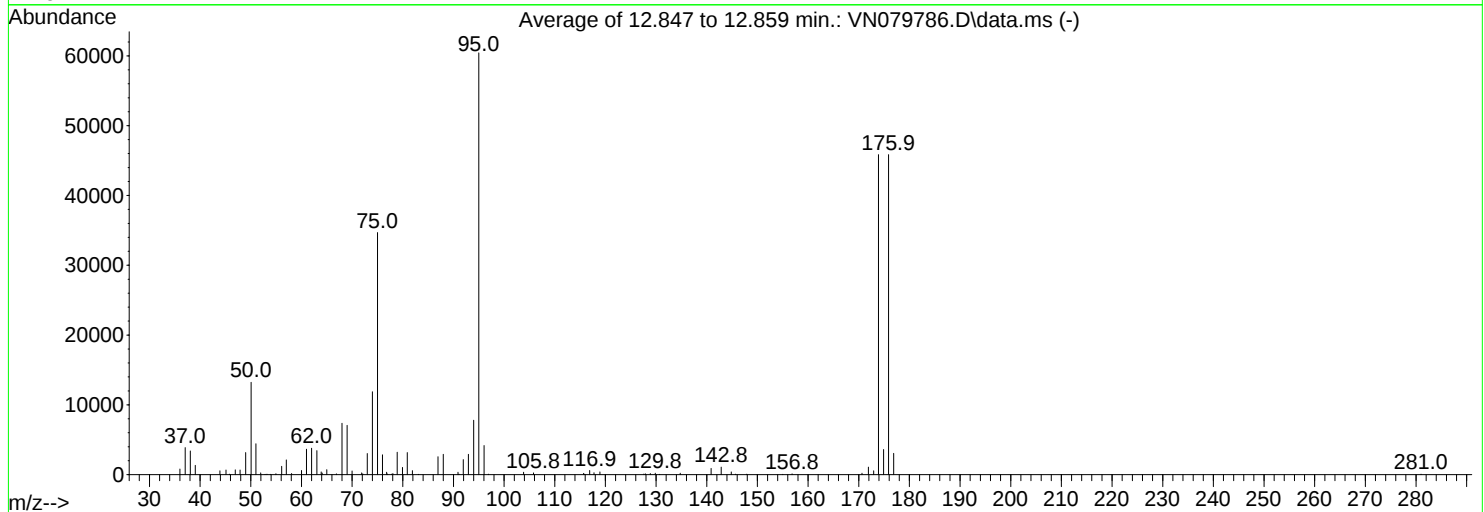


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110223\
Data File : VN079786.D
Acq On : 02 Nov 2023 10:19
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Title : SW846 8260
Last Update : Thu Nov 02 05:49:08 2023

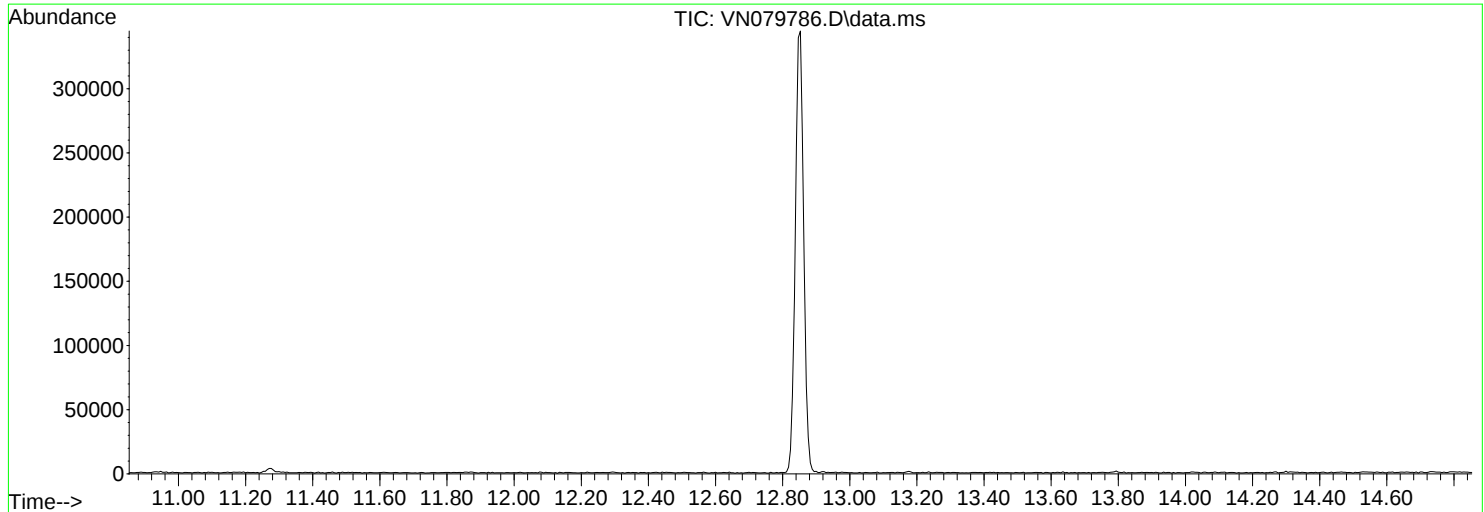

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	13228	PASS
75	95	30	60	57.4	34685	PASS
95	95	100	100	100.0	60435	PASS
96	95	5	9	6.9	4176	PASS
173	174	0.00	2	1.2	547	PASS
174	95	50	100	75.9	45845	PASS
175	174	5	9	7.9	3610	PASS
176	174	95	101	100.0	45861	PASS
177	176	5	9	6.6	3040	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	806	51.00	4417	62.00	3793	73.00	303
37.05	3877	51.95	260	63.05	3450	74.00	1187
38.05	3401	52.80	54	63.90	386	75.00	3468
39.05	1331	53.20	65	64.10	239	76.00	283
43.90	563	53.90	57	65.00	723	76.80	349
45.10	664	54.95	149	66.90	125	77.00	85
45.80	72	56.10	1201	68.00	7352	77.80	81
46.95	690	57.00	2115	69.00	7073	78.05	169
47.90	673	58.05	152	70.00	519	78.90	3201
49.00	3164	60.00	590	71.90	251	79.95	1032
50.05	13228	61.00	3647	72.10	120	80.90	3164

Average of 12.847 to 12.859 min.: VN079786.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.90	578	96.90	62	129.85	219	171.90	1088
83.10	50	103.85	357	130.70	52	172.95	547
86.95	2560	105.80	242	134.75	199	173.90	45845
88.00	2908	115.70	189	140.85	890	174.90	3610
90.90	353	115.90	77	142.85	1083	175.90	45861
91.10	79	116.90	595	144.85	400	176.90	3040
91.95	2164	117.75	272	145.70	79	281.00	66
92.95	2919	118.90	393	147.90	62		
94.00	7784	127.60	92	155.00	54		
95.00	60435	127.90	112	156.85	108		
96.05	4176	128.85	165	170.65	198		

Instrument :

MSVOA_N

ClientSampleId :

BFB