
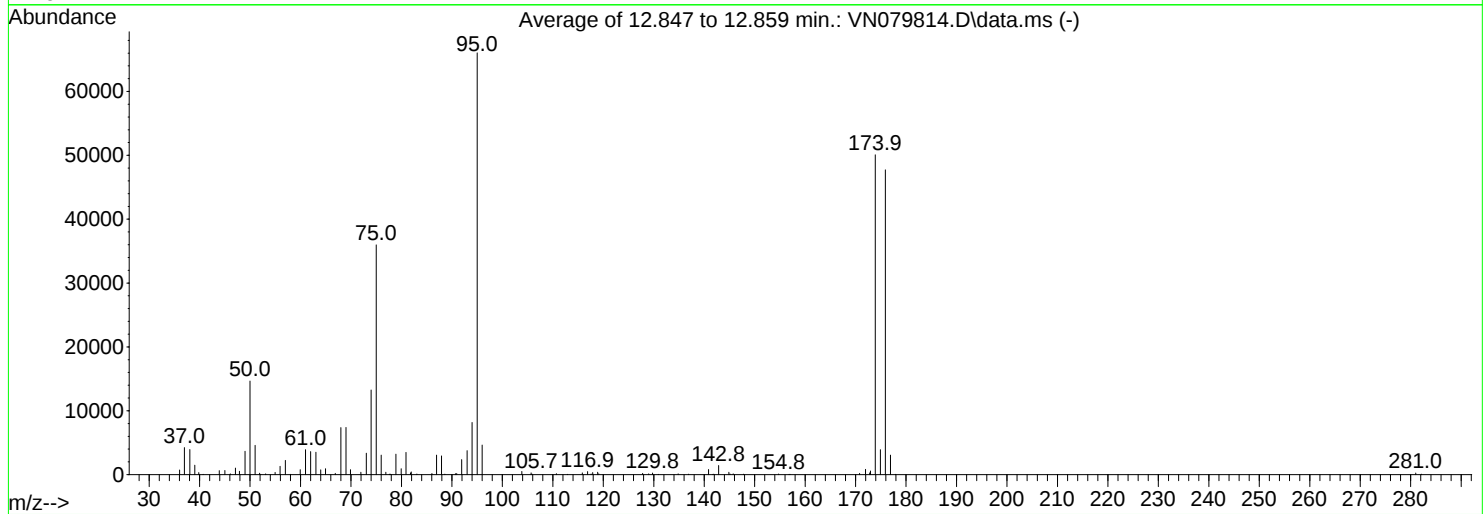


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110223\
Data File : VN079814.D
Acq On : 02 Nov 2023 23:35
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Title : SW846 8260
Last Update : Thu Nov 02 05:49:08 2023

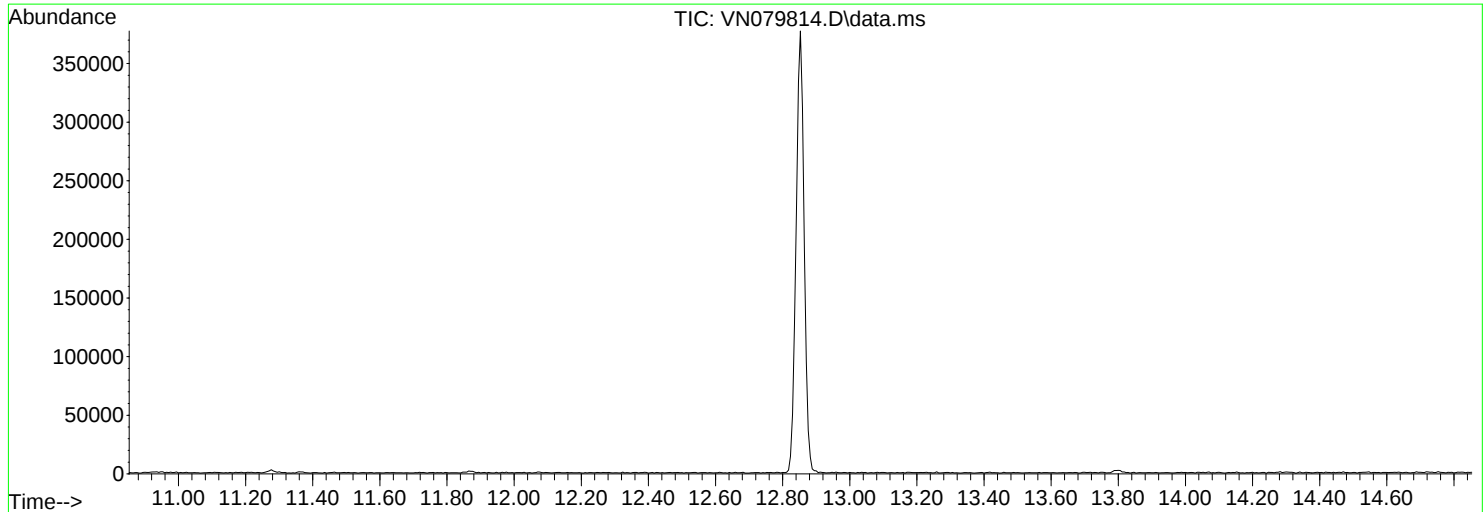

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	14657	PASS
75	95	30	60	54.5	35981	PASS
95	95	100	100	100.0	66045	PASS
96	95	5	9	7.0	4630	PASS
173	174	0.00	2	1.1	573	PASS
174	95	50	100	75.8	50093	PASS
175	174	5	9	7.8	3903	PASS
176	174	95	101	95.3	47739	PASS
177	176	5	9	6.4	3055	PASS

Average of 12.847 to 12.859 min.: VN079814.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	738	49.00	3648	61.00	3902	74.00	1325
37.00	4233	50.00	14657	62.00	3604	75.00	3598
38.05	3928	51.00	4582	63.05	3508	76.00	306
39.05	1484	51.90	232	64.00	740	76.90	37
39.85	316	52.10	56	64.95	930	77.60	72
40.70	57	53.10	119	66.90	198	77.80	77
43.90	621	54.95	365	68.00	7367	78.90	3219
45.00	662	55.95	1308	69.00	7385	79.95	917
46.10	124	57.00	2220	69.90	768	80.90	3486
47.10	1018	58.00	62	71.95	388	81.80	277
47.90	538	59.95	781	73.05	3370	81.95	422

Average of 12.847 to 12.859 min.: VN079814.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
83.05	107	96.00	4630	119.10	116	144.90	381
86.05	175	103.85	502	127.80	211	145.10	93
86.95	3055	105.70	281	129.00	116	145.75	133
87.95	2944	105.90	70	129.75	258	147.80	70
88.60	81	110.70	144	130.90	60	154.75	106
90.70	144	112.90	62	134.85	122	156.80	52
90.95	188	115.85	287	136.90	66	157.00	56
91.95	2364	116.90	479	140.85	792	170.80	195
93.00	3765	117.60	93	141.70	57	171.95	843
94.00	8156	117.90	339	141.90	71	172.80	271
95.00	66045	118.90	377	142.85	1435	172.95	573

Average of 12.847 to 12.859 min.: VN079814.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.90	50093						
174.90	3903						
175.90	47739						
176.90	3055						
177.90	51						
281.00	242						
282.10	71						