

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110322\
 Data File : VN075137.D
 Acq On : 03 Nov 2022 12:13
 Operator : JC\MD
 Sample : VN1103MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1103MBL01

Quant Time: Nov 04 04:09:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 09:48:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	95229	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	177182	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	149896	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	57387	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	74527	58.084	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 116.160%	
35) Dibromofluoromethane	8.171	113	55437	53.297	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 106.600%	
50) Toluene-d8	10.571	98	208109	51.570	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 103.140%	
62) 4-Bromofluorobenzene	12.853	95	62777	44.284	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 88.560%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110322\
Data File : VN075137.D
Acq On : 03 Nov 2022 12:13
Operator : JC\MD
Sample : VN1103MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1103MBL01

Quant Time: Nov 04 04:09:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 09:48:49 2022
Response via : Initial Calibration




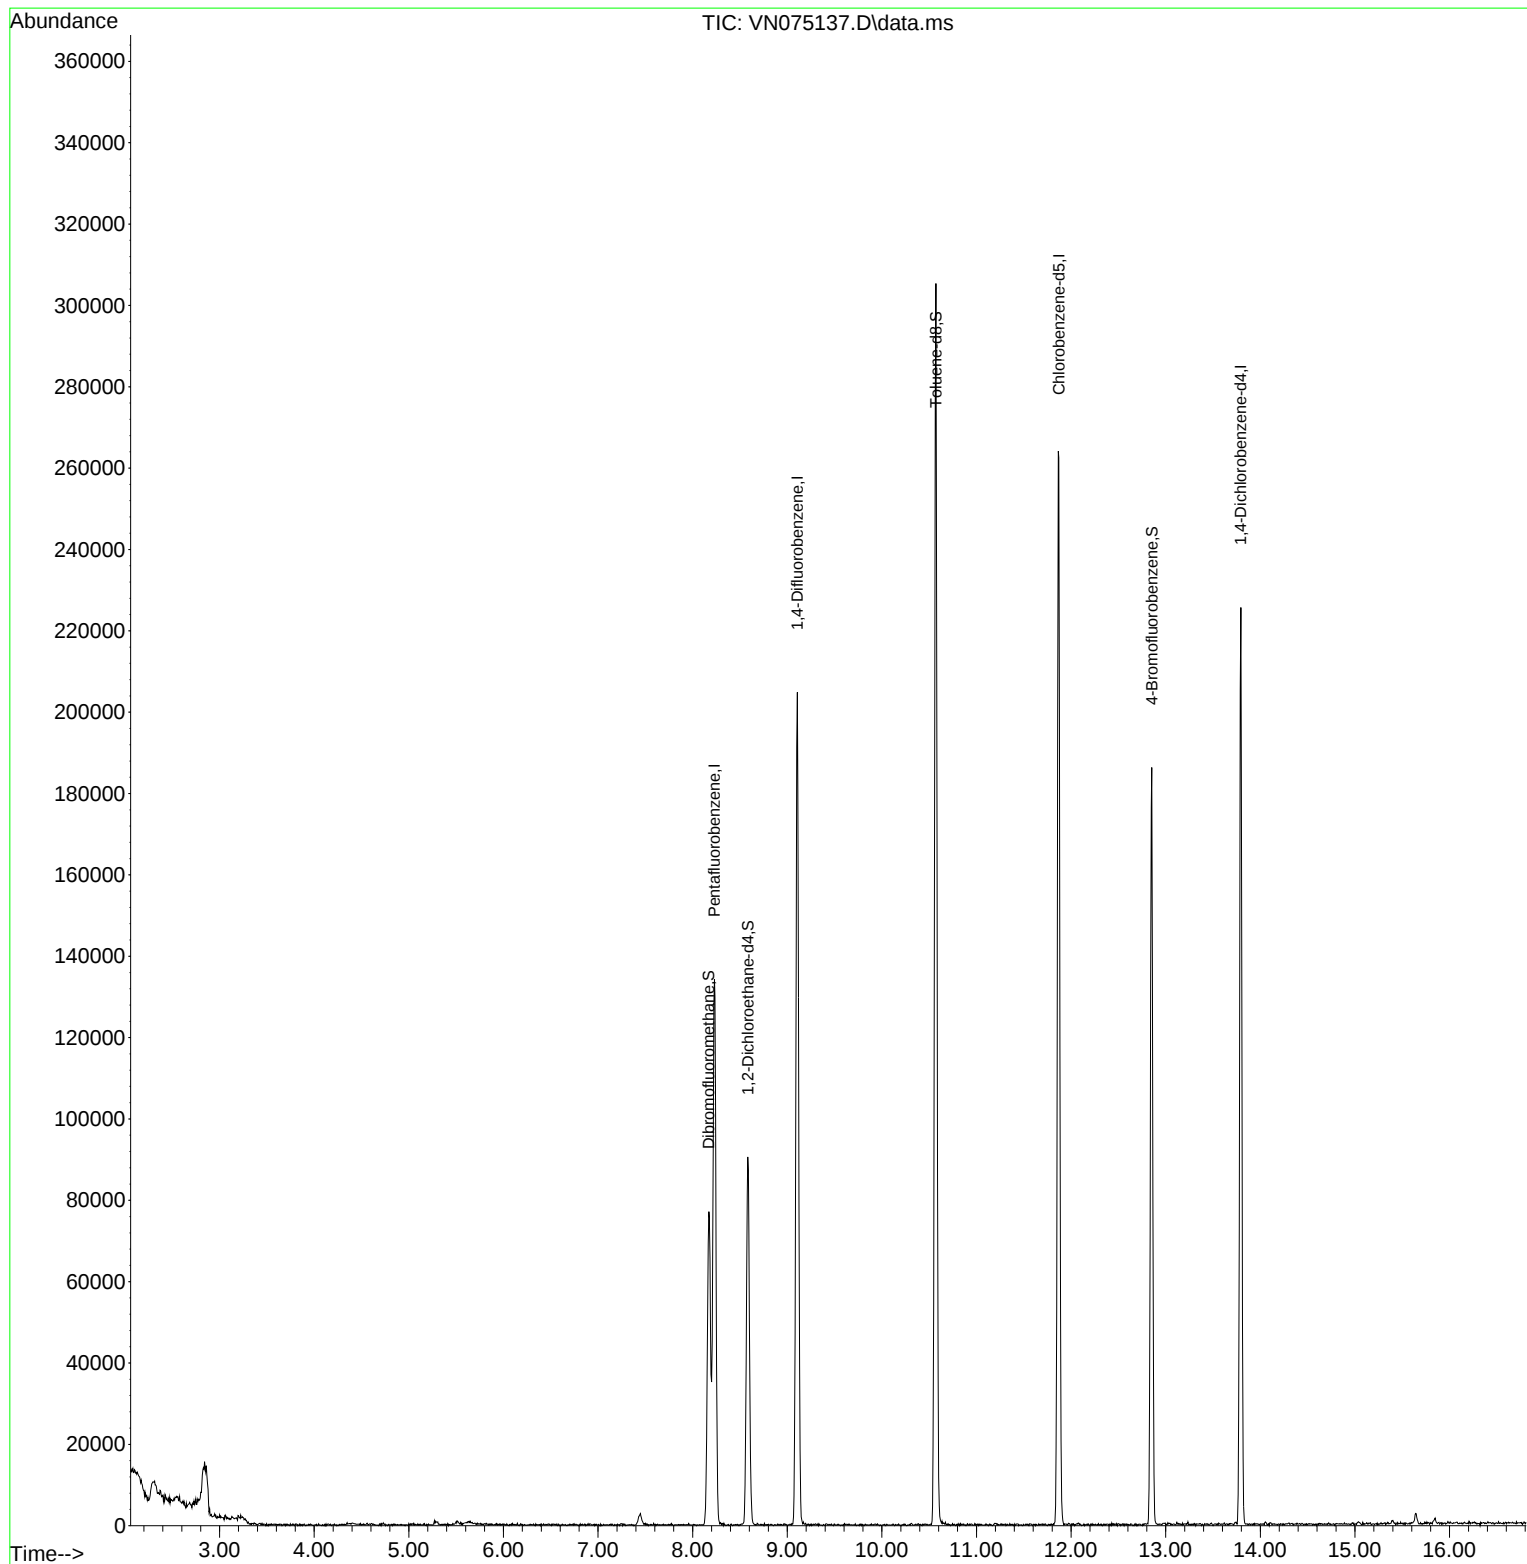


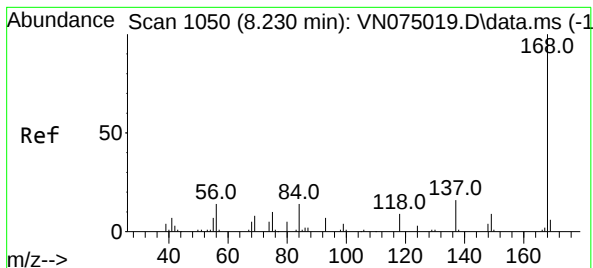

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1100
Delta R.T. -0.000 min
Lab File: VN075137.D
Acq: 03 Nov 2022 12:13




Instrument :
MSVOA_N
ClientSampleId :
VN1103MBL01


Tgt Ion:168 Resp: 95229
Ion Ratio Lower Upper
168 100
99 62.3 51.6 77.4

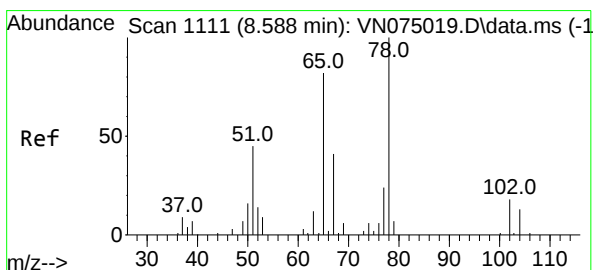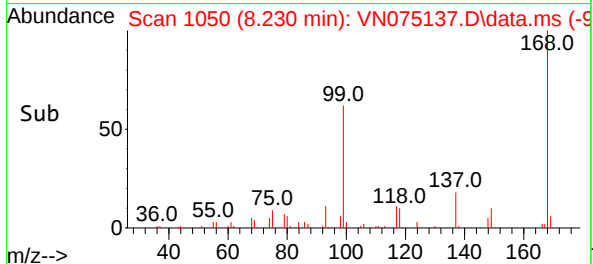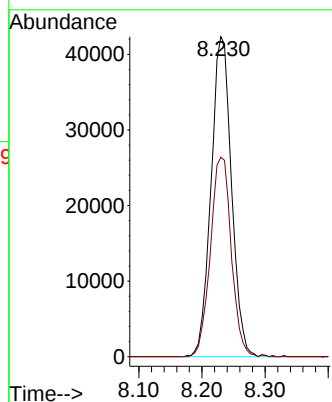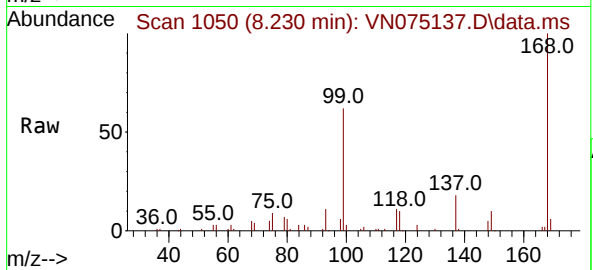

#33
1,2-Dichloroethane-d4
Concen: 58.084 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. -0.005 min
Lab File: VN075137.D
Acq: 03 Nov 2022 12:13

Tgt Ion: 65 Resp: 74527
Ion Ratio Lower Upper
65 100
67 50.4 0.0 102.0

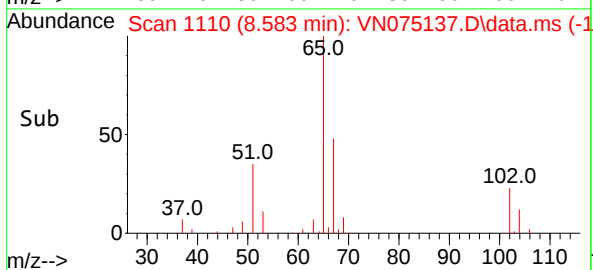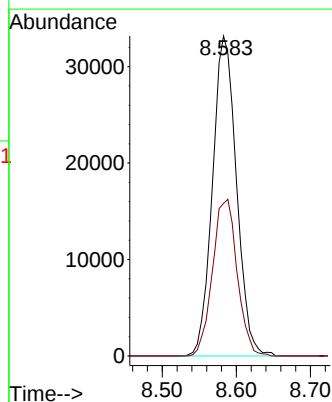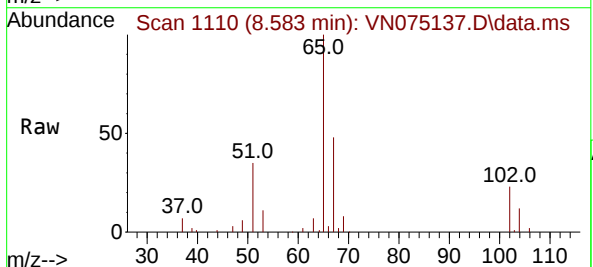

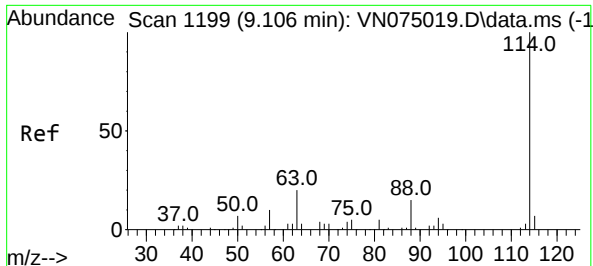

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN075137.D

Acq: 03 Nov 2022 12:13

Instrument :

MSVOA_N

ClientSampleId :

VN1103MBL01





Tgt Ion:114 Resp: 177182

Ion Ratio Lower Upper

114 100

63 20.4 0.0 39.6

88 15.9 0.0 29.0

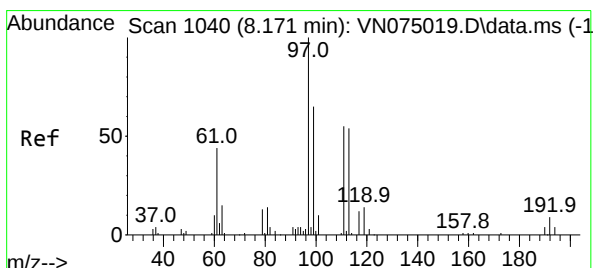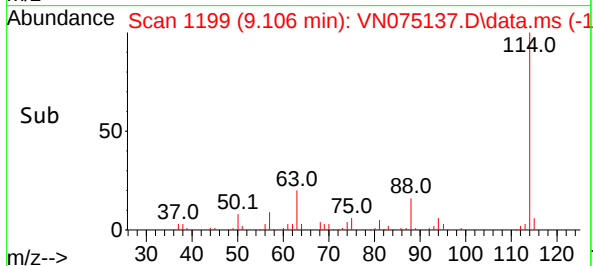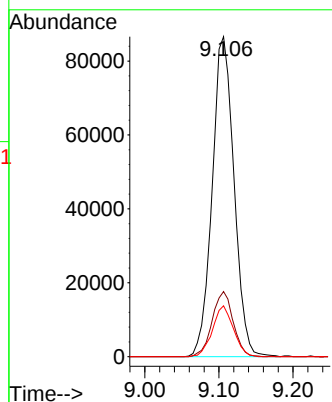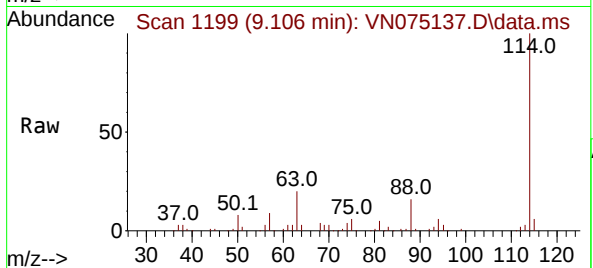

#35

Dibromofluoromethane

Concen: 53.297 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VN075137.D

Acq: 03 Nov 2022 12:13




Tgt Ion:113 Resp: 55437


Ion Ratio Lower Upper

113 100

111 104.3 80.5 120.7

192 17.3 13.2 19.8


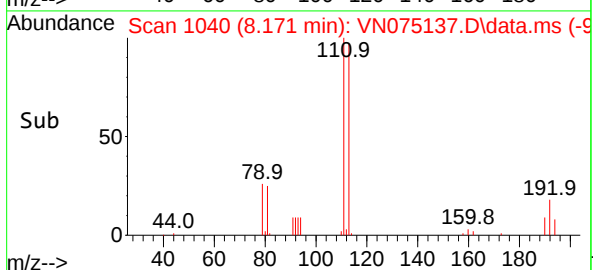
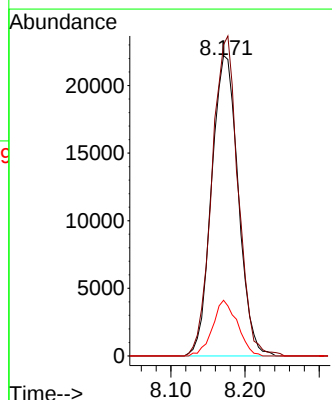
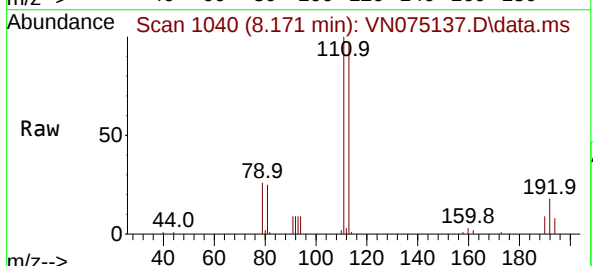


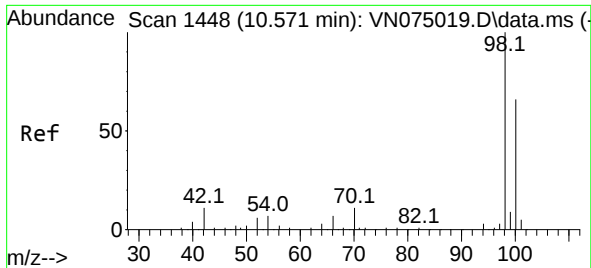

#50
Toluene-d8
Concen: 51.570 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN075137.D
Acq: 03 Nov 2022 12:13




Instrument :
MSVOA_N
ClientSampleId :
VN1103MBL01


Tgt Ion: 98 Resp: 208109
Ion Ratio Lower Upper
98 100
100 64.9 53.0 79.6

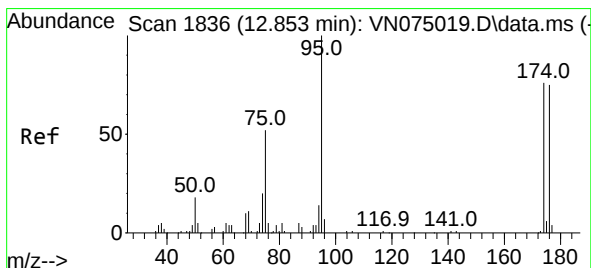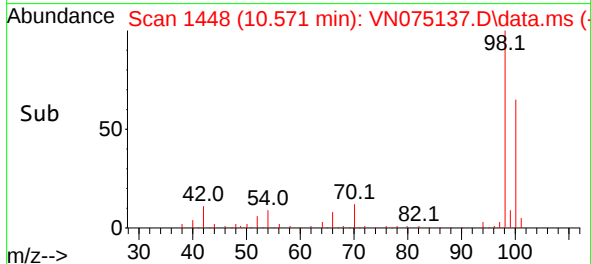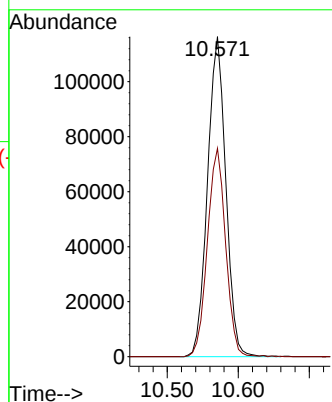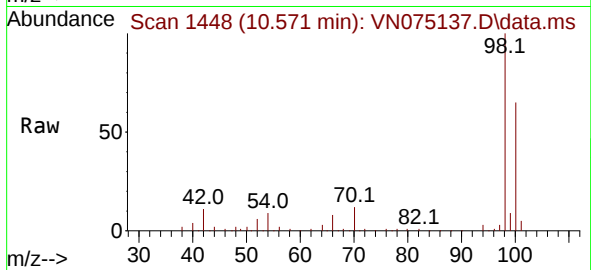

#62
4-Bromofluorobenzene
Concen: 44.284 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN075137.D
Acq: 03 Nov 2022 12:13

Tgt Ion: 95 Resp: 62777
Ion Ratio Lower Upper
95 100
174 72.0 0.0 147.4
176 70.5 0.0 142.2


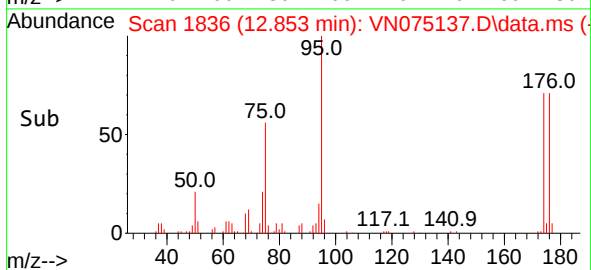
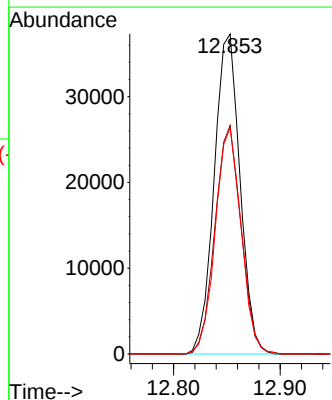
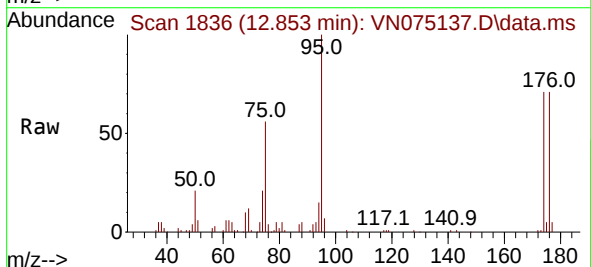


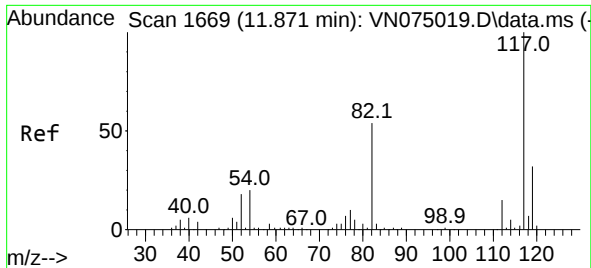

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1170
Delta R.T. -0.000 min
Lab File: VN075137.D
Acq: 03 Nov 2022 12:13

Instrument :
MSVOA_N
ClientSampleId :
VN1103MBL01

Tgt Ion:117 Resp: 149896
Ion Ratio Lower Upper
117 100
82 57.1 43.1 64.7
119 31.1 25.5 38.3

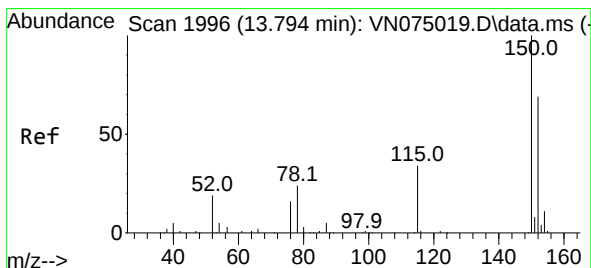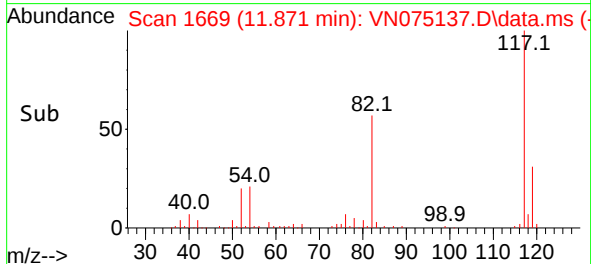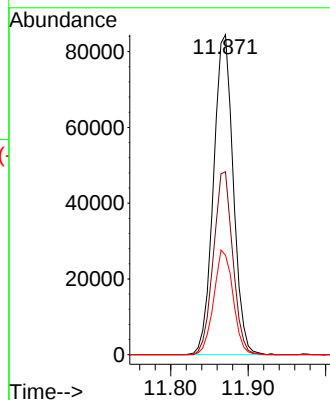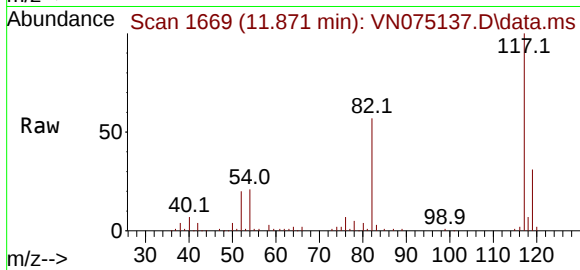

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. 0.000 min
Lab File: VN075137.D
Acq: 03 Nov 2022 12:13

Tgt Ion:152 Resp: 57387
Ion Ratio Lower Upper
152 100
115 62.1 30.2 90.6
150 158.8 0.0 348.4

