
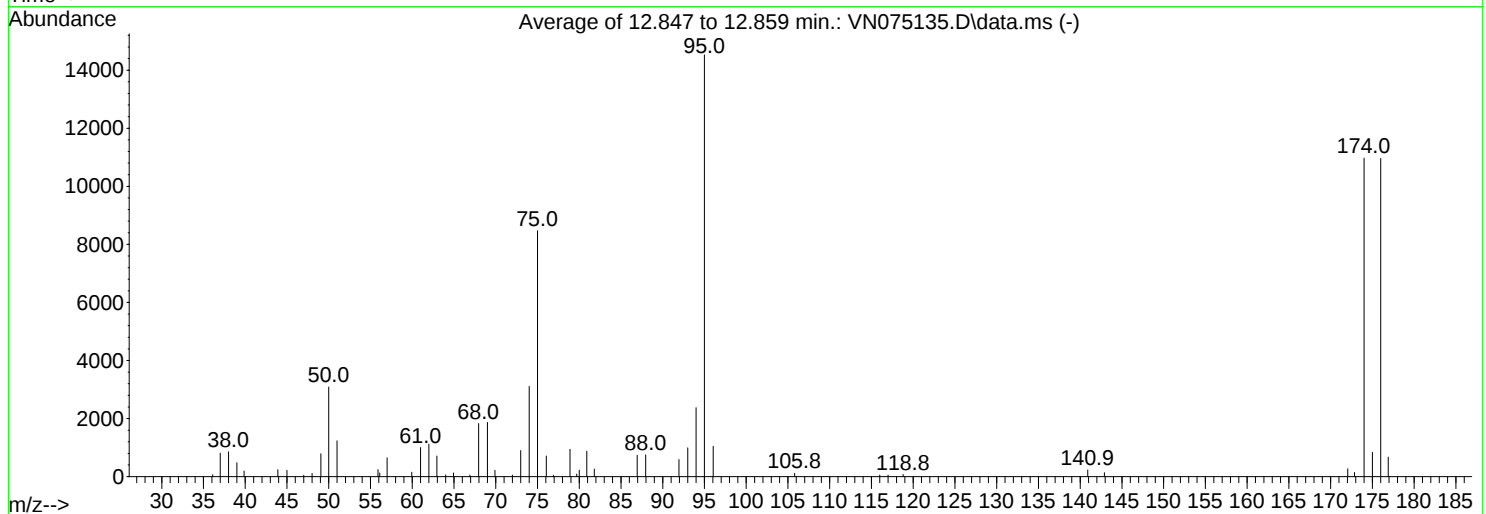


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110322\
Data File : VN075135.D
Acq On : 03 Nov 2022 11:06
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 09:48:49 2022

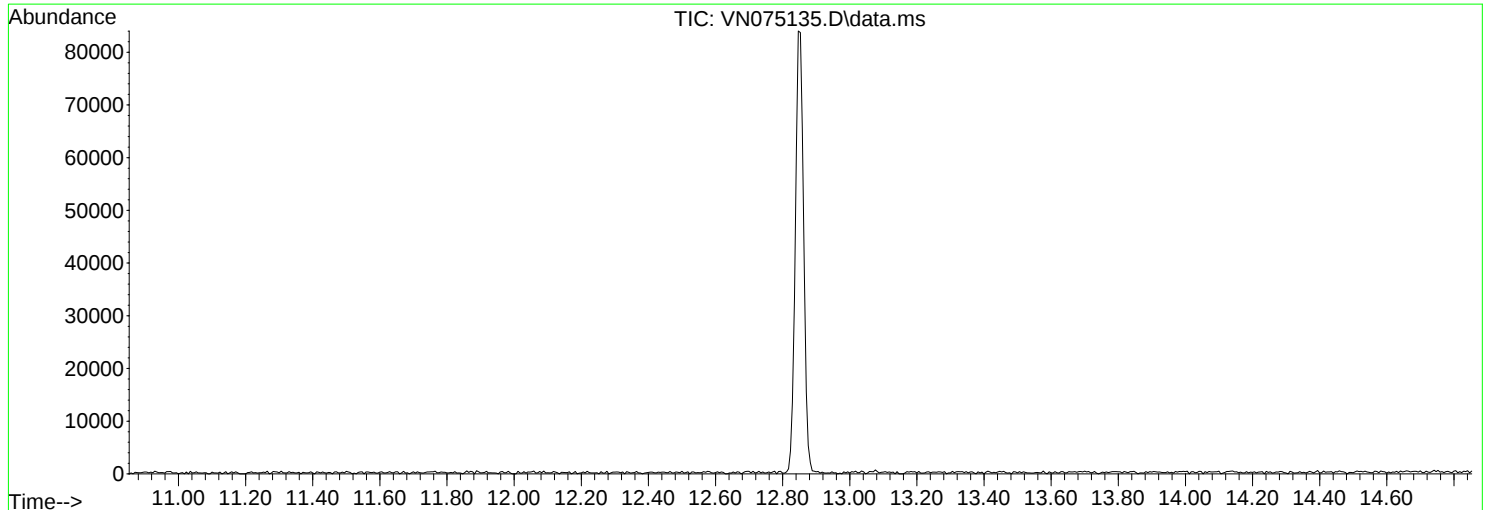

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	3089	PASS
75	95	30	60	58.3	8473	PASS
95	95	100	100	100.0	14529	PASS
96	95	5	9	7.2	1048	PASS
173	174	0.00	2	1.3	144	PASS
174	95	50	100	75.5	10971	PASS
175	174	5	9	7.6	838	PASS
176	174	95	101	99.9	10962	PASS
177	176	5	9	6.1	672	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	66	51.00	1232	67.95	1832	80.00	222
37.00	810	55.90	243	69.00	1868	80.90	87
38.00	857	56.10	125	69.90	220	81.80	26
39.00	478	57.00	648	72.00	53	86.95	74
39.85	192	59.95	157	73.00	896	87.95	752
43.90	239	61.00	1004	74.00	3107	91.95	589
45.00	222	62.00	1119	75.00	8473	93.00	991
47.00	51	62.95	709	76.05	713	94.00	2377
48.00	113	64.00	60	76.90	52	95.00	14529
49.05	790	64.95	127	78.90	942	96.05	1048
50.00	3089	66.90	54	79.70	91	105.80	118

Average of 12.847 to 12.859 min.: VN075135.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.00	56						
117.00	53						
118.80	76						
140.90	229						
142.90	140						
172.05	271						
172.85	144						
174.00	10971						
175.00	838						
176.00	10962						
176.90	672						

Instrument :

MSVOA_N

ClientSampleId :

BFB