

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110323\
 Data File : VN079839.D
 Acq On : 03 Nov 2023 11:06
 Operator : JC\MD
 Sample : VN1103MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 04 00:48:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 02 05:49:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	250556	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	481695	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	494716	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	201584	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	217824	57.062	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 114.120%	
35) Dibromofluoromethane	8.171	113	180114	52.831	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 105.660%	
50) Toluene-d8	10.571	98	643018	51.234	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 102.460%	
62) 4-Bromofluorobenzene	12.853	95	218824	52.571	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 105.140%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.365	50	1396	Below Cal		89
5) Bromomethane	2.965	94	1013	0.422	ug/l #	79
6) Chloroethane	3.159	64	1144	0.366	ug/l #	43
10) Methyl Iodide	4.589	142	1559	0.479	ug/l #	81
11) Tert butyl alcohol	5.512	59	179	0.367	ug/l #	72
13) Acrolein	4.183	56	255	3.126	ug/l	86
15) Acrylonitrile	5.730	53	892	0.587	ug/l #	79
16) Acetone	4.436	43	614	0.458	ug/l #	40
17) Carbon Disulfide	4.724	76	4722	0.607	ug/l #	75
18) Methyl Acetate	5.036	43	1314	0.205	ug/l #	50
20) Methylene Chloride	5.289	84	734	0.217	ug/l #	80
29) Tetrahydrofuran	7.859	42	396	0.310	ug/l #	20
31) Cyclohexane	8.230	56	6575	1.303	ug/l #	1
36) 1,1-Dichloropropene	8.224	75	21794	4.477	ug/l #	47
38) Carbon Tetrachloride	8.230	117	26689	5.440	ug/l #	15
51) 4-Methyl-2-Pentanone	10.447	43	1556	0.353	ug/l #	66
59) 2-Hexanone	11.200	43	2474	0.734	ug/l	73
76) 1,2,3-Trichloropropane	12.853	75	121939	25.766	ug/l #	1
77) Bromobenzene	12.982	156	788	0.210	ug/l #	53
81) trans-1,4-Dichloro-2-b...	12.853	75	121939	70.103	ug/l #	15
82) 4-Chlorotoluene	13.229	91	2256	0.203	ug/l	91
87) 1,3-Dichlorobenzene	13.729	146	1895	0.272	ug/l	95
88) 1,4-Dichlorobenzene	13.729	146	1895	0.268	ug/l	97
89) n-Butylbenzene	14.059	91	4436	0.468	ug/l	96
91) 1,2-Dichlorobenzene	14.112	146	1991	0.303	ug/l	96
92) 1,2-Dibromo-3-Chloropr...	14.729	75	369	0.401	ug/l #	61
93) 1,2,4-Trichlorobenzene	15.394	180	3356	1.073	ug/l	95
94) Hexachlorobutadiene	15.506	225	2640	1.862	ug/l	90
95) Naphthalene	15.641	128	13745	1.296	ug/l #	97
96) 1,2,3-Trichlorobenzene	15.847	180	3730	1.217	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110323\
Data File : VN079839.D
Acq On : 03 Nov 2023 11:06
Operator : JC\MD
Sample : VN1103MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Nov 04 00:48:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 02 05:49:08 2023
Response via : Initial Calibration

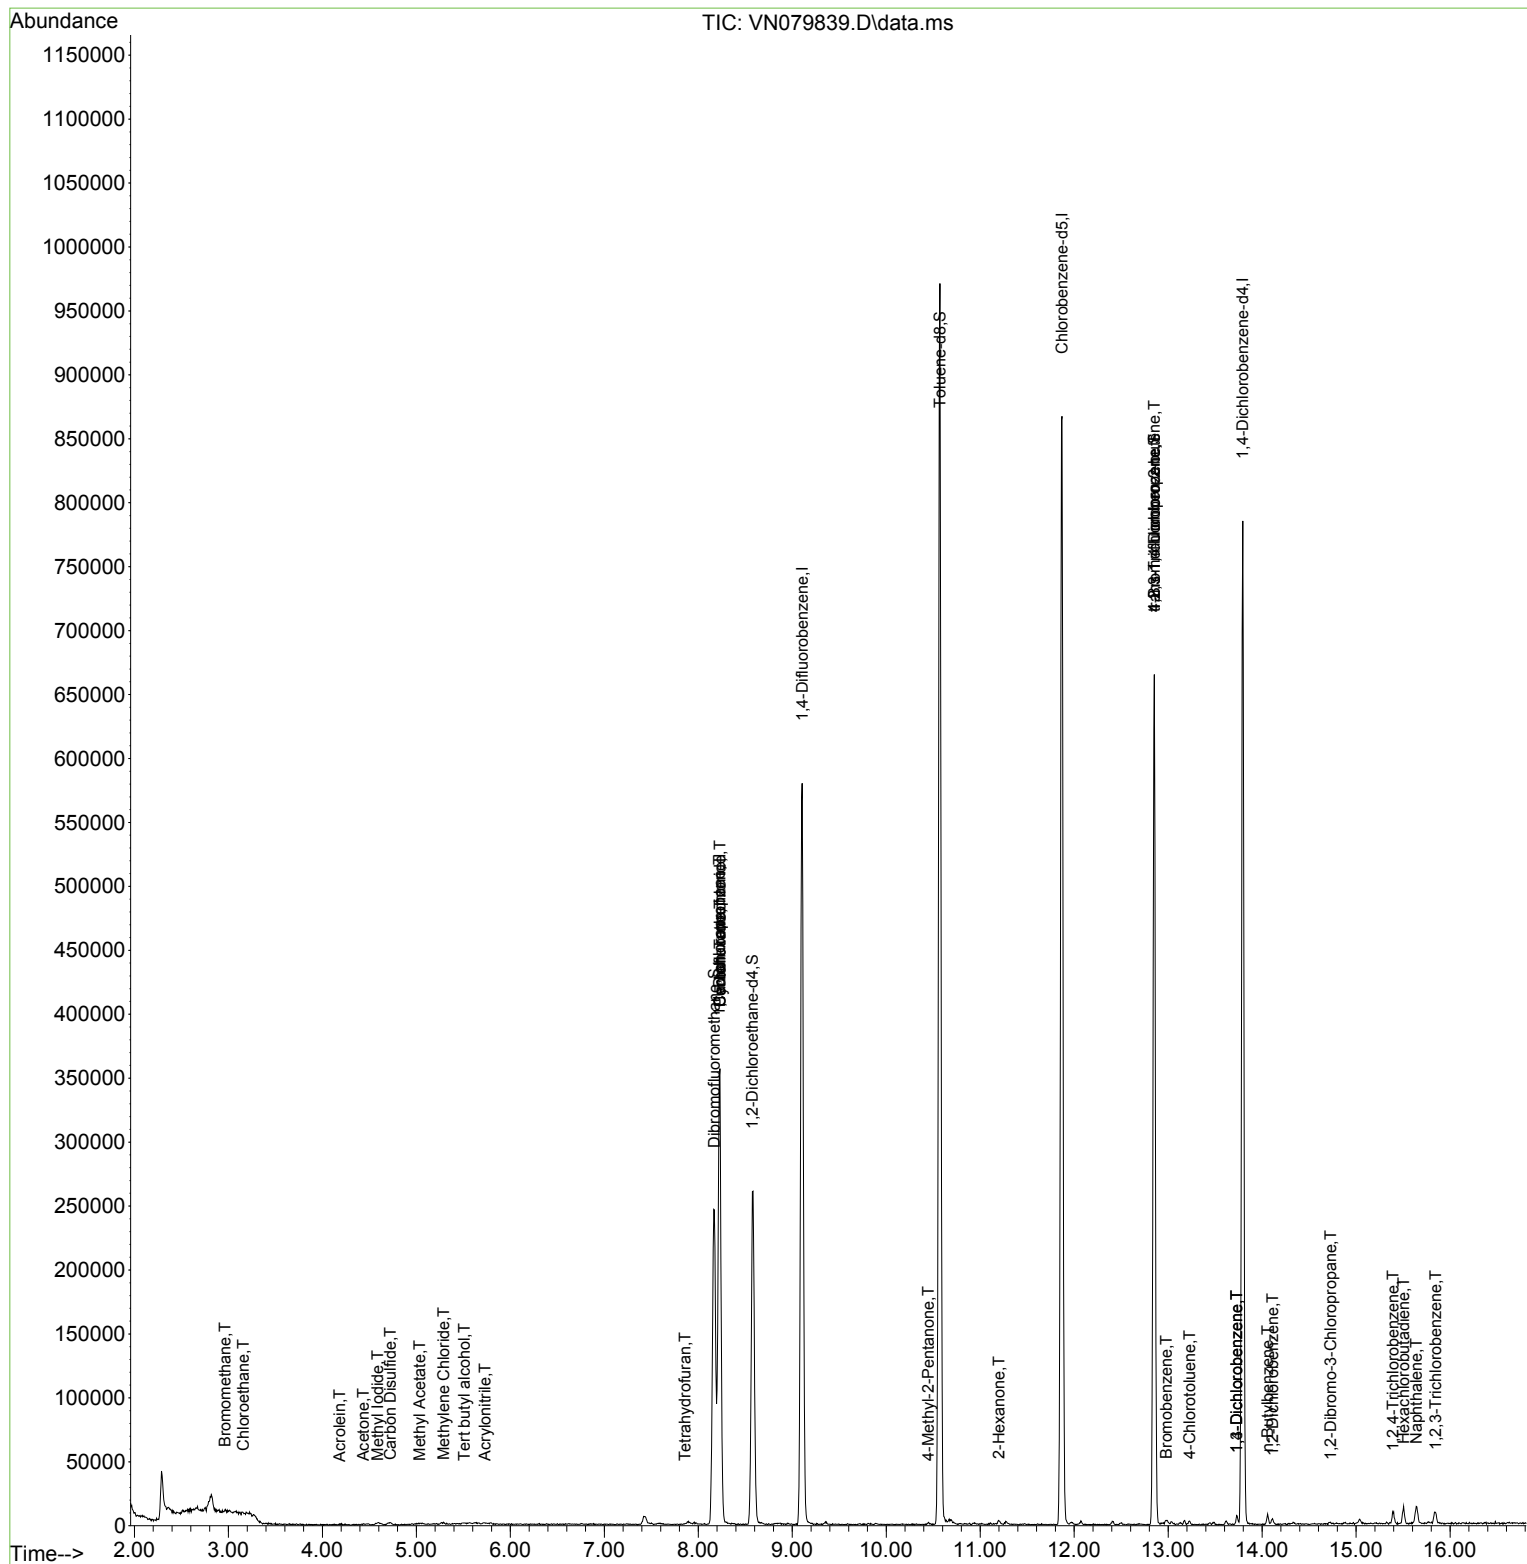



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.230 min Scan# 1

Delta R.T. 0.001 min

Lab File: VN079839.D

Acq: 03 Nov 2023 11:06

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:168 Resp: 250556

Ion Ratio Lower Upper

168 100

99 60.7 53.0 79.6

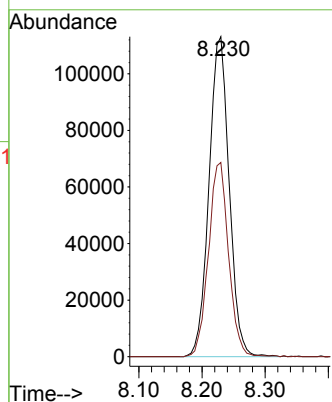

#3

Chloromethane

Concen: Below Cal

RT: 2.365 min Scan# 70

Delta R.T. 0.006 min

Lab File: VN079839.D




Acq: 03 Nov 2023 11:06

Tgt Ion: 50 Resp: 1396

Ion Ratio Lower Upper

50 100

52 39.2 26.5 39.7









#5
Bromomethane
Concen: 0.422 ug/l
RT: 2.965 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 1013
Ion Ratio Lower Upper
94 100
96 111.4 73.1 109.7#

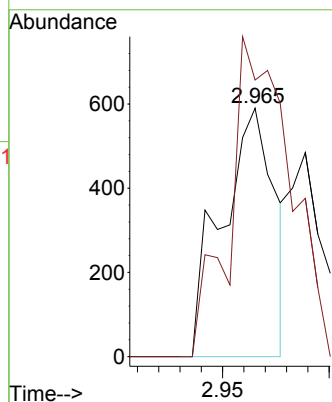

#6
Chloroethane
Concen: 0.366 ug/l
RT: 3.159 min Scan# 205
Delta R.T. 0.041 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06


Tgt Ion: 64 Resp: 1144
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#








#10
Methyl Iodide
Concen: 0.479 ug/l
RT: 4.589 min Scan# 448
Delta R.T. -0.006 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:142 Resp: 1559
Ion Ratio Lower Upper
142 100
127 37.8 37.6 56.4
141 0.0 11.4 17.0#

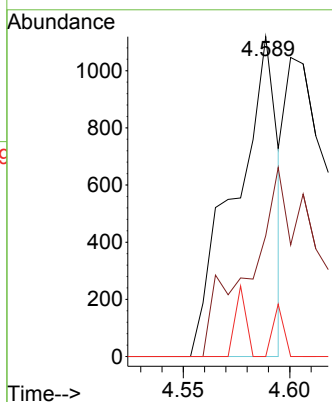

#11
Tert butyl alcohol
Concen: 0.367 ug/l
RT: 5.512 min Scan# 605
Delta R.T. -0.006 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06


Tgt Ion: 59 Resp: 179
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

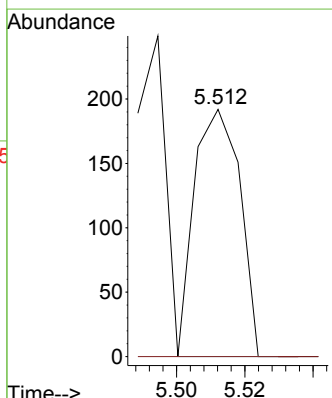



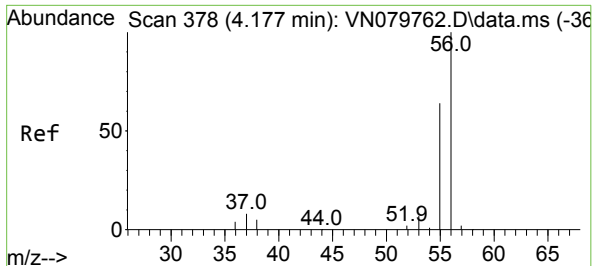


#13
Acrolein
Concen: 3.126 ug/l
RT: 4.183 min Scan# 31
Delta R.T. -0.000 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06

Instrument :
MSVOA_N
ClientSampleId :



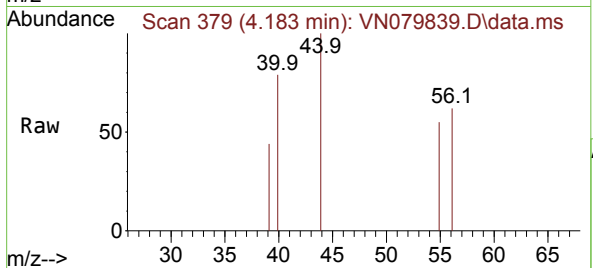



Tgt Ion: 56 Resp: 255
Ion Ratio Lower Upper
56 100
55 56.5 54.5 81.7

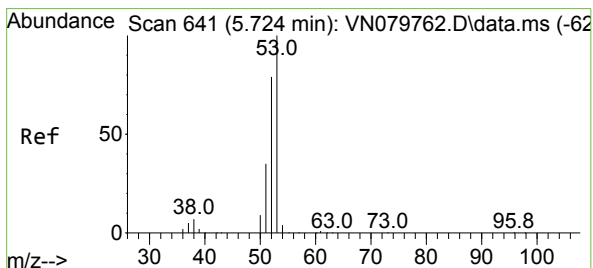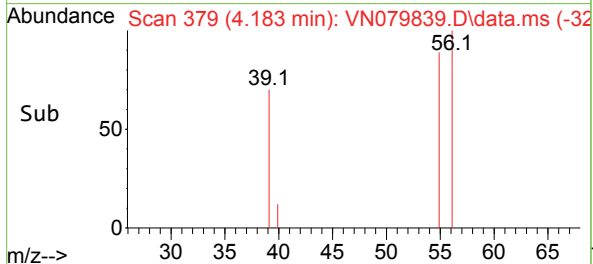

#15
Acrylonitrile
Concen: 0.587 ug/l
RT: 5.730 min Scan# 642
Delta R.T. 0.006 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06

Tgt Ion: 53 Resp: 892
Ion Ratio Lower Upper
53 100
52 89.0 65.3 97.9
51 6.8 28.9 43.3#


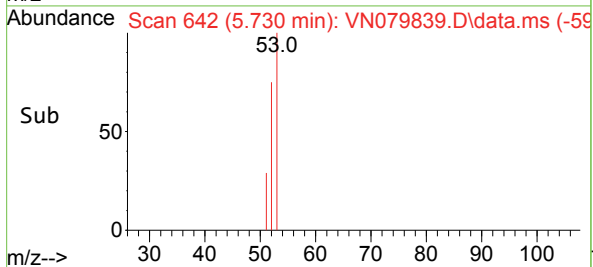

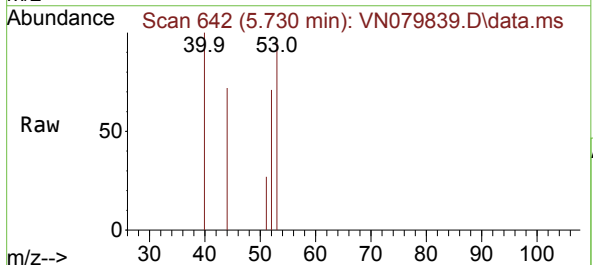




#16
Acetone
Concen: 0.458 ug/l
RT: 4.436 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 614
Ion Ratio Lower Upper
43 100
58 0.0 28.0 42.0#

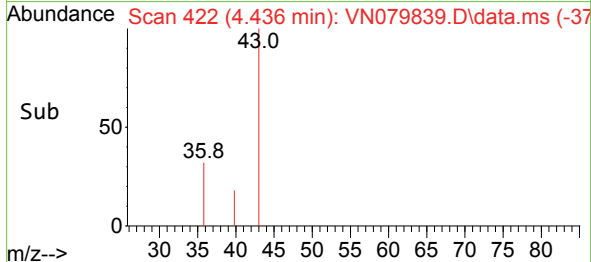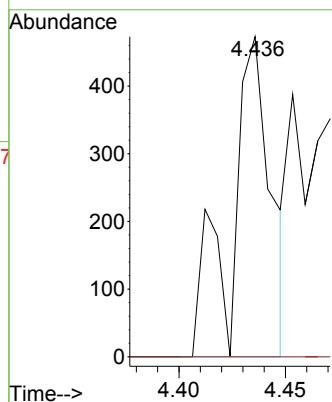

#17
Carbon Disulfide
Concen: 0.607 ug/l
RT: 4.724 min Scan# 471
Delta R.T. 0.012 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06

Tgt Ion: 76 Resp: 4722
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.0#


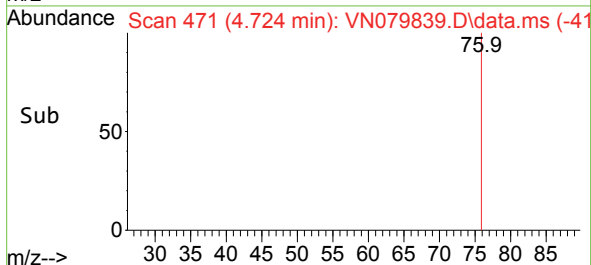

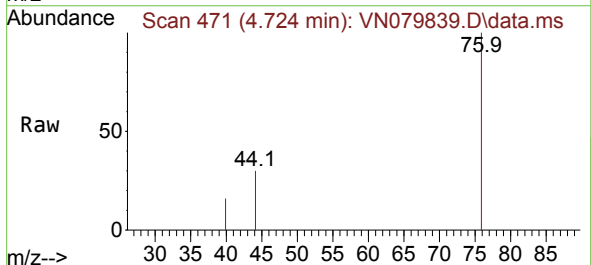




#18
Methyl Acetate
Concen: 0.205 ug/l
RT: 5.036 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 1314
Ion Ratio Lower Upper
43 100
74 4.5 26.2 39.4#

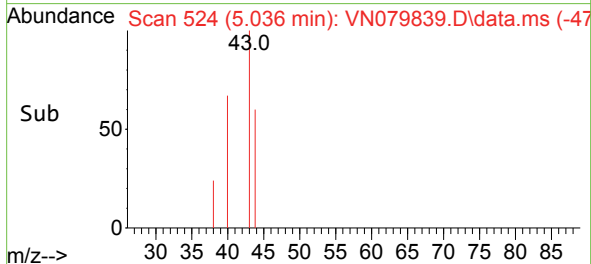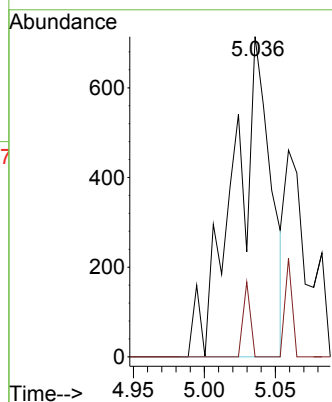

#20
Methylene Chloride
Concen: 0.217 ug/l
RT: 5.289 min Scan# 567
Delta R.T. 0.018 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06

Tgt Ion: 84 Resp: 734
Ion Ratio Lower Upper
84 100
49 86.0 79.7 119.5
51 0.0 25.2 37.8#
86 57.5 53.3 79.9

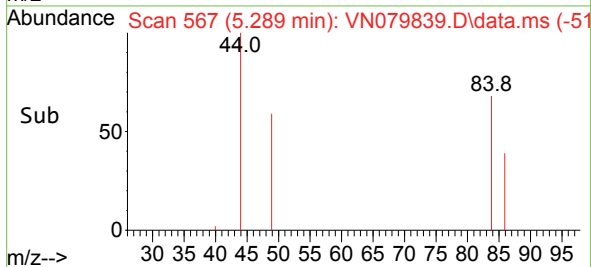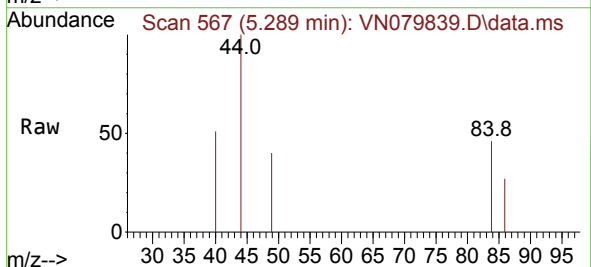



#29

Tetrahydrofuran

Concen: 0.310 ug/l

RT: 7.859 min Scan# 1

Delta R.T. 0.018 min

Lab File: VN079839.D

Acq: 03 Nov 2023 11:06

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 42 Resp: 396

Ion Ratio Lower Upper

42 100

72 0.0 49.8 74.6#

71 0.0 47.4 71.2#

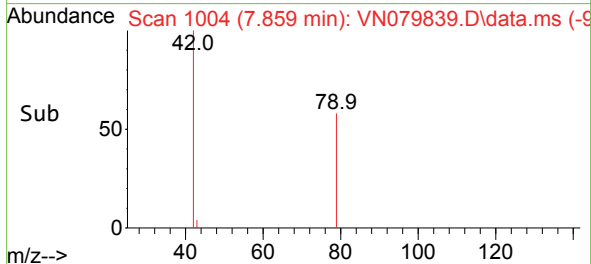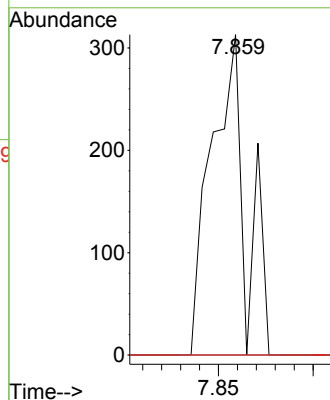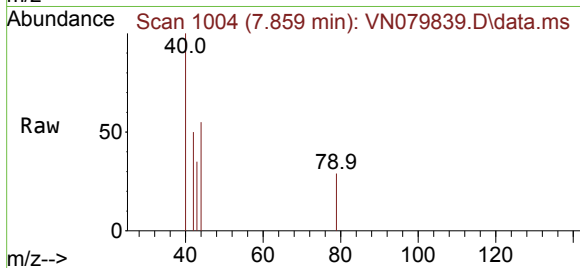

#31

Cyclohexane

Concen: 1.303 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.029 min

Lab File: VN079839.D

Acq: 03 Nov 2023 11:06




Tgt Ion: 56 Resp: 6575


Ion Ratio Lower Upper

56 100

69 179.9 26.8 40.2#

84 152.2 81.8 122.6#

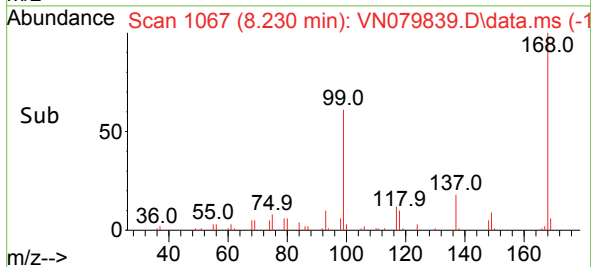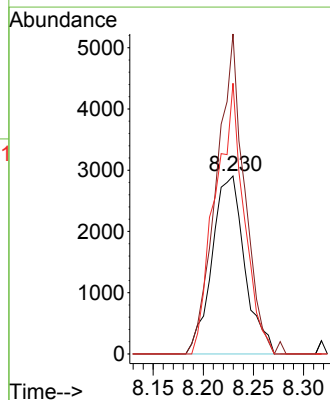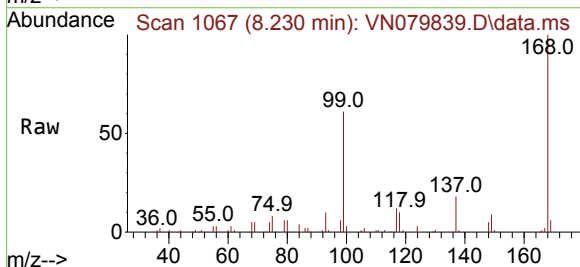



#33

1,2-Dichloroethane-d4

Concen: 57.062 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VN079839.D

Acq: 03 Nov 2023 11:06

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 217824

Ion Ratio Lower Upper

65 100

67 51.0 0.0 106.6

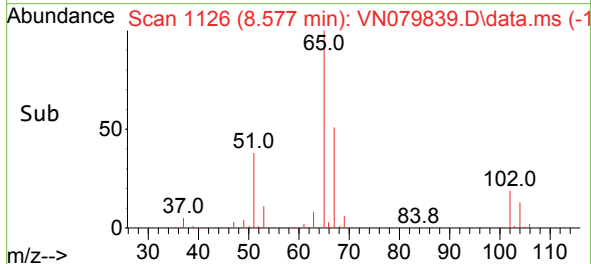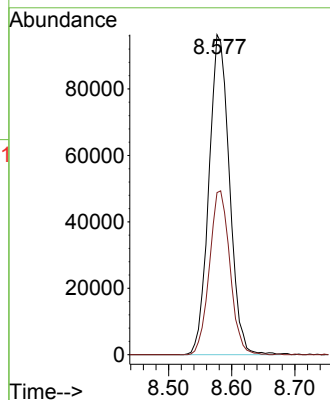

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. 0.000 min

Lab File: VN079839.D

Acq: 03 Nov 2023 11:06




Tgt Ion: 114 Resp: 481695


Ion Ratio Lower Upper

114 100

63 21.0 0.0 36.4

88 15.8 0.0 30.6

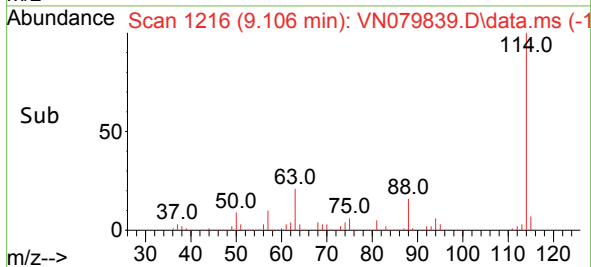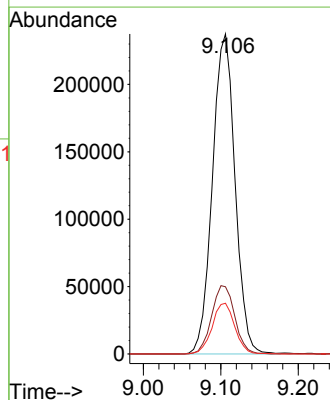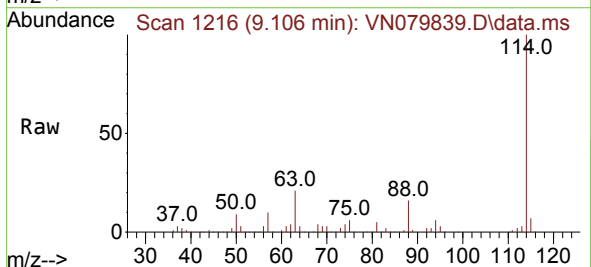



#35

Dibromofluoromethane

Concen: 52.831 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.000 min


Lab File: VN079839.D

Acq: 03 Nov 2023 11:06

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:113 Resp: 180114

Ion Ratio Lower Upper

113 100

111 102.7 82.6 123.8

192 17.9 12.7 19.1

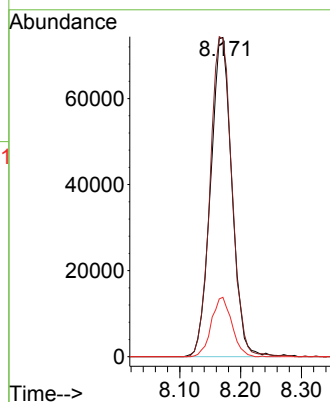

#36

1,1-Dichloropropene

Concen: 4.477 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.153 min

Lab File: VN079839.D

Acq: 03 Nov 2023 11:06




Tgt Ion: 75 Resp: 21794


Ion Ratio Lower Upper

75 100

110 8.4 19.1 57.3#

77 0.0 25.0 37.4#

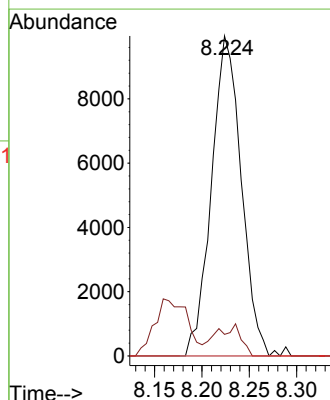



#38

Carbon Tetrachloride

Concen: 5.440 ug/l

RT: 8.230 min Scan# 1

Delta R.T. -0.129 min


Lab File: VN079839.D

Acq: 03 Nov 2023 11:06

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:117 Resp: 26689

Ion Ratio Lower Upper

117 100

119 4.3 77.3 115.9#

121 0.0 23.3 34.9#

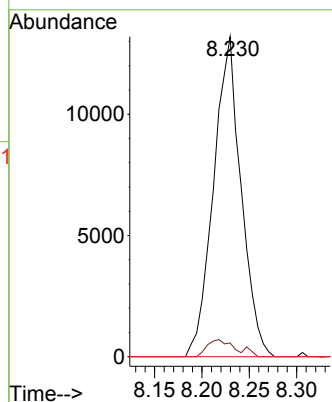

#50

Toluene-d8

Concen: 51.234 ug/l

RT: 10.571 min Scan# 1465

Delta R.T. 0.000 min

Lab File: VN079839.D




Acq: 03 Nov 2023 11:06


Tgt Ion: 98 Resp: 643018

Ion Ratio Lower Upper

98 100

100 64.2 52.0 78.0


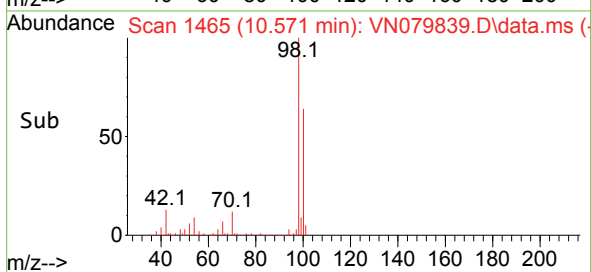
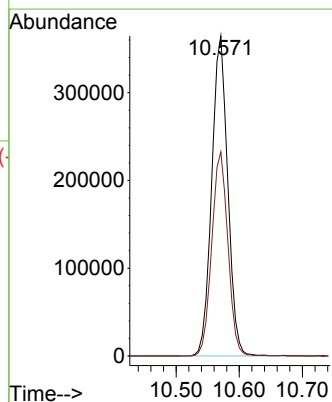
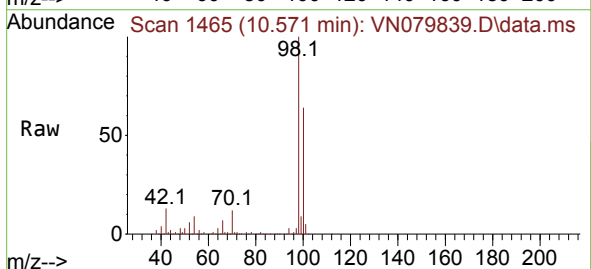


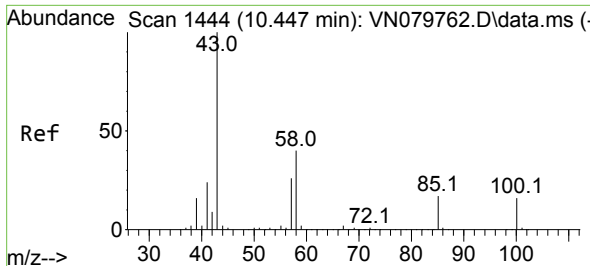

#51
4-Methyl-2-Pentanone
Concen: 0.353 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 1556
Ion Ratio Lower Upper
43 100
58 23.5 36.6 54.8#

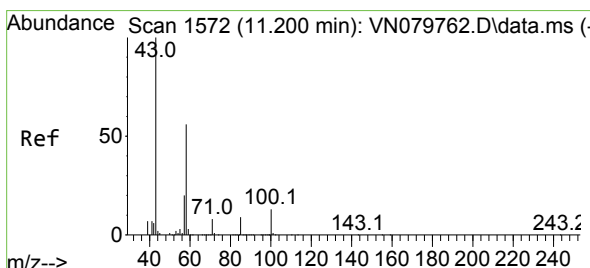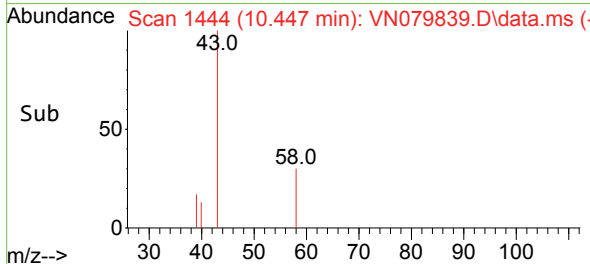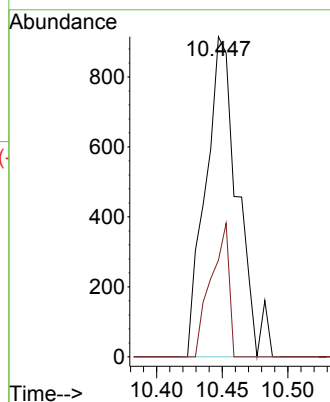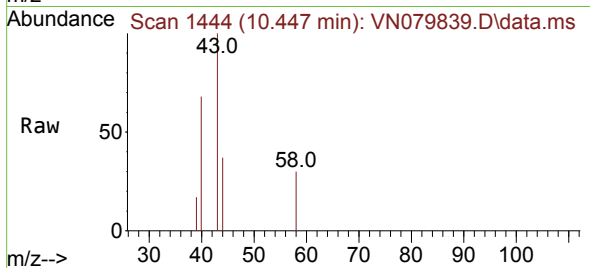

#59
2-Hexanone
Concen: 0.734 ug/l
RT: 11.200 min Scan# 1572
Delta R.T. 0.000 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06

Tgt Ion: 43 Resp: 2474
Ion Ratio Lower Upper
43 100
58 42.7 31.7 95.1


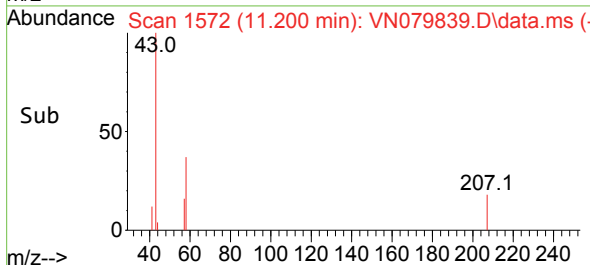
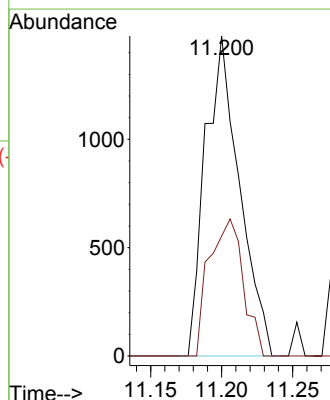
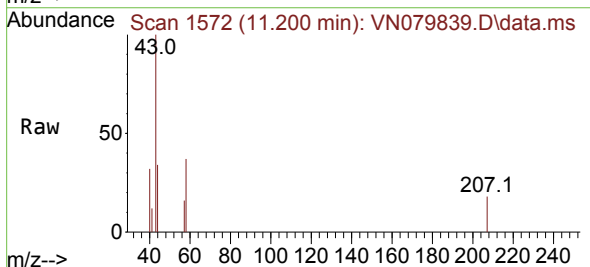


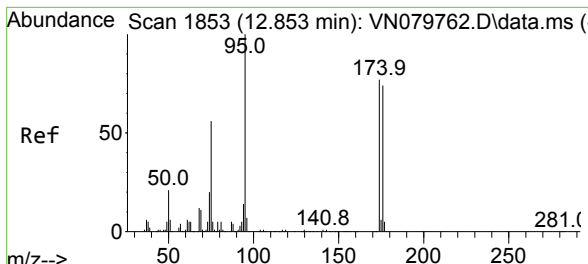

#62
 4-Bromofluorobenzene
 Concen: 52.571 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. 0.000 min
 Lab File: VN079839.D
 Acq: 03 Nov 2023 11:06




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:	95	Resp:	218824
Ion	Ratio	Lower	Upper
95	100		
174	75.5	0.0	143.8
176	71.9	0.0	135.8

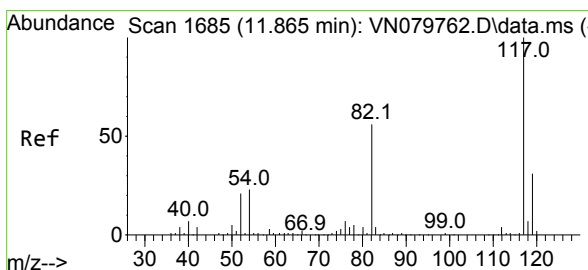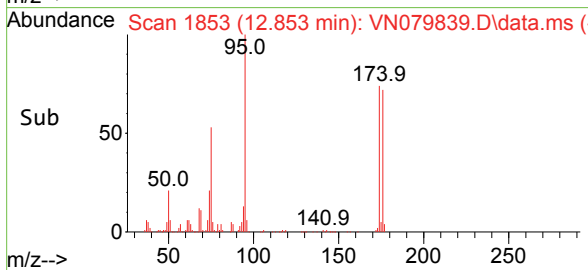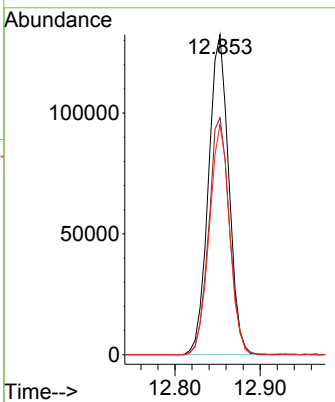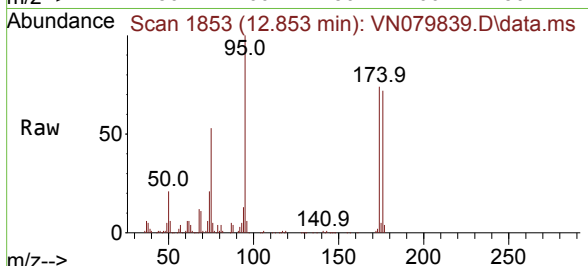

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 11.871 min Scan# 1686
 Delta R.T. 0.000 min
 Lab File: VN079839.D
 Acq: 03 Nov 2023 11:06

Tgt Ion:	117	Resp:	494716
Ion	Ratio	Lower	Upper
117	100		
82	56.7	44.0	66.0
119	32.2	25.6	38.4

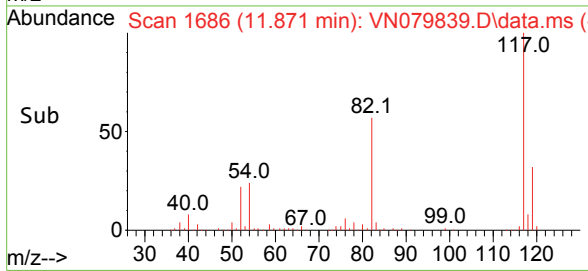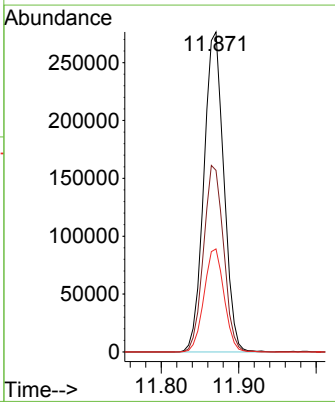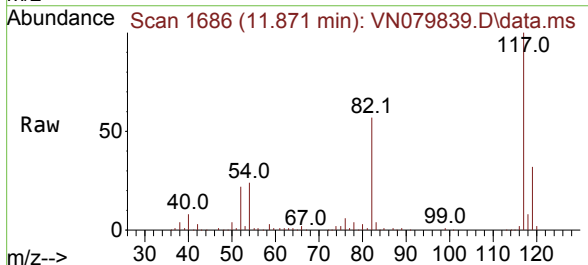



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. 0.000 min

Lab File: VN079839.D

Acq: 03 Nov 2023 11:06

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:152 Resp: 201584

Ion Ratio Lower Upper

152 100

115 59.8 32.3 96.8

150 157.8 0.0 355.8

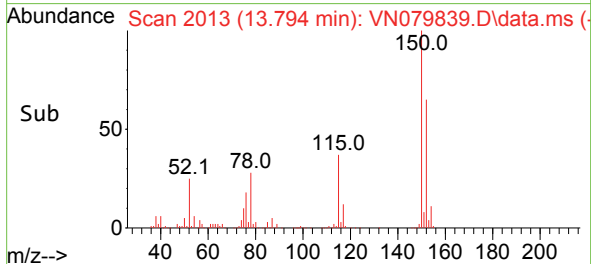

#76

1,2,3-Trichloropropane

Concen: 25.766 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.141 min

Lab File: VN079839.D




Acq: 03 Nov 2023 11:06


Tgt Ion: 75 Resp: 121939

Ion Ratio Lower Upper

75 100

77 1.4 84.5 253.5#




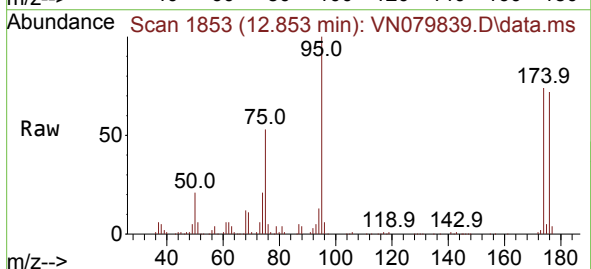




#77
Bromobenzene
Concen: 0.210 ug/l
RT: 12.982 min Scan# 1875
Delta R.T. 0.000 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:156 Resp: 788
Ion Ratio Lower Upper
156 100
77 106.9 107.7 323.3#
158 97.6 48.4 145.3

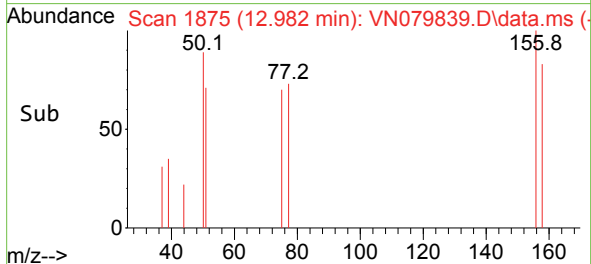

#81
trans-1,4-Dichloro-2-butene
Concen: 70.103 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.118 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06

Tgt Ion: 75 Resp: 121939
Ion Ratio Lower Upper
75 100
53 0.1 67.4 101.2#
89 0.0 38.8 58.2#




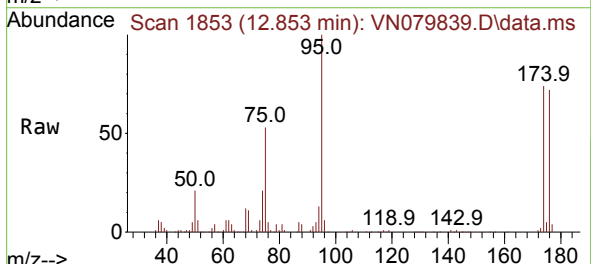


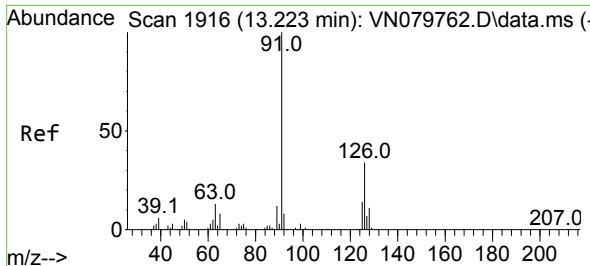

#82
4-Chlorotoluene
Concen: 0.203 ug/l
RT: 13.229 min Scan# 1916
Delta R.T. 0.006 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 2256
Ion Ratio Lower Upper
91 100
126 28.3 16.7 50.0

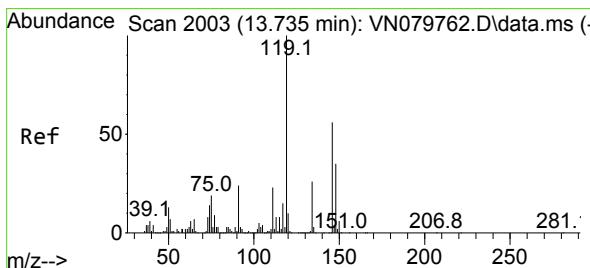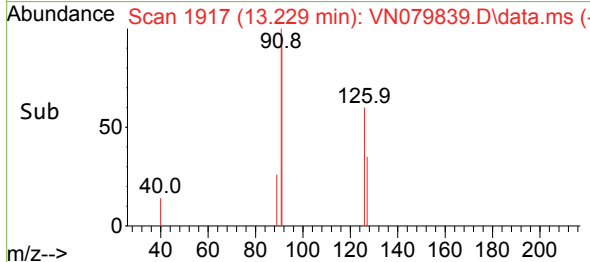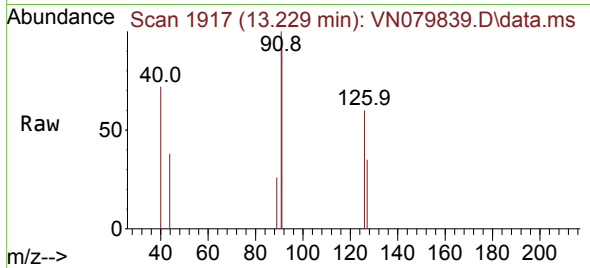

#87
1,3-Dichlorobenzene
Concen: 0.272 ug/l
RT: 13.729 min Scan# 2002
Delta R.T. -0.006 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06

Tgt Ion: 146 Resp: 1895
Ion Ratio Lower Upper
146 100
111 37.6 22.1 66.3
148 62.5 32.0 96.0


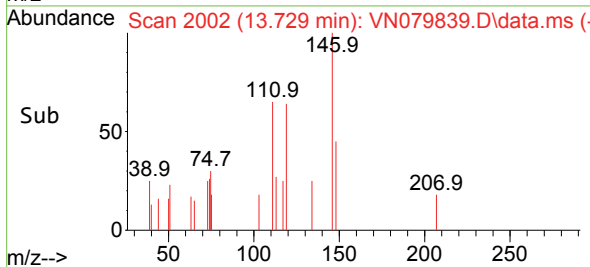

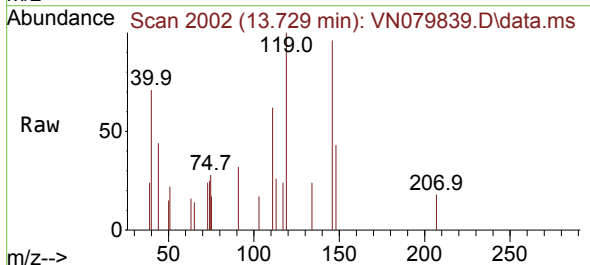


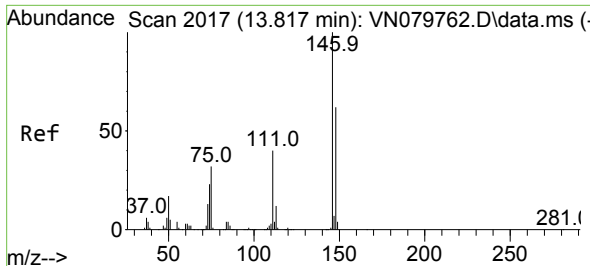

#88
1,4-Dichlorobenzene
Concen: 0.268 ug/l
RT: 13.729 min Scan# 2017
Delta R.T. -0.088 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:146 Resp: 1895
Ion Ratio Lower Upper
146 100
111 37.6 20.6 61.8
148 62.5 31.6 94.8

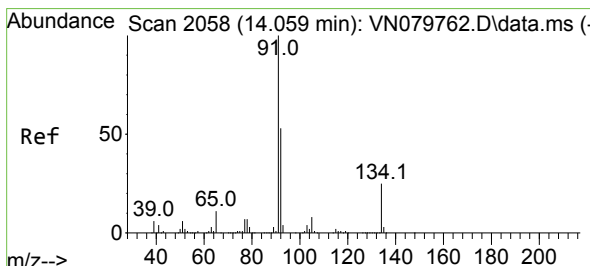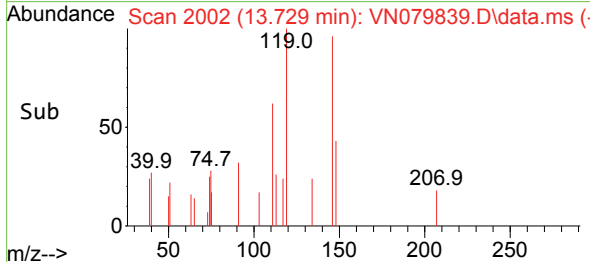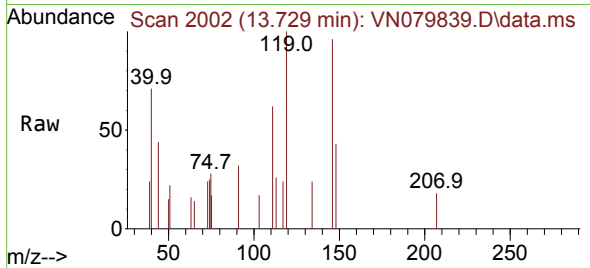

#89
n-Butylbenzene
Concen: 0.468 ug/l
RT: 14.059 min Scan# 2058
Delta R.T. 0.000 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06


Tgt Ion: 91 Resp: 4436
Ion Ratio Lower Upper
91 100
92 51.8 26.4 79.0
134 19.7 12.6 37.6

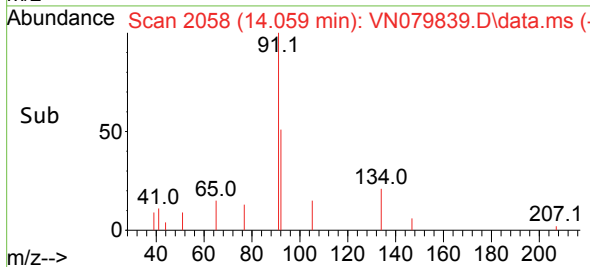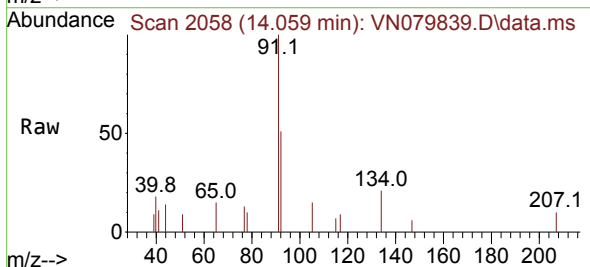






#91
 1,2-Dichlorobenzene
 Concen: 0.303 ug/l
 RT: 14.112 min Scan# 2067
 Delta R.T. 0.006 min
 Lab File: VN079839.D
 Acq: 03 Nov 2023 11:06


Instrument :
 MSVOA_N
 ClientSampleId :





Tgt Ion:146 Resp: 1991
 Ion Ratio Lower Upper
 146 100
 111 44.5 22.0 66.0
 148 58.5 31.8 95.3

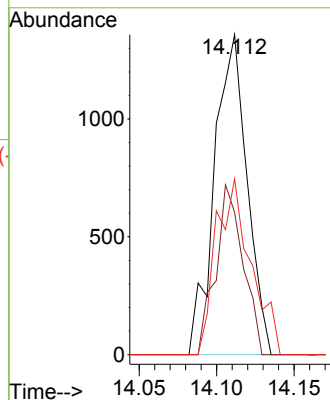


#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.401 ug/l
 RT: 14.729 min Scan# 2172
 Delta R.T. 0.006 min
 Lab File: VN079839.D
 Acq: 03 Nov 2023 11:06

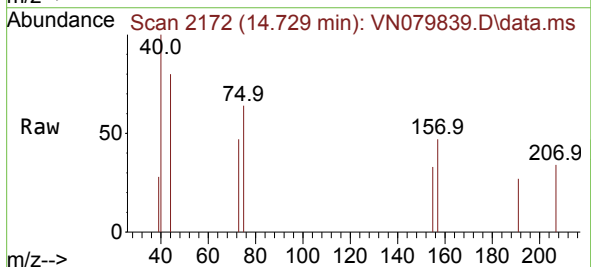


Tgt Ion: 75 Resp: 369
 Ion Ratio Lower Upper
 75 100
 155 33.6 39.1 117.2#
 157 71.5 50.3 150.9

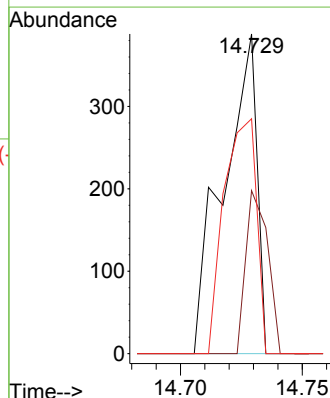



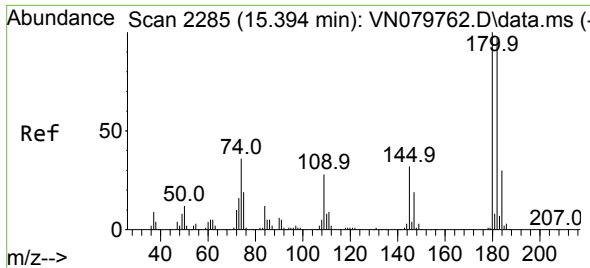


#93
1,2,4-Trichlorobenzene
Concen: 1.073 ug/l
RT: 15.394 min Scan# 21
Delta R.T. 0.000 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06

Instrument :
MSVOA_N
ClientSampleId :



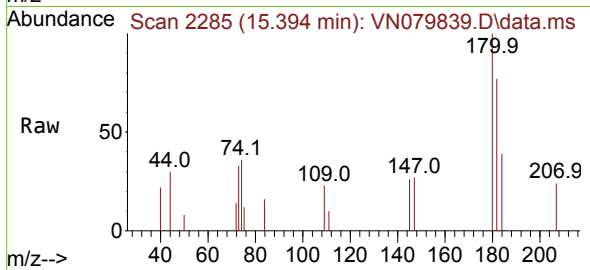



Tgt Ion:180 Resp: 3356
Ion Ratio Lower Upper
180 100
182 86.3 46.1 138.2
145 33.6 16.6 49.8

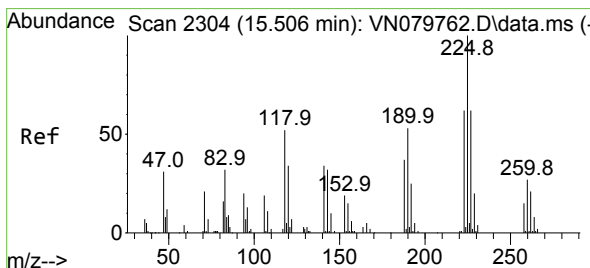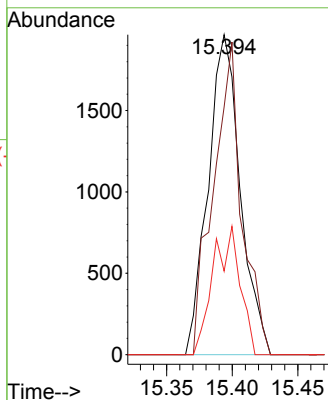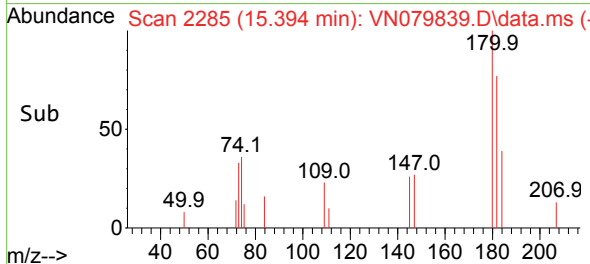

#94
Hexachlorobutadiene
Concen: 1.862 ug/l
RT: 15.506 min Scan# 2304
Delta R.T. 0.000 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06

Tgt Ion:225 Resp: 2640
Ion Ratio Lower Upper
225 100
223 55.9 31.3 93.8
227 55.3 31.9 95.9


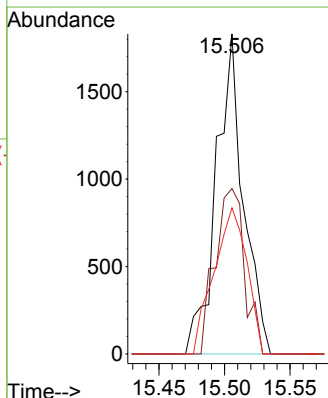
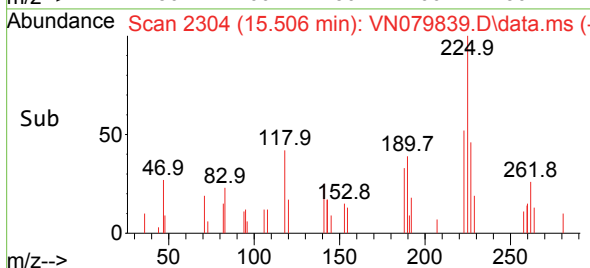
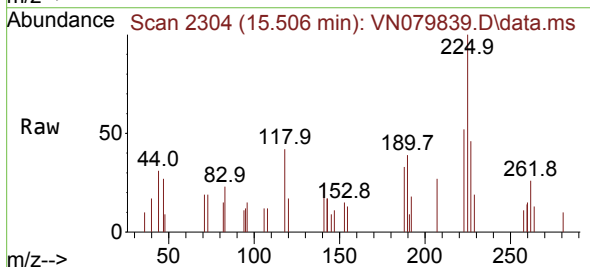


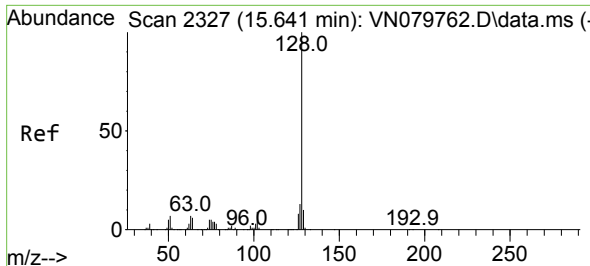

#95
Naphthalene
Concen: 1.296 ug/l
RT: 15.641 min Scan# 2327
Delta R.T. 0.000 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:128 Resp: 13745
Ion Ratio Lower Upper
128 100
127 12.4 10.0 15.0
129 13.2 8.7 13.1#

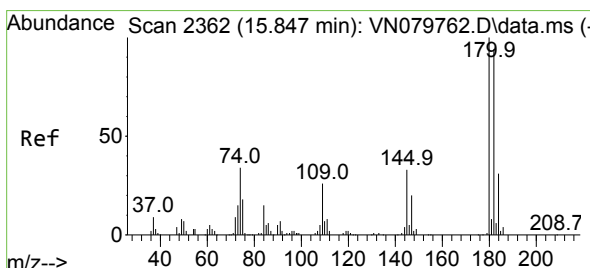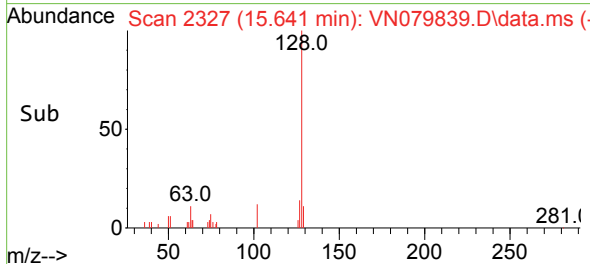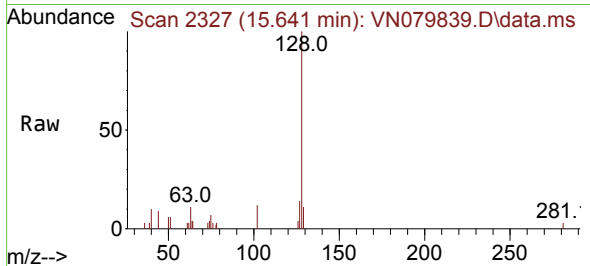

#96
1,2,3-Trichlorobenzene
Concen: 1.217 ug/l
RT: 15.847 min Scan# 2362
Delta R.T. 0.006 min
Lab File: VN079839.D
Acq: 03 Nov 2023 11:06

Tgt Ion:180 Resp: 3730
Ion Ratio Lower Upper
180 100
182 92.3 46.2 138.6
145 35.7 17.5 52.6

