

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110323\
 Data File : VN079851.D
 Acq On : 03 Nov 2023 16:04
 Operator : JC\MD
 Sample : 05139-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Nov 04 00:54:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 02 05:49:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	259141	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	515651	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	514574	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	199411	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	223435	56.593	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	113.180%
35) Dibromofluoromethane	8.171	113	182029	49.877	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.760%
50) Toluene-d8	10.571	98	636315	47.361	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	94.720%
62) 4-Bromofluorobenzene	12.853	95	208871	46.876	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110323\
Data File : VN079851.D
Acq On : 03 Nov 2023 16:04
Operator : JC\MD
Sample : 05139-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Nov 04 00:54:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 02 05:49:08 2023
Response via : Initial Calibration




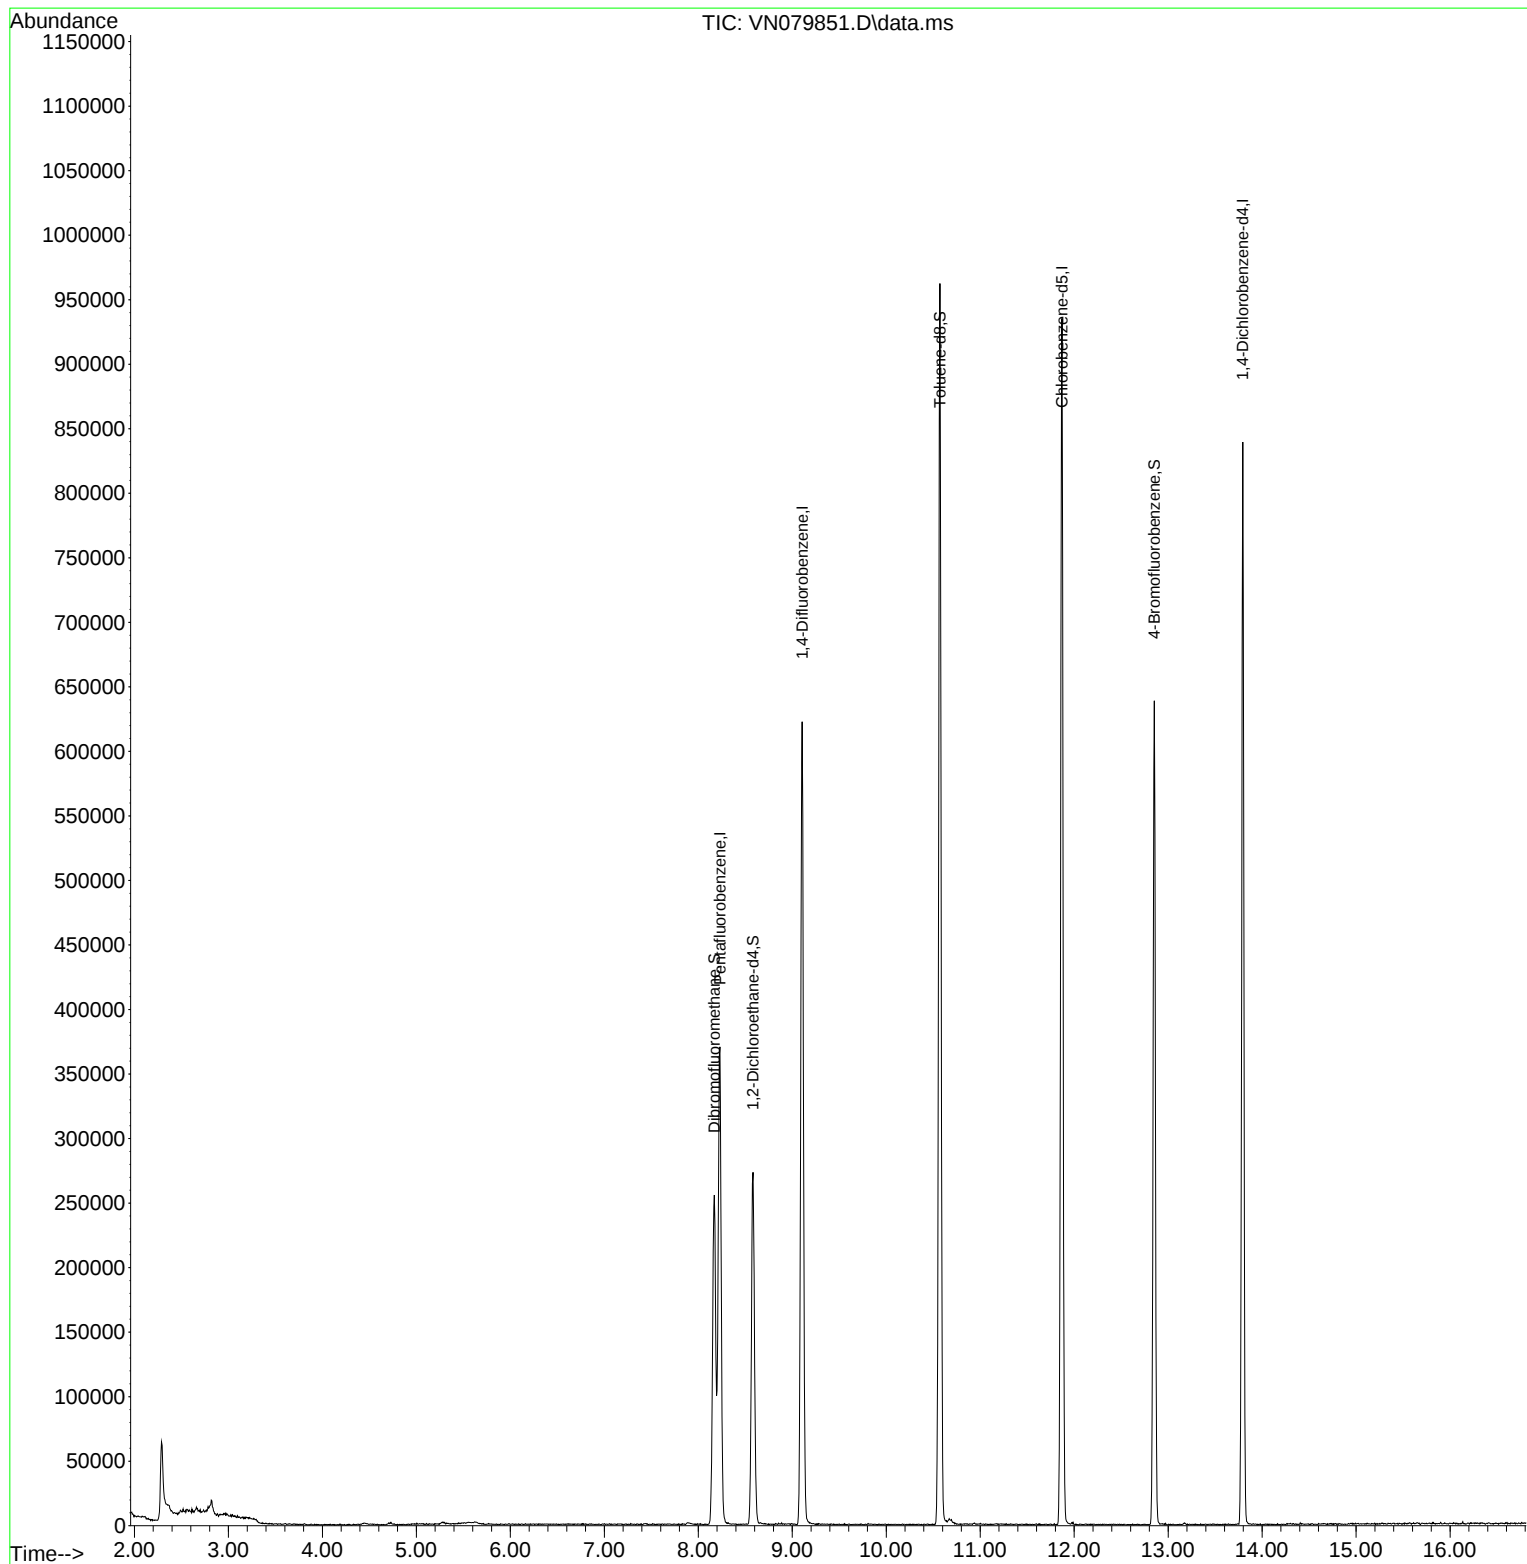


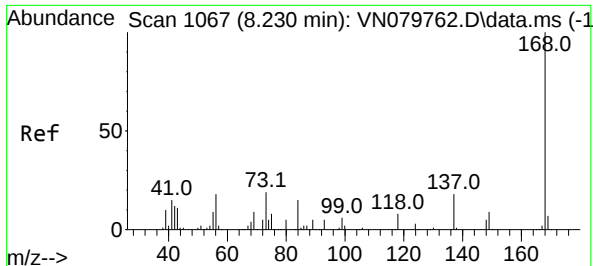

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. 0.001 min
Lab File: VN079851.D
Acq: 03 Nov 2023 16:04




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:168 Resp: 259141
Ion Ratio Lower Upper
168 100
99 62.3 53.0 79.6

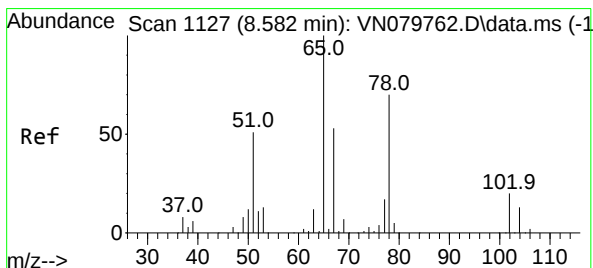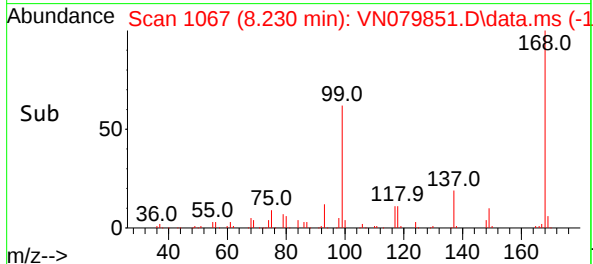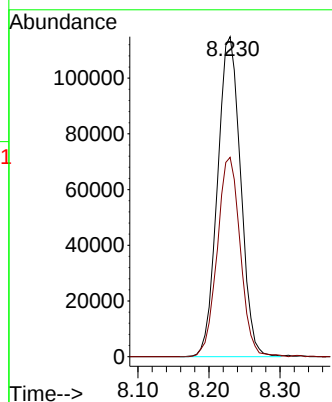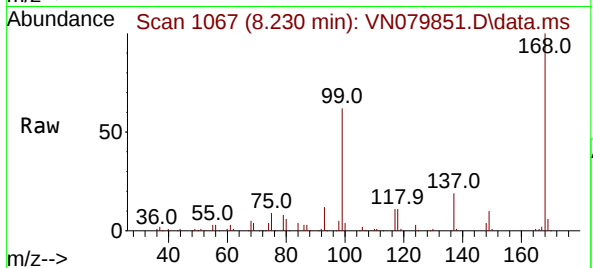

#33
1,2-Dichloroethane-d4
Concen: 56.593 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VN079851.D
Acq: 03 Nov 2023 16:04

Tgt Ion: 65 Resp: 223435
Ion Ratio Lower Upper
65 100
67 52.6 0.0 106.6


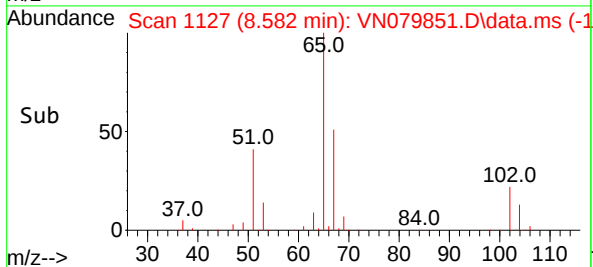
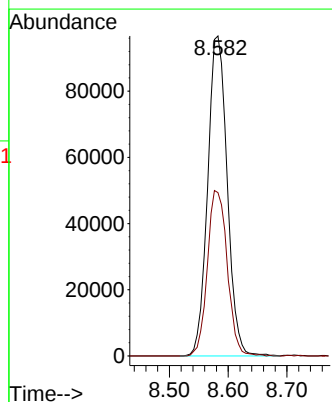
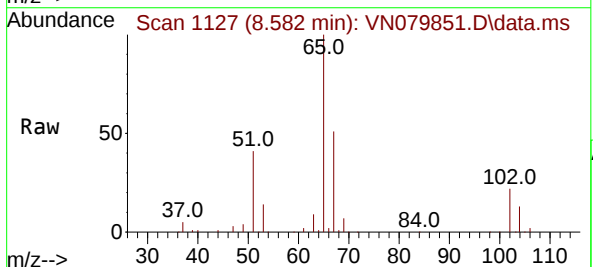


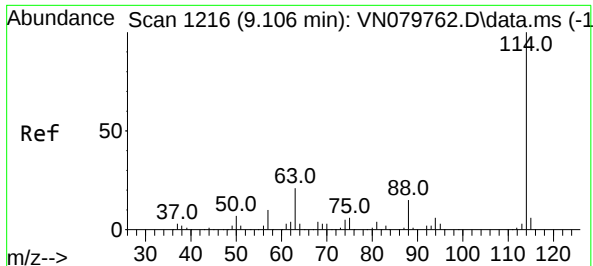

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN079851.D
Acq: 03 Nov 2023 16:04




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:114 Resp: 515651
Ion Ratio Lower Upper
114 100
63 22.8 0.0 36.4
88 15.7 0.0 30.6

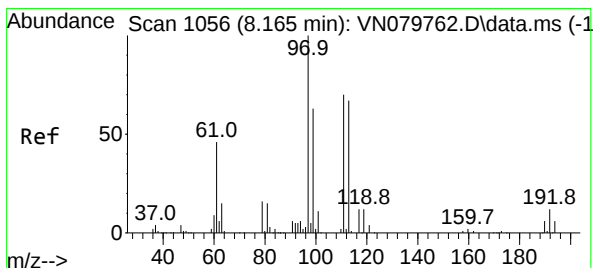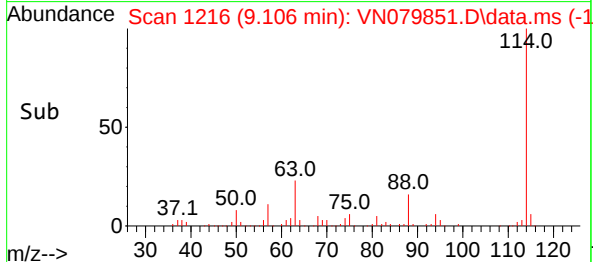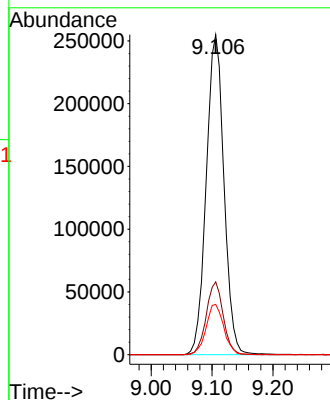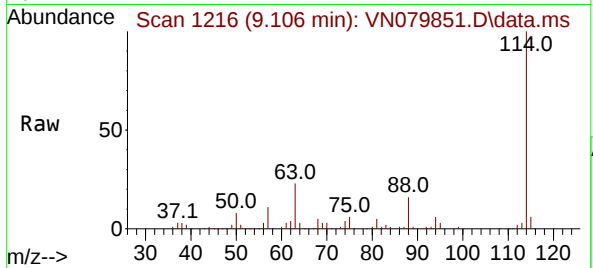

#35
Dibromofluoromethane
Concen: 49.877 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. 0.000 min
Lab File: VN079851.D
Acq: 03 Nov 2023 16:04

Tgt Ion:113 Resp: 182029
Ion Ratio Lower Upper
113 100
111 103.9 82.6 123.8
192 17.8 12.7 19.1


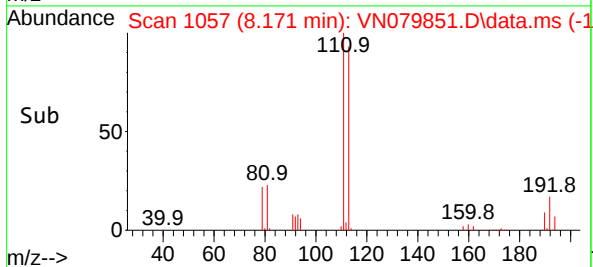
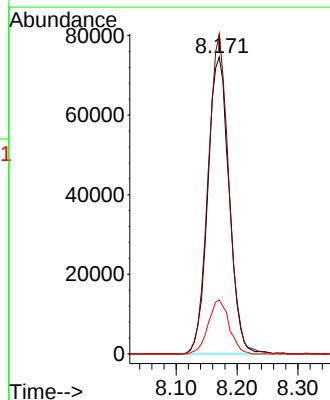
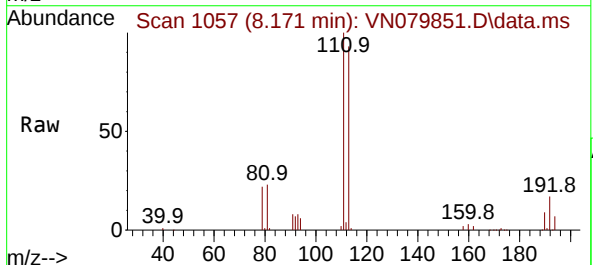


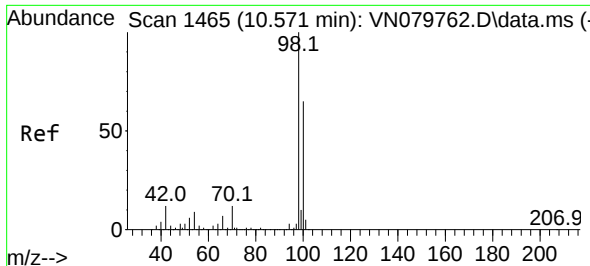

#50
Toluene-d8
Concen: 47.361 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN079851.D
Acq: 03 Nov 2023 16:04




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion: 98 Resp: 636315
Ion Ratio Lower Upper
98 100
100 63.9 52.0 78.0

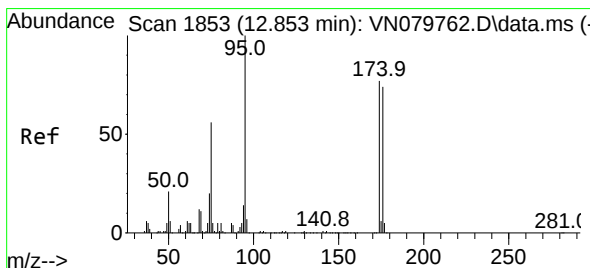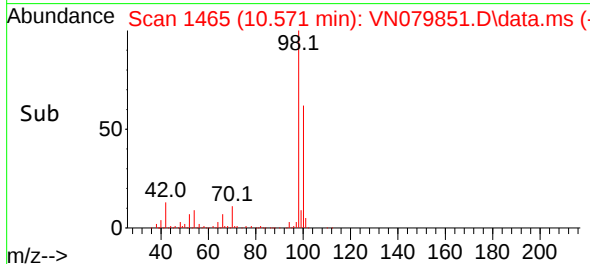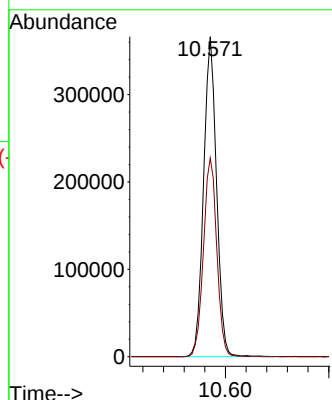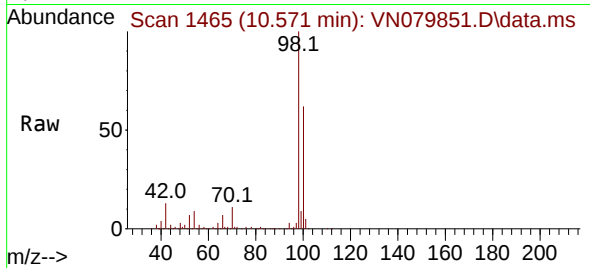

#62
4-Bromofluorobenzene
Concen: 46.876 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN079851.D
Acq: 03 Nov 2023 16:04

Tgt Ion: 95 Resp: 208871
Ion Ratio Lower Upper
95 100
174 77.6 0.0 143.8
176 71.7 0.0 135.8


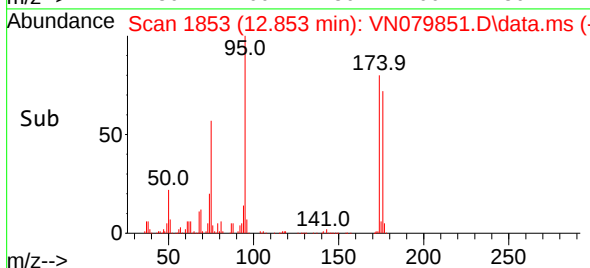
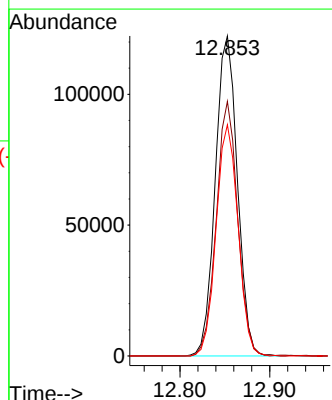
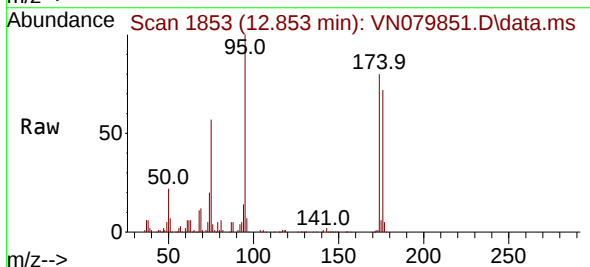


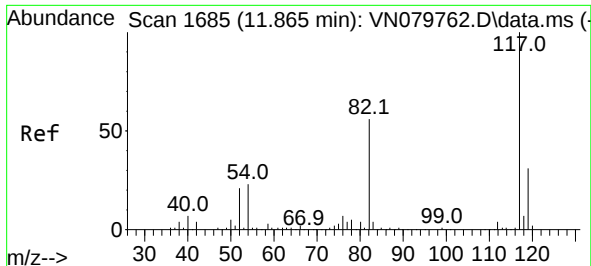

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN079851.D
Acq: 03 Nov 2023 16:04

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tgt Ion:117 Resp: 514574
Ion Ratio Lower Upper
117 100
82 57.7 44.0 66.0
119 31.9 25.6 38.4

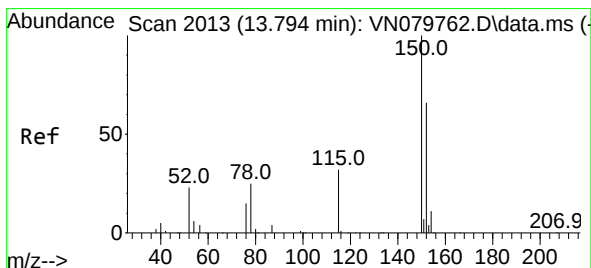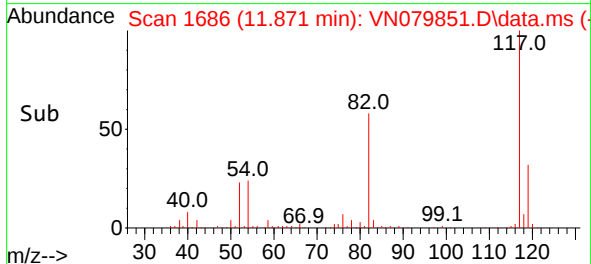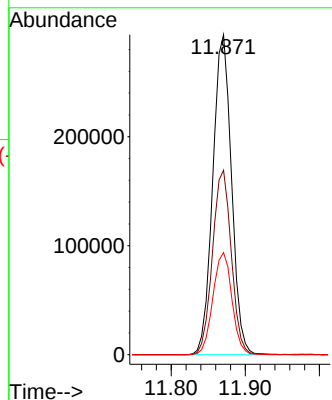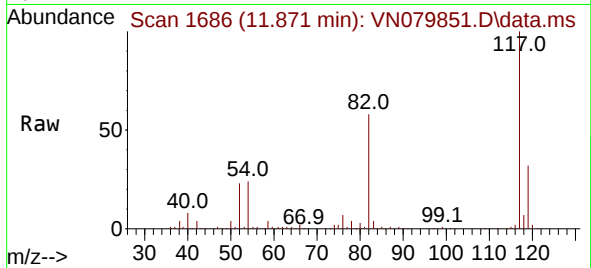

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN079851.D
Acq: 03 Nov 2023 16:04

Tgt Ion:152 Resp: 199411
Ion Ratio Lower Upper
152 100
115 63.5 32.3 96.8
150 164.3 0.0 355.8

