
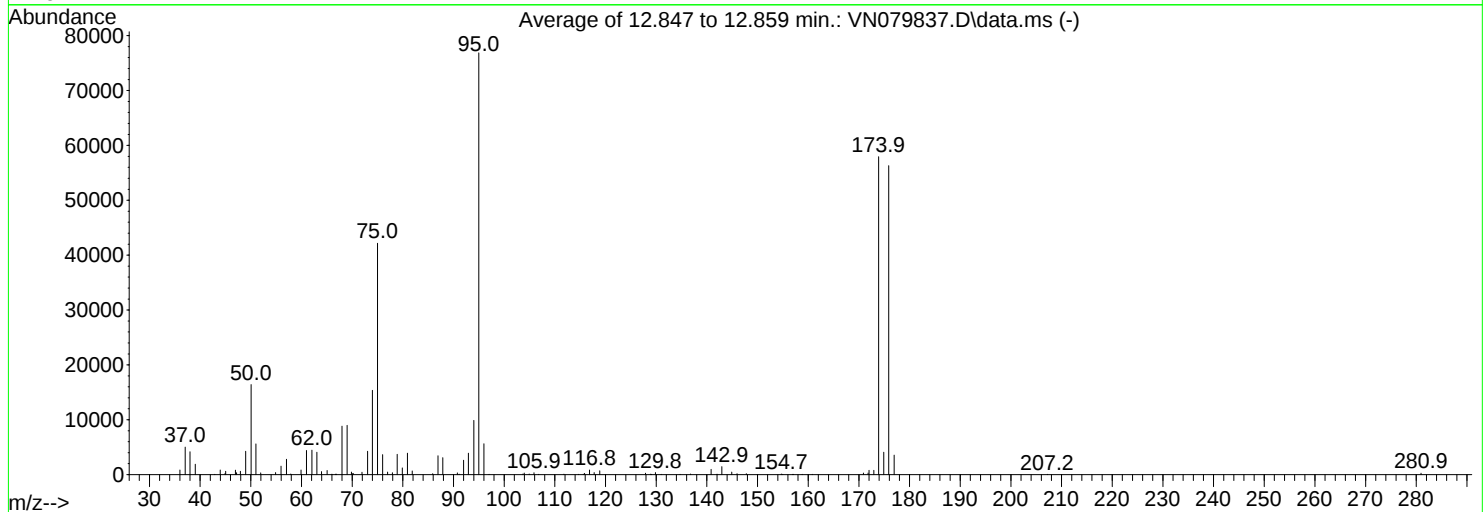


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110323\
Data File : VN079837.D
Acq On : 03 Nov 2023 09:59
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Title : SW846 8260
Last Update : Thu Nov 02 05:49:08 2023

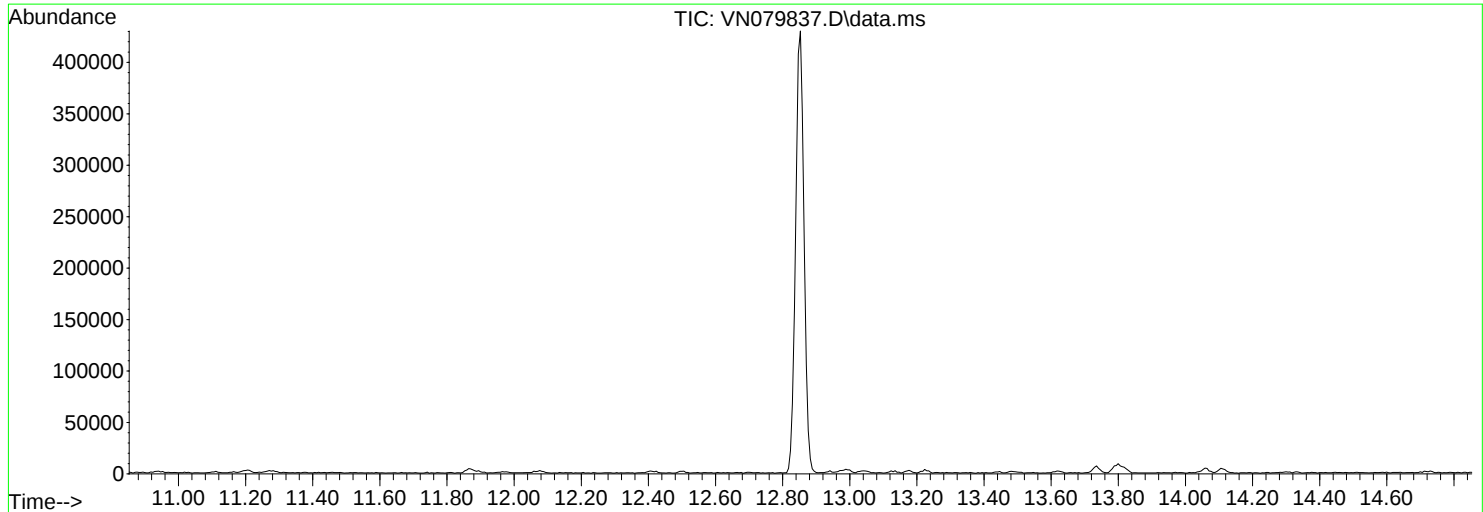

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.3	16406	PASS
75	95	30	60	54.9	42165	PASS
95	95	100	100	100.0	76867	PASS
96	95	5	9	7.3	5643	PASS
173	174	0.00	2	1.4	788	PASS
174	95	50	100	75.4	57949	PASS
175	174	5	9	7.0	4080	PASS
176	174	95	101	97.2	56304	PASS
177	176	5	9	6.3	3573	PASS

Average of 12.847 to 12.859 min.: VN079837.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	834	49.00	4267	63.05	4095	71.95	4216
37.05	5029	50.05	16406	63.95	555	73.05	4241
38.00	4171	51.00	5604	65.05	749	74.00	1537
39.05	1885	51.95	328	66.00	83	75.00	4216
42.90	50	54.90	387	66.70	81	76.00	3642
43.95	833	55.95	1536	66.90	92	77.00	458
44.90	217	57.05	2792	68.00	8834	77.95	355
45.05	626	57.90	105	69.00	8988	78.90	3709
46.95	811	59.90	860	69.85	469	79.90	1223
47.20	346	61.00	4411	70.00	201	80.90	3896
47.95	618	62.05	4450	70.20	235	81.85	678

Average of 12.847 to 12.859 min.: VN079837.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.90	182	103.70	122	118.85	690	144.90	472
86.95	3436	103.95	283	127.90	266	145.95	177
87.90	3081	104.95	113	128.90	86	147.80	182
90.75	308	105.90	362	129.10	53	154.70	119
91.10	86	106.80	63	129.85	392	155.00	73
92.00	2612	111.80	80	131.00	62	156.90	54
92.95	3896	114.70	56	134.70	64	157.10	75
94.00	9880	115.60	90	136.80	108	158.80	64
95.00	76867	115.85	247	140.85	959	160.80	66
96.00	5643	116.85	854	142.00	83	170.90	282
97.00	51	117.75	383	142.95	1455	171.80	307

Average of 12.847 to 12.859 min.: VN079837.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.00	789						
172.95	788						
173.90	57949						
174.90	4080						
175.90	56304						
176.95	3573						
207.20	51						
280.95	257						