


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110323\
Data File : VN079865.D
Acq On : 03 Nov 2023 23:26
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Title : SW846 8260
Last Update : Thu Nov 02 05:49:08 2023

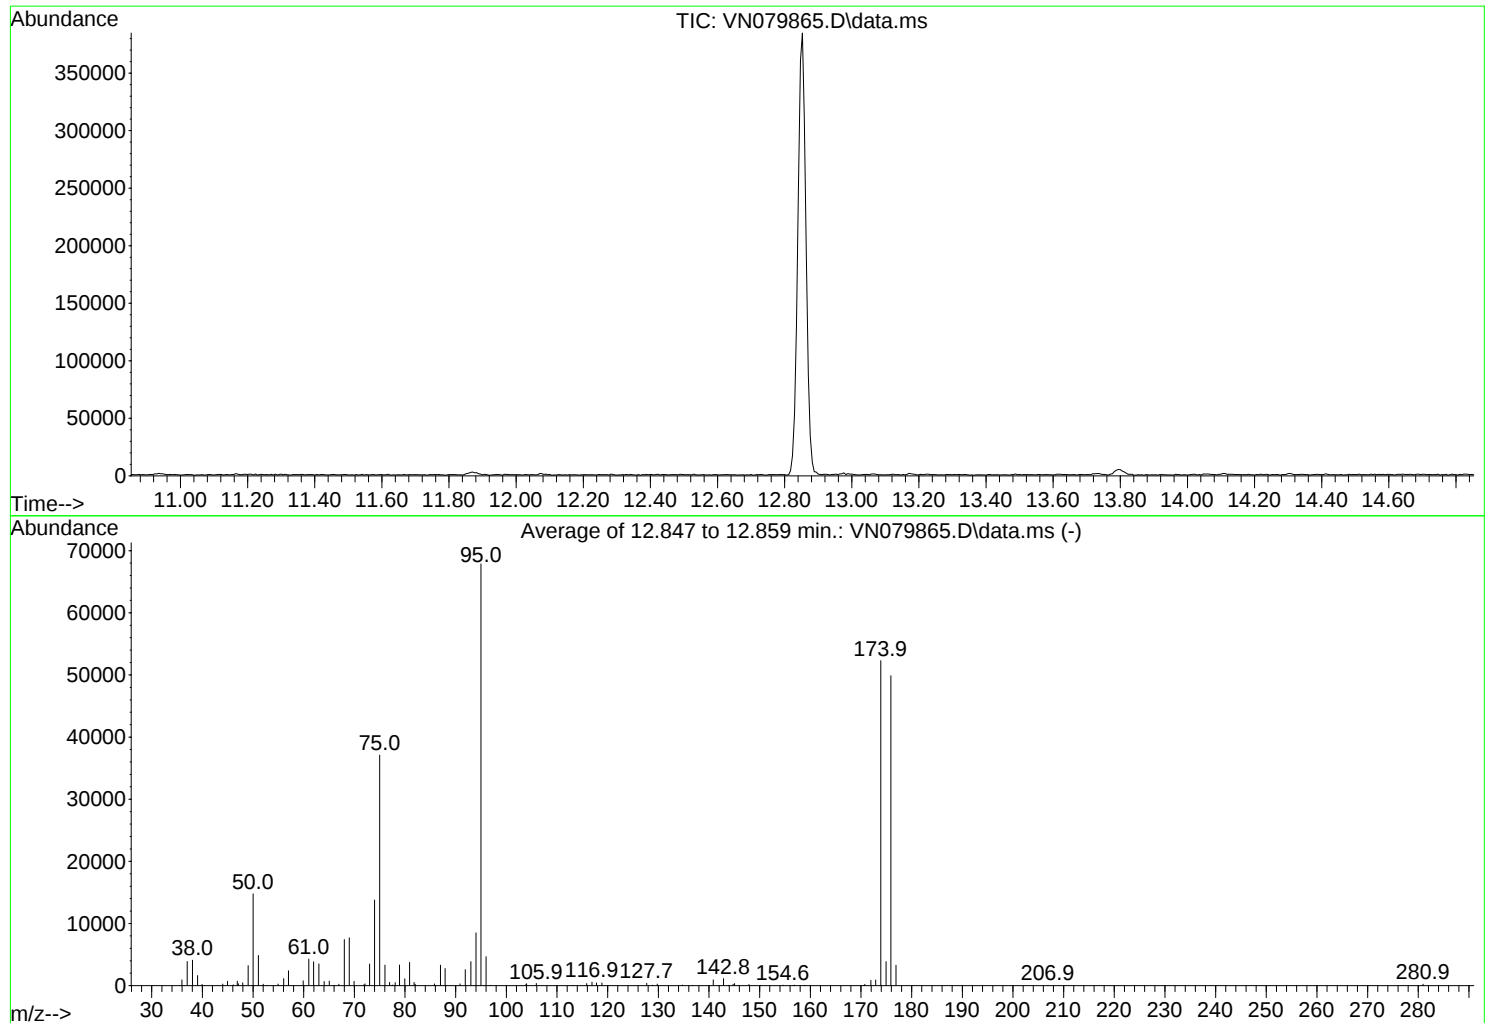

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	14789	PASS
75	95	30	60	54.6	37096	PASS
95	95	100	100	100.0	67888	PASS
96	95	5	9	6.9	4662	PASS
173	174	0.00	2	1.7	910	PASS
174	95	50	100	77.0	52301	PASS
175	174	5	9	7.4	3866	PASS
176	174	95	101	95.4	49891	PASS
177	176	5	9	6.6	3305	PASS

Average of 12.847 to 12.859 min.: VN079865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	934	49.05	3213	63.00	3510	74.00	13784
37.00	3893	50.00	14789	64.05	675	75.00	3709
38.05	4093	51.05	4866	65.05	720	76.05	329
39.05	1624	52.00	232	66.00	53	76.95	52
39.95	200	52.80	57	66.95	247	77.50	108
44.00	270	54.95	258	68.00	7426	78.05	502
44.95	691	56.05	1135	69.00	7697	78.90	3329
46.10	120	57.00	2387	69.95	703	79.95	1099
46.90	721	59.90	777	71.90	160	80.90	3736
47.10	320	61.00	4266	72.10	278	81.80	510
47.95	470	61.95	3829	73.00	3469	82.00	226

Average of 12.847 to 12.859 min.: VN079865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.80	281	104.00	319	136.70	65	156.60	59
87.00	3292	105.90	359	140.85	925	156.90	71
87.90	2750	113.10	67	141.80	50	158.90	51
90.85	285	115.85	329	142.85	1136	170.60	56
91.90	2572	116.90	562	143.80	50	170.75	199
93.00	3862	117.80	428	144.75	246	171.95	858
94.00	8491	118.85	428	145.05	332	172.90	910
95.00	67888	127.70	392	145.90	60	173.90	52301
96.00	4662	128.80	85	147.90	183	174.95	3866
96.80	66	129.80	271	150.10	54	175.90	49891
103.80	127	134.75	112	154.60	85	176.90	3305

Average of 12.847 to 12.859 min.: VN079865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
206.90	57						
280.95	243						

Instrument :

MSVOA_N

ClientSampleId :

BFB